

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN072220\
 Data File : VN062609.D
 Acq On : 22 Jul 2020 20:50
 Operator : JC/MD
 Sample : VSTDCCC050
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 23 07:18:50 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072120W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 21 18:48:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.63
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.55
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.38
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.32

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount	50.000		Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN072220\
Data File : VN062609.D
Acq On : 22 Jul 2020 20:50
Operator : JC/MD
Sample : VSTDCCC050
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 23 07:18:50 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072120W.M
Quant Title : SW846 8260
QLast Update : Tue Jul 21 18:48:59 2020
Response via : Initial Calibration

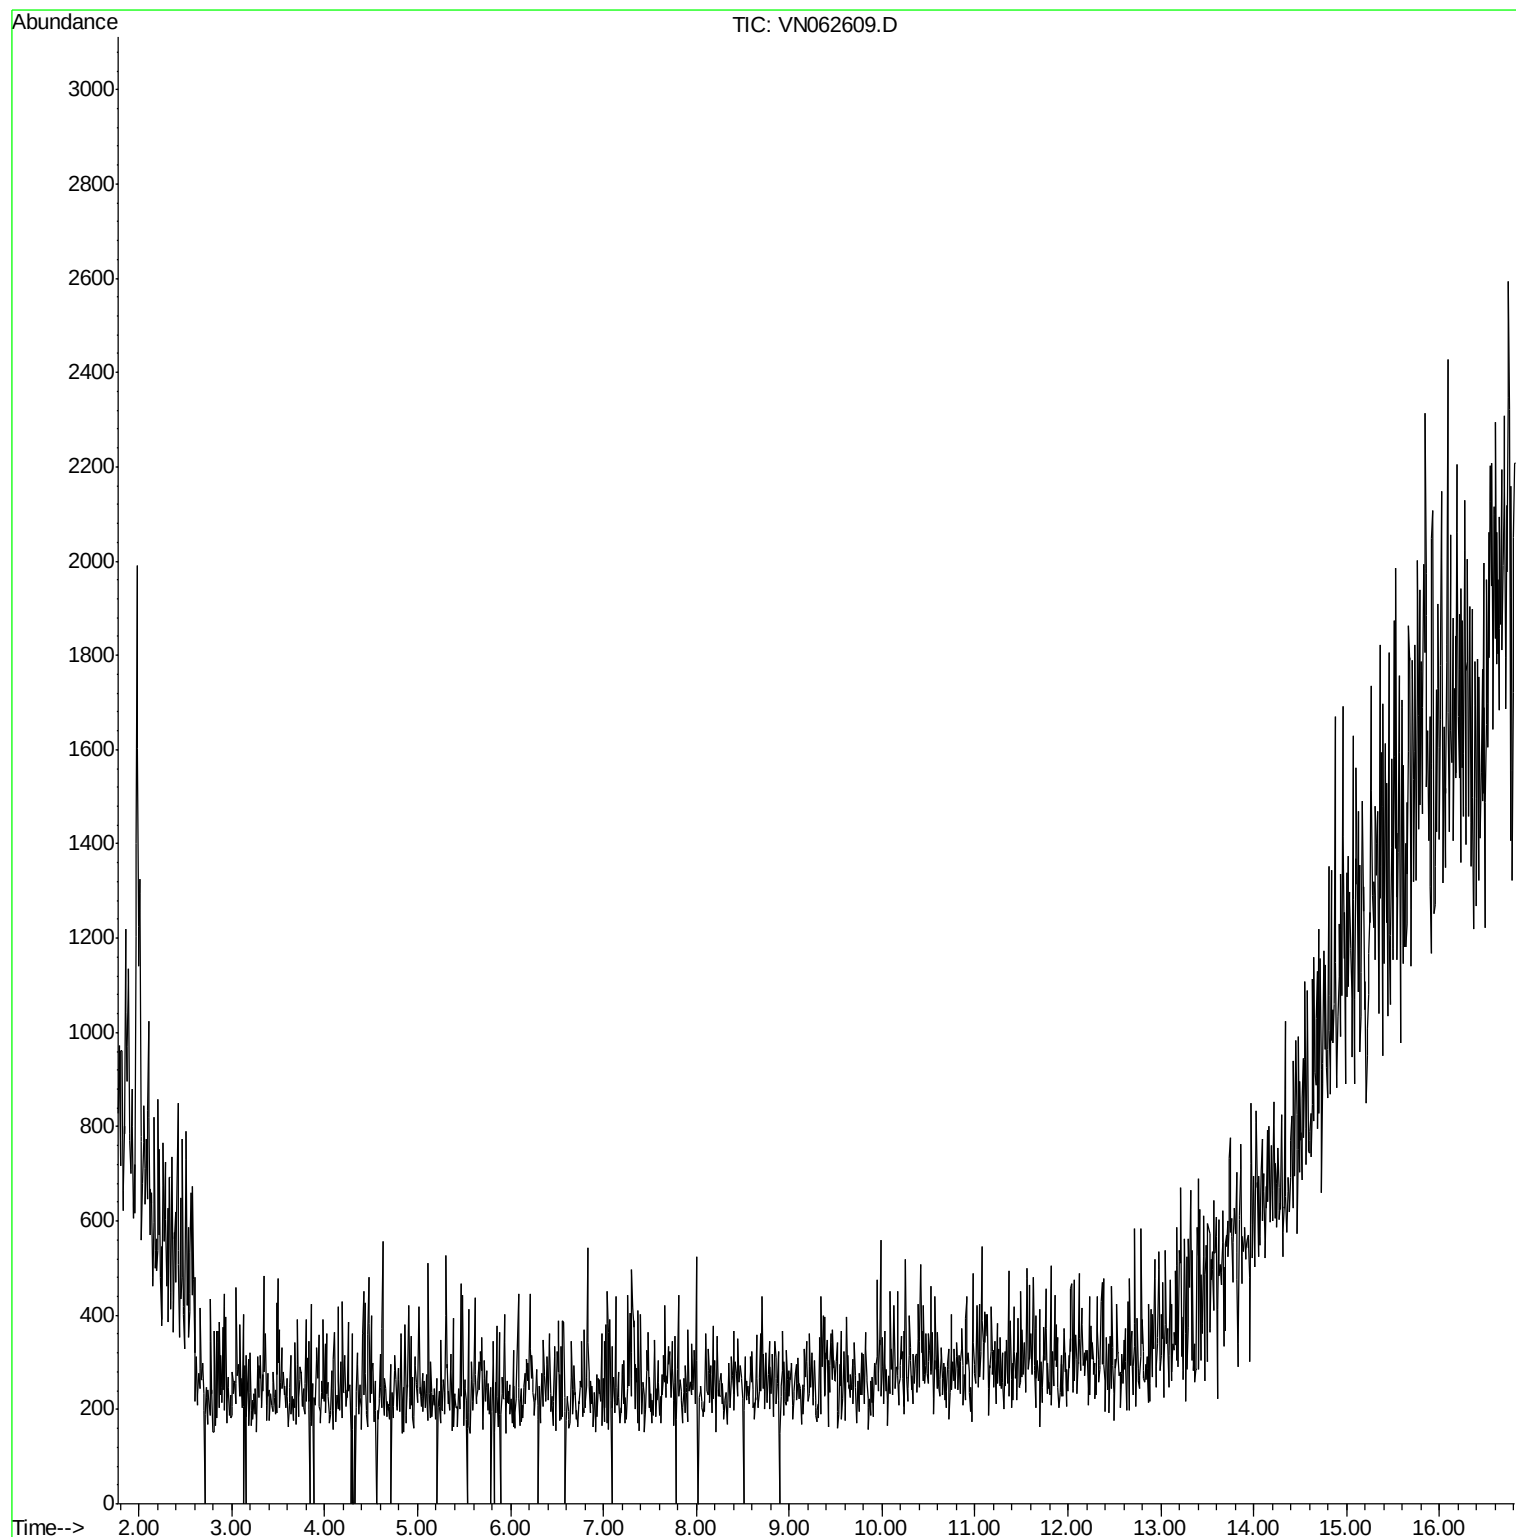

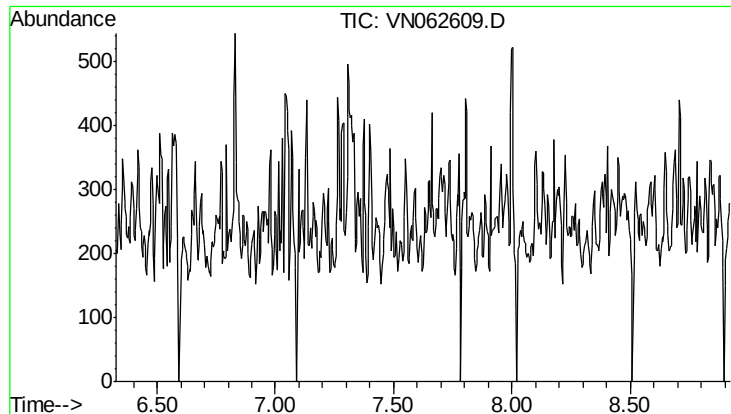

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.63 min

Lab File: VN062609.D

Acq: 22 Jul 2020 20:50

Tot Ion: 168

Sig Exp Ratio



168 100

99 60.5

Instrument :

MSVOA_N

ClientSampleId :

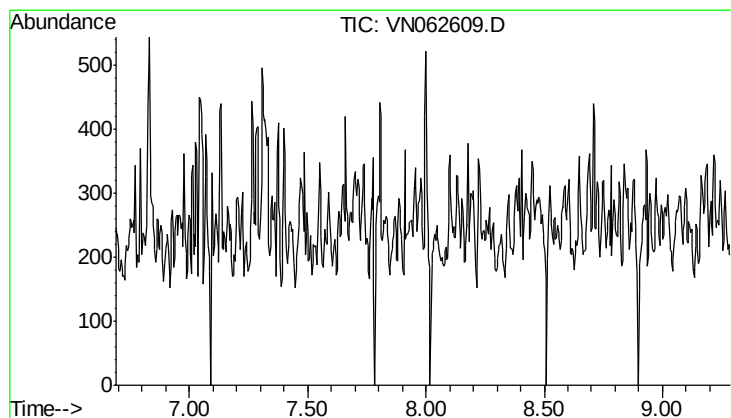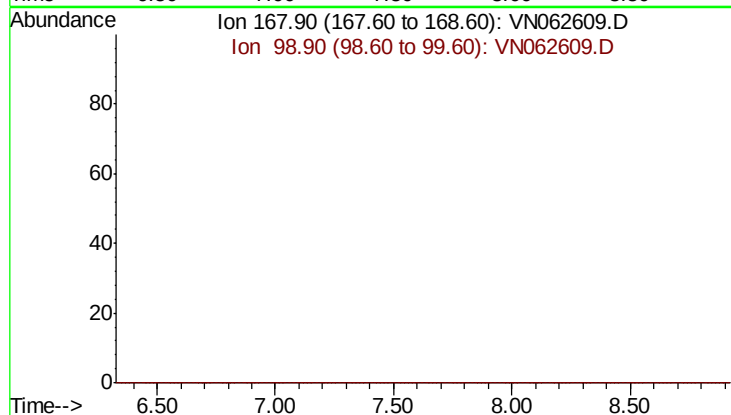

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l

Expected RT: 7.99 min

Lab File: VN062609.D


Acq: 22 Jul 2020 20:50


Tgt Ion: 65

Sig Exp Ratio

65 100

67 53.0


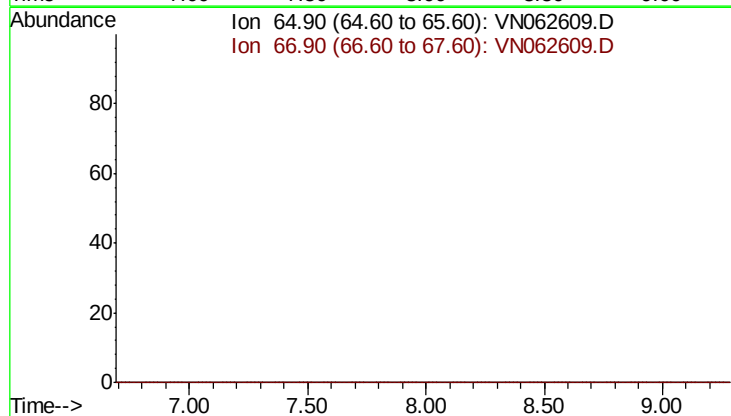


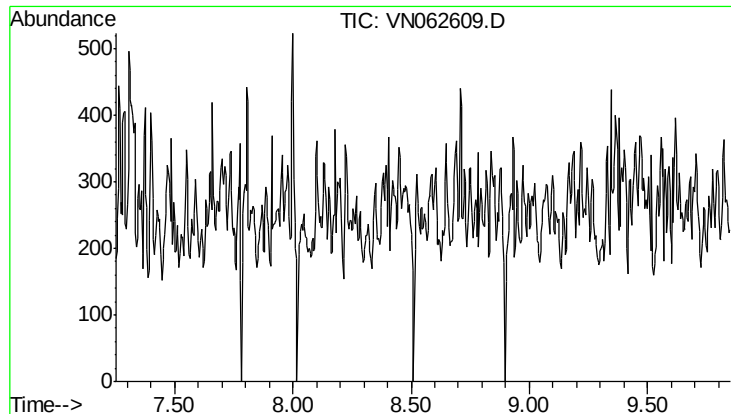

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.55 min
 Lab File: VN062609.D
 Acq: 22 Jul 2020 20:50


Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion	114
Sig	Exp Ratio
114	100
63	24.2
88	16.9

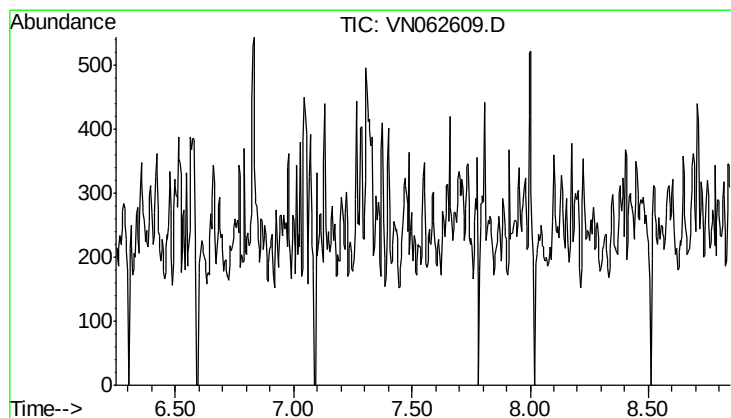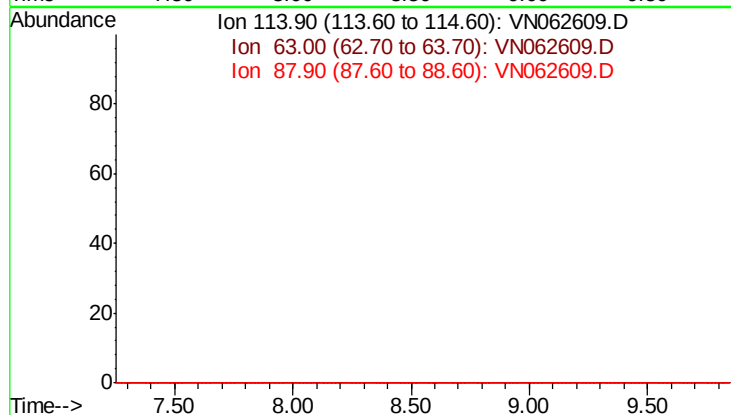

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.55 min
 Lab File: VN062609.D
 Acq: 22 Jul 2020 20:50

Tgt Ion	113
Sig	Exp Ratio
113	100
111	103.4
192	18.5

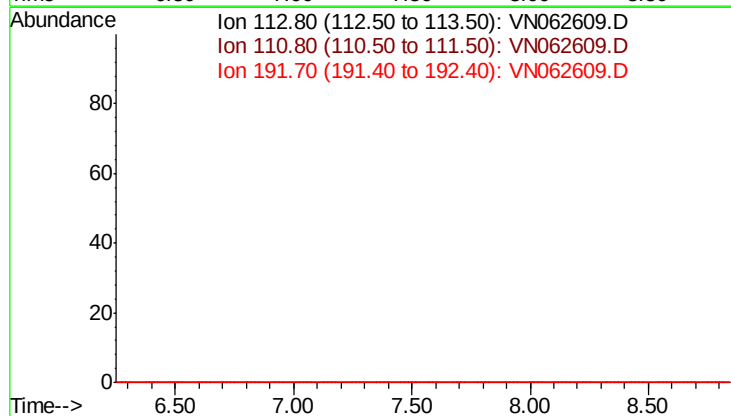


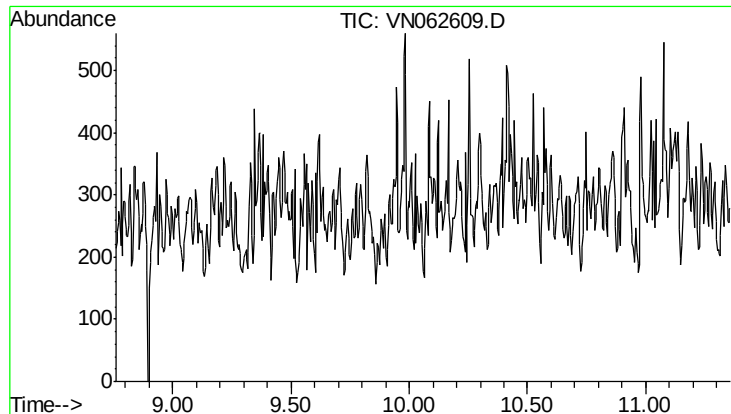


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.06 min

Lab File: VN062609.D
Acq: 22 Jul 2020 20:50

Instrument :
MSVOA_N
ClientSampleId :


Tot Ion	98
Sig	Exp Ratio
98	100
100	63.6

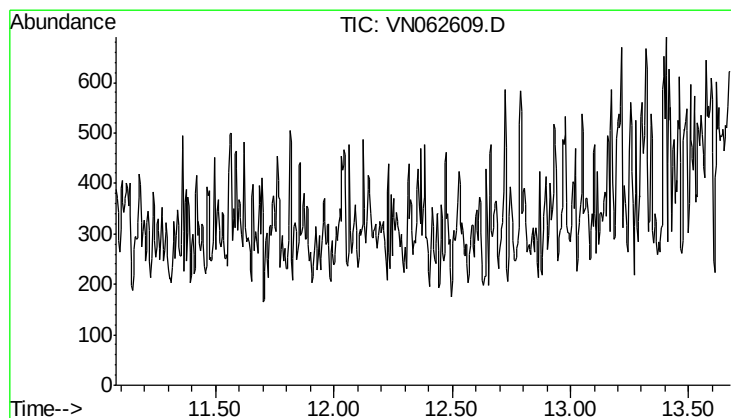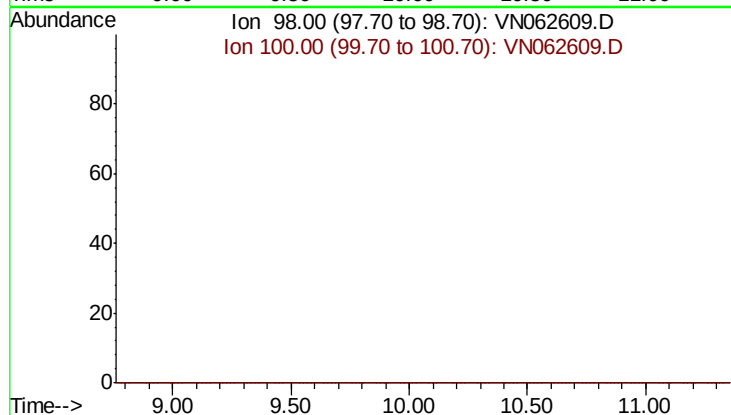


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.38 min

Lab File: VN062609.D
Acq: 22 Jul 2020 20:50

Tgt Ion	95
Sig	Exp Ratio
95	100
174	72.3
176	69.7


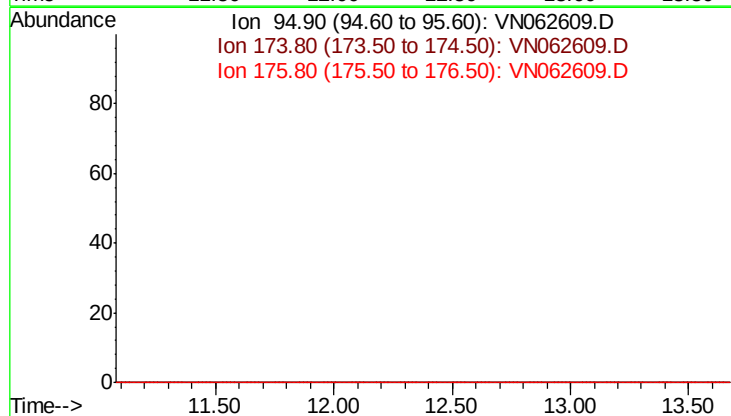


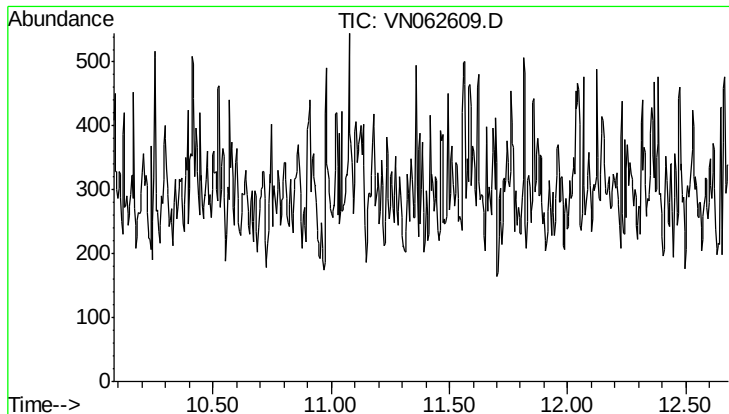

#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.38 min
 Lab File: VN062609.D
 Acq: 22 Jul 2020 20:50

Instrument :
 MSVOA_N
 ClientSampleId :

Tot Ion	117
Sig	Exp Ratio
117	100
82	61.3
119	31.8

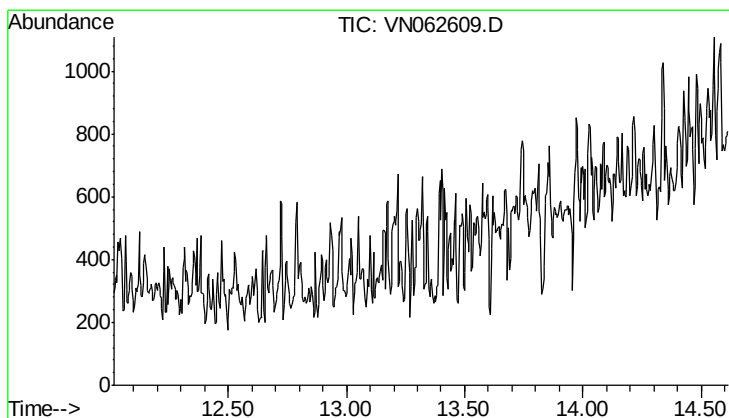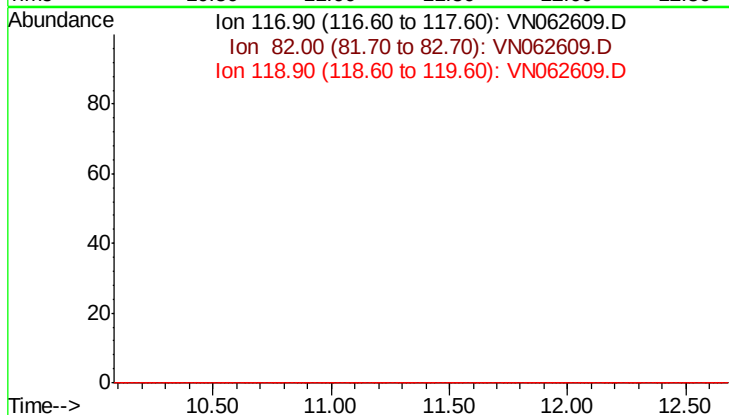

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.32 min
 Lab File: VN062609.D
 Acq: 22 Jul 2020 20:50

Tgt Ion	152
Sig	Exp Ratio
152	100
115	63.6
150	175.7

