


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN072220\
Data File : VN062585.D
Acq On : 22 Jul 2020 9:21
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072120W.M
Title : SW846 8260
Last Update : Tue Jul 21 18:48:59 2020

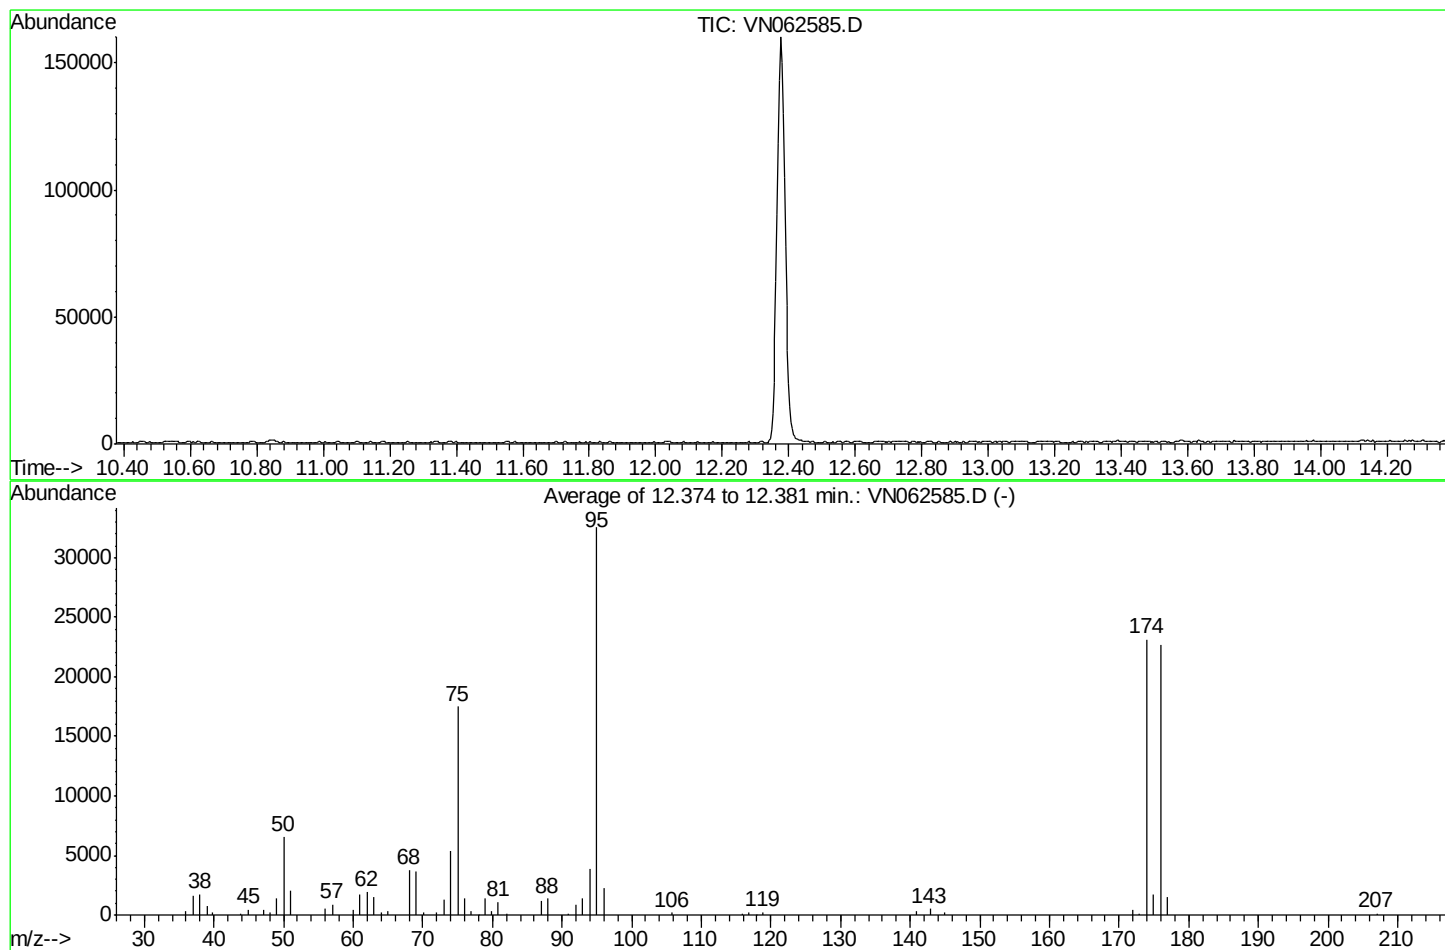

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	6582	PASS
75	95	30	60	53.8	17496	PASS
95	95	100	100	100.0	32549	PASS
96	95	5	9	6.9	2243	PASS
173	174	0.00	2	0.6	137	PASS
174	95	50	100	71.0	23122	PASS
175	174	5	9	7.4	1721	PASS
176	174	95	101	98.0	22666	PASS
177	176	5	9	6.6	1505	PASS