

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN072221\  
 Data File : VN067865.D  
 Acq On : 22 Jul 2021 16:16  
 Operator : JC/MD  
 Sample : M3120-02  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 TT-RW6B-IDWGW-20210719

Integration Parameters: RTEINT3.P  
 Integrator: RTE  
 Smoothing : OFF Filtering: 5  
 Sampling : 1 Min Area: 0 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N071421W.M  
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VN067865.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.197       | 799           | 823         | 850          | rVB8     | 32668          | 113456        | 3.38%           | 1.475%        |
| 2         | 7.662       | 2093          | 2115        | 2142         | rBV3     | 157331         | 412159        | 12.28%          | 5.357%        |
| 3         | 8.206       | 2300          | 2318        | 2335         | rVB4     | 15719          | 39126         | 1.17%           | 0.509%        |
| 4         | 8.439       | 2384          | 2405        | 2432         | rBV      | 176374         | 402053        | 11.98%          | 5.226%        |
| 5         | 8.970       | 2585          | 2603        | 2630         | rVB      | 370598         | 773199        | 23.04%          | 10.050%       |
| 6         | 9.217       | 2674          | 2695        | 2740         | rBV      | 1637136        | 3356080       | 100.00%         | 43.623%       |
| 7         | 10.443      | 3129          | 3152        | 3179         | rBV      | 578753         | 1093060       | 32.57%          | 14.208%       |
| 8         | 11.746      | 3622          | 3638        | 3677         | rVB      | 504510         | 916154        | 27.30%          | 11.908%       |
| 9         | 12.733      | 3988          | 4006        | 4030         | rBV      | 331708         | 588014        | 17.52%          | 7.643%        |


Sum of corrected areas: 7693301

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN072221\  
Data File : VN067865.D  
Acq On : 22 Jul 2021 16:16  
Operator : JC/MD  
Sample : M3120-02  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TT-RW6B-IDWGW-20210719

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N071421W.M  
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

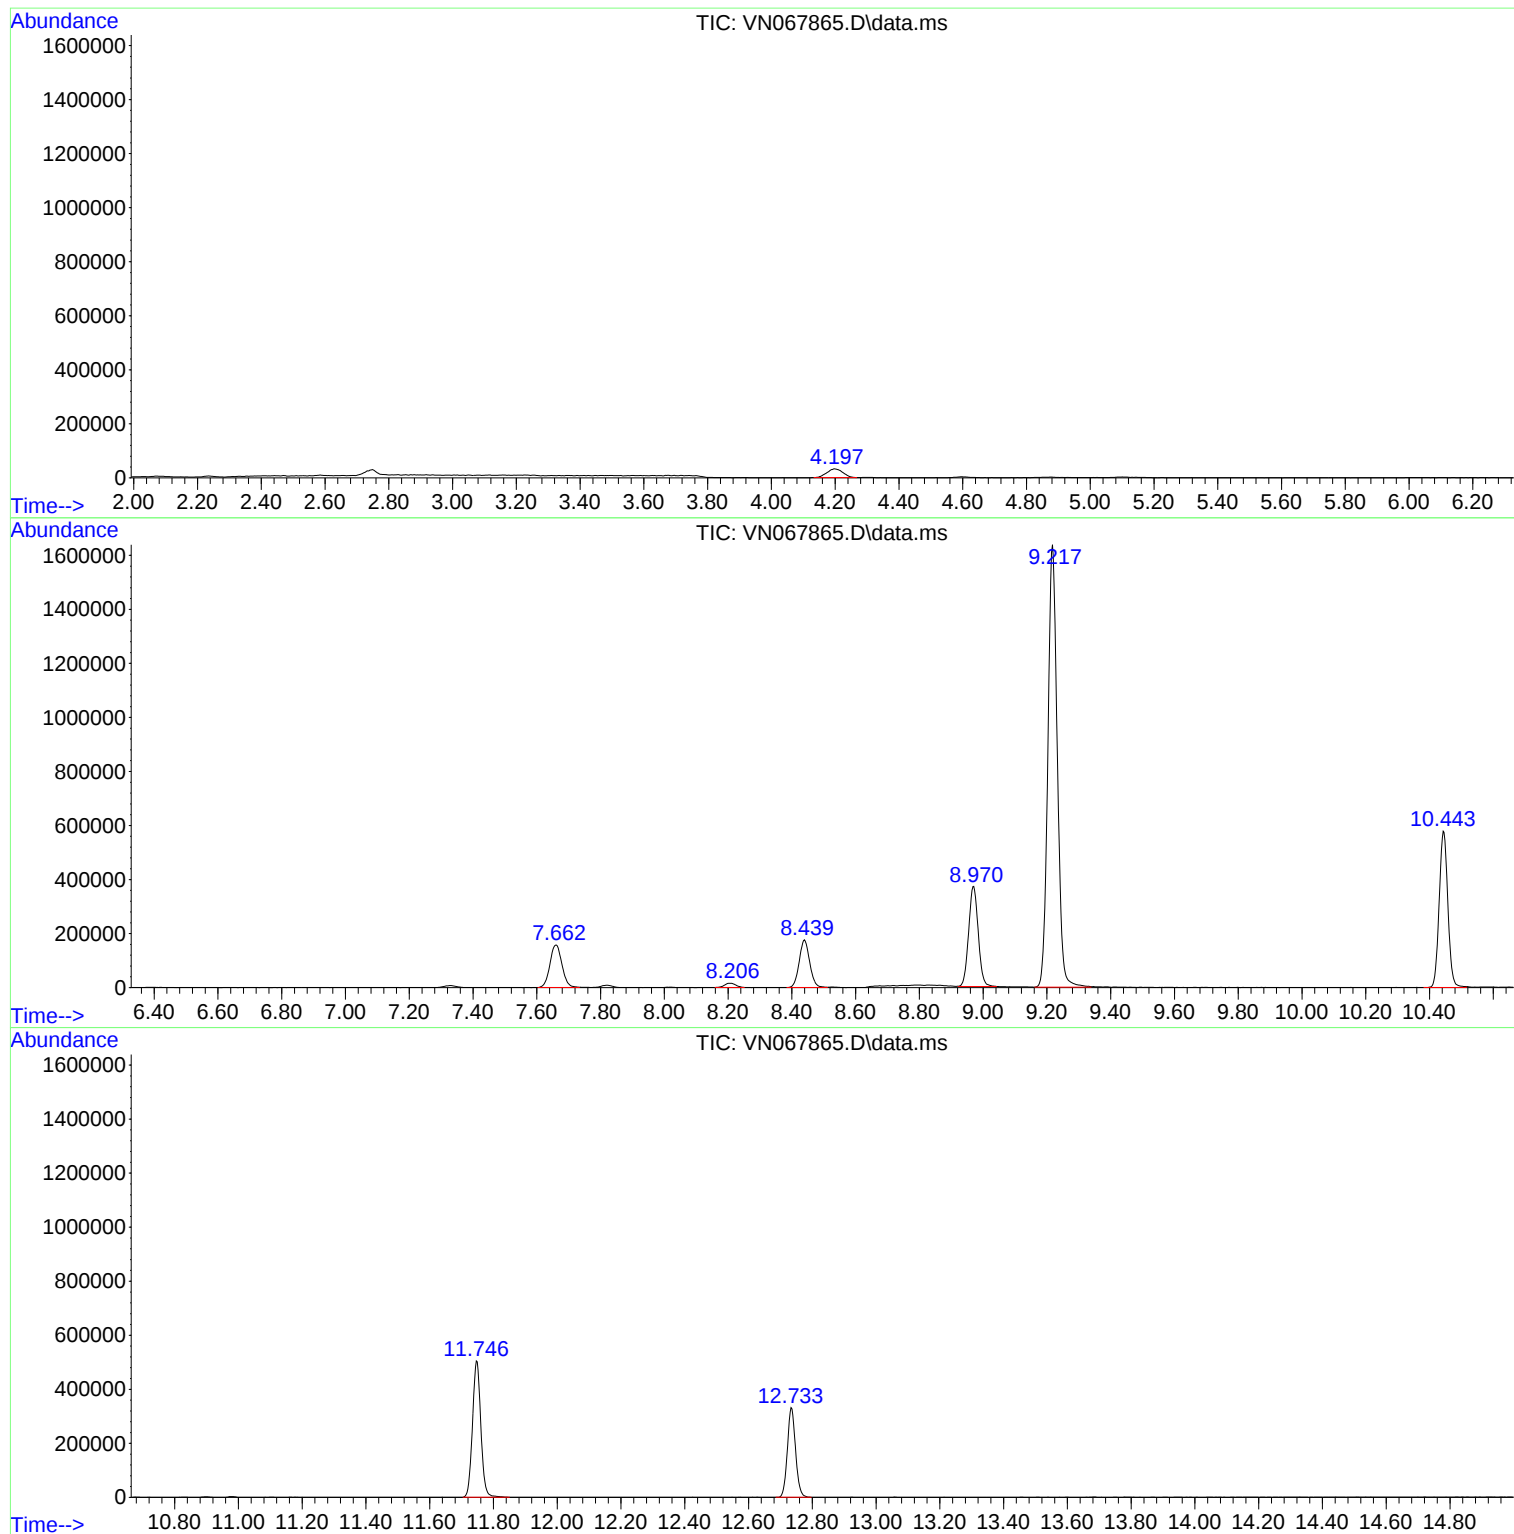

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN072221\  
Data File : VN067865.D  
Acq On : 22 Jul 2021 16:16  
Operator : JC/MD  
Sample : M3120-02  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TT-RW6B-IDWGW-20210719

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N071421W.M  
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN072221\  
Data File : VN067865.D  
Acq On : 22 Jul 2021 16:16  
Operator : JC/MD  
Sample : M3120-02  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TT-RW6B-IDWGW-20210719

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N071421W.M  
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|