


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072221\
 Data File : VN067855.D
 Acq On : 22 Jul 2021 8:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N071421W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Jul 14 01:19:19 2021

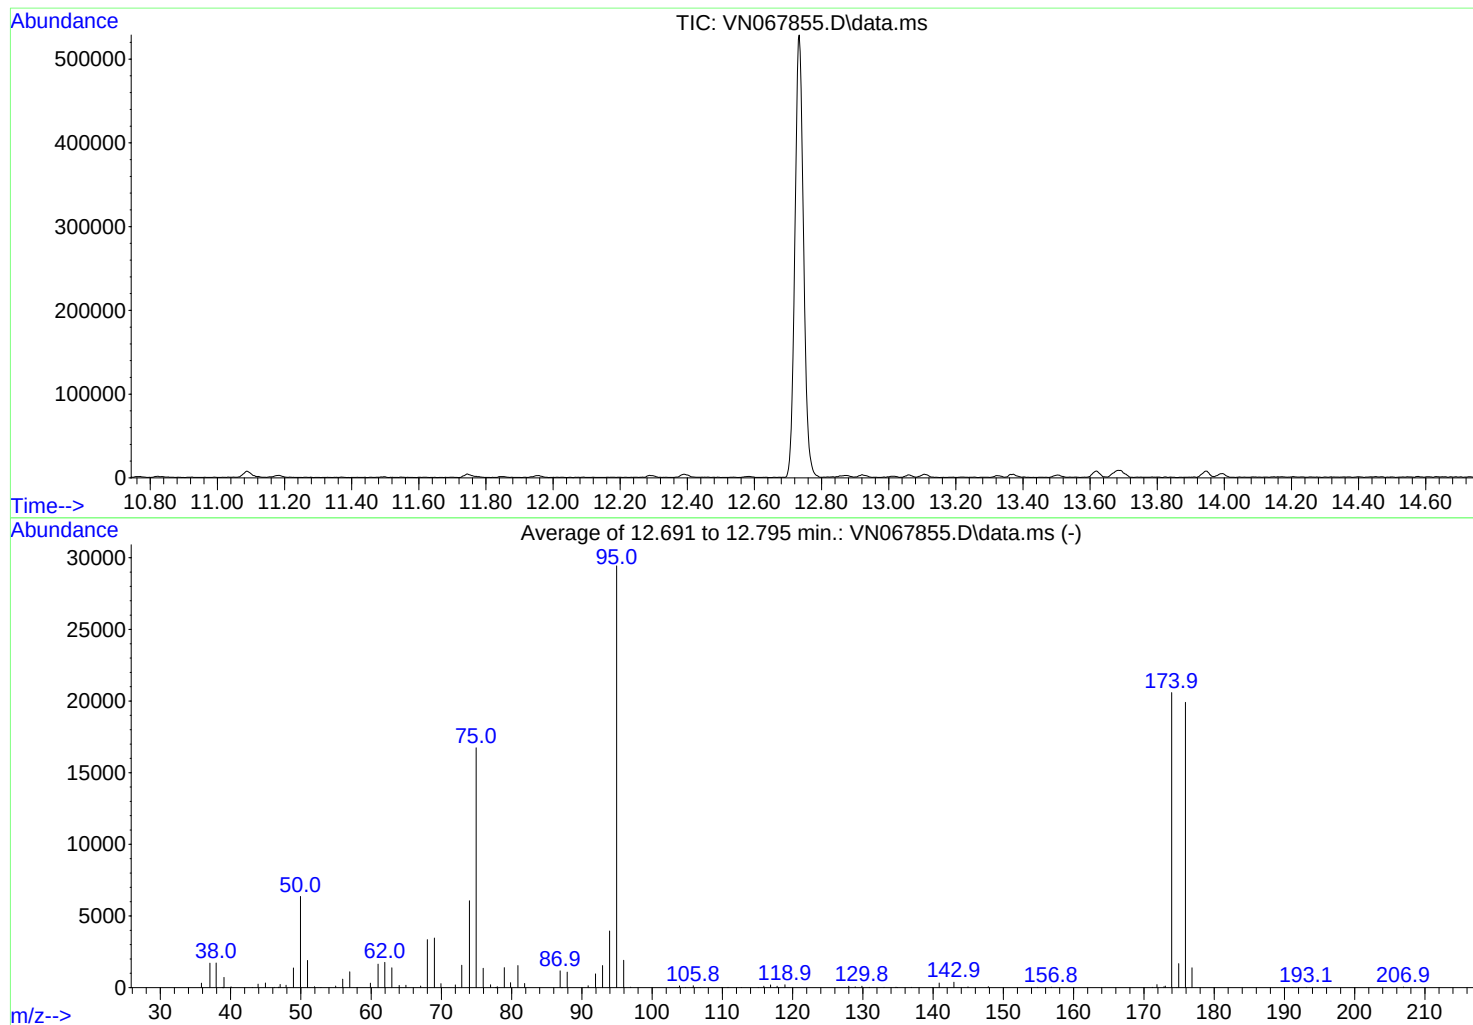

AutoFind: Averaged scan 3990 to 4029; Bkg corrected with scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	6361	PASS
75	95	30	60	56.9	16740	PASS
95	95	100	100	100.0	29436	PASS
96	95	5	9	6.5	1914	PASS
173	174	0.00	2	0.5	113	PASS
174	95	50	100	69.9	20589	PASS
175	174	5	9	8.1	1670	PASS
176	174	95	101	96.7	19909	PASS
177	176	5	9	7.0	1388	PASS