

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072224\
 Data File : VN083004.D
 Acq On : 22 Jul 2024 15:12
 Operator : JC\MD
 Sample : P3323-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 Storage-Blank-WATER-REF-5

Quant Time: Jul 23 03:51:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 08 13:46:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	72363	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	139452	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	140228	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	54662	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	57075	56.266	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	112.540%
35) Dibromofluoromethane	8.171	113	47446	53.022	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	106.040%
50) Toluene-d8	10.571	98	164115	49.656	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.320%
62) 4-Bromofluorobenzene	12.853	95	51812	43.642	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	87.280%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072224\
Data File : VN083004.D
Acq On : 22 Jul 2024 15:12
Operator : JC\MD
Sample : P3323-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
Storage-Blank-WATER-REF-5

Quant Time: Jul 23 03:51:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 08 13:46:04 2024
Response via : Initial Calibration




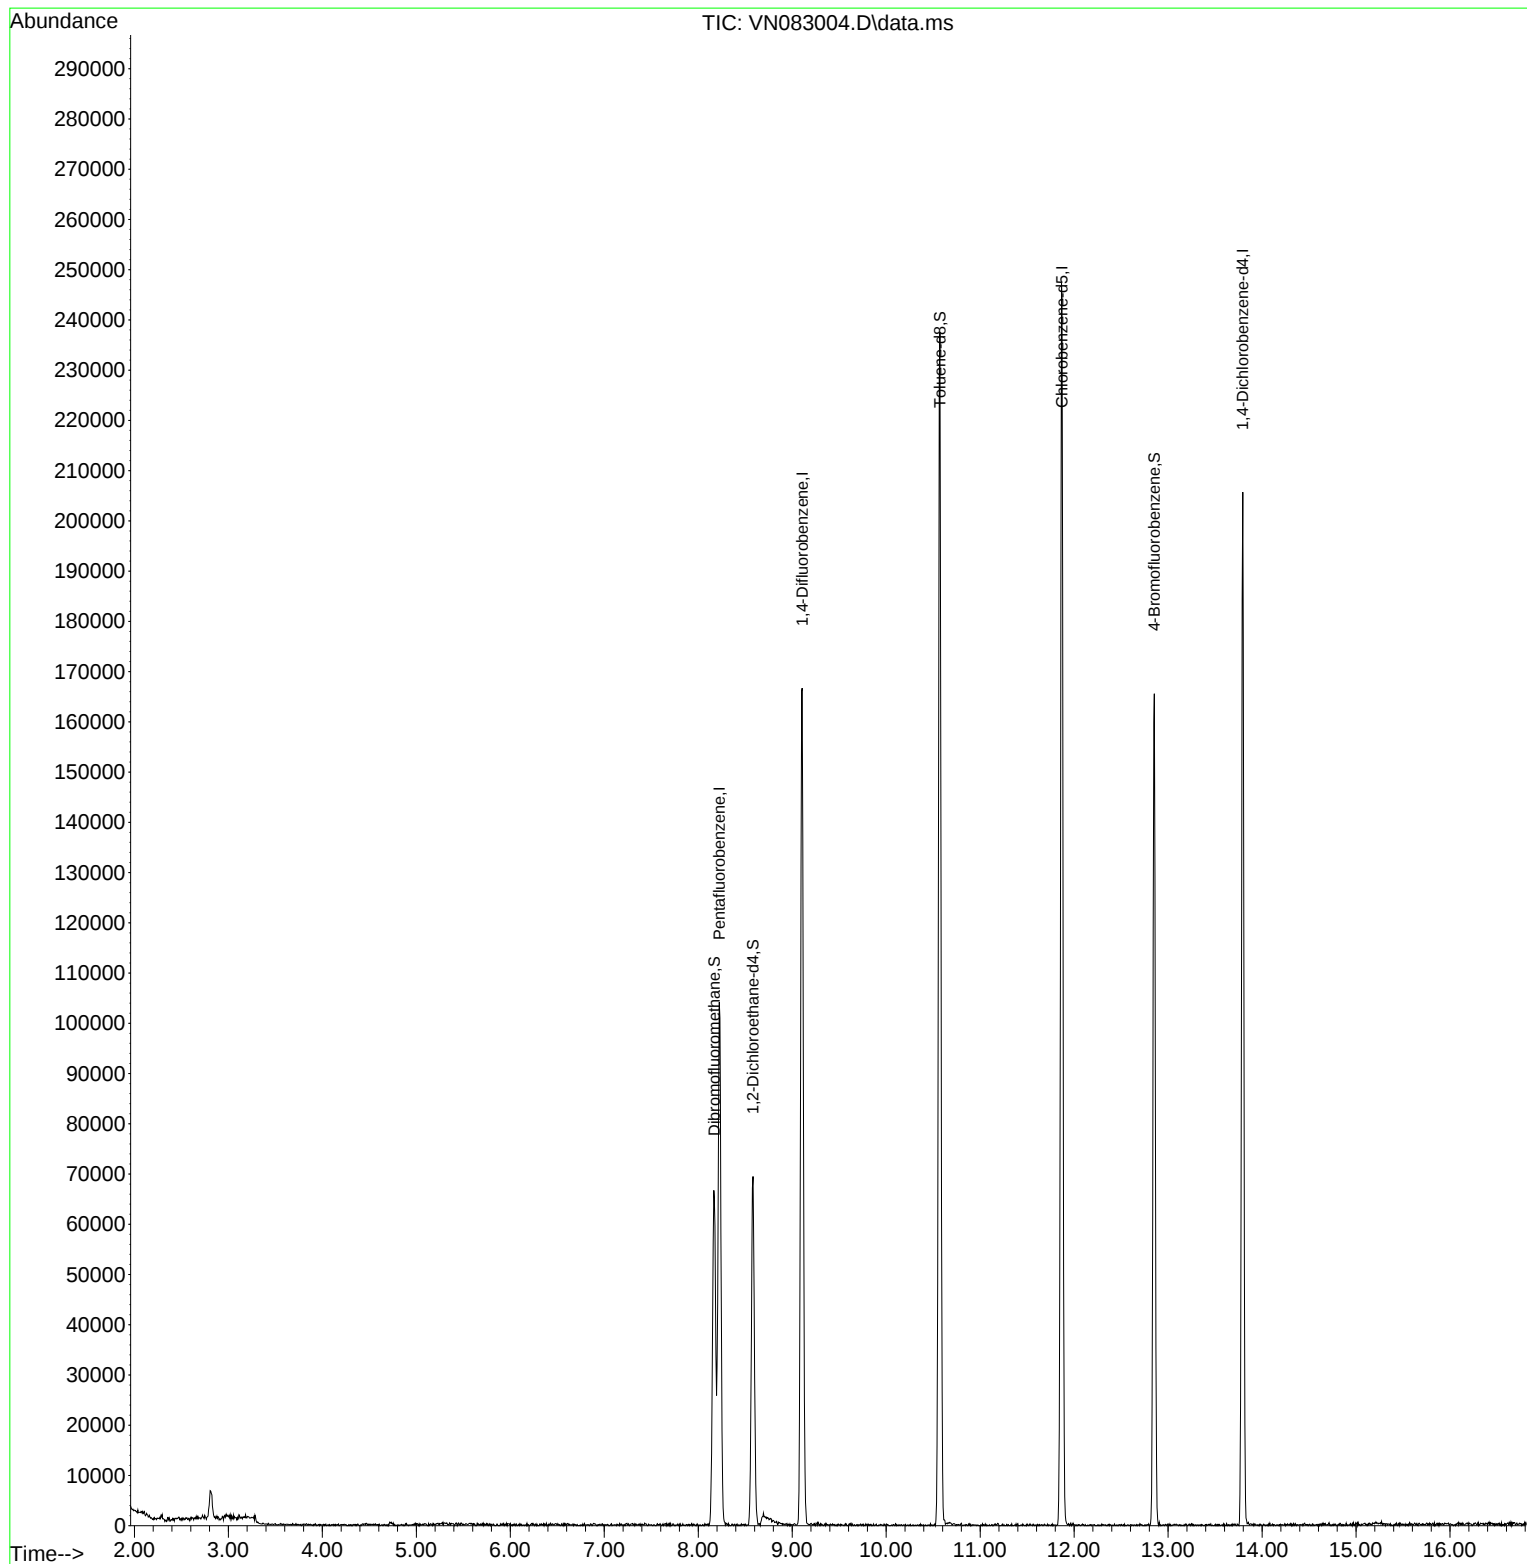


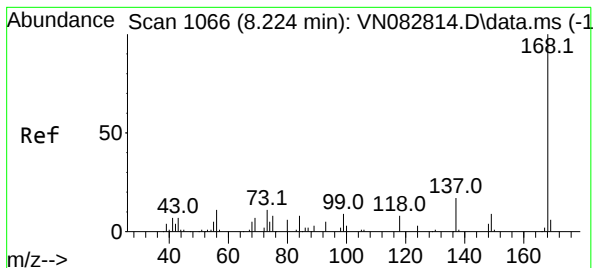

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.005 min
Lab File: VN083004.D
Acq: 22 Jul 2024 15:12




Instrument : MSVOA_N
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion:168 Resp: 72363
Ion Ratio Lower Upper
168 100
99 61.0 48.2 72.4

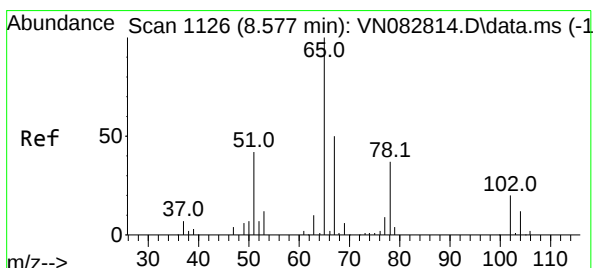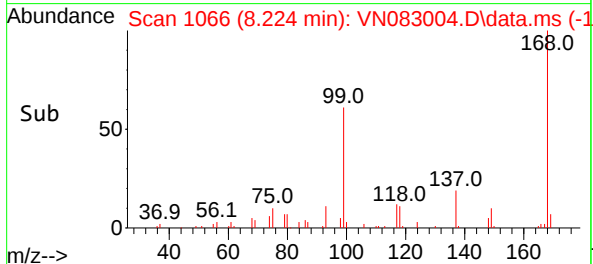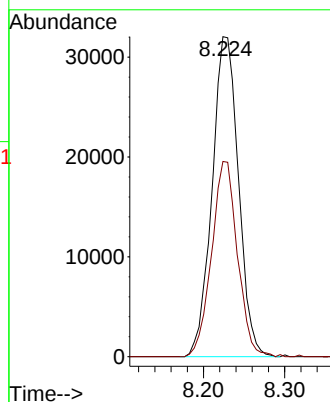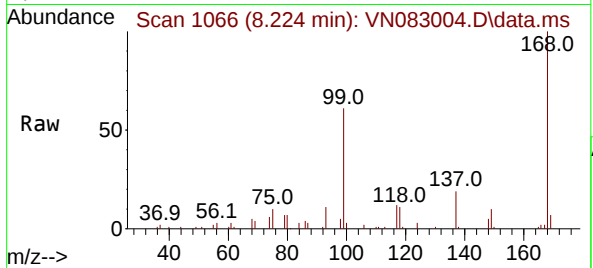

#33
1,2-Dichloroethane-d4
Concen: 56.266 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.001 min
Lab File: VN083004.D
Acq: 22 Jul 2024 15:12

Tgt Ion: 65 Resp: 57075
Ion Ratio Lower Upper
65 100
67 49.9 0.0 104.4


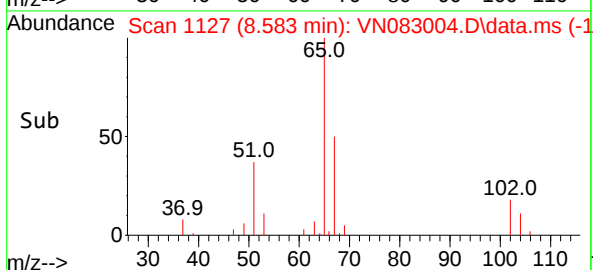
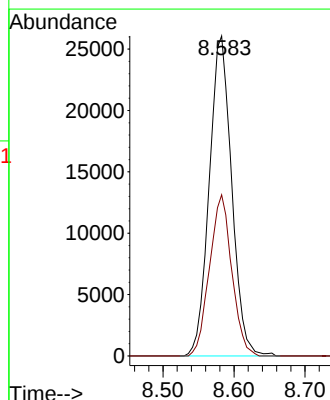
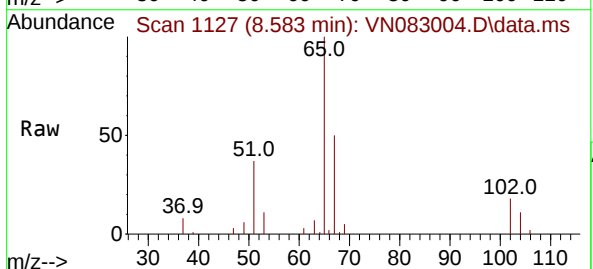


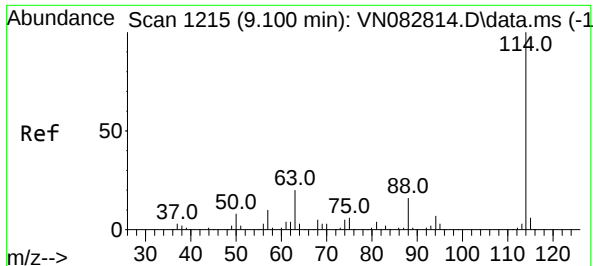

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN083004.D
Acq: 22 Jul 2024 15:12




Instrument :
MSVOA_N
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion:114 Resp: 139452
Ion Ratio Lower Upper
114 100
63 21.1 0.0 44.6
88 15.7 0.0 31.4

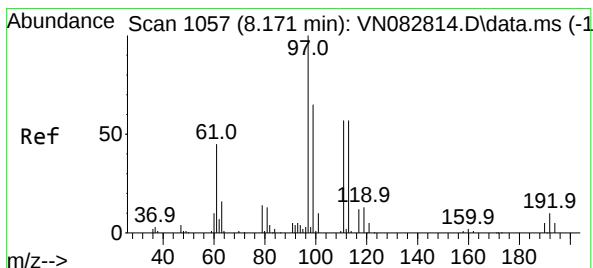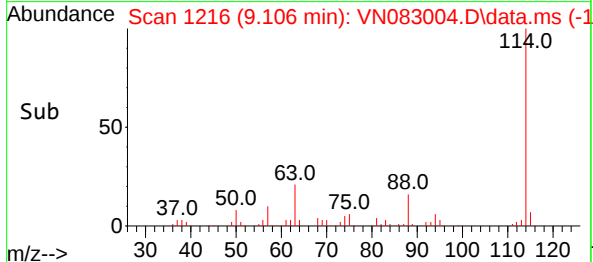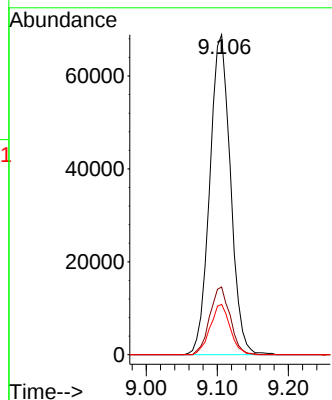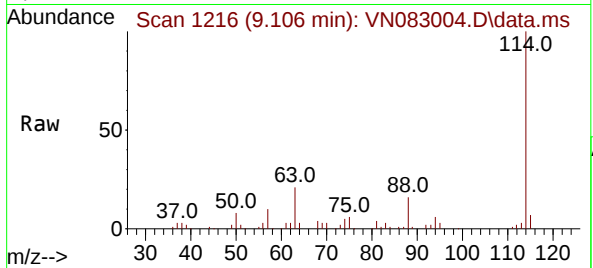

#35
Dibromofluoromethane
Concen: 53.022 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. 0.006 min
Lab File: VN083004.D
Acq: 22 Jul 2024 15:12

Tgt Ion:113 Resp: 47446
Ion Ratio Lower Upper
113 100
111 103.8 82.4 123.6
192 18.2 14.9 22.3


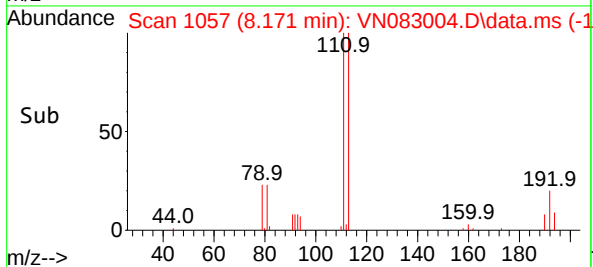
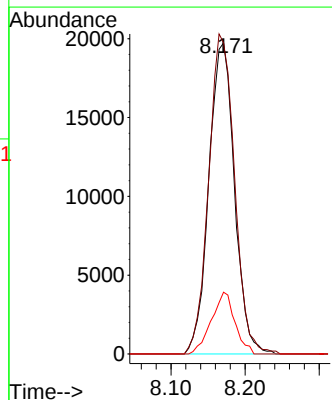
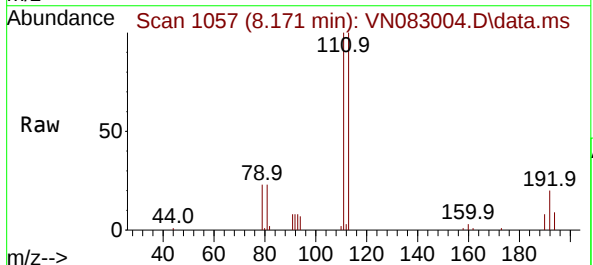


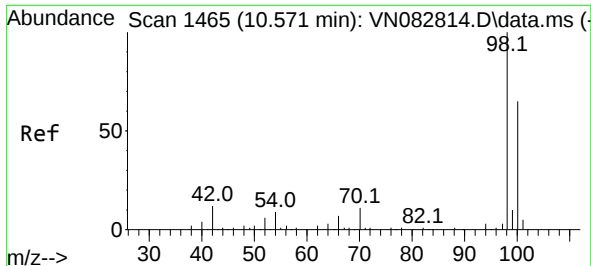

#50
Toluene-d8
Concen: 49.656 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.001 min
Lab File: VN083004.D
Acq: 22 Jul 2024 15:12




Instrument :
MSVOA_N
ClientSampleId :
Storage-Blank-WATER-REF-5


Tgt Ion: 98 Resp: 164115
Ion Ratio Lower Upper
98 100
100 62.9 51.5 77.3

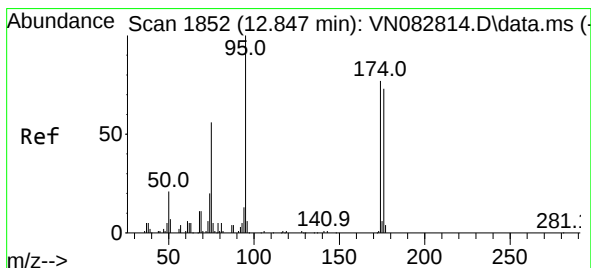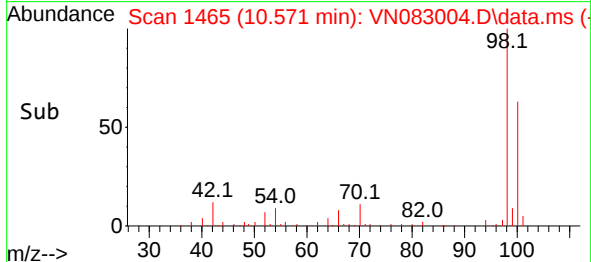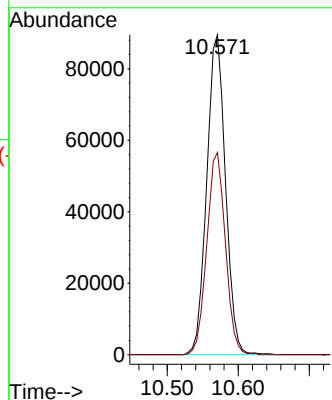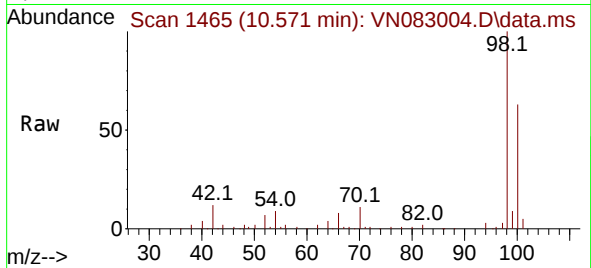

#62
4-Bromofluorobenzene
Concen: 43.642 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN083004.D
Acq: 22 Jul 2024 15:12

Tgt Ion: 95 Resp: 51812
Ion Ratio Lower Upper
95 100
174 84.3 0.0 159.2
176 81.0 0.0 147.6


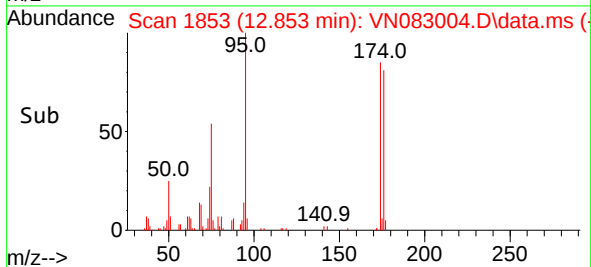
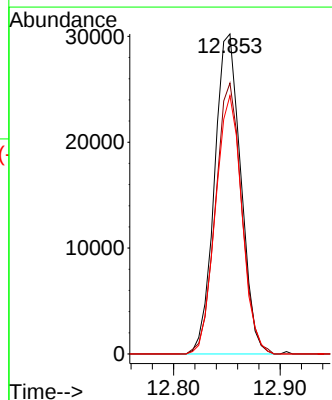
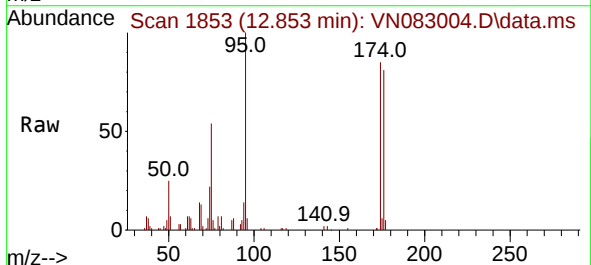


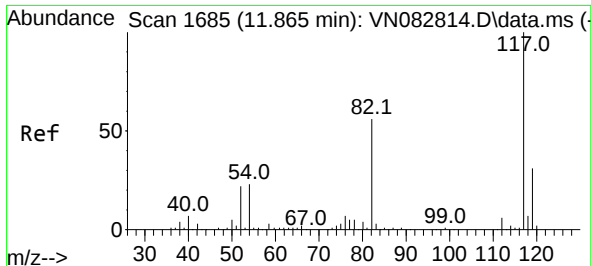

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1
Delta R.T. 0.001 min
Lab File: VN083004.D
Acq: 22 Jul 2024 15:12

Instrument :
MSVOA_N
ClientSampleId :
Storage-Blank-WATER-REF-5

Tgt Ion:117 Resp: 140228
Ion Ratio Lower Upper
117 100
82 55.7 47.5 71.3
119 31.6 25.6 38.4

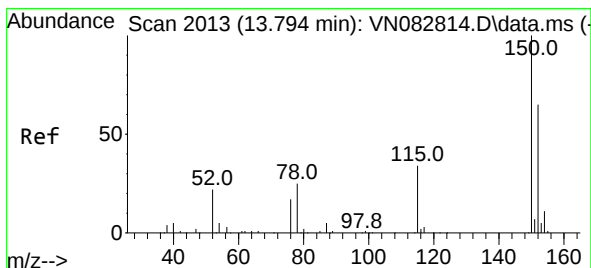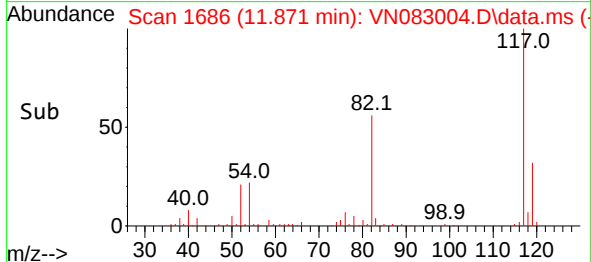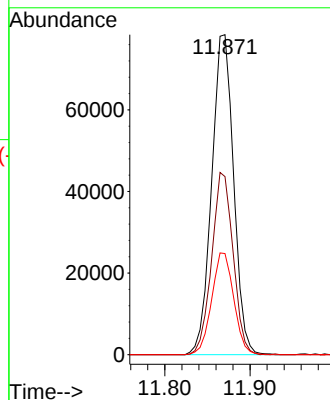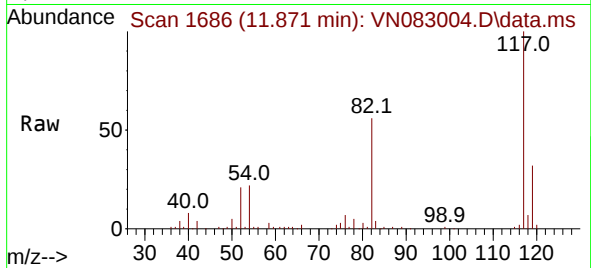

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN083004.D
Acq: 22 Jul 2024 15:12

Tgt Ion:152 Resp: 54662
Ion Ratio Lower Upper
152 100
115 59.0 30.6 91.6
150 154.5 0.0 348.6

