
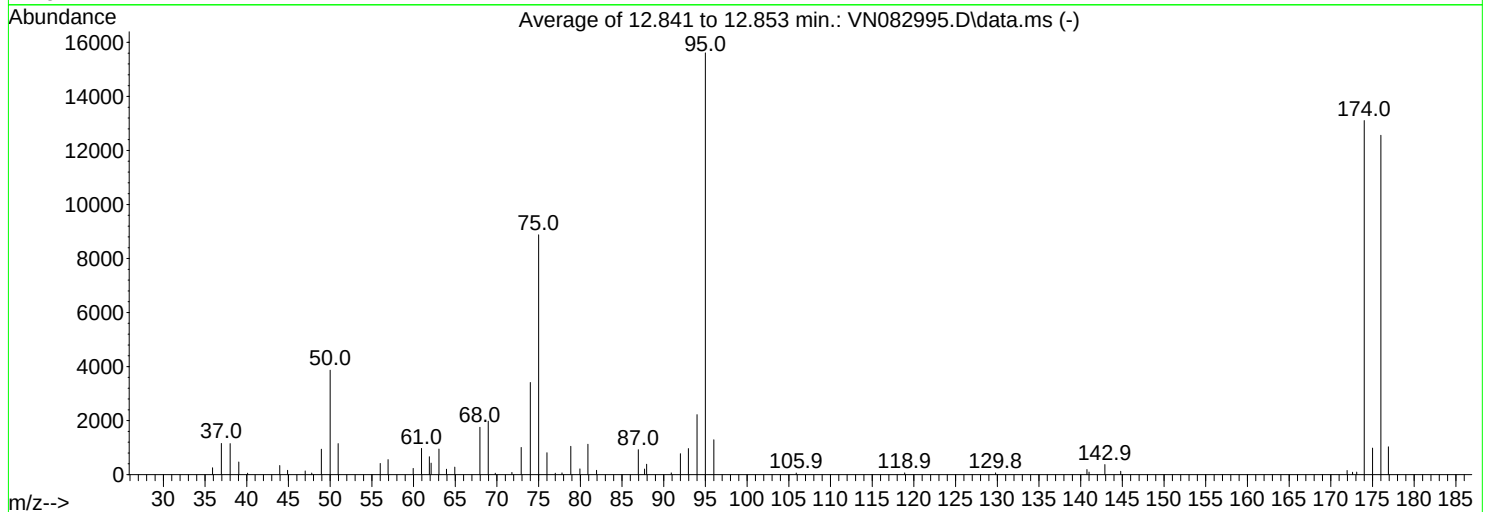


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072224\
Data File : VN082995.D
Acq On : 22 Jul 2024 10:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

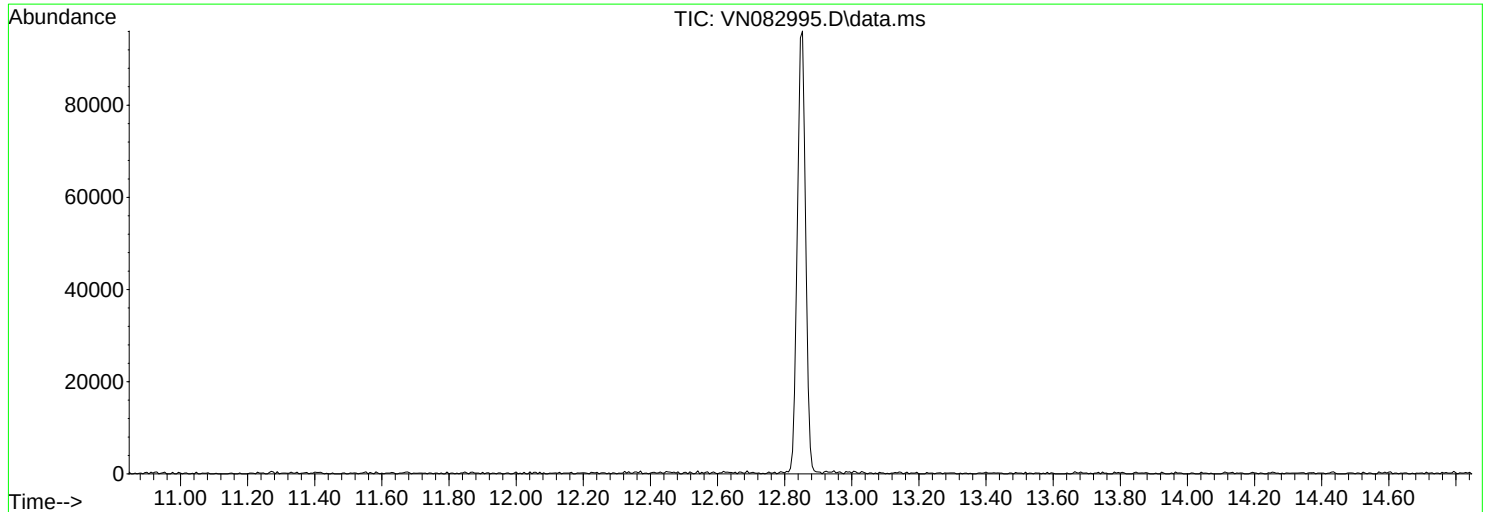

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.8	3868	PASS
75	95	30	60	56.8	8875	PASS
95	95	100	100	100.0	15612	PASS
96	95	5	9	8.3	1294	PASS
173	174	0.00	2	0.7	94	PASS
174	95	50	100	83.9	13104	PASS
175	174	5	9	7.5	983	PASS
176	174	95	101	95.9	12563	PASS
177	176	5	9	8.2	1028	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	253	50.95	1151	68.95	1977	80.90	1124
36.95	1155	56.00	414	69.80	53	81.95	161
38.00	1149	56.95	556	71.80	82	86.95	92
39.05	467	59.95	233	72.90	1009	87.70	20
40.10	53	60.95	971	74.00	3414	87.95	386
43.95	338	61.90	666	75.00	8875	90.90	63
44.90	159	62.10	426	76.00	813	92.00	774
47.00	134	63.05	950	77.00	56	92.95	963
47.80	61	63.95	204	77.80	63	94.00	2224
48.95	940	64.95	278	78.85	1051	95.00	15612
50.00	3868	67.95	1751	79.95	216	96.00	1294

Average of 12.841 to 12.853 min.: VN082995.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.90	62	175.00	983				
118.90	65	176.00	12563				
129.80	65	176.90	1028				
140.75	189						
141.00	95						
142.90	376						
144.80	126						
171.95	157						
172.60	90						
173.10	94						
174.00	13104						

Instrument :

MSVOA_N

ClientSampleId :

BFB