

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN072321\  
 Data File : VN067880.D  
 Acq On : 23 Jul 2021 15:15  
 Operator : JC/MD  
 Sample : M3147-01  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Quant Time: Jul 24 01:42:08 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N070721W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Jul 07 16:18:53 2021  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response            | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|---------------------|-----------|--------|----------|
| -----                         |                |      |                     |           |        |          |
| Internal Standards            |                |      |                     |           |        |          |
| 1) Pentafluorobenzene         | 8.088          | 168  | 283299              | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 8.971          | 114  | 542274              | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.747         | 117  | 533183              | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.678         | 152  | 189259              | 50.000    | ug/l   | 0.00     |
|                               |                |      |                     |           |        |          |
| System Monitoring Compounds   |                |      |                     |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.440          | 65   | 224653              | 52.470    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 61 - 141 |      | Recovery = 104.940% |           |        |          |
| 35) Dibromofluoromethane      | 8.024          | 113  | 166513              | 50.824    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 69 - 133 |      | Recovery = 101.640% |           |        |          |
| 50) Toluene-d8                | 10.443         | 98   | 699053              | 50.975    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 126 |      | Recovery = 101.940% |           |        |          |
| 62) 4-Bromofluorobenzene      | 12.734         | 95   | 231994              | 47.889    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 58 - 135 |      | Recovery = 95.780%  |           |        |          |
|                               |                |      |                     |           |        |          |
| Target Compounds              |                |      |                     |           | Qvalue |          |
| 3) Chloromethane              | 2.306          | 50   | 1179                | 0.309     | ug/l   | 94       |
| 5) Bromomethane               | 2.845          | 94   | 175                 | Below Cal | #      | 4        |
| 6) Chloroethane               | 2.993          | 64   | 108                 | Below Cal | #      | 44       |
| 13) Acrolein                  | 4.052          | 56   | 255                 | Below Cal | #      | 46       |
| 16) Acetone                   | 4.291          | 43   | 1784                | 1.324     | ug/l # | 77       |
| 18) Methyl Acetate            | 4.870          | 43   | 1900                | 0.502     | ug/l # | 61       |
| 20) Methylene Chloride        | 5.093          | 84   | 362                 | Below Cal | #      | 47       |
| 27) cis-1,2-Dichloroethene    | 7.332          | 96   | 14091               | 3.781     | ug/l   | 76       |
| 31) Cyclohexane               | 8.086          | 56   | 7752                | 1.291     | ug/l # | 20       |
| 36) 1,1-Dichloropropene       | 8.086          | 75   | 26620               | 5.285     | ug/l # | 46       |
| 38) Carbon Tetrachloride      | 8.088          | 117  | 31897               | 6.420     | ug/l # | 17       |
| 43) Isopropyl Acetate         | 8.652          | 43   | 3351                | 0.390     | ug/l # | 58       |
| 44) Trichloroethene           | 9.217          | 130  | 10741               | 2.807     | ug/l   | 79       |
| 53) t-1,3-Dichloropropene     | 10.446         | 75   | 57                  | 1.753     | ug/l # | 51       |
| 55) 1,1,2-Trichloroethane     | 10.977         | 97   | 2089                | 0.552     | ug/l # | 34       |
| 60) Dibromochloromethane      | 10.980         | 129  | 200567              | 43.496    | ug/l # | 11       |
| 64) Tetrachloroethene         | 10.980         | 164  | 199572              | 53.026    | ug/l   | 97       |
| 71) Bromoform                 | 12.712         | 173  | 62                  | 3.193     | ug/l # | 29       |
| 76) 1,2,3-Trichloropropane    | 12.734         | 75   | 130341              | 33.723    | ug/l # | 100      |
| 81) trans-1,4-Dichloro-2-b... | 12.734         | 75   | 130341              | 108.727   | ug/l # | 6        |
| 85) sec-Butylbenzene          | 13.503         | 105  | 13066               | 0.895     | ug/l   | 94       |
| 90) Hexachloroethane          | 14.209         | 117  | 878                 | 0.449     | ug/l # | 36       |
| 93) 1,2,4-Trichlorobenzene    | 15.265         | 180  | 874                 | 2.937     | ug/l # | 82       |
| 95) Naphthalene               | 15.509         | 128  | 1649                | 3.179     | ug/l # | 79       |
| 96) 1,2,3-Trichlorobenzene    | 15.702         | 180  | 286                 | 2.722     | ug/l # | 70       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN072321\  
Data File : VN067880.D  
Acq On : 23 Jul 2021 15:15  
Operator : JC/MD  
Sample : M3147-01  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :

Quant Time: Jul 24 01:42:08 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N070721W.M  
Quant Title : SW846 8260  
QLast Update : Wed Jul 07 16:18:53 2021  
Response via : Initial Calibration




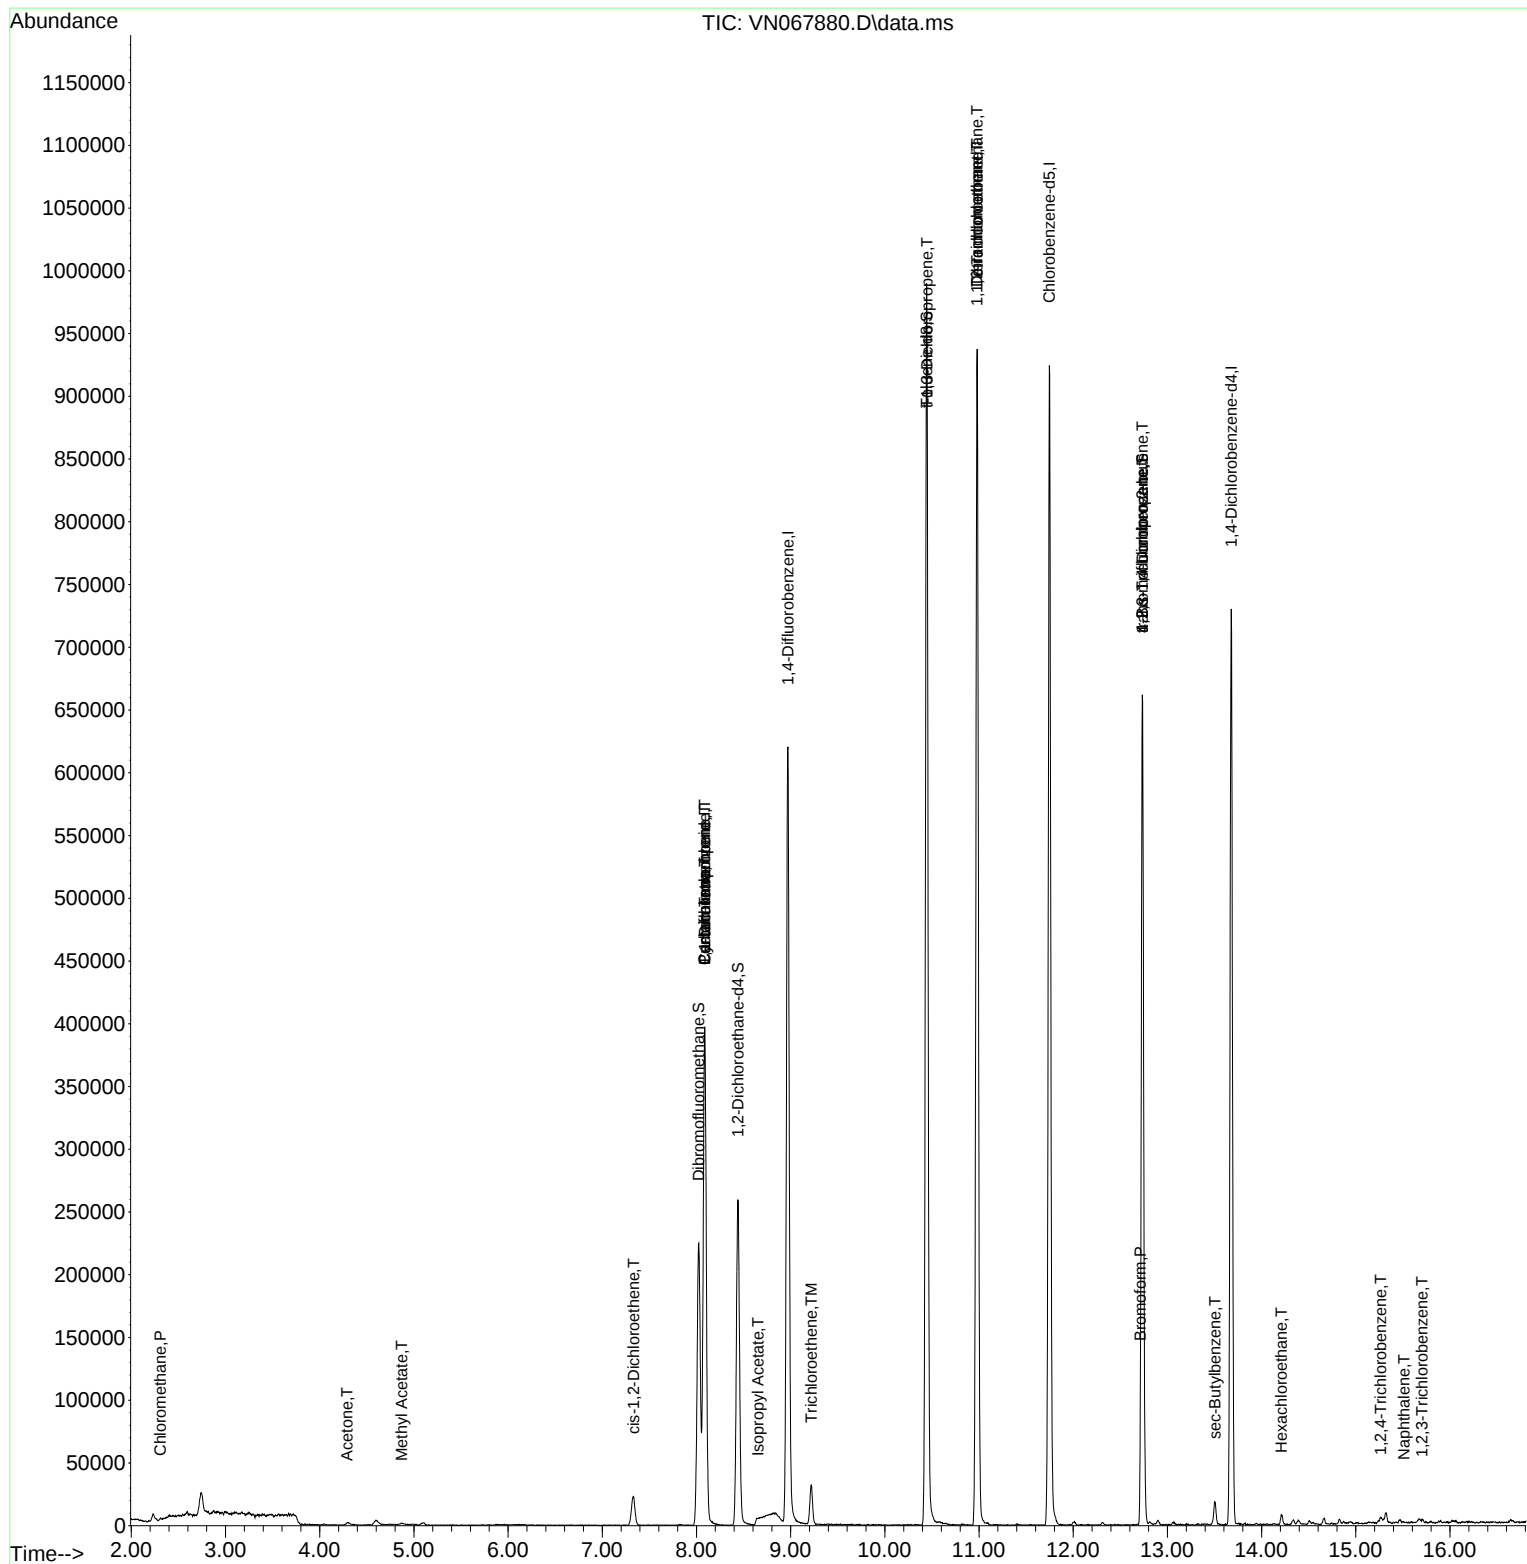




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.088 min Scan# 2274  
Delta R.T. 0.002 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion:168 Resp: 283299  
Ion Ratio Lower Upper  
168 100  
99 64.4 62.9 94.3

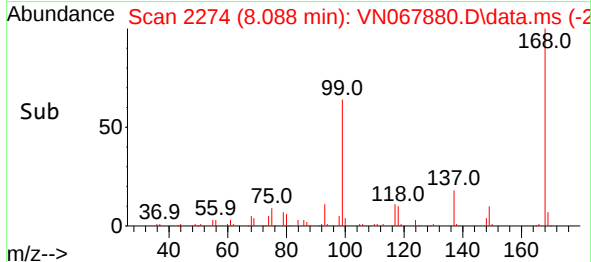

#3  
Chloromethane  
Concen: 0.309 ug/l  
RT: 2.306 min Scan# 118  
Delta R.T. 0.005 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15


Tgt Ion: 50 Resp: 1179  
Ion Ratio Lower Upper  
50 100  
52 35.3 25.6 38.4

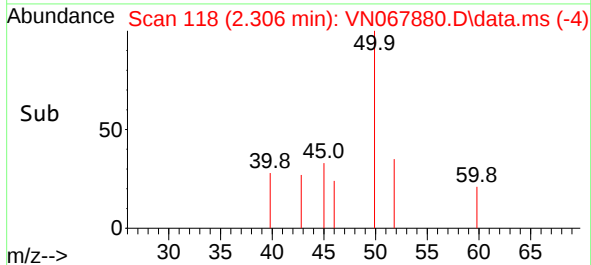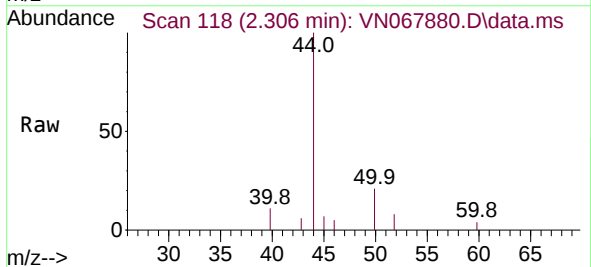



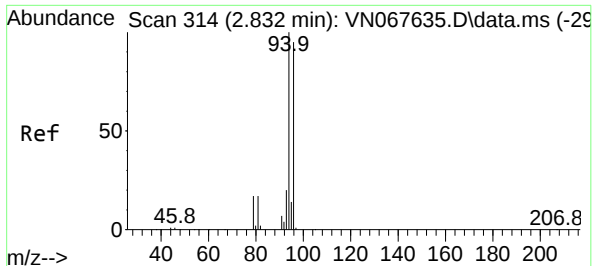


#5  
Bromomethane  
Concen: Below Cal  
RT: 2.845 min Scan# 319  
Delta R.T. 0.013 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Instrument :  
MSVOA\_N  
ClientSampled :



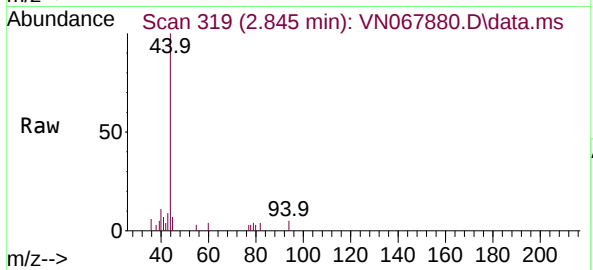



Tgt Ion: 94 Resp: 175  
Ion Ratio Lower Upper  
94 100  
96 0.0 73.7 110.5#

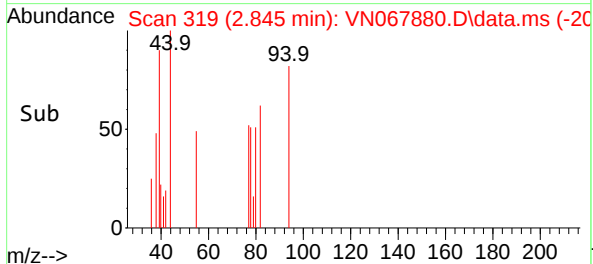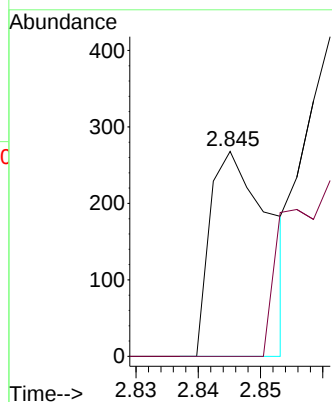

#6  
Chloroethane  
Concen: Below Cal  
RT: 2.993 min Scan# 374  
Delta R.T. -0.013 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Tgt Ion: 64 Resp: 108  
Ion Ratio Lower Upper  
64 100  
66 0.0 24.7 37.1#


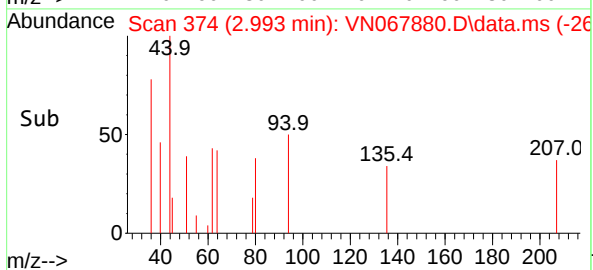
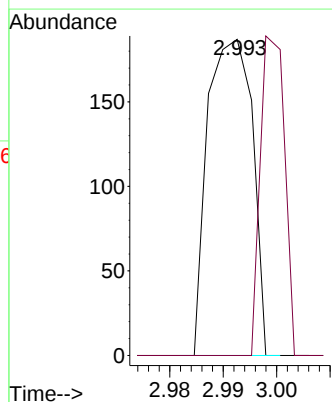
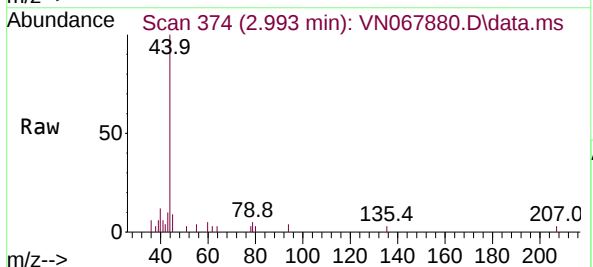


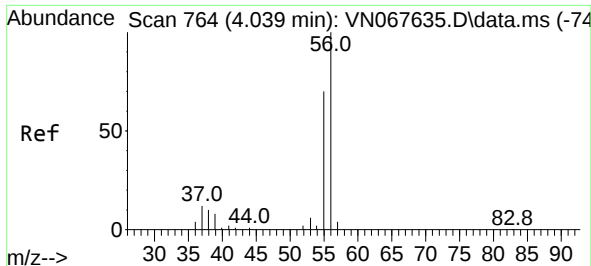

#13  
Acrolein  
Concen: Below Cal  
RT: 4.052 min Scan# 769  
Delta R.T. 0.013 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 56 Resp: 255  
Ion Ratio Lower Upper  
56 100  
55 116.9 57.4 86.0#

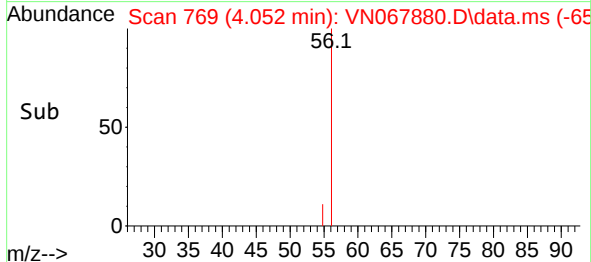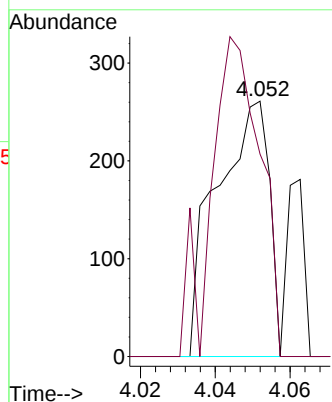

#16  
Acetone  
Concen: 1.324 ug/l  
RT: 4.291 min Scan# 858  
Delta R.T. 0.003 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Tgt Ion: 43 Resp: 1784  
Ion Ratio Lower Upper  
43 100  
58 14.6 21.2 31.8#


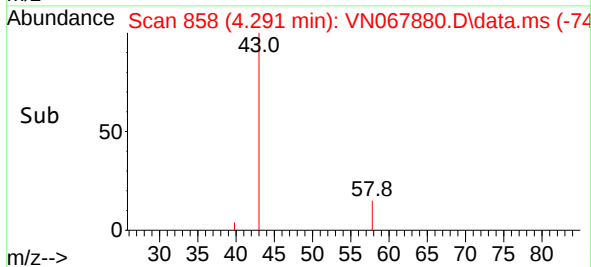
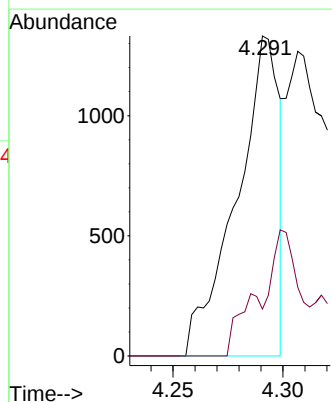
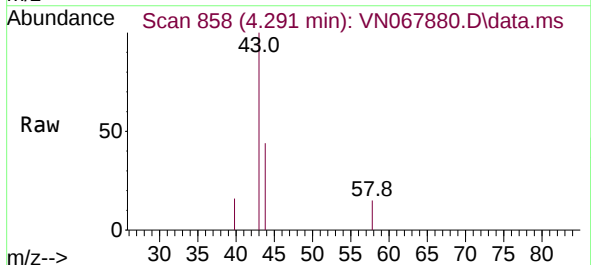




#18  
Methyl Acetate  
Concen: 0.502 ug/l  
RT: 4.870 min Scan# 1074  
Delta R.T. 0.013 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 43 Resp: 1900  
Ion Ratio Lower Upper  
43 100  
74 3.3 17.4 26.0#

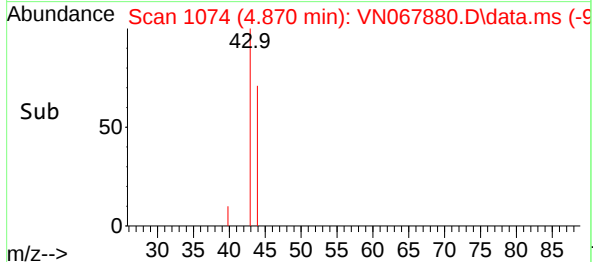

#20  
Methylene Chloride  
Concen: Below Cal  
RT: 5.093 min Scan# 1157  
Delta R.T. 0.003 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Tgt Ion: 84 Resp: 362  
Ion Ratio Lower Upper  
84 100  
49 43.8 110.9 166.3#  
51 65.7 32.6 49.0#  
86 68.6 51.6 77.4


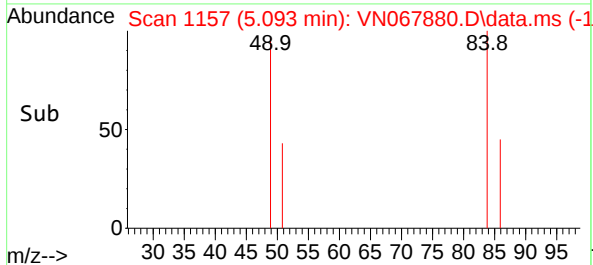

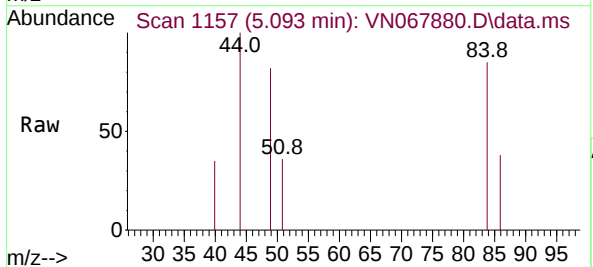




#27  
 cis-1,2-Dichloroethene  
 Concen: 3.781 ug/l  
 RT: 7.332 min Scan# 1992  
 Delta R.T. 0.008 min  
 Lab File: VN067880.D  
 Acq: 23 Jul 2021 15:15




Instrument :  
 MSVOA\_N  
 ClientSampled :


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 96    | Resp: | 14091 |
| Ion      | Ratio | Lower | Upper |
| 96       | 100   |       |       |
| 61       | 125.2 | 0.0   | 338.8 |
| 98       | 64.3  | 0.0   | 129.8 |

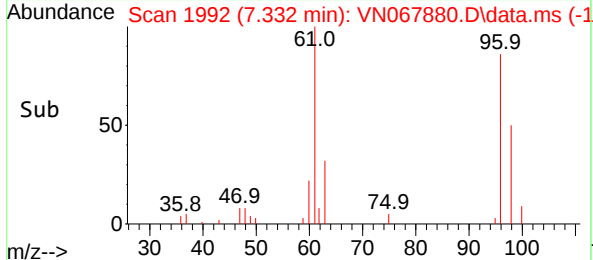

#31  
 Cyclohexane  
 Concen: 1.291 ug/l  
 RT: 8.086 min Scan# 2273  
 Delta R.T. -0.008 min  
 Lab File: VN067880.D  
 Acq: 23 Jul 2021 15:15

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 56    | Resp: | 7752  |
| Ion      | Ratio | Lower | Upper |
| 56       | 100   |       |       |
| 69       | 152.0 | 27.3  | 40.9# |
| 84       | 105.4 | 64.9  | 97.3# |


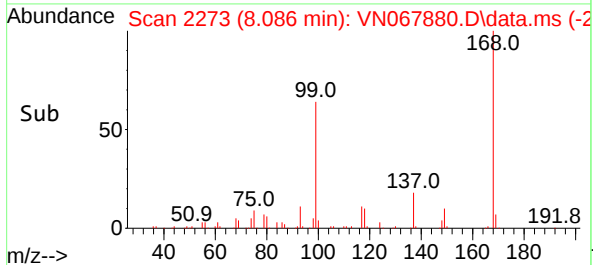

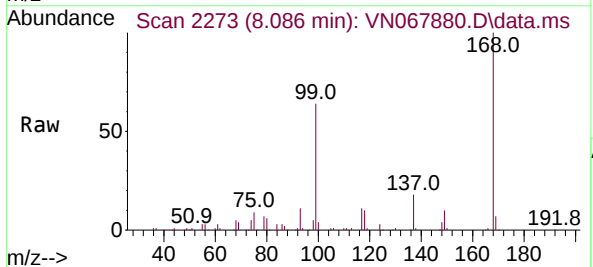




#33  
 1,2-Dichloroethane-d4  
 Concen: 52.470 ug/l  
 RT: 8.440 min Scan# 2405  
 Delta R.T. -0.000 min  
 Lab File: VN067880.D  
 Acq: 23 Jul 2021 15:15




Instrument :  
 MSVOA\_N  
 ClientSampled :


Tgt Ion: 65 Resp: 224653  
 Ion Ratio Lower Upper  
 65 100  
 67 50.4 0.0 98.6

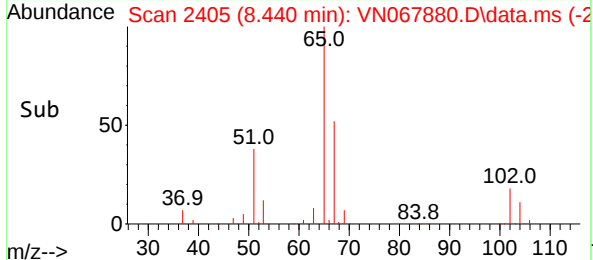

#34  
 1,4-Difluorobenzene  
 Concen: 50.000 ug/l  
 RT: 8.971 min Scan# 2603  
 Delta R.T. 0.003 min  
 Lab File: VN067880.D  
 Acq: 23 Jul 2021 15:15

Tgt Ion: 114 Resp: 542274  
 Ion Ratio Lower Upper  
 114 100  
 63 21.0 0.0 49.0  
 88 15.1 0.0 36.6


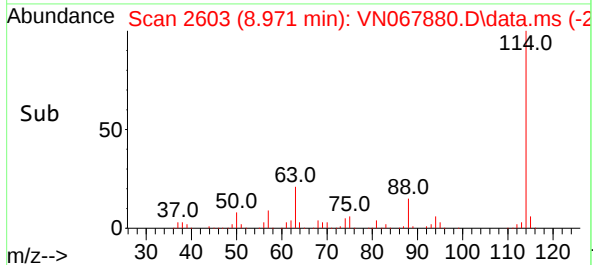

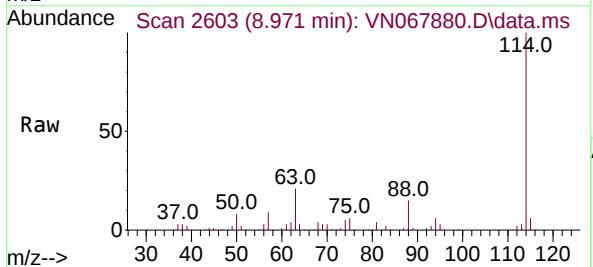




#35  
Dibromofluoromethane  
Concen: 50.824 ug/l  
RT: 8.024 min Scan# 2250  
Delta R.T. 0.003 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:113 Resp: 166513  
Ion Ratio Lower Upper  
113 100  
111 102.7 83.8 125.8  
192 15.3 13.4 20.0

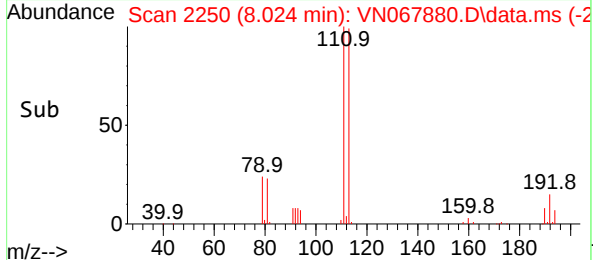

#36  
1,1-Dichloropropene  
Concen: 5.285 ug/l  
RT: 8.086 min Scan# 2273  
Delta R.T. -0.136 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15


Tgt Ion: 75 Resp: 26620  
Ion Ratio Lower Upper  
75 100  
110 3.2 15.7 47.0#  
77 0.0 24.6 37.0#

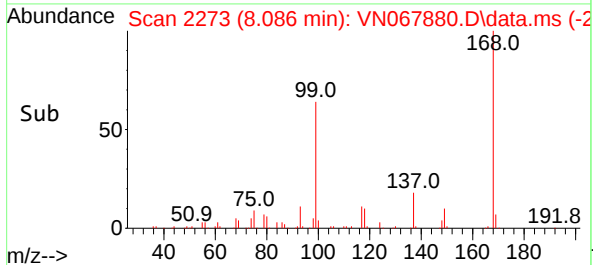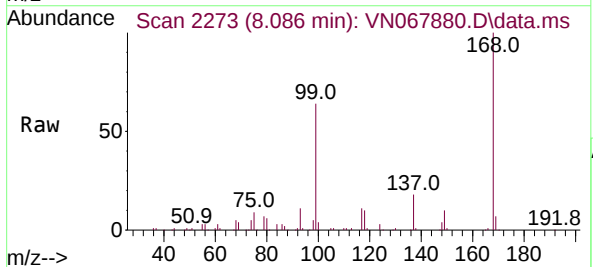



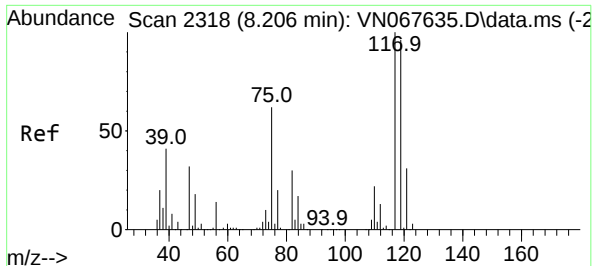


#38  
Carbon Tetrachloride  
Concen: 6.420 ug/l  
RT: 8.088 min Scan# 2274  
Delta R.T. -0.118 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Instrument :  
MSVOA\_N  
ClientSampleId :



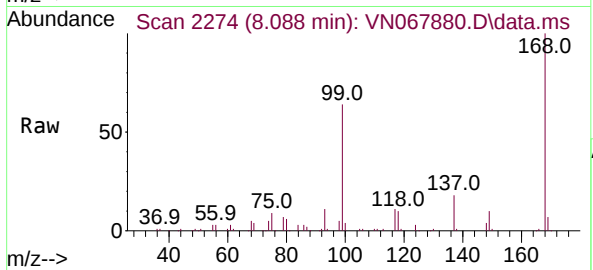



Tgt Ion:117 Resp: 31897  
Ion Ratio Lower Upper  
117 100  
119 5.7 75.4 113.2#  
121 0.0 23.5 35.3#

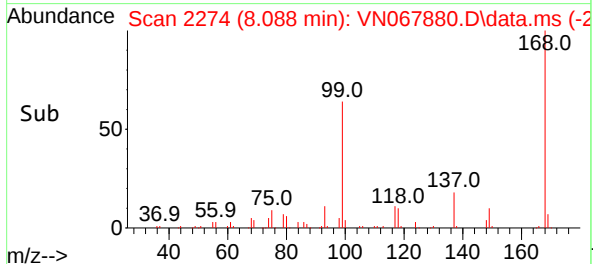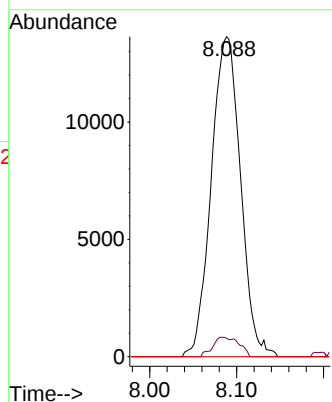

#43  
Isopropyl Acetate  
Concen: 0.390 ug/l  
RT: 8.652 min Scan# 2484  
Delta R.T. 0.089 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Tgt Ion: 43 Resp: 3351  
Ion Ratio Lower Upper  
43 100  
61 0.0 19.0 28.4#  
87 0.0 9.5 14.3#


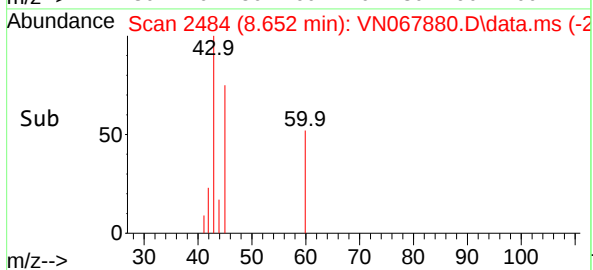
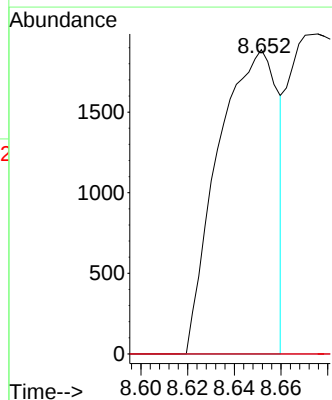
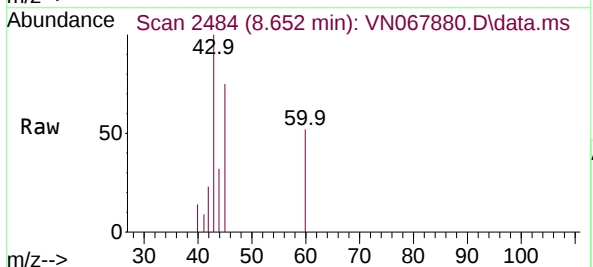


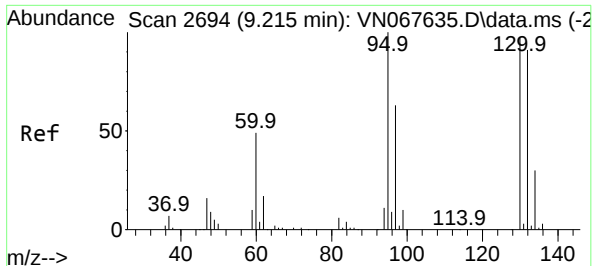

#44  
Trichloroethene  
Concen: 2.807 ug/l  
RT: 9.217 min Scan# 2695  
Delta R.T. 0.002 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:130 Resp: 10741  
Ion Ratio Lower Upper  
130 100  
95 94.5 0.0 234.4

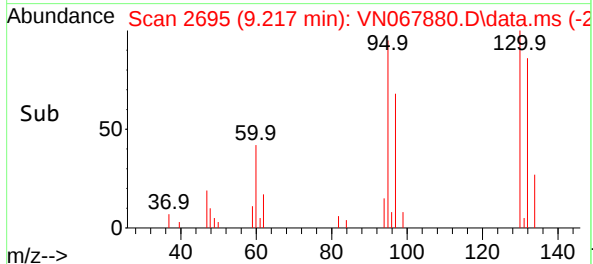

#50  
Toluene-d8  
Concen: 50.975 ug/l  
RT: 10.443 min Scan# 3152  
Delta R.T. 0.000 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Tgt Ion: 98 Resp: 699053  
Ion Ratio Lower Upper  
98 100  
100 63.2 51.7 77.5




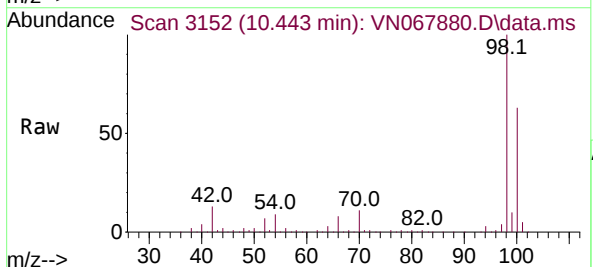


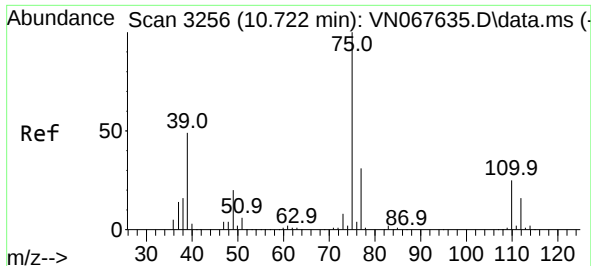

#53  
t-1,3-Dichloropropene  
Concen: 1.753 ug/l  
RT: 10.446 min Scan# 3153  
Delta R.T. -0.276 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 75 Resp: 57  
Ion Ratio Lower Upper  
75 100  
77 58.5 25.1 37.7#

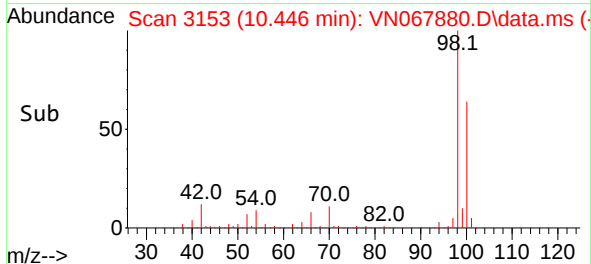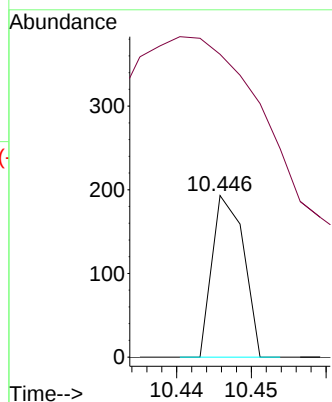

#55  
1,1,2-Trichloroethane  
Concen: 0.552 ug/l  
RT: 10.977 min Scan# 3351  
Delta R.T. 0.075 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Tgt Ion: 97 Resp: 2089  
Ion Ratio Lower Upper  
97 100  
83 179.7 72.0 108.0#  
85 36.7 46.8 70.2#  
99 17.5 49.8 74.6#


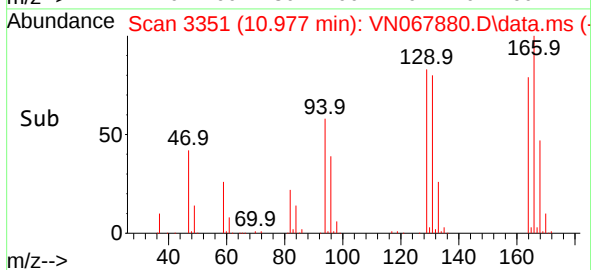
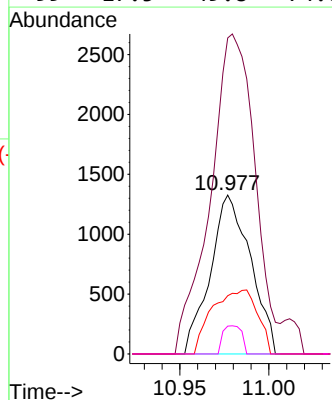
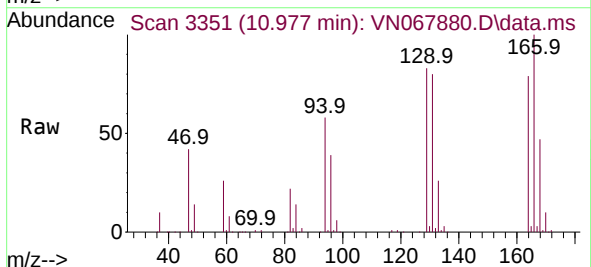


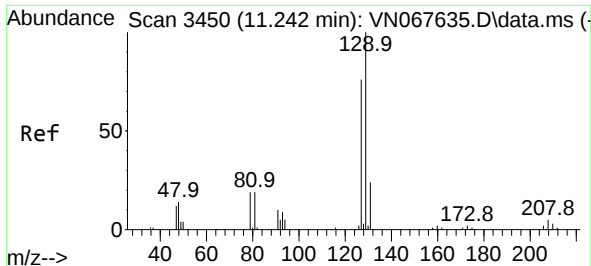

#60  
Dibromochloromethane  
Concen: 43.496 ug/l  
RT: 10.980 min Scan# 3352  
Delta R.T. -0.262 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:129 Resp: 200567  
Ion Ratio Lower Upper  
129 100  
127 0.0 38.6 115.8#

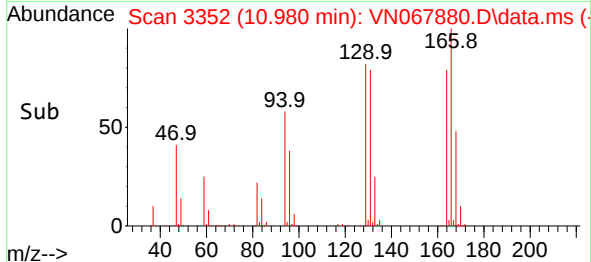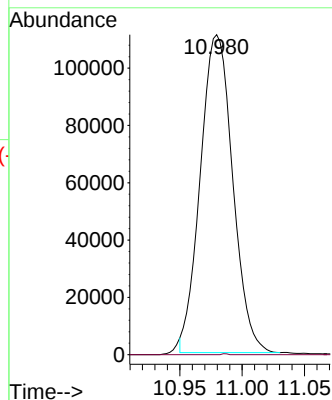

#62  
4-Bromofluorobenzene  
Concen: 47.889 ug/l  
RT: 12.734 min Scan# 4006  
Delta R.T. 0.001 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Tgt Ion: 95 Resp: 231994  
Ion Ratio Lower Upper  
95 100  
174 71.0 0.0 122.0  
176 67.9 0.0 117.6


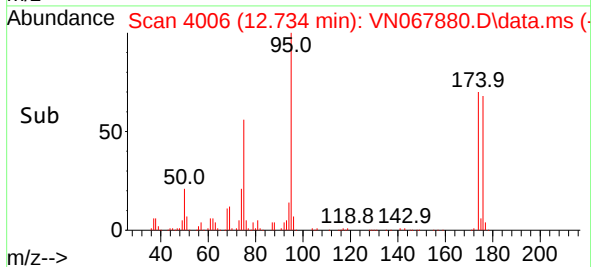
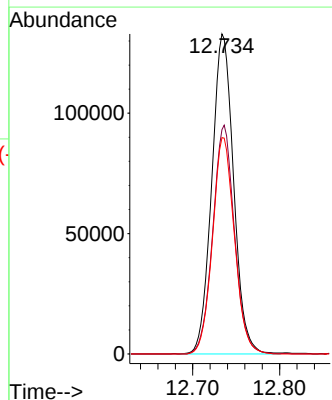
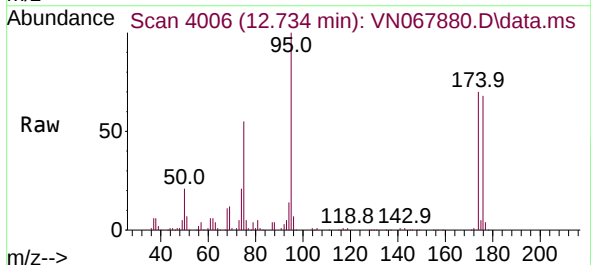




#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.747 min Scan# 3638  
Delta R.T. 0.000 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:117 Resp: 533183  
Ion Ratio Lower Upper  
117 100  
82 58.3 53.1 79.7  
119 32.9 25.5 38.3

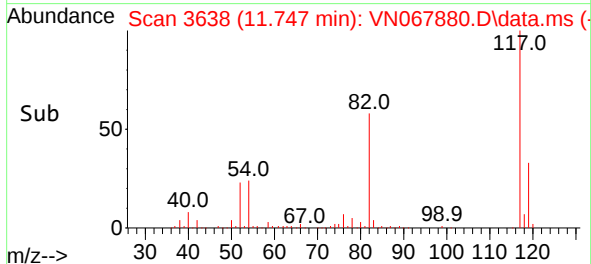

#64  
Tetrachloroethene  
Concen: 53.026 ug/l  
RT: 10.980 min Scan# 3352  
Delta R.T. 0.001 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15


Tgt Ion:164 Resp: 199572  
Ion Ratio Lower Upper  
164 100  
166 127.1 102.1 153.1  
129 104.5 86.9 130.3  
131 100.1 83.6 125.4

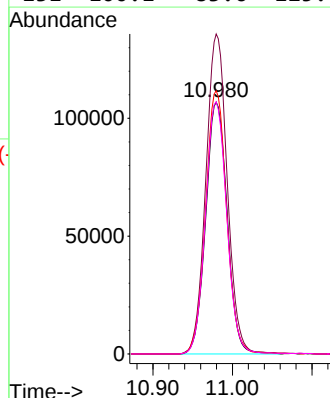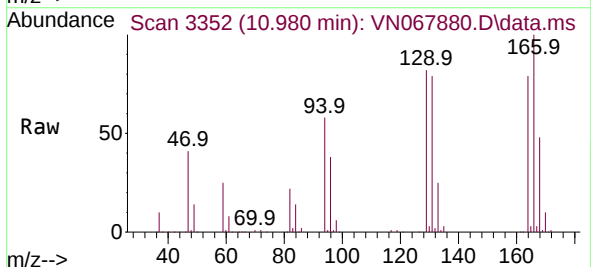



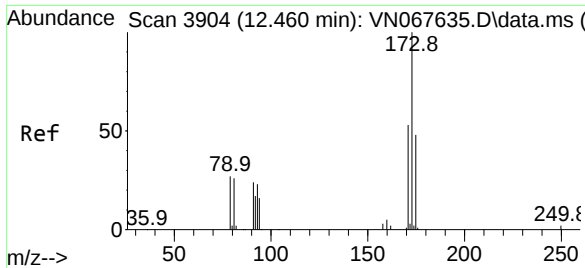


#71  
Bromoform  
Concen: 3.193 ug/l  
RT: 12.712 min Scan# 3998  
Delta R.T. 0.252 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15


Instrument :  
MSVOA\_N  
ClientSampled :

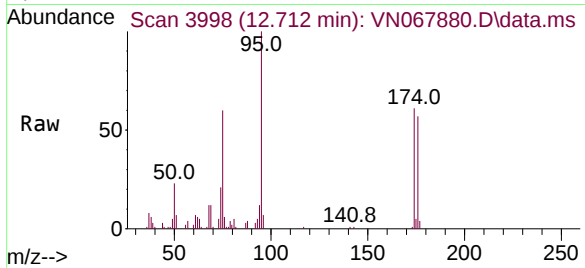



Tgt Ion:173 Resp: 62  
Ion Ratio Lower Upper  
173 100  
175 0.0 23.9 71.8#  
254 0.0 0.0 0.0

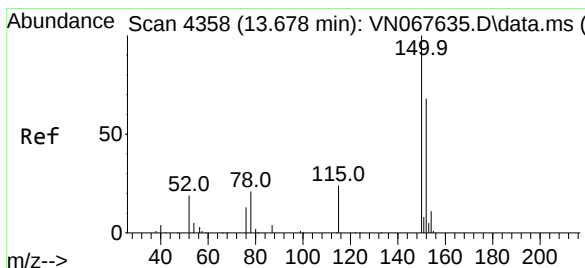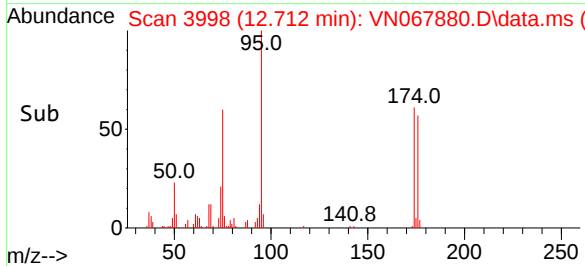


#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.678 min Scan# 4358  
Delta R.T. 0.000 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

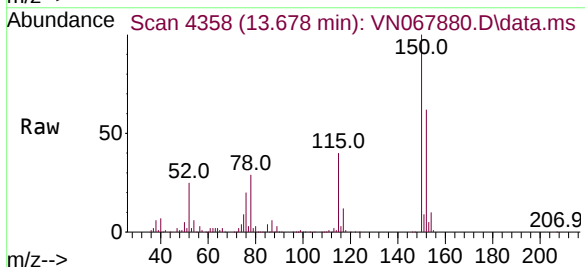

Tgt Ion:152 Resp: 189259  
Ion Ratio Lower Upper  
152 100  
115 63.4 36.1 108.5  
150 159.5 0.0 351.8



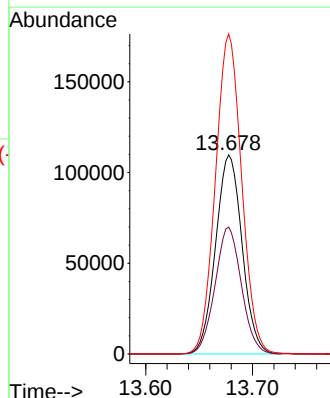
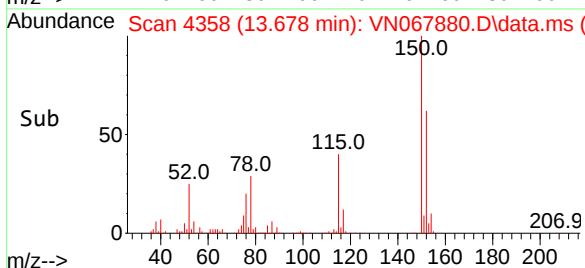


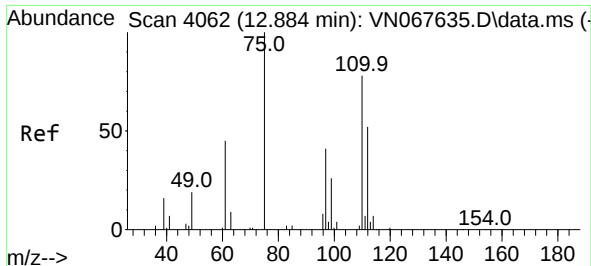

#76  
1,2,3-Trichloropropane  
Concen: 33.723 ug/l  
RT: 12.734 min Scan# 4006  
Delta R.T. -0.150 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 75 Resp: 130341  
Ion Ratio Lower Upper  
75 100  
77 1.1 0.0 0.0#

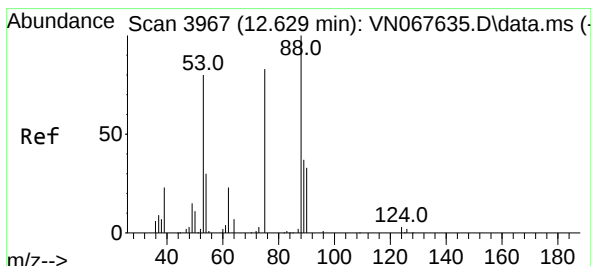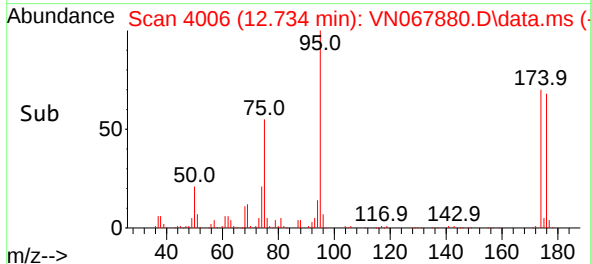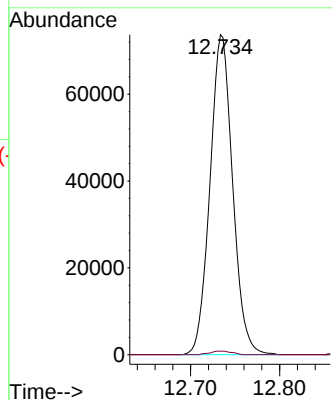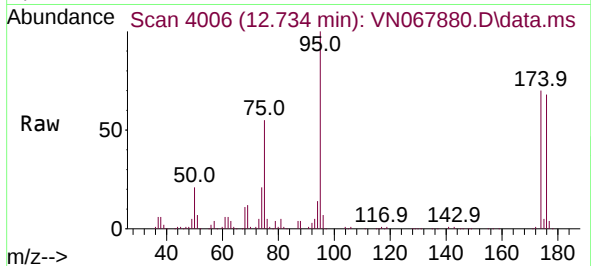

#81  
trans-1,4-Dichloro-2-butene  
Concen: 108.727 ug/l  
RT: 12.734 min Scan# 4006  
Delta R.T. 0.105 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

Tgt Ion: 75 Resp: 130341  
Ion Ratio Lower Upper  
75 100  
53 0.0 87.6 131.4#  
89 0.0 37.8 56.8#


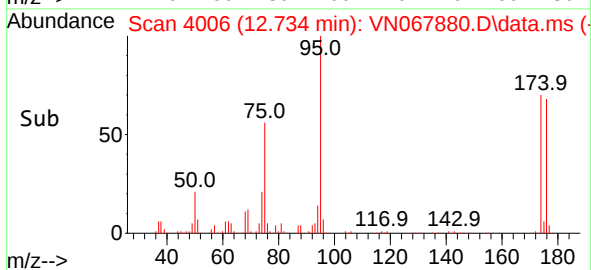
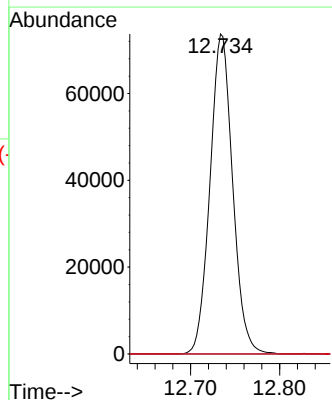
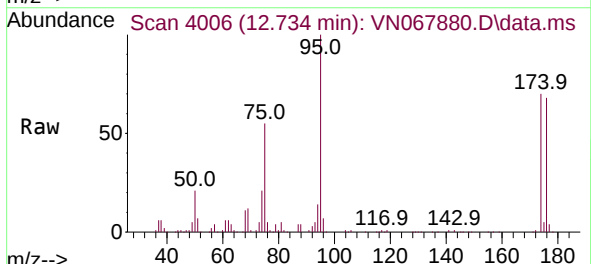


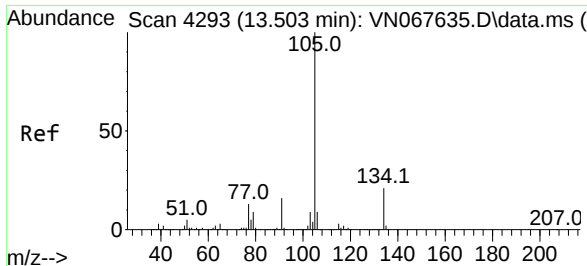

#85  
 sec-Butylbenzene  
 Concen: 0.895 ug/l  
 RT: 13.503 min Scan# 4293  
 Delta R.T. 0.000 min  
 Lab File: VN067880.D  
 Acq: 23 Jul 2021 15:15




Instrument :  
 MSVOA\_N  
 ClientSampled :


Tgt Ion:105 Resp: 13066  
 Ion Ratio Lower Upper  
 105 100  
 134 21.0 9.0 27.1

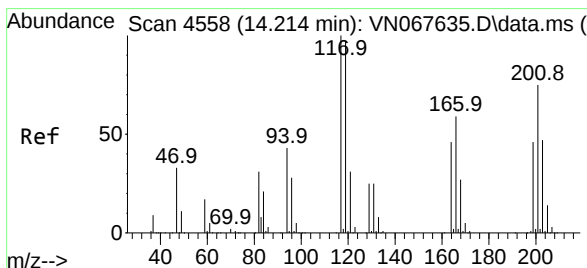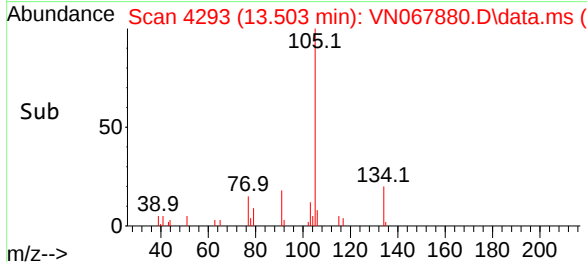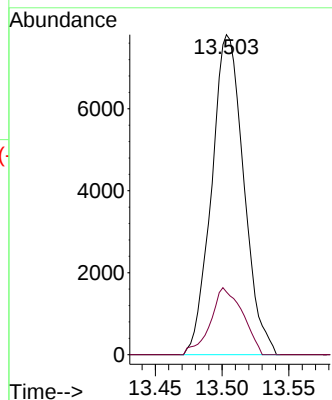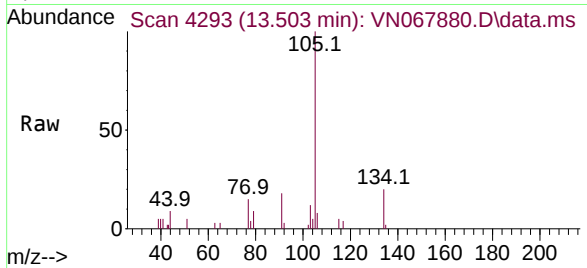

#90  
 Hexachloroethane  
 Concen: 0.449 ug/l  
 RT: 14.209 min Scan# 4556  
 Delta R.T. -0.005 min  
 Lab File: VN067880.D  
 Acq: 23 Jul 2021 15:15


Tgt Ion:117 Resp: 878  
 Ion Ratio Lower Upper  
 117 100  
 201 15.7 33.5 100.5#

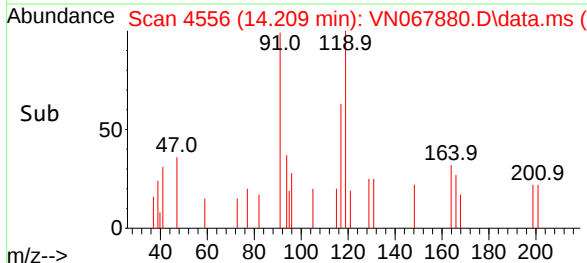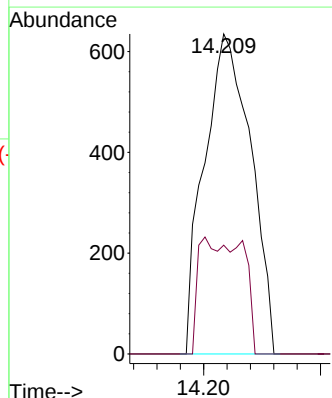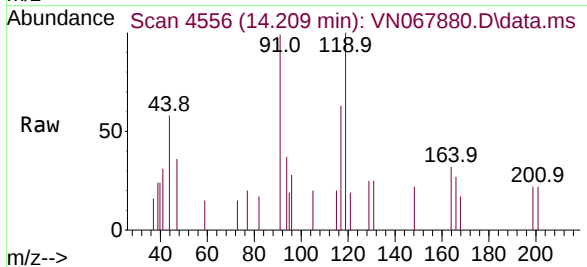



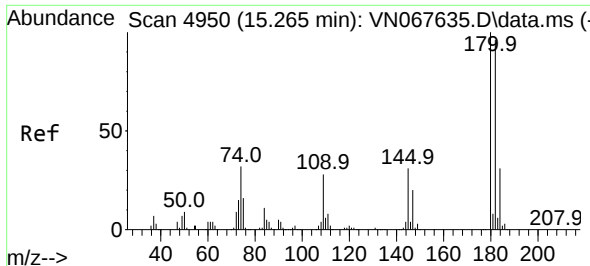


#93  
1,2,4-Trichlorobenzene  
Concen: 2.937 ug/l  
RT: 15.265 min Scan# 4950  
Delta R.T. 0.000 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15


Instrument :  
MSVOA\_N  
ClientSampled :

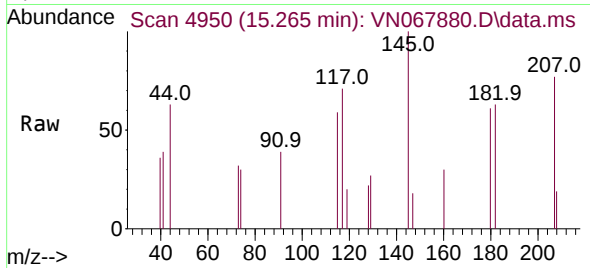



Tgt Ion:180 Resp: 874  
Ion Ratio Lower Upper  
180 100  
182 92.4 47.5 142.5  
145 0.0 17.2 51.6#

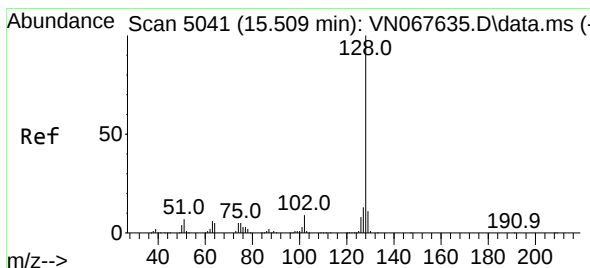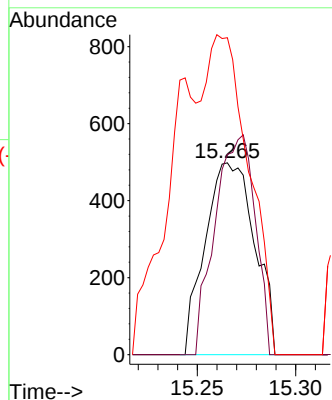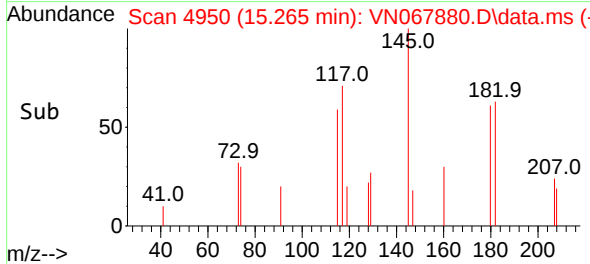


#95  
Naphthalene  
Concen: 3.179 ug/l  
RT: 15.509 min Scan# 5041  
Delta R.T. 0.000 min  
Lab File: VN067880.D  
Acq: 23 Jul 2021 15:15

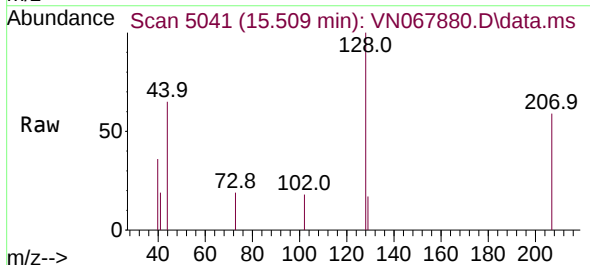


Tgt Ion:128 Resp: 1649  
Ion Ratio Lower Upper  
128 100  
127 0.0 10.6 15.8#  
129 8.5 8.6 12.8#

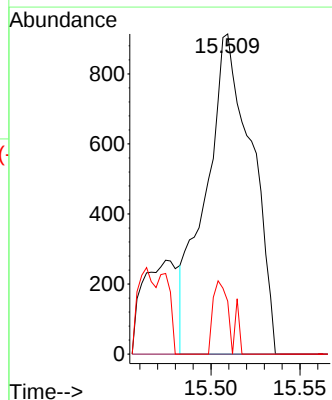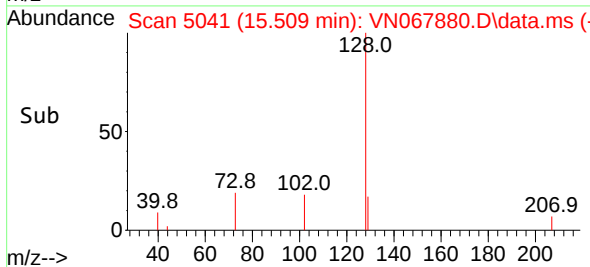

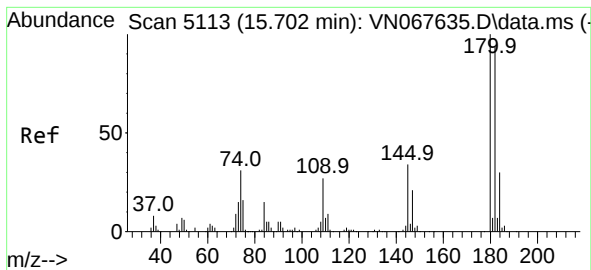

#96  
 1,2,3-Trichlorobenzene  
 Concen: 2.722 ug/l  
 RT: 15.702 min Scan# 5113  
 Delta R.T. 0.000 min  
 Lab File: VN067880.D  
 Acq: 23 Jul 2021 15:15

Instrument :  
 MSVOA\_N  
 ClientSampleId :

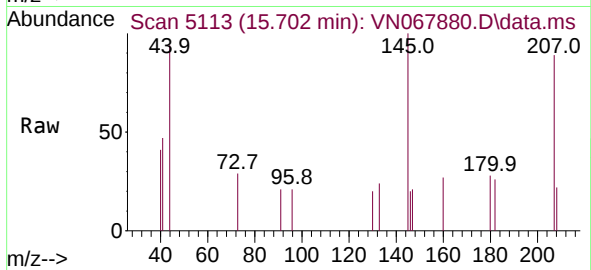

Tgt Ion:180 Resp: 286  
 Ion Ratio Lower Upper  
 180 100  
 182 78.3 47.8 143.3  
 145 0.0 18.2 54.6#

