

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072321\
 Data File : VN067888.D
 Acq On : 23 Jul 2021 18:31
 Operator : JC/MD
 Sample : PB137886TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 24 01:43:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	273452	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	524831	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	555020	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	186456	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	224166	54.242	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 108.480%			
35) Dibromofluoromethane	8.024	113	163152	51.453	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 102.900%			
50) Toluene-d8	10.446	98	698113	52.598	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 105.200%			
62) 4-Bromofluorobenzene	12.733	95	234394	49.992	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 99.980%			
Target Compounds						
					Qvalue	
5) Bromomethane	2.805	94	57	Below Cal	#	4
6) Chloroethane	2.998	64	104	Below Cal	#	44
11) Tert butyl alcohol	5.382	59	386	0.650	ug/l #	71
13) Acrolein	4.041	56	118	Below Cal		91
16) Acetone	4.296	43	49577	38.125	ug/l #	86
18) Methyl Acetate	4.856	43	1841	0.504	ug/l #	76
20) Methylene Chloride	5.095	84	27588	8.510	ug/l	88
25) 2-Butanone	7.356	43	9241	4.280	ug/l	95
29) Tetrahydrofuran	7.694	42	3451	2.430	ug/l #	75
31) Cyclohexane	8.086	56	7642	1.319	ug/l #	14
36) 1,1-Dichloropropene	8.088	75	25156	5.160	ug/l #	54
37) Ethyl Acetate	7.356	43	9241	1.956	ug/l #	69
38) Carbon Tetrachloride	8.091	117	30739	6.392	ug/l #	16
41) Methacrylonitrile	7.699	41	2329	0.959	ug/l #	37
43) Isopropyl Acetate	8.563	43	37906	4.562	ug/l #	90
45) 1,2-Dichloropropane	9.625	63	2555	0.692	ug/l #	44
48) Methyl methacrylate	9.550	41	9244	2.515	ug/l #	12
49) 1,4-Dioxane	9.614	88	84	33.245	ug/l #	20
51) 4-Methyl-2-Pentanone	10.333	43	9810	1.922	ug/l	89
53) t-1,3-Dichloropropene	10.459	75	53	1.753	ug/l #	1
54) cis-1,3-Dichloropropene	10.247	75	65831	11.550	ug/l #	60
57) 1,3-Dichloropropane	11.095	76	42137	6.708	ug/l #	43
59) 2-Hexanone	11.095	43	618336	173.536	ug/l #	54
60) Dibromochloromethane	11.492	129	312	2.423	ug/l #	11
71) Bromoform	12.715	173	78	3.196	ug/l #	1
74) N-amyl acetate	12.361	43	1214	0.222	ug/l #	47
76) 1,2,3-Trichloropropane	12.733	75	130388	34.243	ug/l #	100
80) 1,3,5-Trimethylbenzene	13.063	105	3601	0.295	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.733	75	130388	110.402	ug/l #	6
95) Naphthalene	15.509	128	265	3.040	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072321\
Data File : VN067888.D
Acq On : 23 Jul 2021 18:31
Operator : JC/MD
Sample : PB137886TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 24 01:43:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration




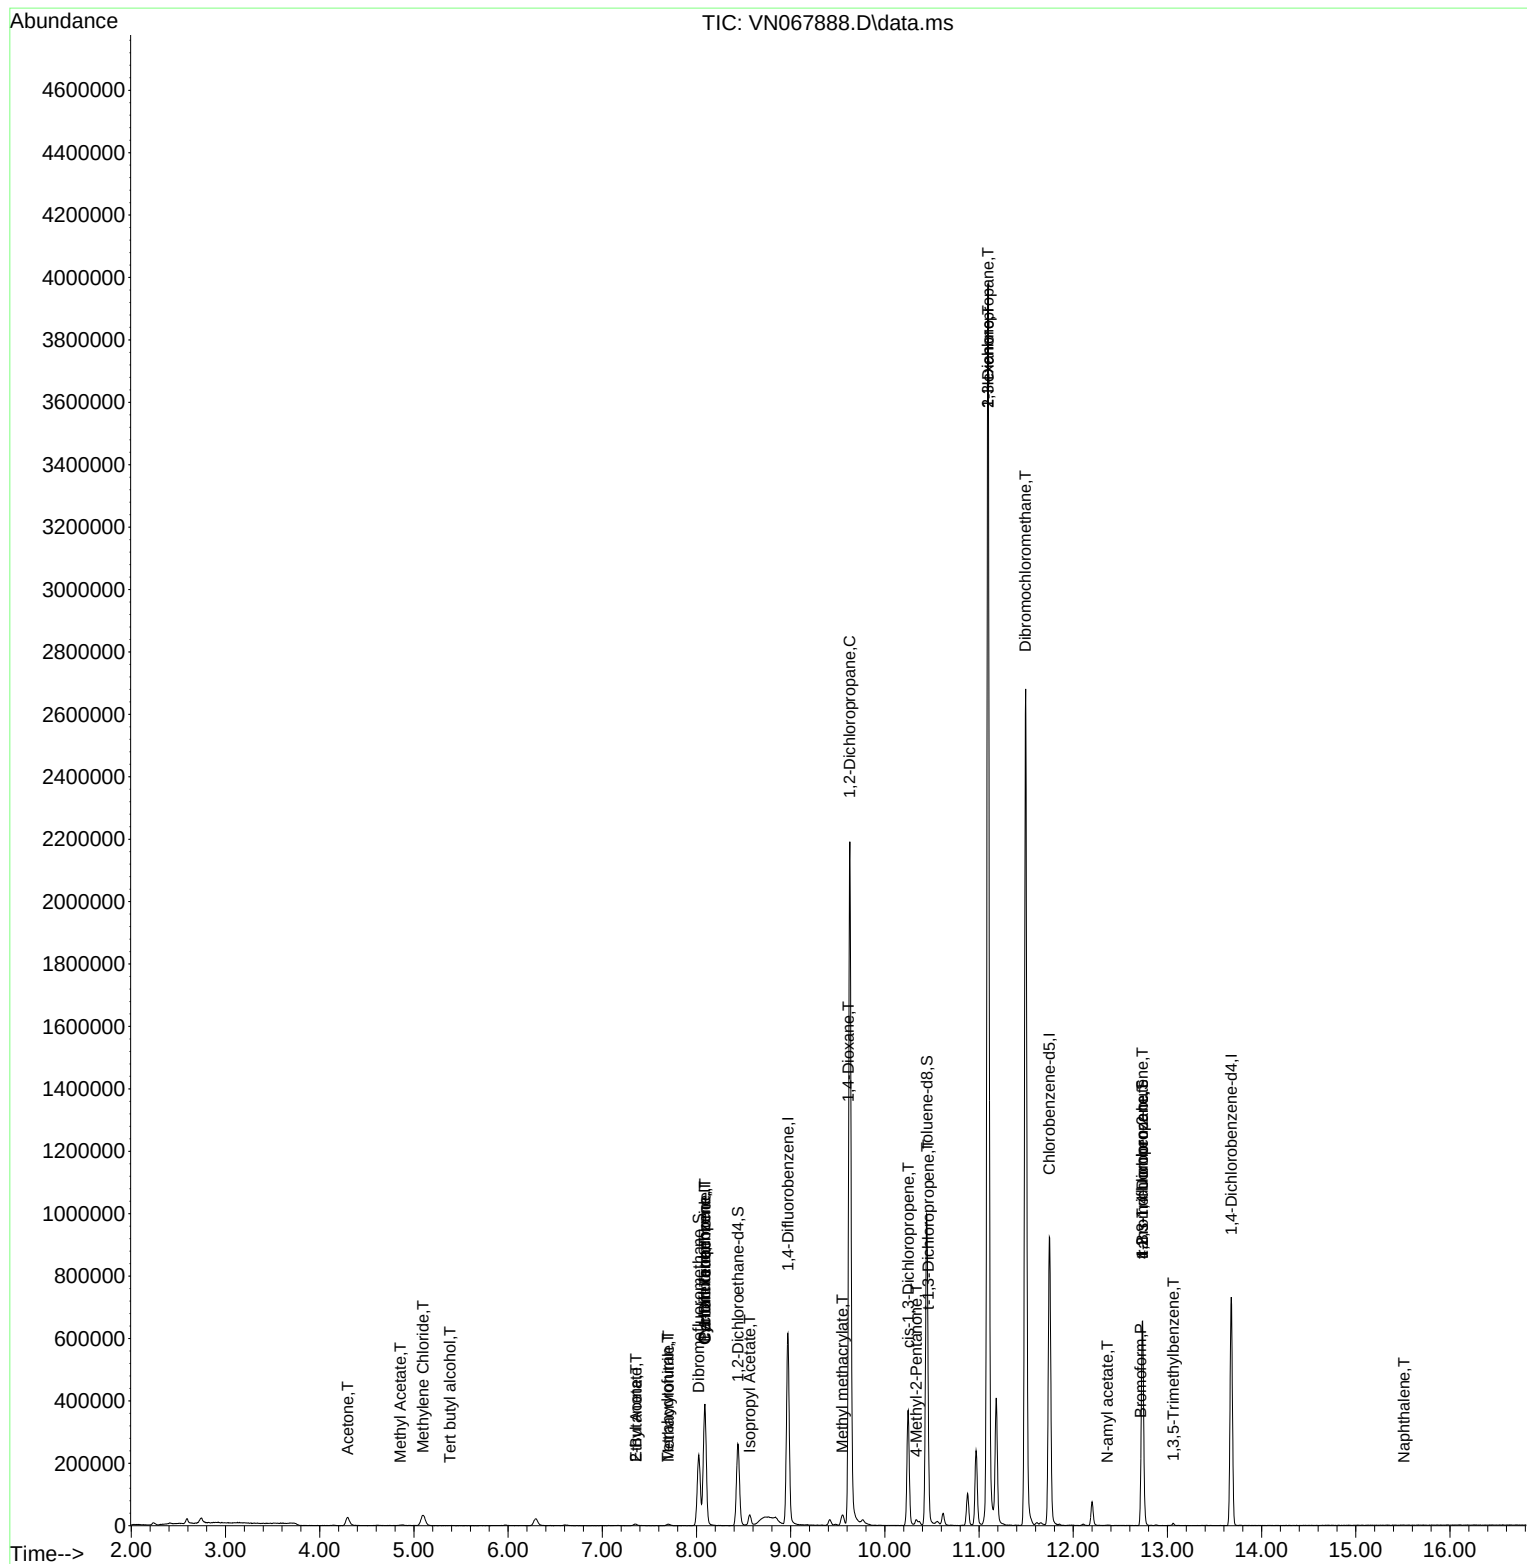




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 273452
Ion Ratio Lower Upper
168 100
99 67.7 62.9 94.3

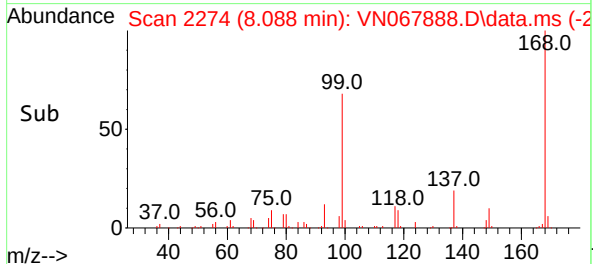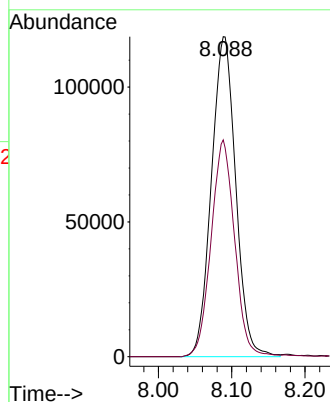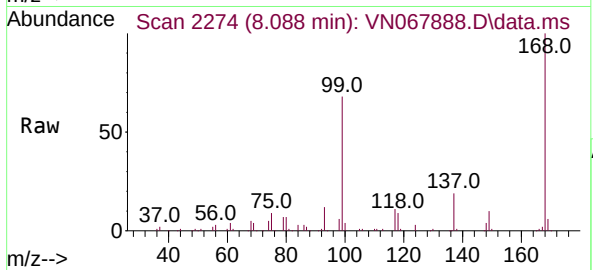

#5
Bromomethane
Concen: Below Cal
RT: 2.805 min Scan# 304
Delta R.T. -0.027 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 94 Resp: 57
Ion Ratio Lower Upper
94 100
96 0.0 73.7 110.5#


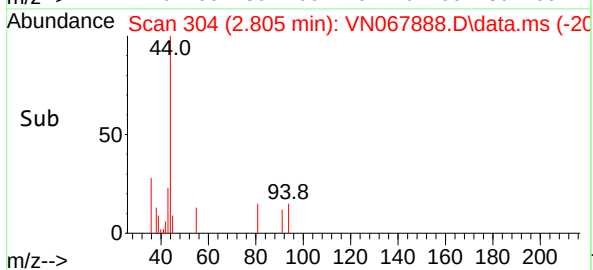
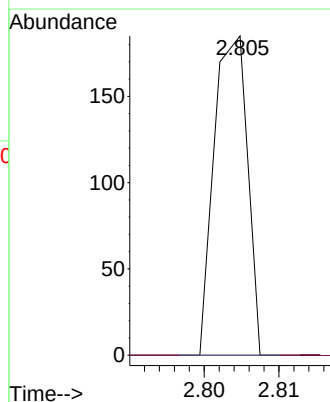
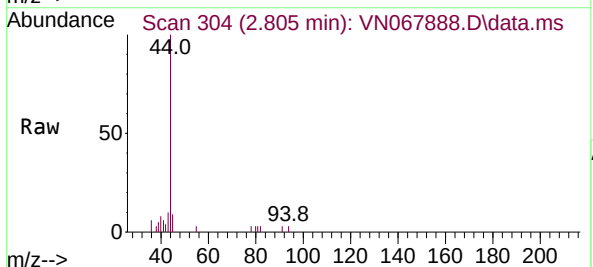


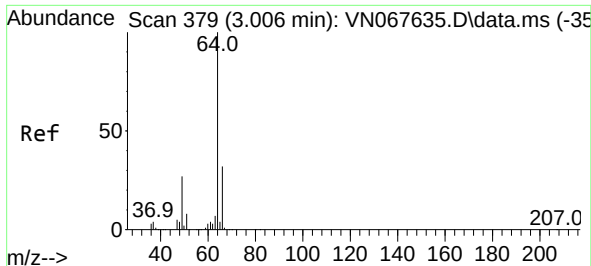

#6
Chloroethane
Concen: Below Cal
RT: 2.998 min Scan# 376
Delta R.T. -0.008 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31



Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 64 Resp: 104
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#

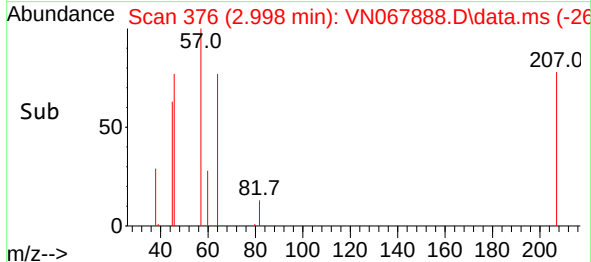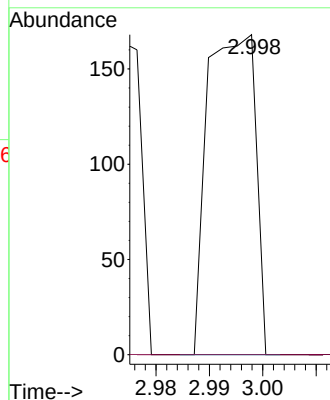

#11
Tert butyl alcohol
Concen: 0.650 ug/l
RT: 5.382 min Scan# 1265
Delta R.T. -0.008 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 59 Resp: 386
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#



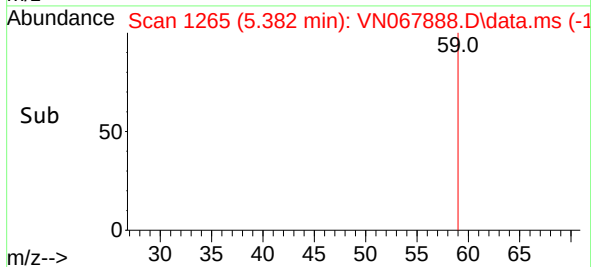
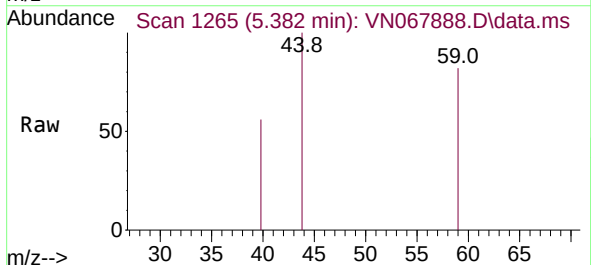


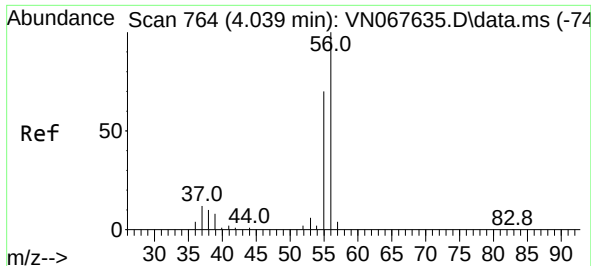

#13
Acrolein
Concen: Below Cal
RT: 4.041 min Scan# 765
Delta R.T. 0.002 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 118
Ion Ratio Lower Upper
56 100
55 64.4 57.4 86.0

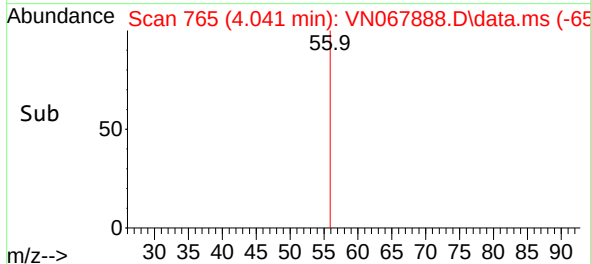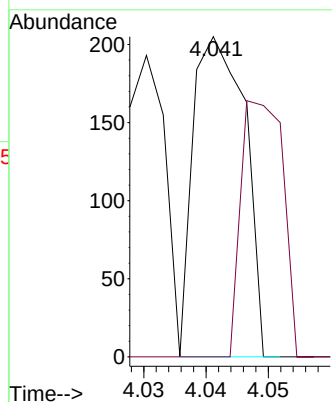

#16
Acetone
Concen: 38.125 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.008 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 43 Resp: 49577
Ion Ratio Lower Upper
43 100
58 33.5 21.2 31.8#


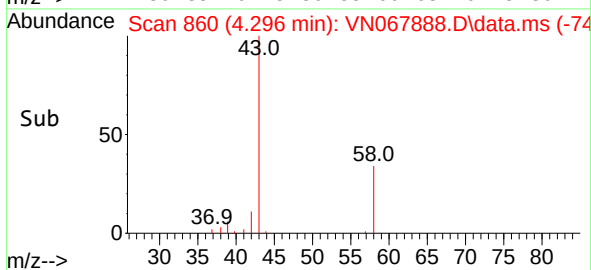
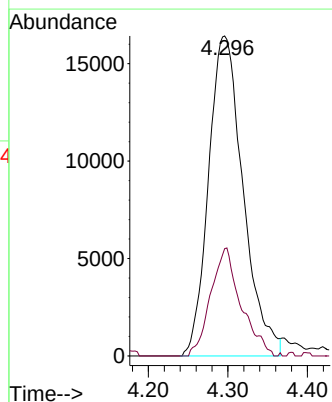
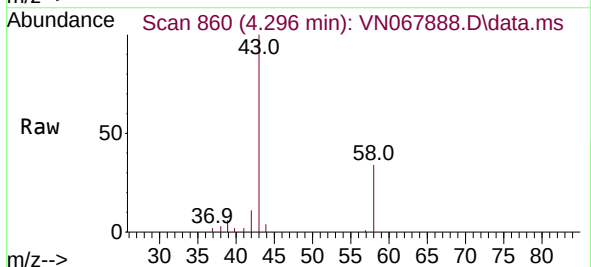




#18
Methyl Acetate
Concen: 0.504 ug/l
RT: 4.856 min Scan# 1069
Delta R.T. -0.001 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 1841
Ion Ratio Lower Upper
43 100
74 10.3 17.4 26.0#

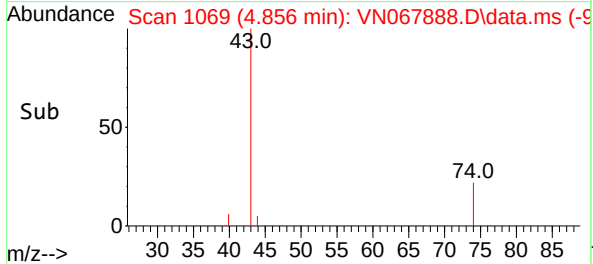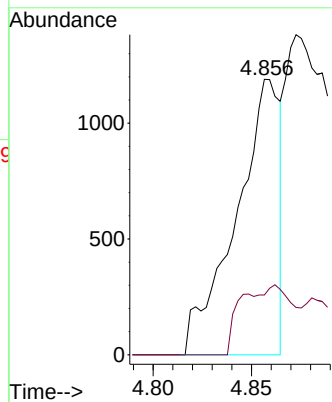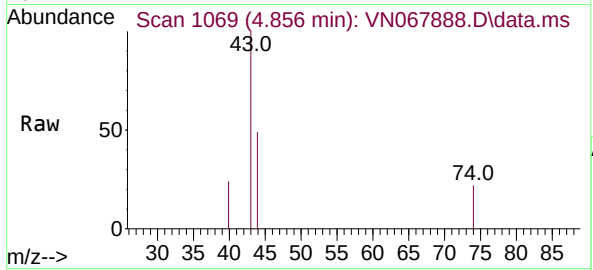

#20
Methylene Chloride
Concen: 8.510 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.005 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 84 Resp: 27588
Ion Ratio Lower Upper
84 100
49 116.8 110.9 166.3
51 36.1 32.6 49.0
86 61.5 51.6 77.4


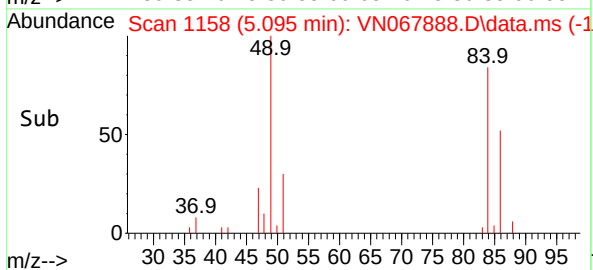

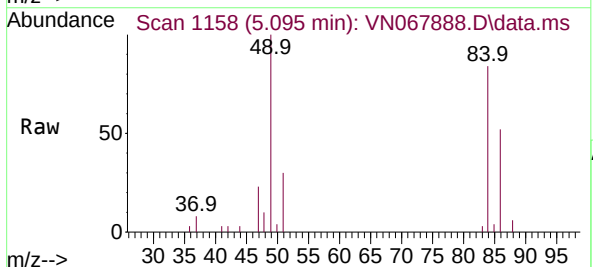


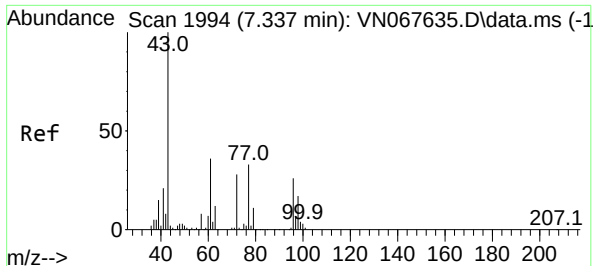

#25
2-Butanone
Concen: 4.280 ug/l
RT: 7.356 min Scan# 2001
Delta R.T. 0.019 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 9241
Ion Ratio Lower Upper
43 100
72 22.0 19.7 29.5

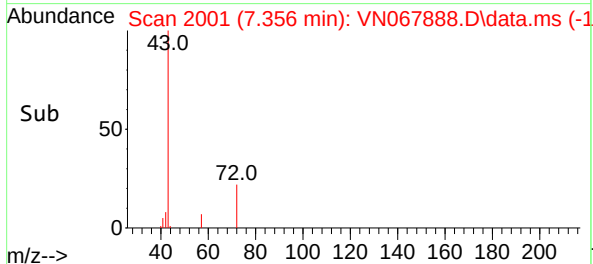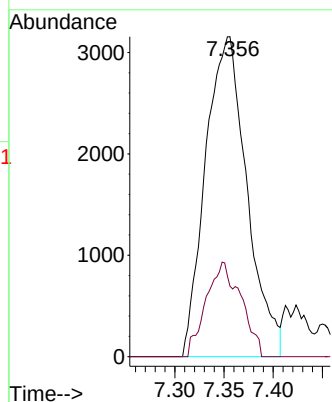

#29
Tetrahydrofuran
Concen: 2.430 ug/l
RT: 7.694 min Scan# 2127
Delta R.T. 0.005 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 42 Resp: 3451
Ion Ratio Lower Upper
42 100
72 29.3 32.8 49.2#
71 20.0 31.2 46.8#


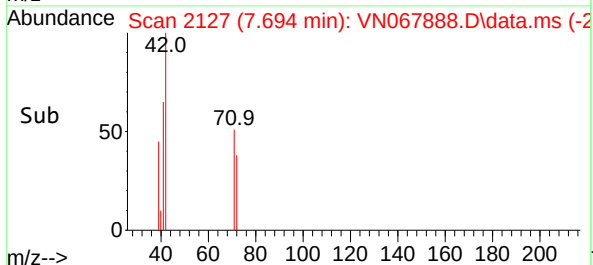

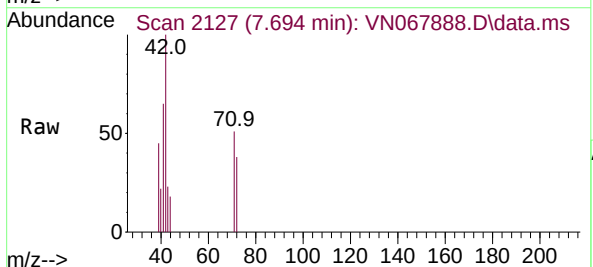




#31
Cyclohexane
Concen: 1.319 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.008 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 7642
Ion Ratio Lower Upper
56 100
69 157.0 27.3 40.9#
84 109.4 64.9 97.3#

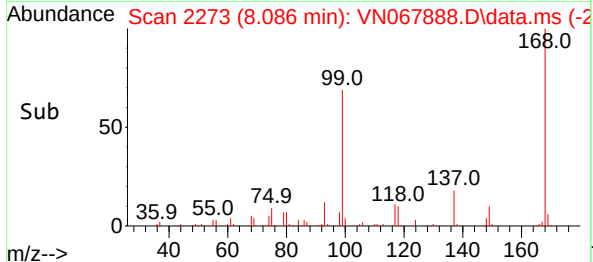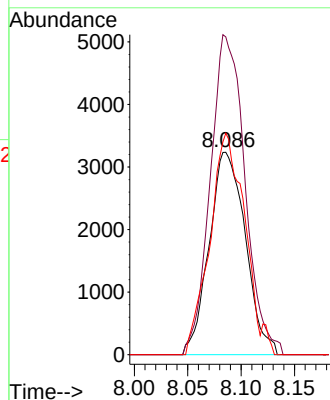

#33
1,2-Dichloroethane-d4
Concen: 54.242 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 65 Resp: 224166
Ion Ratio Lower Upper
65 100
67 50.3 0.0 98.6


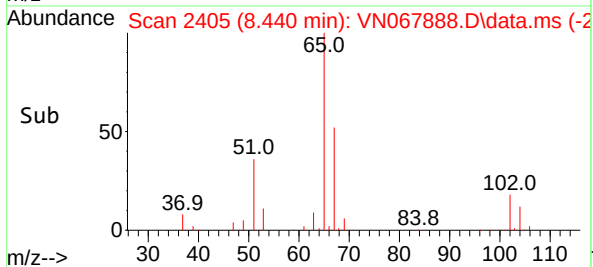
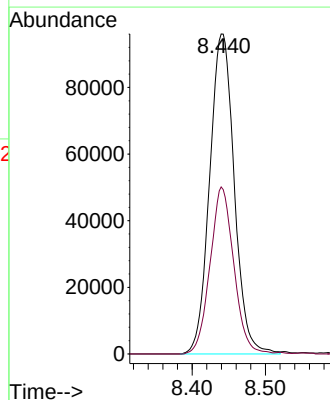
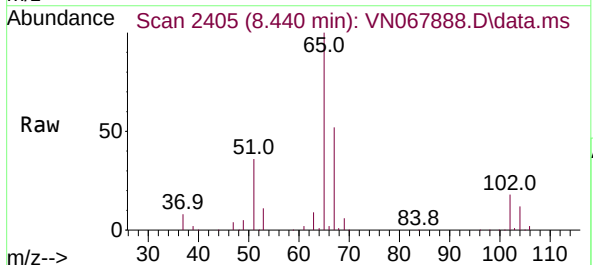


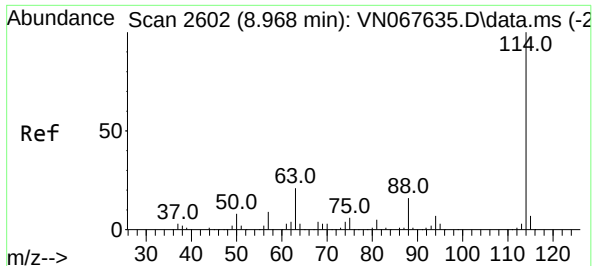

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:114 Resp: 524831
Ion Ratio Lower Upper
114 100
63 22.2 0.0 49.0
88 15.5 0.0 36.6

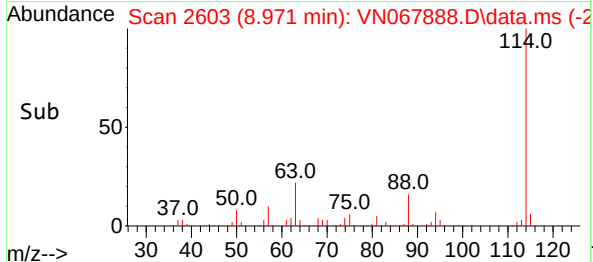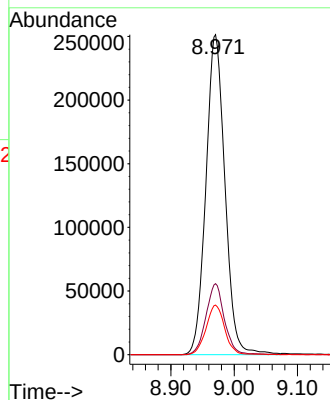

#35
Dibromofluoromethane
Concen: 51.453 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31


Tgt Ion:113 Resp: 163152
Ion Ratio Lower Upper
113 100
111 104.2 83.8 125.8
192 15.8 13.4 20.0

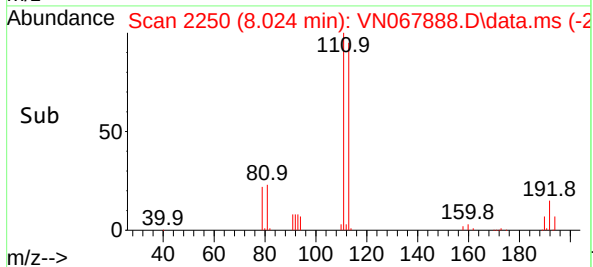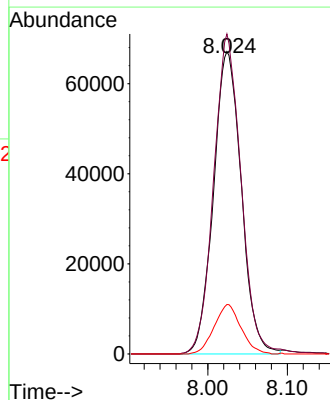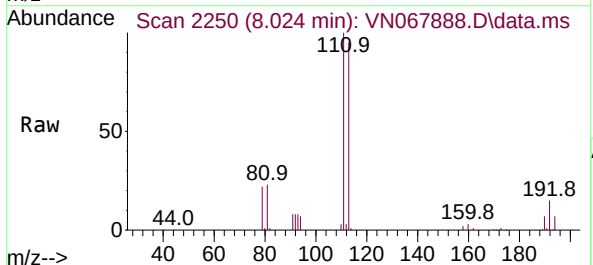



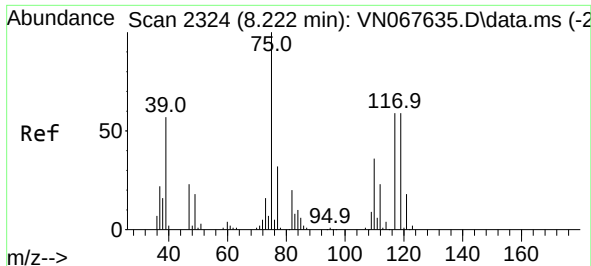


#36
 1,1-Dichloropropene
 Concen: 5.160 ug/l
 RT: 8.088 min Scan# 2274
 Delta R.T. -0.134 min
 Lab File: VN067888.D
 Acq: 23 Jul 2021 18:31

Instrument :
 MSVOA_N
 ClientSampled :







Tgt Ion: 75 Resp: 25156
 Ion Ratio Lower Upper
 75 100
 110 11.3 15.7 47.0#
 77 0.0 24.6 37.0#

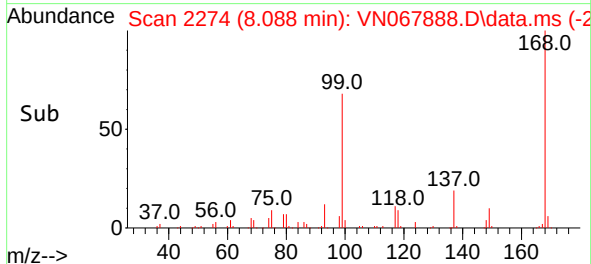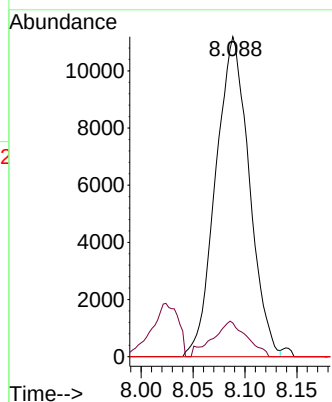

#37
 Ethyl Acetate
 Concen: 1.956 ug/l
 RT: 7.356 min Scan# 2001
 Delta R.T. -0.062 min
 Lab File: VN067888.D
 Acq: 23 Jul 2021 18:31

Tgt Ion: 43 Resp: 9241
 Ion Ratio Lower Upper
 43 100
 61 0.0 10.6 16.0#
 70 0.0 8.1 12.1#


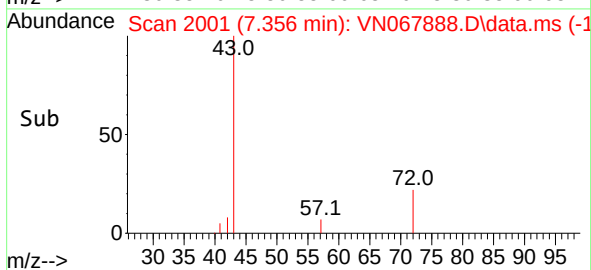

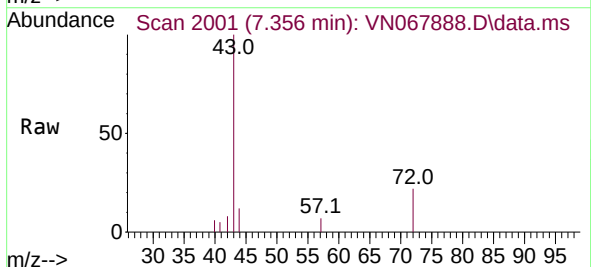


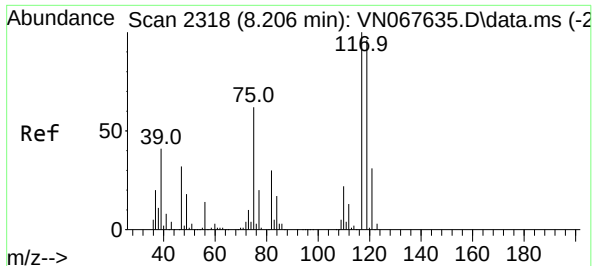

#38
Carbon Tetrachloride
Concen: 6.392 ug/l
RT: 8.091 min Scan# 2275
Delta R.T. -0.115 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 30739
Ion Ratio Lower Upper
117 100
119 4.8 75.4 113.2#
121 0.0 23.5 35.3#

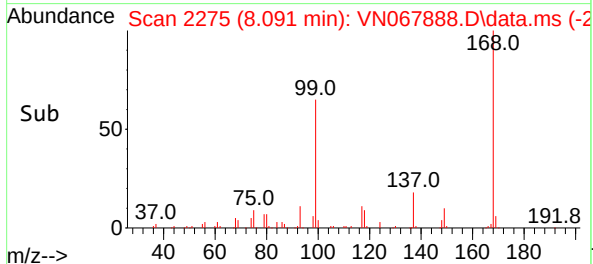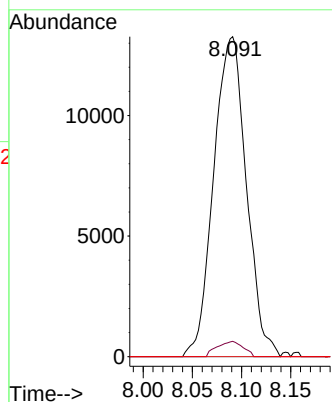

#41
Methacrylonitrile
Concen: 0.959 ug/l
RT: 7.699 min Scan# 2129
Delta R.T. 0.059 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 41 Resp: 2329
Ion Ratio Lower Upper
41 100
39 30.9 47.6 71.4#
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#


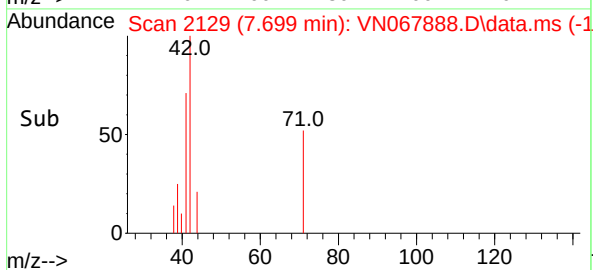

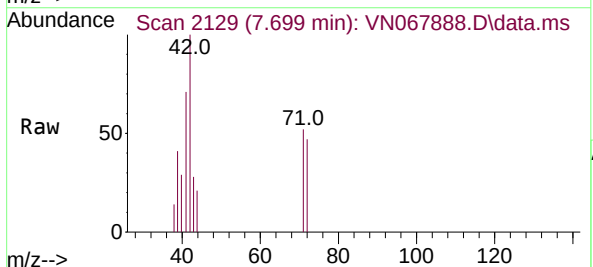




#43
Isopropyl Acetate
Concen: 4.562 ug/l
RT: 8.563 min Scan# 2451
Delta R.T. -0.000 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 37906
Ion Ratio Lower Upper
43 100
61 17.5 19.0 28.4#
87 13.5 9.5 14.3

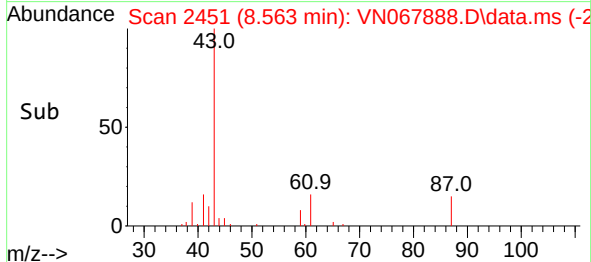

#45
1,2-Dichloropropane
Concen: 0.692 ug/l
RT: 9.625 min Scan# 2847
Delta R.T. 0.134 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 63 Resp: 2555
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#


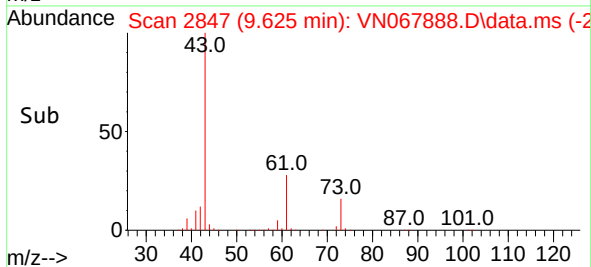

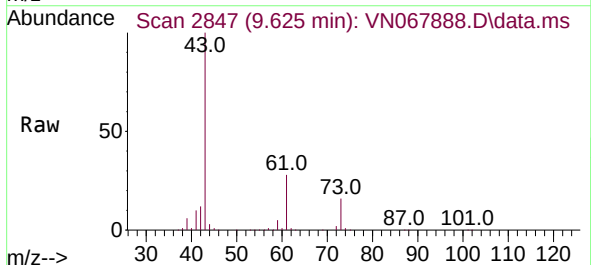




#48
Methyl methacrylate
Concen: 2.515 ug/l
RT: 9.550 min Scan# 2819
Delta R.T. -0.013 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 9244
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

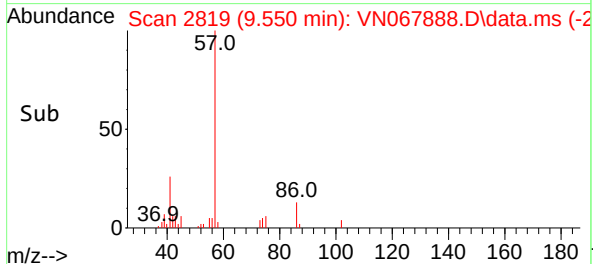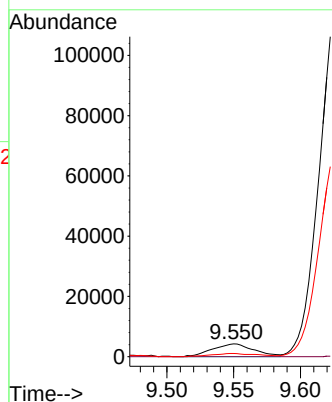

#49
1,4-Dioxane
Concen: 33.245 ug/l
RT: 9.614 min Scan# 2843
Delta R.T. 0.043 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 88 Resp: 84
Ion Ratio Lower Upper
88 100
43 0.0 28.8 43.2#
58 0.0 60.4 90.6#


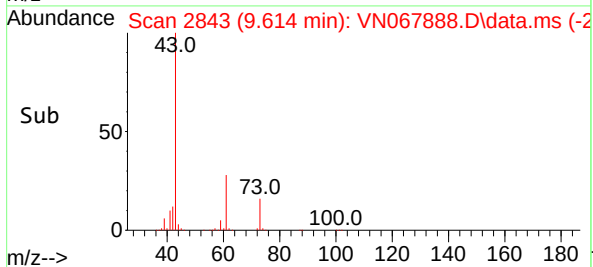

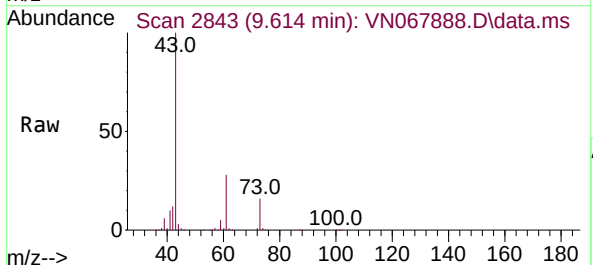


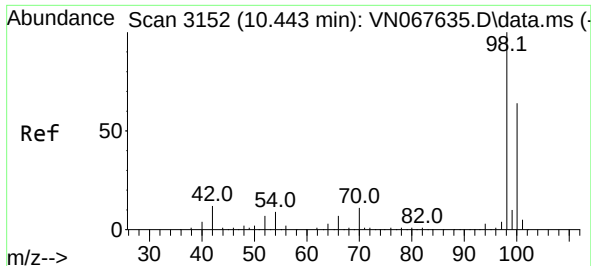

#50
Toluene-d8
Concen: 52.598 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 698113
Ion Ratio Lower Upper
98 100
100 63.8 51.7 77.5

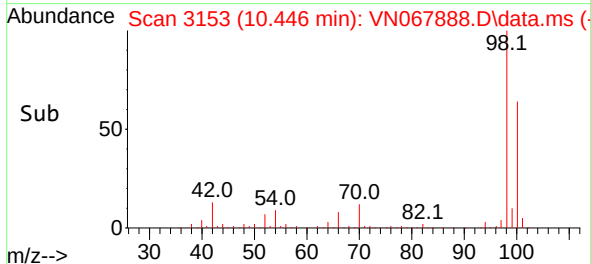

#51
4-Methyl-2-Pentanone
Concen: 1.922 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 43 Resp: 9810
Ion Ratio Lower Upper
43 100
58 42.0 28.6 43.0


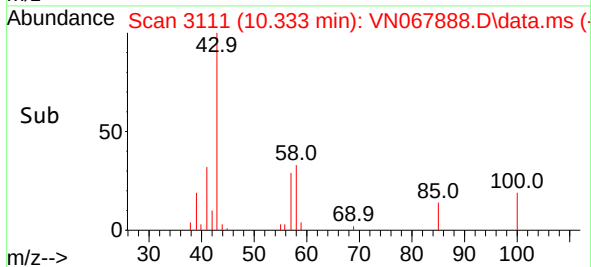

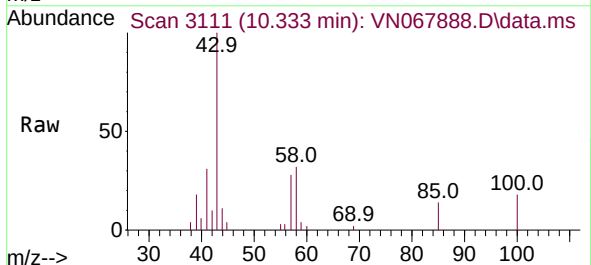


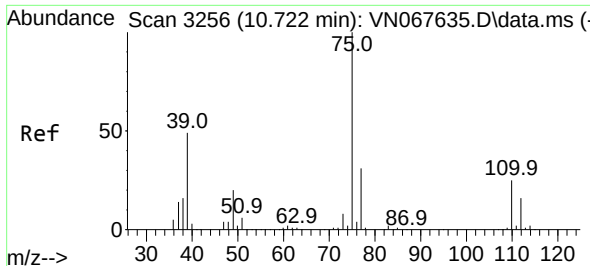

#53
t-1,3-Dichloropropene
Concen: 1.753 ug/l
RT: 10.459 min Scan# 3158
Delta R.T. -0.263 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 53
Ion Ratio Lower Upper
75 100
77 127.0 25.1 37.7#

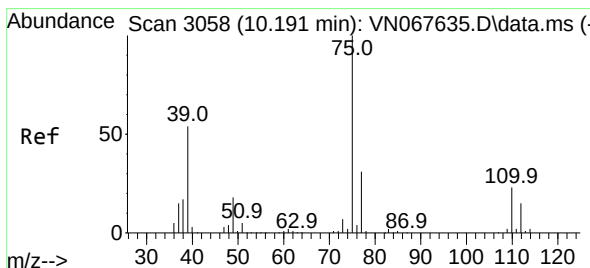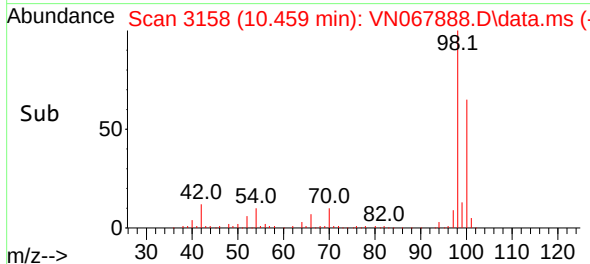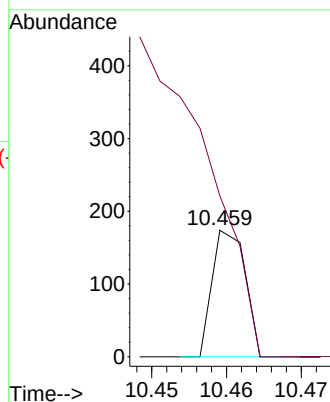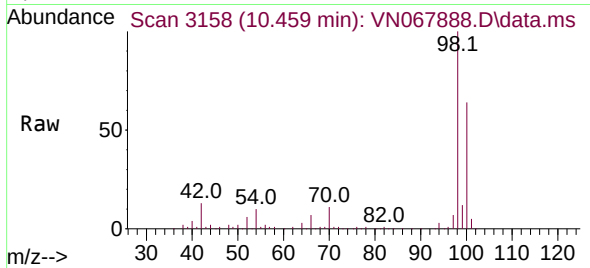

#54
cis-1,3-Dichloropropene
Concen: 11.550 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 75 Resp: 65831
Ion Ratio Lower Upper
75 100
77 0.0 24.6 37.0#
39 38.4 50.7 76.1#


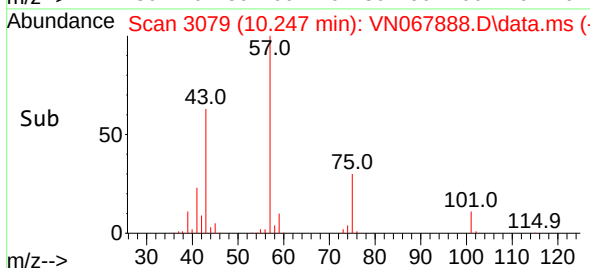
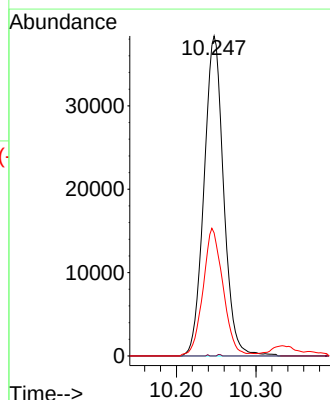
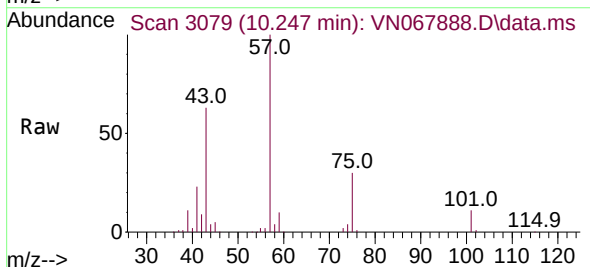




#57
1,3-Dichloropropane
Concen: 6.708 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 42137
Ion Ratio Lower Upper
76 100
78 0.1 25.7 38.5#

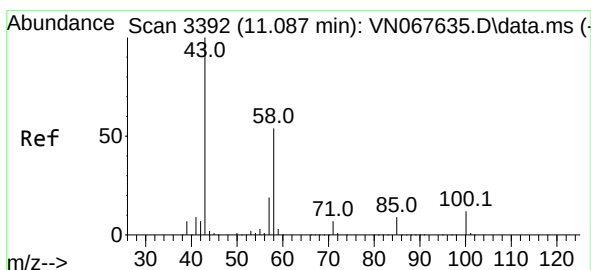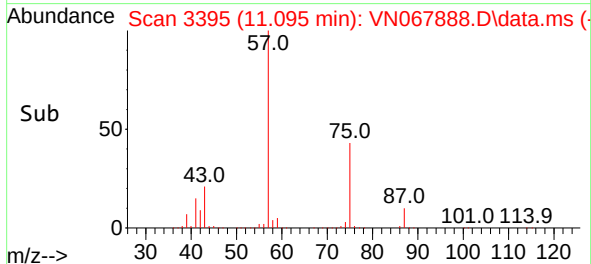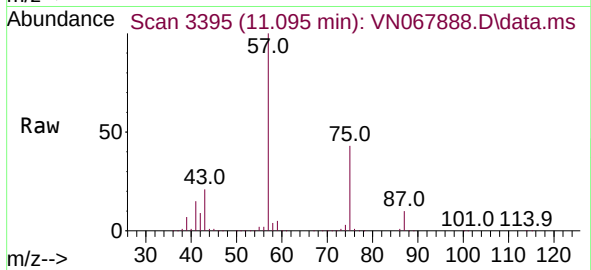

#59
2-Hexanone
Concen: 173.536 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 43 Resp: 618336
Ion Ratio Lower Upper
43 100
58 17.9 24.7 74.1#




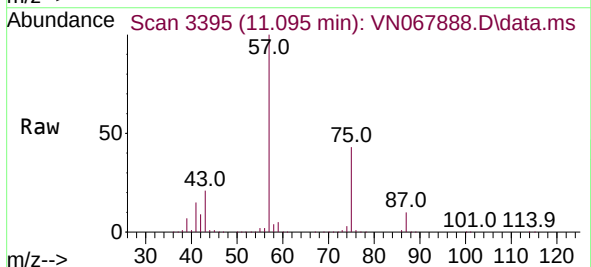


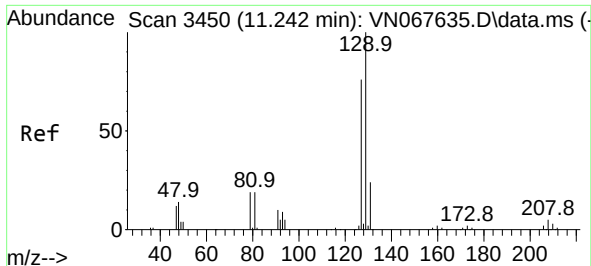

#60
Dibromochloromethane
Concen: 2.423 ug/l
RT: 11.492 min Scan# 3543
Delta R.T. 0.250 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:129 Resp: 312
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

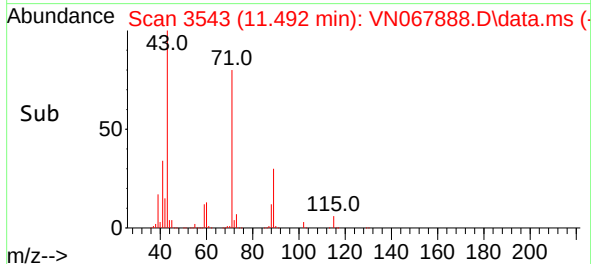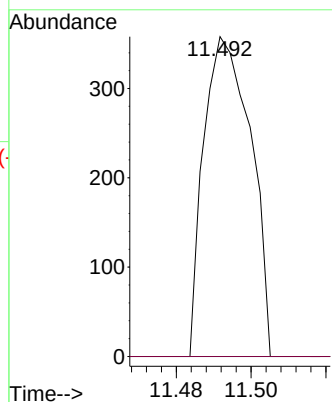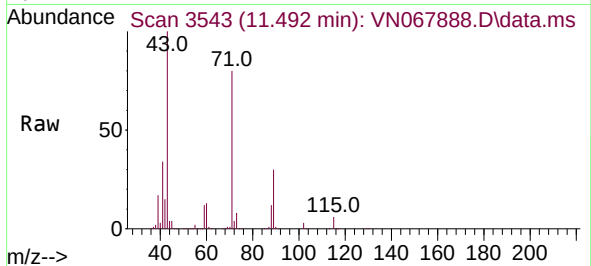

#62
4-Bromofluorobenzene
Concen: 49.992 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 95 Resp: 234394
Ion Ratio Lower Upper
95 100
174 70.3 0.0 122.0
176 67.5 0.0 117.6


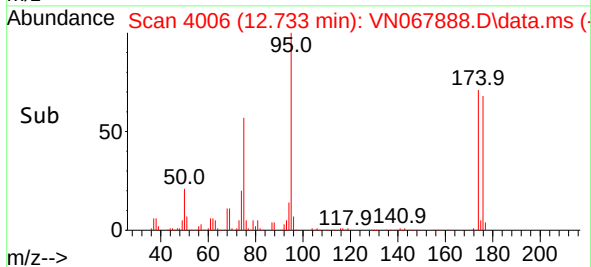
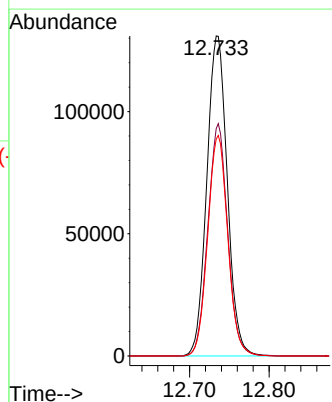
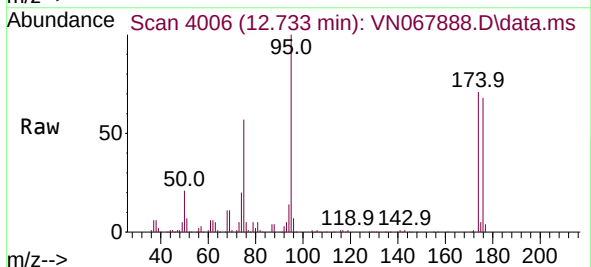


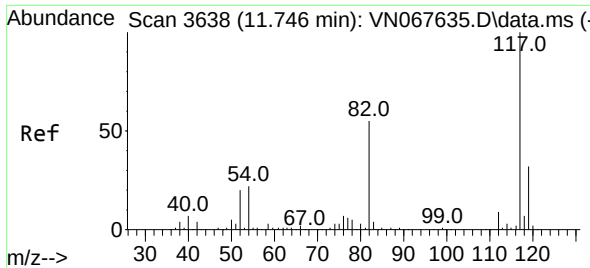

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 555020
Ion Ratio Lower Upper
117 100
82 56.4 53.1 79.7
119 31.8 25.5 38.3

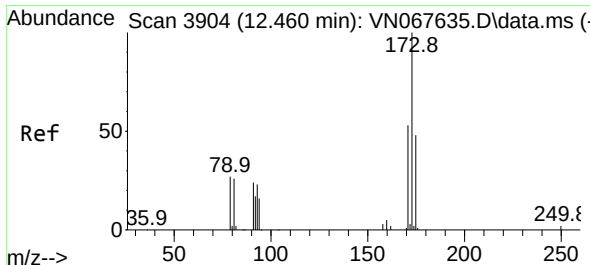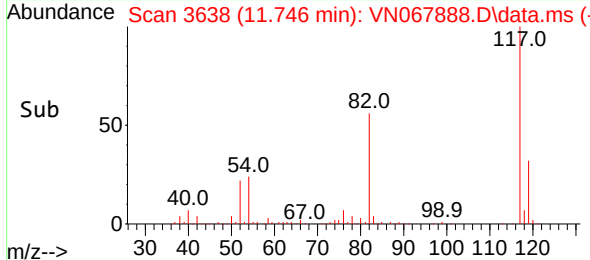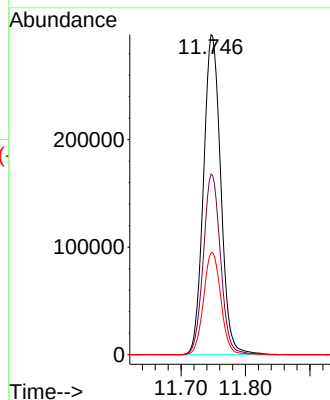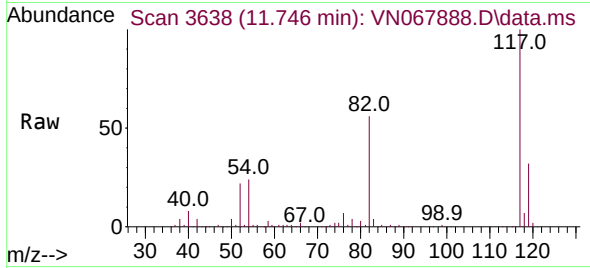

#71
Bromoform
Concen: 3.196 ug/l
RT: 12.715 min Scan# 3999
Delta R.T. 0.255 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion:173 Resp: 78
Ion Ratio Lower Upper
173 100
175 15166.7 23.9 71.8#
254 0.0 0.0 0.0


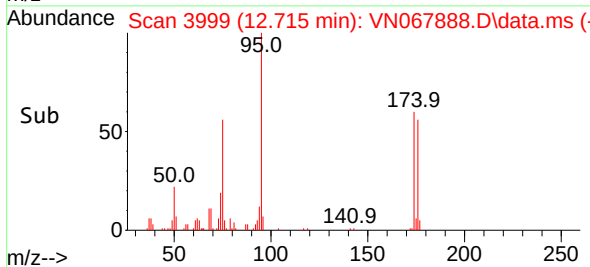
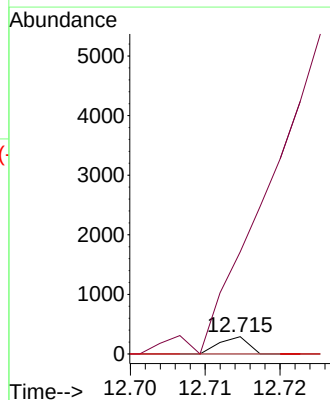
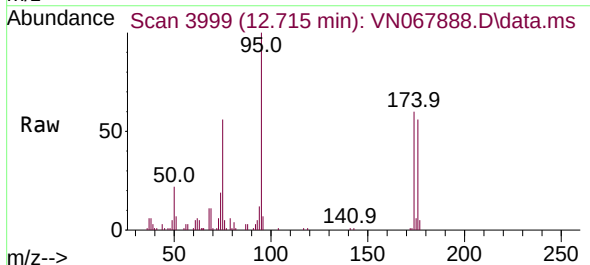


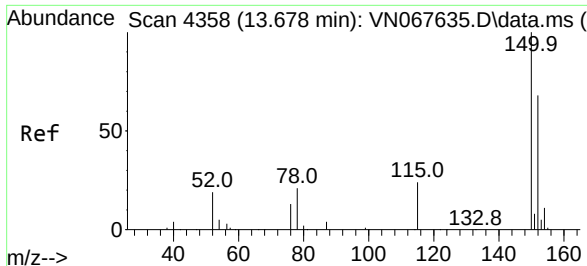

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.677 min Scan# 4358
Delta R.T. -0.000 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 186456
Ion Ratio Lower Upper
152 100
115 64.5 36.1 108.5
150 161.7 0.0 351.8

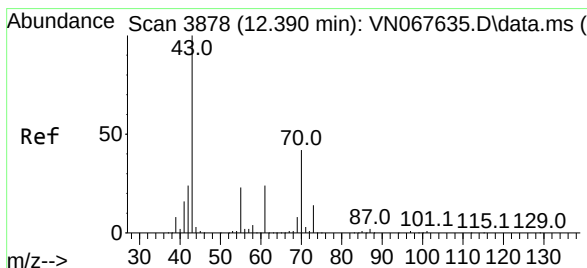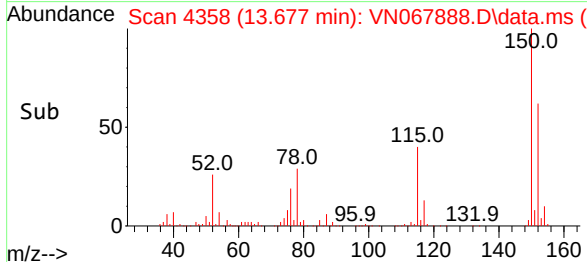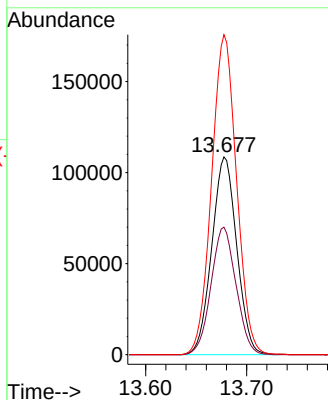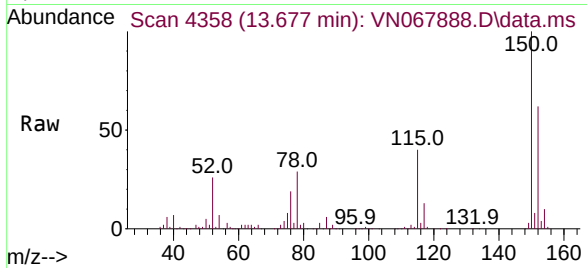

#74
N-ethyl acetate
Concen: 0.222 ug/l
RT: 12.361 min Scan# 3867
Delta R.T. -0.029 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion: 43 Resp: 1214
Ion Ratio Lower Upper
43 100
70 0.0 29.4 44.2#
55 0.0 17.0 25.4#
61 0.0 17.6 26.4#


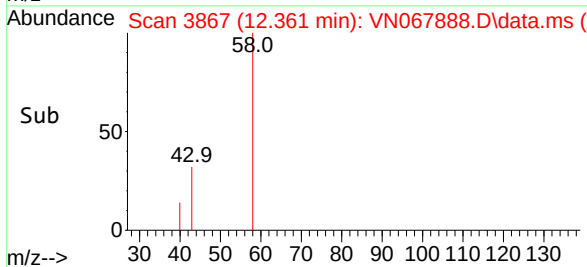
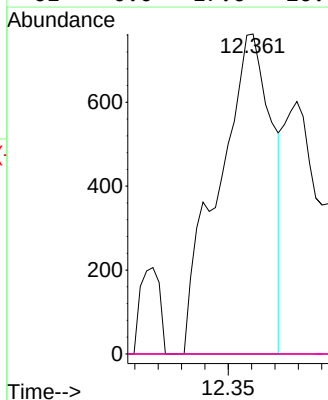
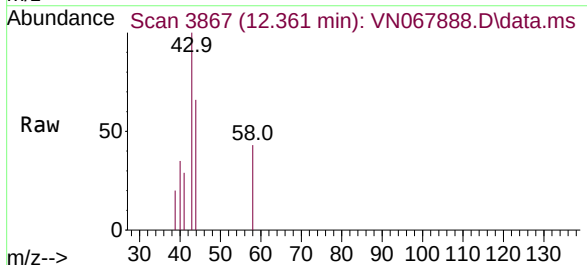




#76
1,2,3-Trichloropropane
Concen: 34.243 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 130388
Ion Ratio Lower Upper
75 100
77 1.1 0.0 0.0#

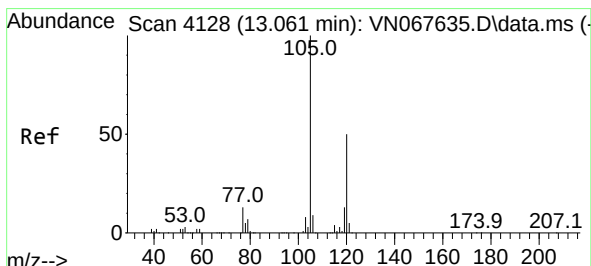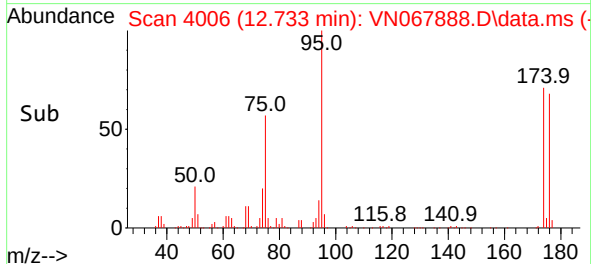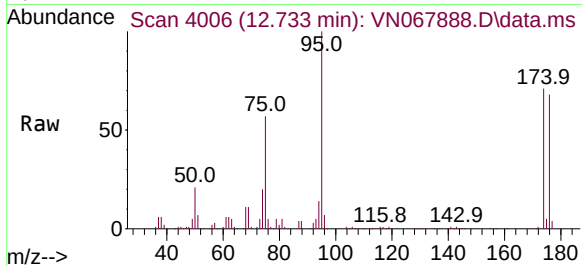

#80
1,3,5-Trimethylbenzene
Concen: 0.295 ug/l
RT: 13.063 min Scan# 4129
Delta R.T. 0.002 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion:105 Resp: 3601
Ion Ratio Lower Upper
105 100
120 46.6 22.2 66.6


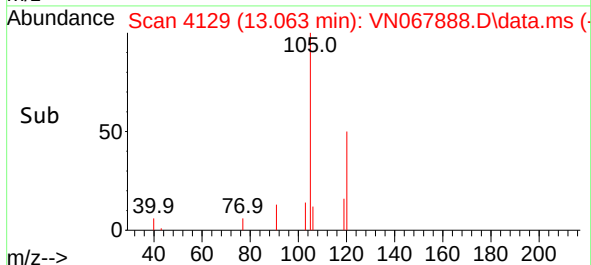
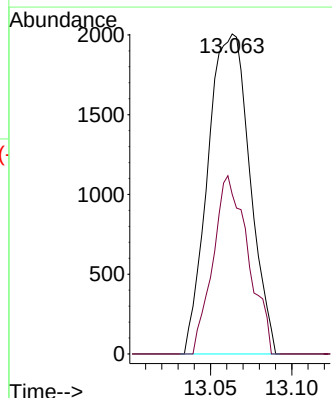
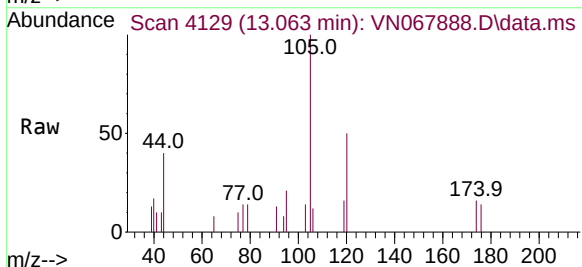


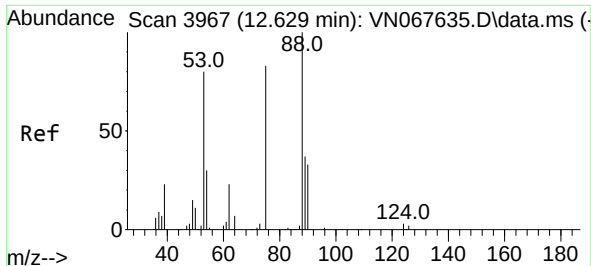

#81
trans-1,4-Dichloro-2-butene
Concen: 110.402 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion: 75 Resp: 130388
Ion Ratio Lower Upper
75 100
53 0.1 87.6 131.4#
89 0.0 37.8 56.8#

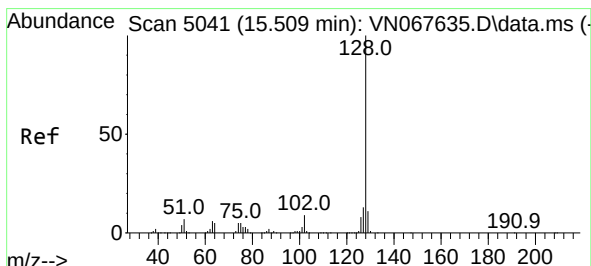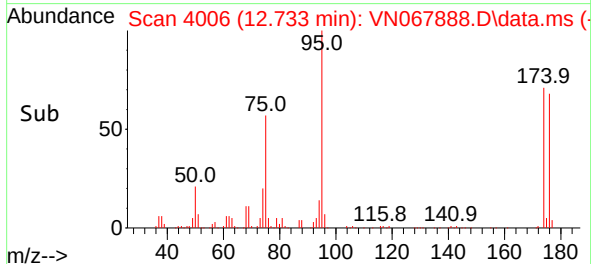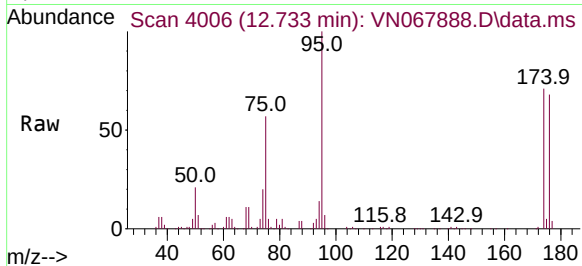

#95
Naphthalene
Concen: 3.040 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.000 min
Lab File: VN067888.D
Acq: 23 Jul 2021 18:31

Tgt Ion:128 Resp: 265
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.6 12.8#

