

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072321\
 Data File : VN067878.D
 Acq On : 23 Jul 2021 14:26
 Operator : JC/MD
 Sample : M3160-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M

Title : SW846 8260

Signal : TIC: VN067878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.228	76	89	111	rBV	250655	372231	19.79%	3.863%
2	2.740	267	280	294	rBV4	19157	43970	2.34%	0.456%
3	8.024	2226	2250	2261	rBV2	229705	544986	28.98%	5.656%
4	8.086	2261	2273	2305	rVB2	398986	922200	49.03%	9.571%
5	8.440	2384	2405	2434	rBV	263236	610369	32.45%	6.335%
6	8.971	2584	2603	2637	rVB	619955	1292996	68.75%	13.419%
7	10.443	3133	3152	3183	rBV	972669	1880759	100.00%	19.519%
8	11.746	3621	3638	3677	rBV	907827	1651115	87.79%	17.136%
9	12.733	3990	4006	4032	rBV	637270	1116147	59.35%	11.584%
10	13.678	4342	4358	4379	rBV	701151	1200600	63.84%	12.460%




Sum of corrected areas: 9635373

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072321\
Data File : VN067878.D
Acq On : 23 Jul 2021 14:26
Operator : JC/MD
Sample : M3160-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

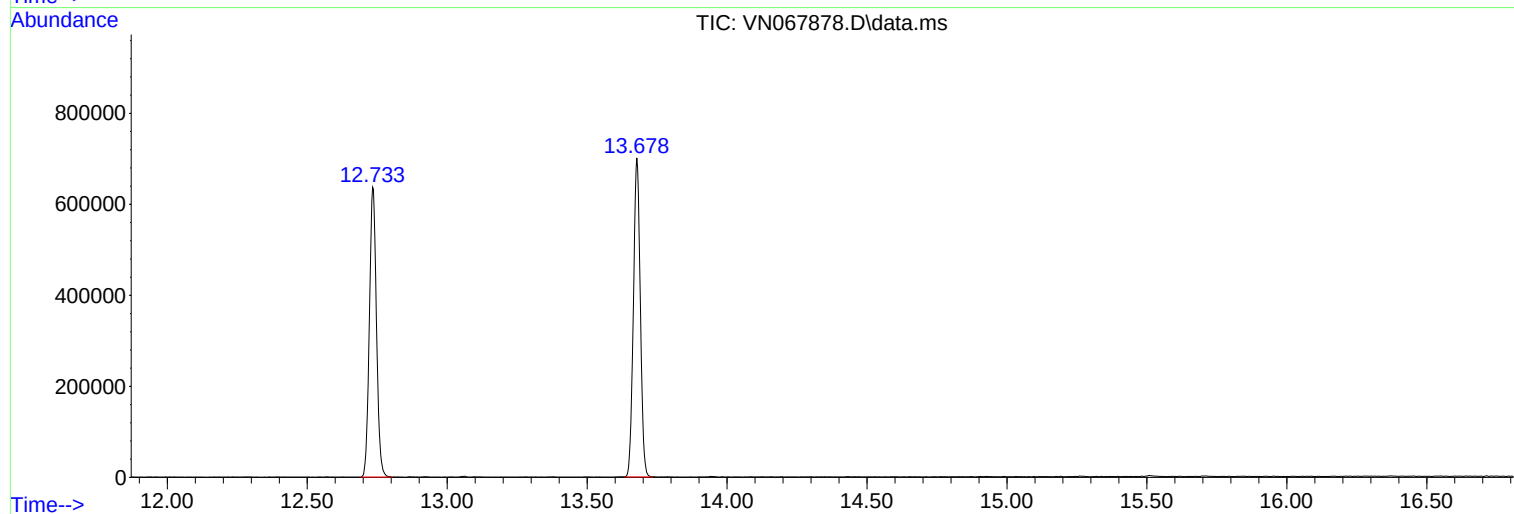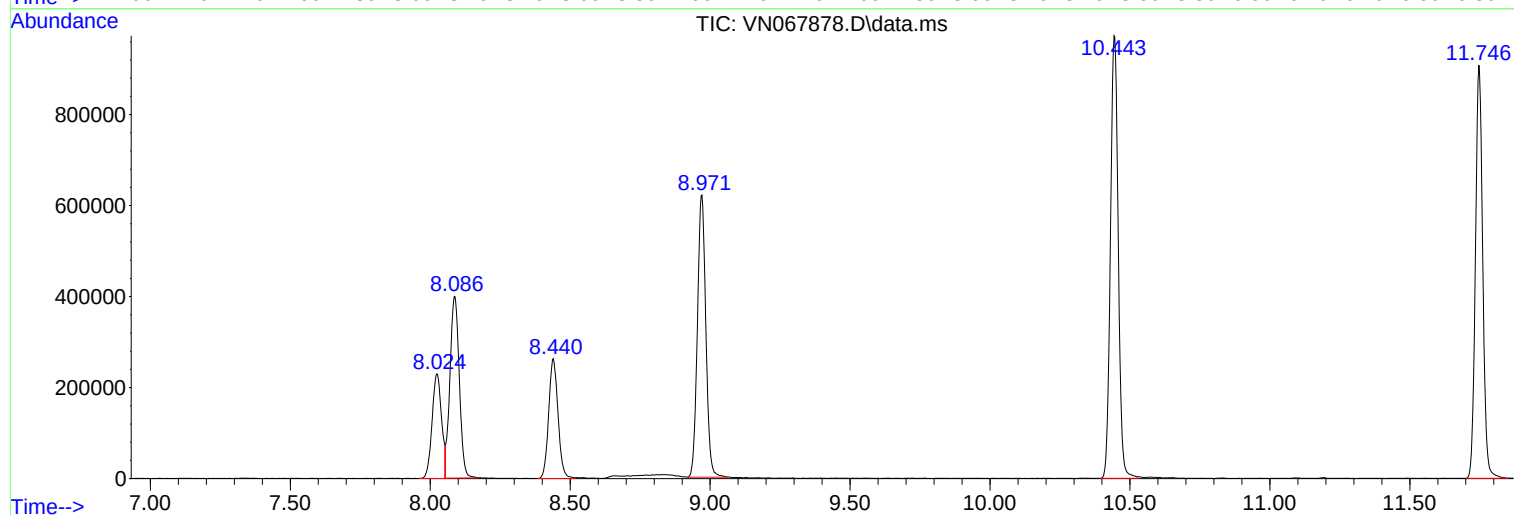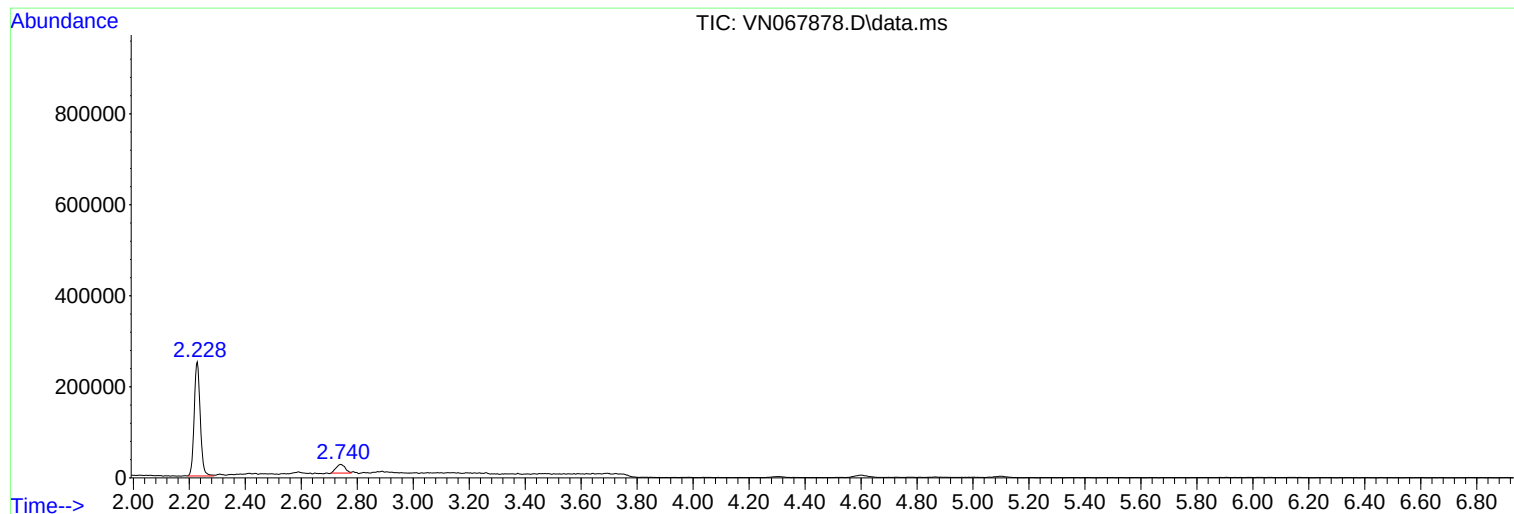

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072321\
Data File : VN067878.D
Acq On : 23 Jul 2021 14:26
Operator : JC/MD
Sample : M3160-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072321\
Data File : VN067878.D
Acq On : 23 Jul 2021 14:26
Operator : JC/MD
Sample : M3160-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
