

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072324\
 Data File : VN083012.D
 Acq On : 23 Jul 2024 15:07
 Operator : JC\MD
 Sample : VN0723WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0723WBL01

Quant Time: Jul 24 02:28:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 08 13:46:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	66765	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	130690	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	132778	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	54995	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	54148	57.856	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	115.720%
35) Dibromofluoromethane	8.165	113	46638	55.614	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	111.220%
50) Toluene-d8	10.571	98	156080	50.391	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.780%
62) 4-Bromofluorobenzene	12.853	95	46993	42.237	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	84.480%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072324\
Data File : VN083012.D
Acq On : 23 Jul 2024 15:07
Operator : JC\MD
Sample : VN0723WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0723WBL01

Quant Time: Jul 24 02:28:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 08 13:46:04 2024
Response via : Initial Calibration




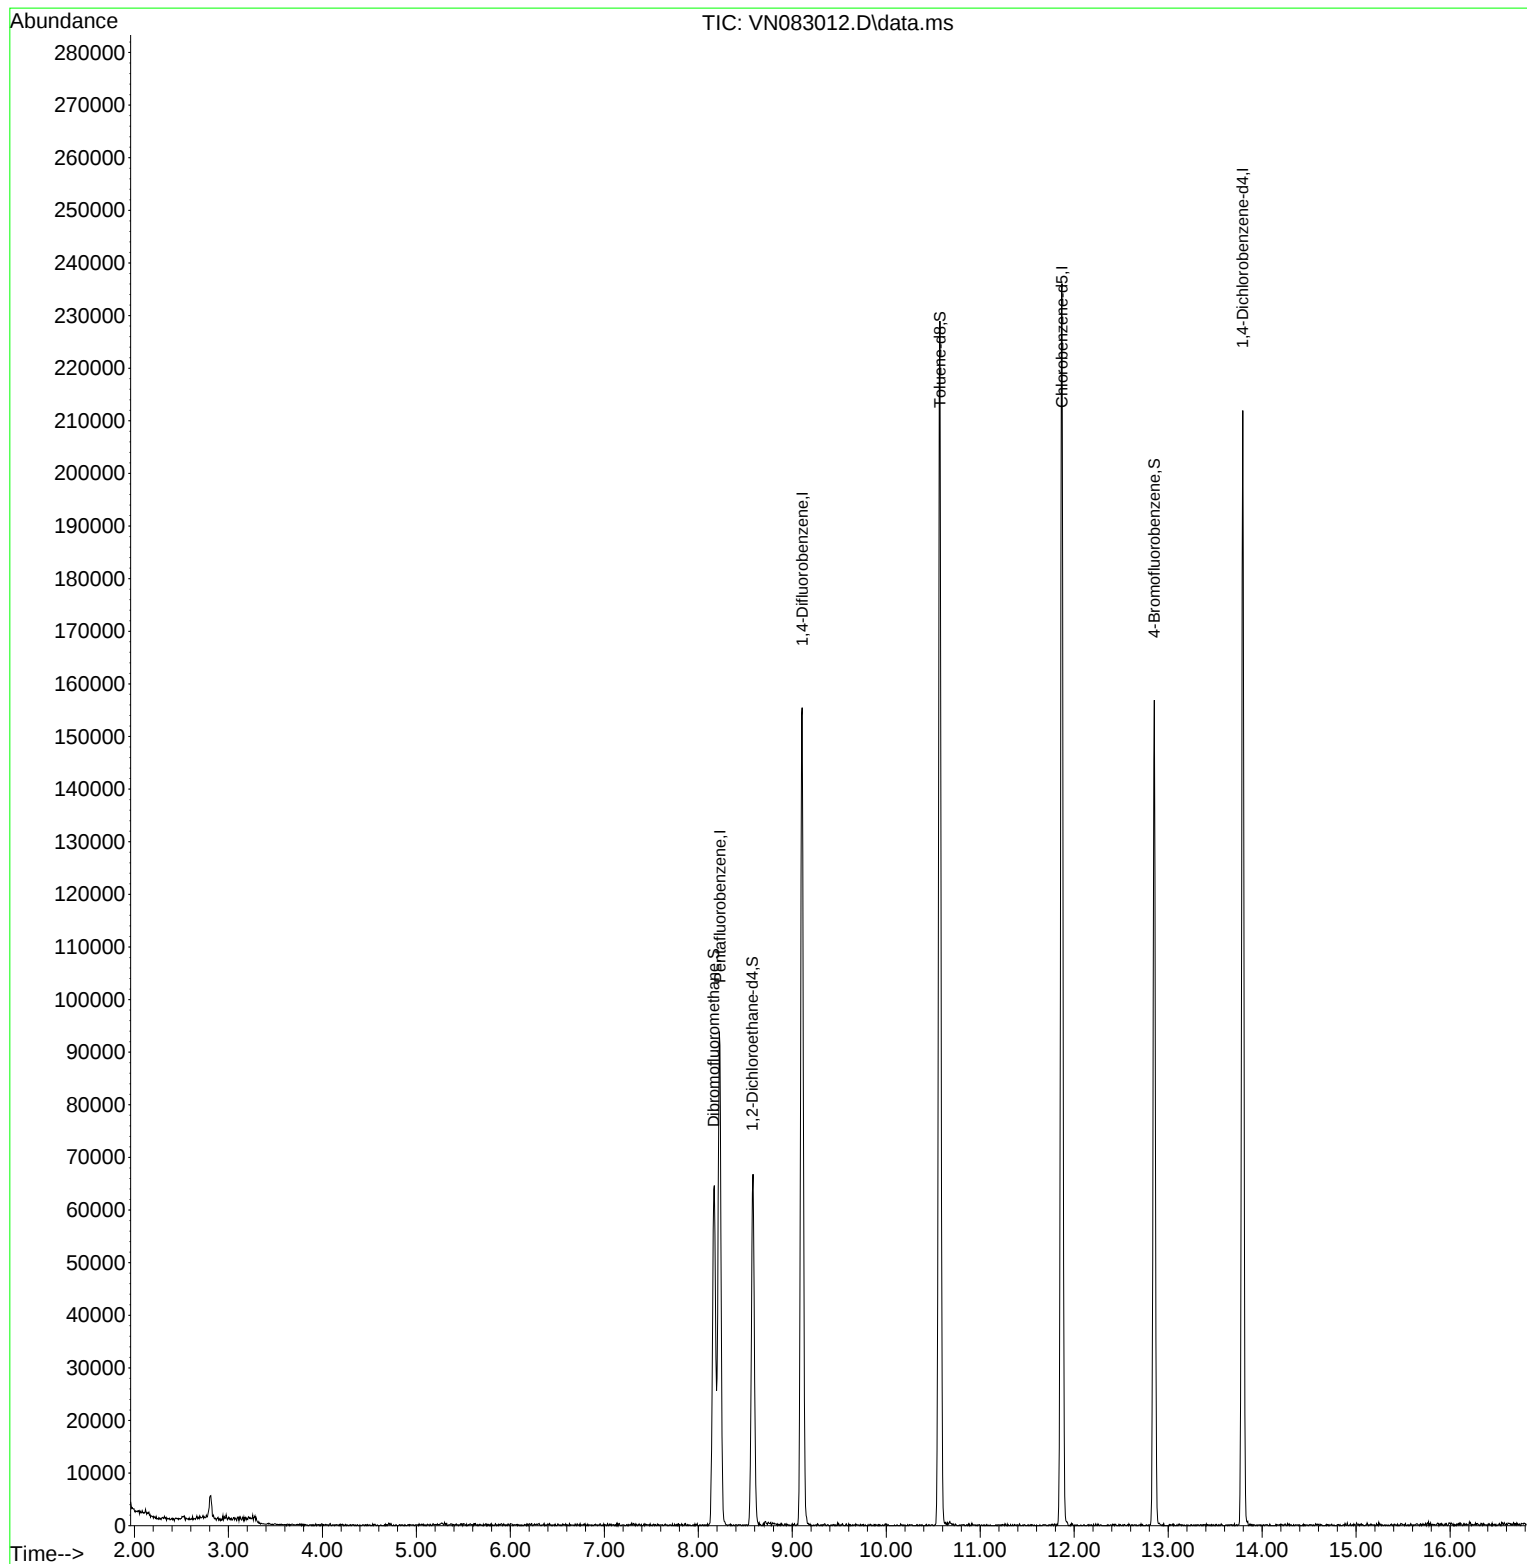


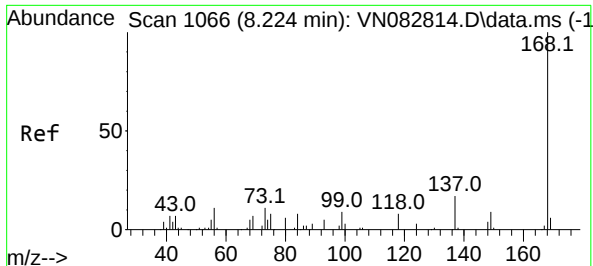

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1066
Delta R.T. 0.001 min
Lab File: VN083012.D
Acq: 23 Jul 2024 15:07




Instrument :
MSVOA_N
ClientSampleId :
VN0723WBL01


Tgt Ion:168 Resp: 66765
Ion Ratio Lower Upper
168 100
99 59.6 48.2 72.4

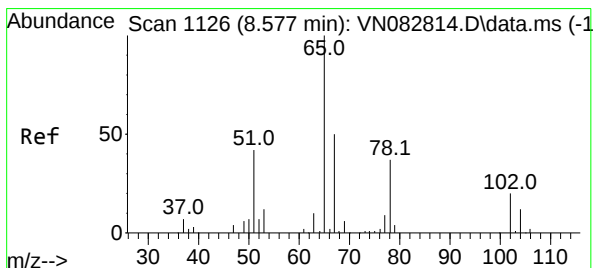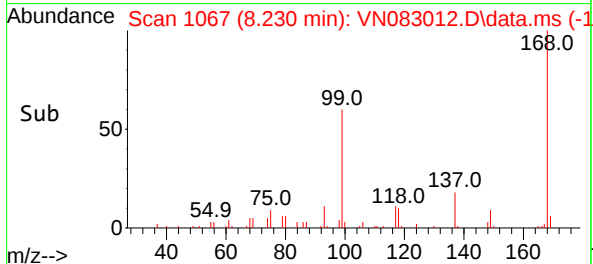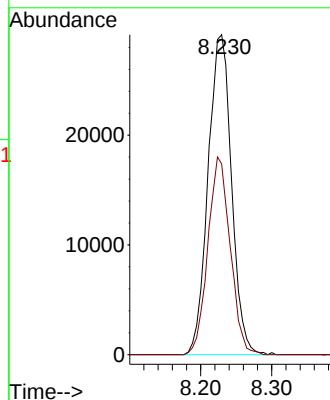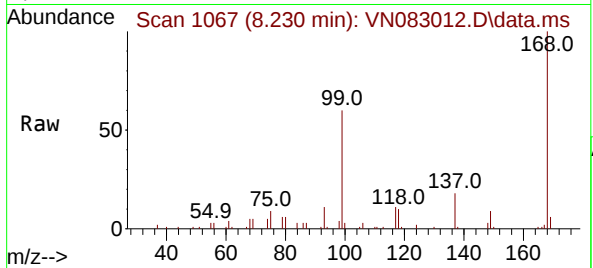

#33
1,2-Dichloroethane-d4
Concen: 57.856 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.005 min
Lab File: VN083012.D
Acq: 23 Jul 2024 15:07

Tgt Ion: 65 Resp: 54148
Ion Ratio Lower Upper
65 100
67 51.3 0.0 104.4

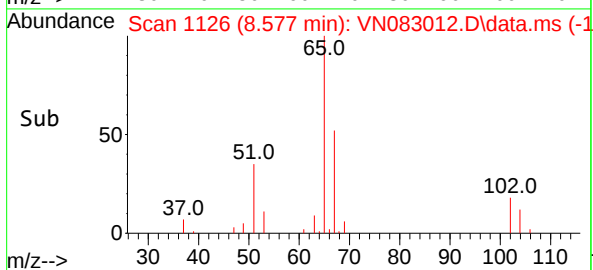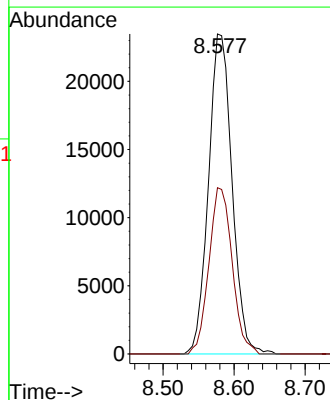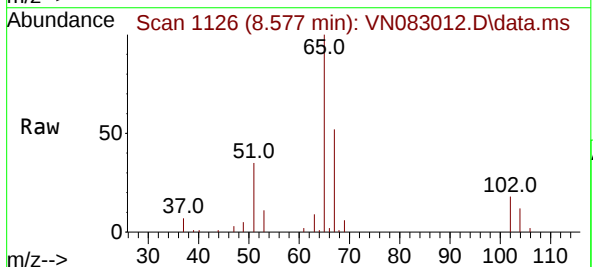

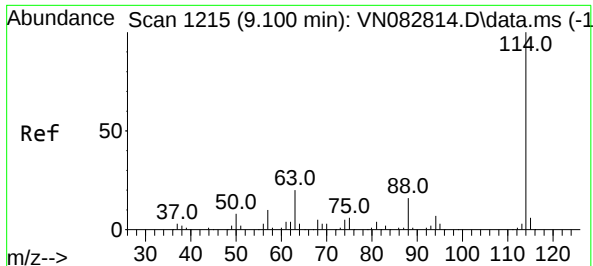

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN083012.D

Acq: 23 Jul 2024 15:07

Instrument :

MSVOA_N

ClientSampleId :

VN0723WBL01





Tgt Ion:114 Resp: 130690

Ion Ratio Lower Upper

114 100

63 19.1 0.0 44.6

88 15.4 0.0 31.4

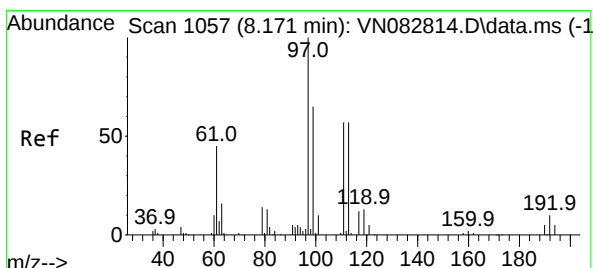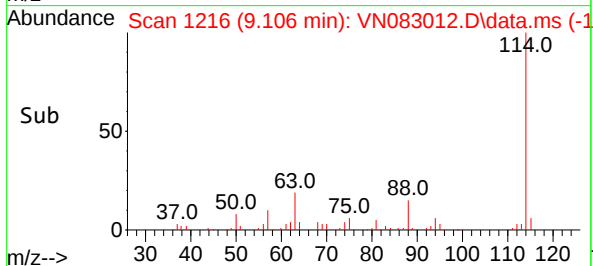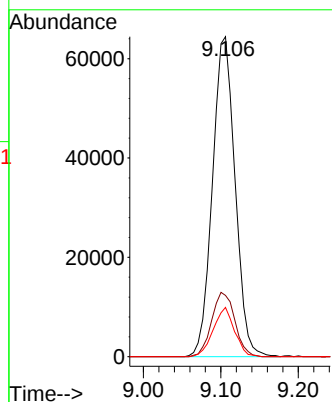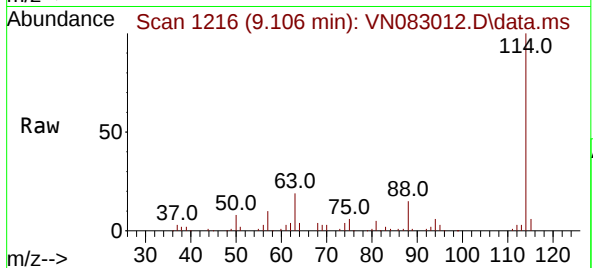

#35

Dibromofluoromethane

Concen: 55.614 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN083012.D

Acq: 23 Jul 2024 15:07




Tgt Ion:113 Resp: 46638


Ion Ratio Lower Upper

113 100

111 101.3 82.4 123.6

192 17.8 14.9 22.3


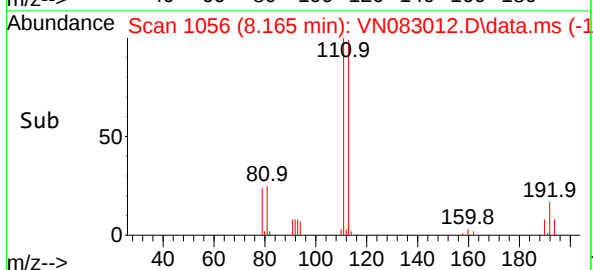
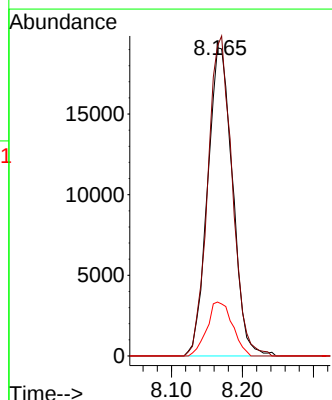
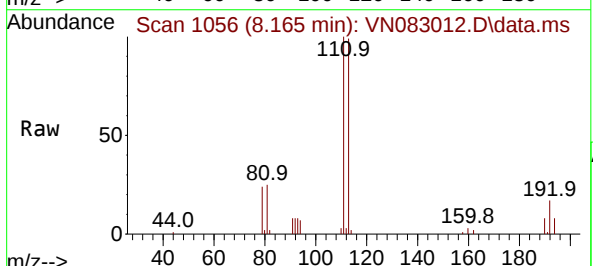


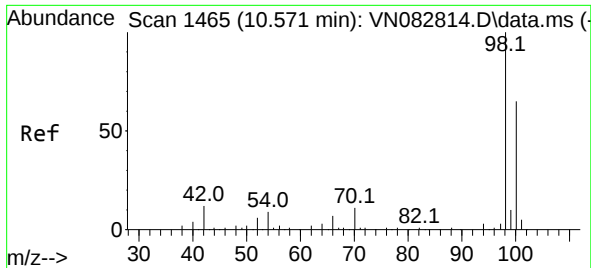

#50
Toluene-d8
Concen: 50.391 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.001 min
Lab File: VN083012.D
Acq: 23 Jul 2024 15:07




Instrument :
MSVOA_N
ClientSampleId :
VN0723WBL01


Tgt Ion: 98 Resp: 156080
Ion Ratio Lower Upper
98 100
100 61.5 51.5 77.3

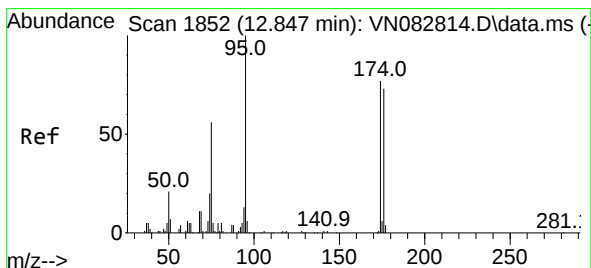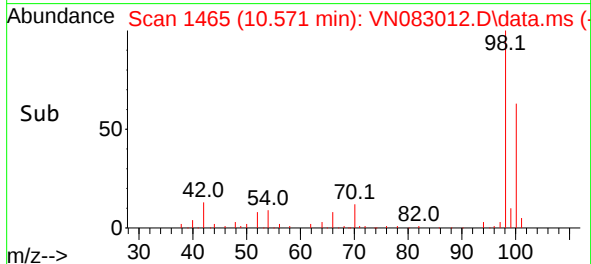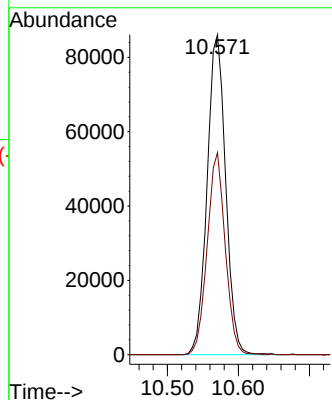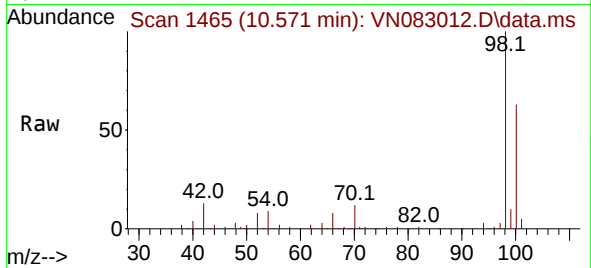

#62
4-Bromofluorobenzene
Concen: 42.237 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN083012.D
Acq: 23 Jul 2024 15:07

Tgt Ion: 95 Resp: 46993
Ion Ratio Lower Upper
95 100
174 85.4 0.0 159.2
176 81.1 0.0 147.6


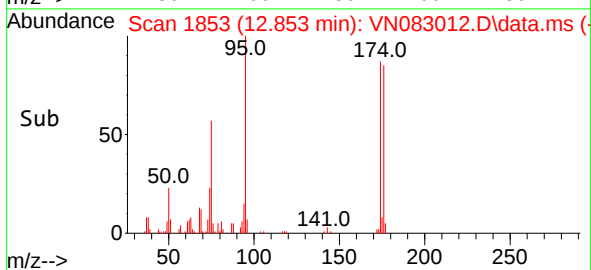
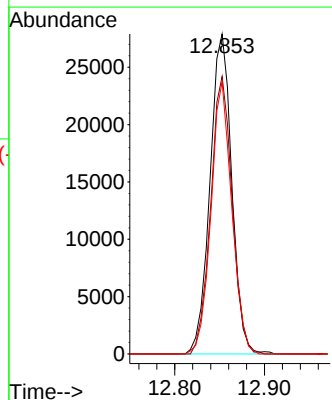
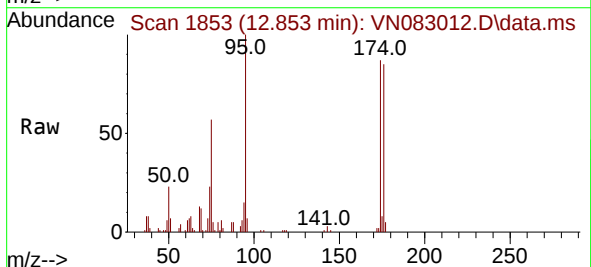


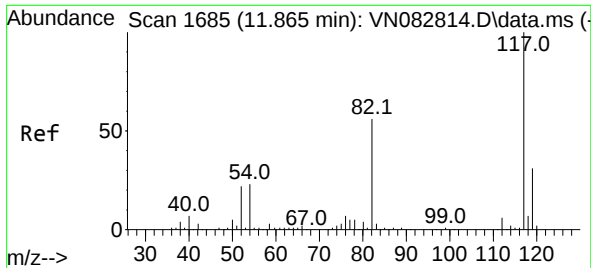

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN083012.D
Acq: 23 Jul 2024 15:07

Instrument :
MSVOA_N
ClientSampleId :
VN0723WBL01

Tgt Ion:117 Resp: 132778
Ion Ratio Lower Upper
117 100
82 53.3 47.5 71.3
119 32.0 25.6 38.4

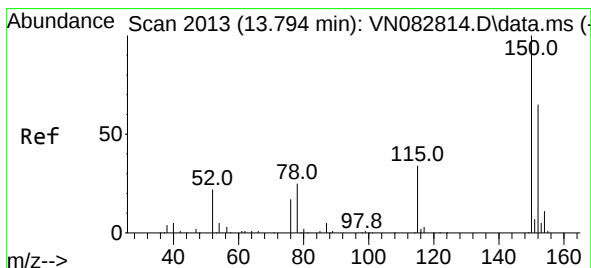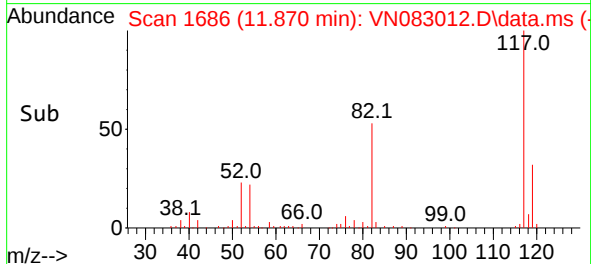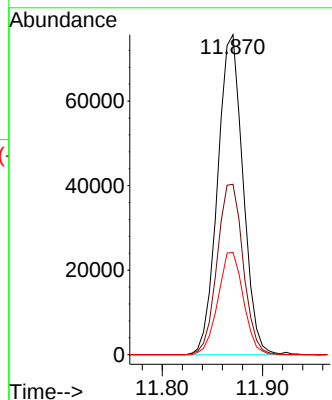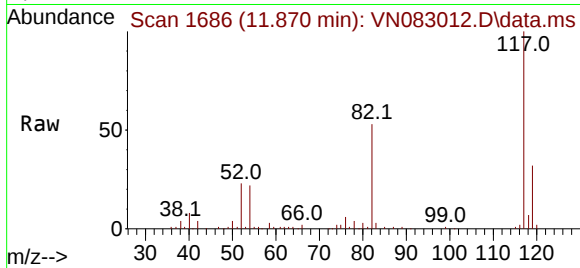

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN083012.D
Acq: 23 Jul 2024 15:07

Tgt Ion:152 Resp: 54995
Ion Ratio Lower Upper
152 100
115 58.7 30.6 91.6
150 158.7 0.0 348.6

