
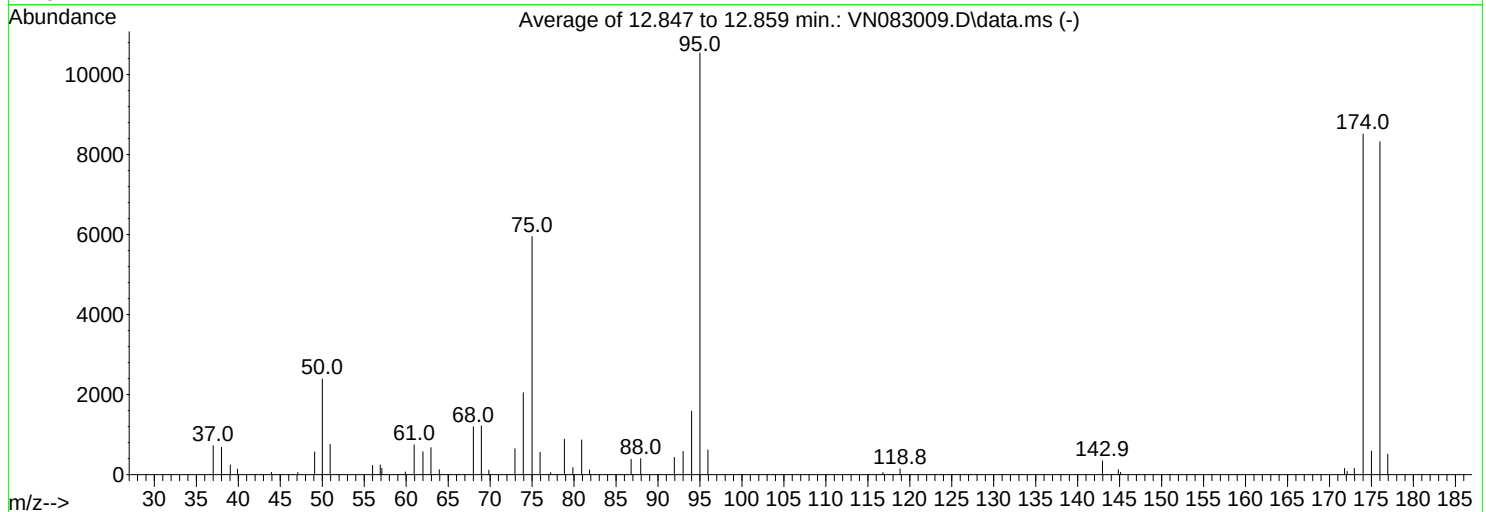


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072324\
Data File : VN083009.D
Acq On : 23 Jul 2024 11:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

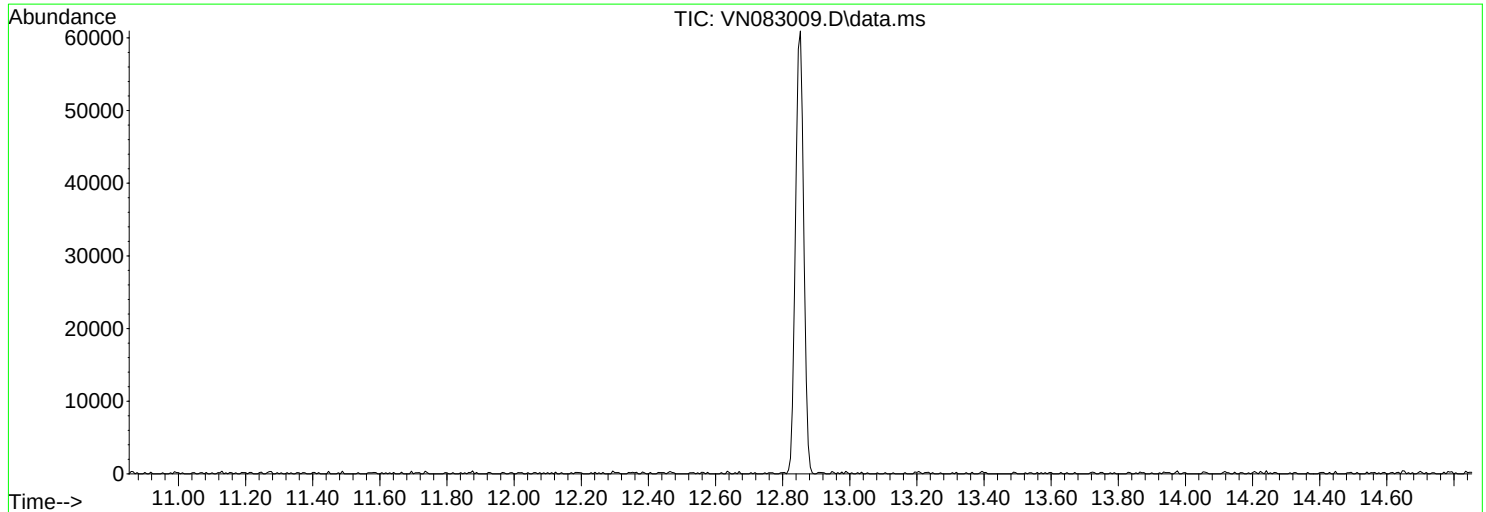

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.7	2390	PASS
75	95	30	60	56.5	5953	PASS
95	95	100	100	100.0	10543	PASS
96	95	5	9	5.9	617	PASS
173	174	0.00	2	1.9	161	PASS
174	95	50	100	80.8	8515	PASS
175	174	5	9	6.9	587	PASS
176	174	95	101	97.8	8324	PASS
177	176	5	9	6.2	512	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
37.00	724	57.10	160	75.00	5953	94.00	158
38.00	685	59.90	70	75.95	561	95.00	1054
39.05	243	60.95	745	77.20	51	95.95	61
39.90	135	62.00	572	78.85	883	116.80	5
43.95	55	62.95	677	79.85	176	118.85	149
47.10	56	63.95	126	80.90	868	142.95	345
49.10	568	68.00	1199	81.85	117	144.85	126
50.00	2390	68.95	1220	86.80	384	145.10	58
50.95	761	69.85	111	87.95	402	171.80	158
56.00	233	72.95	650	91.95	433	172.10	79
56.90	242	73.95	2048	93.00	580	172.95	161

Average of 12.847 to 12.859 min.: VN083009.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
174.00	8515						
175.00	587						
176.00	8324						
176.95	512						

Instrument :

MSVOA_N

ClientSampleId :

BFB