


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072325\
Data File : VN087398.D
Acq On : 23 Jul 2025 09:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N072325W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Jul 24 05:11:26 2025

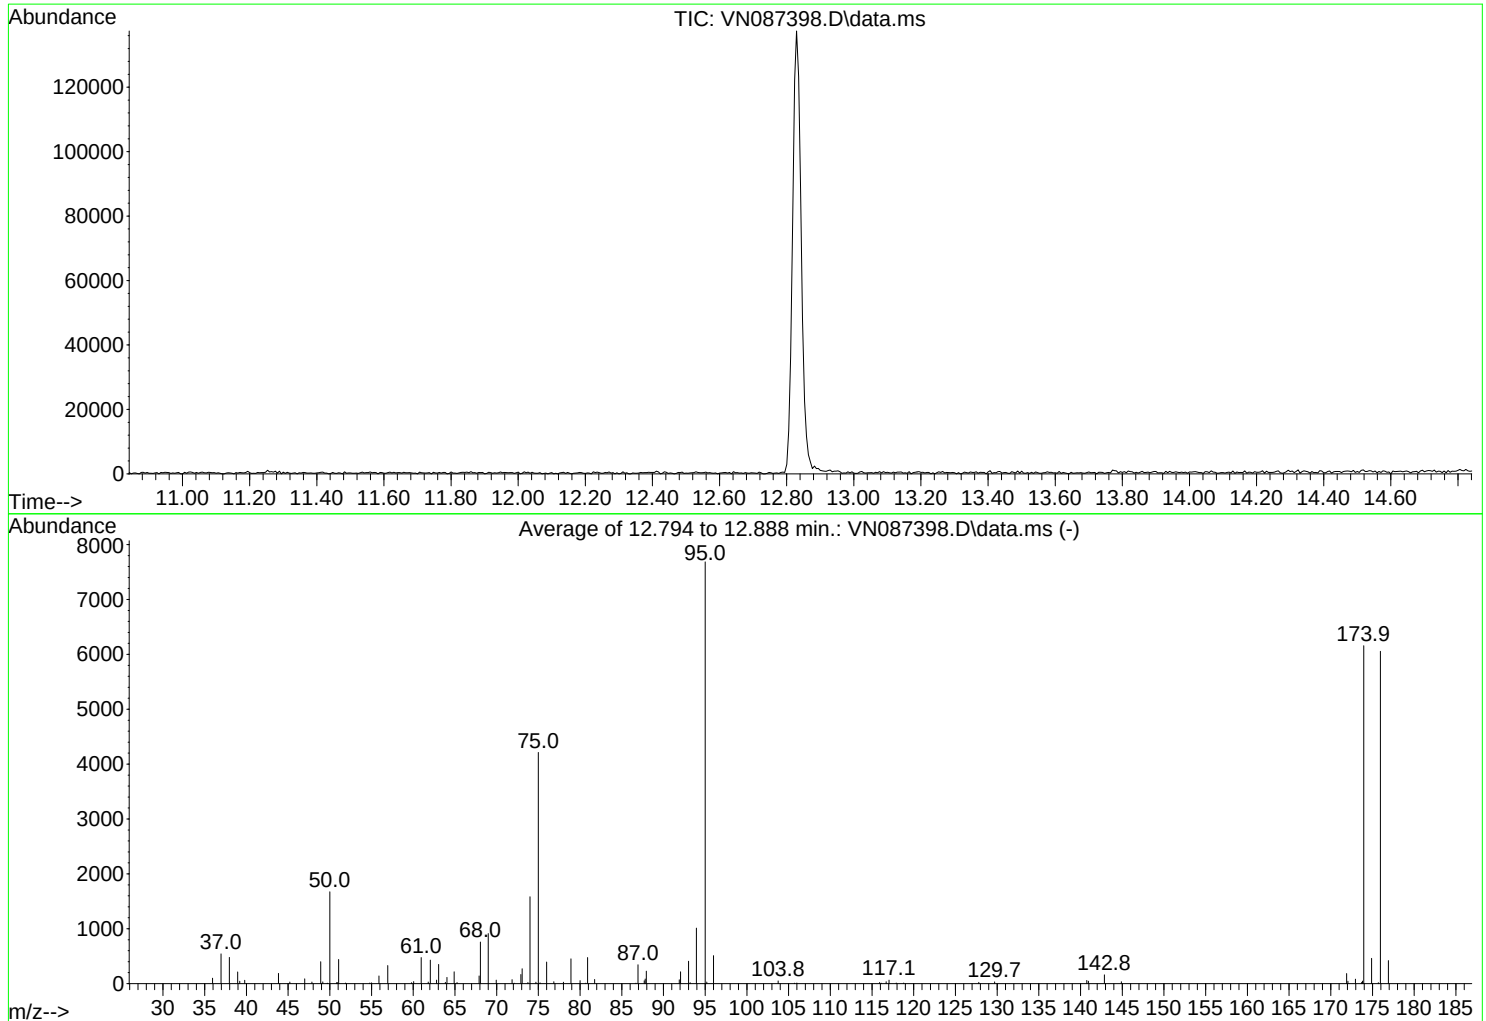

AutoFind: Averaged scan 1843 to 1859; Bkg corrected with scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.8	1673	PASS
75	95	30	60	54.8	4212	PASS
95	95	100	100	100.0	7686	PASS
96	95	5	9	6.6	511	PASS
173	174	0.00	2	1.3	83	PASS
174	95	50	100	80.1	6157	PASS
175	174	5	9	7.5	460	PASS
176	174	95	101	98.3	6055	PASS
177	176	5	9	6.9	420	PASS