




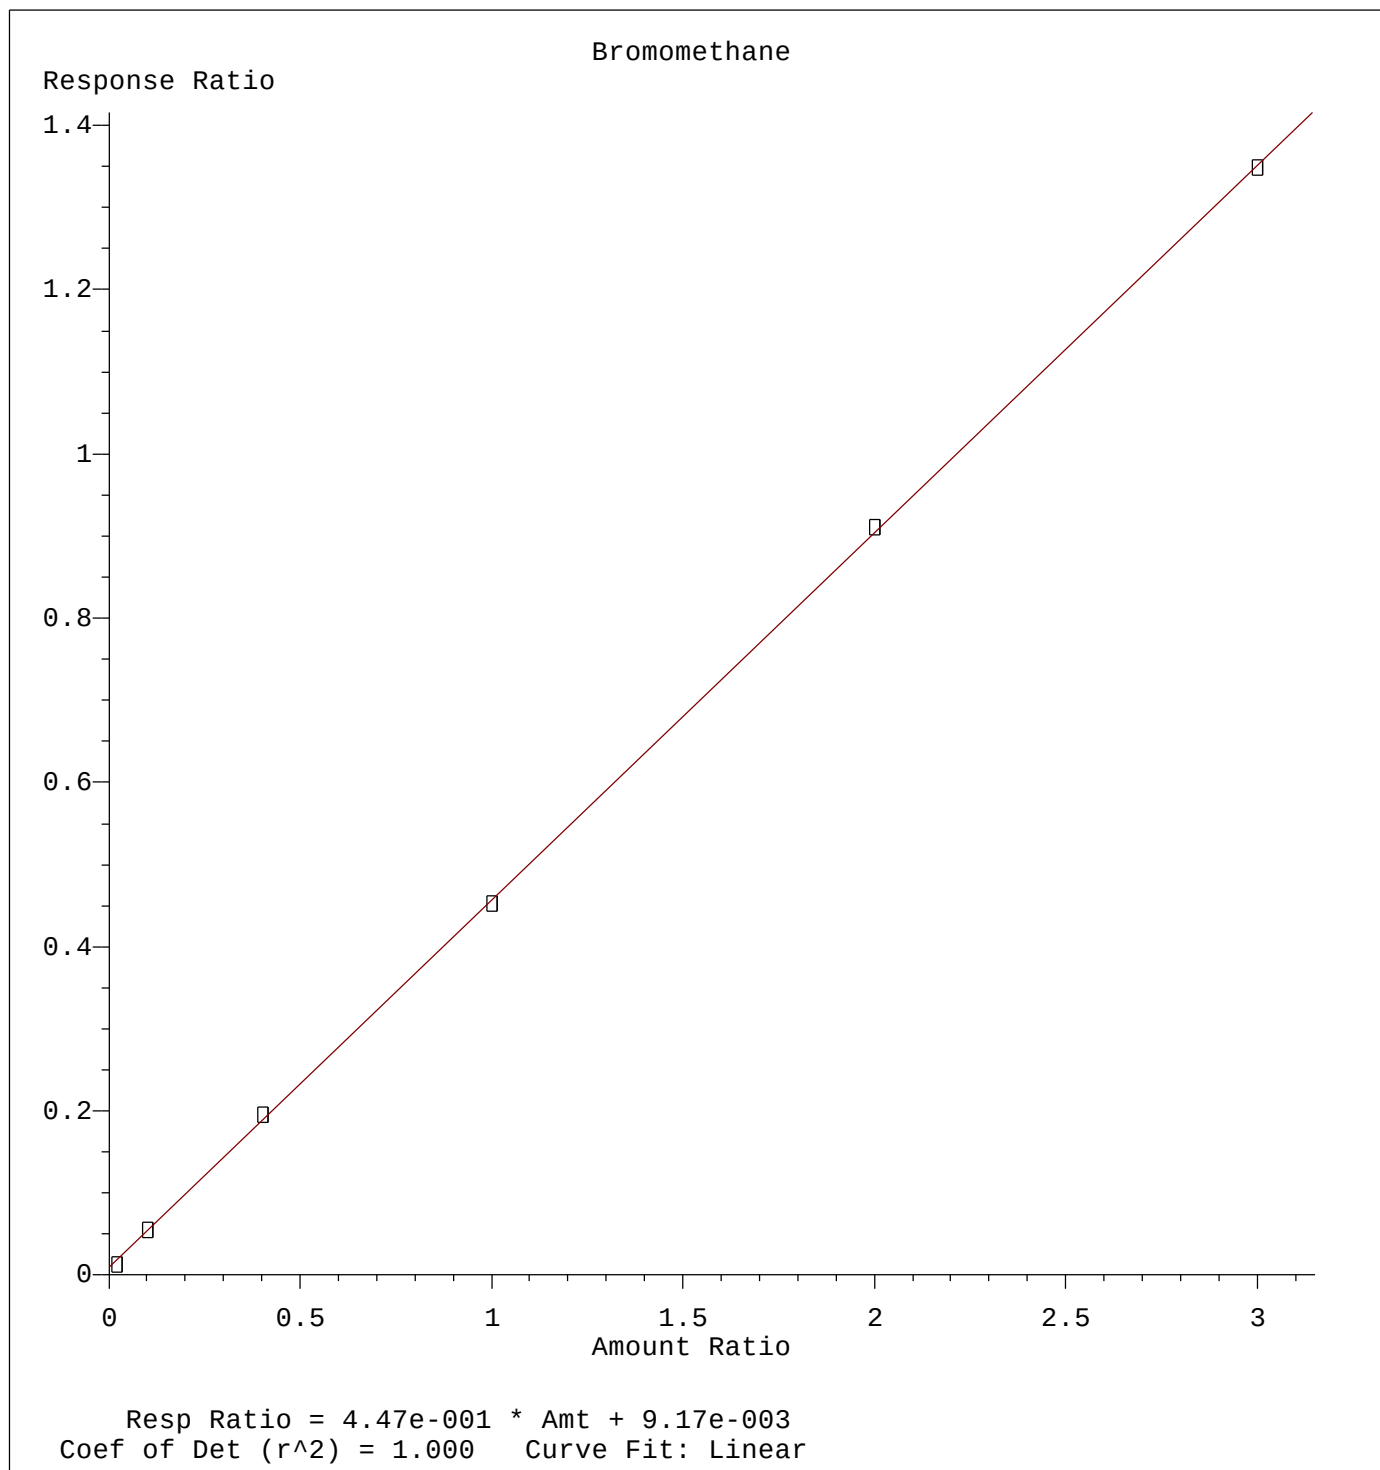


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

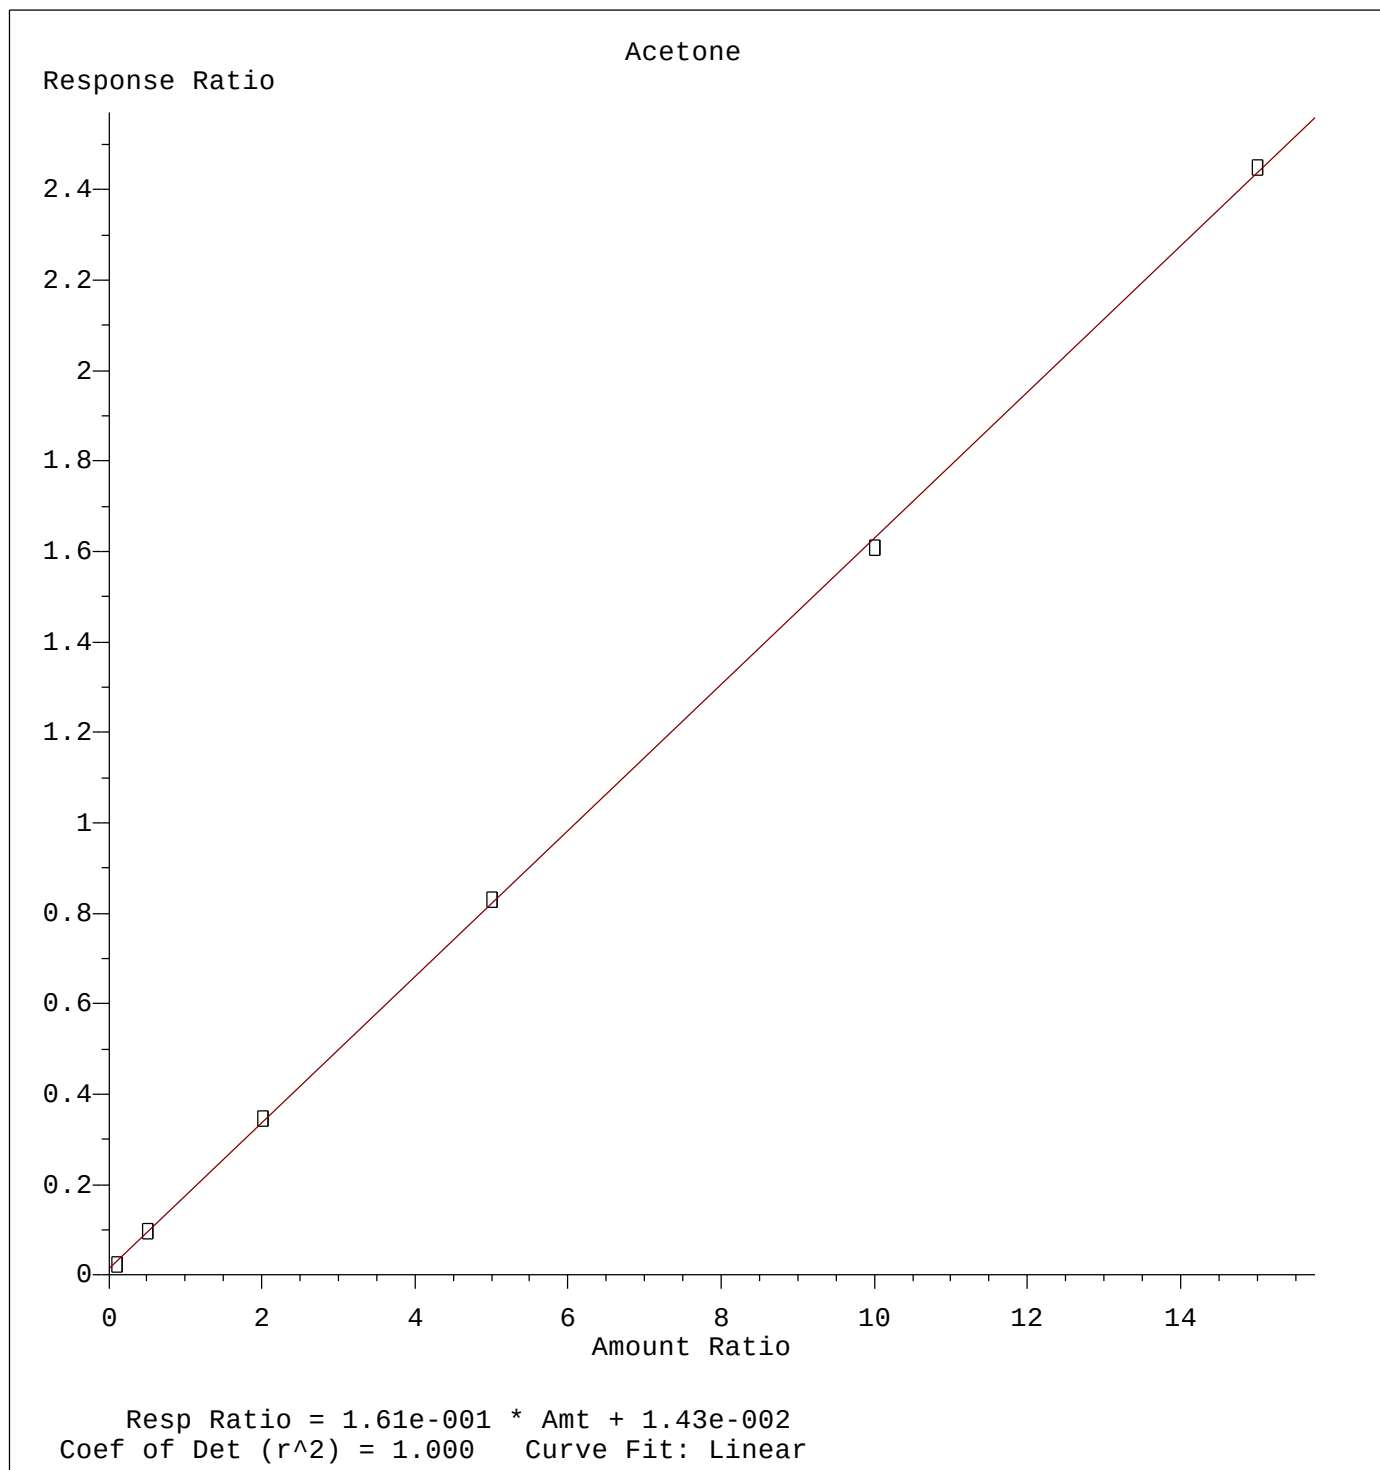


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

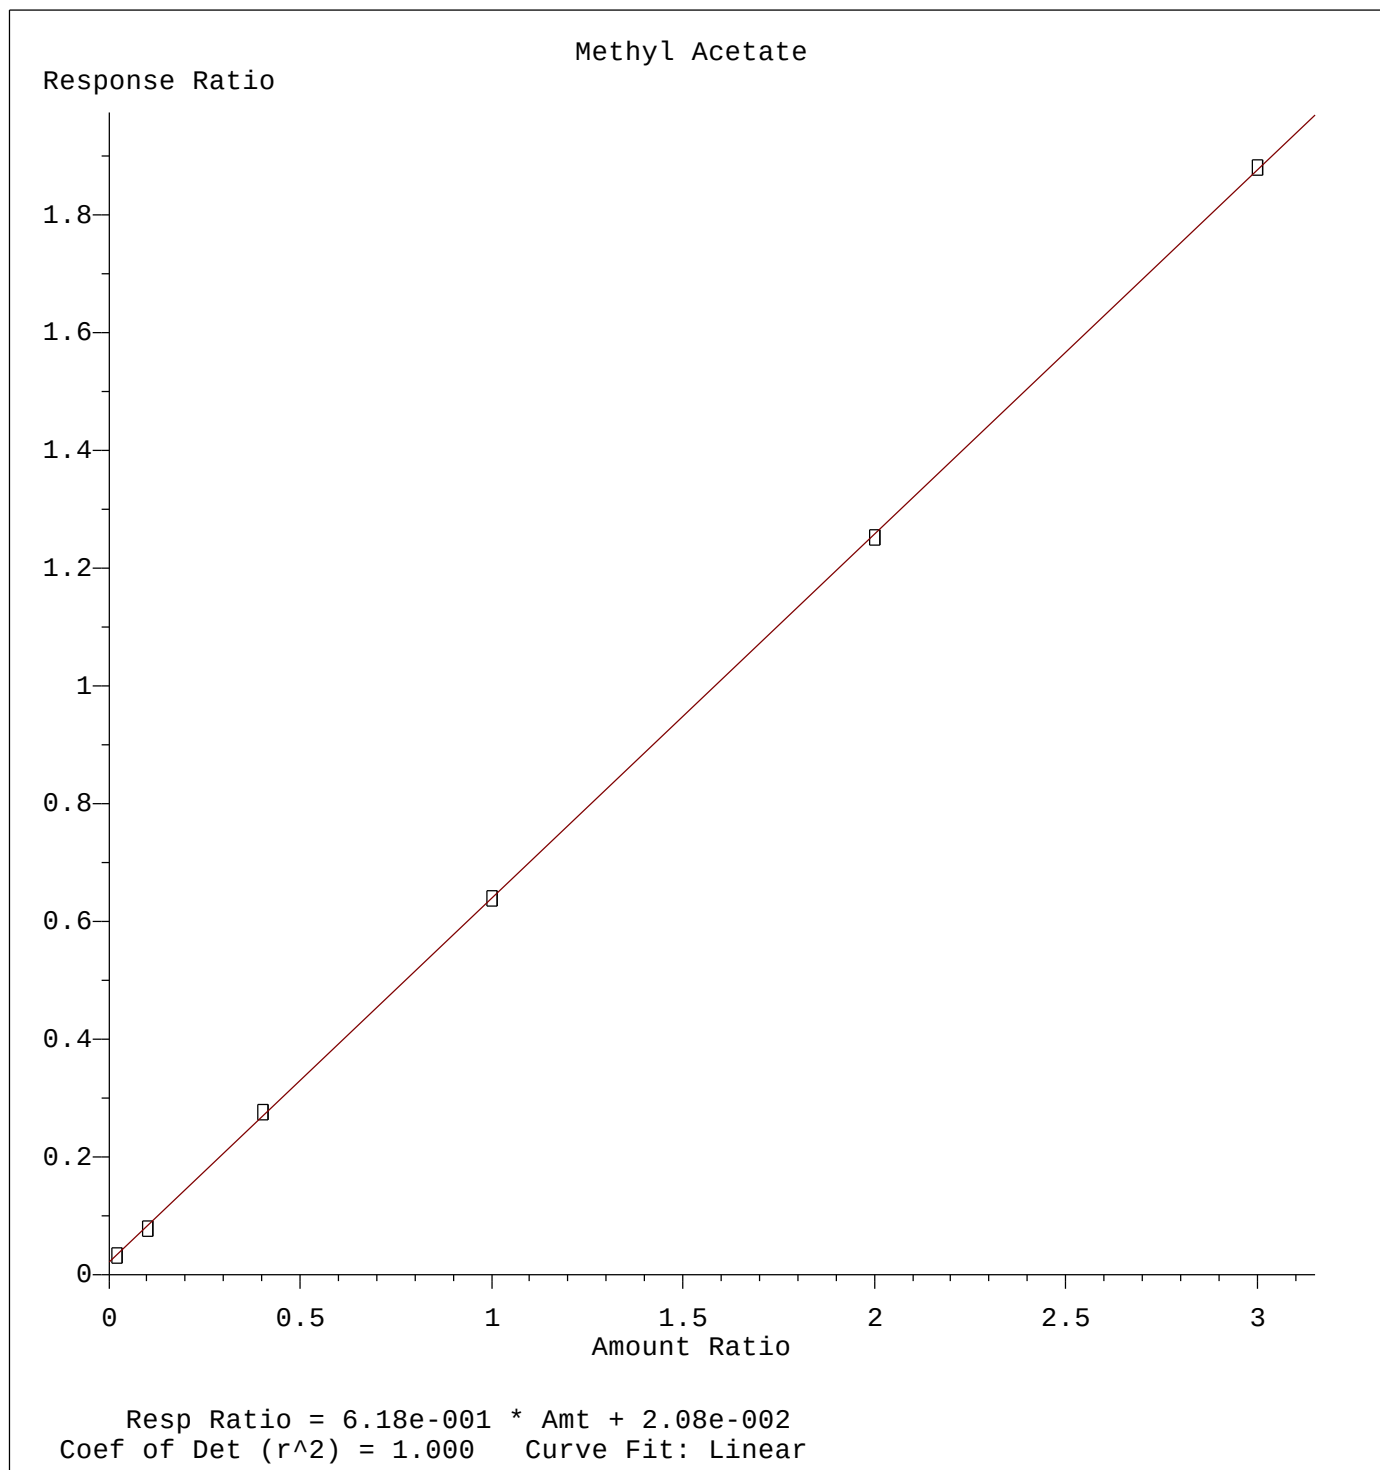


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

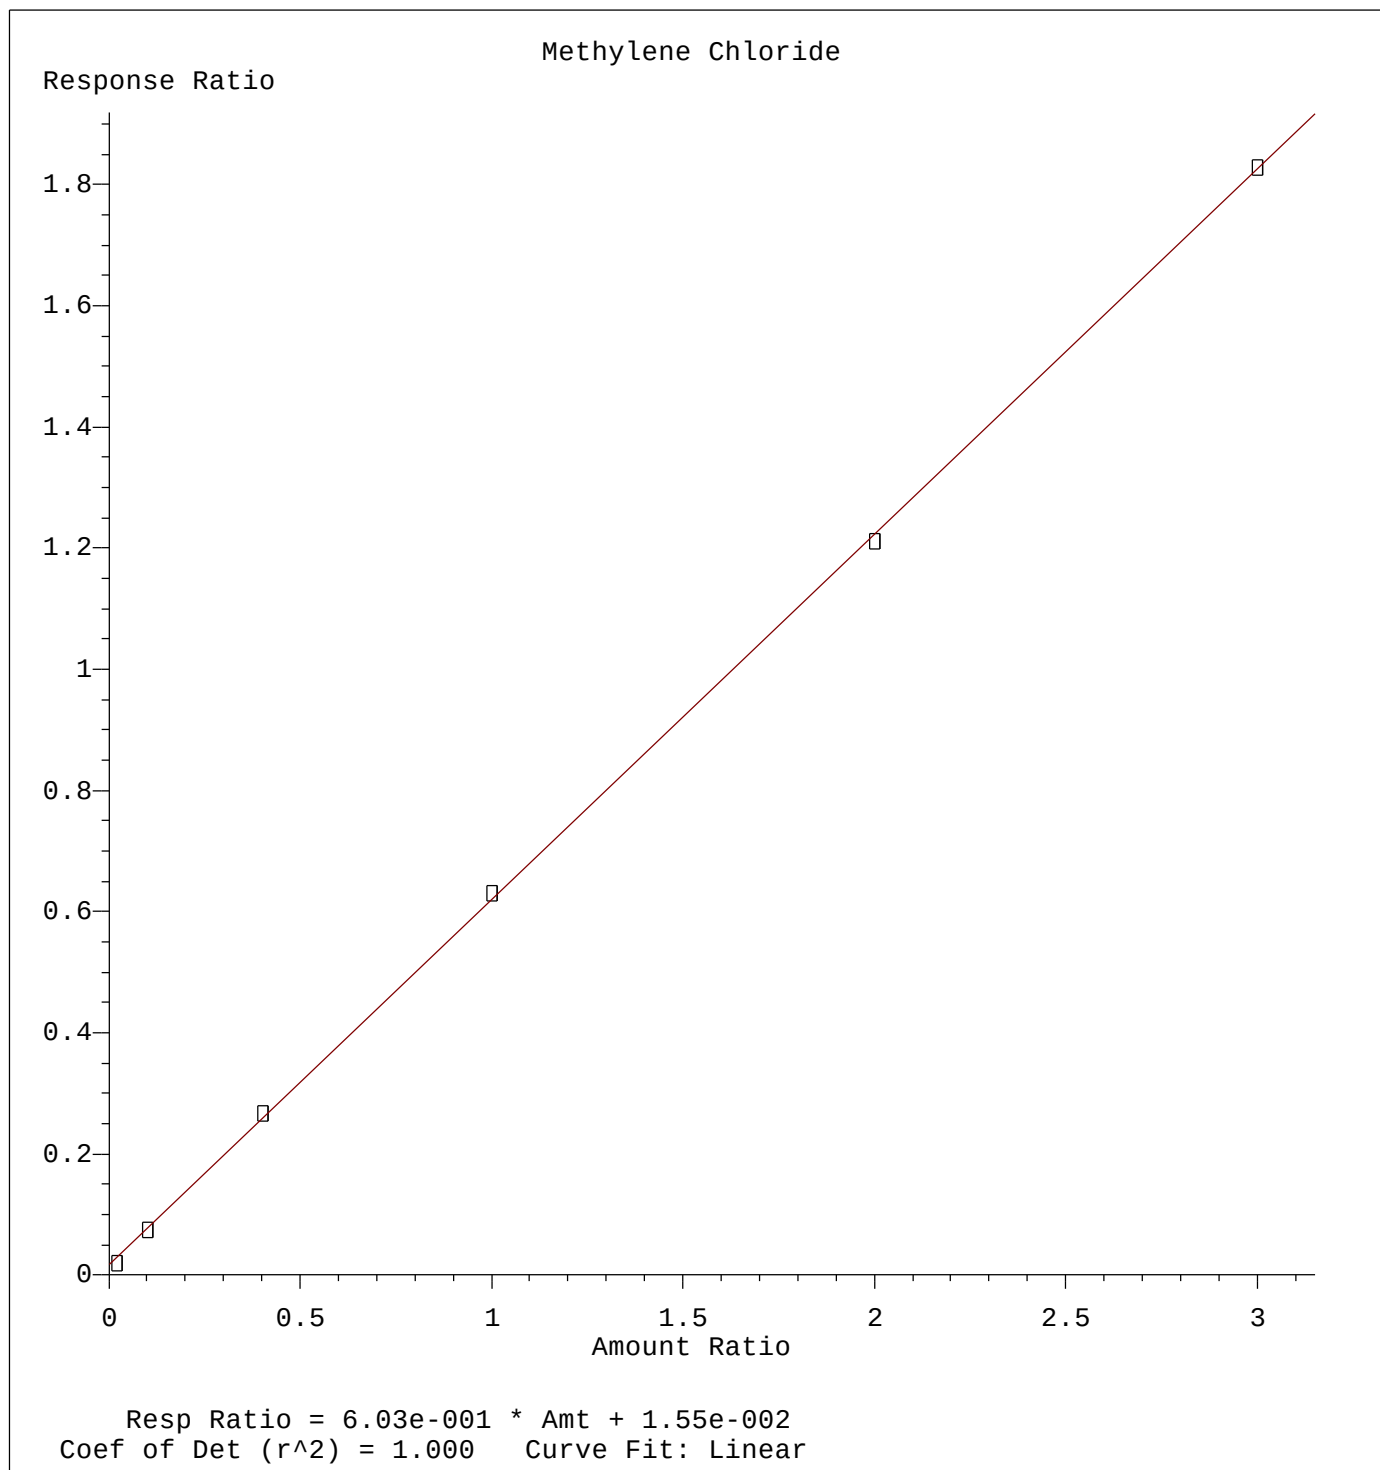

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

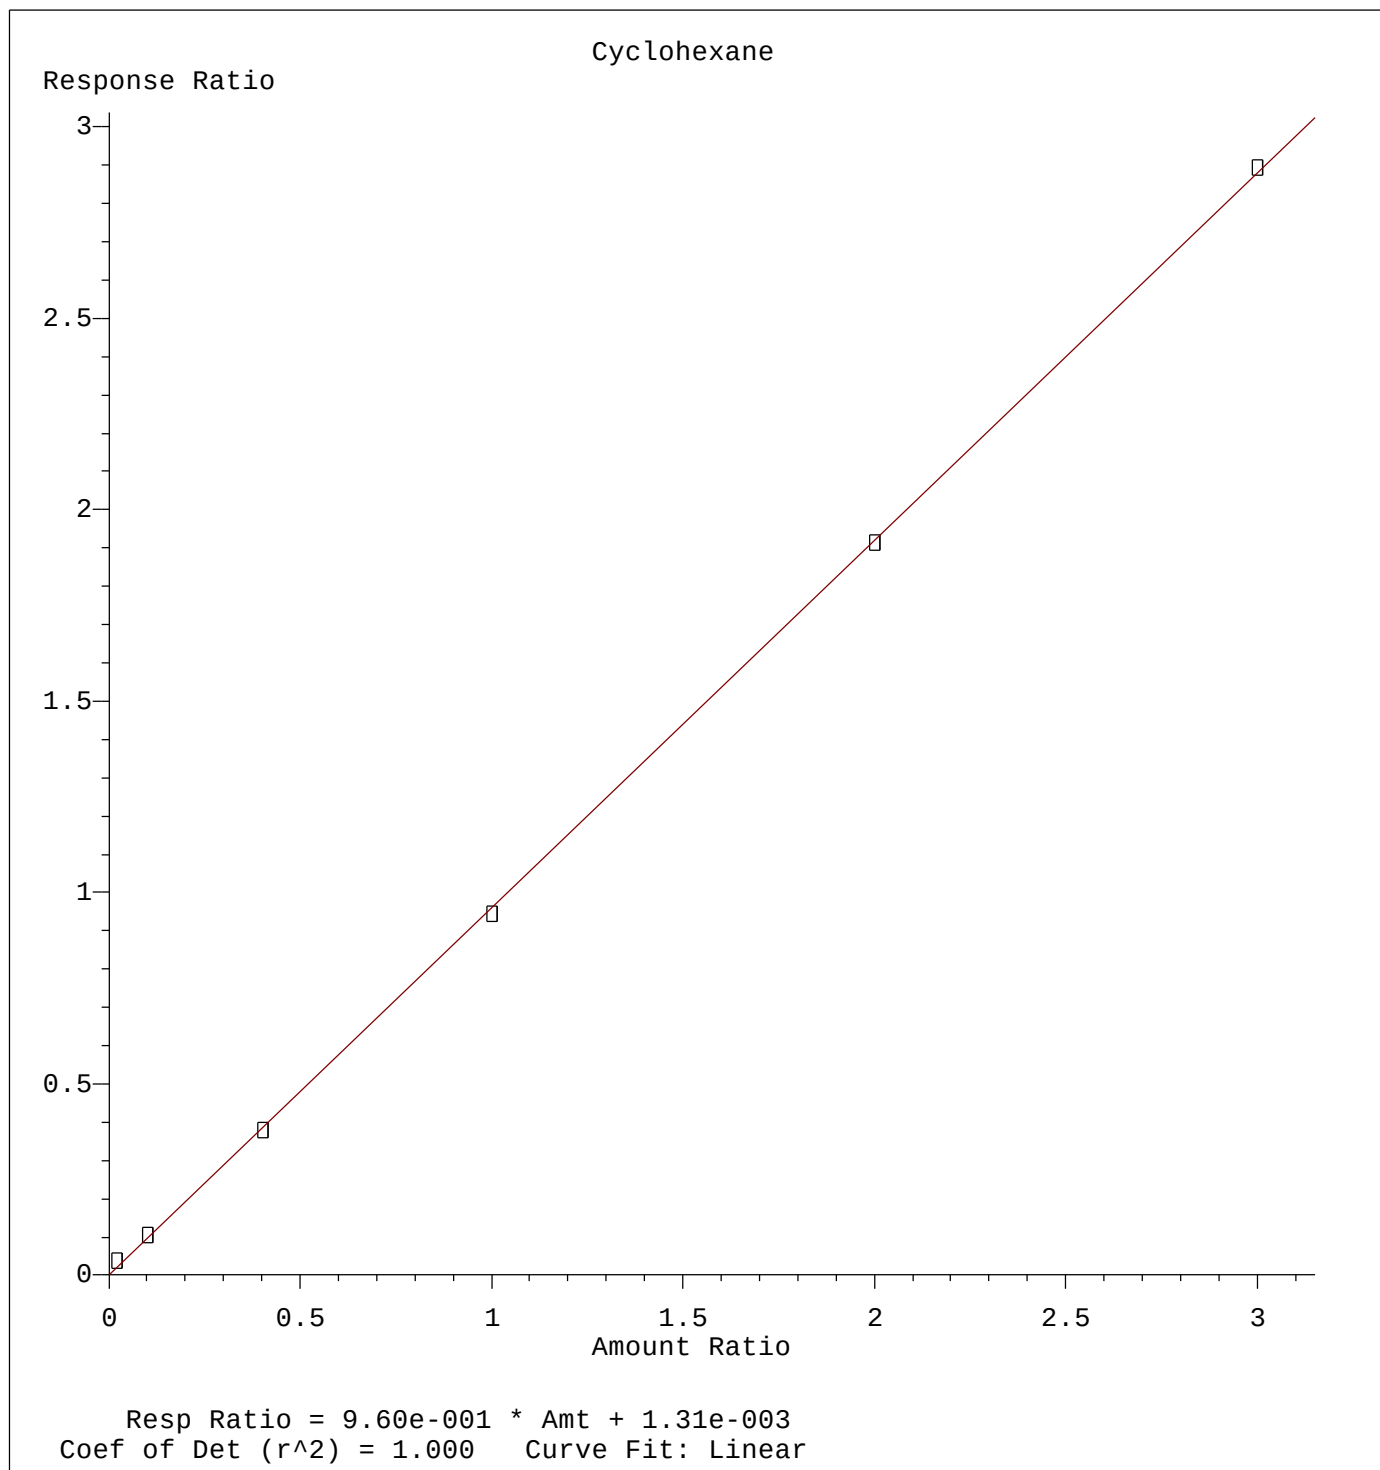


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

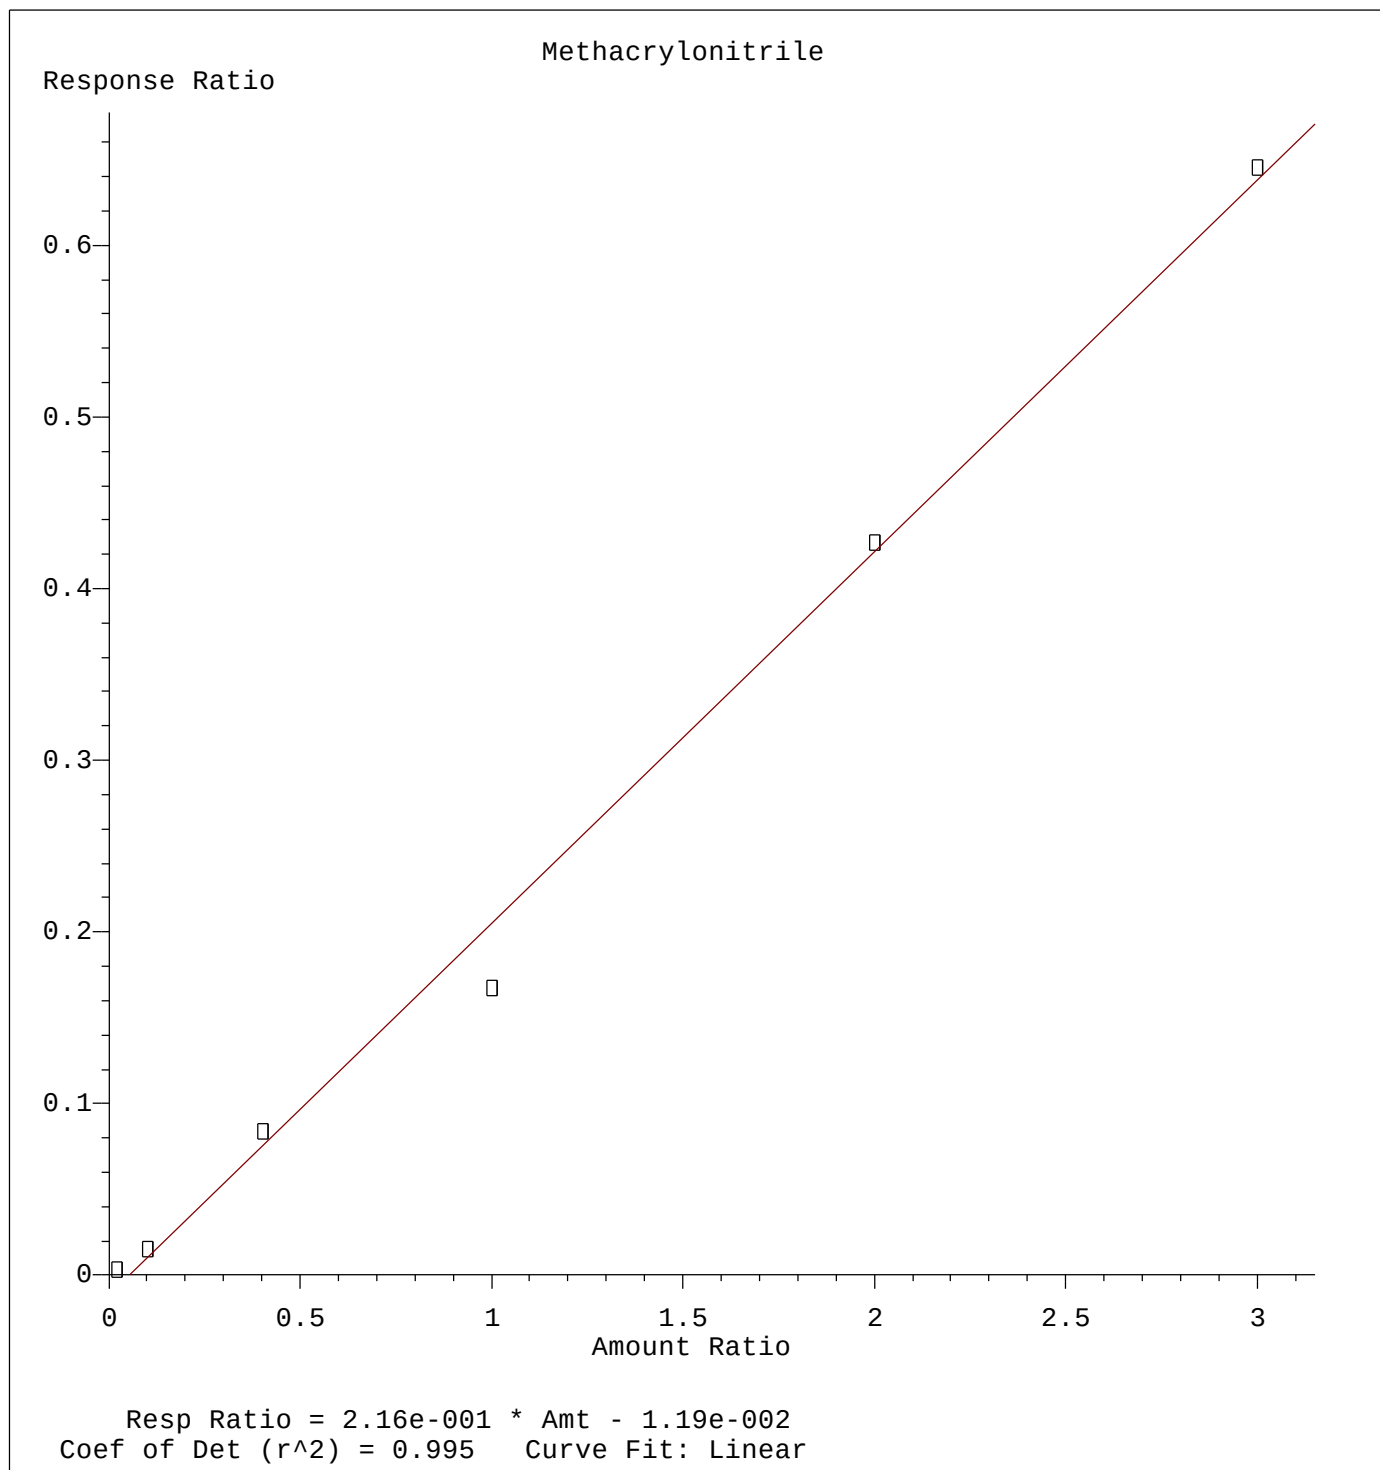

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018


Isopropyl Acetate

Response Ratio

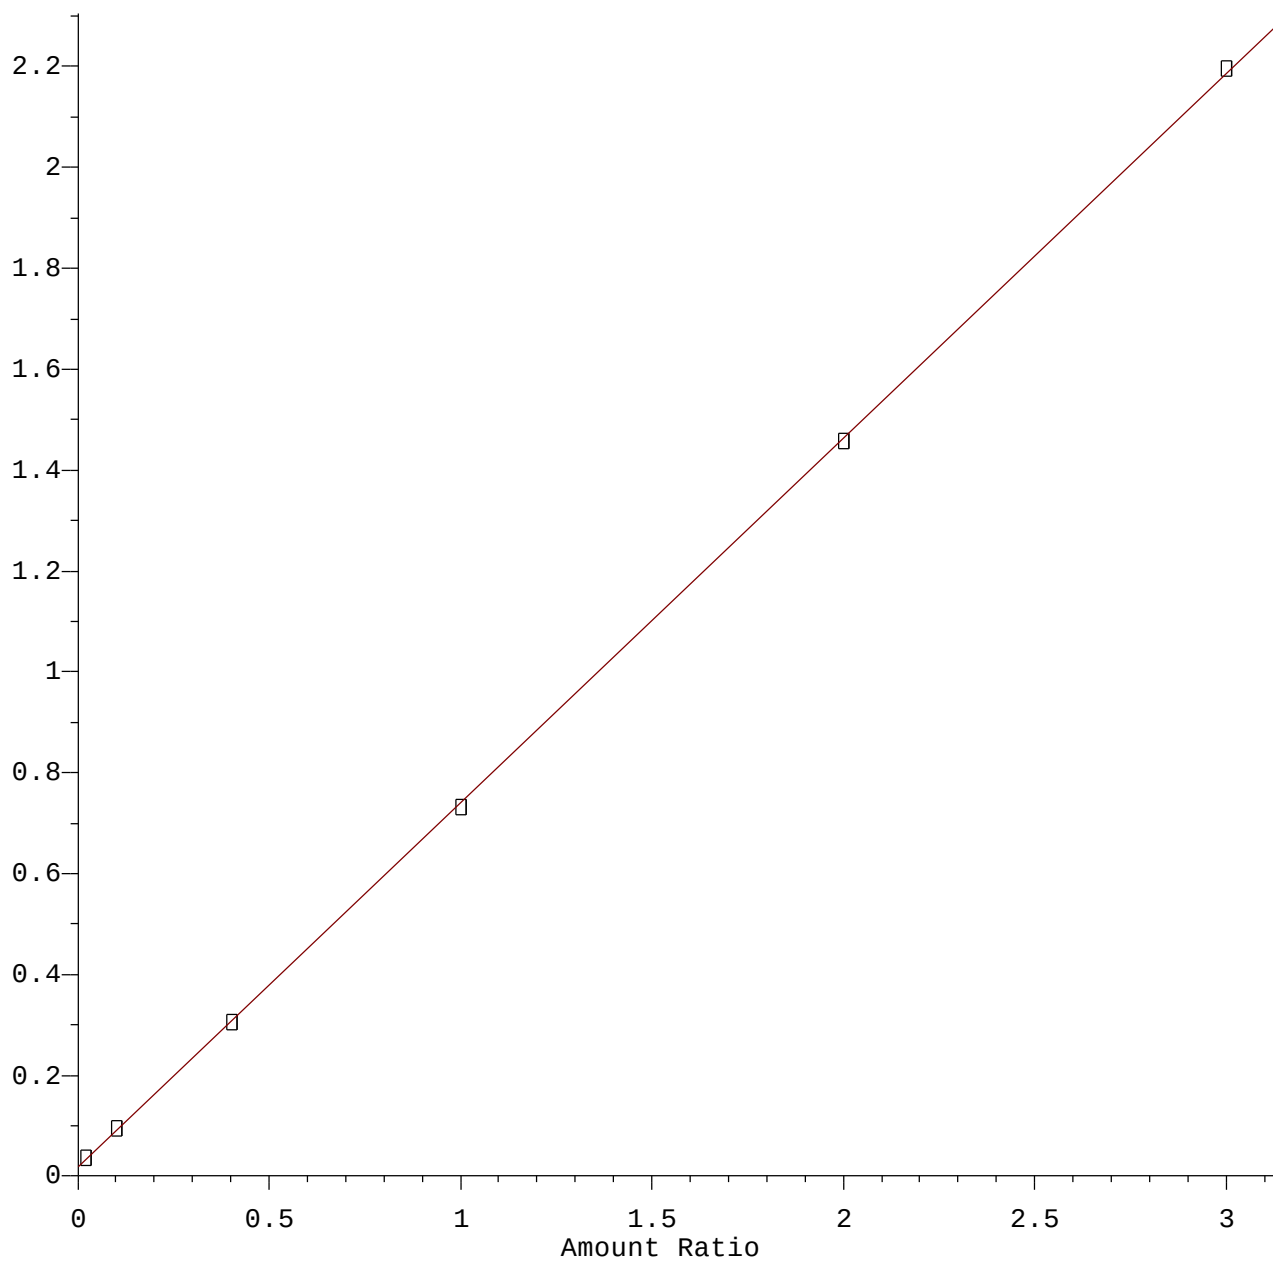

Resp Ratio = 7.23e-001 * Amt + 1.69e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

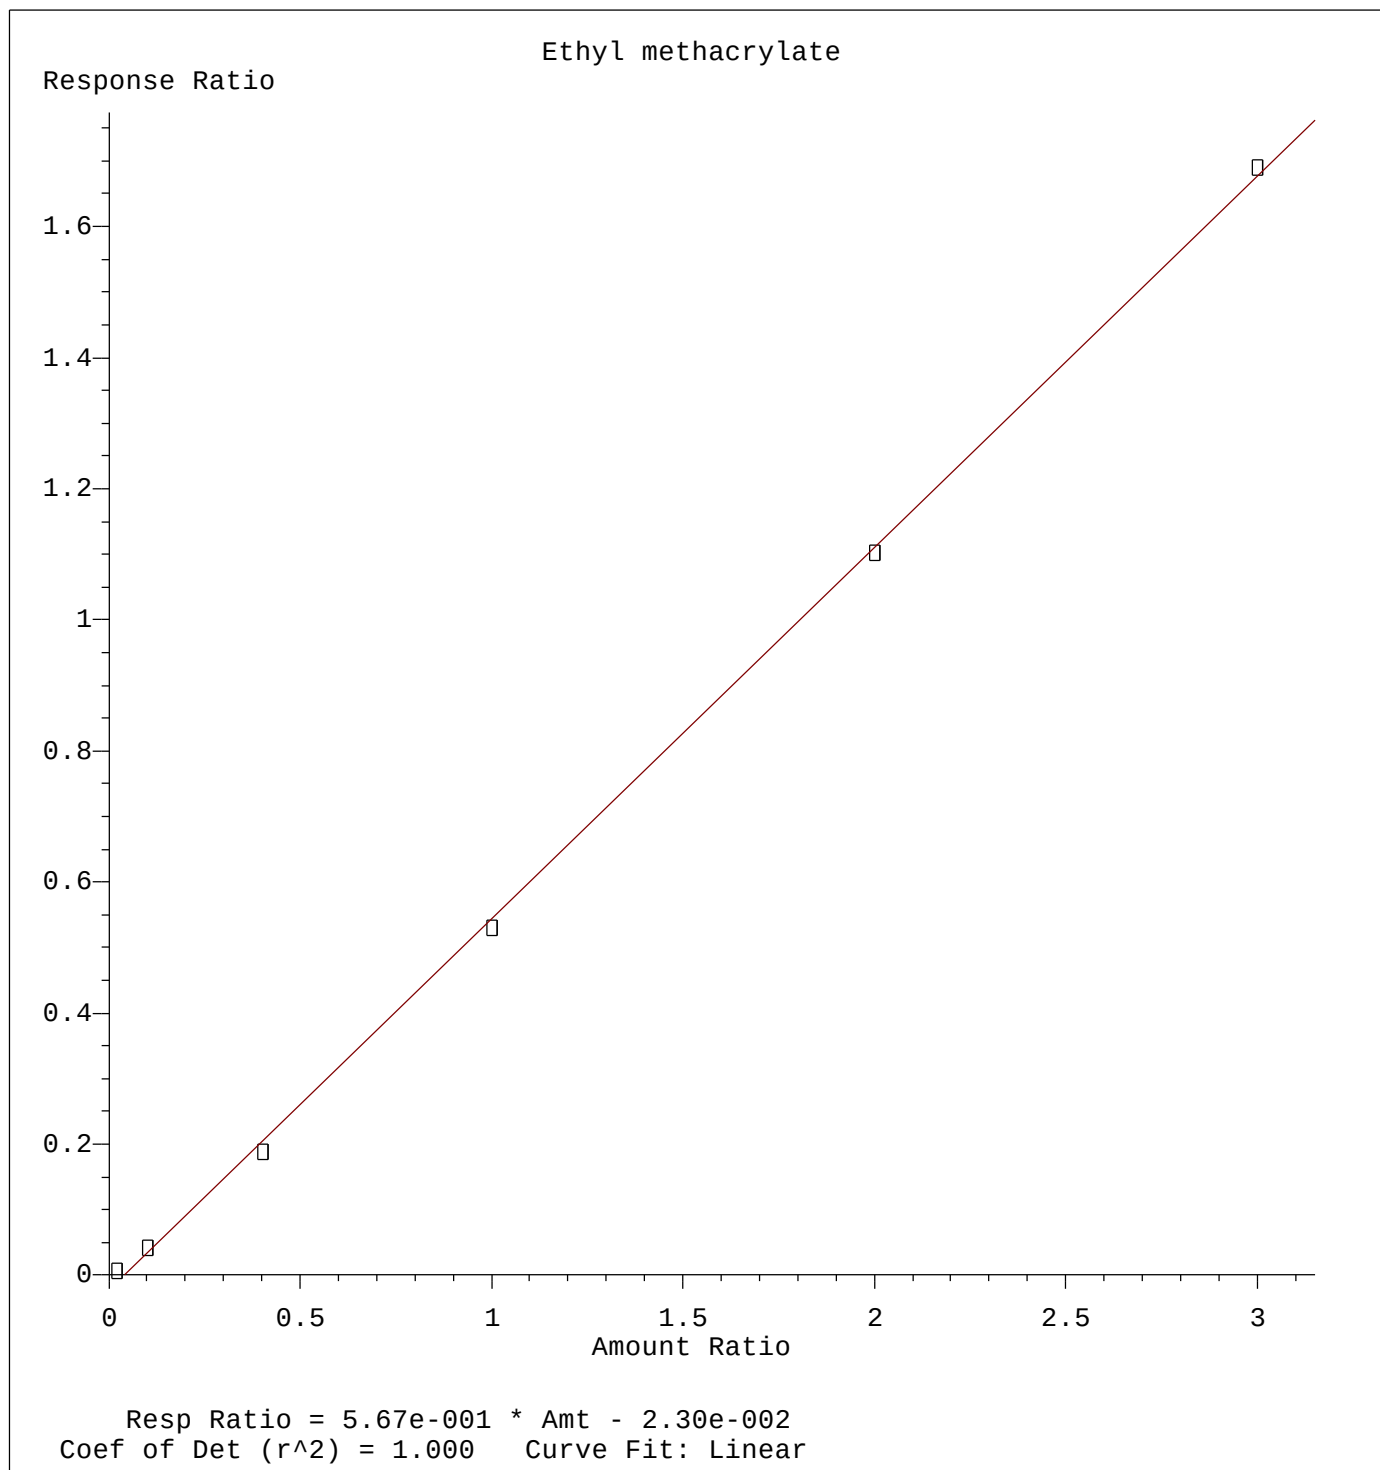

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

2-Chloroethyl Vinyl ether

Response Ratio

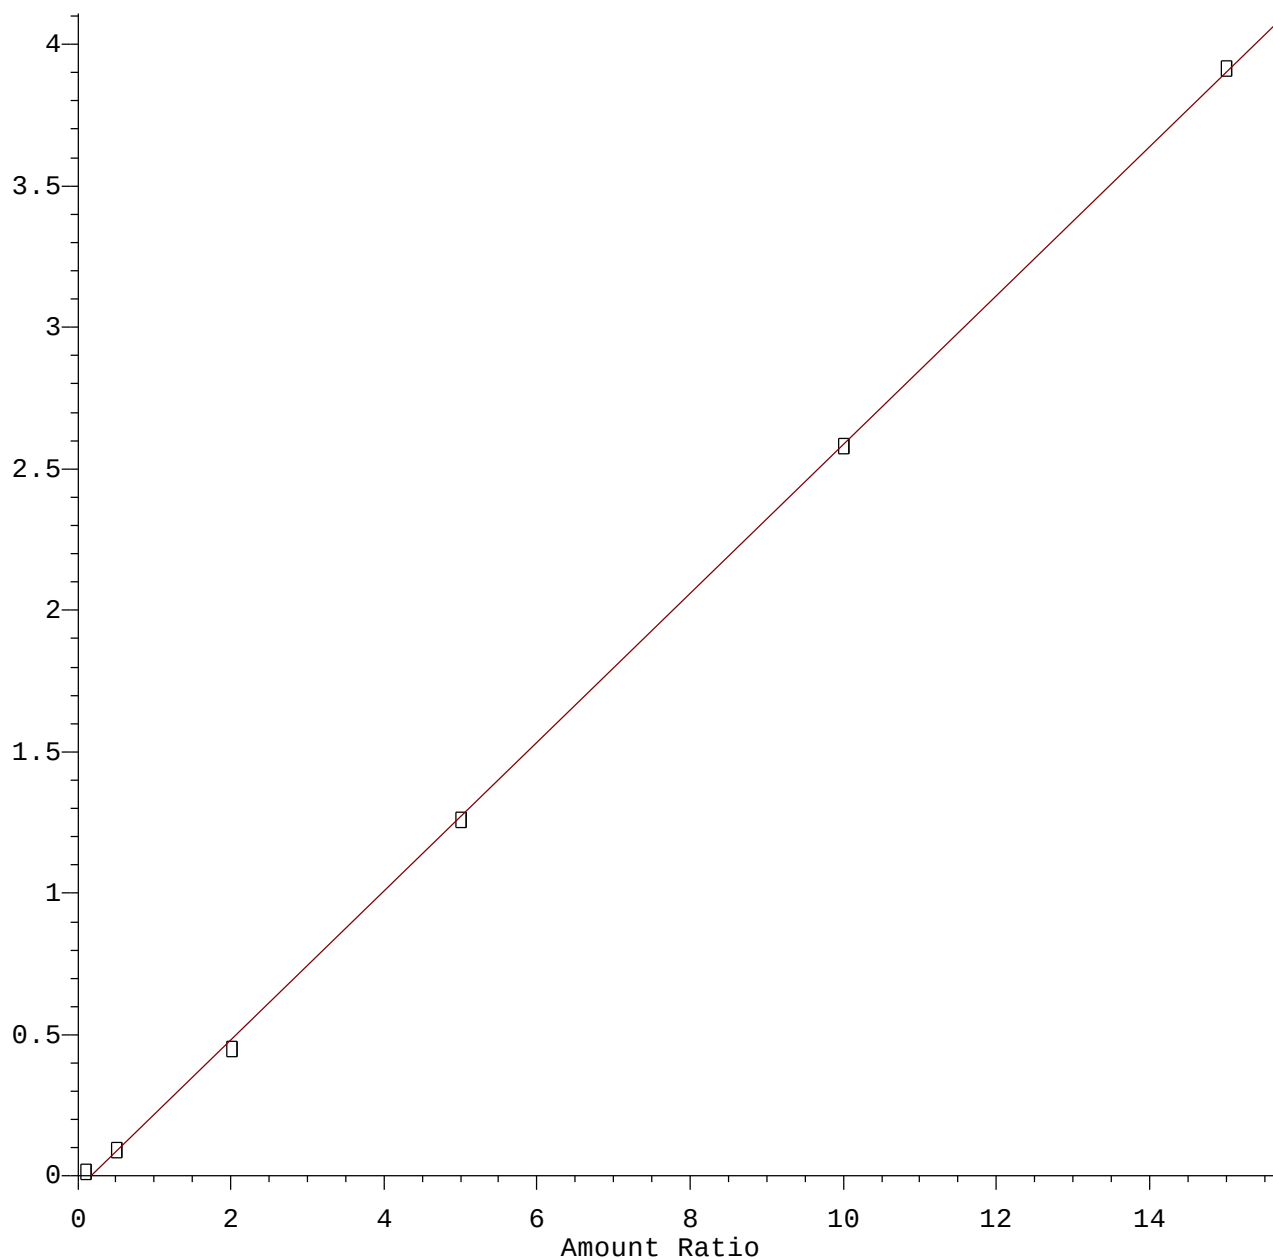


Resp Ratio = $2.63 \times 10^{-1} \times \text{Amt} - 4.48 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018


2-Hexanone

Response Ratio

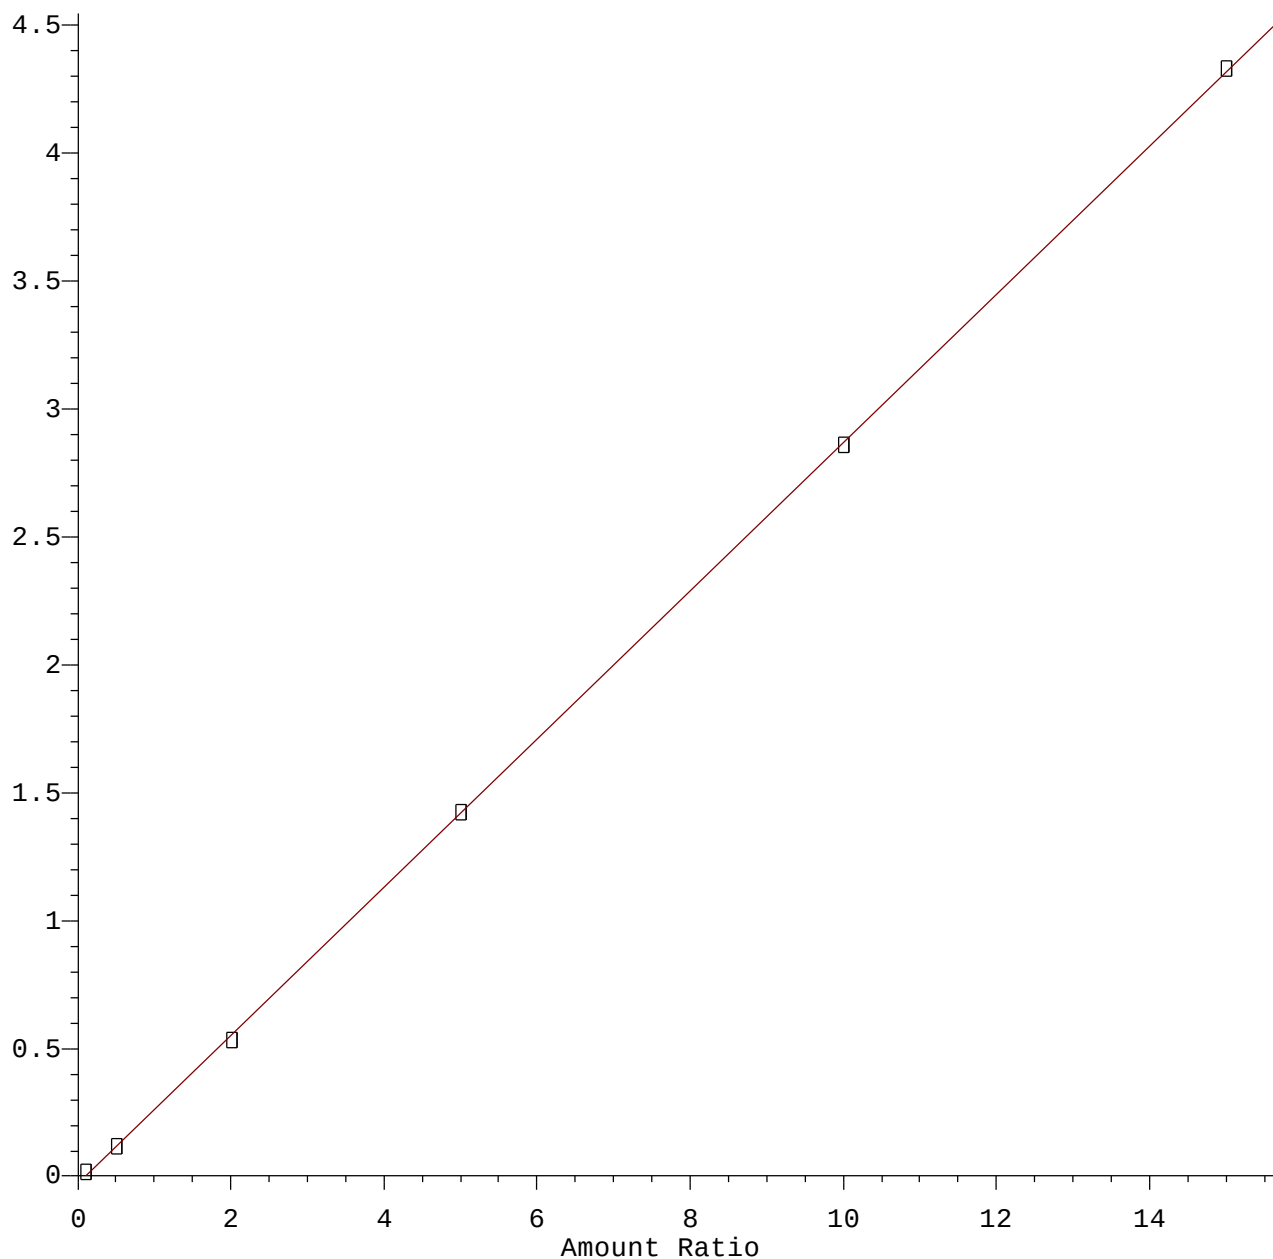

Resp Ratio = $2.90 \times 10^{-1} \times \text{Amt} - 3.00 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

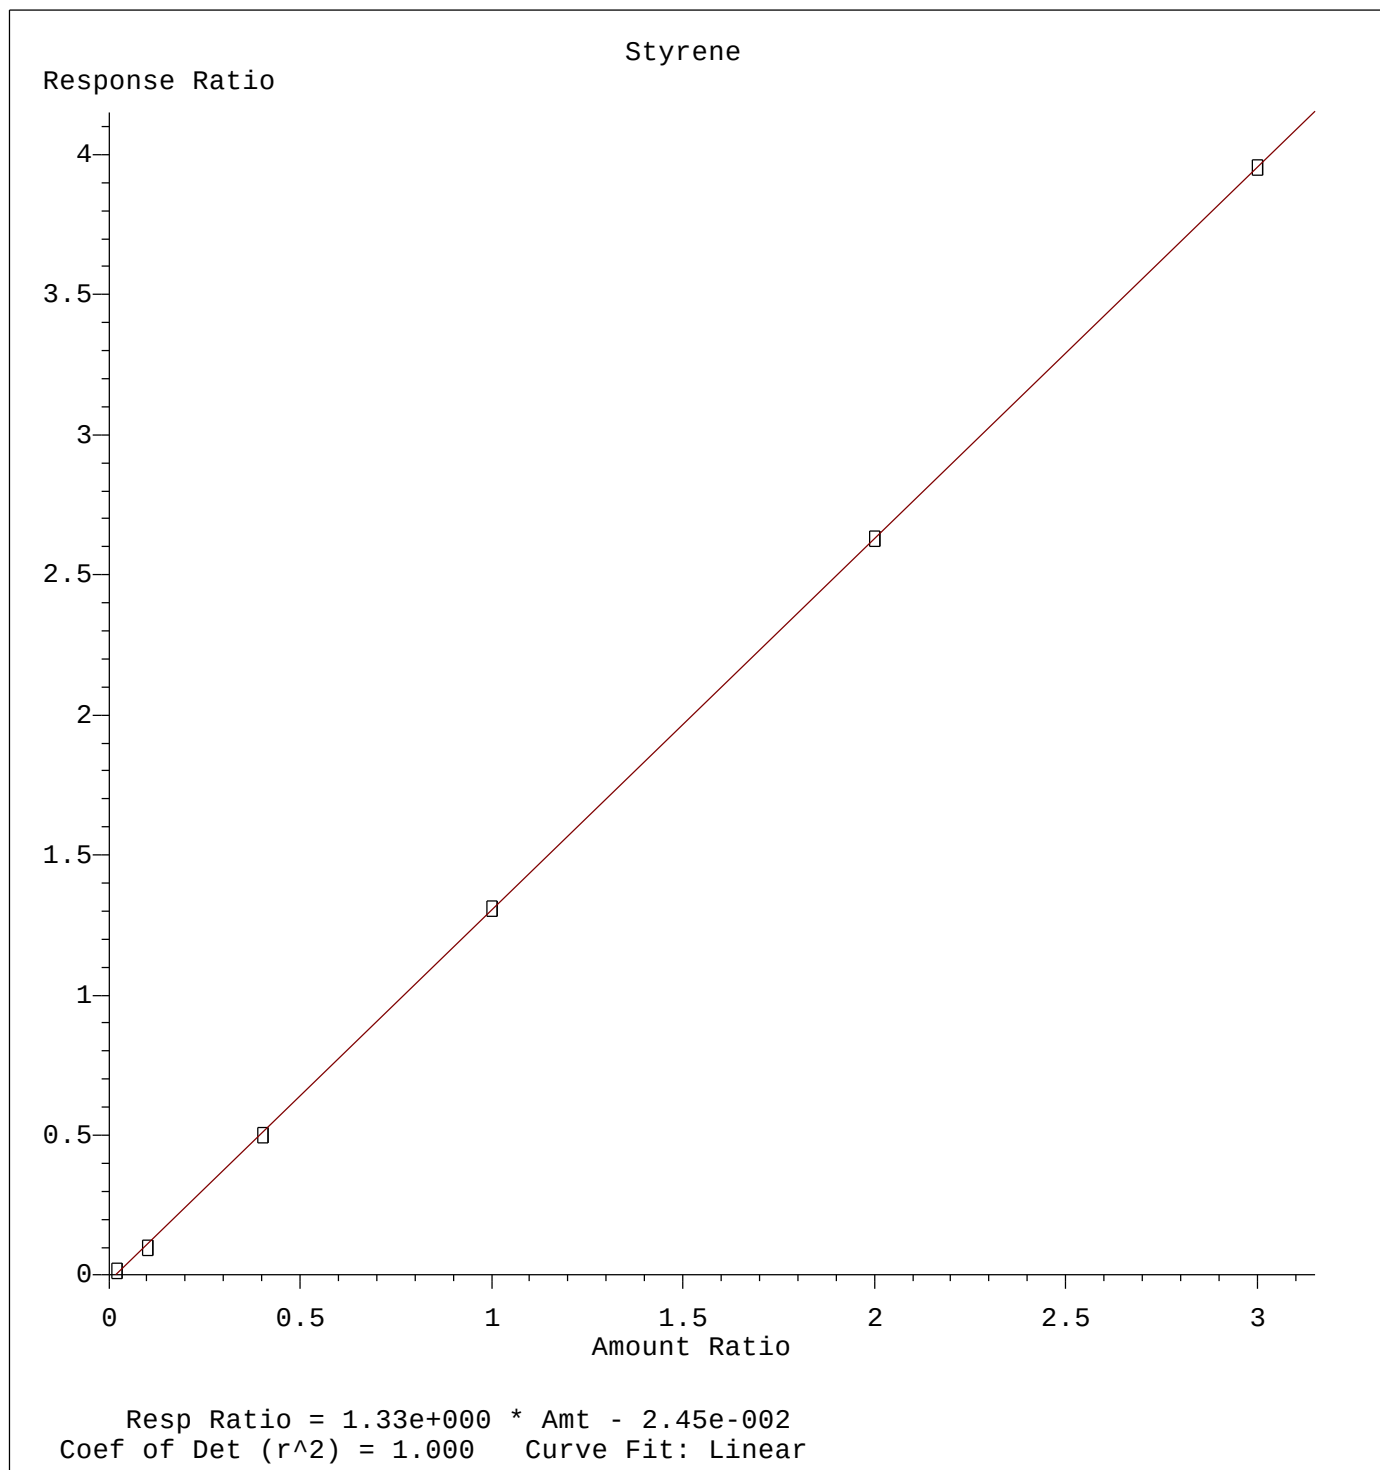

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018


1,1,2,2-Tetrachloroethane

Response Ratio

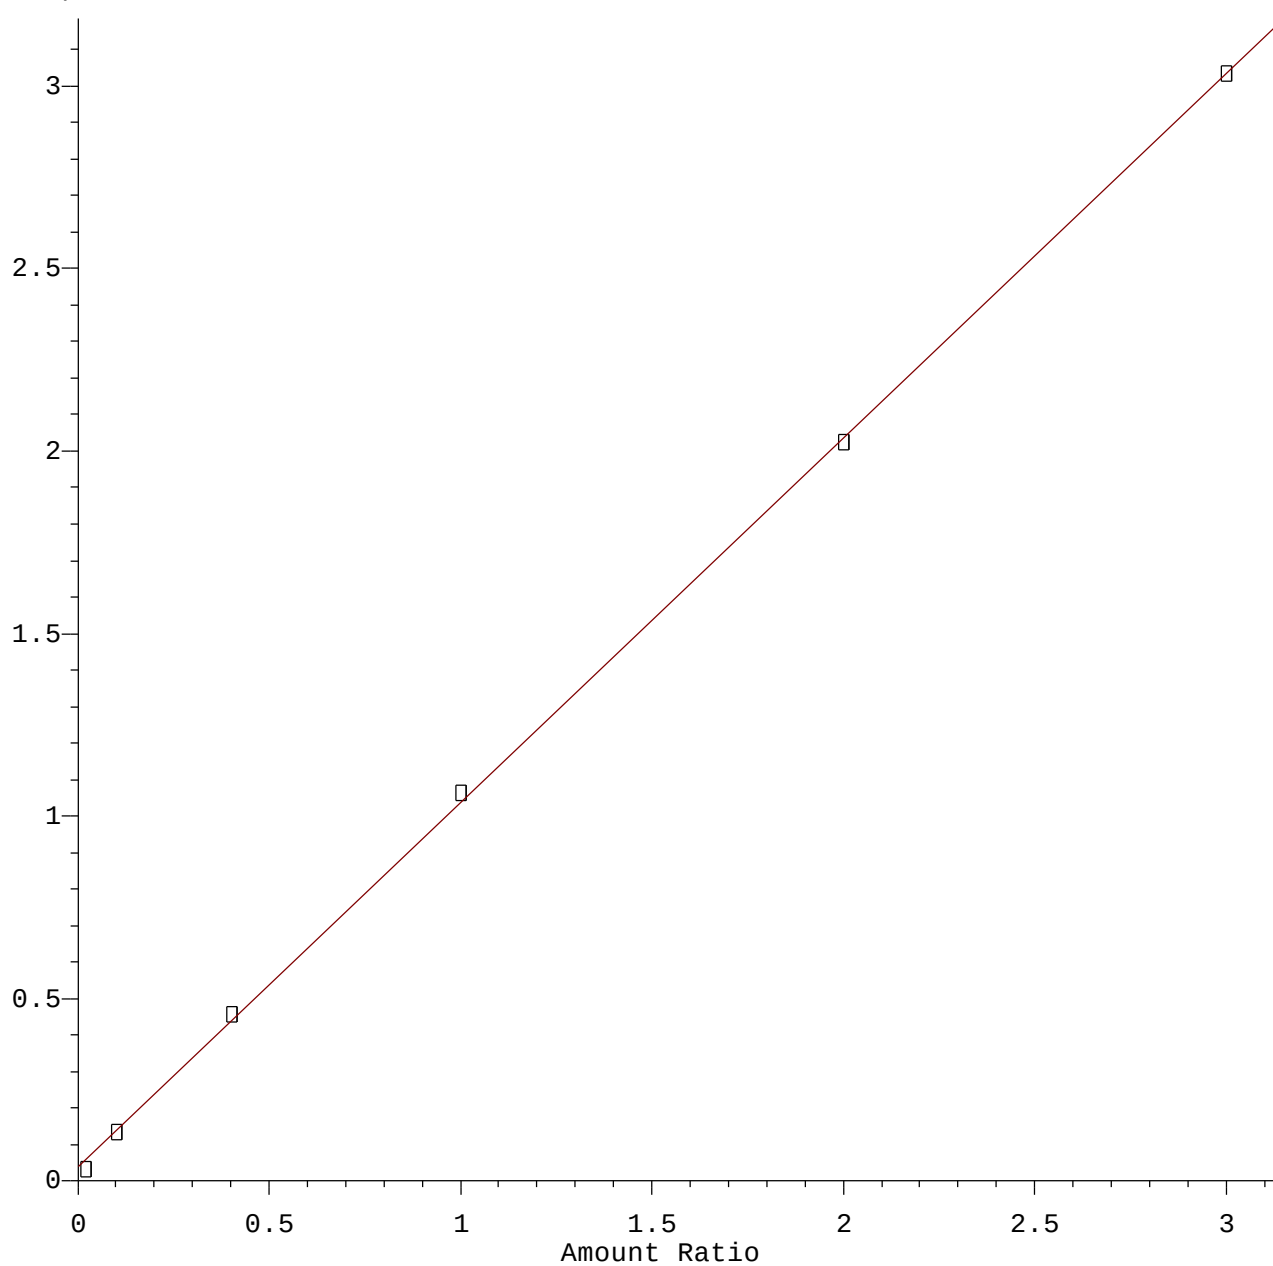

Resp Ratio = 9.99e-001 * Amt + 3.66e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

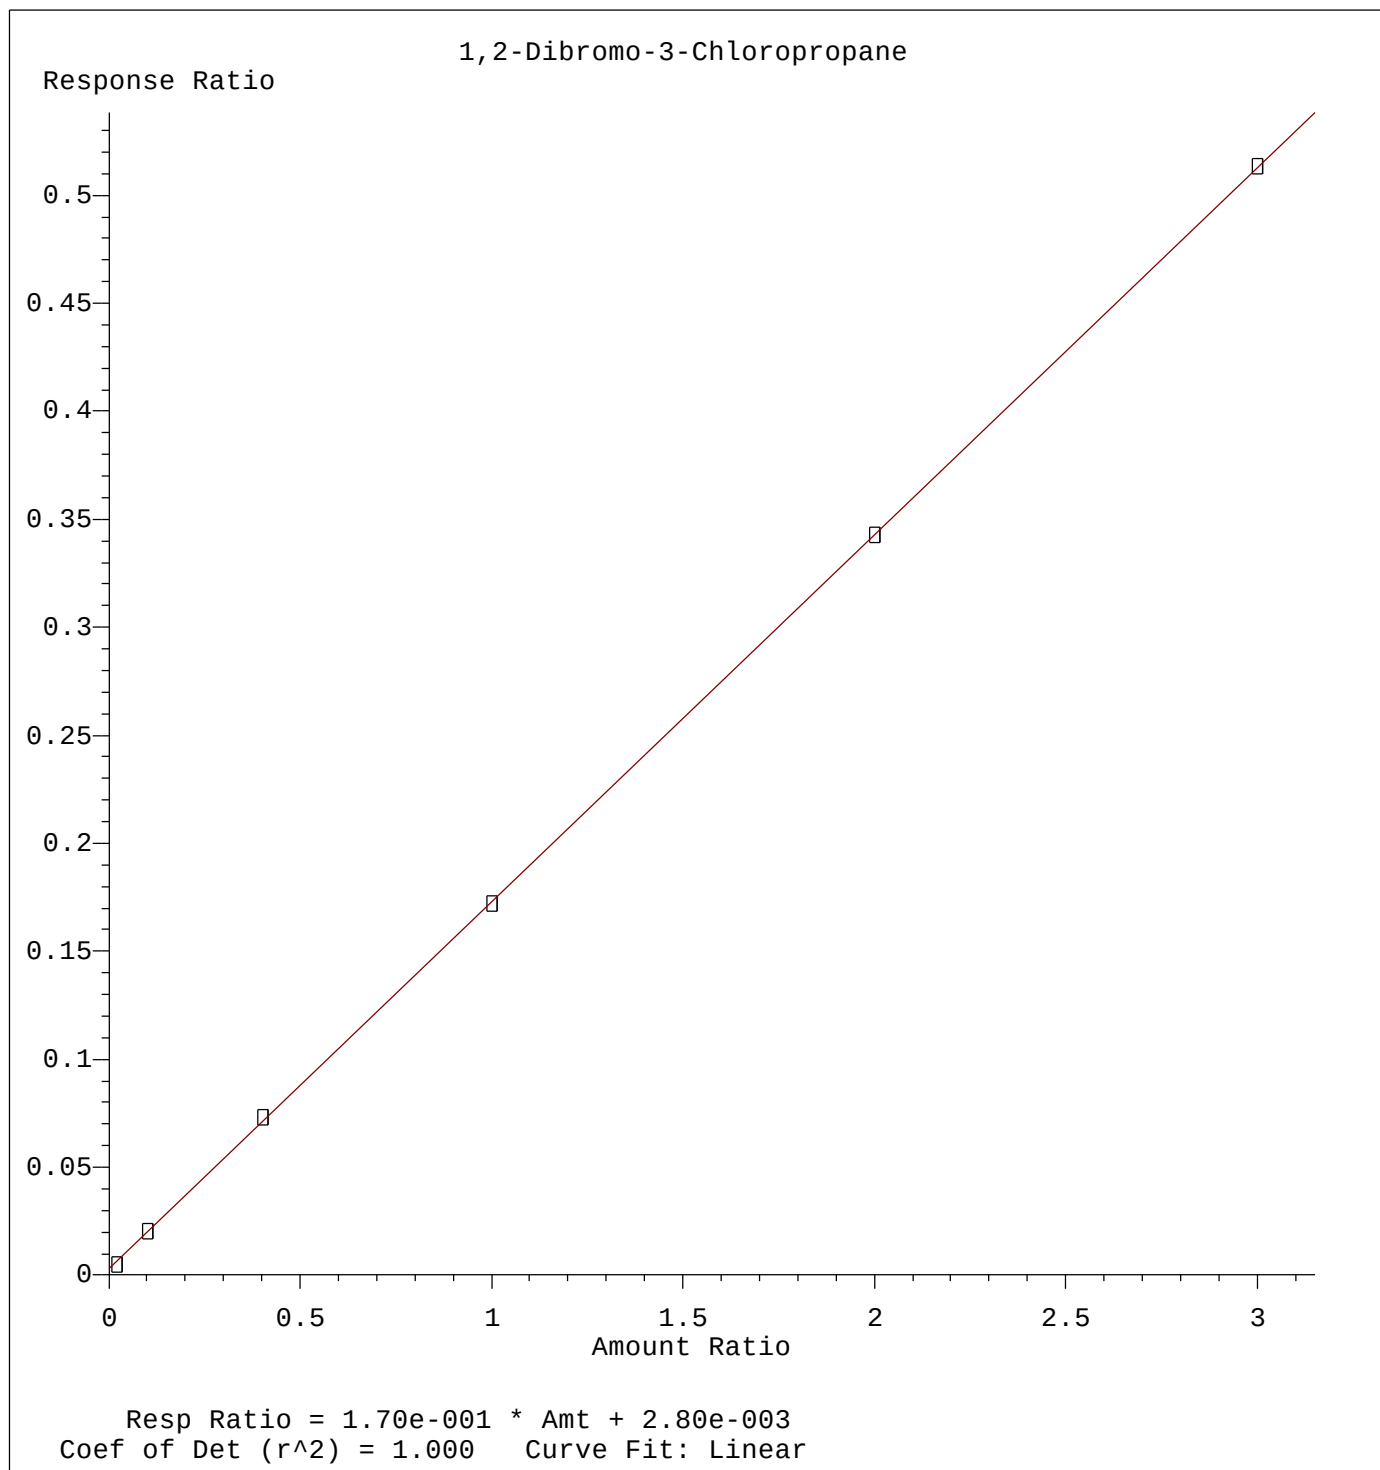

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

1,2,4-Trichlorobenzene

Response Ratio

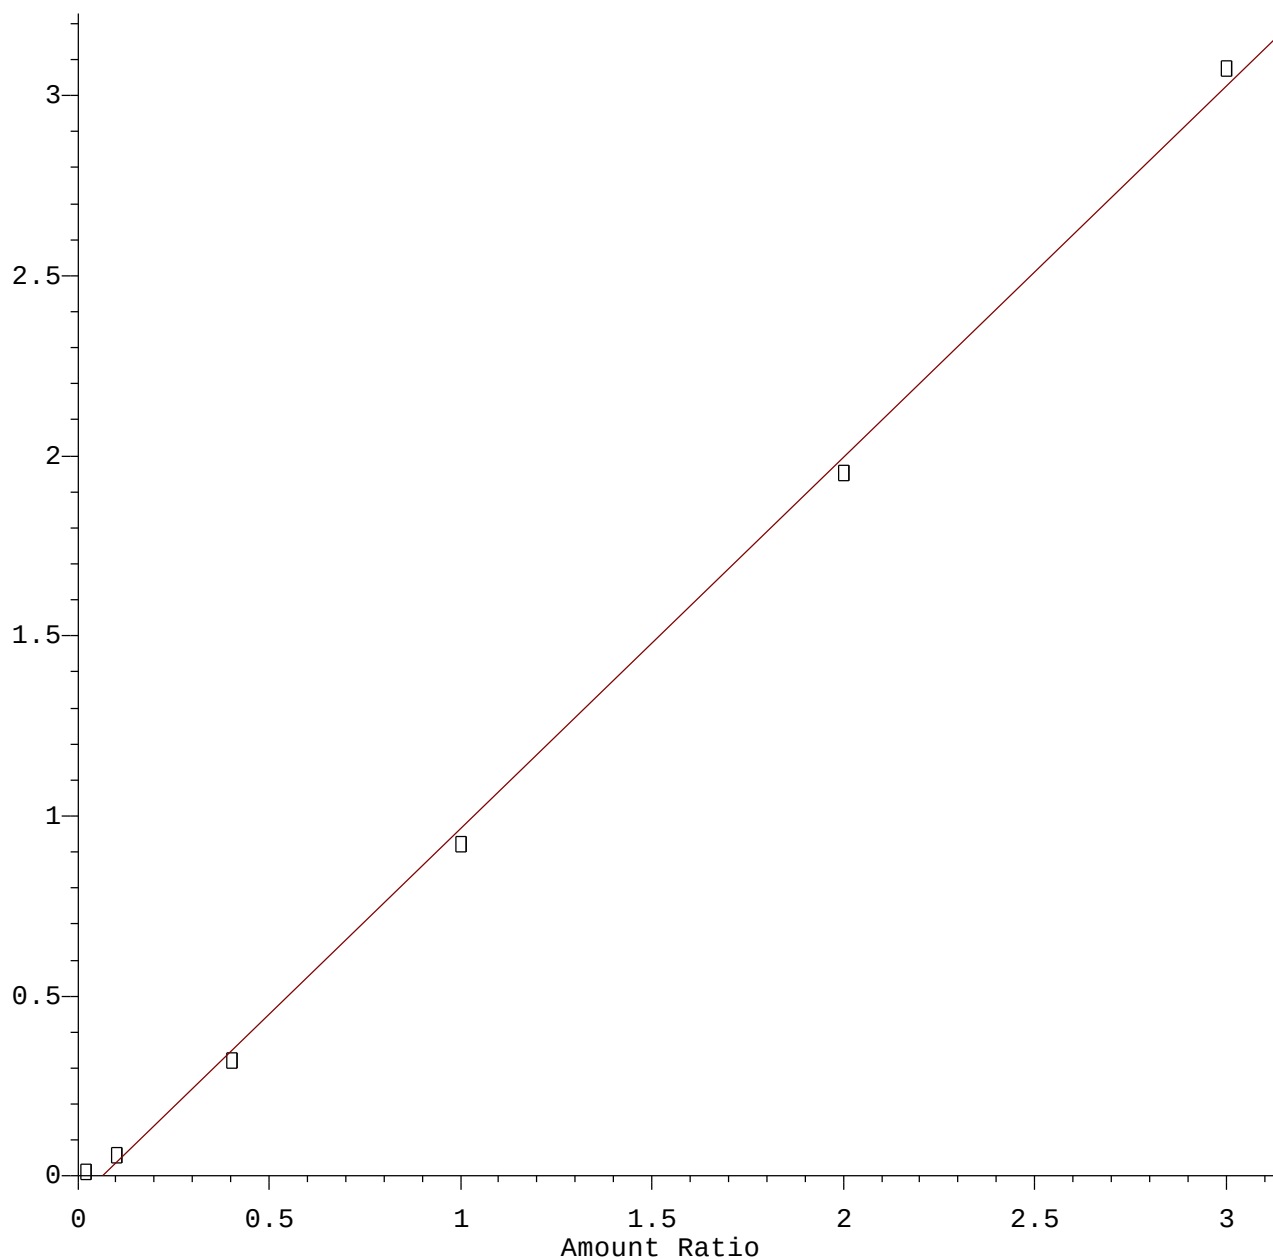


Resp Ratio = 1.03e+000 * Amt - 6.35e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

Naphthalene

Response Ratio

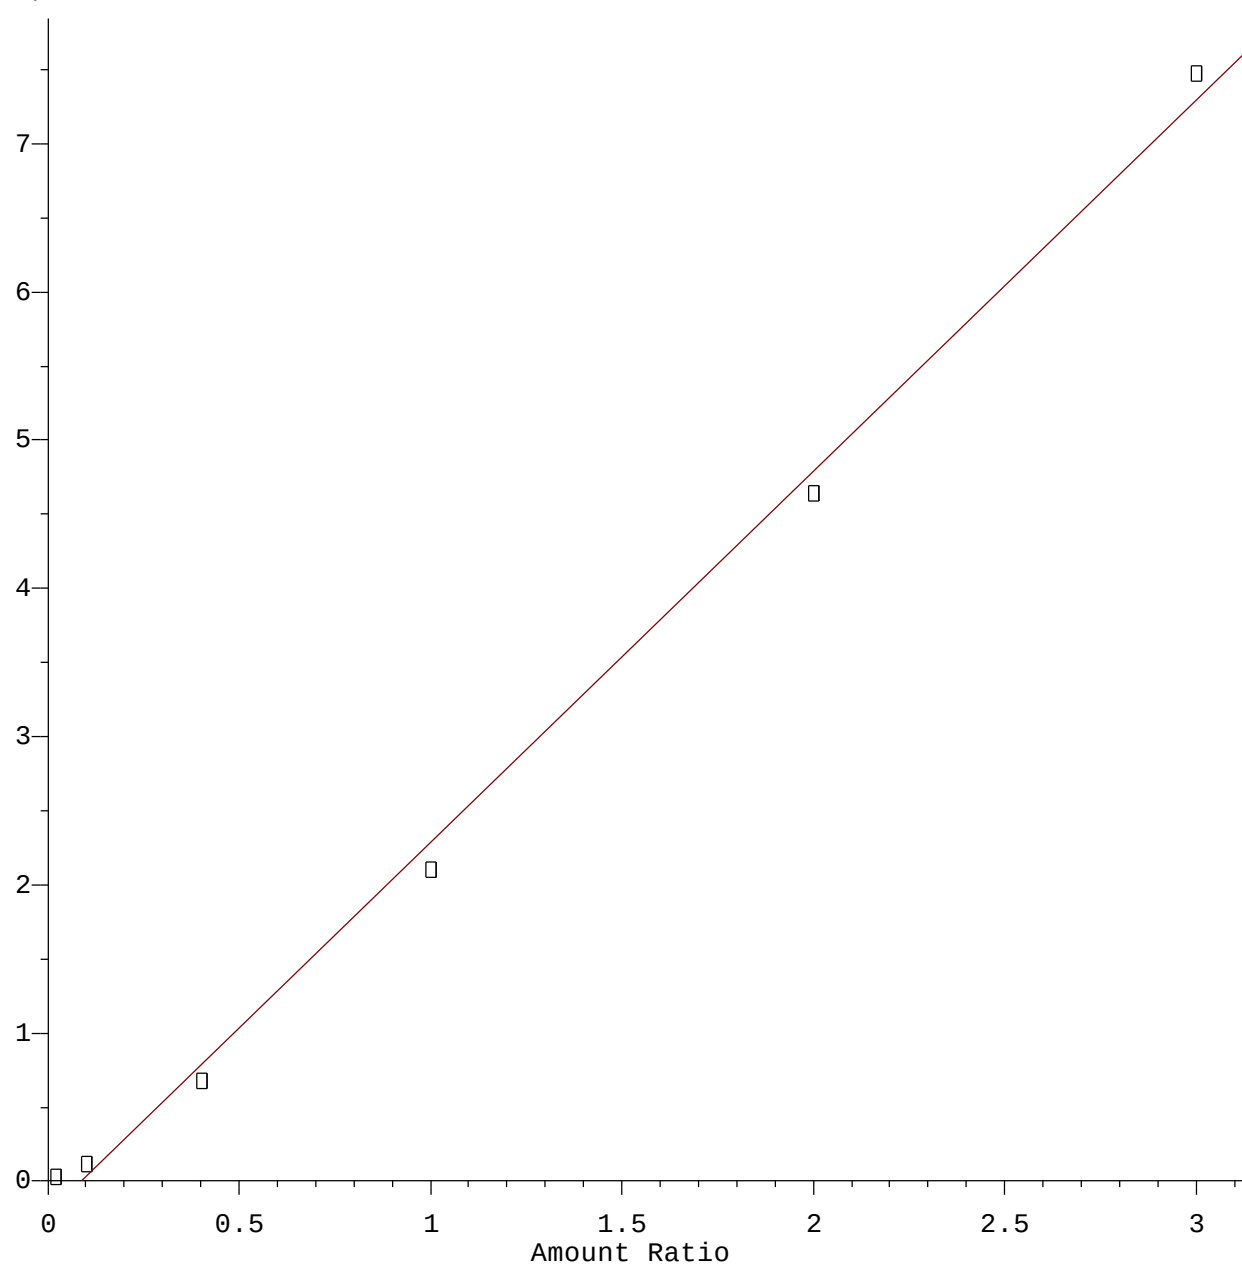


Resp Ratio = 2.50×10^0 * Amt - 2.21×10^{-1}
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018


1,2,3-Trichlorobenzene

Response Ratio

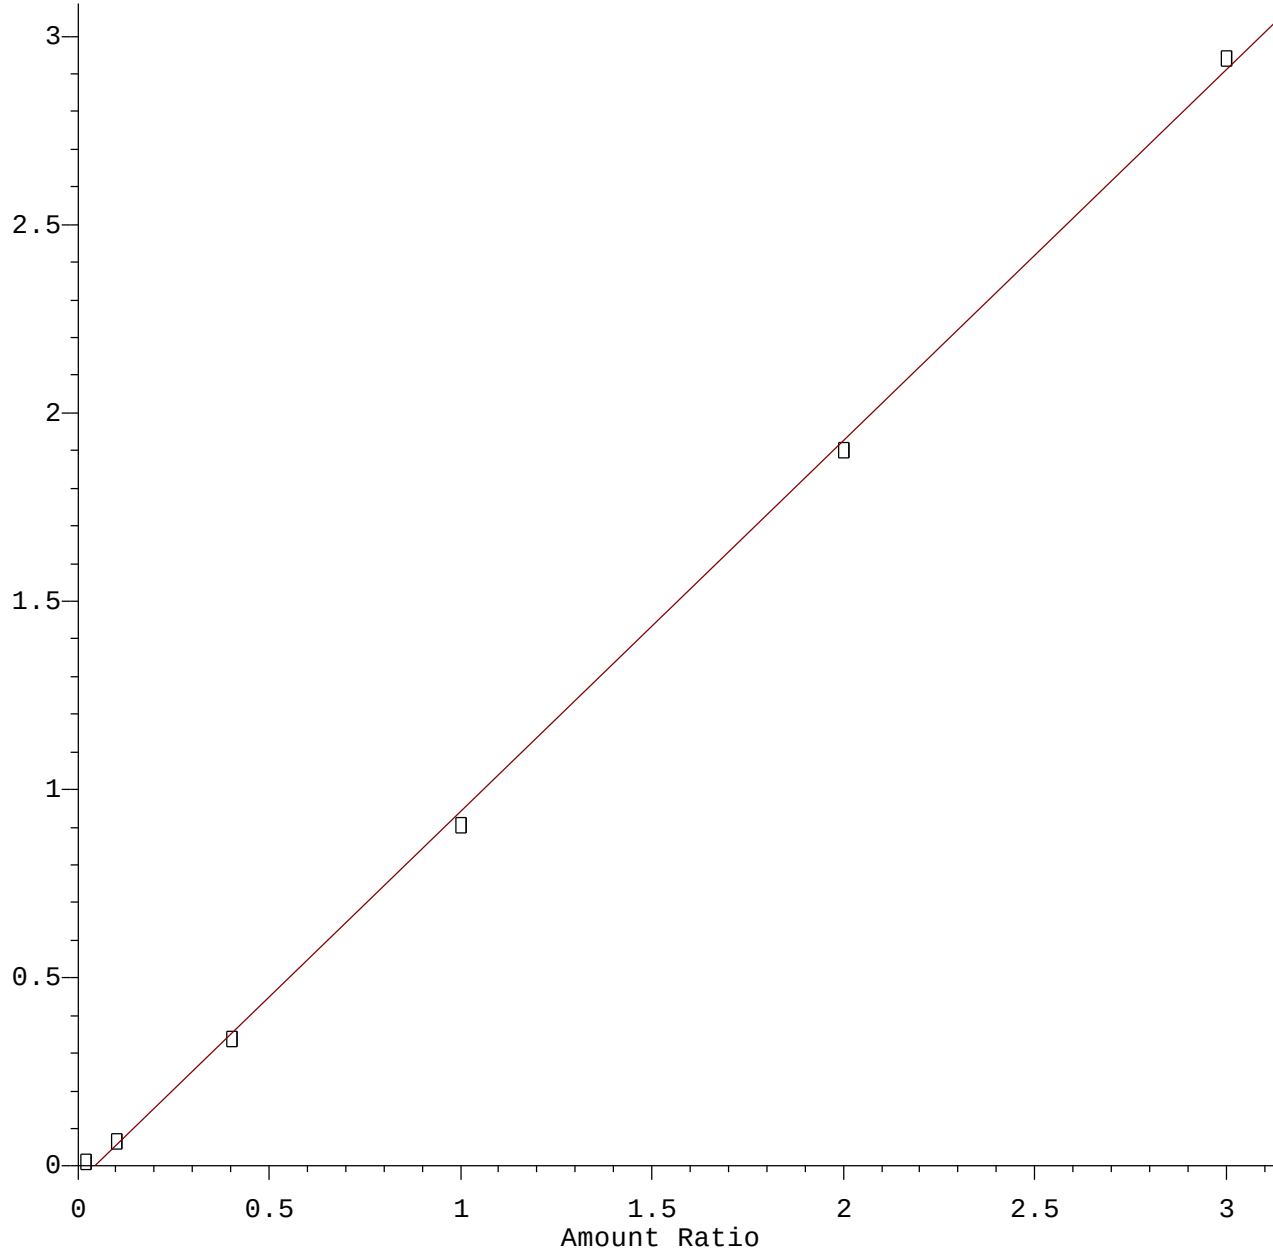

Resp Ratio = $9.84 \times 10^{-1} \times \text{Amt} - 4.34 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018

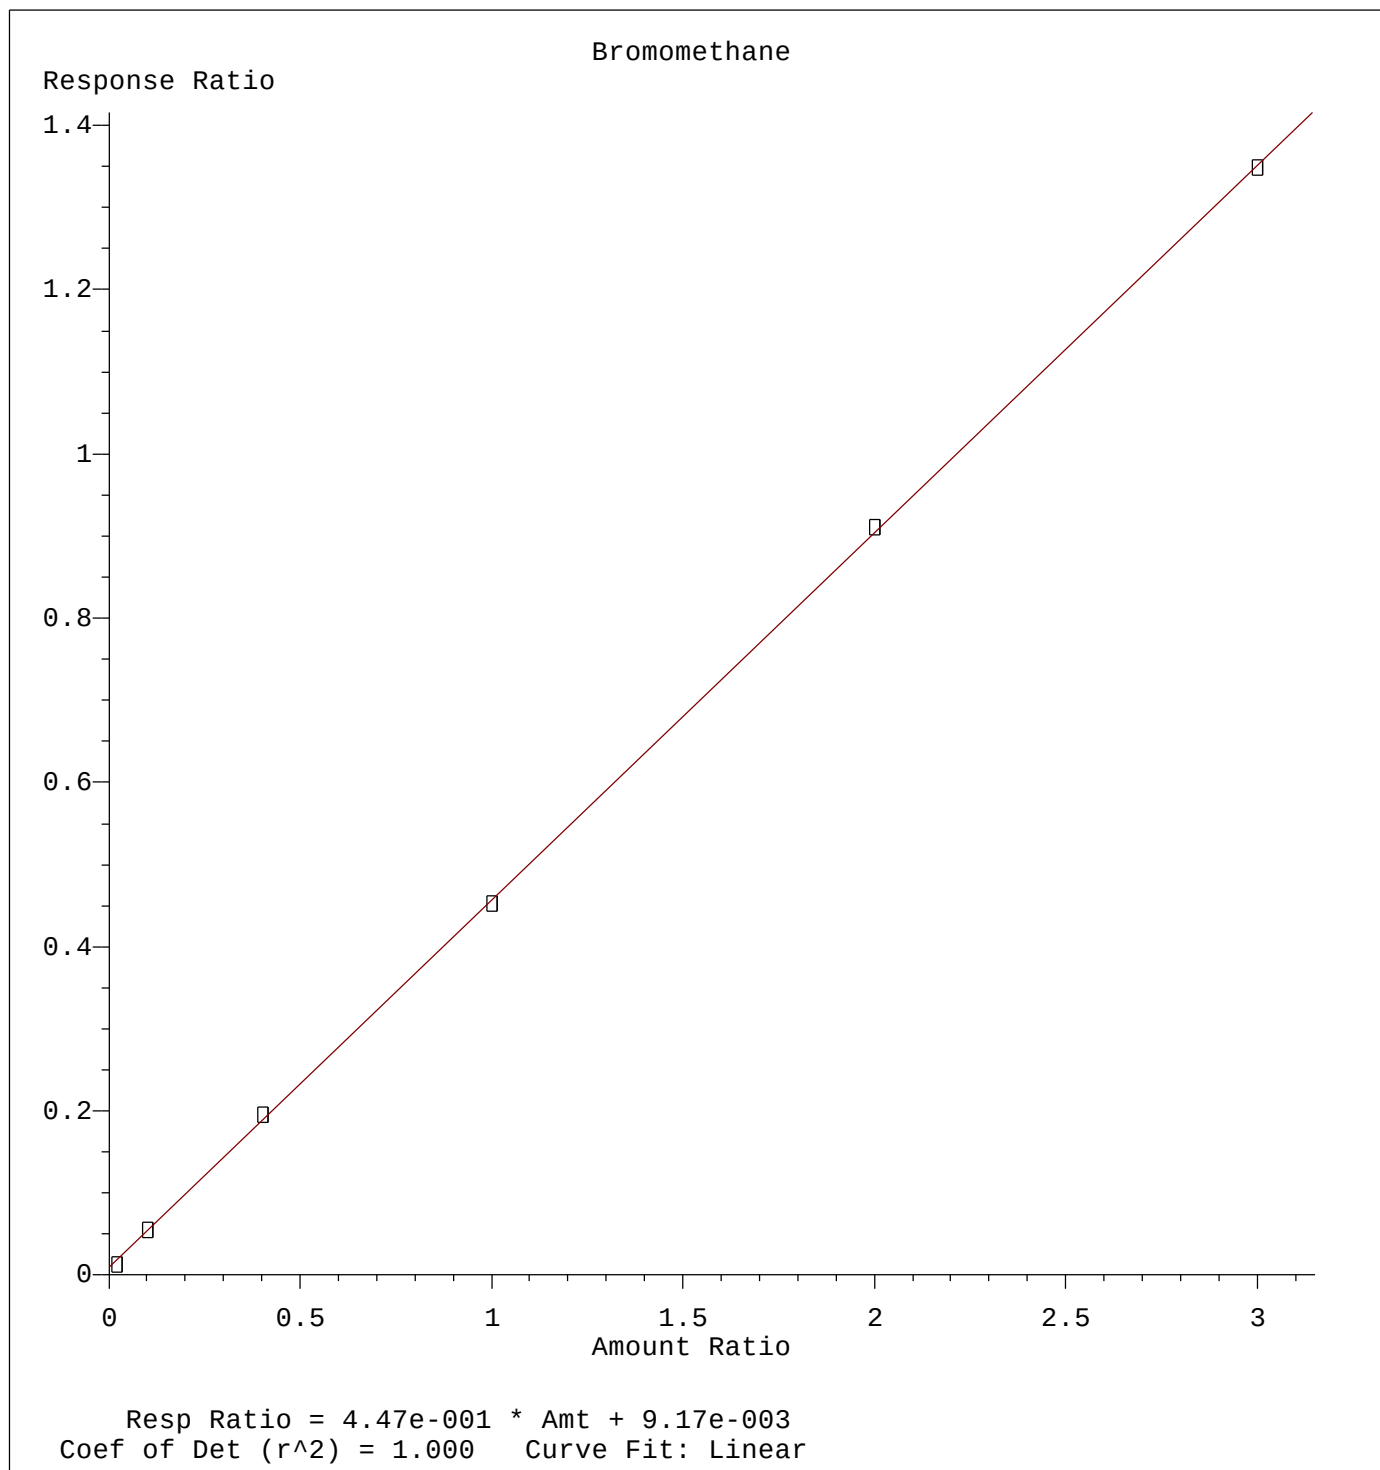

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Calibration Table Last Updated: Thu Jul 26 18:10:10 2018