


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN072418\
 Data File : VN050017.D
 Acq On : 24 Jul 2018 9:49
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
 Title : SW846 8260
 Last Update : Thu Jul 26 18:10:10 2018

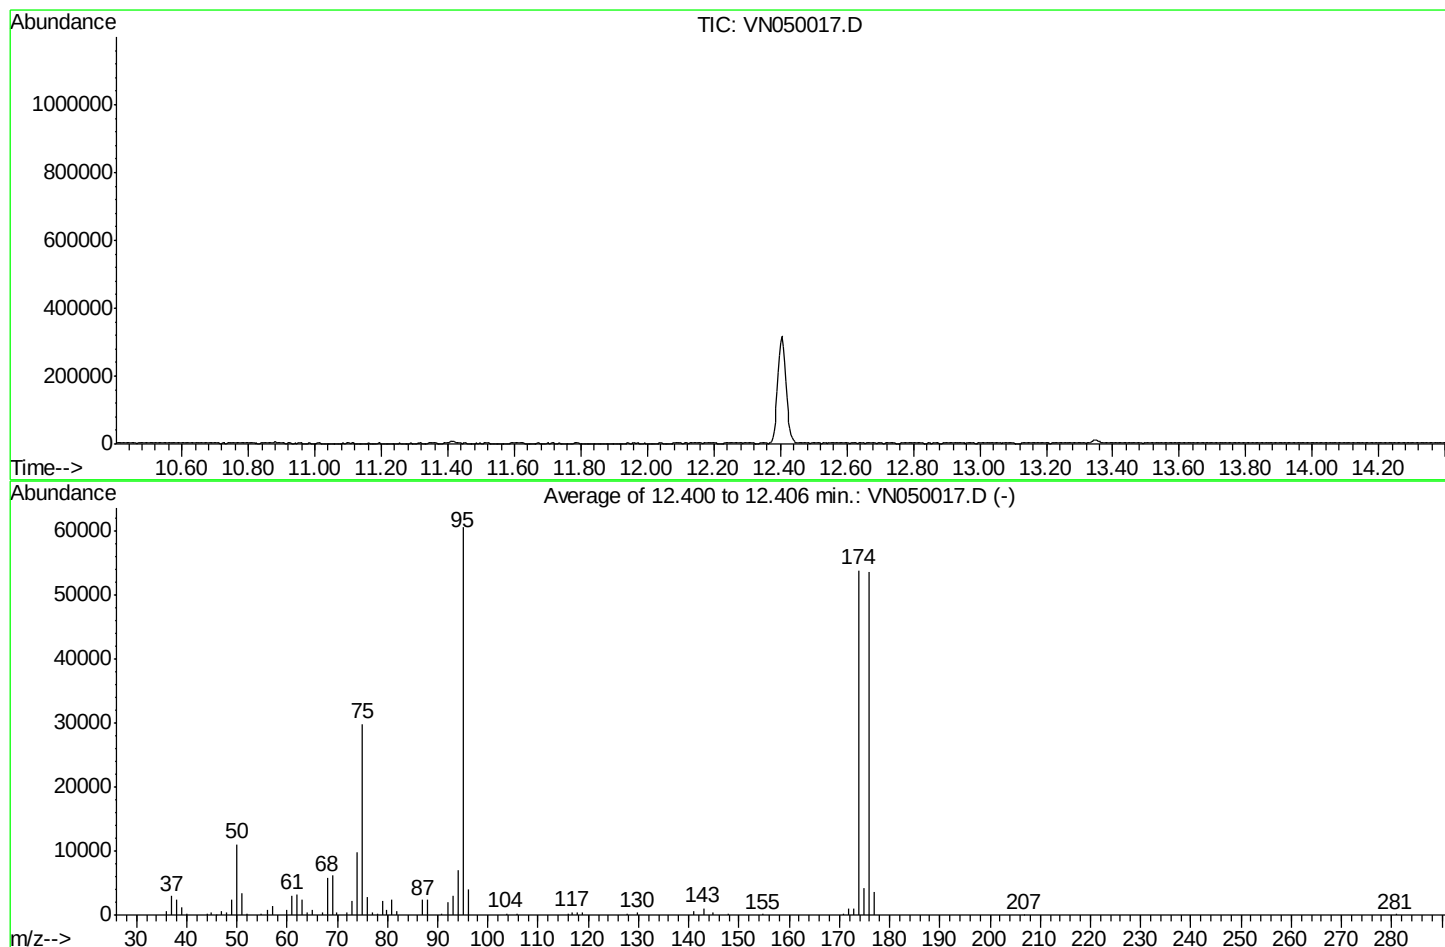

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	11001	PASS
75	95	30	60	49.3	29840	PASS
95	95	100	100	100.0	60490	PASS
96	95	5	9	6.7	4032	PASS
173	174	0.00	2	1.7	915	PASS
174	95	50	100	88.9	53797	PASS
175	174	5	9	7.9	4239	PASS
176	174	95	101	99.4	53453	PASS
177	176	5	9	6.8	3616	PASS