


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN072419\
 Data File : VN056885.D
 Acq On : 23 Jul 2019 18:15
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N072419W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Jul 24 04:19:57 2019

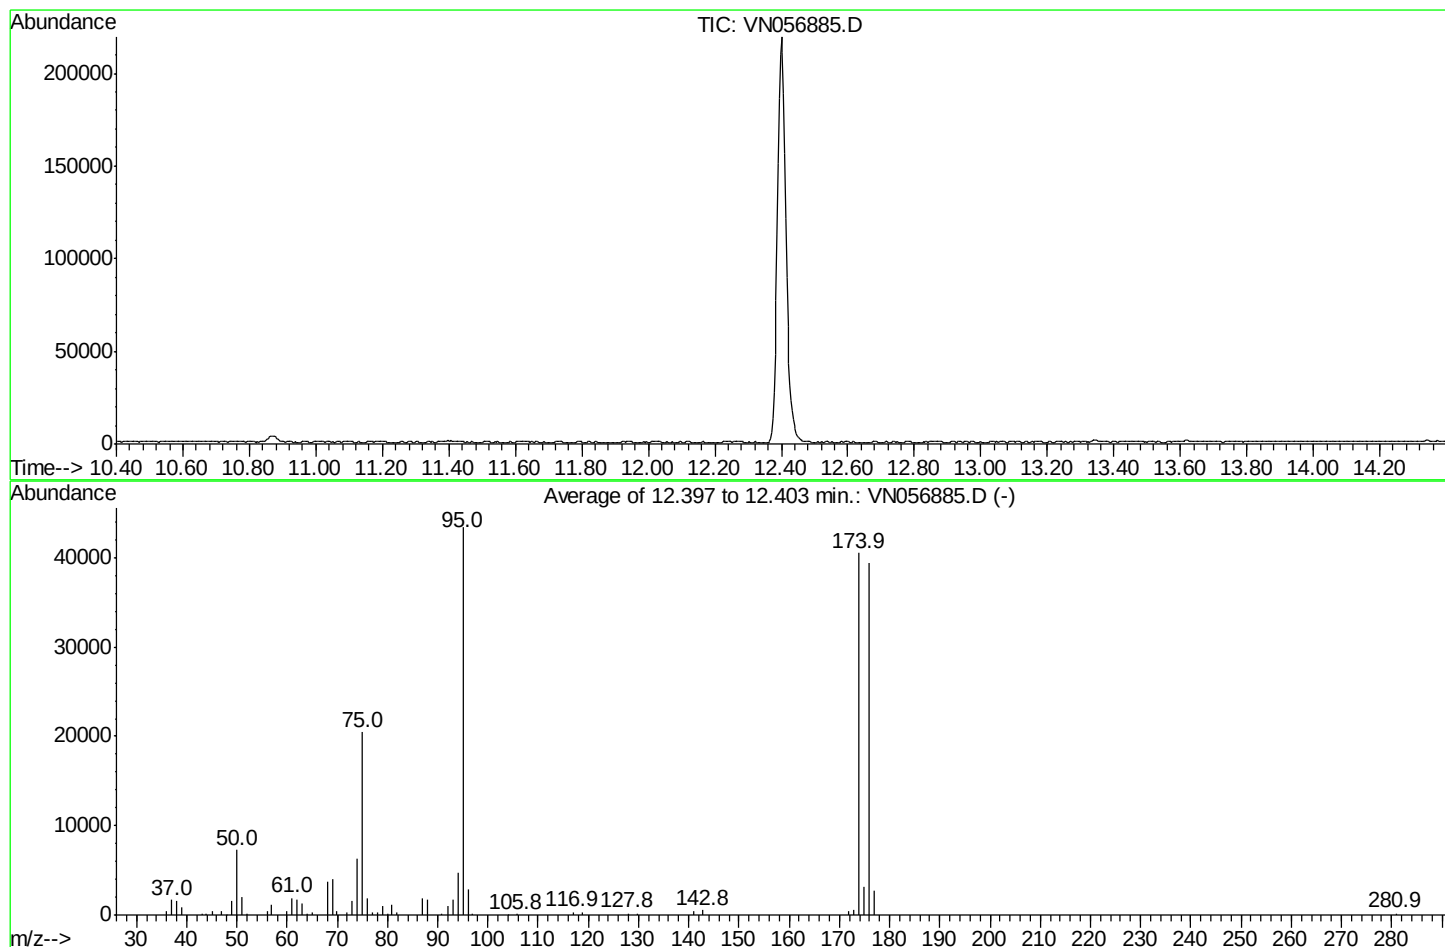

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	7271	PASS
75	95	30	60	47.2	20480	PASS
95	95	100	100	100.0	43405	PASS
96	95	5	9	6.7	2926	PASS
173	174	0.00	2	1.3	537	PASS
174	95	50	100	93.4	40552	PASS
175	174	5	9	7.9	3204	PASS
176	174	95	101	97.4	39480	PASS
177	176	5	9	6.9	2707	PASS