
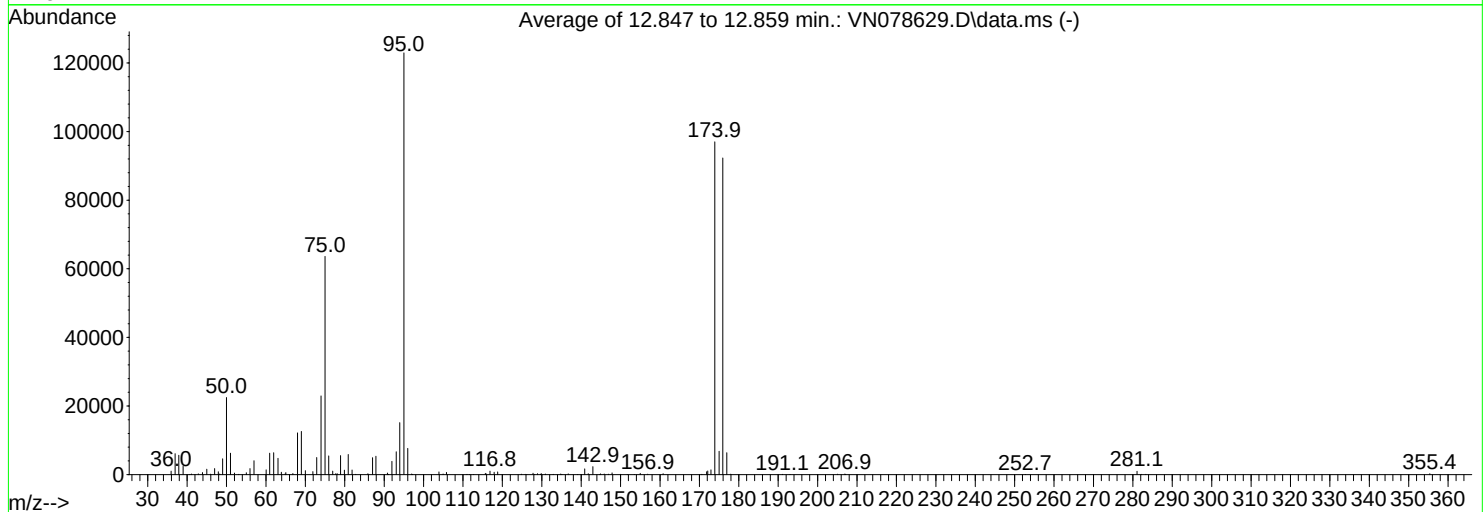


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072423\
Data File : VN078629.D
Acq On : 24 Jul 2023 09:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

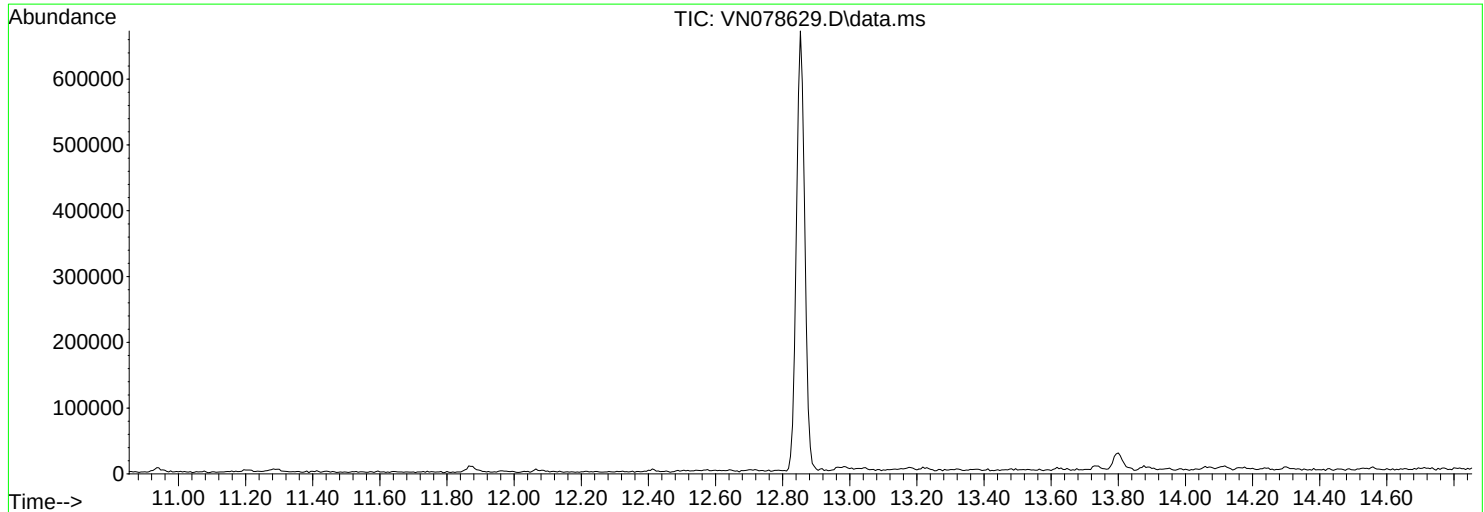

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	22488	PASS
75	95	30	60	51.7	63605	PASS
95	95	100	100	100.0	122944	PASS
96	95	5	9	6.2	7639	PASS
173	174	0.00	2	1.4	1380	PASS
174	95	50	100	78.9	97013	PASS
175	174	5	9	7.0	6808	PASS
176	174	95	101	95.1	92307	PASS
177	176	5	9	6.9	6369	PASS

Average of 12.847 to 12.859 min.: VN078629.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	1033	47.00	1761	60.05	1410	70.00	115
36.95	6095	47.90	840	60.95	6235	71.90	90
37.90	5628	48.30	193	61.95	6396	72.90	501
39.00	2416	49.00	4620	63.05	4750	74.00	2296
40.70	52	50.00	22488	63.90	710	75.00	63605
41.10	188	51.00	6268	64.90	246	75.95	5443
42.00	71	52.00	475	65.05	595	76.95	1016
42.85	226	53.10	101	65.90	55	77.70	282
43.90	601	55.00	558	66.85	331	78.10	292
45.00	1596	55.95	1763	68.00	12173	78.95	5528
45.95	150	56.95	4039	69.00	12611	79.90	1300

Average of 12.847 to 12.859 min.: VN078629.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	5869	93.95	15156	115.70	359	129.70	126
81.85	1336	95.00	122944	115.90	225	129.90	288
82.80	99	96.00	7639	116.85	1010	130.90	200
85.85	249	96.95	181	117.90	688	132.90	77
86.10	123	97.20	77	118.80	780	134.80	183
87.05	4938	103.90	816	124.80	124	135.10	98
87.90	5344	104.95	171	125.80	119	136.70	224
90.85	459	105.80	662	126.20	51	139.10	52
91.10	117	111.00	119	127.80	435	140.00	51
91.95	3866	111.70	53	128.10	115	140.90	1671
93.05	6662	112.70	59	128.90	274	141.80	292

Average of 12.847 to 12.859 min.: VN078629.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.00	52	156.90	150	191.10	79		
142.95	2332	160.80	299	193.00	64		
144.70	55	170.60	91	205.10	146		
144.90	246	171.85	855	206.90	180		
145.85	170	172.10	1079	207.10	79		
146.90	140	172.95	1380	252.70	62		
147.85	519	173.90	97013	281.05	980		
150.00	76	175.00	6808	282.10	74		
151.70	50	175.95	92307	283.30	92		
153.50	53	176.95	6369	355.35	290		
155.00	398	177.95	134				

Instrument :

MSVOA_N

ClientSampleId :

BFB