
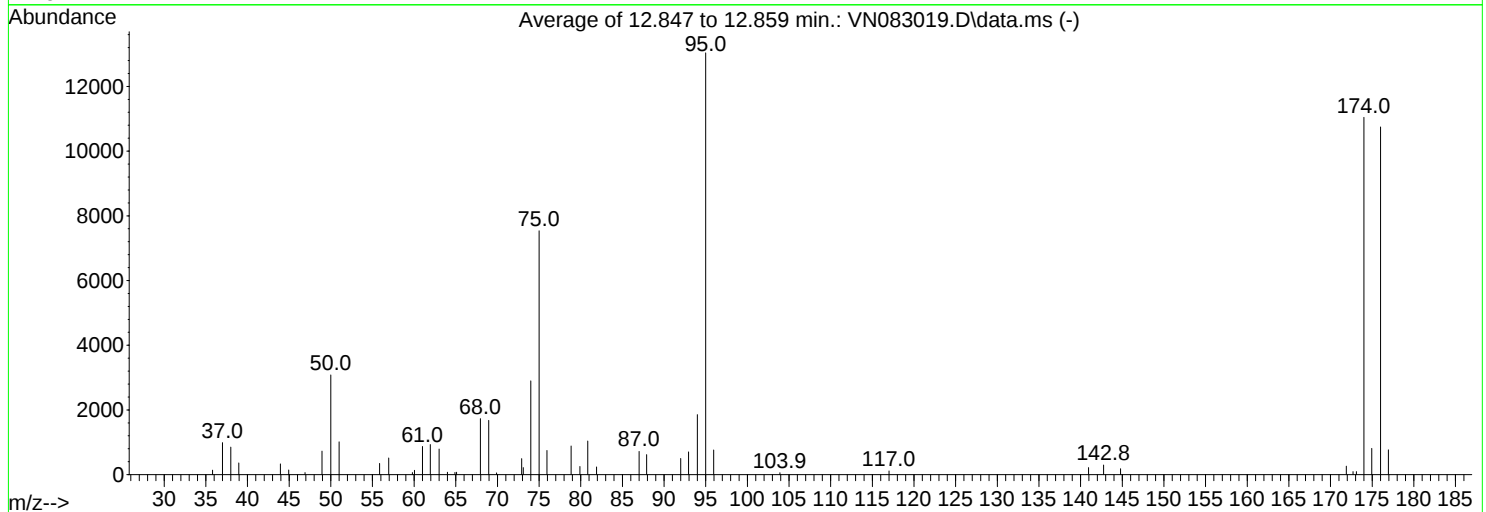


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072424\
Data File : VN083019.D
Acq On : 24 Jul 2024 08:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

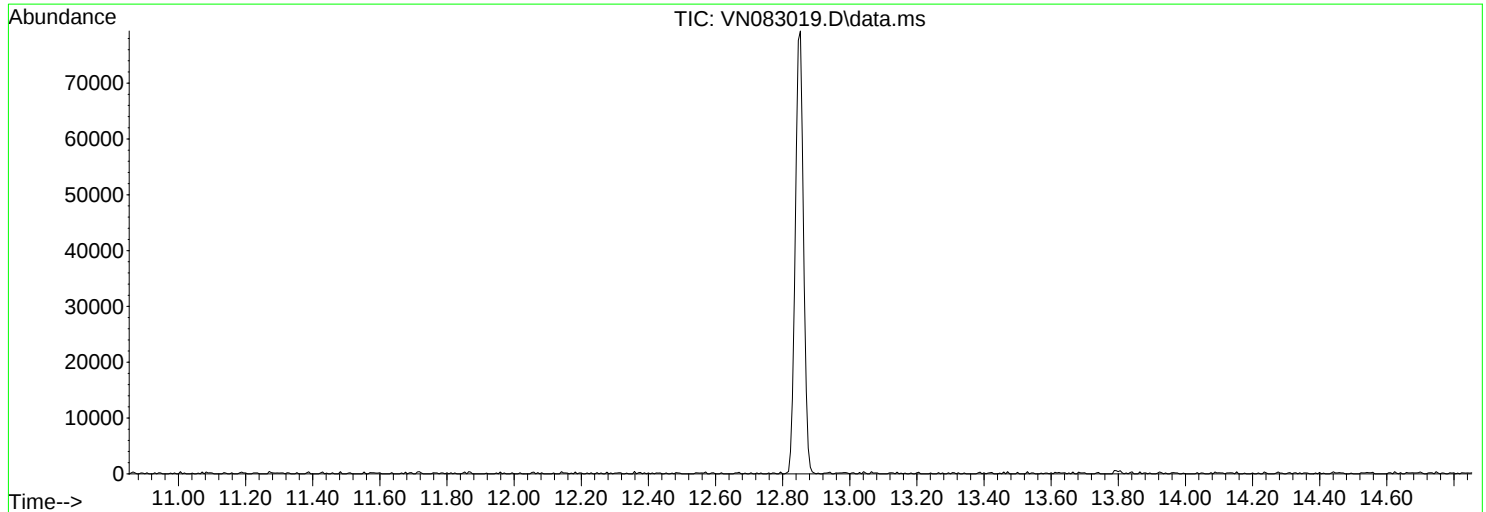

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	3080	PASS
75	95	30	60	57.8	7539	PASS
95	95	100	100	100.0	13038	PASS
96	95	5	9	5.9	764	PASS
173	174	0.00	2	0.8	93	PASS
174	95	50	100	84.7	11043	PASS
175	174	5	9	7.4	813	PASS
176	174	95	101	97.3	10747	PASS
177	176	5	9	7.1	765	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	137	56.95	514	69.90	55	87.90	61
37.00	987	59.80	63	72.90	494	92.00	49
38.00	852	60.05	135	73.10	219	92.95	70
38.95	362	61.00	872	74.00	2898	94.00	185
43.95	330	61.95	931	75.00	7539	95.00	13038
44.95	142	63.00	793	75.95	747	95.95	764
46.90	66	64.00	73	78.85	884	103.90	61
48.95	727	64.90	67	79.90	252	117.00	113
50.00	3080	65.10	72	80.85	1041	140.95	217
51.00	1015	67.95	1729	81.90	236	142.75	298
55.85	346	68.95	1679	87.00	718	144.80	182

Average of 12.847 to 12.859 min.: VN083019.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.90	260						
172.70	92						
173.10	93						
174.00	11043						
174.95	813						
176.00	10747						
176.95	765						

Instrument :

MSVOA_N

ClientSampleId :

BFB