
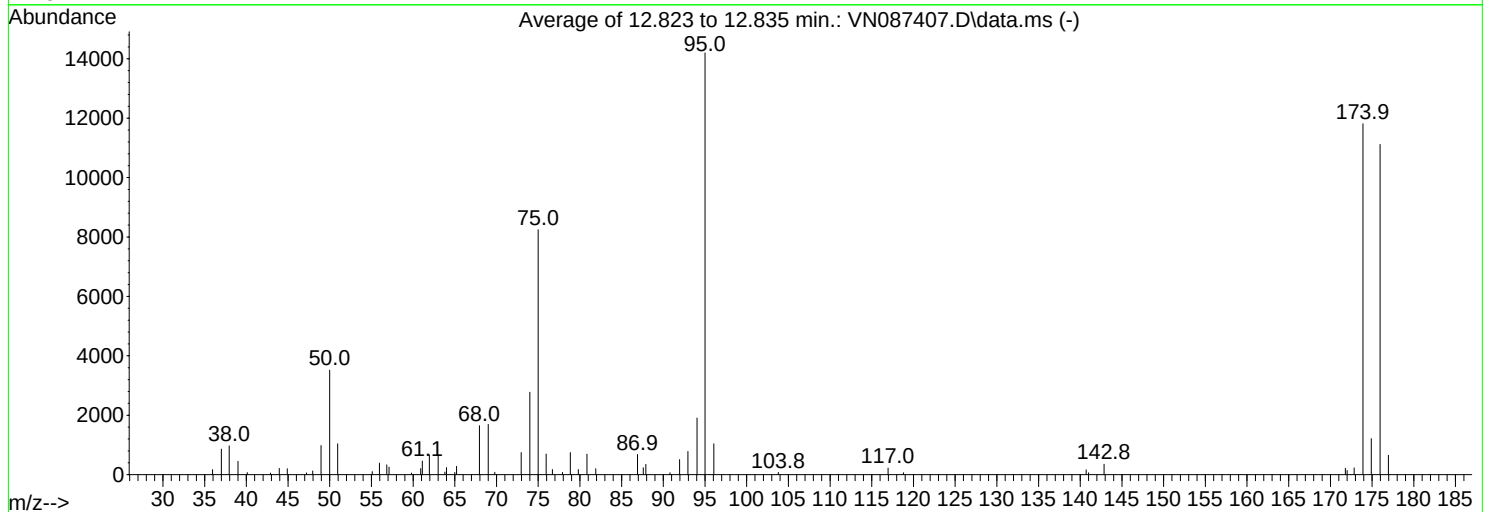


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072425\
Data File : VN087407.D
Acq On : 24 Jul 2025 08:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N072325W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Jul 24 05:11:26 2025

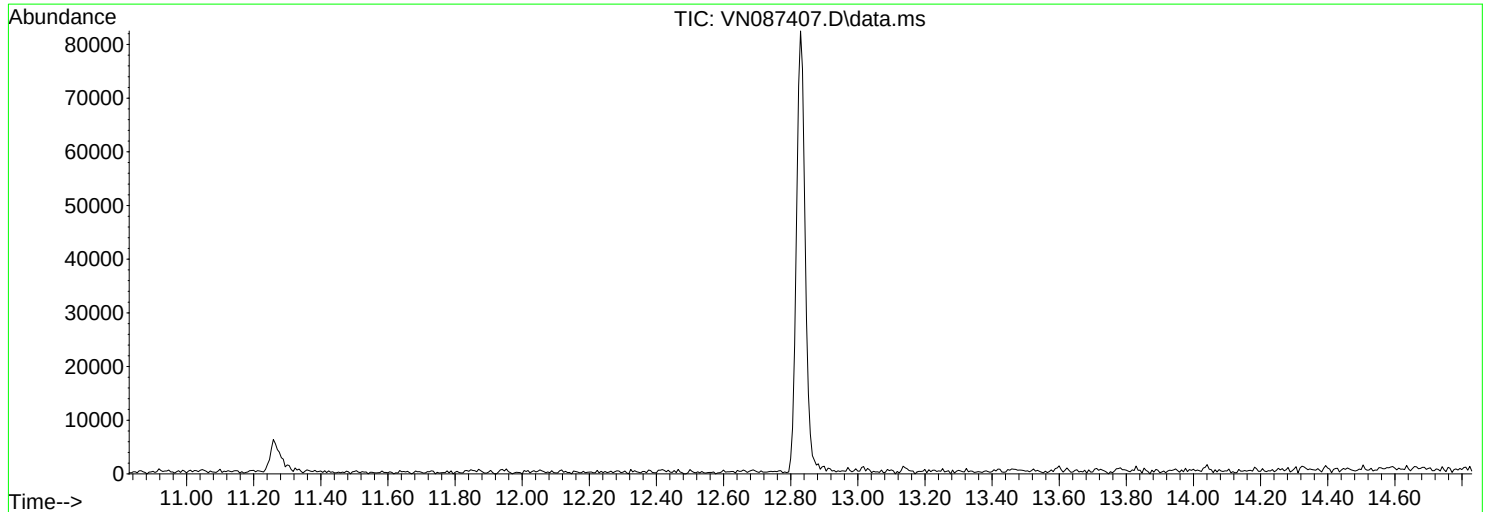

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.8	3520	PASS
75	95	30	60	58.1	8249	PASS
95	95	100	100	100.0	14199	PASS
96	95	5	9	7.3	1039	PASS
173	174	0.00	2	1.9	224	PASS
174	95	50	100	83.2	11814	PASS
175	174	5	9	10.3	1213	FAIL*
176	174	95	101	94.1	11115	FAIL*
177	176	5	9	5.9	652	PASS