

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN072519\
 Data File : VN056912.D
 Acq On : 24 Jul 2019 15:02
 Operator : JC/SP
 Sample : K3921-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SU19-MSW0619

Quant Time: Jul 25 01:33:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072519SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 25 01:27:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	48137	5.00	ug/l	0.00
4) 1,4-Difluorobenzene	8.58	114	79482	5.00	ug/l	0.00
8) Chlorobenzene-d5	11.41	117	46612	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.35	152	6924	5.00	ug/l	0.00

System Monitoring Compounds						
3) 1,2-Dichloroethane-d4	8.01	65	27763	4.99	ug/l	0.00
Spiked Amount	5.000	Range	81 - 118	Recovery	=	99.80%
5) Dibromofluoromethane	7.59	113	22648	4.93	ug/l	0.00
Spiked Amount	5.000	Range	80 - 119	Recovery	=	98.60%
6) Toluene-d8	10.09	98	46070	4.89	ug/l	0.00
Spiked Amount	5.000	Range	89 - 112	Recovery	=	97.80%
7) 4-Bromofluorobenzene	12.40	95	11357	4.66	ug/l	0.00
Spiked Amount	5.000	Range	85 - 114	Recovery	=	93.20%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN072519\
Data File : VN056912.D
Acq On : 24 Jul 2019 15:02
Operator : JC/SP
Sample : K3921-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SU19-MSW0619

Quant Time: Jul 25 01:33:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072519SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Thu Jul 25 01:27:20 2019
Response via : Initial Calibration

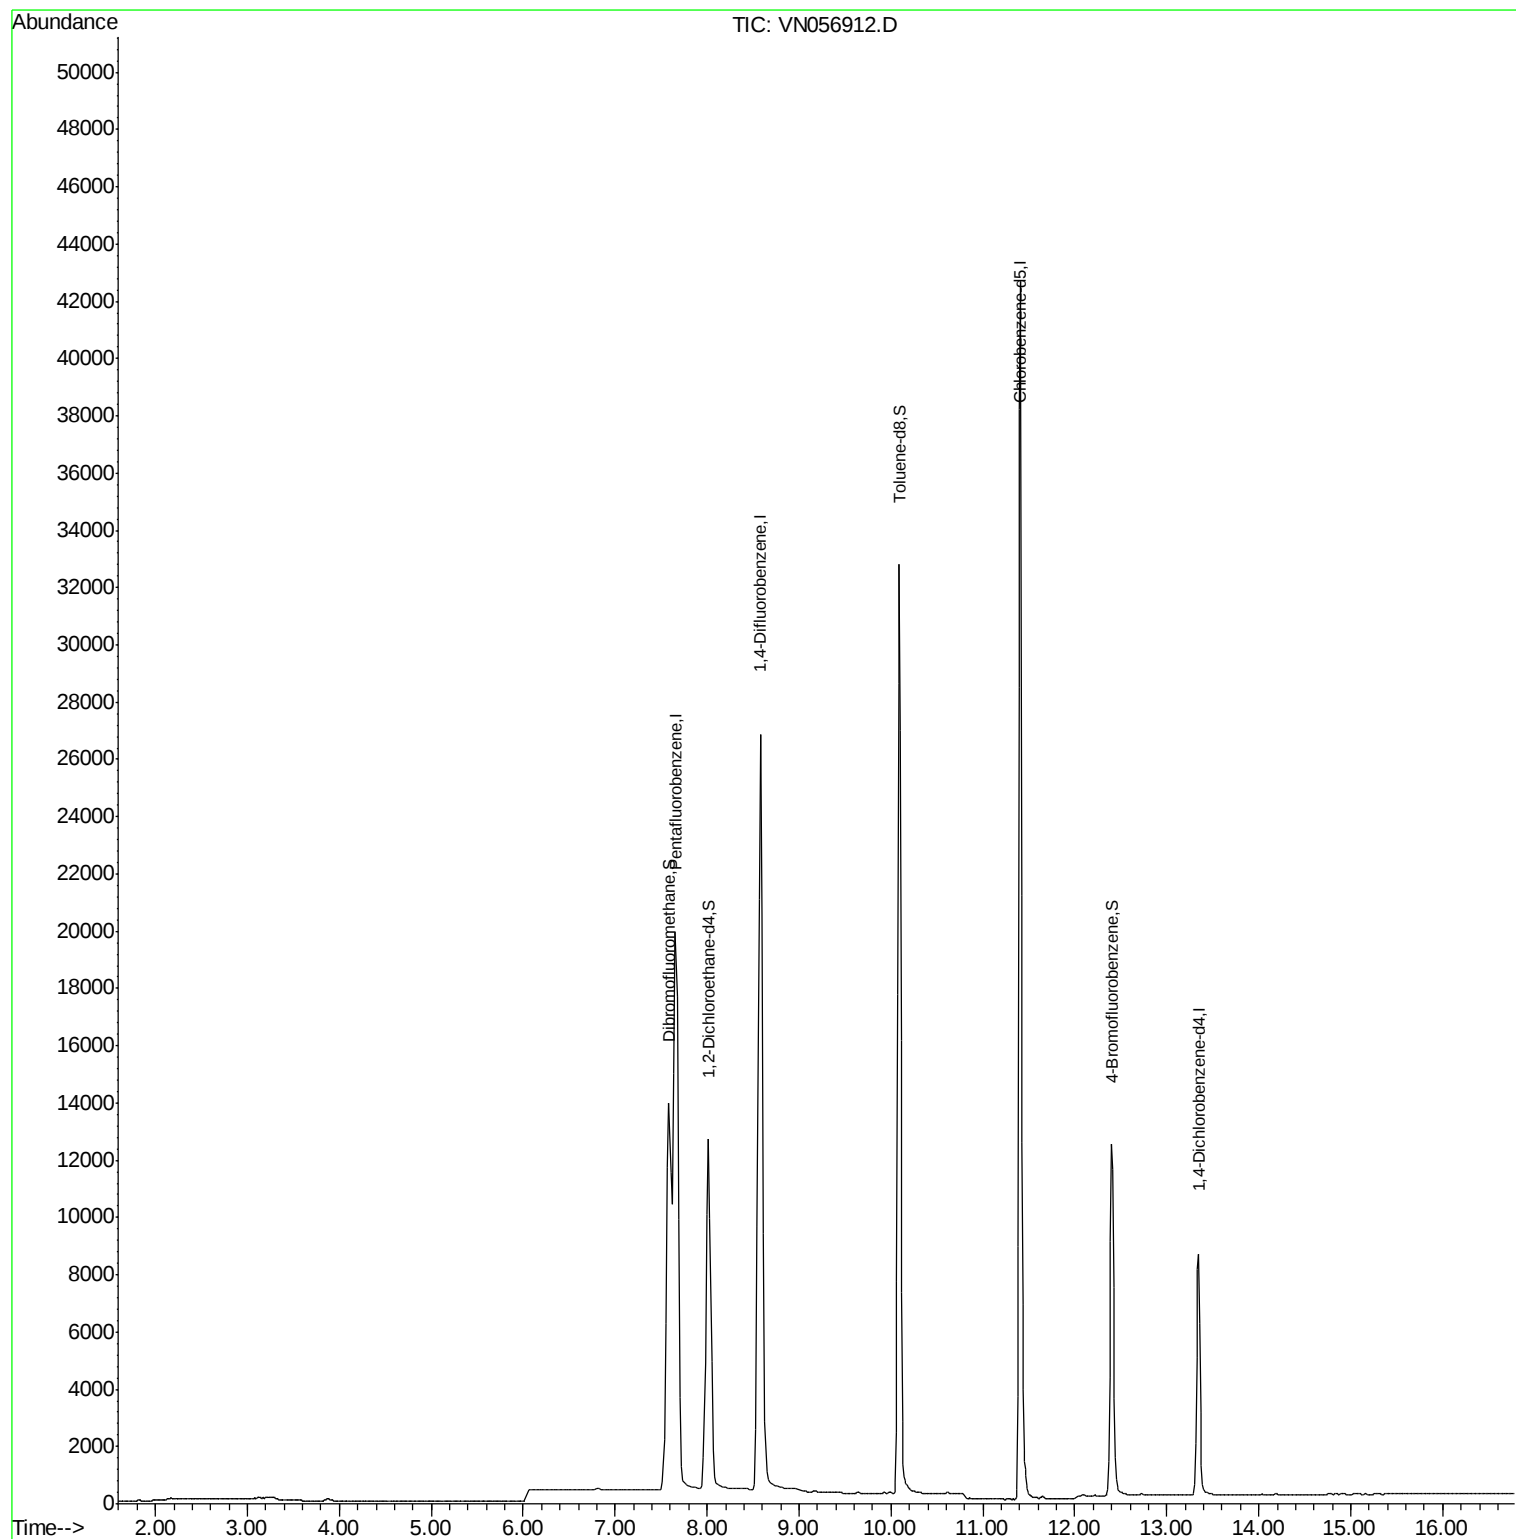

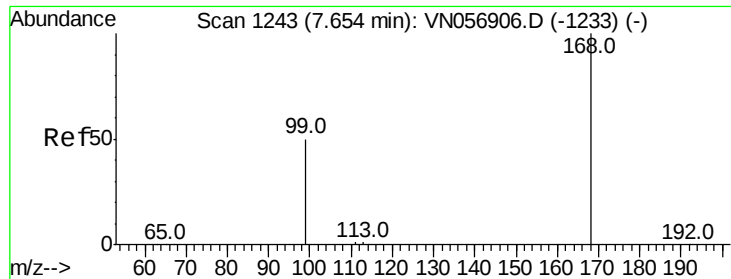

#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.65 min Scan# 1243

Delta R.T. -0.00 min

Lab File: VN056912.D

Acq: 24 Jul 2019 15:02

Instrument :

MSVOA_N

ClientSampleId :


SU19-MSW0619

Tot Ion:168 Resp: 48137

Ion Ratio Lower Upper

168 100

99 50.4 40.1 60.1

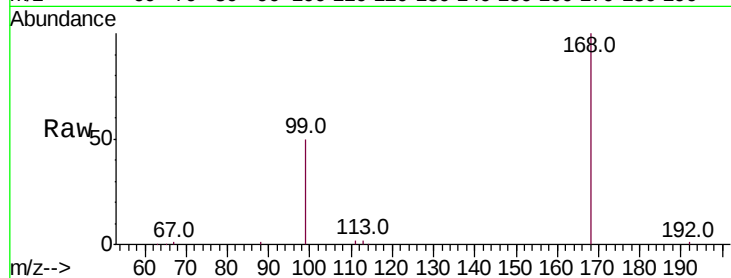

Abundance Ion 168.00 (167.70 to 168.70): VN056912.D (-1233) (-)

Ion 99.00 (98.70 to 99.70): VN056912.D (-1233) (-)

7.65

15000



10000

5000

0

Time-->

7.40 7.60 7.80 8.00

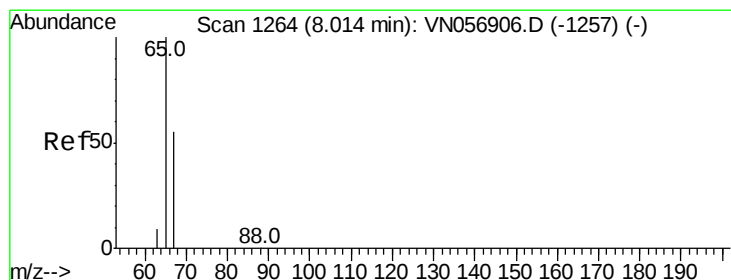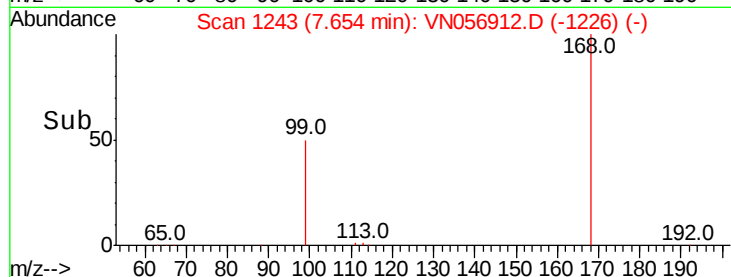

#3

1,2-Dichloroethane-d4

Concen: 4.993 ug/l

RT: 8.01 min Scan# 1264

Delta R.T. -0.00 min

Lab File: VN056912.D


Acq: 24 Jul 2019 15:02

Tgt Ion: 65 Resp: 27763

Ion Ratio Lower Upper

65 100

67 54.1 0.0 110.2

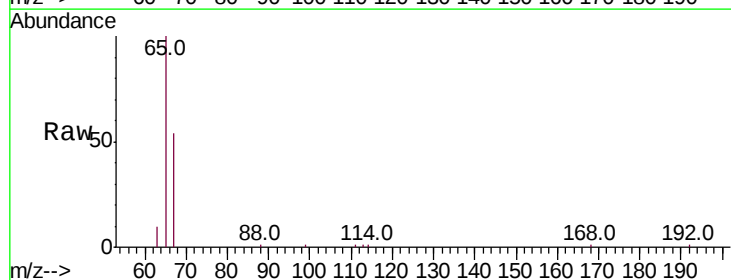

Abundance Ion 65.00 (64.70 to 65.70): VN056912.D (-1247) (-)

Ion 67.00 (66.70 to 67.70): VN056912.D (-1247) (-)

8.01

8000

6000


4000


2000

0

Time-->

7.80 8.00 8.20

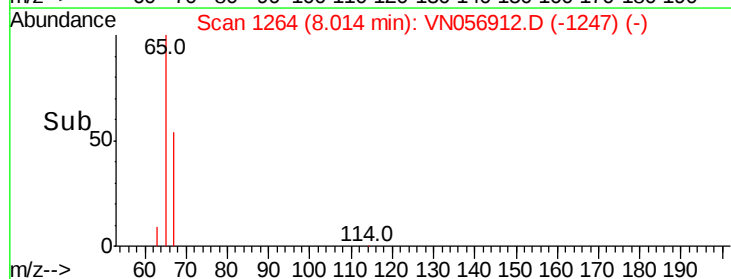

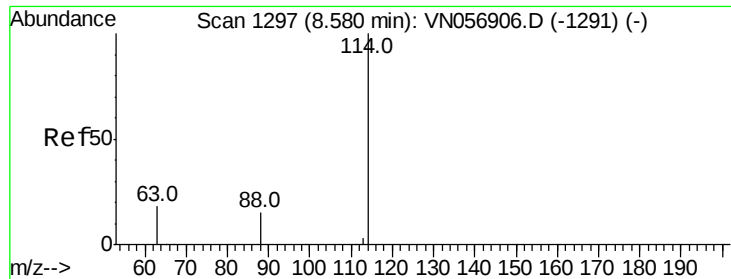

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.58 min Scan# 1297

Delta R.T. -0.00 min

Lab File: VN056912.D

Acq: 24 Jul 2019 15:02

Instrument :

MSVOA_N

ClientSampleId :

SU19-MSW0619


Tot Ion:114 Resp: 79482

Ion Ratio Lower Upper

114 100

63 18.1 0.0 36.2




88 15.1 0.0 30.2

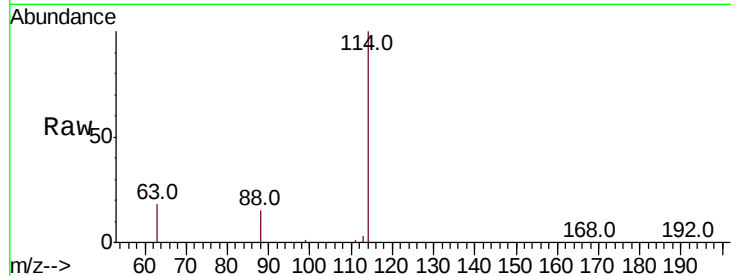

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VN

Ion 88.00 (87.70 to 88.70): VN

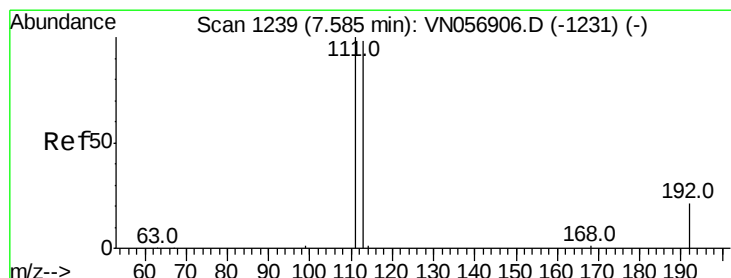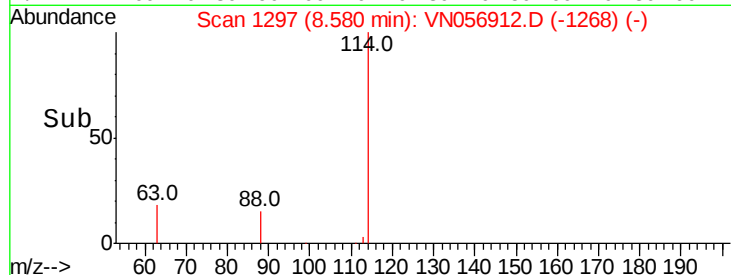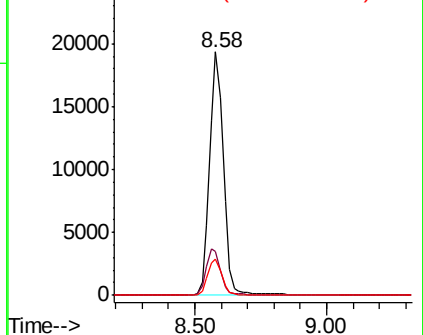

#5

Dibromofluoromethane

Concen: 4.930 ug/l

RT: 7.59 min Scan# 1239

Delta R.T. -0.00 min

Lab File: VN056912.D

Acq: 24 Jul 2019 15:02


Tgt Ion:113 Resp: 22648

Ion Ratio Lower Upper

113 100

111 101.5 81.5 122.3



192 21.8 17.4 26.0

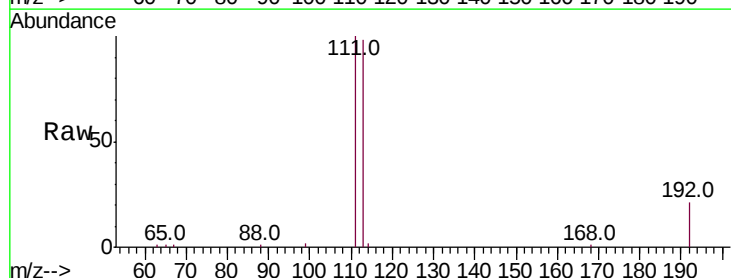


Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V

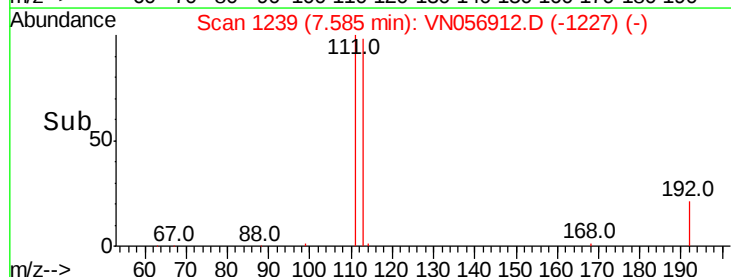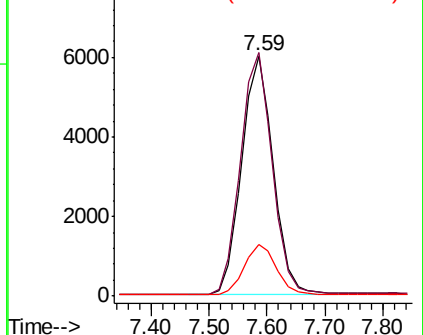

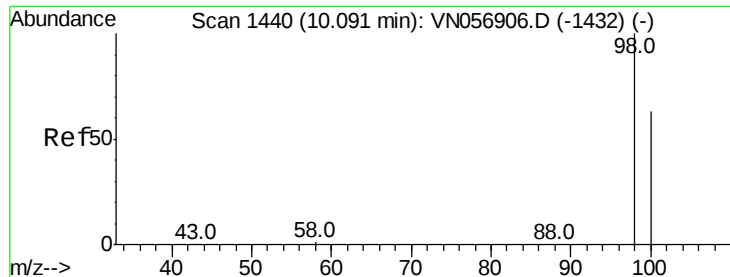

#6

Toluene-d8

Concen: 4.889 ug/l

RT: 10.09 min Scan# 1440

Delta R.T. 0.00 min

Lab File: VN056912.D

Acq: 24 Jul 2019 15:02

Instrument :

MSVOA_N

ClientSampleId :


SU19-MSW0619

Tot Ion: 98 Resp: 46070

Ion Ratio Lower Upper

98 100

100 63.0 50.5 75.7

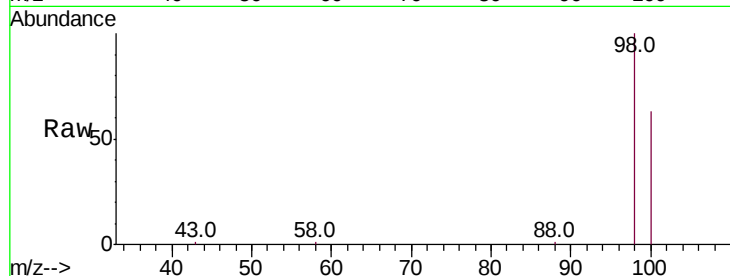

Abundance Ion 98.00 (97.70 to 98.70): VN056912.D (-1432) (-)

Ion 100.00 (99.70 to 100.70): VN056912.D (-1432) (-)

10.09

20000



15000

10000

5000

0

Time-->

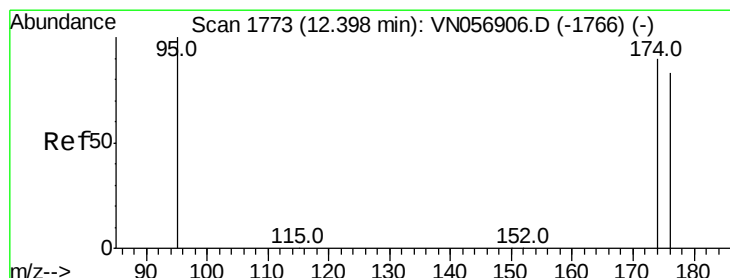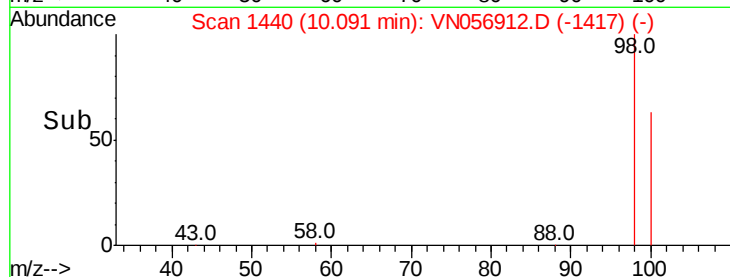

#7

4-Bromofluorobenzene

Concen: 4.663 ug/l

RT: 12.40 min Scan# 1773

Delta R.T. -0.00 min

Lab File: VN056912.D

Acq: 24 Jul 2019 15:02


Tgt Ion: 95 Resp: 11357

Ion Ratio Lower Upper

95 100

174 90.3 0.0 179.8

176 83.0 0.0 166.6

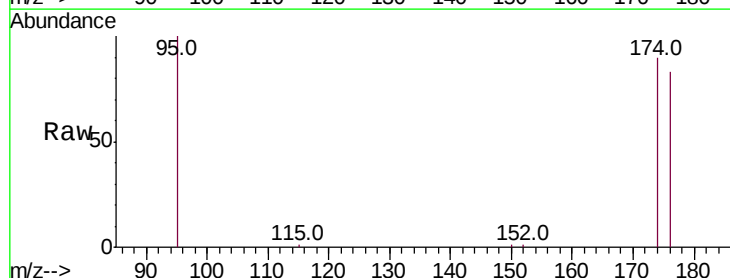

Abundance Ion 95.00 (94.70 to 95.70): VN056912.D (-1766) (-)

Ion 174.00 (173.70 to 174.70): VN056912.D (-1766) (-)

Ion 176.00 (175.70 to 176.70): VN056912.D (-1766) (-)

12.40

6000

5000

4000


3000


2000

1000

0

Time-->

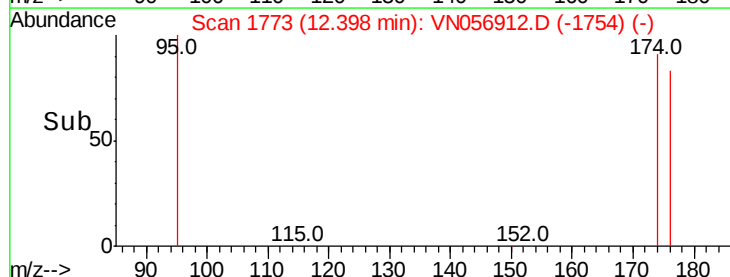

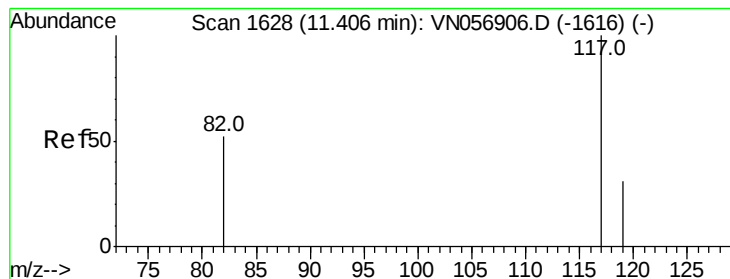

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.41 min Scan# 1628

Delta R.T. 0.00 min

Lab File: VN056912.D

Acq: 24 Jul 2019 15:02

Instrument :

MSVOA_N

ClientSampleId :

SU19-MSW0619


Tot Ion:117 Resp: 46612

Ion Ratio Lower Upper

117 100

82 52.3 42.0 63.0




119 31.7 25.1 37.7

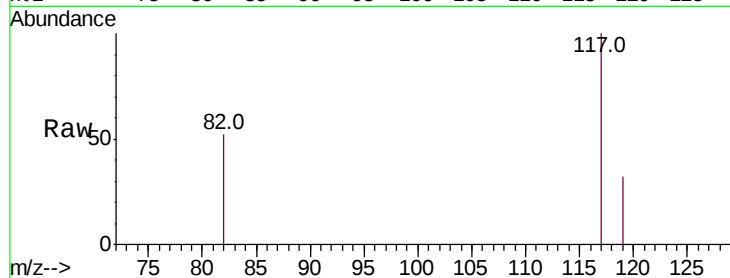

Abundance Ion 117.00 (116.70 to 117.70): V

Ion 82.00 (81.70 to 82.70): VN

Ion 119.00 (118.70 to 119.70): V

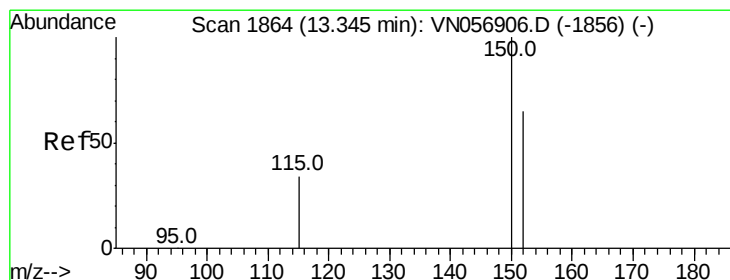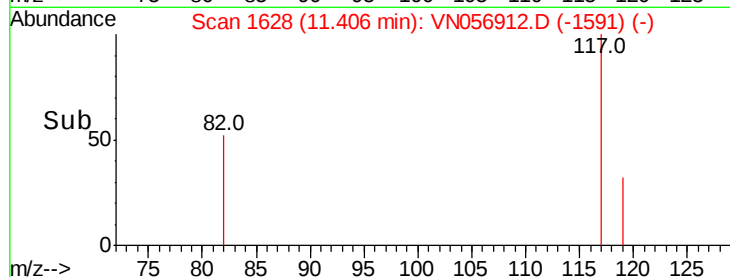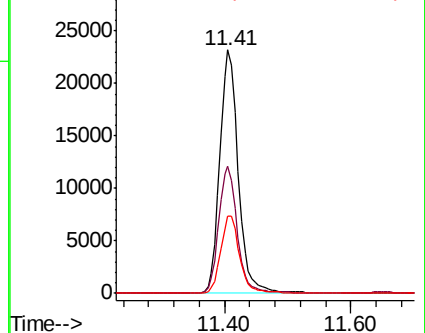

#9

1,4-Dichlorobenzene-d4

Concen: 5.000 ug/l

RT: 13.35 min Scan# 1864

Delta R.T. -0.00 min

Lab File: VN056912.D

Acq: 24 Jul 2019 15:02


Tgt Ion:152 Resp: 6924

Ion Ratio Lower Upper

152 100

115 53.7 26.5 79.4

150 153.8 0.0 306.2

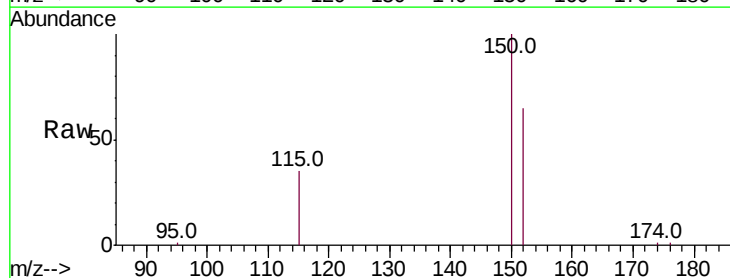

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

