


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN072519\
Data File : VN056901.D
Acq On : 24 Jul 2019 8:20
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072519SIM-VINYL.M
Title : SW846 8260
Last Update : Thu Jul 25 01:27:20 2019

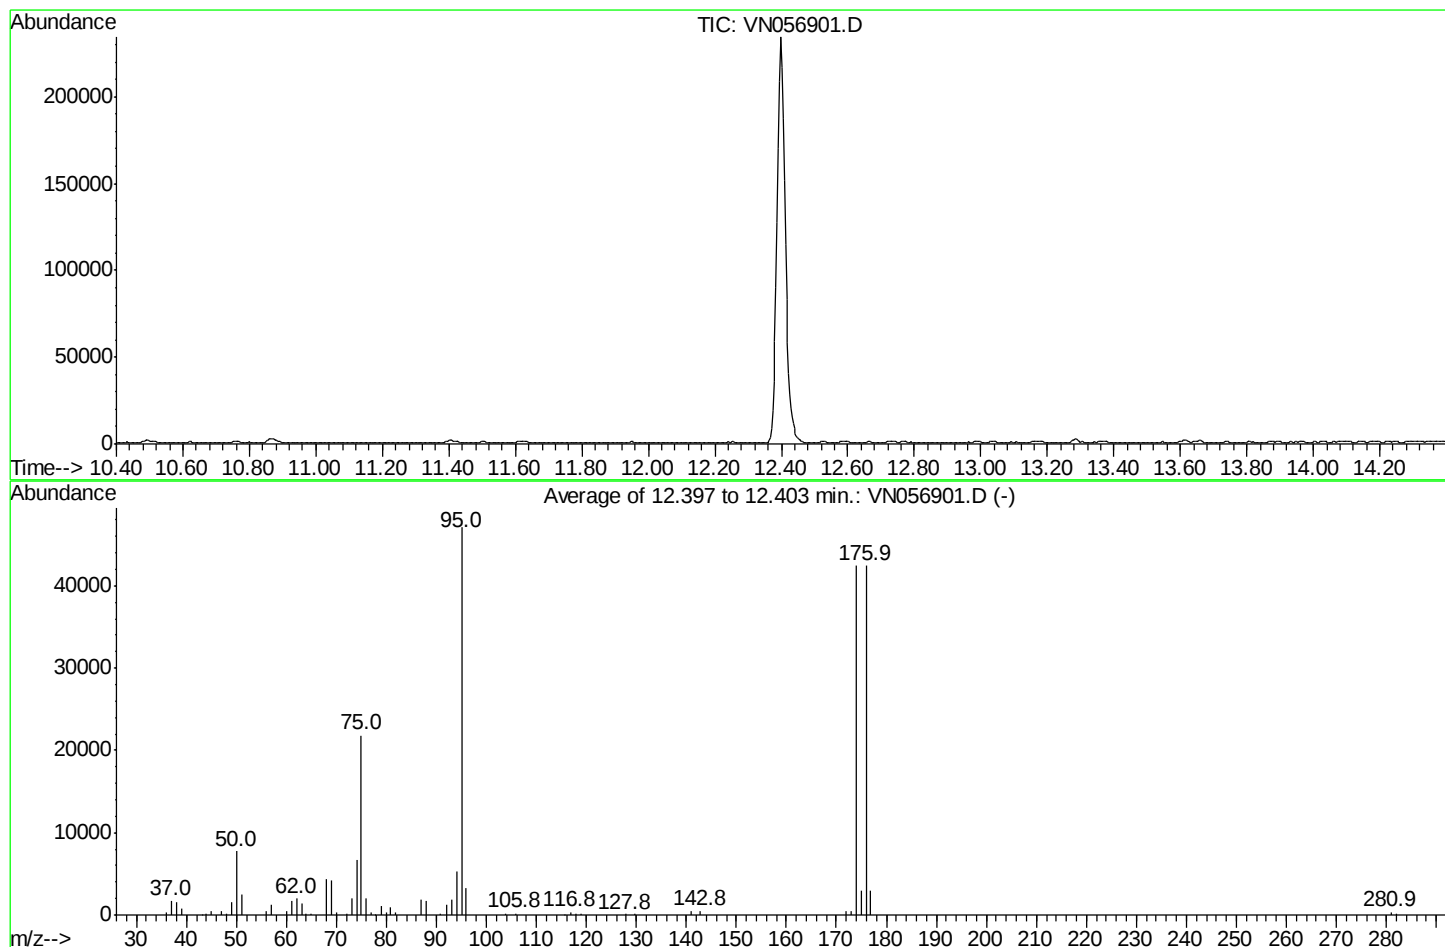

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	7712	PASS
75	95	30	60	46.4	21837	PASS
95	95	100	100	100.0	47098	PASS
96	95	5	9	7.0	3289	PASS
173	174	0.00	2	1.0	436	PASS
174	95	50	100	90.1	42426	PASS
175	174	5	9	6.9	2946	PASS
176	174	95	101	100.0	42429	PASS
177	176	5	9	6.9	2927	PASS