

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072522\
 Data File : VN073578.D
 Acq On : 25 Jul 2022 14:44
 Operator : JC\MD
 Sample : N3771-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-9F

Quant Time: Jul 26 02:17:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.022	168	236231	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	392906	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	363175	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	176375	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.375	65	153526	45.019	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	90.040%		
35) Dibromofluoromethane	7.951	113	127867	48.915	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	97.840%		
50) Toluene-d8	10.380	98	425402	45.820	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	91.640%		
62) 4-Bromofluorobenzene	12.674	95	173276	48.565	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	97.140%		
Target Compounds						Qvalue
3) Chloromethane	2.269	50	998	0.298	ug/l	100
6) Chloroethane	2.969	64	764	0.456	ug/l #	48
10) Methyl Iodide	4.357	142	53	3.749	ug/l #	44
12) 1,1-Dichloroethene	4.122	96	658	0.237	ug/l #	51
16) Acetone	4.240	43	11520	6.018	ug/l	96
18) Methyl Acetate	4.998	43	11225	2.093	ug/l #	48
20) Methylene Chloride	4.998	84	1344	0.400	ug/l #	75
25) 2-Butanone	7.269	43	3735	1.226	ug/l #	89
27) cis-1,2-Dichloroethene	7.239	96	782	0.222	ug/l	92
28) Bromochloromethane	7.745	49	4384	1.850	ug/l #	8
30) Chloroform	7.745	83	50974	8.946	ug/l	96
31) Cyclohexane	8.010	56	7494	1.342	ug/l #	61
36) 1,1-Dichloropropene	8.016	75	19482	4.844	ug/l #	49
38) Carbon Tetrachloride	8.022	117	24651	5.926	ug/l #	17
40) Benzene	8.398	78	3401	0.274	ug/l #	74
44) Trichloroethene	9.157	130	2915	0.923	ug/l	68
47) Bromodichloromethane	9.704	83	11748	2.824	ug/l #	91
52) Toluene	10.445	92	4107	0.535	ug/l	99
59) 2-Hexanone	11.027	43	1221	0.289	ug/l #	40
60) Dibromochloromethane	11.180	129	1955	0.649	ug/l	95
64) Tetrachloroethene	10.916	164	1181	0.398	ug/l #	68
67) Ethyl Benzene	11.786	91	35921	2.409	ug/l	96
68) m/p-Xylenes	11.904	106	5307	0.943	ug/l	99
69) o-Xylene	12.227	106	3674	0.640	ug/l	88
73) Isopropylbenzene	12.522	105	3330	0.219	ug/l	92
76) 1,2,3-Trichloropropane	12.674	75	93428	20.258	ug/l #	1
78) n-propylbenzene	12.863	91	5374	0.318	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.674	75	93428	55.557	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.310	105	14321	1.155	ug/l	97
95) Naphthalene	15.439	128	4346	0.320	ug/l #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072522\
Data File : VN073578.D
Acq On : 25 Jul 2022 14:44
Operator : JC\MD
Sample : N3771-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-9F

Quant Time: Jul 26 02:17:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




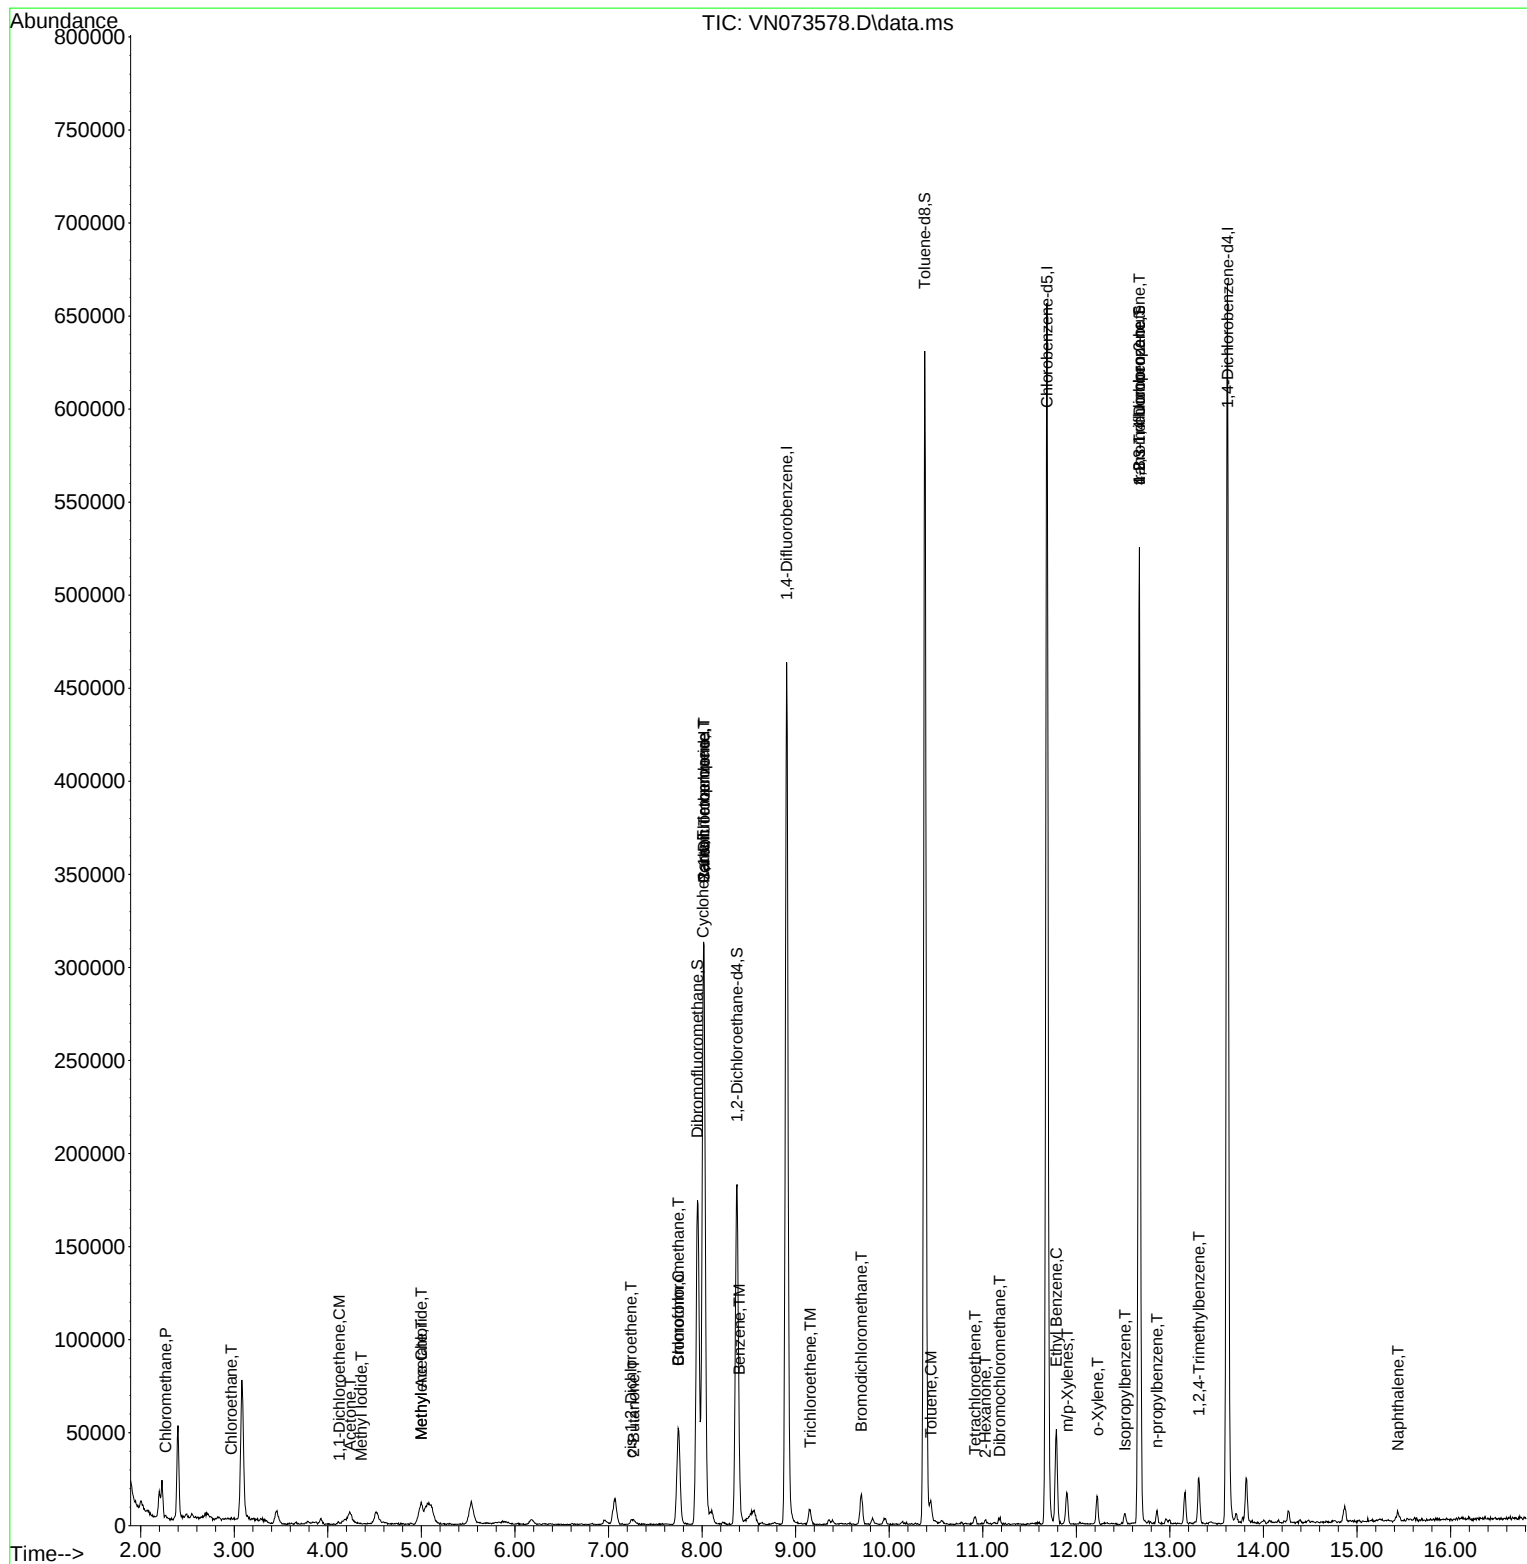




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. 0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion:168 Resp: 236231
Ion Ratio Lower Upper
168 100
99 57.4 42.3 63.5



#3
Chloromethane
Concen: 0.298 ug/l
RT: 2.269 min Scan# 65
Delta R.T. 0.000 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 50 Resp: 998
Ion Ratio Lower Upper
50 100
52 32.2 25.7 38.5


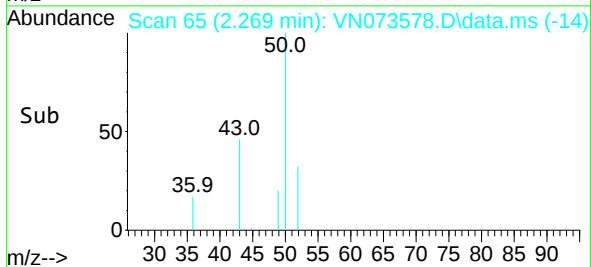

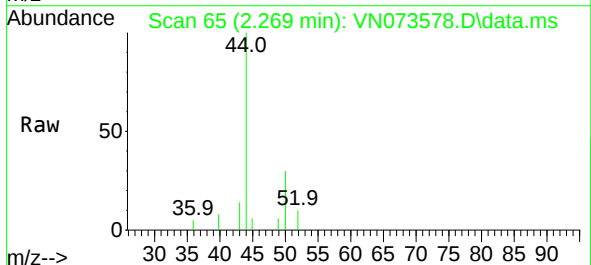




#6
Chloroethane
Concen: 0.456 ug/l
RT: 2.969 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 64 Resp: 764
Ion Ratio Lower Upper
64 100
66 3.4 26.2 39.4#

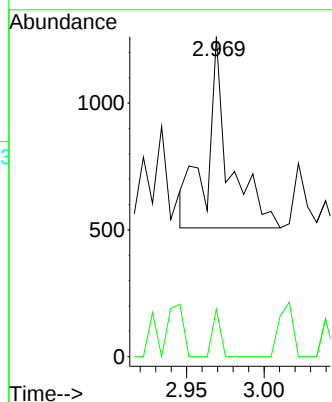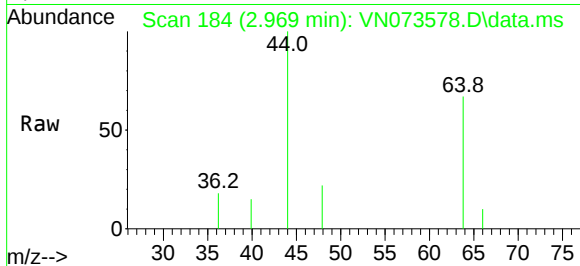

#10
Methyl Iodide
Concen: 3.749 ug/l
RT: 4.357 min Scan# 420
Delta R.T. 0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 142 Resp: 53
Ion Ratio Lower Upper
142 100
127 0.0 31.3 46.9#
141 0.0 11.2 16.8#


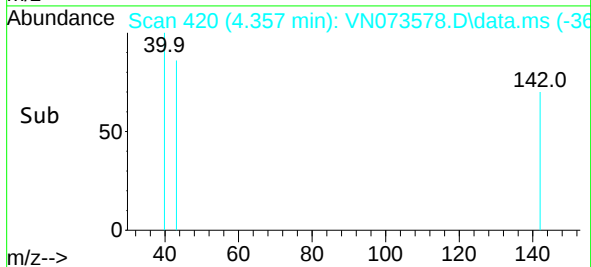

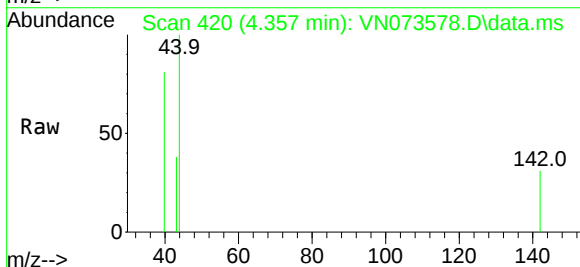




#12
1,1-Dichloroethene
Concen: 0.237 ug/l
RT: 4.122 min Scan# 379
Delta R.T. 0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 96 Resp: 658
Ion Ratio Lower Upper
96 100
61 112.4 127.6 191.4#
98 0.0 51.2 76.8#

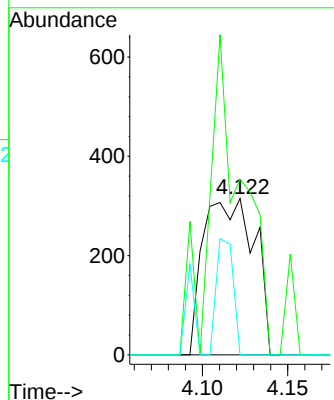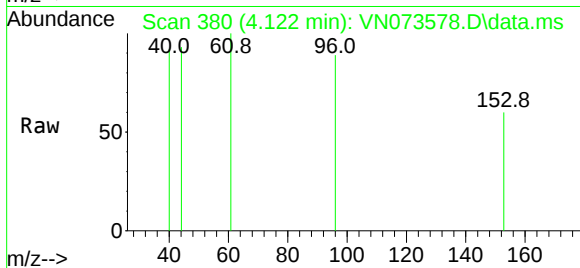

#16
Acetone
Concen: 6.018 ug/l
RT: 4.240 min Scan# 400
Delta R.T. 0.018 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 43 Resp: 11520
Ion Ratio Lower Upper
43 100
58 34.6 26.0 39.0


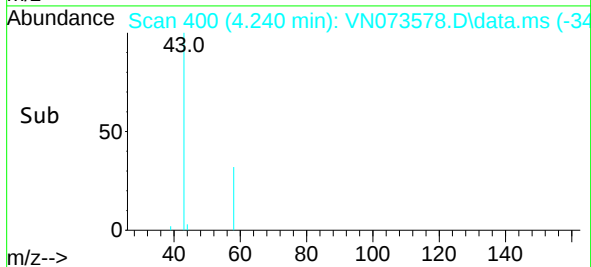
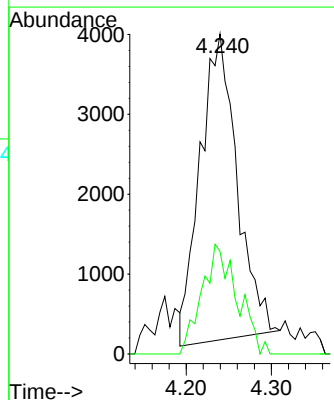
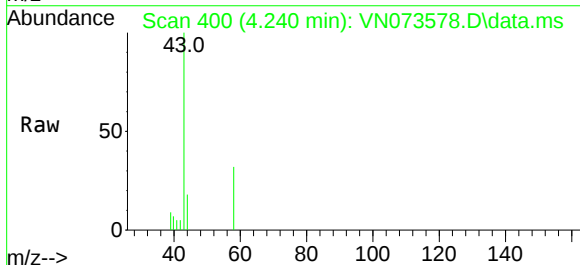




#18
Methyl Acetate
Concen: 2.093 ug/l
RT: 4.998 min Scan# 51
Delta R.T. 0.223 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 43 Resp: 11225
Ion Ratio Lower Upper
43 100
74 0.0 21.6 32.4#

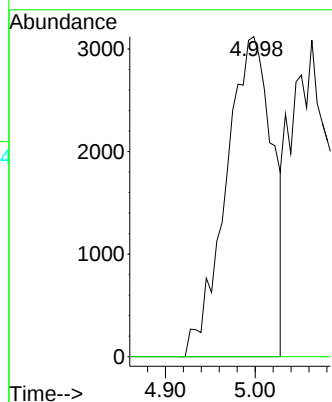

#20
Methylene Chloride
Concen: 0.400 ug/l
RT: 4.998 min Scan# 529
Delta R.T. -0.018 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 84 Resp: 1344
Ion Ratio Lower Upper
84 100
49 80.1 88.3 132.5#
51 39.7 28.2 42.2
86 41.2 50.6 76.0#


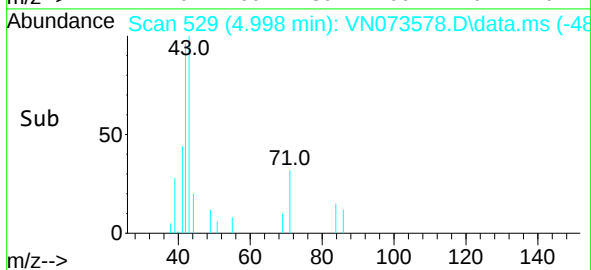






#25
2-Butanone
Concen: 1.226 ug/l
RT: 7.269 min Scan# 910
Delta R.T. 0.012 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 43 Resp: 3735
Ion Ratio Lower Upper
43 100
72 35.5 23.7 35.5#

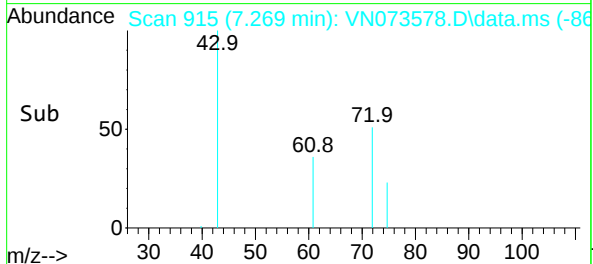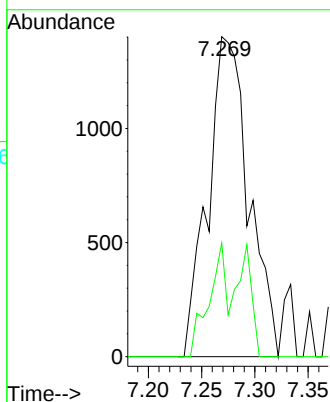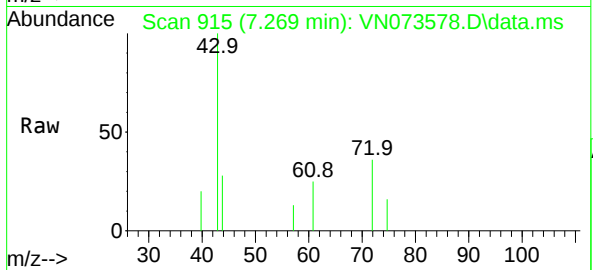

#27
cis-1,2-Dichloroethene
Concen: 0.222 ug/l
RT: 7.239 min Scan# 910
Delta R.T. -0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 96 Resp: 782
Ion Ratio Lower Upper
96 100
61 143.1 0.0 280.6
98 47.7 0.0 128.4


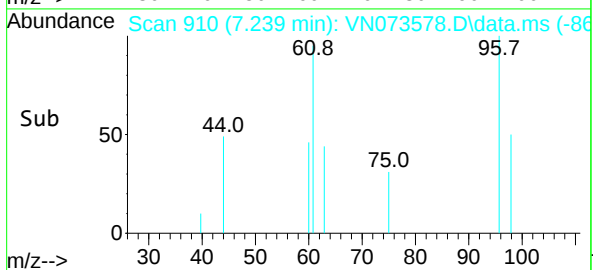
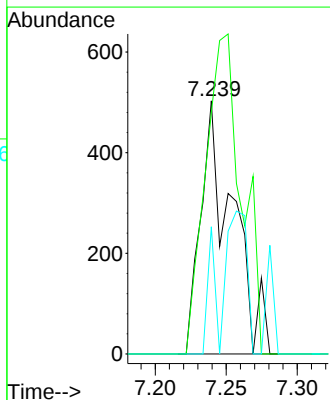
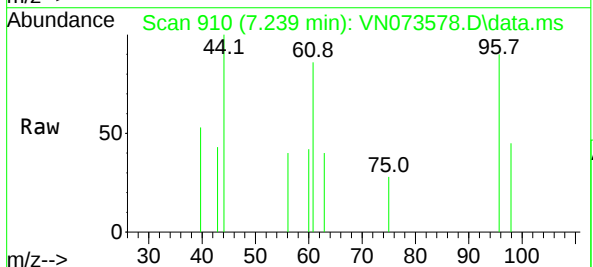




#28
Bromochloromethane
Concen: 1.850 ug/l
RT: 7.745 min Scan# 996
Delta R.T. 0.164 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 49 Resp: 4384
Ion Ratio Lower Upper
49 100
129 0.0 0.0 4.6
130 0.0 69.7 104.5#

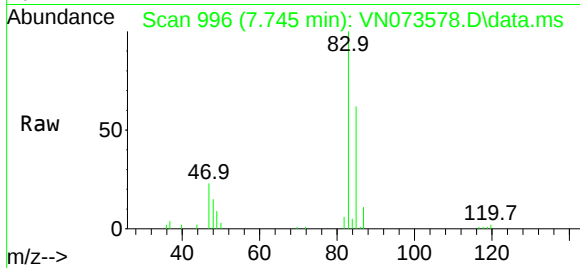

#30
Chloroform
Concen: 8.946 ug/l
RT: 7.745 min Scan# 996
Delta R.T. 0.000 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44


Tgt Ion: 83 Resp: 50974
Ion Ratio Lower Upper
83 100
85 61.7 51.8 77.8

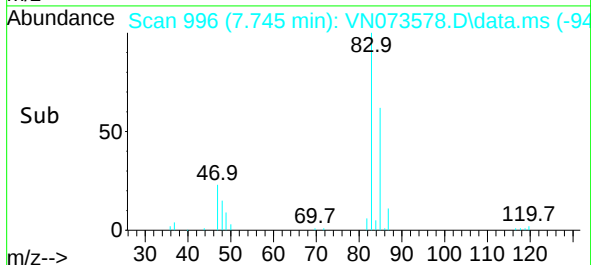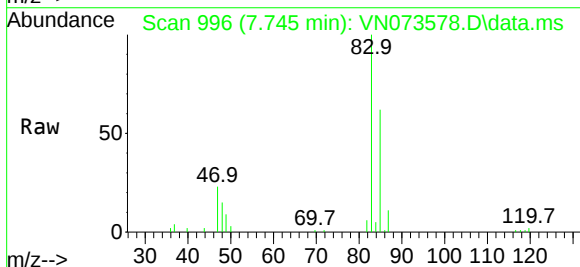



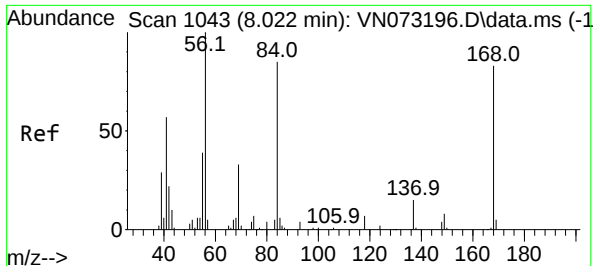


#31
Cyclohexane
Concen: 1.342 ug/l
RT: 8.010 min Scan# 1103
Delta R.T. -0.012 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Instrument :
MSVOA_N
ClientSampleId :
MW-9F







Tgt Ion: 56 Resp: 7494
Ion Ratio Lower Upper
56 100
69 115.3 27.8 41.8#
84 99.4 76.9 115.3

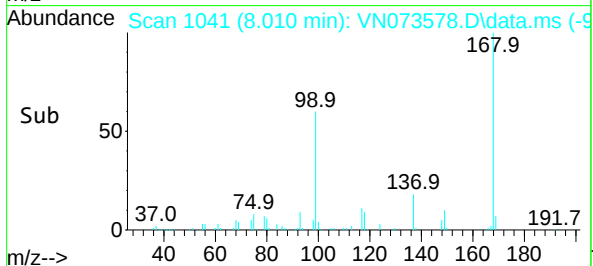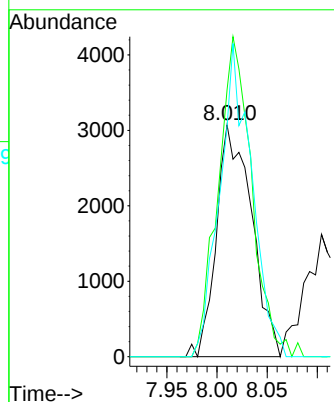

#33
1,2-Dichloroethane-d4
Concen: 45.019 ug/l
RT: 8.375 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 65 Resp: 153526
Ion Ratio Lower Upper
65 100
67 50.8 0.0 104.8

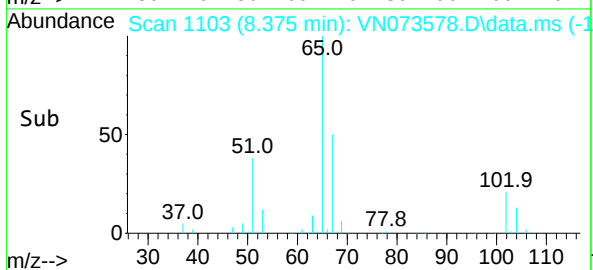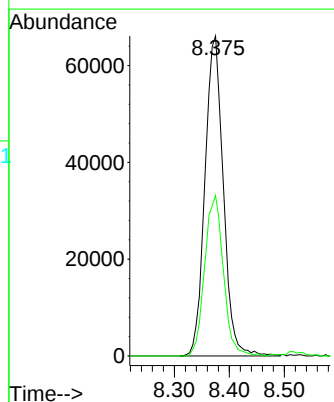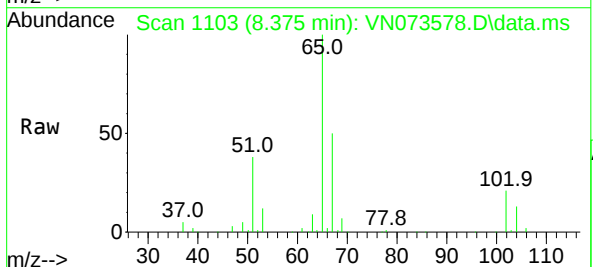

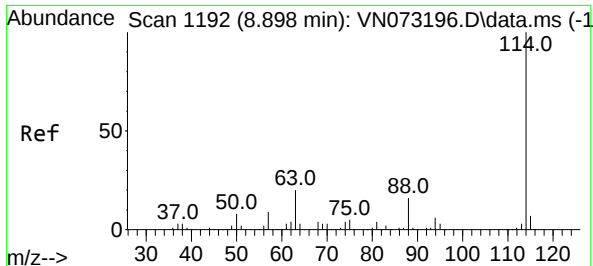

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1192

Delta R.T. 0.006 min

Lab File: VN073578.D

Acq: 25 Jul 2022 14:44

Instrument :

MSVOA_N

ClientSampleId :

MW-9F





Tgt Ion:114 Resp: 392906

Ion Ratio Lower Upper

114 100

63 21.2 0.0 40.0

88 15.9 0.0 32.6

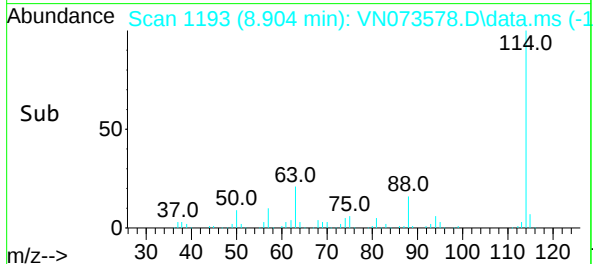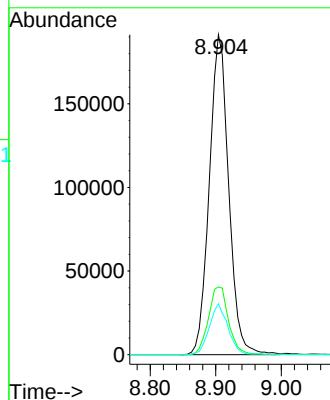

#35

Dibromofluoromethane

Concen: 48.915 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073578.D

Acq: 25 Jul 2022 14:44




Tgt Ion:113 Resp: 127867


Ion Ratio Lower Upper

113 100

111 105.0 81.4 122.0

192 19.1 17.0 25.6


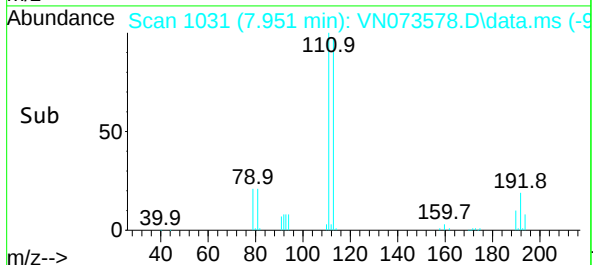
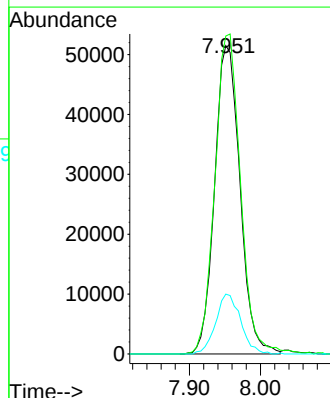
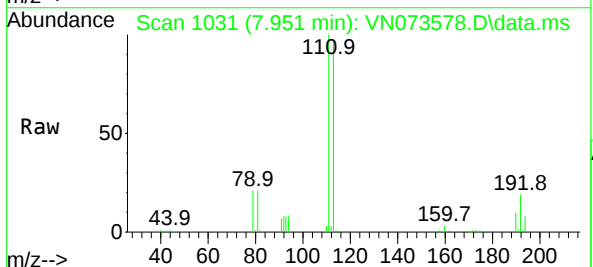


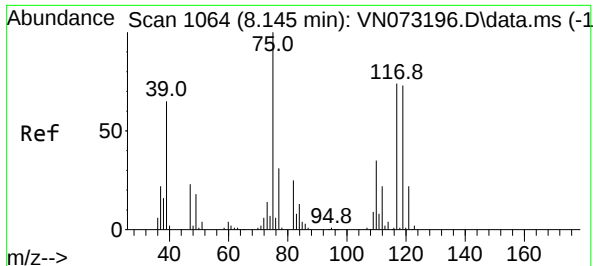

#36
1,1-Dichloropropene
Concen: 4.844 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.129 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 75 Resp: 19482
Ion Ratio Lower Upper
75 100
110 9.4 18.3 54.8#
77 0.0 25.1 37.7#

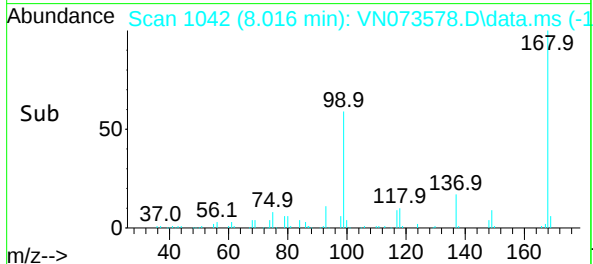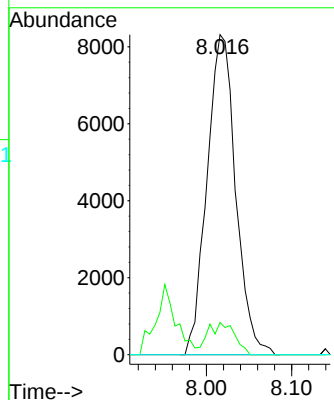

#38
Carbon Tetrachloride
Concen: 5.926 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. -0.112 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 117 Resp: 24651
Ion Ratio Lower Upper
117 100
119 5.6 75.8 113.8#
121 0.0 24.6 37.0#


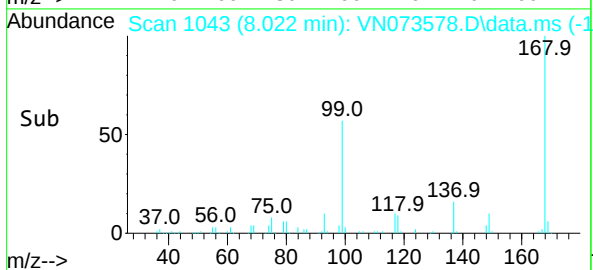
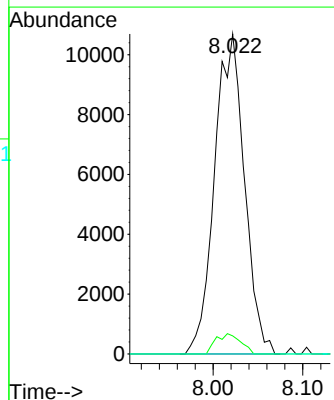
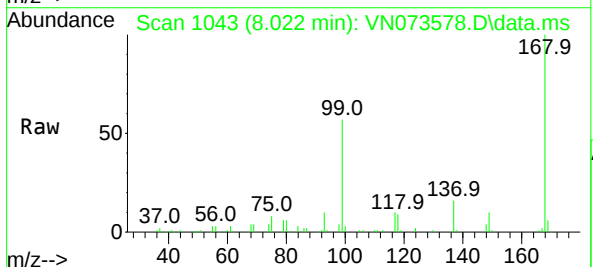




#40
Benzene
Concen: 0.274 ug/l
RT: 8.398 min Scan# 1105
Delta R.T. 0.012 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 78 Resp: 3401
Ion Ratio Lower Upper
78 100
77 11.5 19.4 29.0#

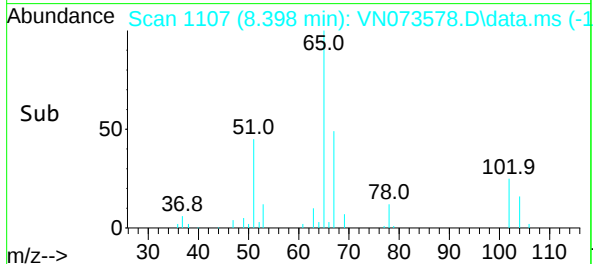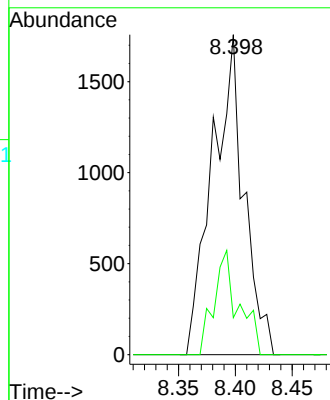

#44
Trichloroethene
Concen: 0.923 ug/l
RT: 9.157 min Scan# 1236
Delta R.T. 0.012 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion:130 Resp: 2915
Ion Ratio Lower Upper
130 100
95 124.0 0.0 186.8



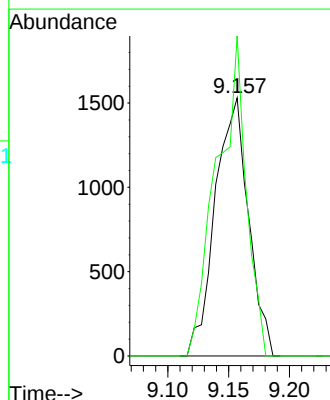
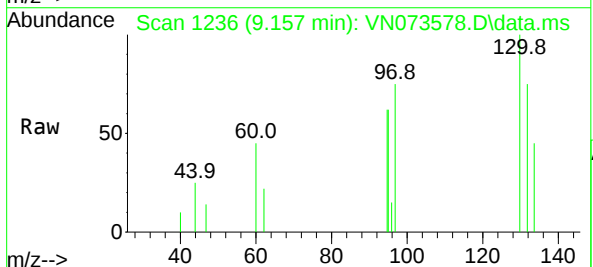




#47
Bromodichloromethane
Concen: 2.824 ug/l
RT: 9.704 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 83 Resp: 11748
Ion Ratio Lower Upper
83 100
85 70.7 50.5 75.7
127 10.4 6.8 10.2#

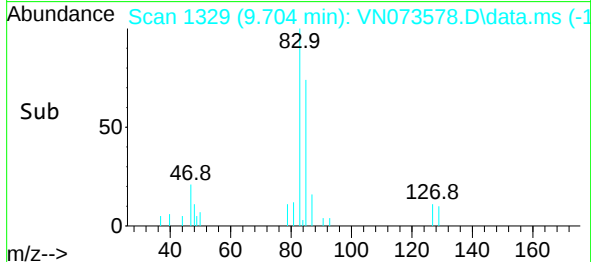

#50
Toluene-d8
Concen: 45.820 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.005 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 98 Resp: 425402
Ion Ratio Lower Upper
98 100
100 64.2 52.6 78.8


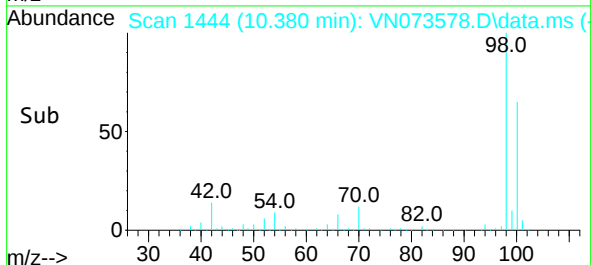
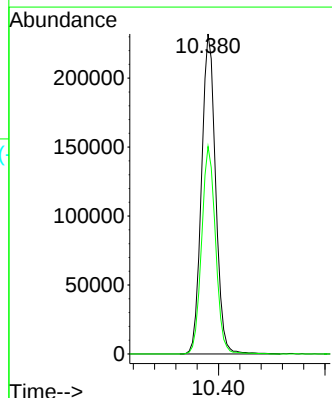
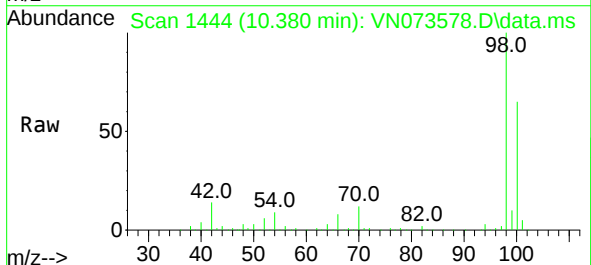




#52
Toluene
Concen: 0.535 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. 0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 92 Resp: 4107
Ion Ratio Lower Upper
92 100
91 171.8 138.6 207.8

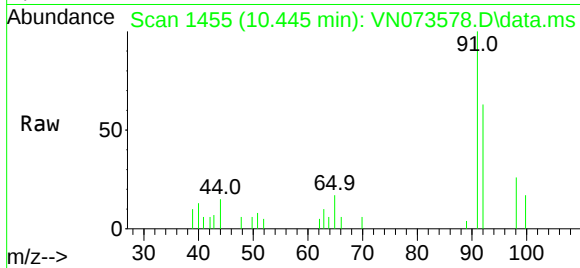

#59
2-Hexanone
Concen: 0.289 ug/l
RT: 11.027 min Scan# 1554
Delta R.T. 0.005 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 43 Resp: 1221
Ion Ratio Lower Upper
43 100
58 14.5 29.7 89.1#


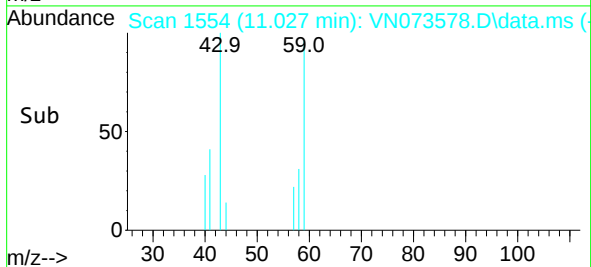

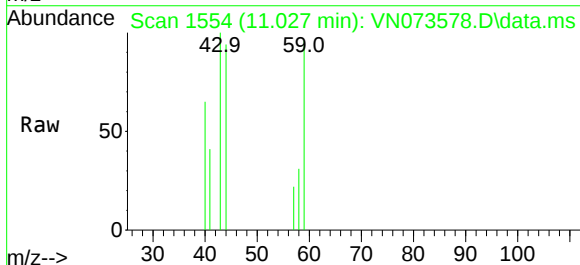




#60
Dibromochloromethane
Concen: 0.649 ug/l
RT: 11.180 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion:129 Resp: 1955
Ion Ratio Lower Upper
129 100
127 73.1 38.8 116.4

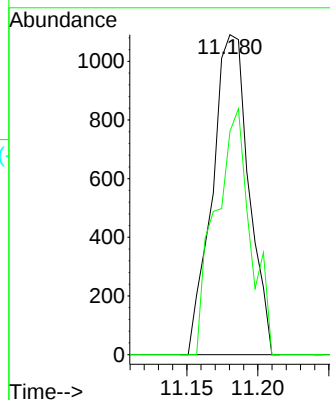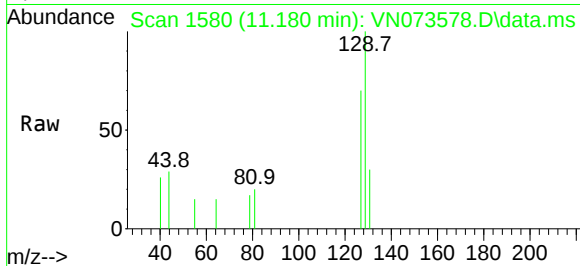

#62
4-Bromofluorobenzene
Concen: 48.565 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.005 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion: 95 Resp: 173276
Ion Ratio Lower Upper
95 100
174 78.5 0.0 167.6
176 74.2 0.0 163.4

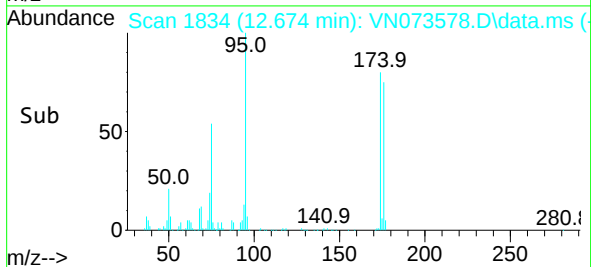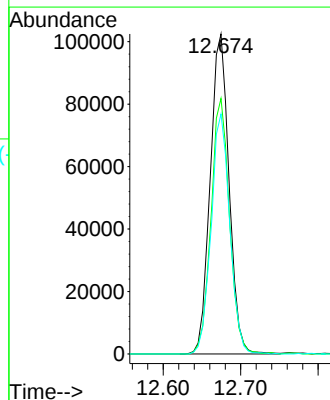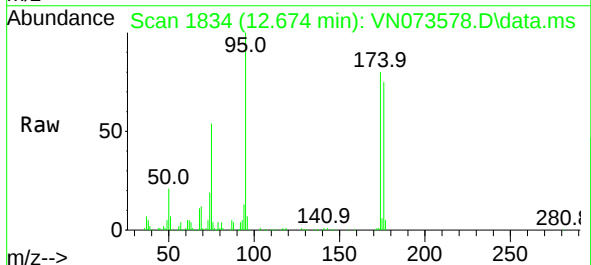

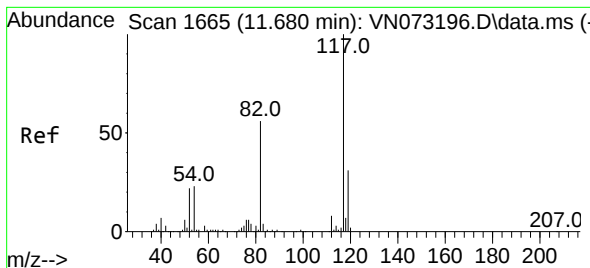

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.686 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN073578.D

Acq: 25 Jul 2022 14:44

Instrument :

MSVOA_N

ClientSampleId :

MW-9F





Tgt Ion:117 Resp: 363175

Ion Ratio Lower Upper

117 100

82 55.3 44.2 66.2

119 32.5 25.4 38.0

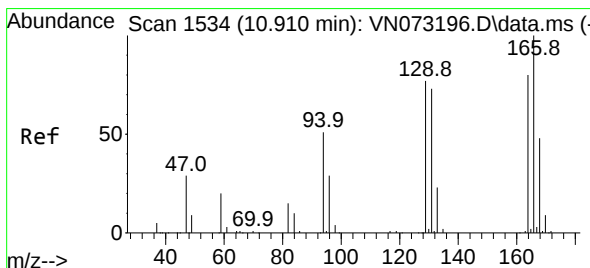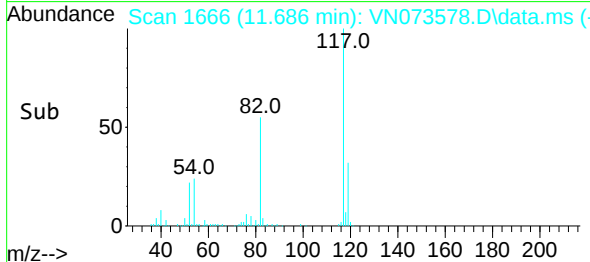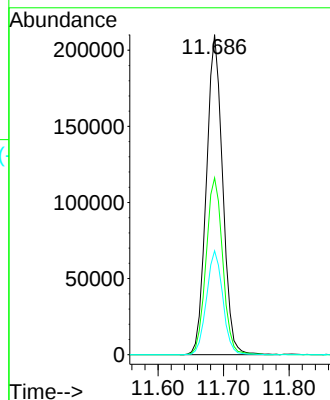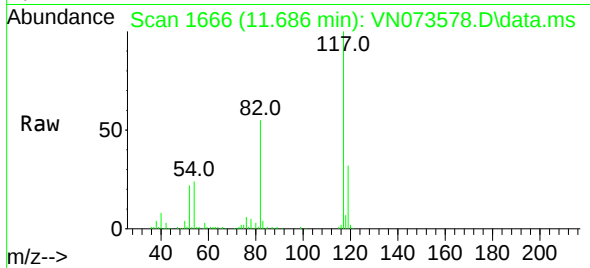

#64

Tetrachloroethene

Concen: 0.398 ug/l

RT: 10.916 min Scan# 1535

Delta R.T. 0.006 min

Lab File: VN073578.D

Acq: 25 Jul 2022 14:44

Tgt Ion:164 Resp: 1181




Ion Ratio Lower Upper


164 100

166 94.3 104.2 156.2#

129 52.6 73.9 110.9#

131 64.6 69.4 104.2#


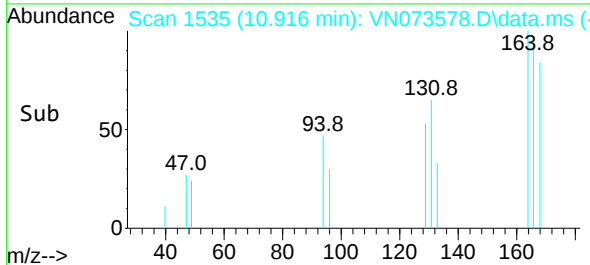
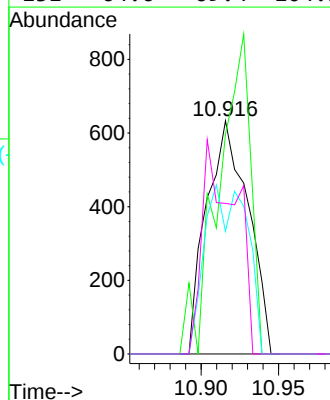
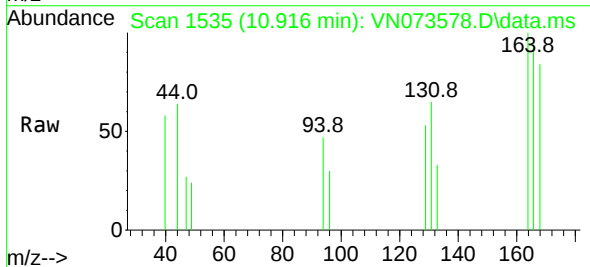




#67
Ethyl Benzene
Concen: 2.409 ug/l
RT: 11.786 min Scan# 1170
Delta R.T. 0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion: 91 Resp: 35921
Ion Ratio Lower Upper
91 100
106 33.4 24.9 37.3

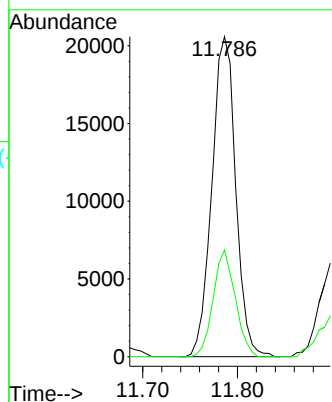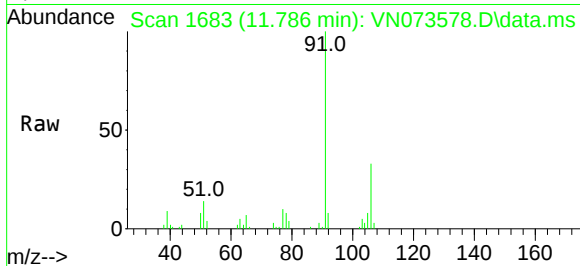

#68
m/p-Xylenes
Concen: 0.943 ug/l
RT: 11.904 min Scan# 1703
Delta R.T. 0.012 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion:106 Resp: 5307
Ion Ratio Lower Upper
106 100
91 199.4 158.9 238.3


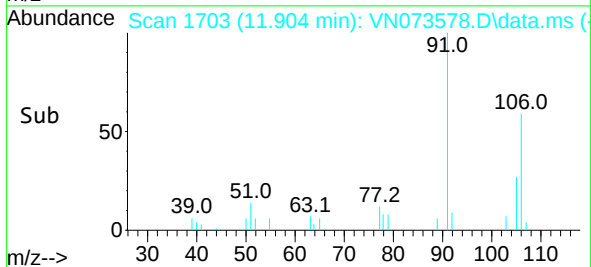
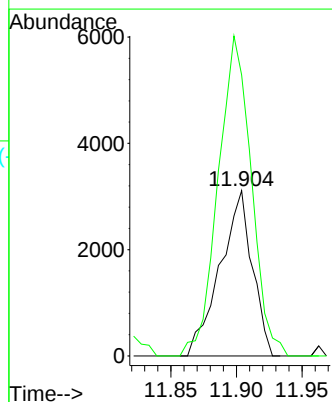
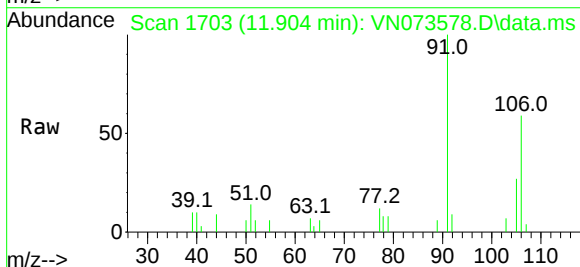




#69
o-Xylene
Concen: 0.640 ug/l
RT: 12.227 min Scan# 11
Delta R.T. 0.011 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44




Instrument :
MSVOA_N
ClientSampleId :
MW-9F


Tgt Ion:106 Resp: 3674
Ion Ratio Lower Upper
106 100
91 231.4 106.0 318.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.616 min Scan# 1994
Delta R.T. 0.006 min
Lab File: VN073578.D
Acq: 25 Jul 2022 14:44

Tgt Ion:152 Resp: 176375
Ion Ratio Lower Upper
152 100
115 60.0 28.9 86.7
150 158.8 0.0 356.2

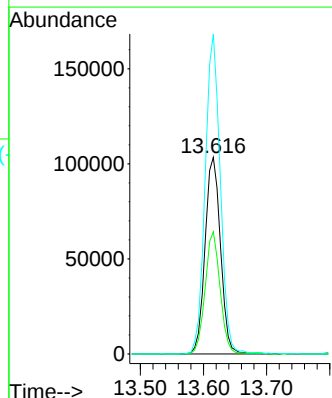

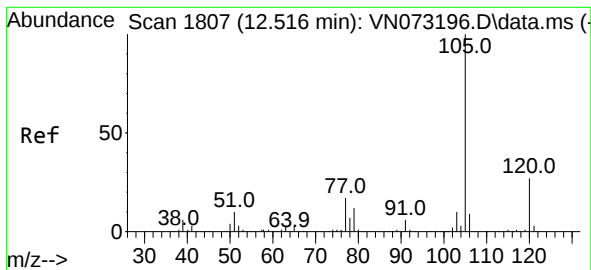

#73

Isopropylbenzene

Concen: 0.219 ug/l

RT: 12.522 min Scan# 1808

Delta R.T. 0.005 min

Lab File: VN073578.D

Acq: 25 Jul 2022 14:44

Instrument :

MSVOA_N

ClientSampleId :





MW-9F

Tgt Ion:105 Resp: 3330

Ion Ratio Lower Upper

105 100

120 31.0 13.5 40.4

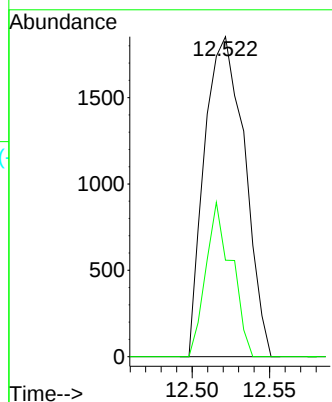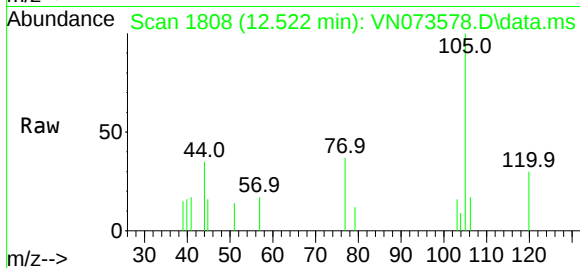

#76

1,2,3-Trichloropropane

Concen: 20.258 ug/l

RT: 12.674 min Scan# 1834

Delta R.T. -0.142 min

Lab File: VN073578.D




Acq: 25 Jul 2022 14:44


Tgt Ion: 75 Resp: 93428

Ion Ratio Lower Upper

75 100

77 1.3 98.5 295.5#

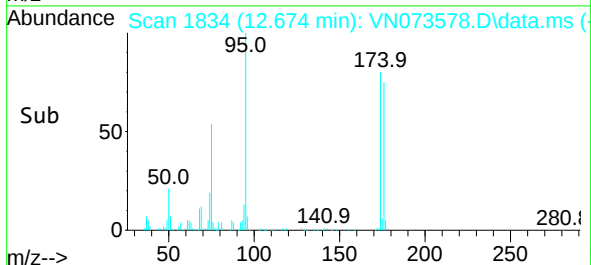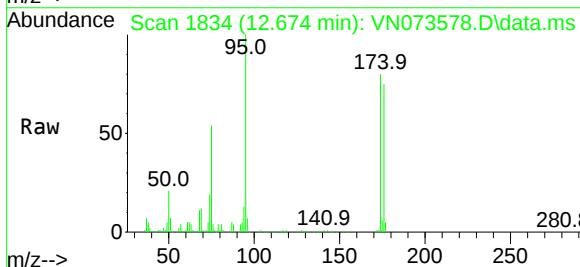

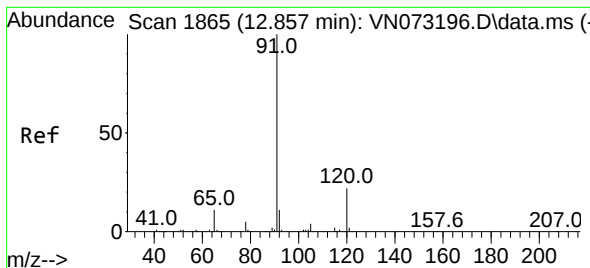

#78

n-propylbenzene

Concen: 0.318 ug/l

RT: 12.863 min Scan# 1866

Delta R.T. 0.006 min

Lab File: VN073578.D

Acq: 25 Jul 2022 14:44

Instrument :

MSVOA_N

ClientSampleId :





MW-9F

Tgt Ion: 91 Resp: 5374

Ion Ratio Lower Upper

91 100

120 22.8 11.9 35.5

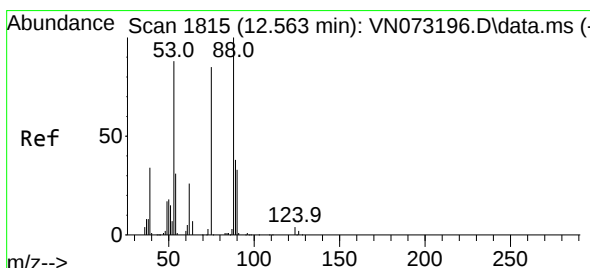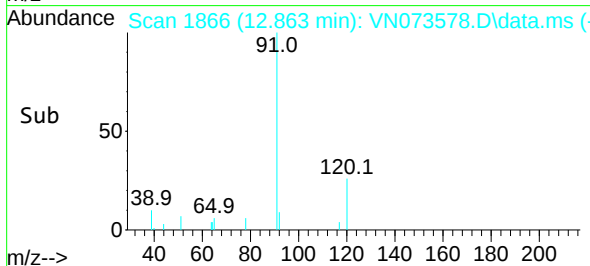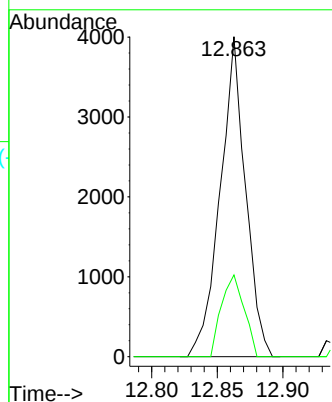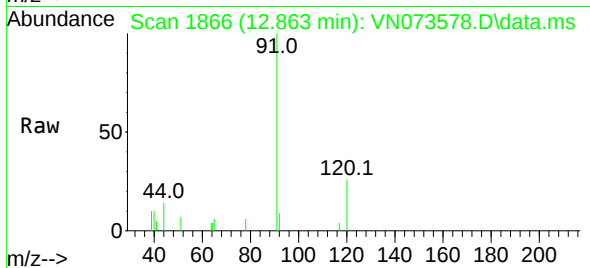

#81

trans-1,4-Dichloro-2-butene

Concen: 55.557 ug/l

RT: 12.674 min Scan# 1834

Delta R.T. 0.111 min

Lab File: VN073578.D

Acq: 25 Jul 2022 14:44




Tgt Ion: 75 Resp: 93428


Ion Ratio Lower Upper

75 100

53 0.2 78.0 117.0#

89 0.0 37.2 55.8#

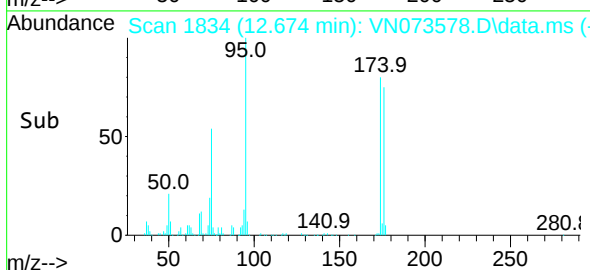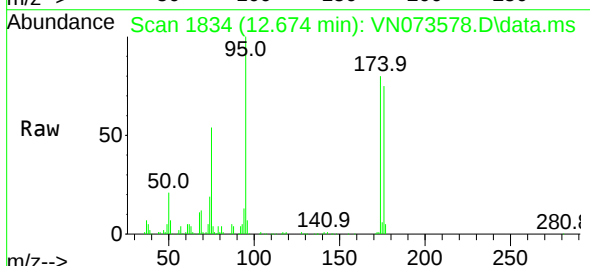



#84

1,2,4-Trimethylbenzene

Concen: 1.155 ug/l

RT: 13.310 min Scan# 1941

Delta R.T. 0.006 min

Lab File: VN073578.D

Acq: 25 Jul 2022 14:44

Instrument :

MSVOA_N

ClientSampleId :





MW-9F

Tgt Ion:105 Resp: 14321

Ion Ratio Lower Upper

105 100

120 44.4 23.3 69.8

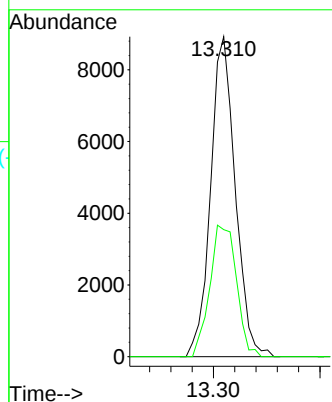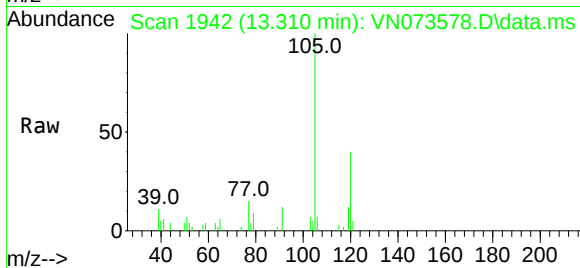

#95

Naphthalene

Concen: 0.320 ug/l

RT: 15.439 min Scan# 2304

Delta R.T. 0.012 min

Lab File: VN073578.D

Acq: 25 Jul 2022 14:44

Tgt Ion:128 Resp: 4346

Ion Ratio Lower Upper

128 100

127 9.2 10.3 15.5#

129 13.2 8.6 13.0#

