


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN072618\
Data File : VN050097.D
Acq On : 26 Jul 2018 21:51
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Title : SW846 8260
Last Update : Thu Jul 26 18:10:10 2018

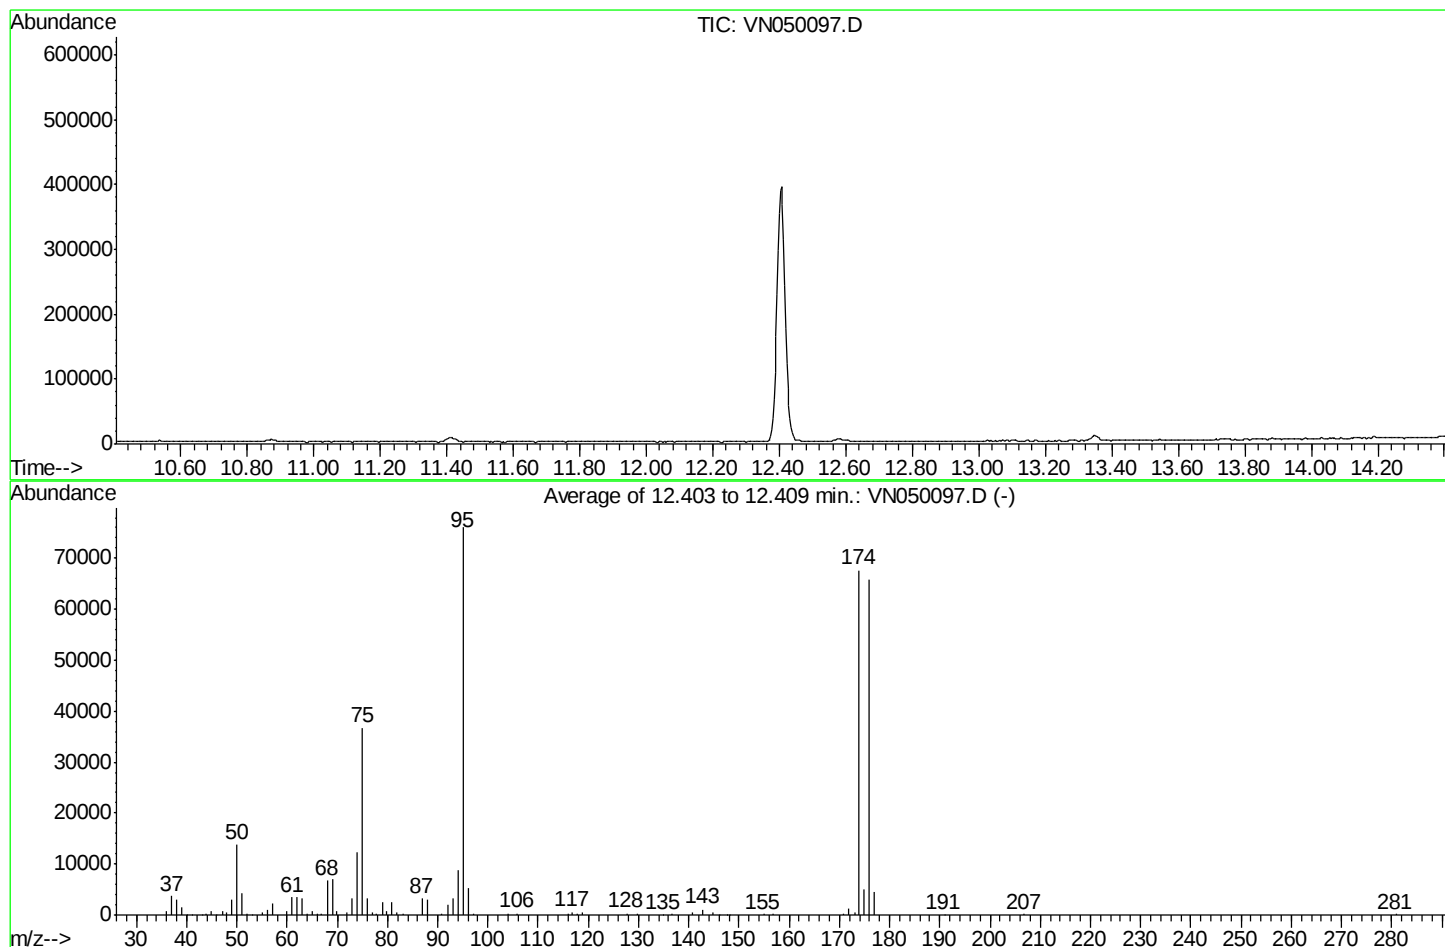

AutoFind: Scans 3363, 3364, 3365; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	13739	PASS
75	95	30	60	48.3	36728	PASS
95	95	100	100	100.0	76080	PASS
96	95	5	9	7.0	5290	PASS
173	174	0.00	2	0.9	589	PASS
174	95	50	100	88.9	67661	PASS
175	174	5	9	7.5	5090	PASS
176	174	95	101	97.2	65776	PASS
177	176	5	9	6.8	4466	PASS