


Instrument :
MSVOA_N
ClientSampleId :

Dichlorodifluoromethane

Response Ratio

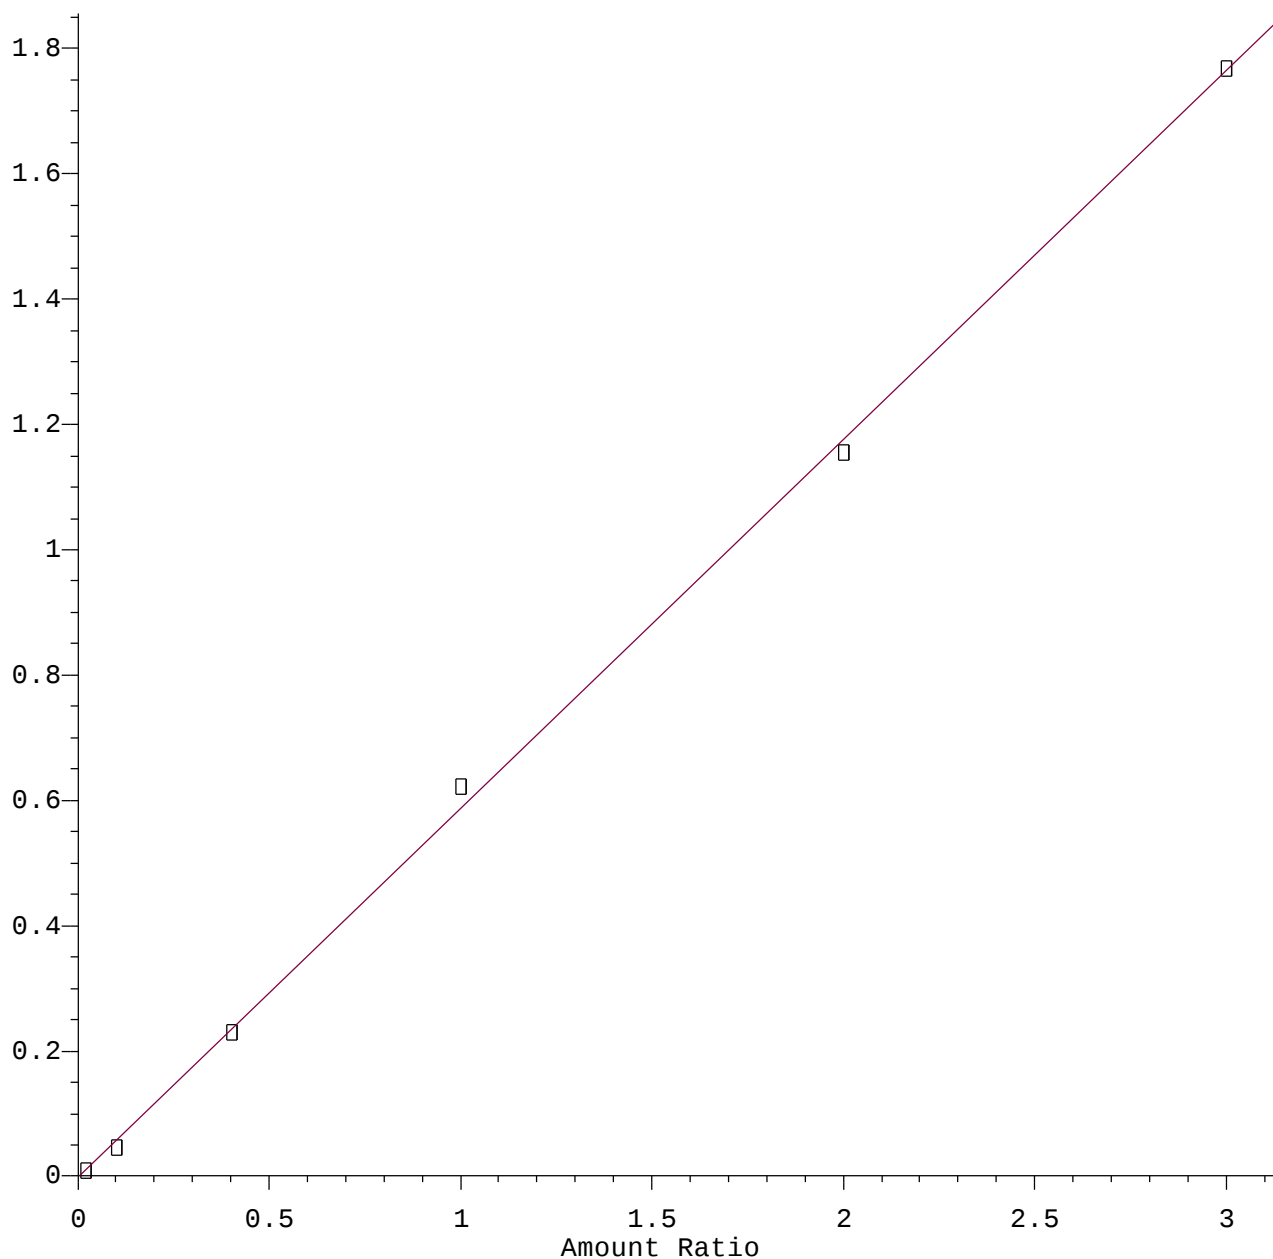


Resp Ratio = $5.89 \times 10^{-1} \times \text{Amt} - 2.03 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

2-Chloroethyl Vinyl ether


Response Ratio

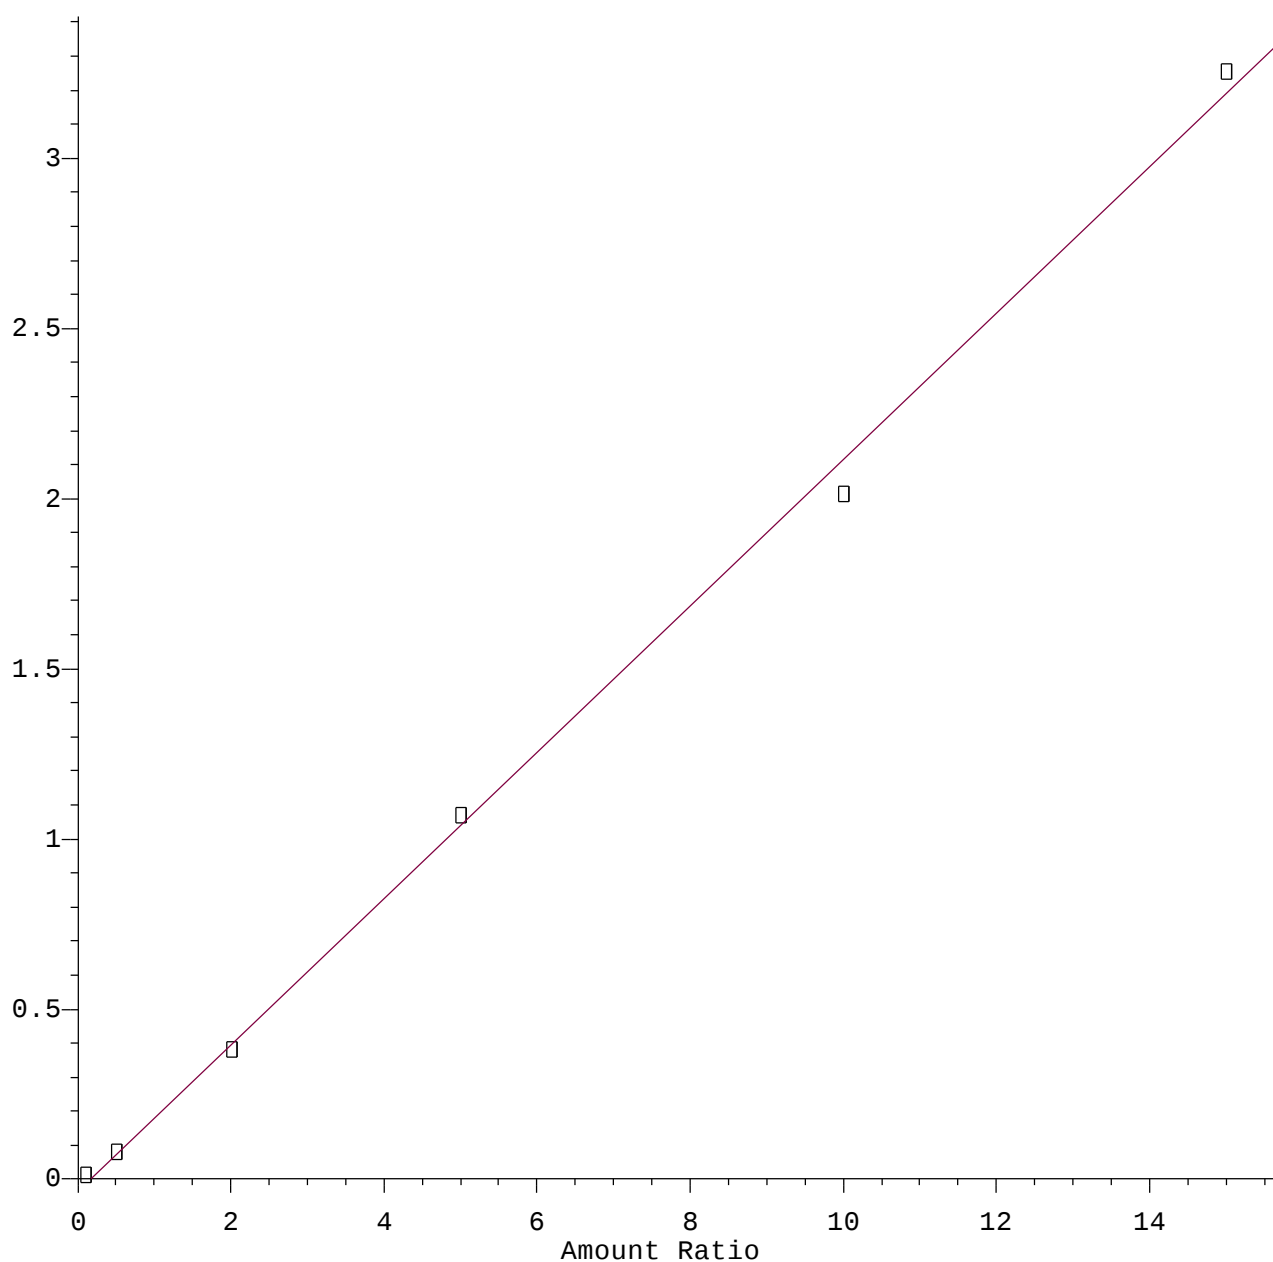

Resp Ratio = $2.15 \times 10^{-1} \times \text{Amt} - 3.38 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

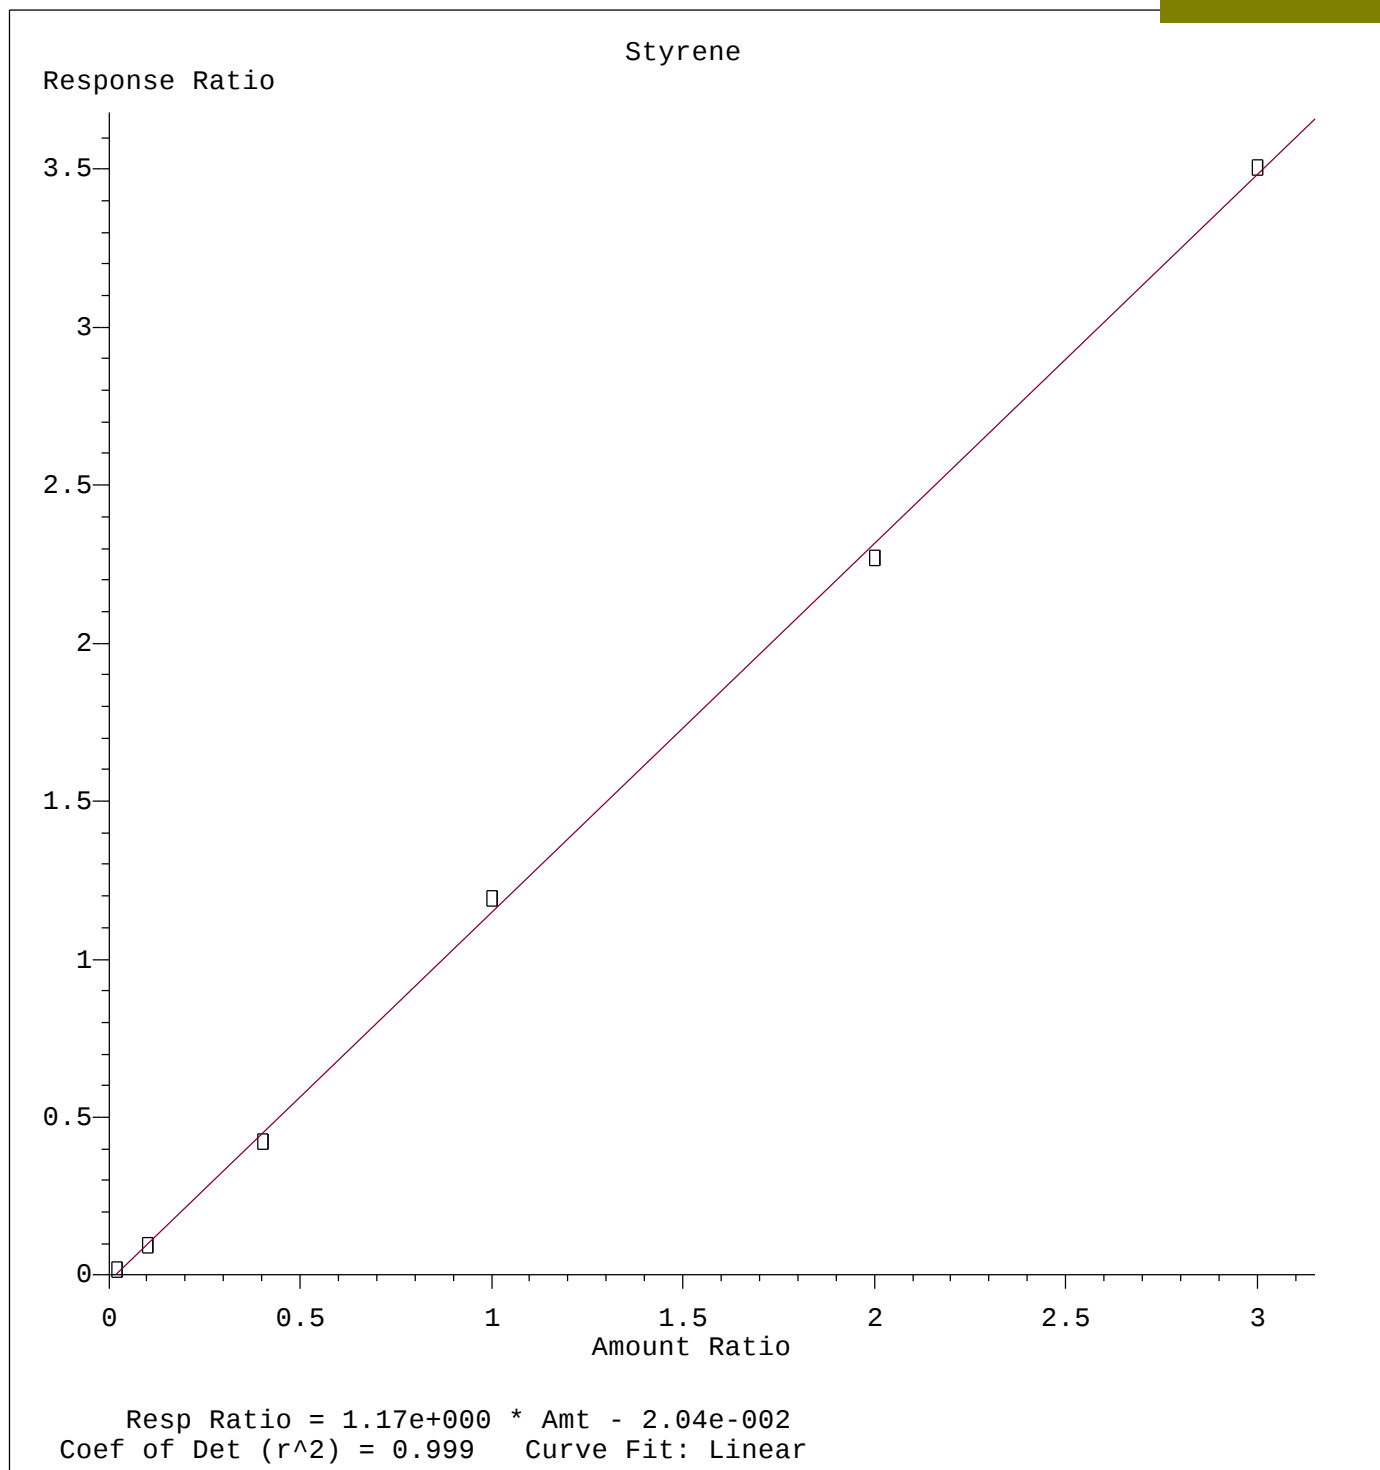

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

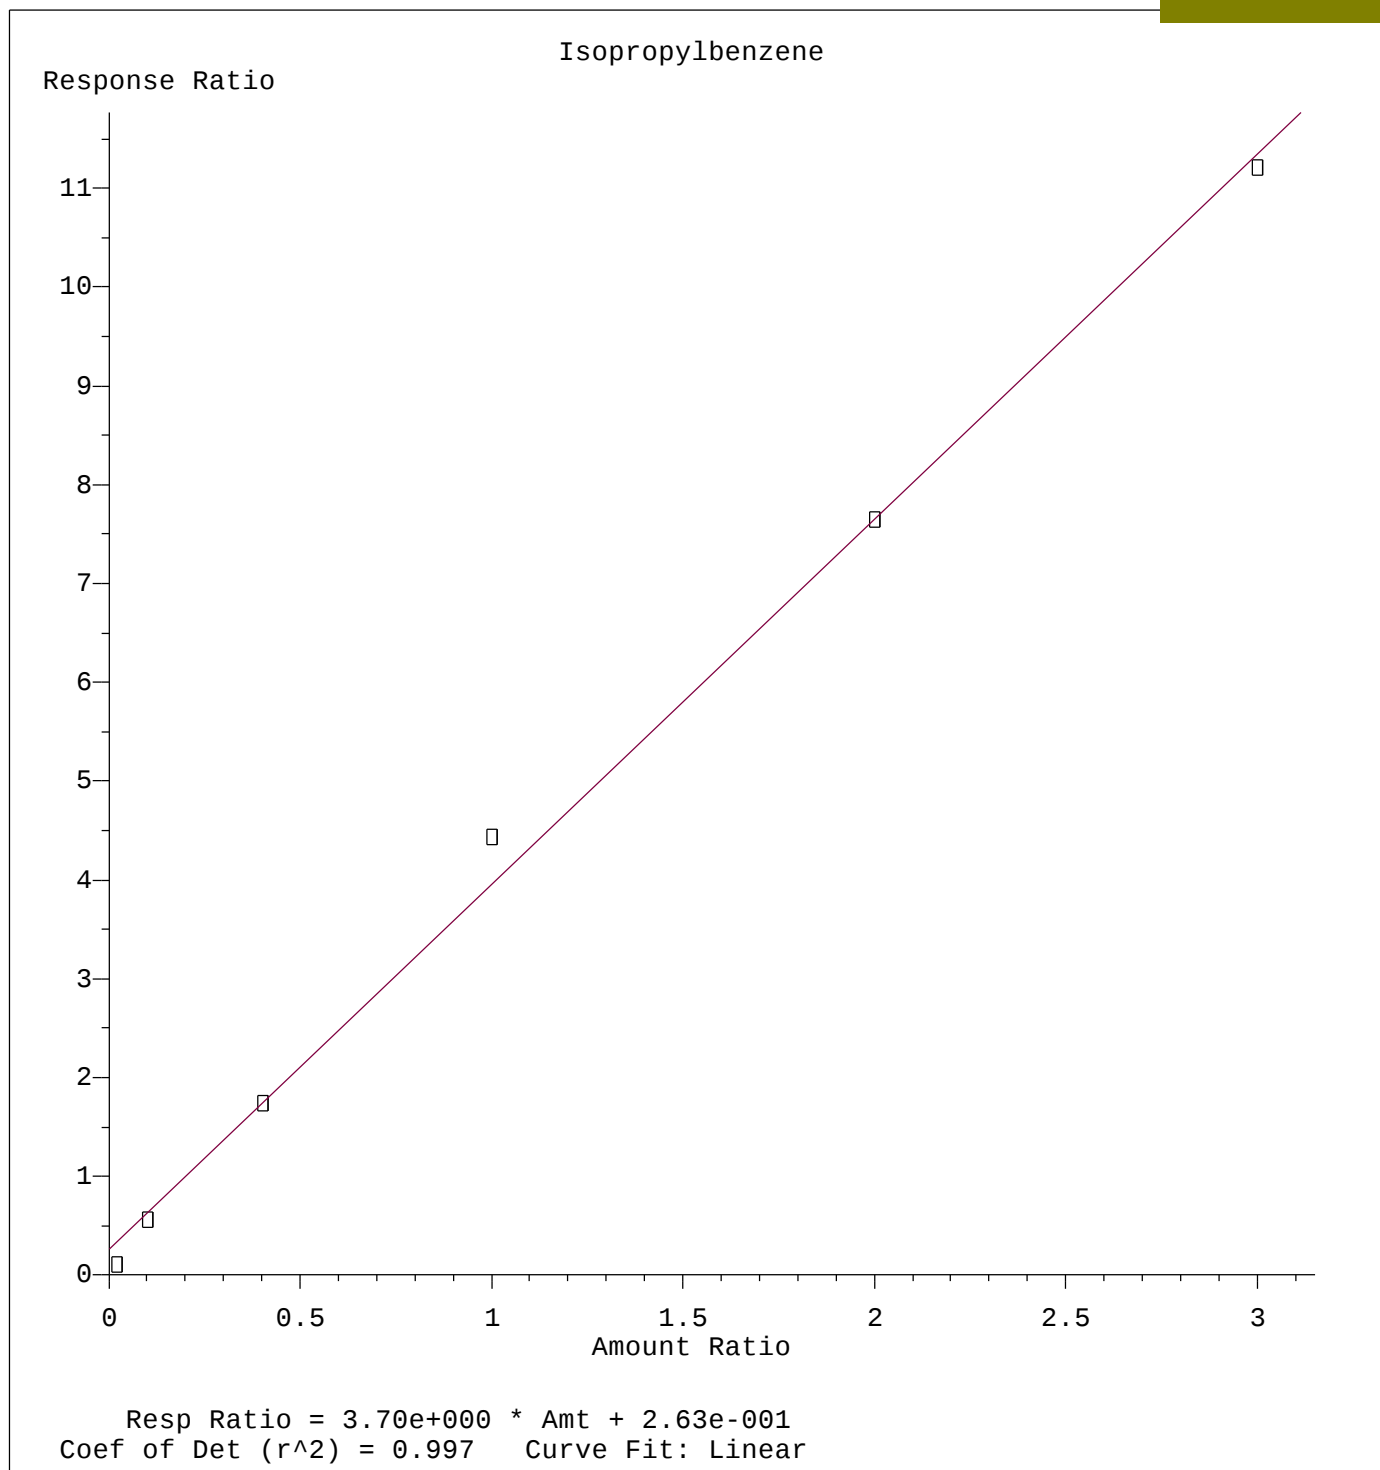


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

1,1,2,2-Tetrachloroethane

Response Ratio

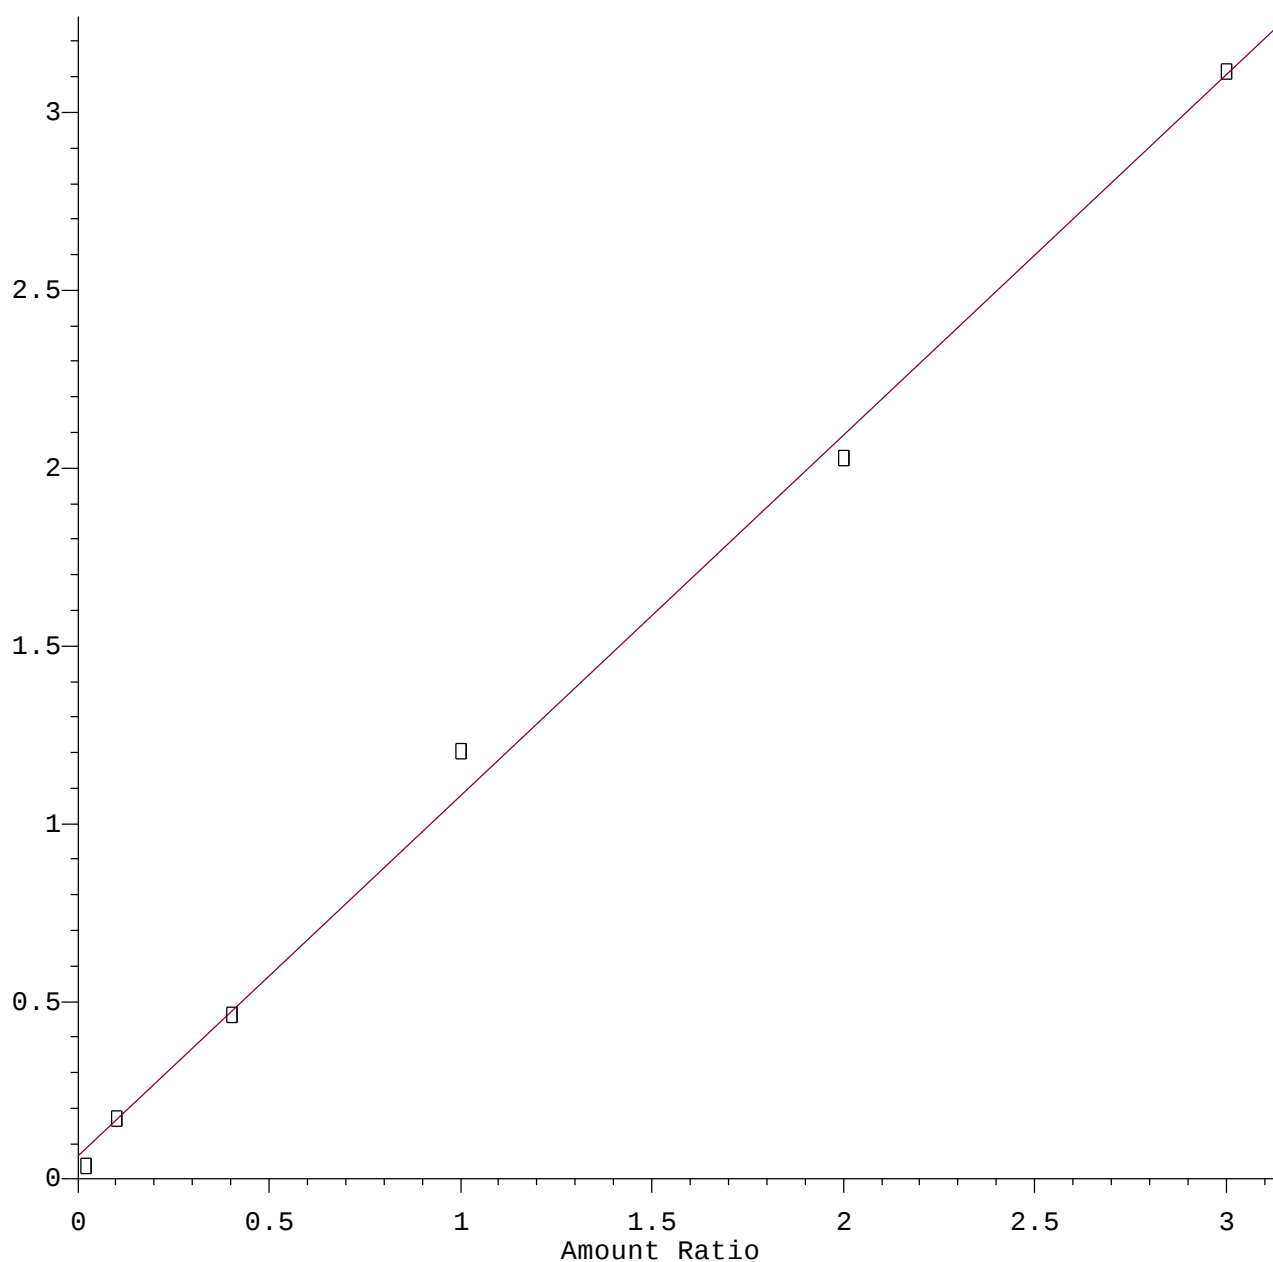


Resp Ratio = 1.01e+000 * Amt + 6.65e-002
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

1,2,3-Trichloropropane

Response Ratio

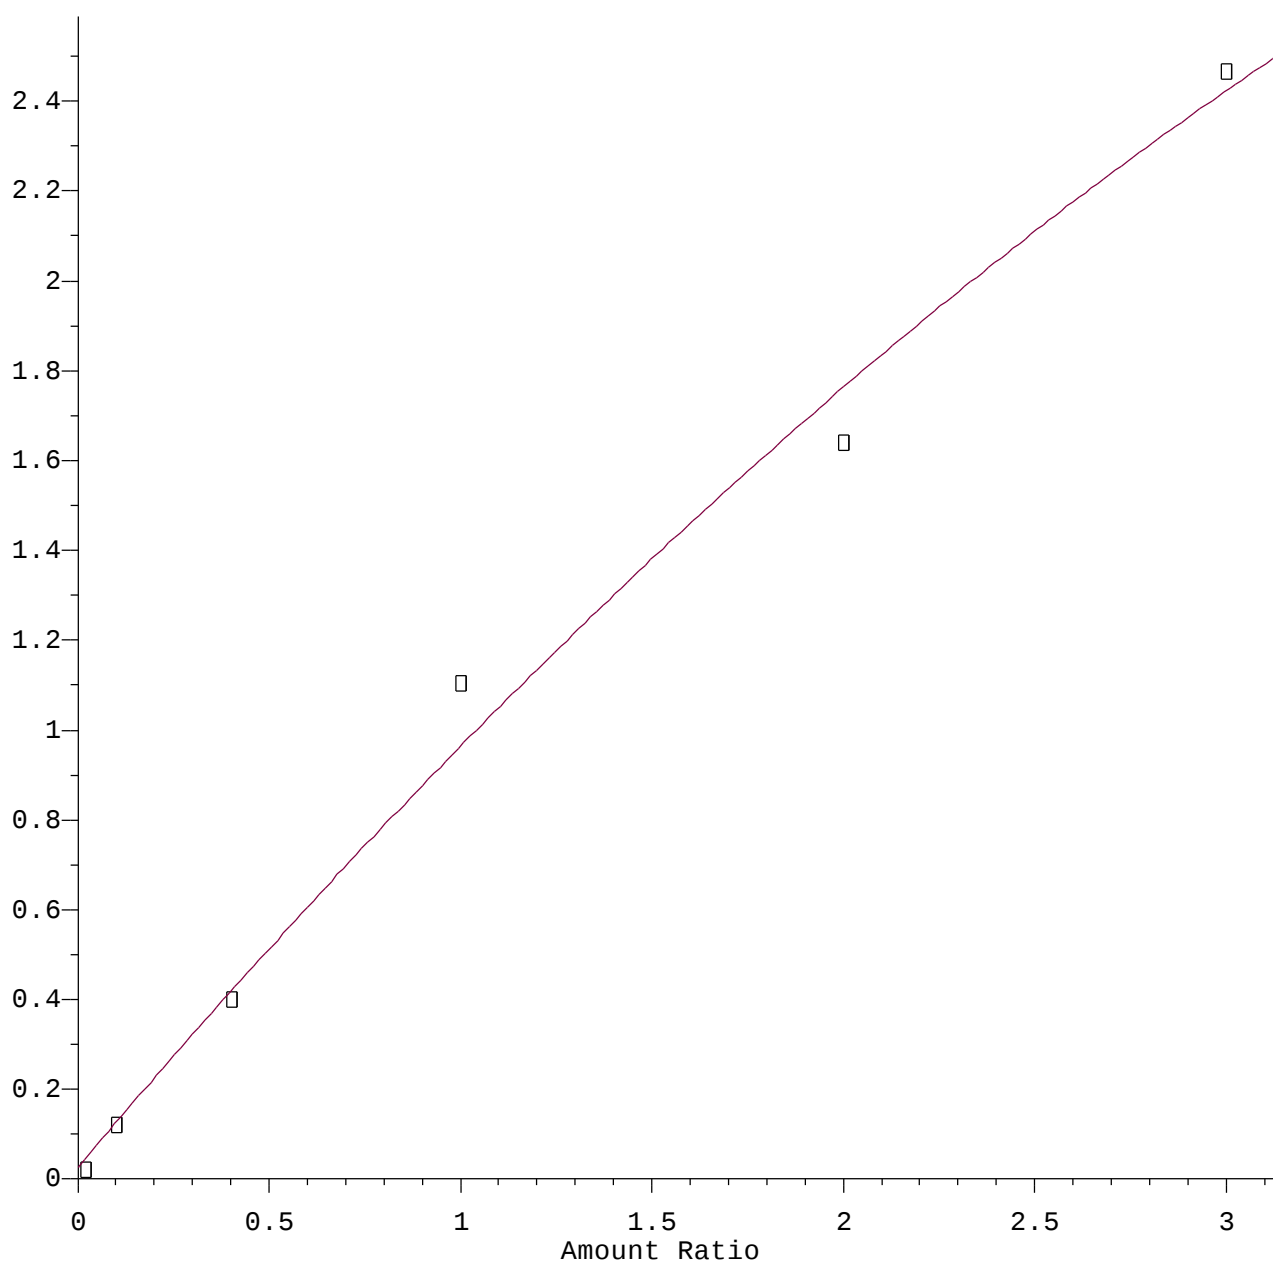


$R = -6.90e-002 A^2 + 1.01e+000 A + 2.75e-002$
Coef of Det (r^2) = 0.992 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

2-Chlorotoluene

Response Ratio

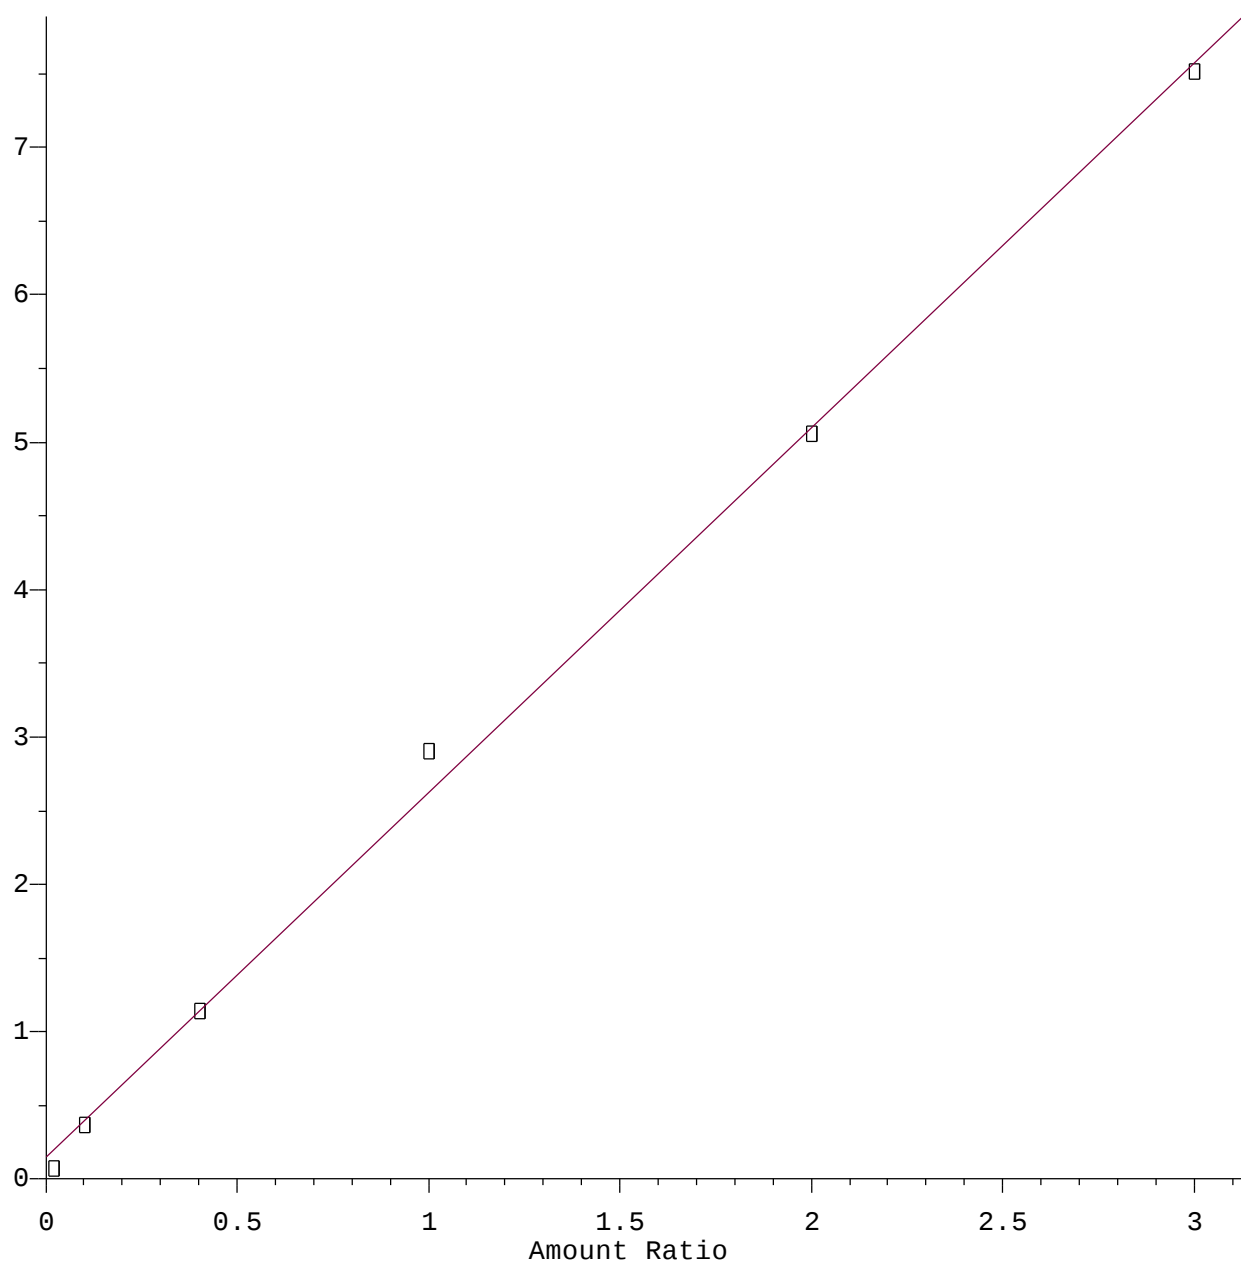


Resp Ratio = $2.47 \times 10^0 * \text{Amt} + 1.51 \times 10^{-1}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

tert-Butylbenzene


Response Ratio

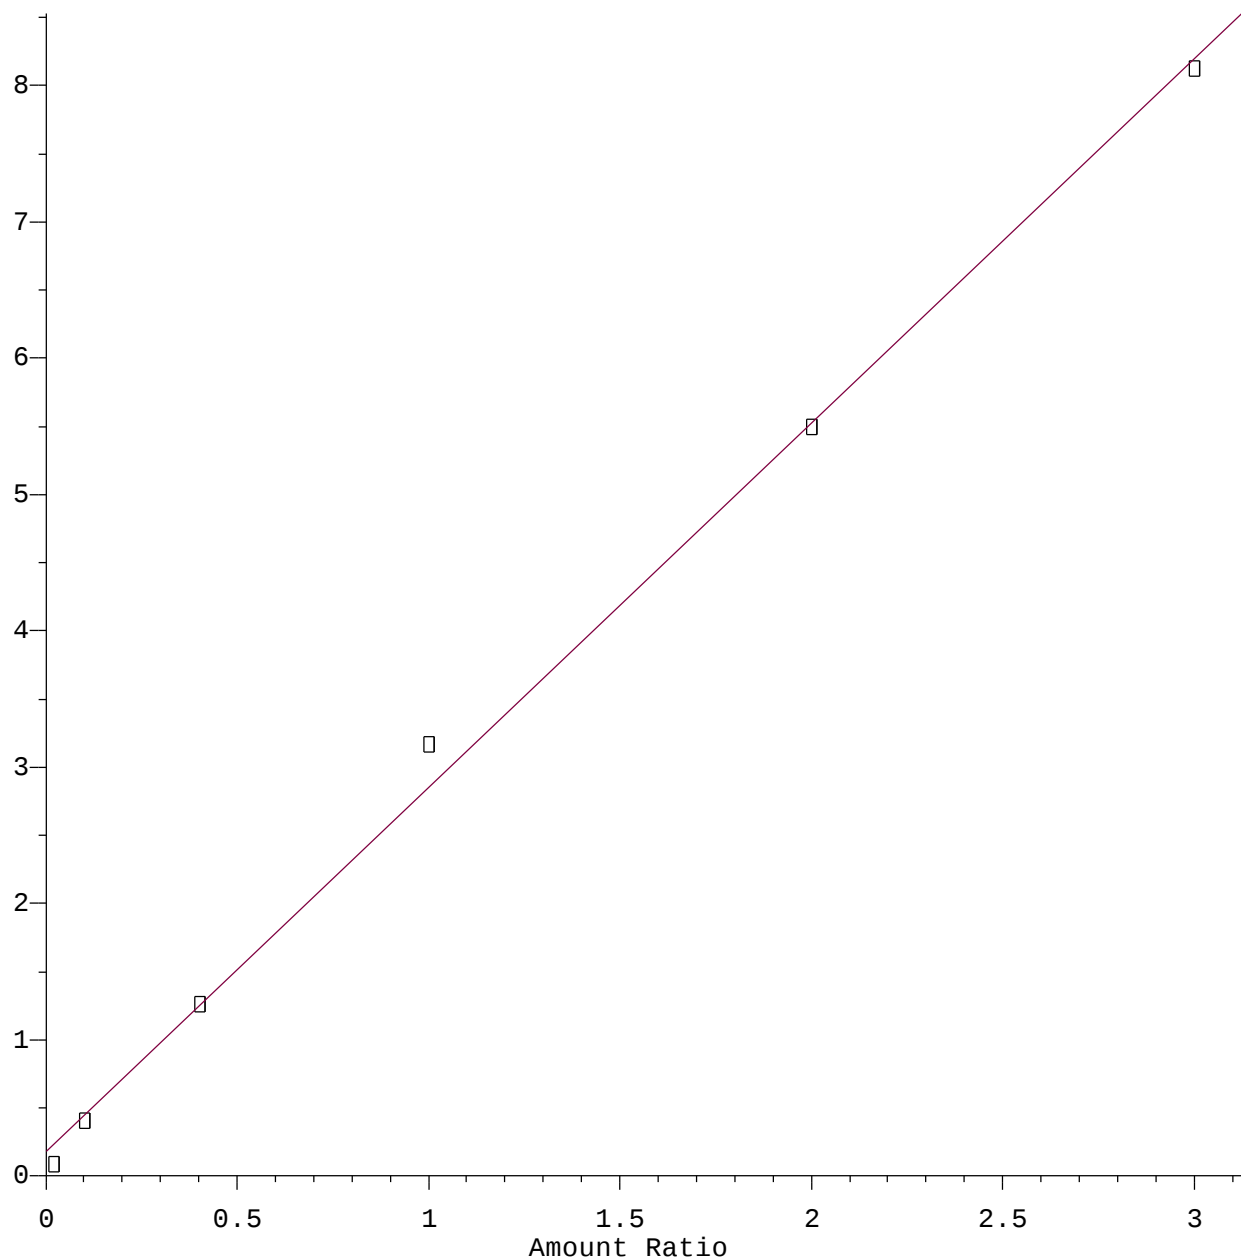

Resp Ratio = 2.67e+000 * Amt + 1.82e-001
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

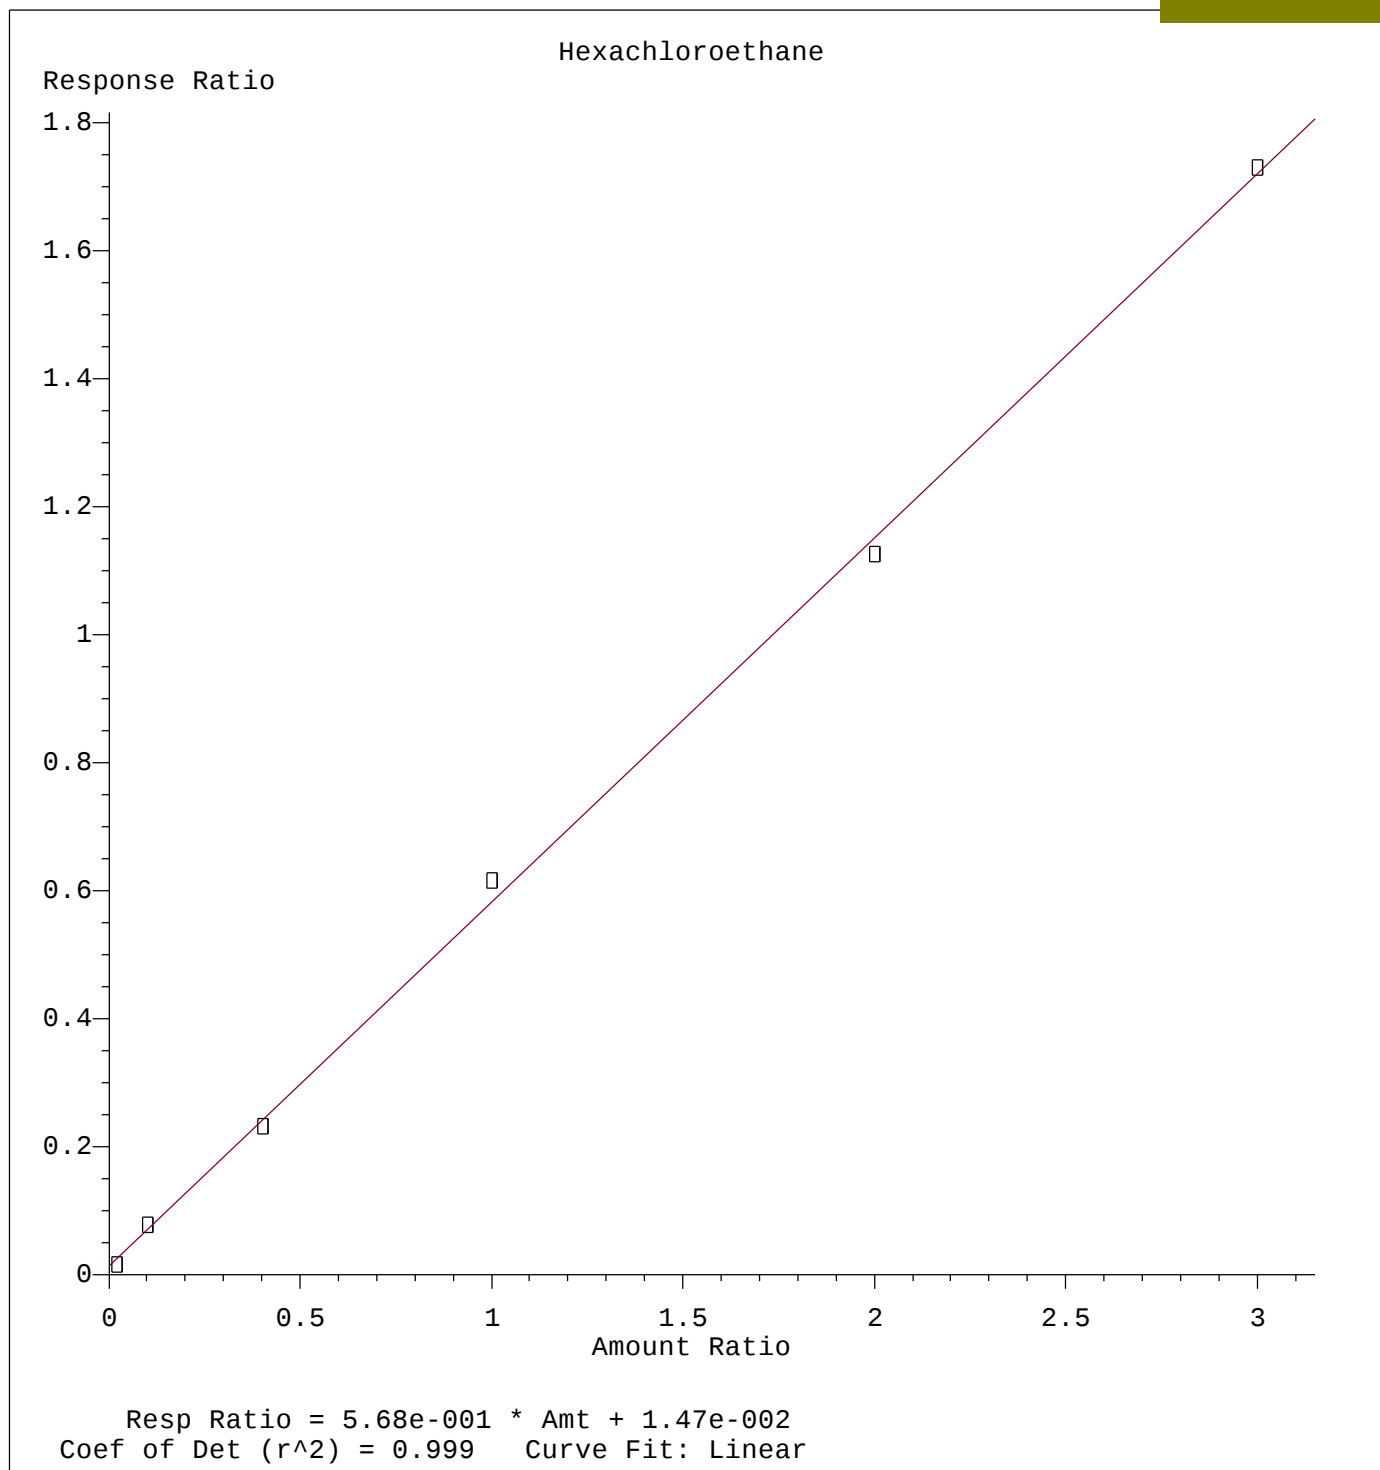


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

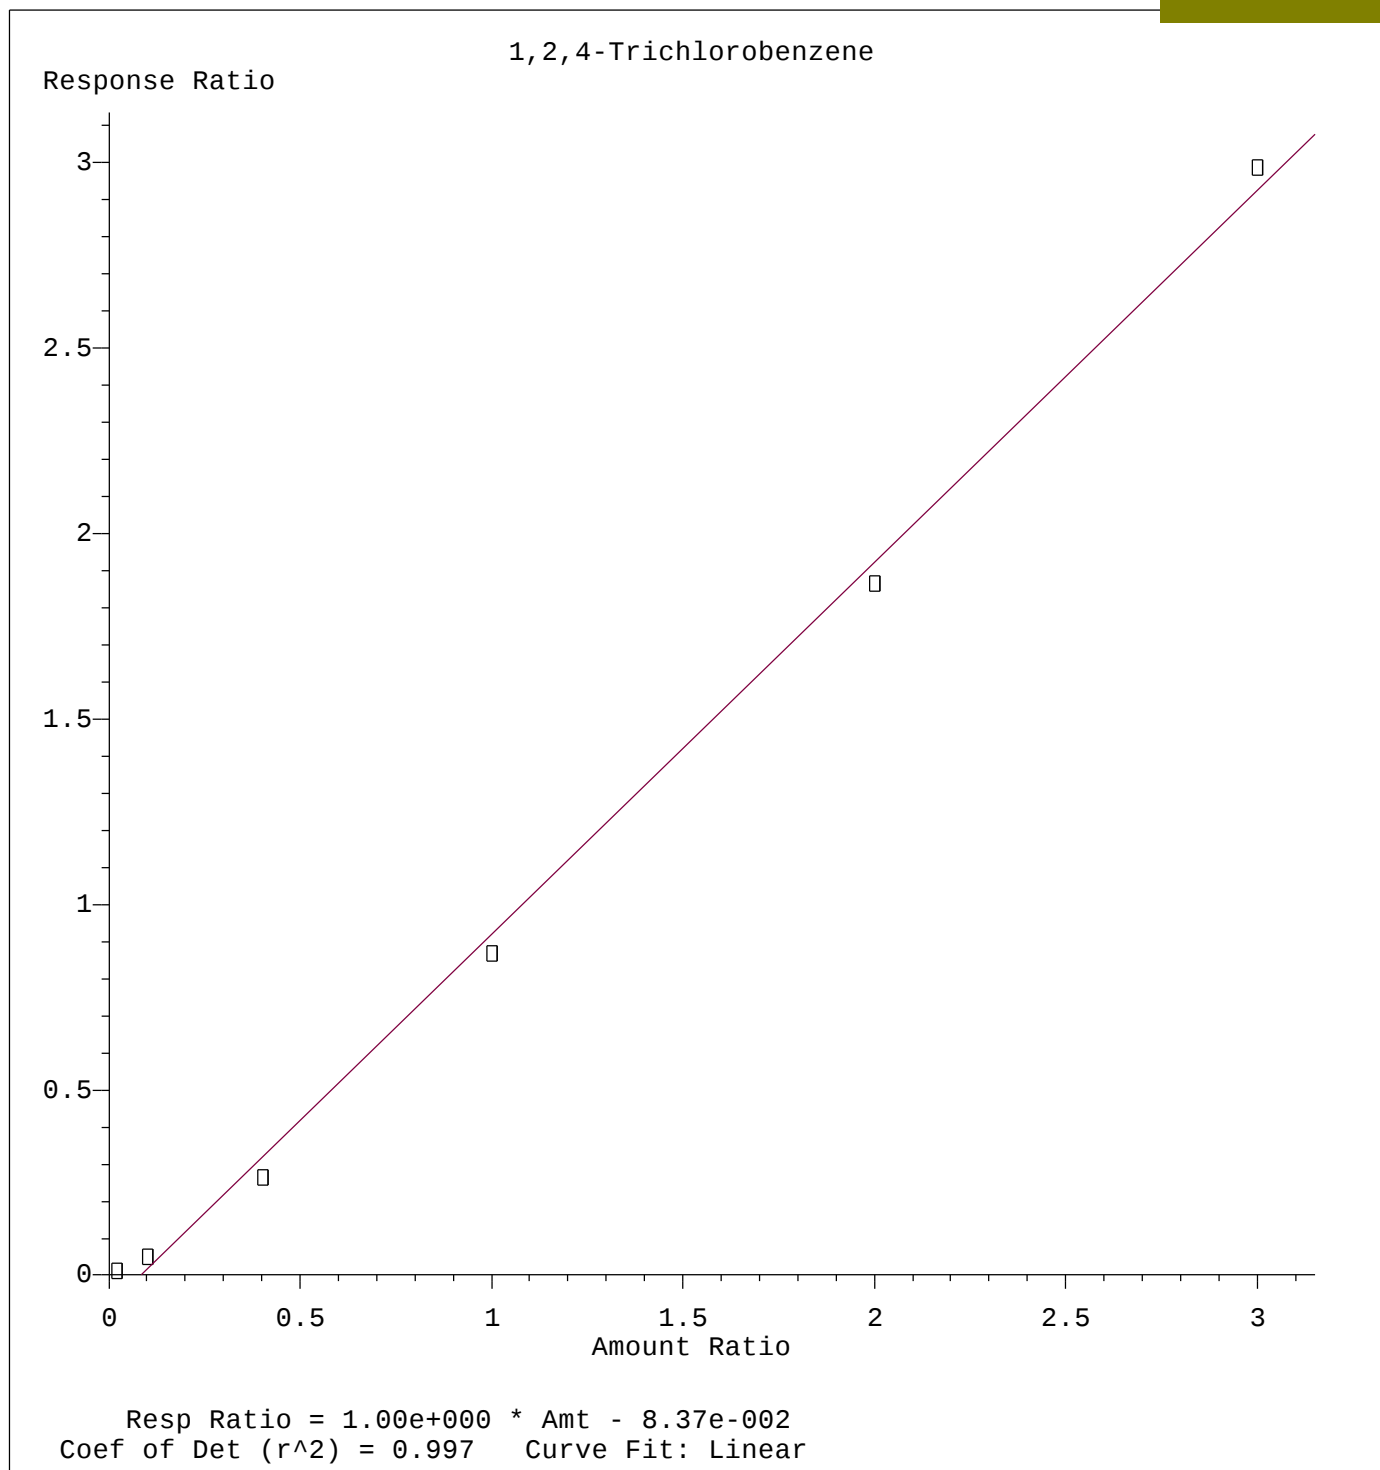

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

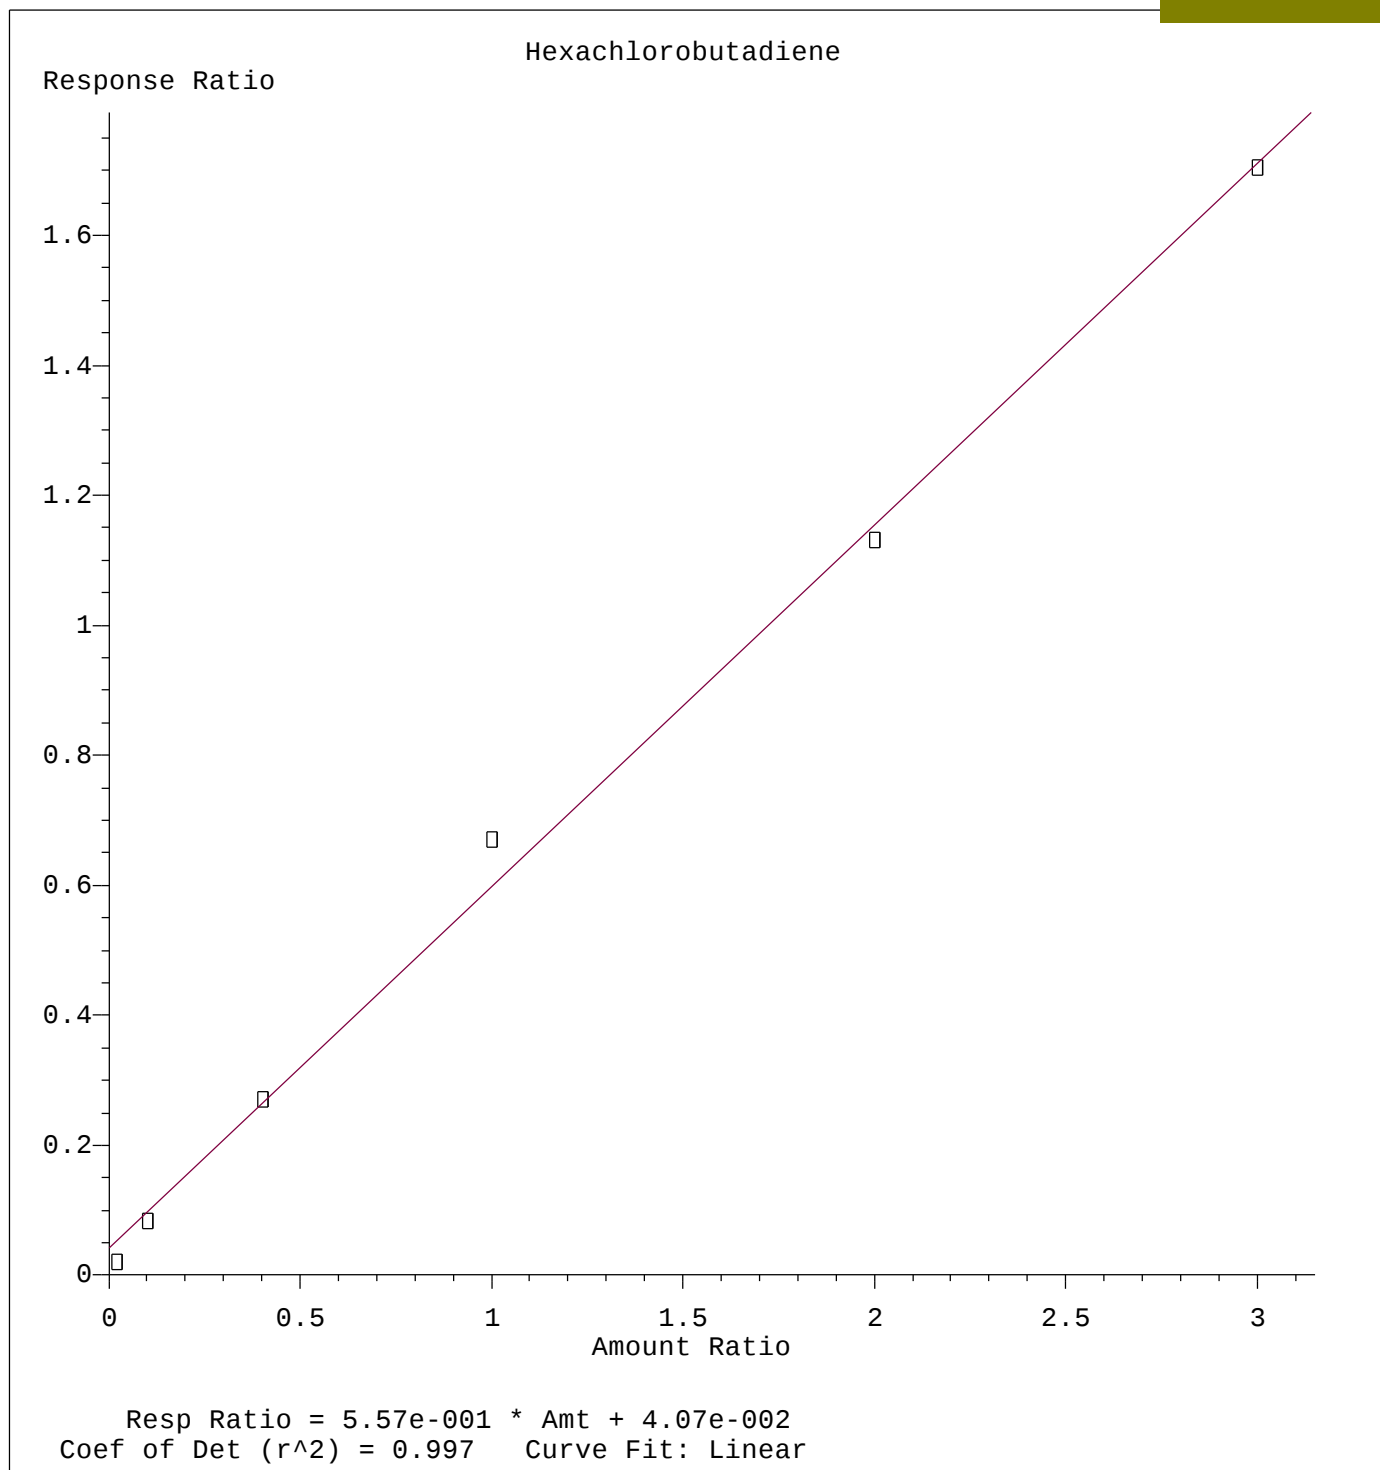


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

Naphthalene


Response Ratio

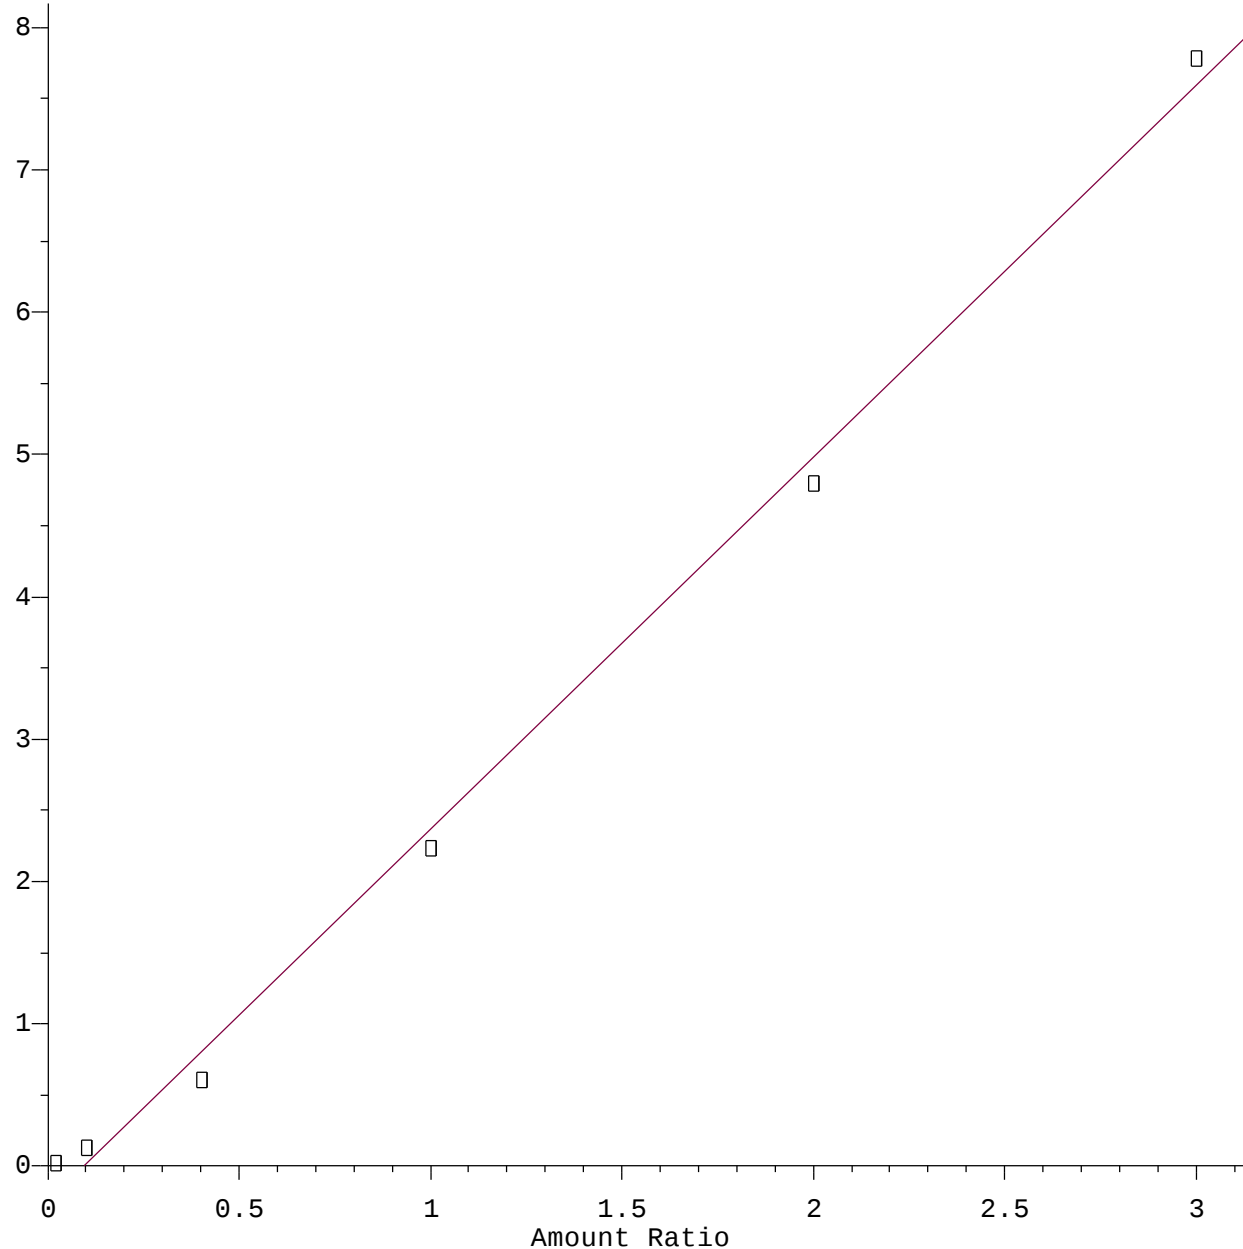

Resp Ratio = 2.61e+000 * Amt - 2.47e-001
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019

Instrument :
MSVOA_N
ClientSampleId :

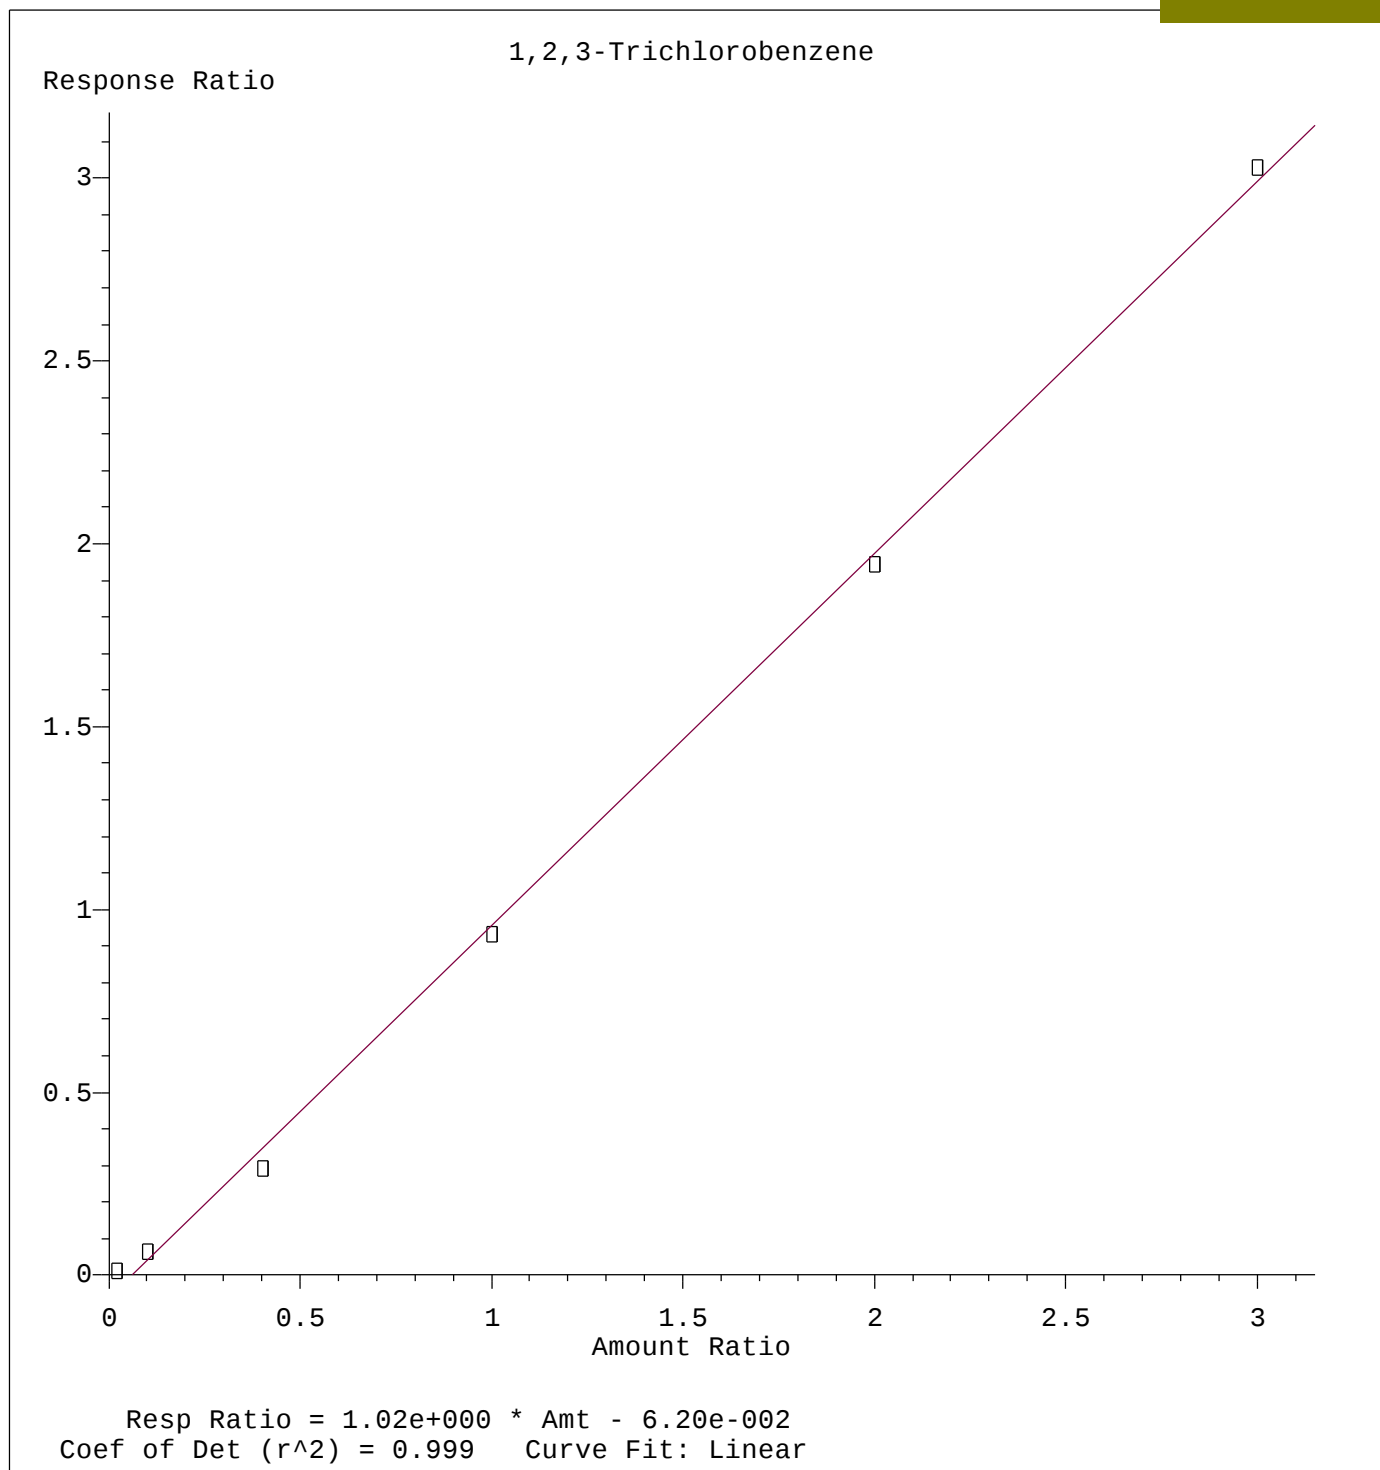

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
Calibration Table Last Updated: Tue Jul 30 15:50:01 2019