


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN072619\
 Data File : VN056919.D
 Acq On : 25 Jul 2019 13:33
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072619W.M
 Title : SW846 8260
 Last Update : Fri Jul 26 05:34:54 2019

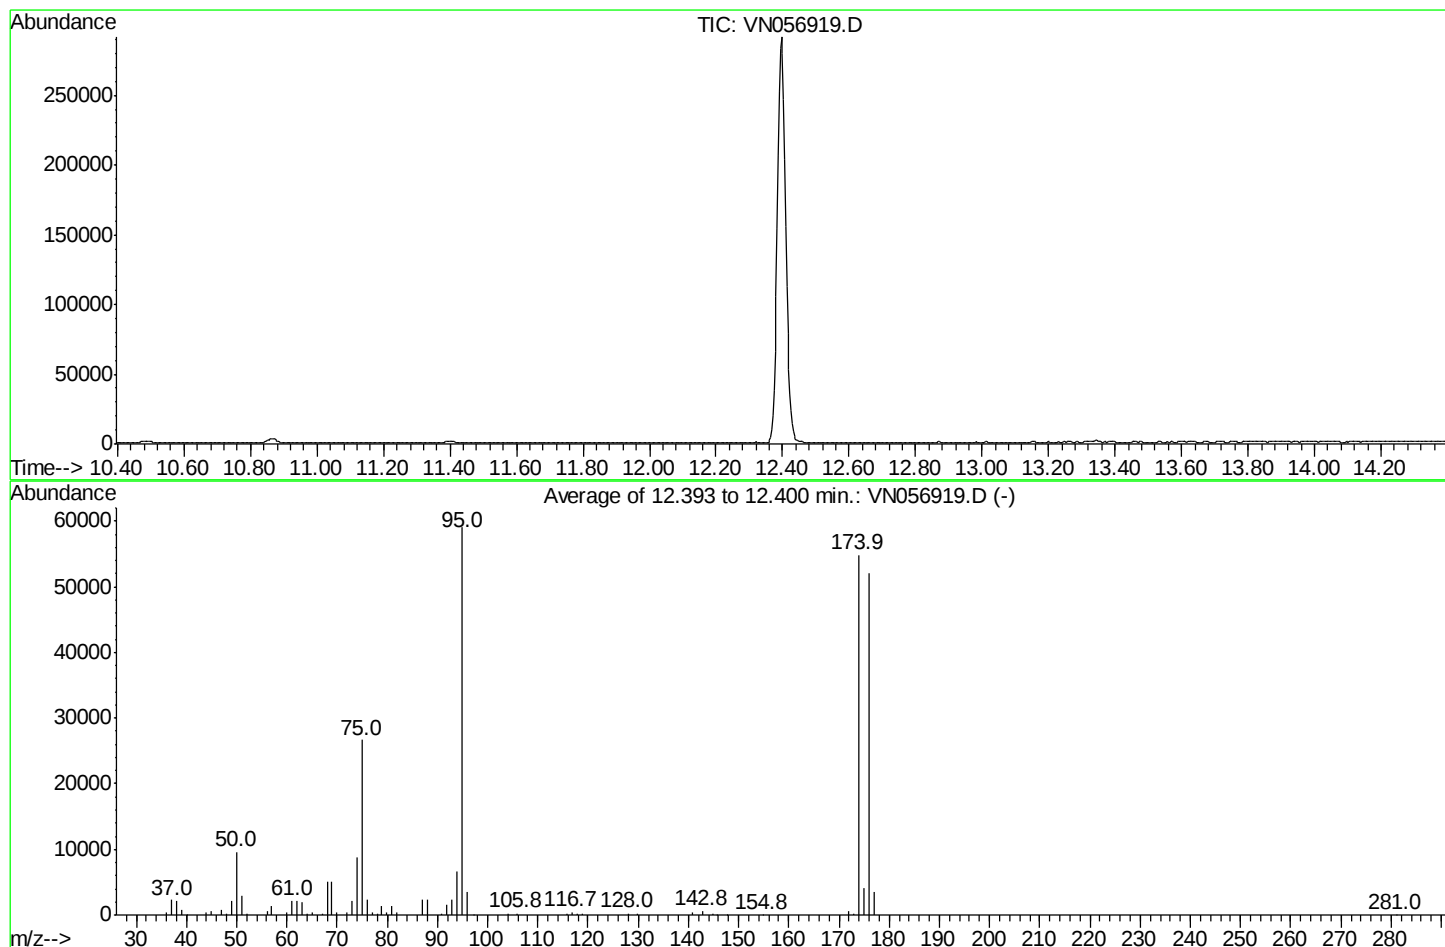

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3289

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	9633	PASS
75	95	30	60	45.1	26666	PASS
95	95	100	100	100.0	59069	PASS
96	95	5	9	5.8	3431	PASS
173	174	0.00	2	0.4	216	PASS
174	95	50	100	92.8	54834	PASS
175	174	5	9	7.4	4085	PASS
176	174	95	101	95.1	52165	PASS
177	176	5	9	6.8	3552	PASS