
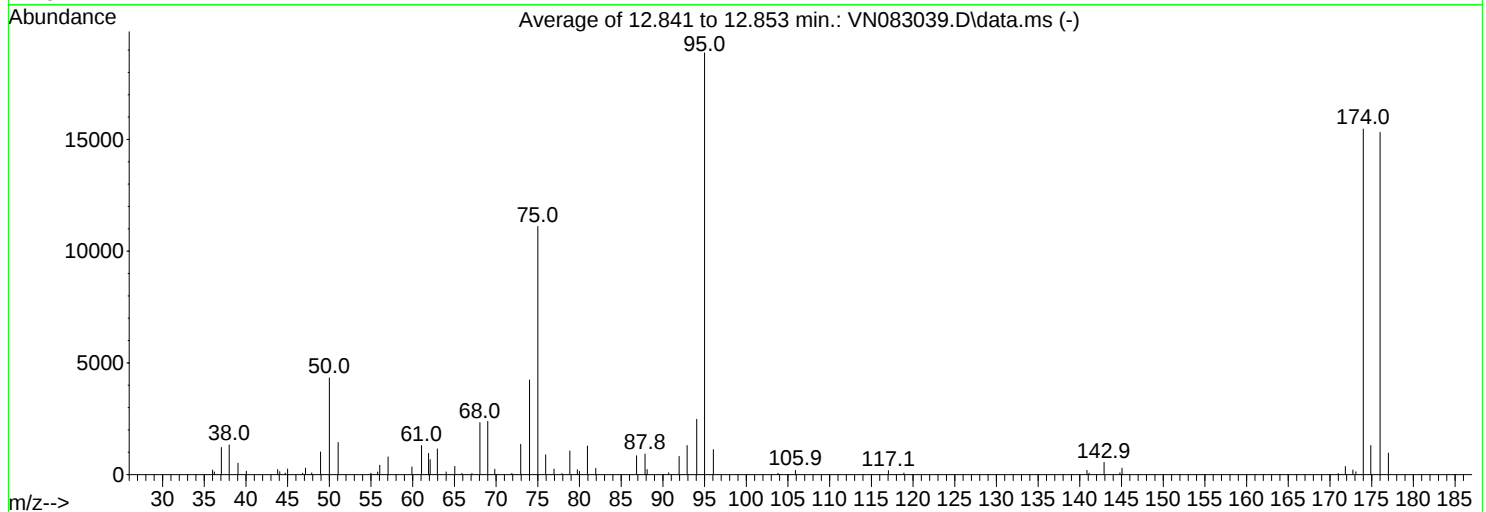


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072624\
Data File : VN083039.D
Acq On : 26 Jul 2024 09:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

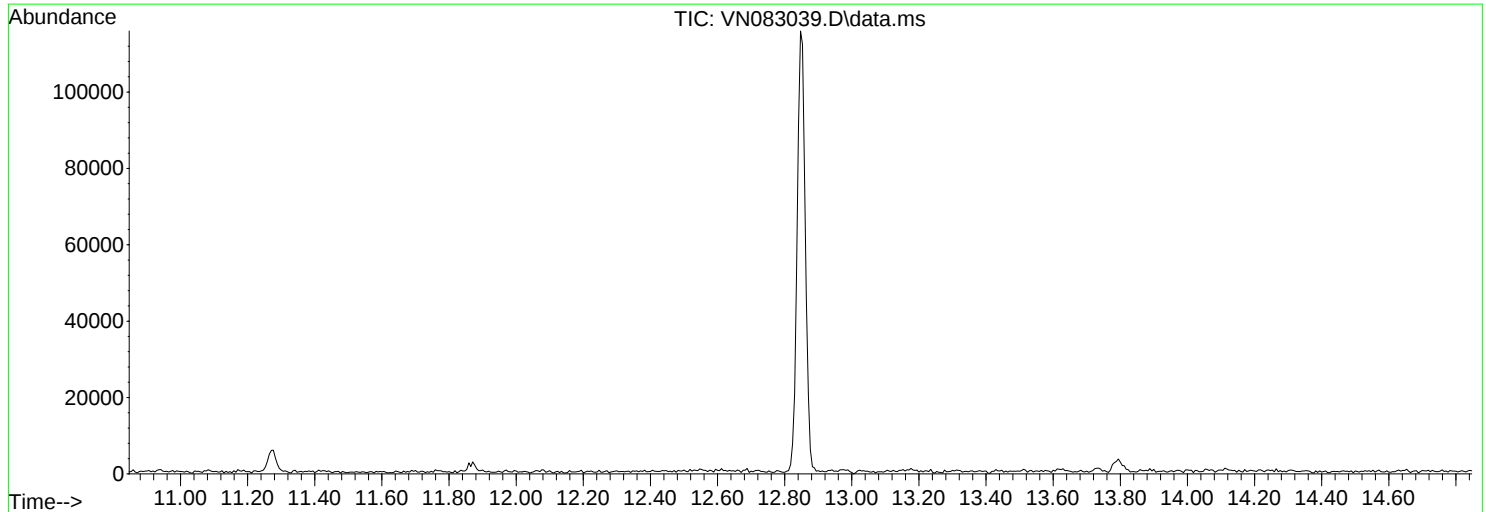

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	4334	PASS
75	95	30	60	58.8	11107	PASS
95	95	100	100	100.0	18875	PASS
96	95	5	9	5.9	1119	PASS
173	174	0.00	2	1.4	209	PASS
174	95	50	100	81.9	15463	PASS
175	174	5	9	8.4	1302	PASS
176	174	95	101	99.1	15317	PASS
177	176	5	9	6.3	967	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	211	47.15	296	61.90	951	72.95	1361
36.20	125	47.90	79	62.10	675	74.00	4241
37.05	1218	48.95	1019	62.95	1156	75.00	1110
38.00	1335	50.00	4334	64.00	122	75.95	88
39.05	515	51.05	1436	65.05	371	76.95	252
40.05	158	55.00	66	65.90	60	77.90	51
43.80	230	55.80	118	67.10	53	78.85	1059
44.05	139	56.05	425	68.05	2326	79.75	223
44.70	75	57.05	797	69.00	2385	80.00	150
45.00	248	59.90	344	69.85	241	80.95	1284
46.80	64	61.05	1303	71.90	59	81.95	277

Average of 12.841 to 12.853 min.: VN083039.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.85	848	117.05	181	174.00	15463		
87.85	922	118.90	72	174.90	1302		
88.10	231	140.85	197	176.00	15317		
90.70	84	141.10	62	177.00	967		
91.95	814	142.90	548				
92.90	1306	144.80	77				
94.05	2481	145.05	292				
95.00	18875	171.00	51				
96.05	1119	171.85	362				
103.80	67	172.75	209				
105.90	195	173.10	129				

Instrument :

MSVOA_N

ClientSampleId :

BFB