

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN072718\
 Data File : VN050144.D
 Acq On : 27 Jul 2018 21:12
 Operator : MD\SY
 Sample : PB111513ZHE#04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB111513ZHE#04

Quant Time: Jul 28 01:03:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 26 18:10:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	709333	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1161311	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	966766	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	330096	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	487244	49.23	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.46%	
35) Dibromofluoromethane	7.59	113	429349	45.28	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.56%	
50) Toluene-d8	10.09	98	1553248	44.56	ug/l	0.00
Spiked Amount 50.000			Recovery	=	89.12%	
62) 4-Bromofluorobenzene	12.41	95	429632	37.43	ug/l	0.00
Spiked Amount 50.000			Recovery	=	74.86%	
Target Compounds						
16) Acetone	3.82	43	102602	40.372	ug/l	98
18) Methyl Acetate	4.34	43	34178	2.212	ug/l	99
20) Methylene Chloride	4.55	84	173887	19.040	ug/l	100
43) Isopropyl Acetate	8.17	43	551888	31.687	ug/l #	83
59) 2-Hexanone	10.77	43	25321	8.937	ug/l #	55
95) Naphthalene	15.14	128	4811	4.706	ug/l #	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN072718\
Data File : VN050144.D
Acq On : 27 Jul 2018 21:12
Operator : MD\SY
Sample : PB111513ZHE#04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB111513ZHE#04

Quant Time: Jul 28 01:03:51 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 26 18:10:10 2018
Response via : Initial Calibration

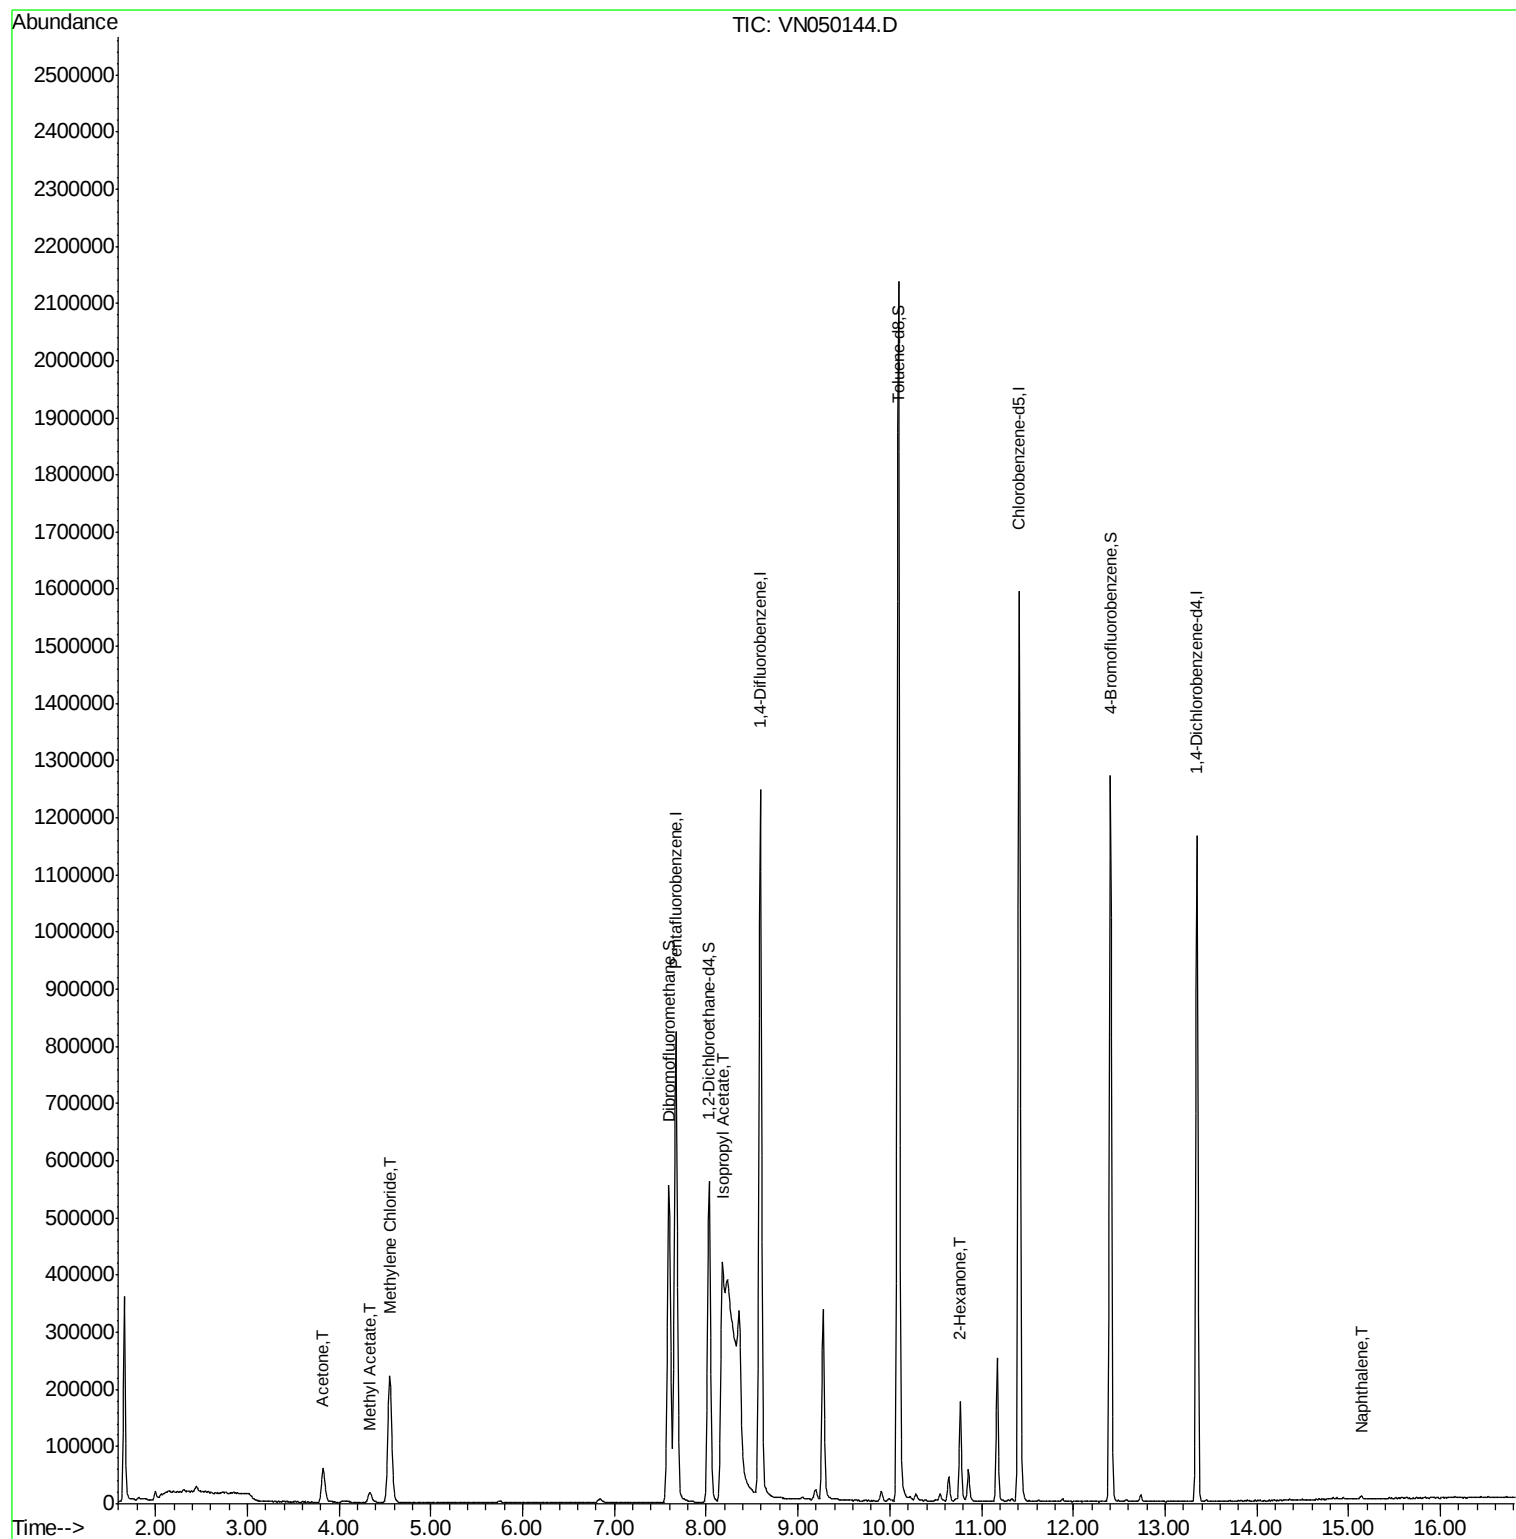



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. -0.00 min

Lab File: VN050144.D

Acq: 27 Jul 2018 21:12

Instrument :

MSVOA_N

ClientSampleId :


PB111513ZHE#04

Tot Ion:168 Resp: 709333

Ion Ratio Lower Upper

168 100

99 51.2 40.0 60.0

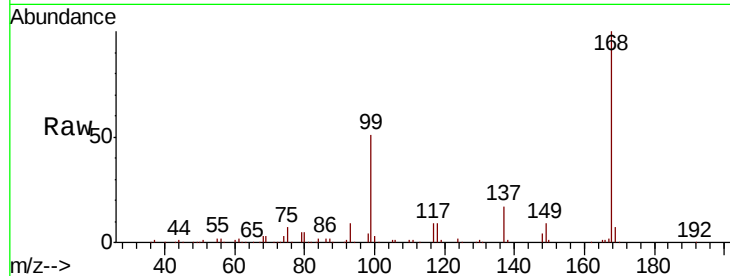

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

7.67



300000

200000

100000

0

Time-->

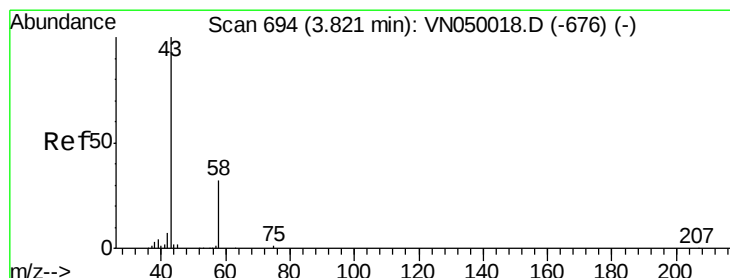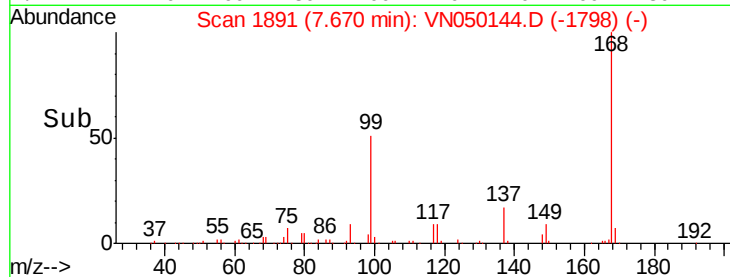

#16

Acetone

Concen: 40.372 ug/l

RT: 3.82 min Scan# 695

Delta R.T. 0.00 min

Lab File: VN050144.D


Acq: 27 Jul 2018 21:12

Tgt Ion: 43 Resp: 102602

Ion Ratio Lower Upper

43 100

58 31.4 25.8 38.8

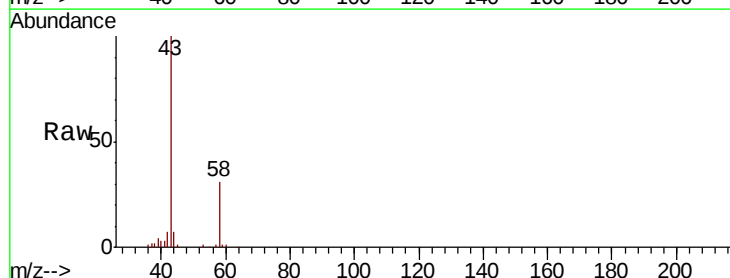

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

3.82

40000


30000


20000

10000

0

Time-->




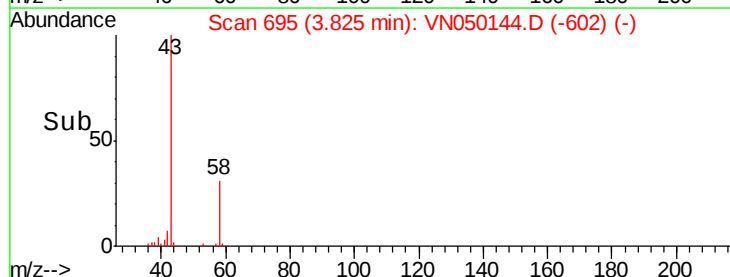


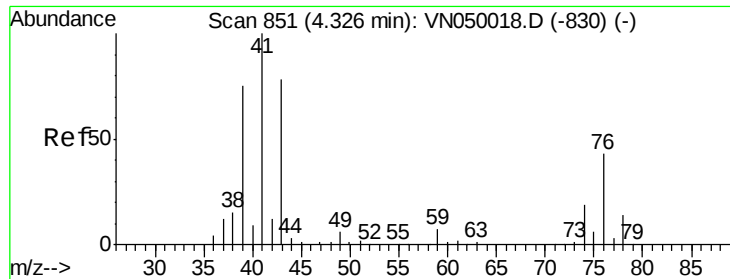

#18
Methyl Acetate
Concen: 2.212 ug/l
RT: 4.34 min Scan# 854
Delta R.T. 0.00 min
Lab File: VN050144.D
Acq: 27 Jul 2018 21:12




Instrument :
MSVOA_N
ClientSampleId :
PB111513ZHE#04


Tot Ion: 43 Resp: 34178
Ion Ratio Lower Upper
43 100
74 23.6 19.2 28.8

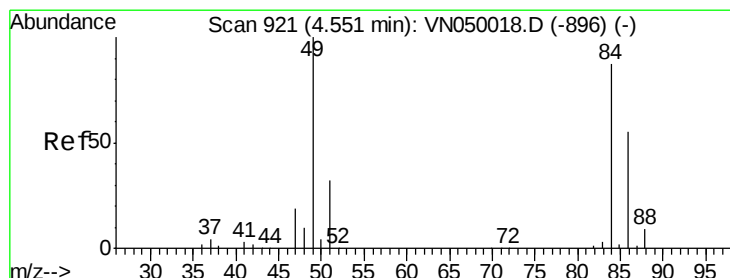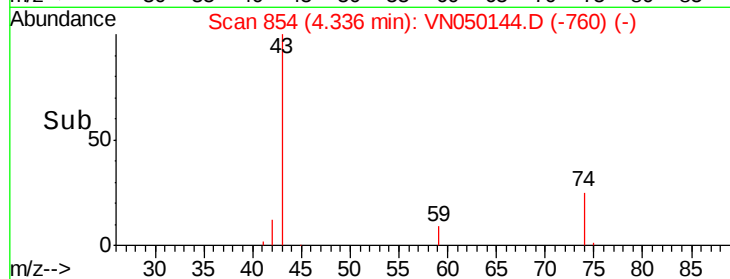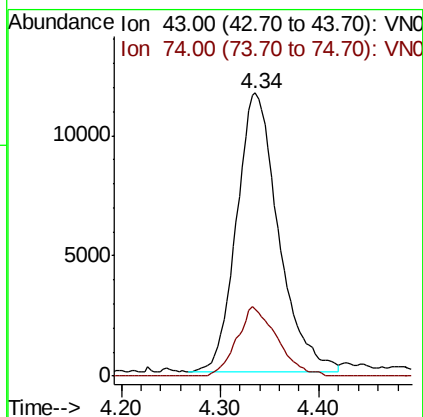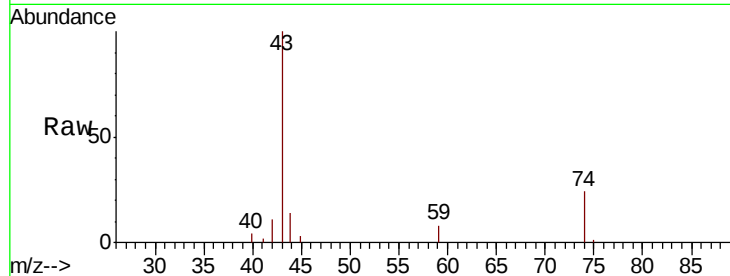

#20
Methylene Chloride
Concen: 19.040 ug/l
RT: 4.55 min Scan# 921
Delta R.T. 0.00 min
Lab File: VN050144.D
Acq: 27 Jul 2018 21:12

Tgt Ion: 84 Resp: 173887
Ion Ratio Lower Upper
84 100
49 118.9 94.8 142.2
51 35.3 28.3 42.5
86 63.6 51.0 76.6


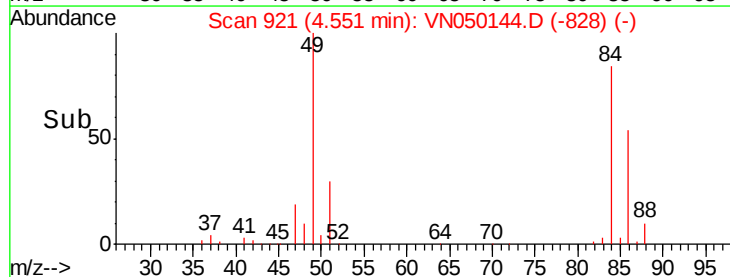
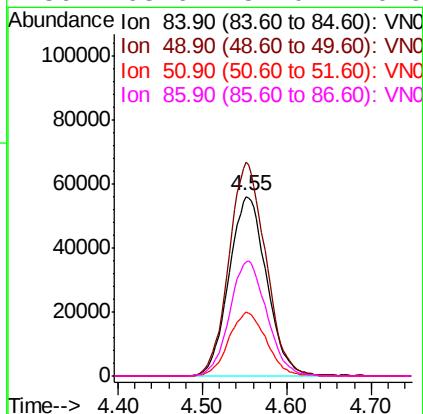
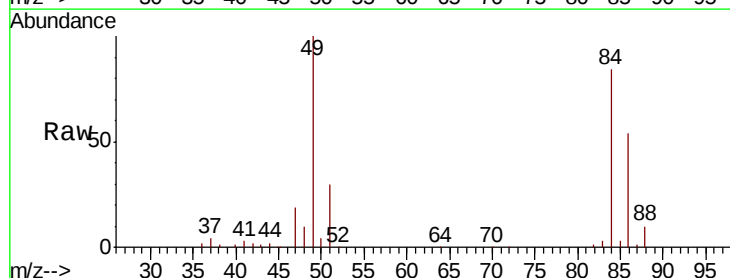


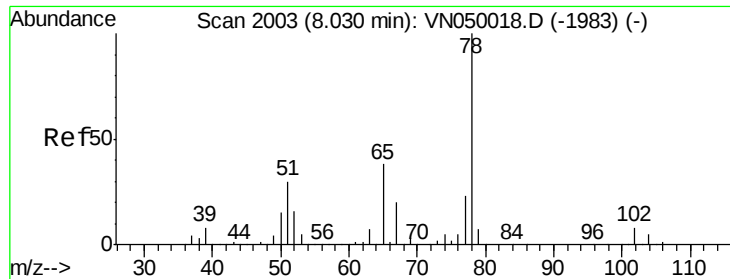

#33
 1,2-Dichloroethane-d4
 Concen: 49.232 ug/l
 RT: 8.03 min Scan# 2004
 Delta R.T. 0.00 min
 Lab File: VN050144.D
 Acq: 27 Jul 2018 21:12




Instrument :
 MSVOA_N
 ClientSampleId :
 PB111513ZHE#04

Tot Ion: 65 Resp: 487244
 Ion Ratio Lower Upper
 65 100
 67 52.7 0.0 108.4

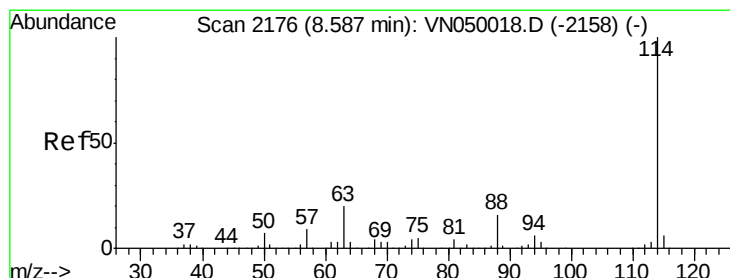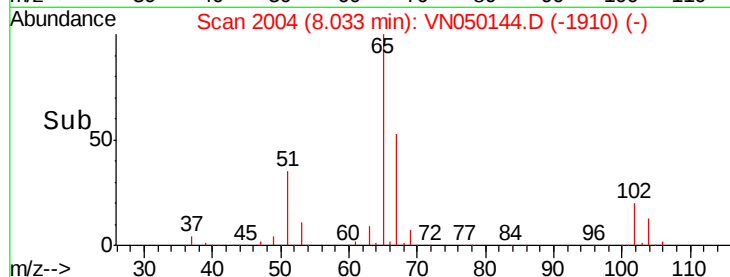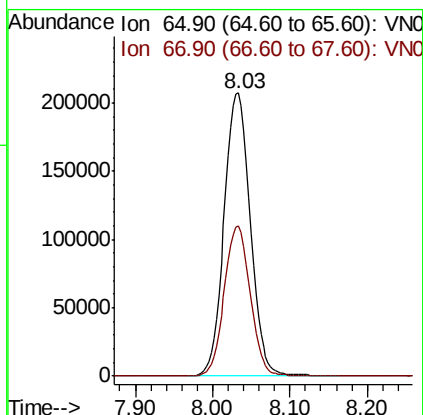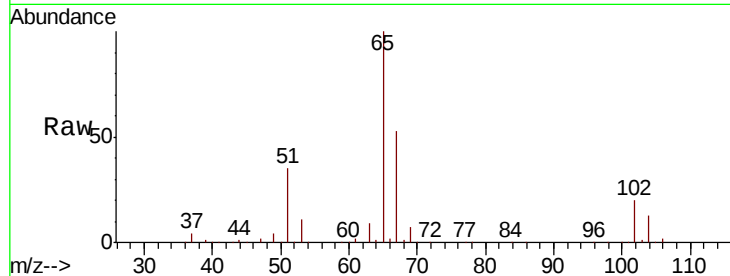

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2177
 Delta R.T. -0.00 min
 Lab File: VN050144.D
 Acq: 27 Jul 2018 21:12

Tgt Ion: 114 Resp: 1161311
 Ion Ratio Lower Upper
 114 100
 63 19.5 0.0 40.0
 88 15.4 0.0 31.2


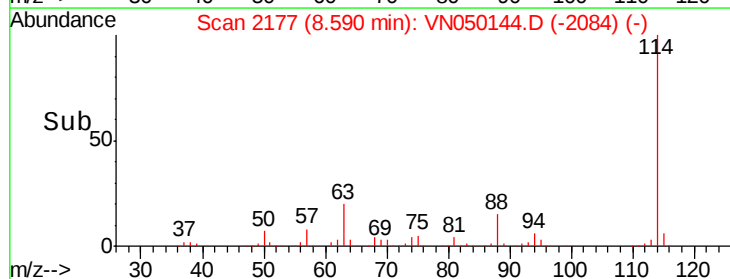
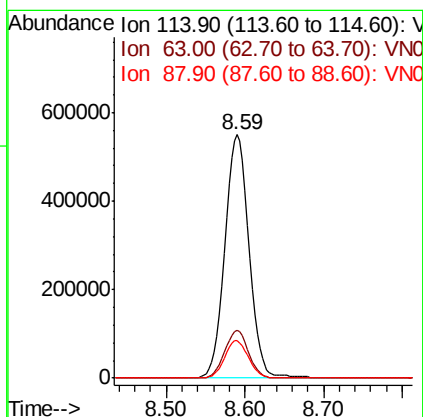
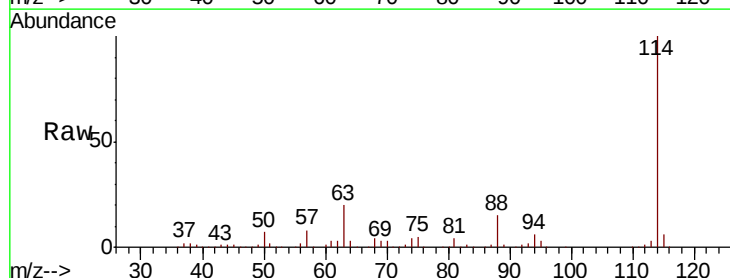




#35
 Dibromofluoromethane
 Concen: 45.281 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. -0.00 min
 Lab File: VN050144.D
 Acq: 27 Jul 2018 21:12




Instrument :
 MSVOA_N
 ClientSampleId :
 PB111513ZHE#04


Tot Ion:113 Resp: 429349
 Ion Ratio Lower Upper
 113 100
 111 102.4 80.7 121.1
 192 22.4 17.8 26.6

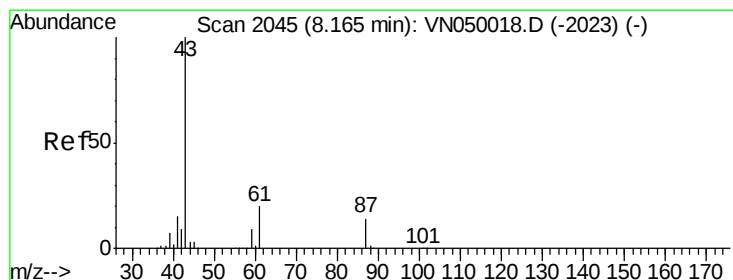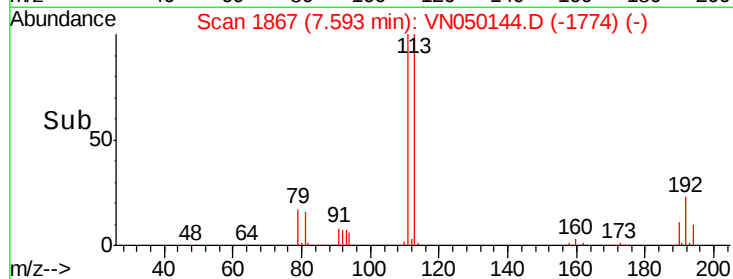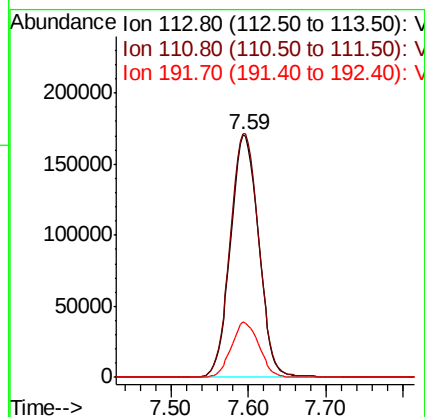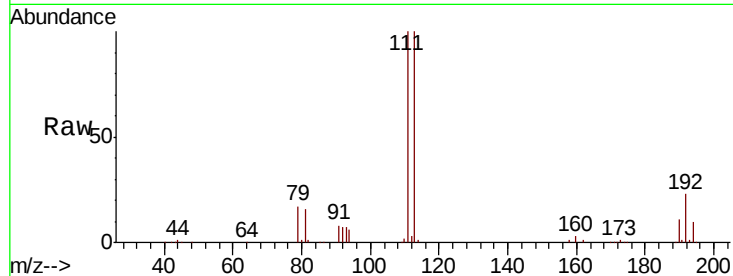

#43
 Isopropyl Acetate
 Concen: 31.687 ug/l
 RT: 8.17 min Scan# 2048
 Delta R.T. 0.01 min
 Lab File: VN050144.D
 Acq: 27 Jul 2018 21:12

Tgt Ion: 43 Resp: 551888
 Ion Ratio Lower Upper
 43 100
 61 11.5 15.8 23.6#
 87 7.2 10.3 15.5#

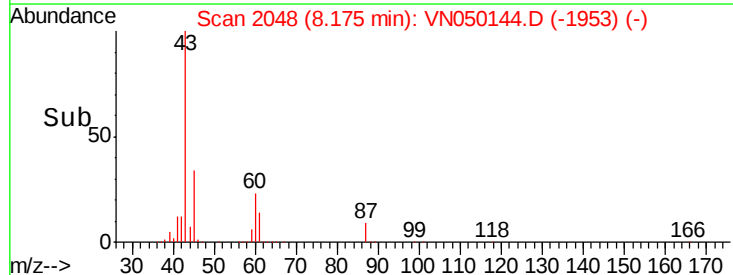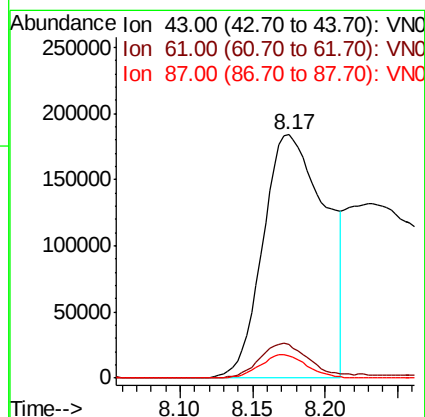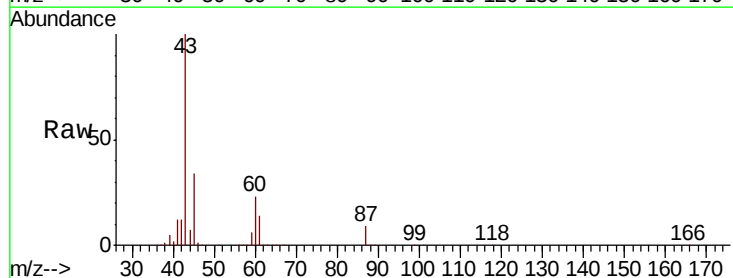

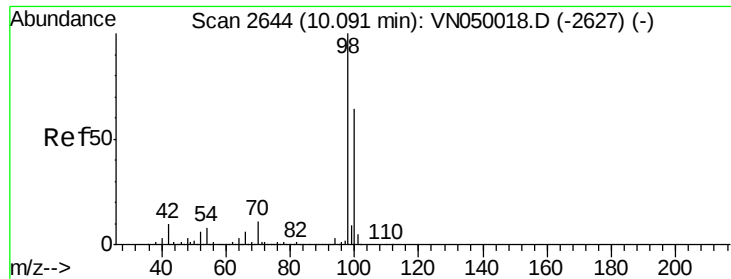

#50

Toluene-d8

Concen: 44.558 ug/l

RT: 10.09 min Scan# 2645

Delta R.T. 0.00 min

Lab File: VN050144.D

Acq: 27 Jul 2018 21:12

Instrument :

MSVOA_N

ClientSampleId :





PB111513ZHE#04

Tot Ion: 98 Resp: 1553248

Ion Ratio Lower Upper

98 100

100 63.9 50.7 76.1

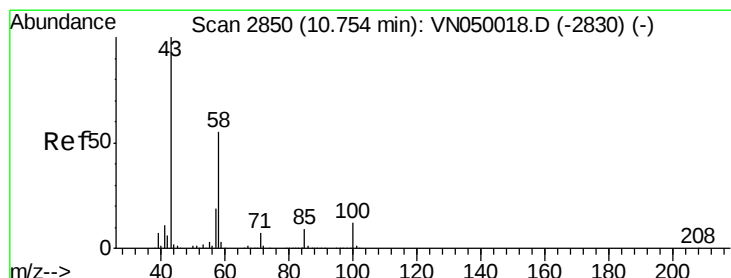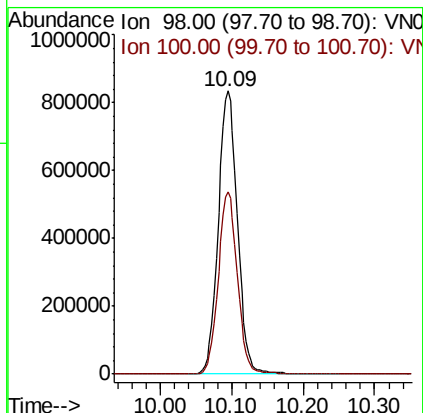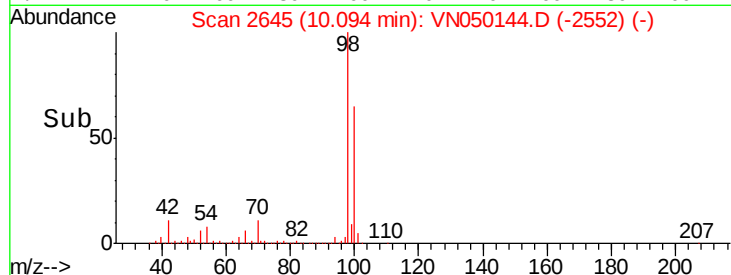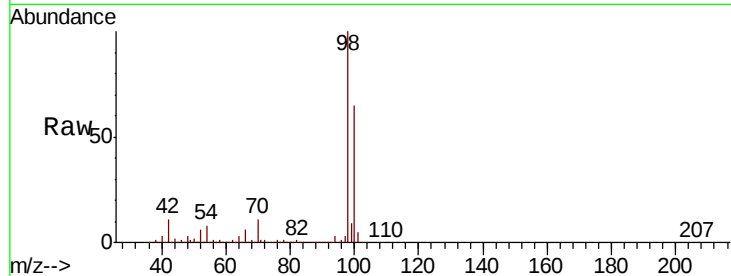

#59

2-Hexanone

Concen: 8.937 ug/l

RT: 10.77 min Scan# 2854

Delta R.T. 0.01 min

Lab File: VN050144.D




Acq: 27 Jul 2018 21:12

Tgt Ion: 43 Resp: 25321

Ion Ratio Lower Upper

43 100

58 22.2 27.6 82.7#

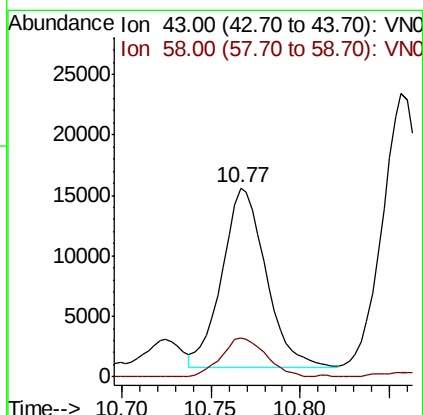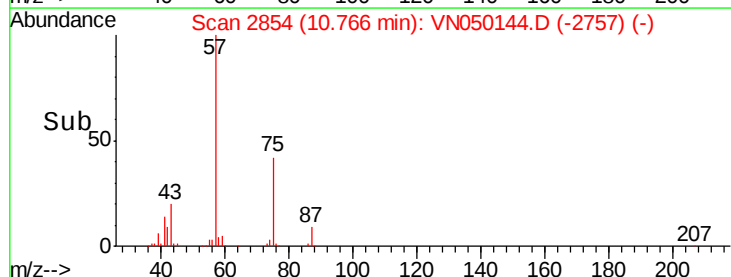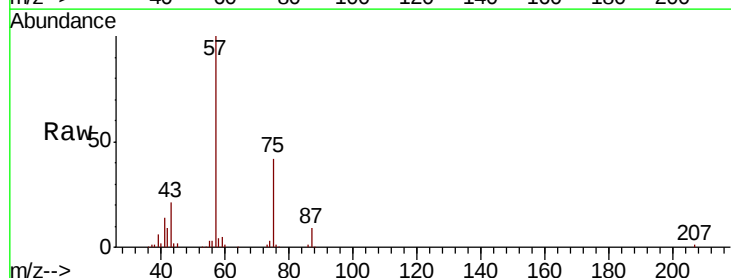



#62

4-Bromofluorobenzene

Concen: 37.430 ug/l

RT: 12.41 min Scan# 3364

Delta R.T. 0.00 min

Lab File: VN050144.D

Acq: 27 Jul 2018 21:12

Instrument :

MSVOA_N

ClientSampleId :

PB111513ZHE#04


Tot Ion: 95 Resp: 429632

Ion Ratio Lower Upper

95 100

174 90.3 0.0 178.2




176 87.2 0.0 173.4

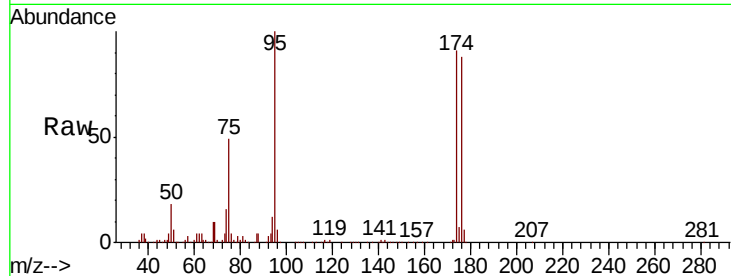

Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): VN0

Ion 175.80 (175.50 to 176.50): VN0

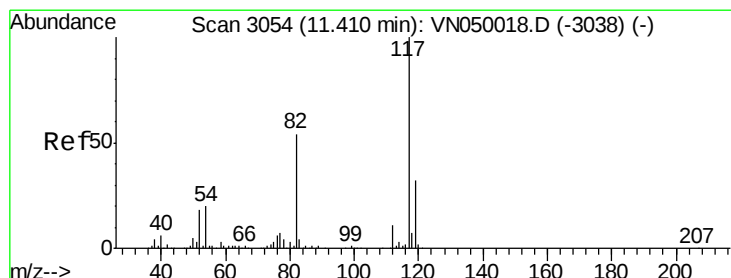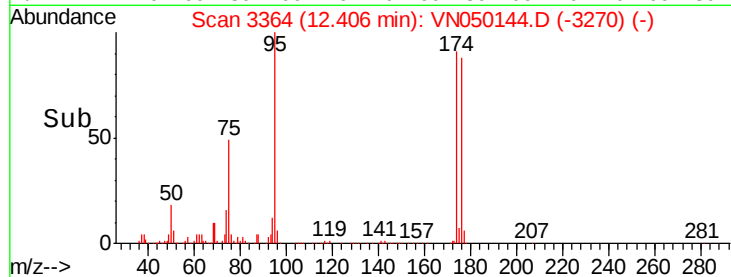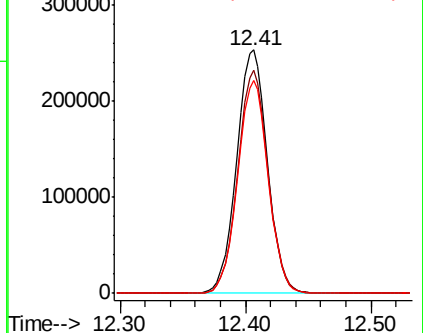

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 3054

Delta R.T. -0.00 min

Lab File: VN050144.D

Acq: 27 Jul 2018 21:12


Tgt Ion: 117 Resp: 966766

Ion Ratio Lower Upper

117 100

82 54.7 43.7 65.5



119 32.6 26.1 39.1

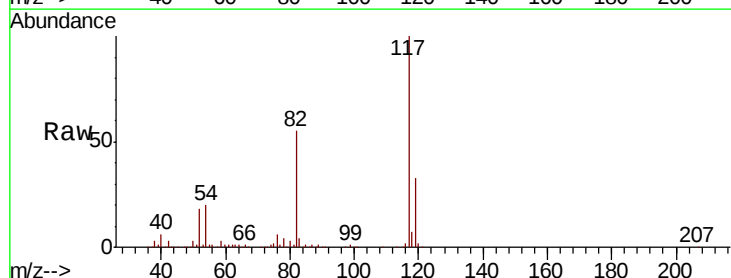


Abundance Ion 116.90 (116.60 to 117.60): VN0

Ion 82.00 (81.70 to 82.70): VN0

Ion 118.90 (118.60 to 119.60): VN0

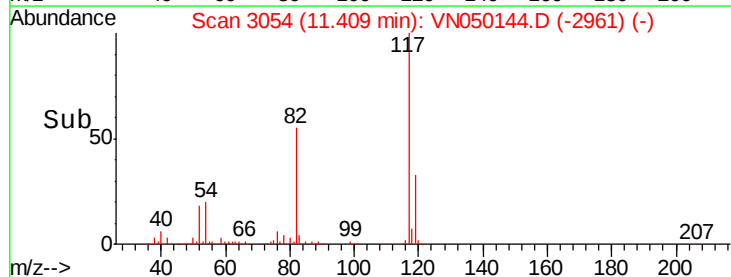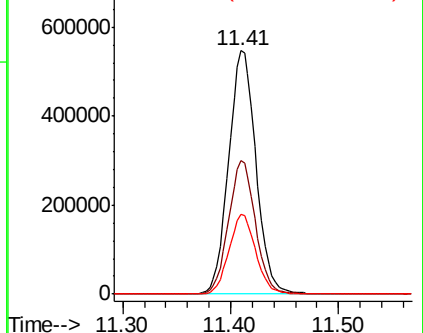

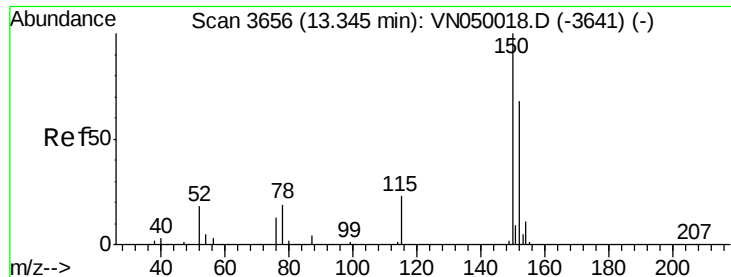

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3657

Delta R.T. 0.00 min

Lab File: VN050144.D

Acq: 27 Jul 2018 21:12

Instrument :

MSVOA_N

ClientSampleId :

PB111513ZHE#04


Tot Ion:152 Resp: 330096

Ion Ratio Lower Upper

152 100

115 56.3 27.8 83.3




150 159.1 0.0 348.6

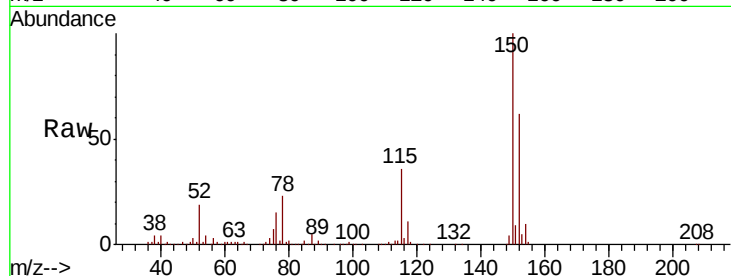

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

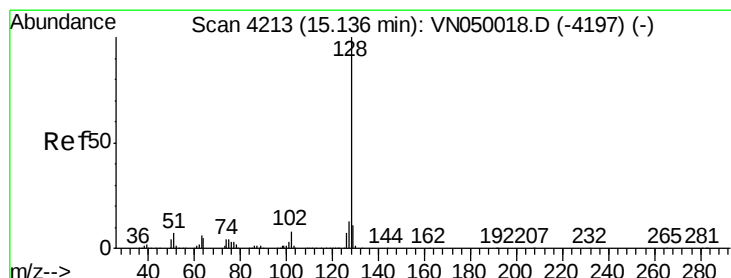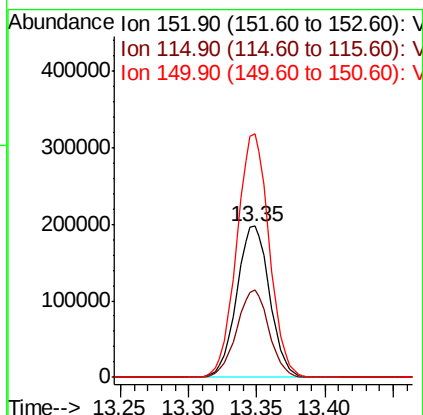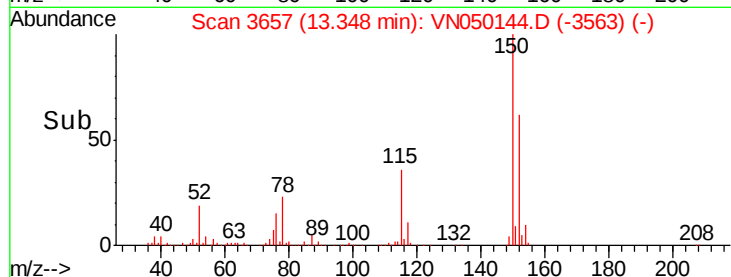

#95

Naphthalene

Concen: 4.706 ug/l

RT: 15.14 min Scan# 4213

Delta R.T. 0.00 min

Lab File: VN050144.D

Acq: 27 Jul 2018 21:12


Tgt Ion:128 Resp: 4811

Ion Ratio Lower Upper

128 100

127 10.3 10.4 15.6#

129 10.3 8.8 13.2

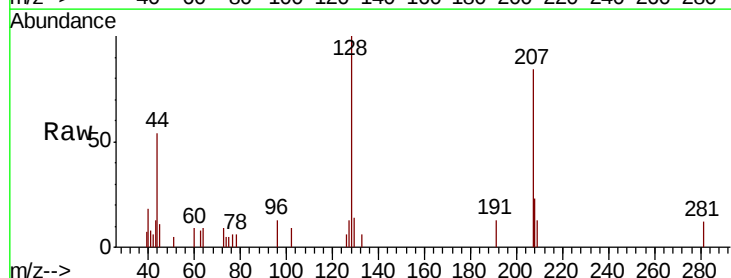

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

