



Instrument :
MSVOA_N
ClientSampleId :

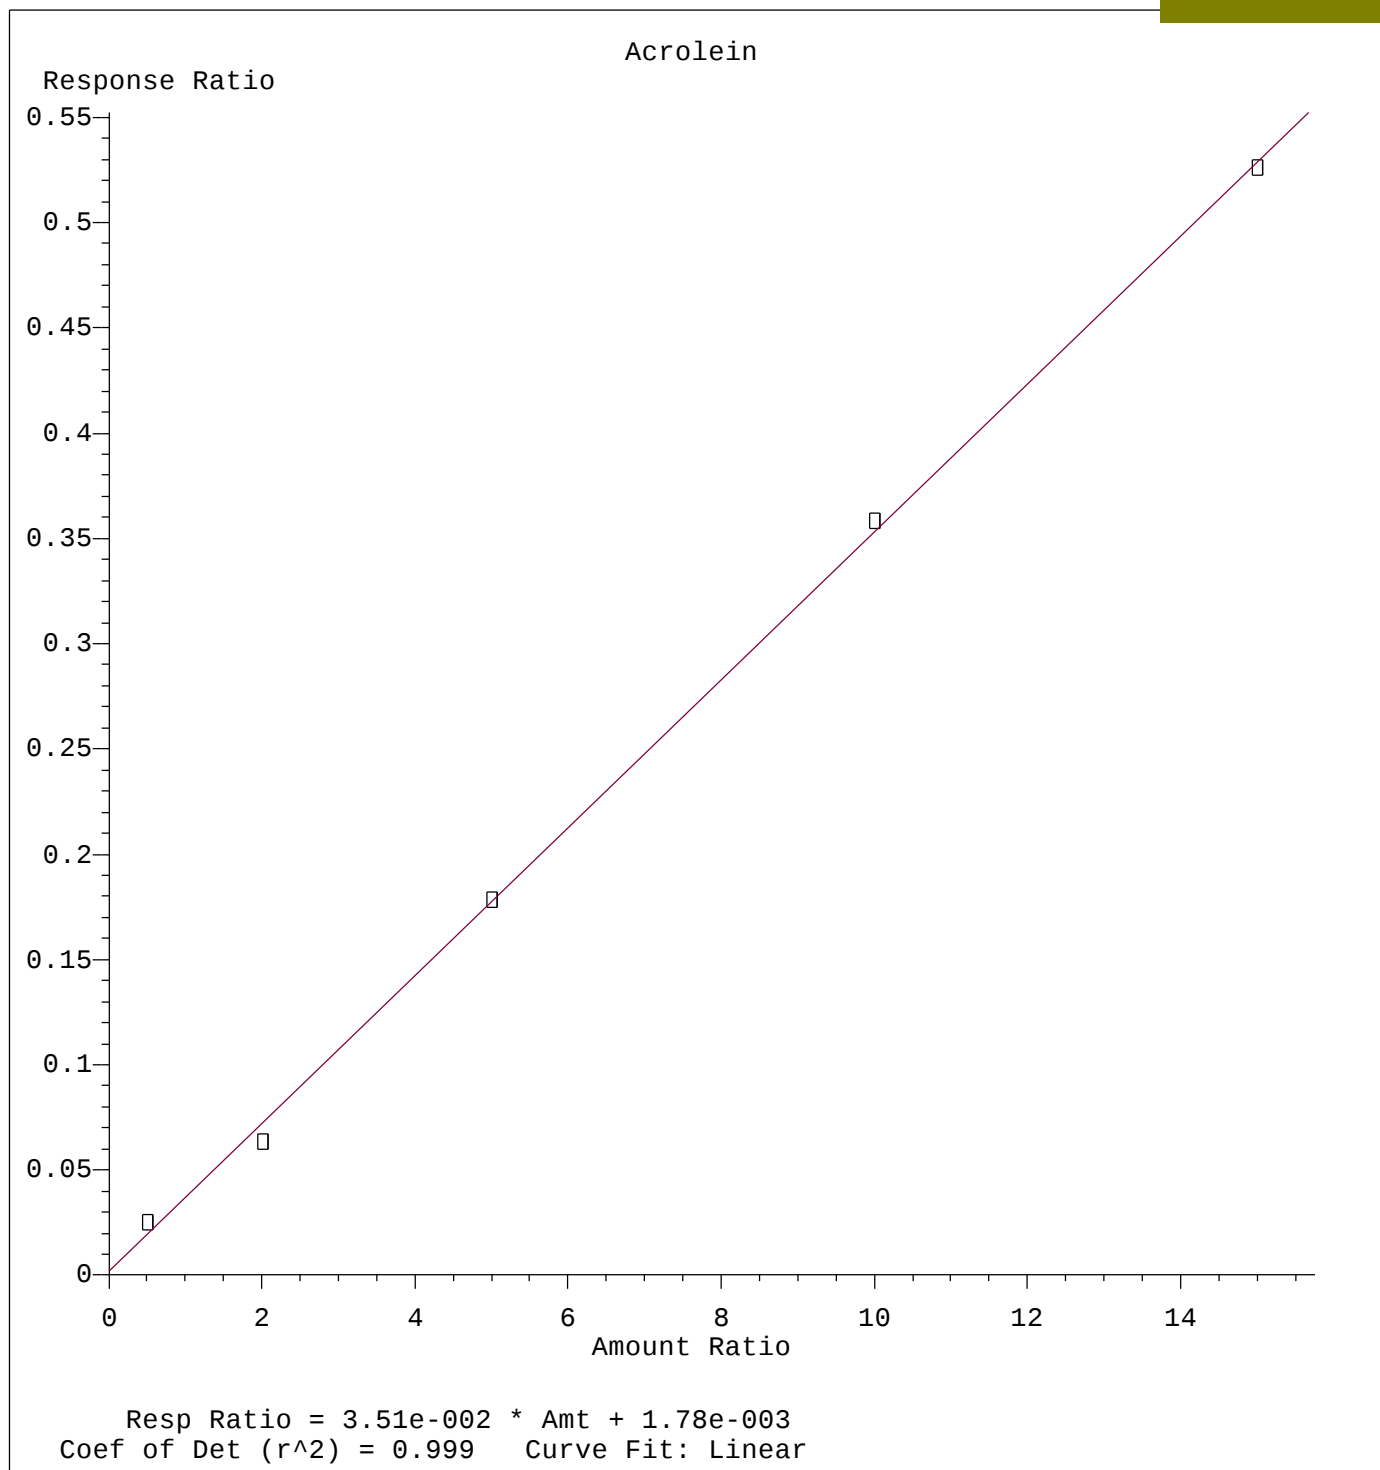

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Calibration Table Last Updated: Fri Aug 02 17:31:55 2019

Instrument :
MSVOA_N
ClientSampleId :

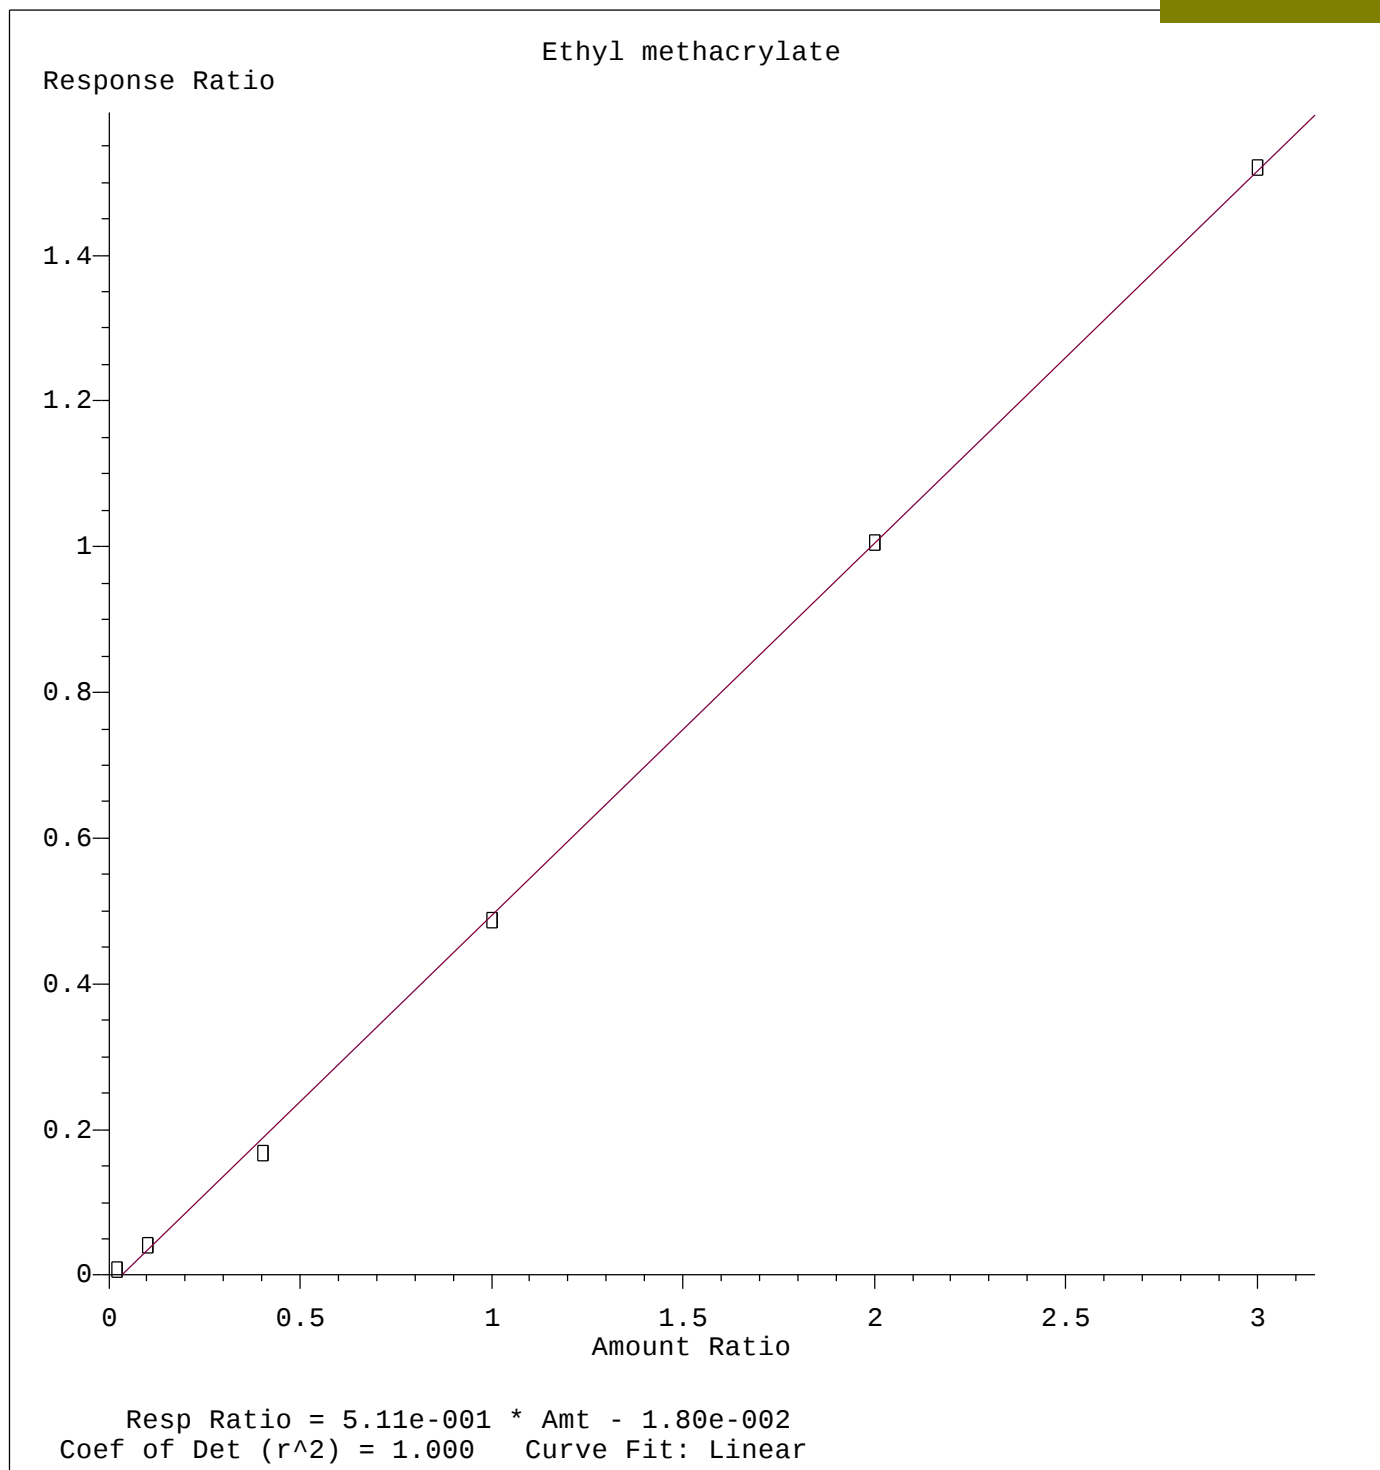


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Calibration Table Last Updated: Fri Aug 02 17:31:55 2019

Instrument :
MSVOA_N
ClientSampleId :

2-Hexanone


Response Ratio

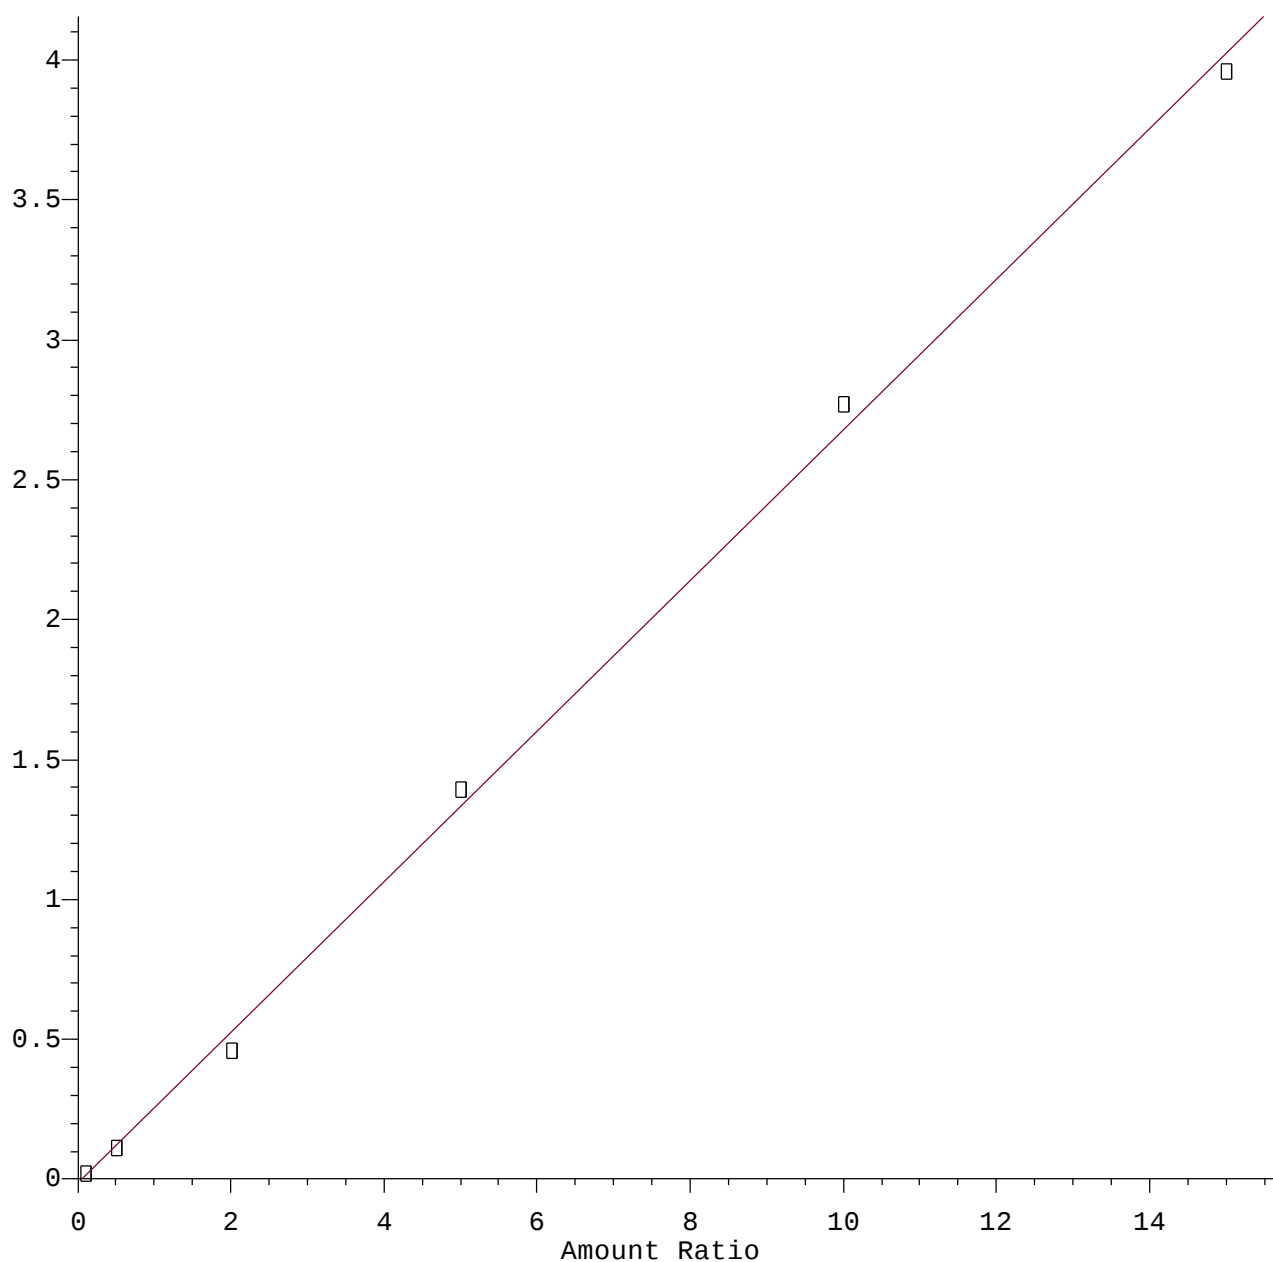

Resp Ratio = $2.69 \times 10^{-1} \times \text{Amt} - 1.35 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Calibration Table Last Updated: Fri Aug 02 17:31:55 2019

Instrument :
MSVOA_N
ClientSampleId :

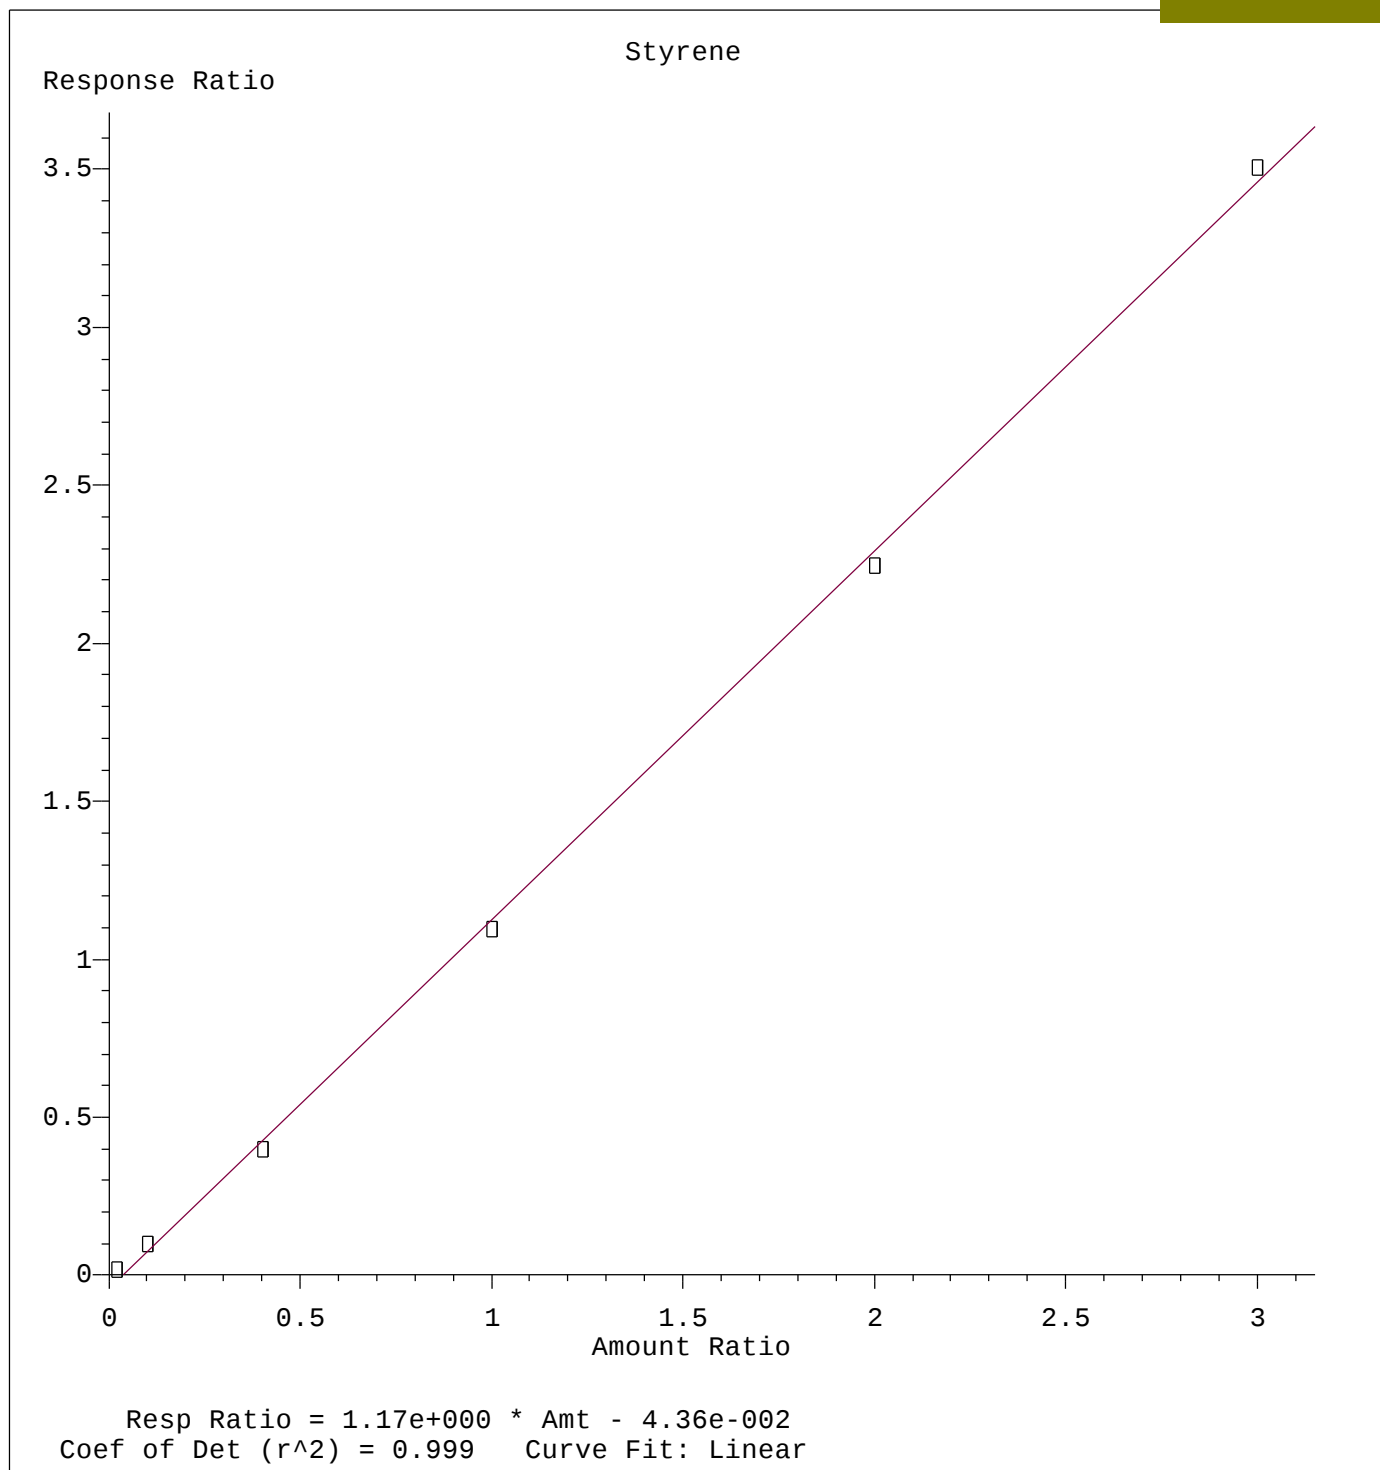


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Calibration Table Last Updated: Fri Aug 02 17:31:55 2019

Instrument :
MSVOA_N
ClientSampleId :

1,1,2,2-Tetrachloroethane


Response Ratio

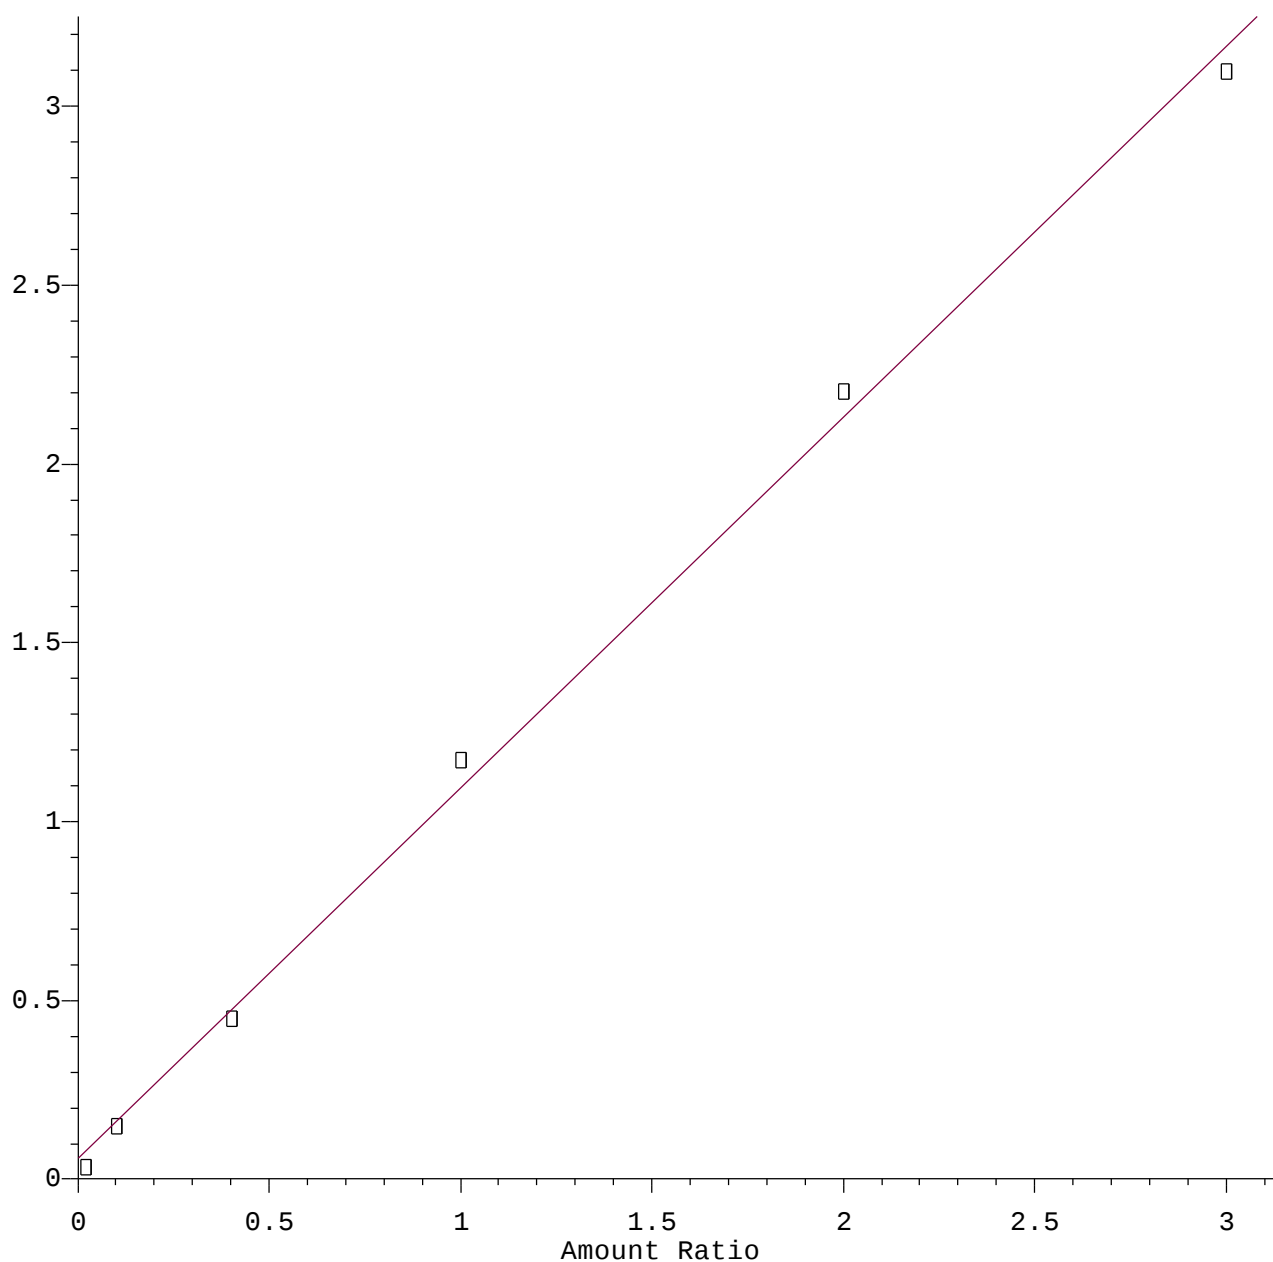

Resp Ratio = 1.04e+000 * Amt + 5.58e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Calibration Table Last Updated: Fri Aug 02 17:31:55 2019

Instrument :
MSVOA_N
ClientSampleId :

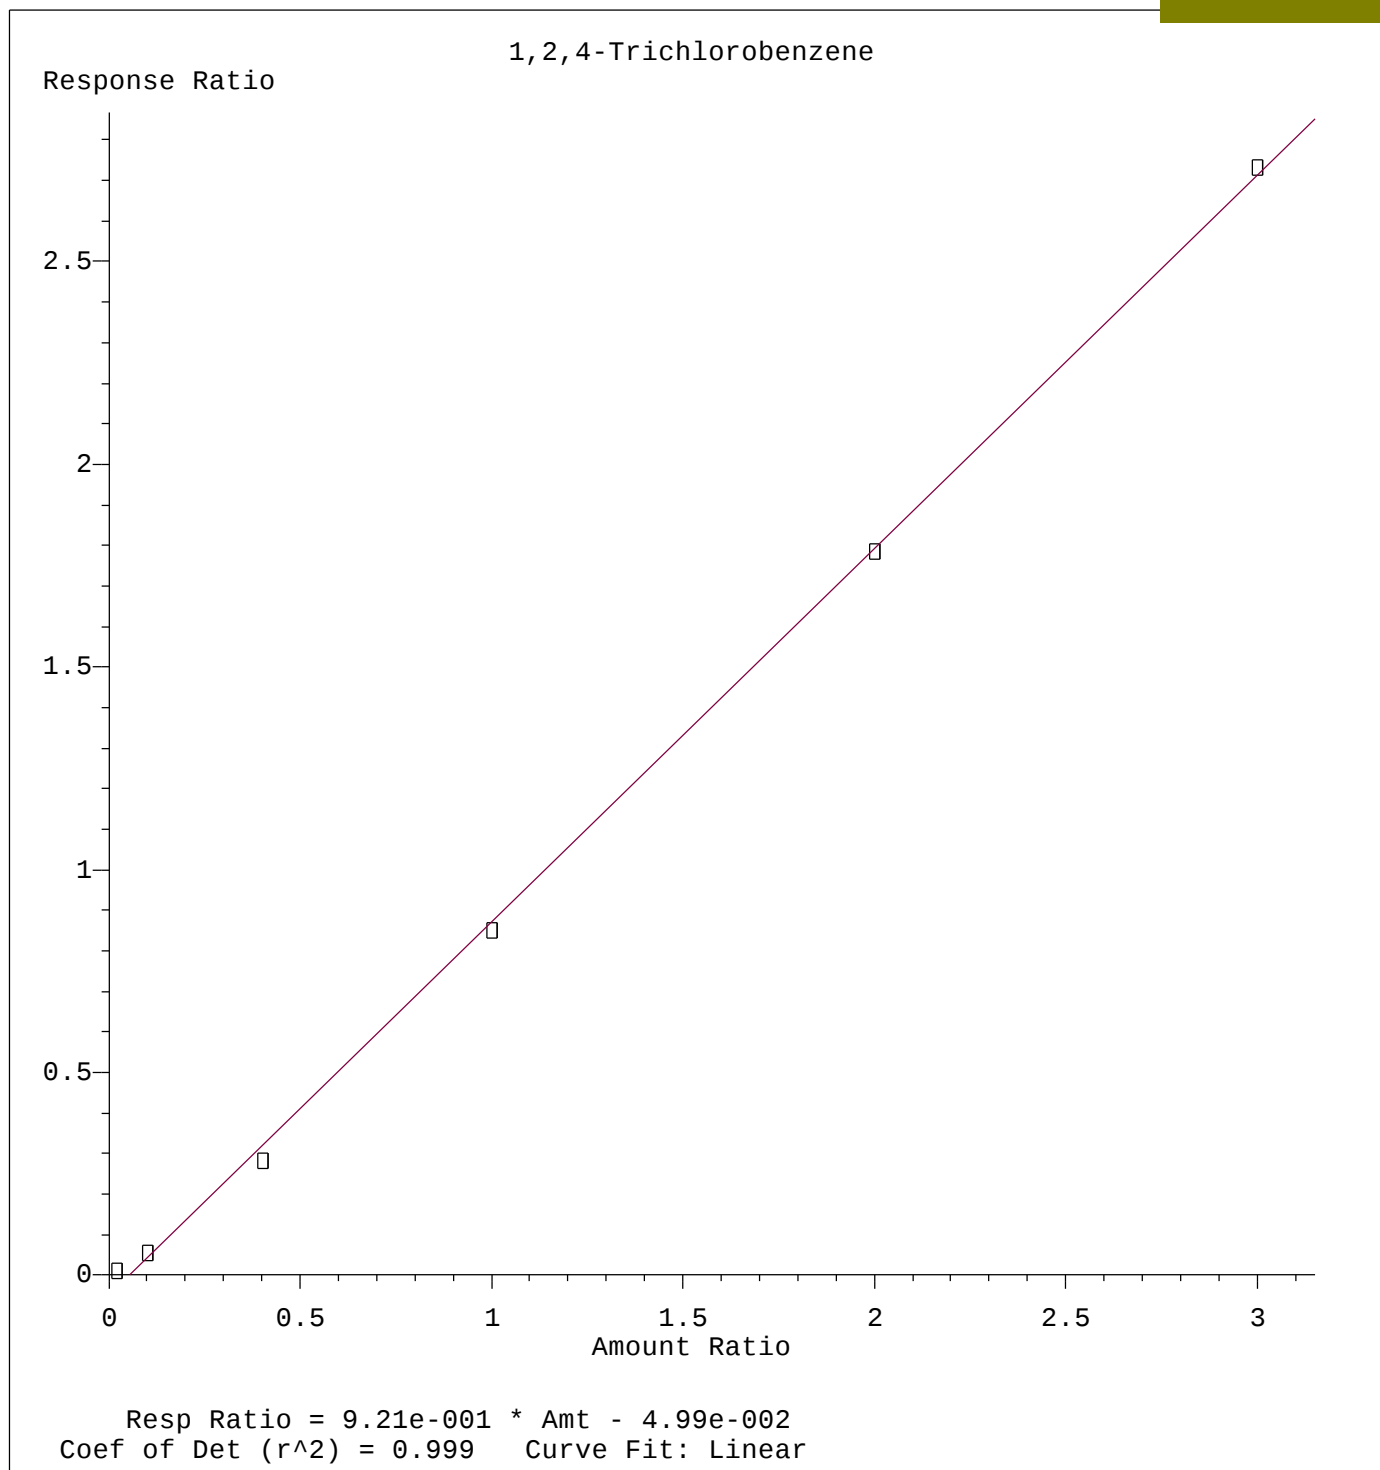

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Calibration Table Last Updated: Fri Aug 02 17:31:55 2019

Instrument :
MSVOA_N
ClientSampleId :

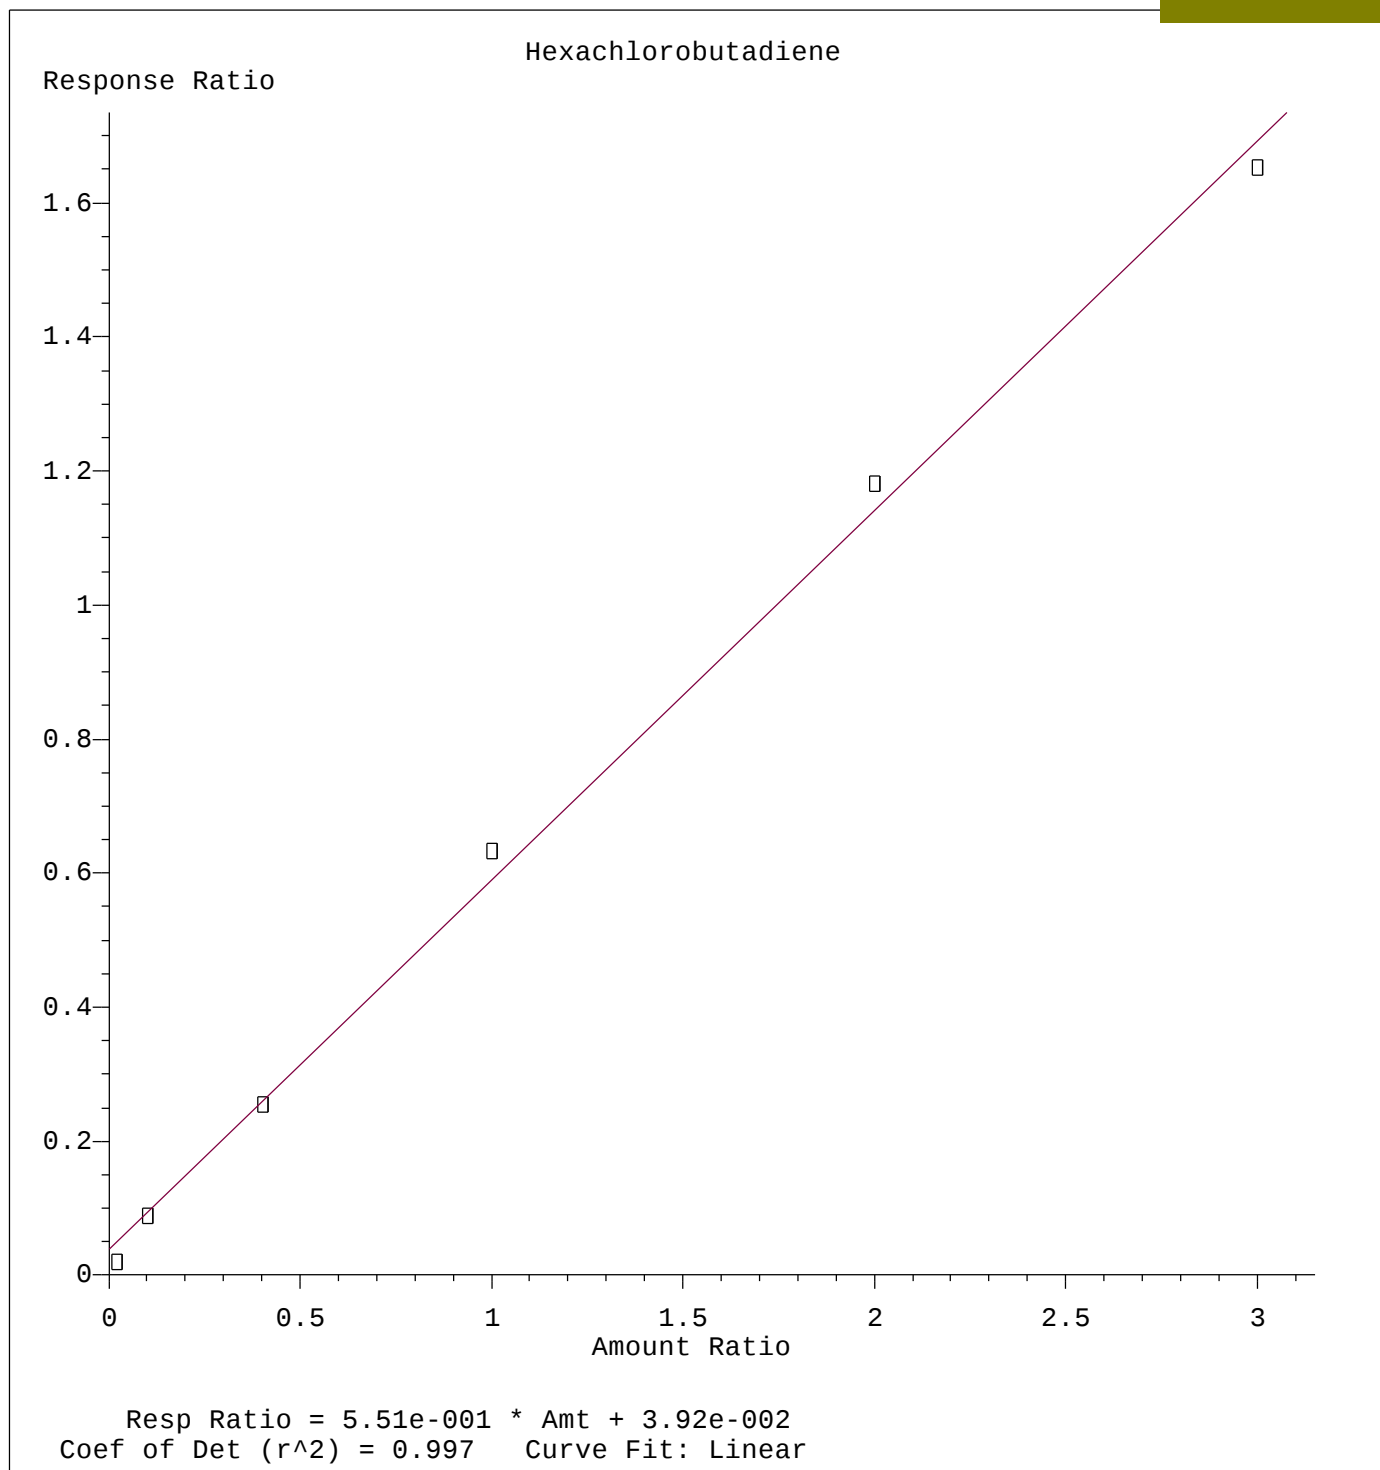


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Calibration Table Last Updated: Fri Aug 02 17:31:55 2019

Instrument :
MSVOA_N
ClientSampleId :

Naphthalene


Response Ratio

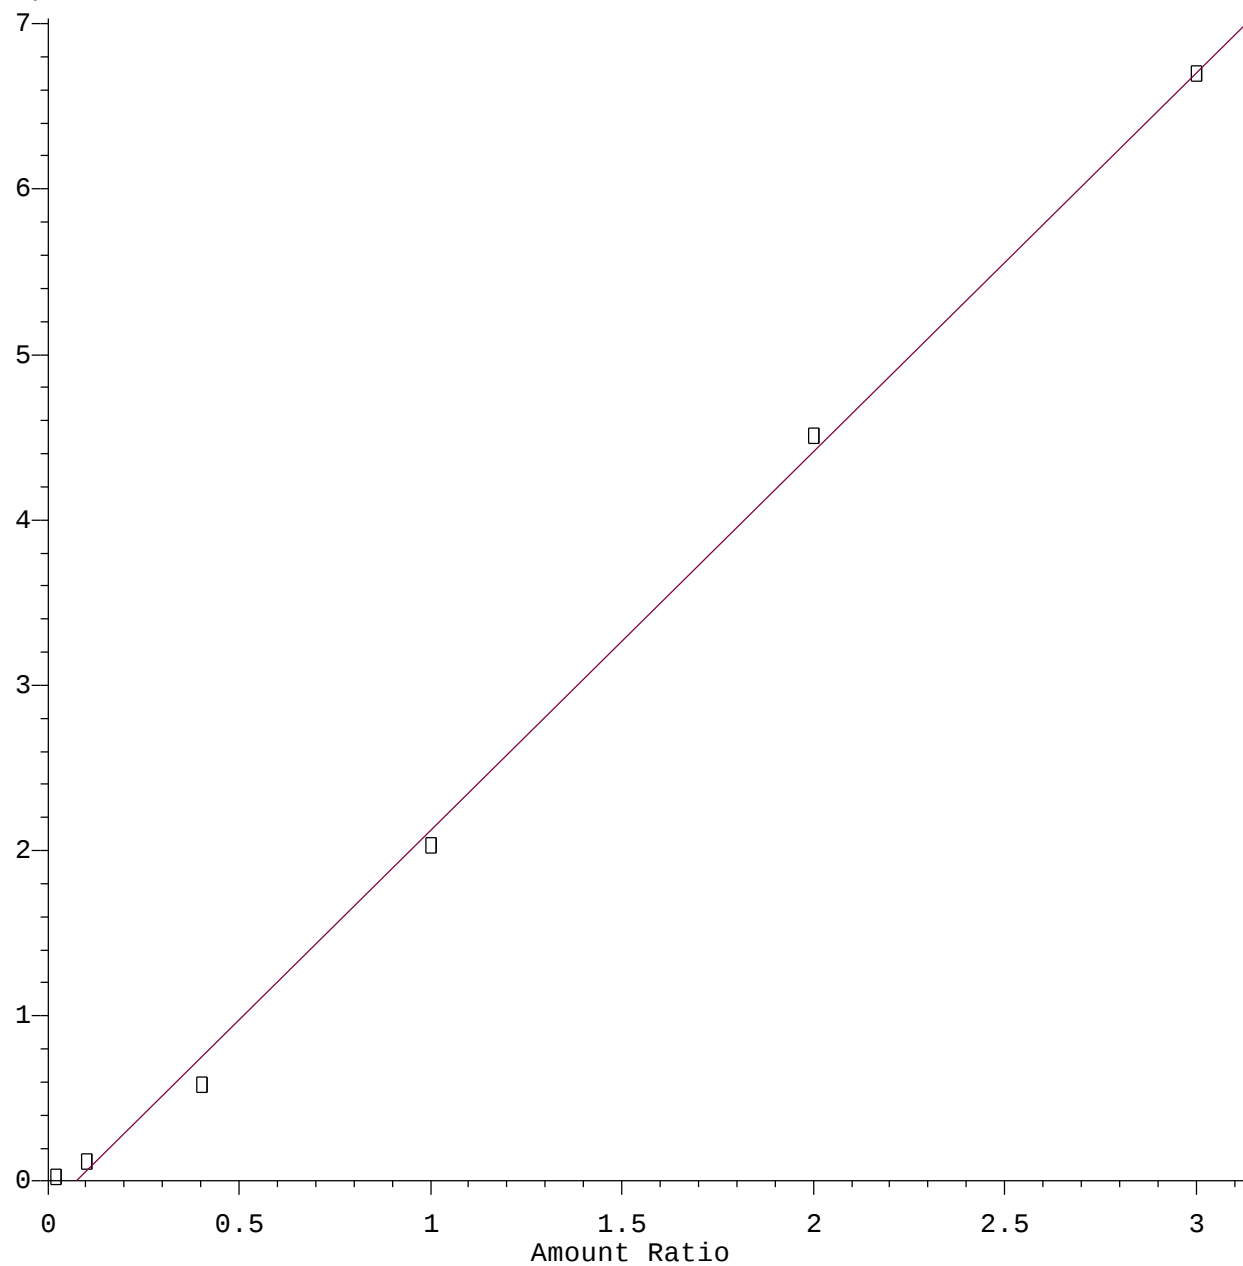

Resp Ratio = 2.29e+000 * Amt - 1.64e-001
Coef of Det (r²) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Calibration Table Last Updated: Fri Aug 02 17:31:55 2019

Instrument :
MSVOA_N
ClientSampleId :

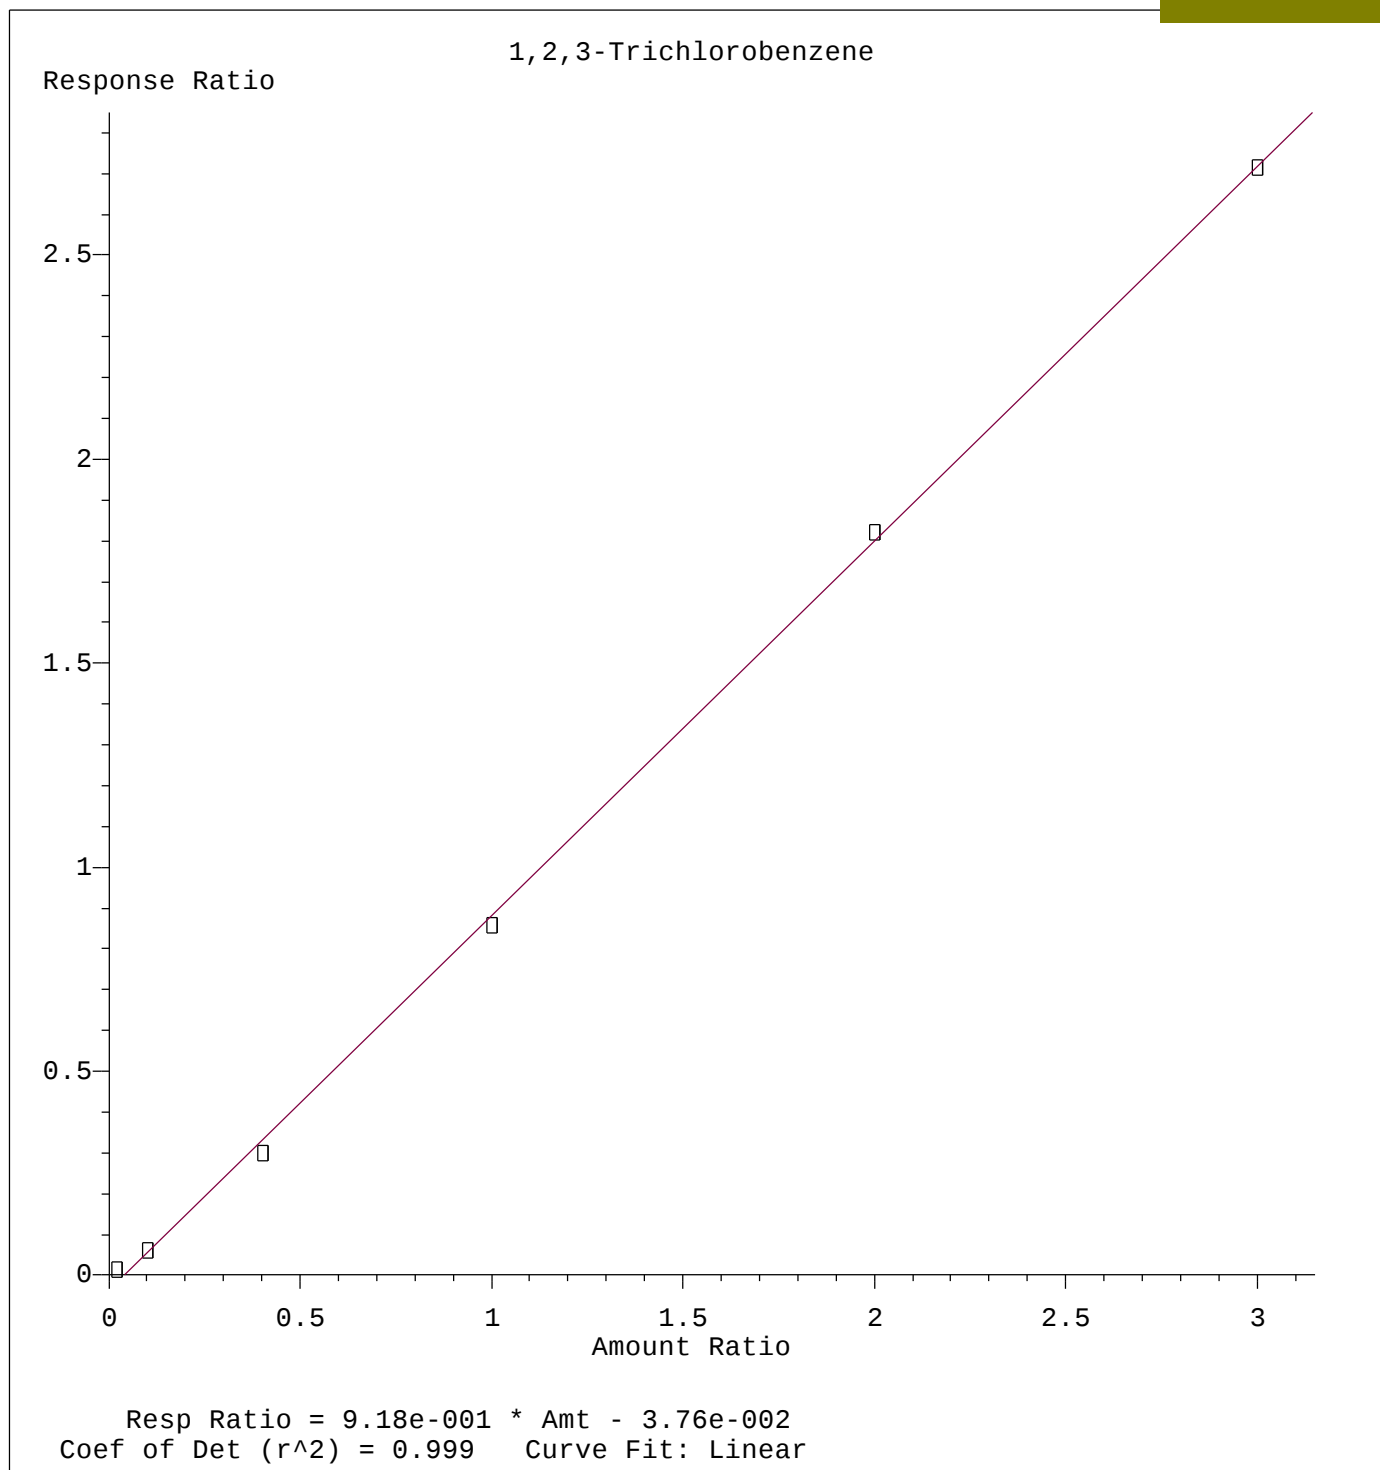

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072719W.M
Calibration Table Last Updated: Fri Aug 02 17:31:55 2019