


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN072719\  
 Data File : VN056937.D  
 Acq On : 26 Jul 2019 8:16  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N072719W.M  
 Title : SW846 8260  
 Last Update : Sat Jul 27 01:33:29 2019

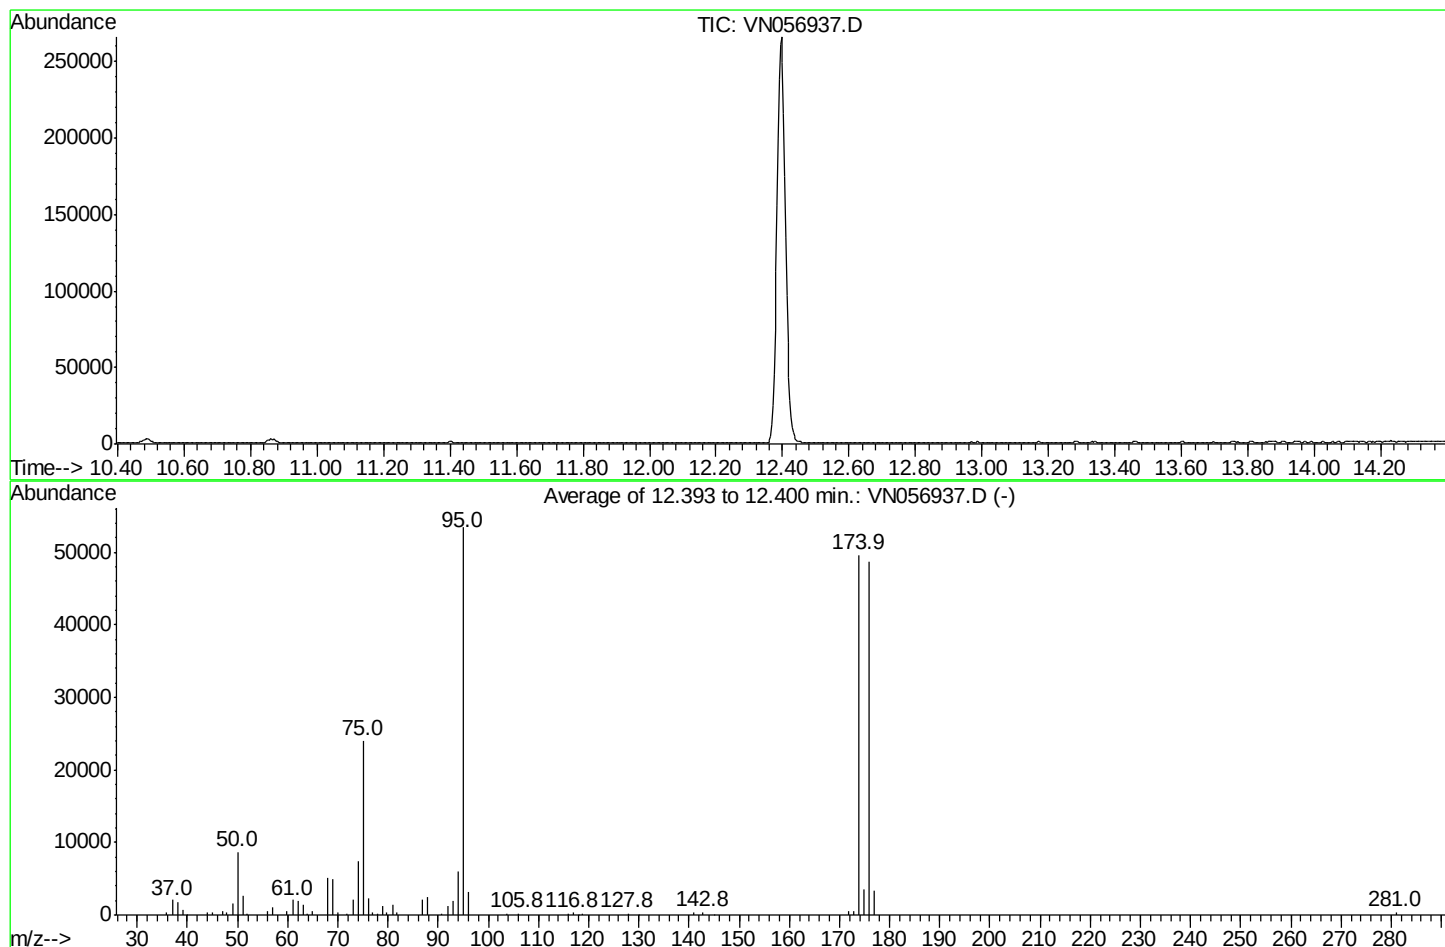

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3289

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.2      | 8650    | PASS             |
| 75          | 95           | 30           | 60           | 45.0      | 24050   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 53456   | PASS             |
| 96          | 95           | 5            | 9            | 6.0       | 3232    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.2       | 591     | PASS             |
| 174         | 95           | 50           | 100          | 92.9      | 49682   | PASS             |
| 175         | 174          | 5            | 9            | 7.3       | 3608    | PASS             |
| 176         | 174          | 95           | 101          | 98.0      | 48677   | PASS             |
| 177         | 176          | 5            | 9            | 6.9       | 3356    | PASS             |