

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072721\
 Data File : VN067943.D
 Acq On : 27 Jul 2021 21:17
 Operator : JC/MD
 Sample : PB137959ZHE#02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 28 05:25:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	316720	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	617689	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	638390	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	225214	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	249862	52.200	ug/l	0.00
Spiked Amount	50.000	Range 61 - 141	Recovery	= 104.400%		
35) Dibromofluoromethane	8.024	113	185241	49.637	ug/l	0.00
Spiked Amount	50.000	Range 69 - 133	Recovery	= 99.280%		
50) Toluene-d8	10.446	98	801712	51.323	ug/l	0.00
Spiked Amount	50.000	Range 65 - 126	Recovery	= 102.640%		
62) 4-Bromofluorobenzene	12.733	95	267261	48.433	ug/l	0.00
Spiked Amount	50.000	Range 58 - 135	Recovery	= 96.860%		
Target Compounds						
					Qvalue	
5) Bromomethane	2.815	94	52	Below Cal	#	4
6) Chloroethane	3.022	64	100	Below Cal	#	1
7) Trichlorofluoromethane	3.368	101	58	Below Cal	#	18
13) Acrolein	4.041	56	45	Below Cal	#	1
16) Acetone	4.290	43	42712	28.358	ug/l	93
18) Methyl Acetate	4.862	43	11264	2.663	ug/l	99
20) Methylene Chloride	5.095	84	29023	7.665	ug/l	98
25) 2-Butanone	7.348	43	8094	3.236	ug/l	94
29) Tetrahydrofuran	7.699	42	3121	1.898	ug/l	# 87
31) Cyclohexane	8.088	56	7986	1.190	ug/l	# 1
36) 1,1-Dichloropropene	8.085	75	28456	4.959	ug/l	# 51
37) Ethyl Acetate	7.348	43	8094	1.456	ug/l	# 69
38) Carbon Tetrachloride	8.088	117	34579	6.110	ug/l	# 16
41) Methacrylonitrile	7.697	41	1019	0.357	ug/l	# 19
43) Isopropyl Acetate	8.566	43	43459	4.444	ug/l	# 91
45) 1,2-Dichloropropane	9.630	63	2804	0.645	ug/l	# 44
48) Methyl methacrylate	9.550	41	10376	2.399	ug/l	# 12
49) 1,4-Dioxane	9.628	88	265	35.114	ug/l	# 1
51) 4-Methyl-2-Pentanone	10.336	43	10891	1.813	ug/l	92
53) t-1,3-Dichloropropene	10.717	75	78	1.755	ug/l	# 1
54) cis-1,3-Dichloropropene	10.247	75	70247	10.472	ug/l	# 59
57) 1,3-Dichloropropane	11.092	76	45167	6.109	ug/l	# 43
59) 2-Hexanone	11.095	43	645637	153.958	ug/l	# 54
60) Dibromochloromethane	11.497	129	445	2.437	ug/l	# 11
71) Bromoform	12.712	173	69	3.192	ug/l	# 29
76) 1,2,3-Trichloropropane	12.733	75	148681	32.327	ug/l	# 100
80) 1,3,5-Trimethylbenzene	13.066	105	3626	0.246	ug/l	90
81) trans-1,4-Dichloro-2-b...	12.733	75	148681	104.226	ug/l	# 6
93) 1,2,4-Trichlorobenzene	15.265	180	580	2.821	ug/l	# 46
95) Naphthalene	15.512	128	4279	3.377	ug/l	97
96) 1,2,3-Trichlorobenzene	15.697	180	421	2.743	ug/l	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072721\
Data File : VN067943.D
Acq On : 27 Jul 2021 21:17
Operator : JC/MD
Sample : PB137959ZHE#02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 28 05:25:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration

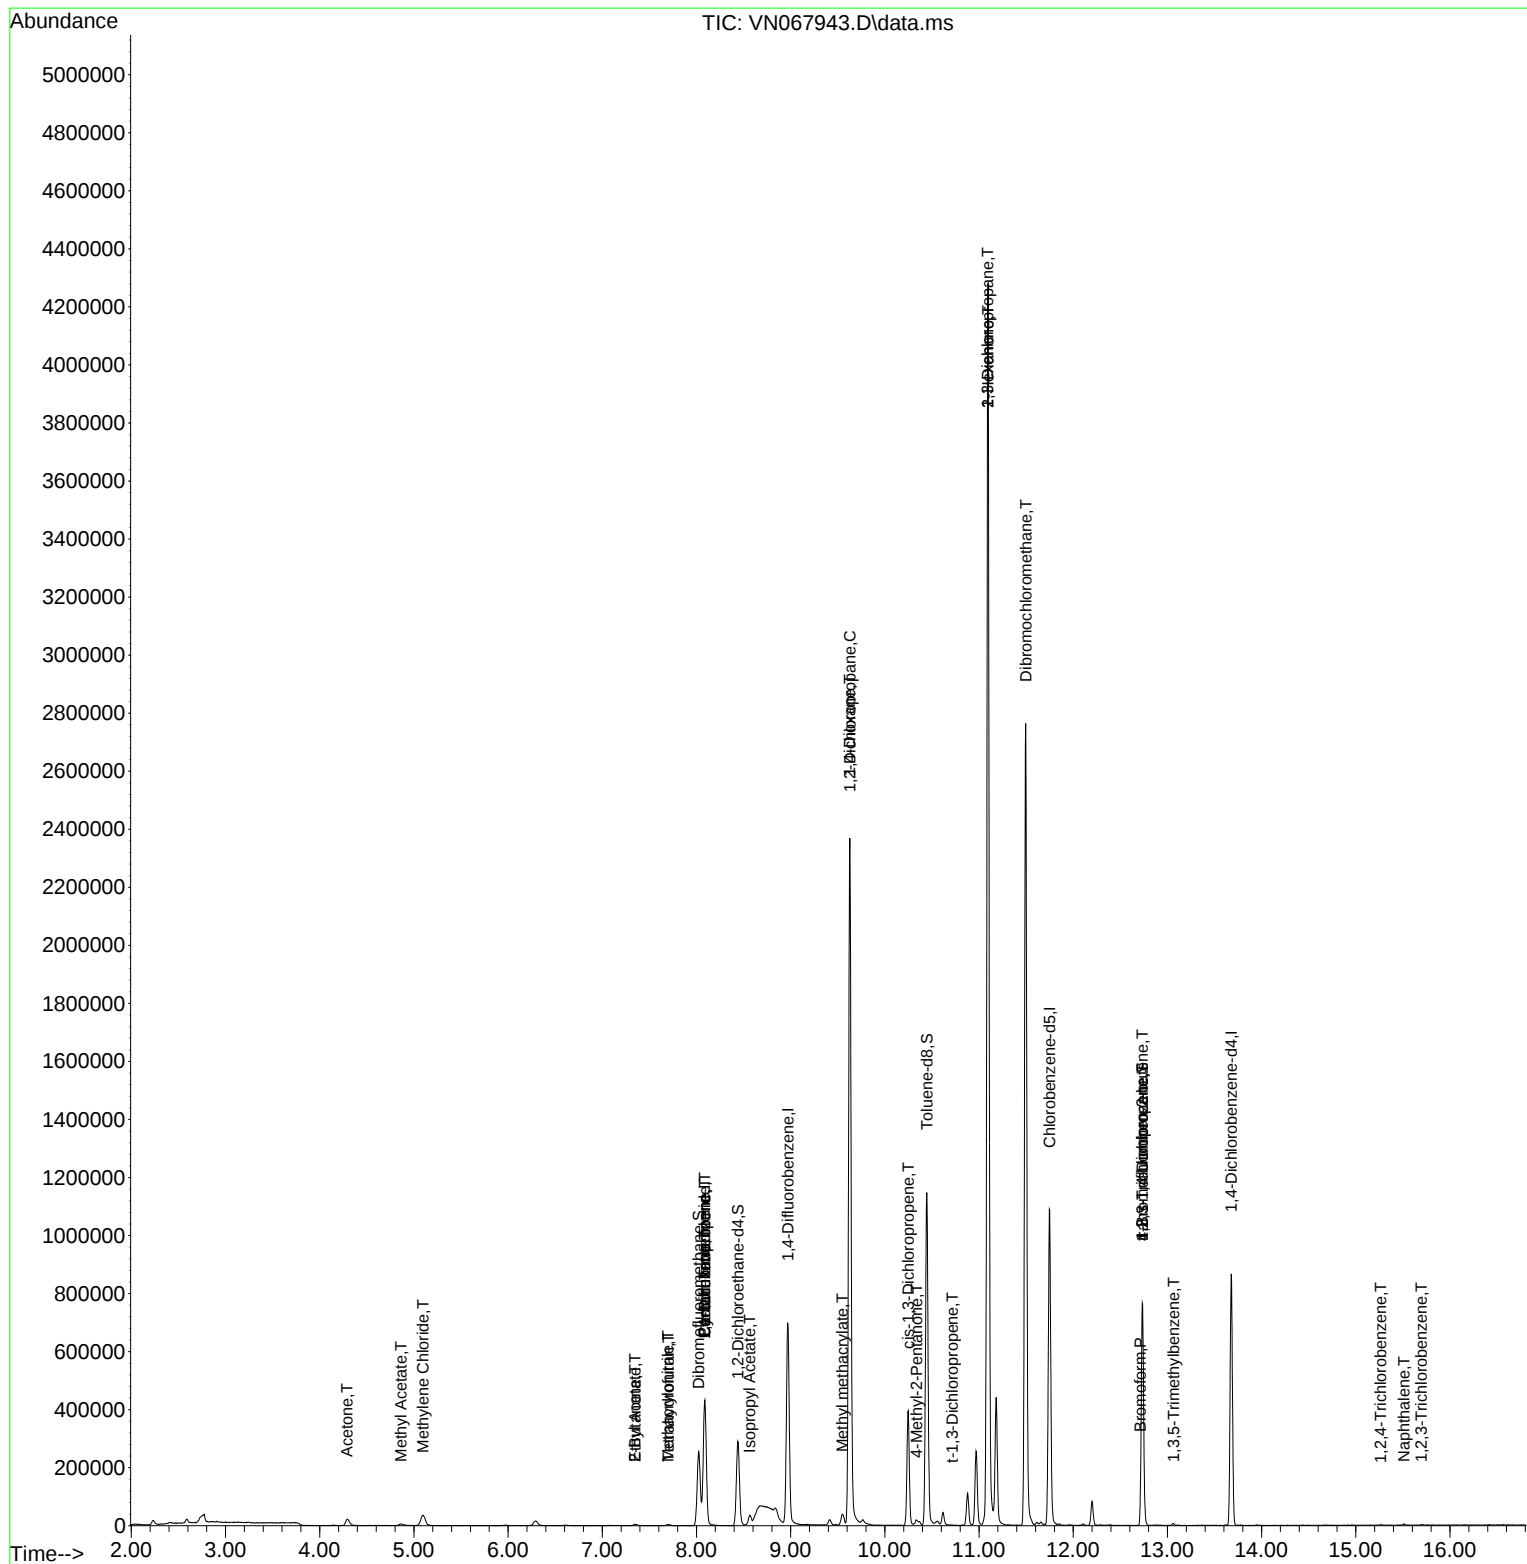

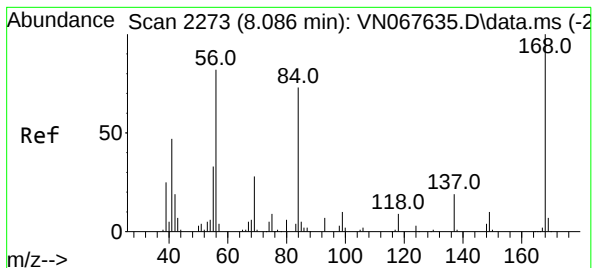

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. 0.002 min

Lab File: VN067943.D





Acq: 27 Jul 2021 21:17

Tgt Ion:168 Resp: 316720

Ion Ratio Lower Upper

168 100

99 64.0 62.9 94.3

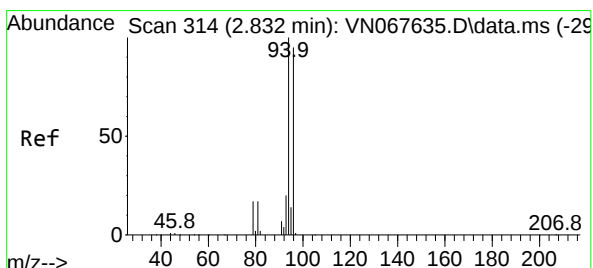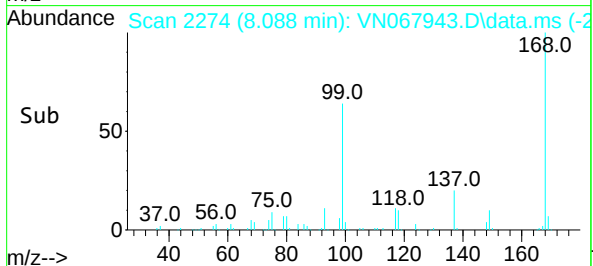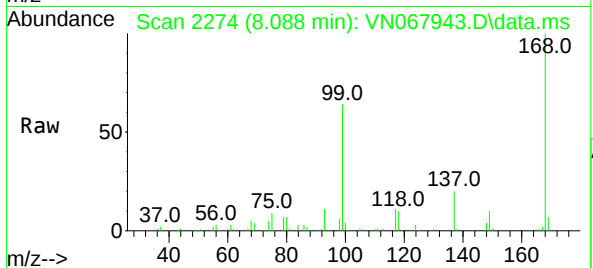

#5

Bromomethane

Concen: Below Cal

RT: 2.815 min Scan# 308

Delta R.T. -0.017 min

Lab File: VN067943.D




Acq: 27 Jul 2021 21:17


Tgt Ion: 94 Resp: 52

Ion Ratio Lower Upper

94 100

96 0.0 73.7 110.5#


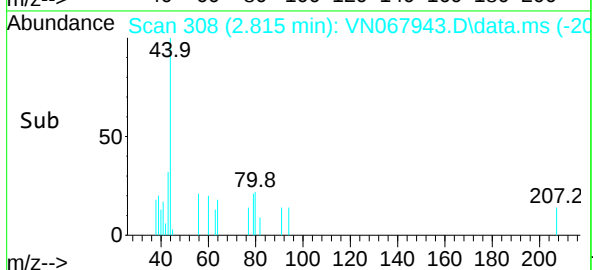

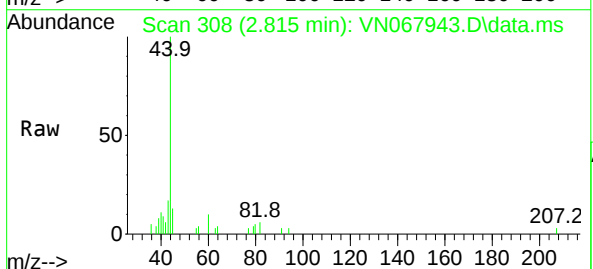




#6
Chloroethane
Concen: Below Cal
RT: 3.022 min Scan# 385
Delta R.T. 0.016 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 100
Ion Ratio Lower Upper
64 100
66 165.8 24.7 37.1#

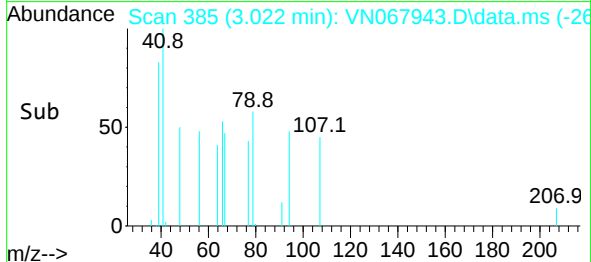

#7
Trichlorofluoromethane
Concen: Below Cal
RT: 3.368 min Scan# 514
Delta R.T. 0.003 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion: 101 Resp: 58
Ion Ratio Lower Upper
101 100
103 0.0 51.2 76.8#


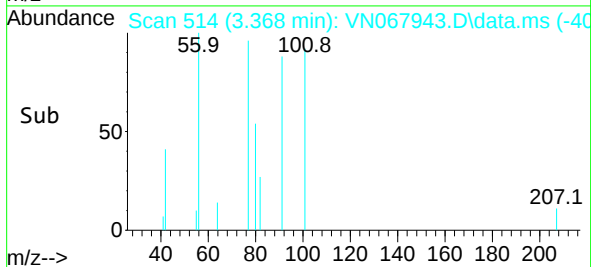

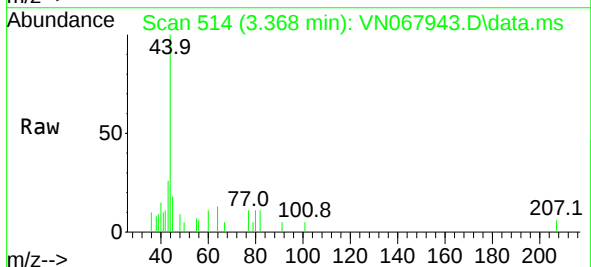




#13
Acrolein
Concen: Below Cal
RT: 4.041 min Scan# 765
Delta R.T. 0.002 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 45
Ion Ratio Lower Upper
56 100
55 248.9 57.4 86.0#

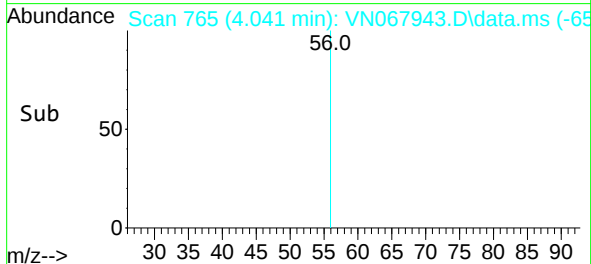

#16
Acetone
Concen: 28.358 ug/l
RT: 4.290 min Scan# 858
Delta R.T. 0.002 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion: 43 Resp: 42712
Ion Ratio Lower Upper
43 100
58 30.2 21.2 31.8

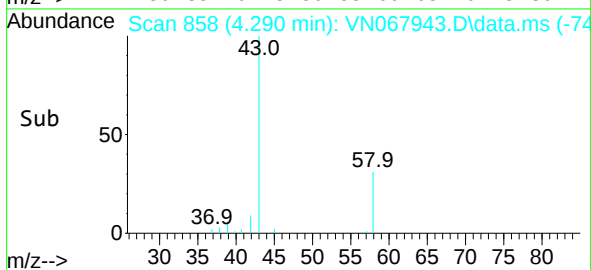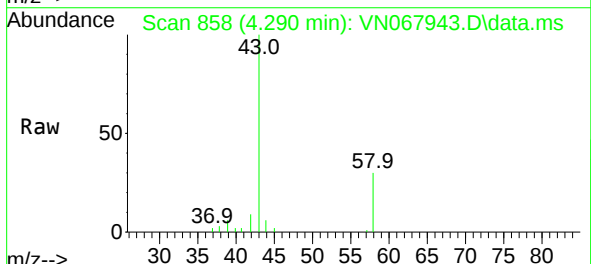

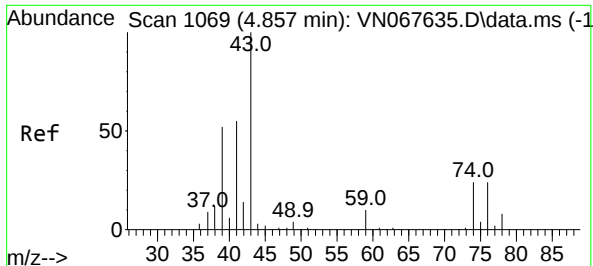

#18

Methyl Acetate

Concen: 2.663 ug/l

RT: 4.862 min Scan# 1071

Delta R.T. 0.005 min

Lab File: VN067943.D





Acq: 27 Jul 2021 21:17

Tgt Ion: 43 Resp: 11264

Ion Ratio Lower Upper

43 100

74 21.2 17.4 26.0

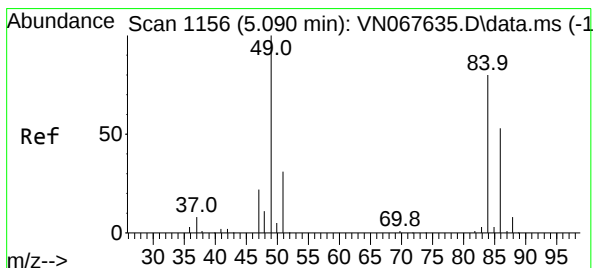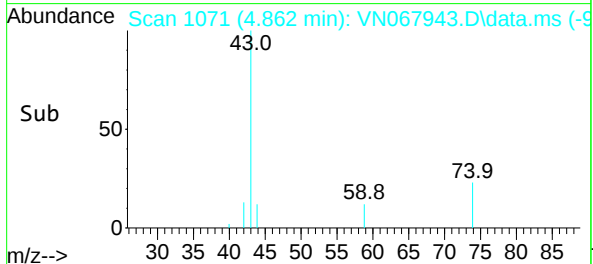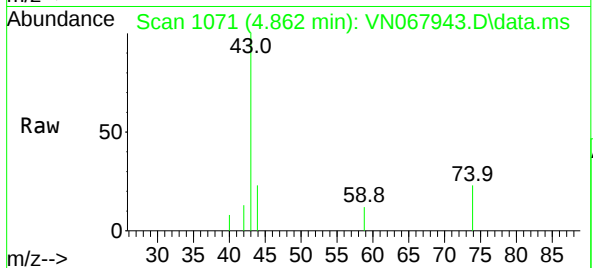

#20

Methylene Chloride

Concen: 7.665 ug/l

RT: 5.095 min Scan# 1158

Delta R.T. 0.005 min

Lab File: VN067943.D

Acq: 27 Jul 2021 21:17

Tgt Ion: 84 Resp: 29023




Ion Ratio Lower Upper


84 100

49 136.2 110.9 166.3

51 44.1 32.6 49.0

86 63.6 51.6 77.4


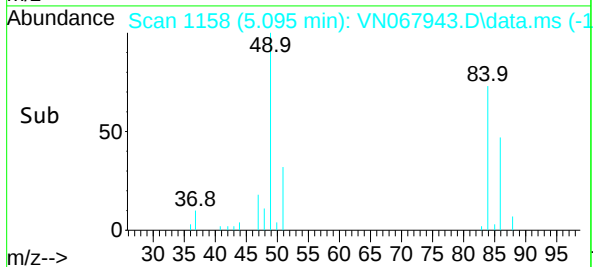

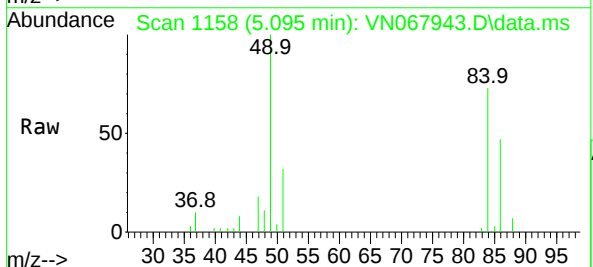


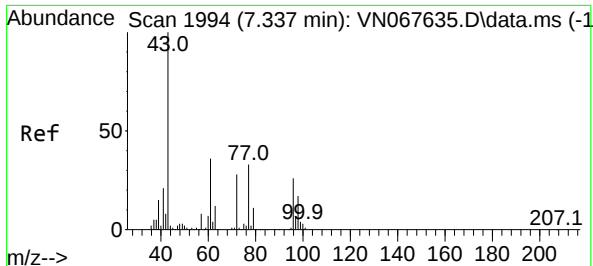

#25
2-Butanone
Concen: 3.236 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. 0.011 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 8094
Ion Ratio Lower Upper
43 100
72 27.3 19.7 29.5

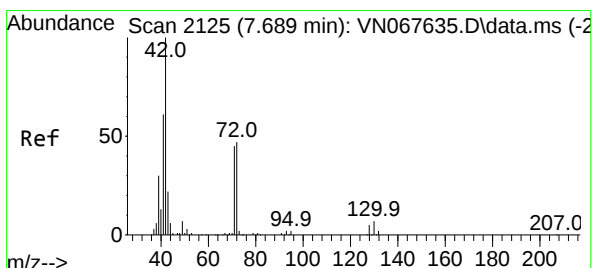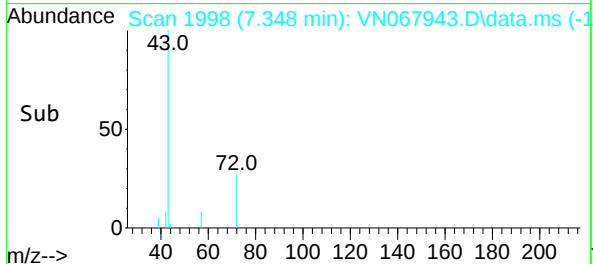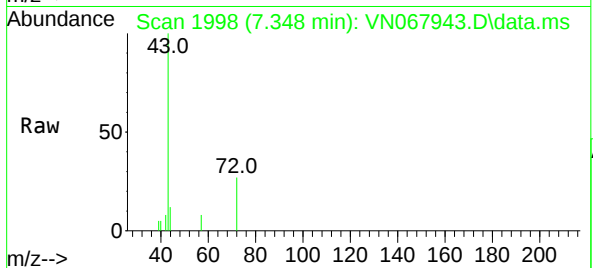

#29
Tetrahydrofuran
Concen: 1.898 ug/l
RT: 7.699 min Scan# 2129
Delta R.T. 0.010 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17


Tgt Ion: 42 Resp: 3121
Ion Ratio Lower Upper
42 100
72 28.8 32.8 49.2#
71 42.7 31.2 46.8

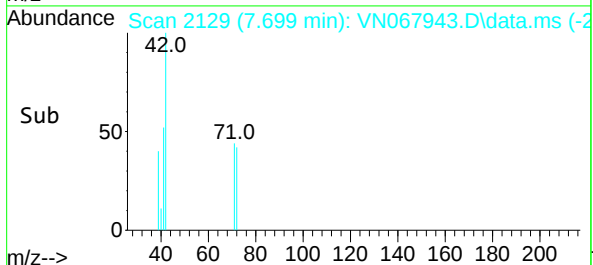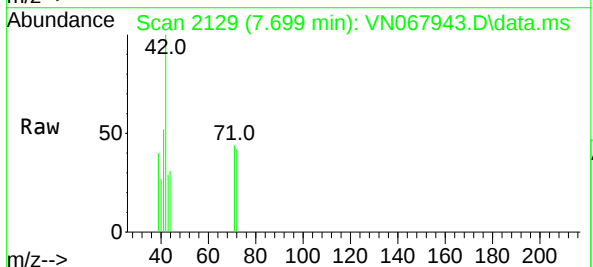






#31
Cyclohexane
Concen: 1.190 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.006 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion: 56 Resp: 7986
Ion Ratio Lower Upper
56 100
69 159.5 27.3 40.9#
84 126.2 64.9 97.3#




#33
1,2-Dichloroethane-d4
Concen: 52.200 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

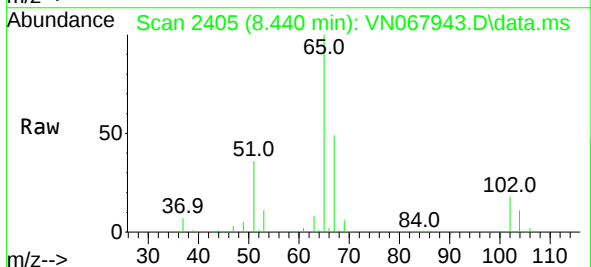

Tgt Ion: 65 Resp: 249862
Ion Ratio Lower Upper
65 100
67 49.3 0.0 98.6









#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:114 Resp: 617689
Ion Ratio Lower Upper
114 100
63 20.5 0.0 49.0
88 15.1 0.0 36.6

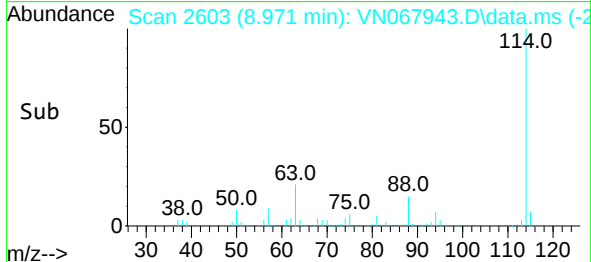

#35
Dibromofluoromethane
Concen: 49.637 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17


Tgt Ion:113 Resp: 185241
Ion Ratio Lower Upper
113 100
111 102.0 83.8 125.8
192 15.7 13.4 20.0

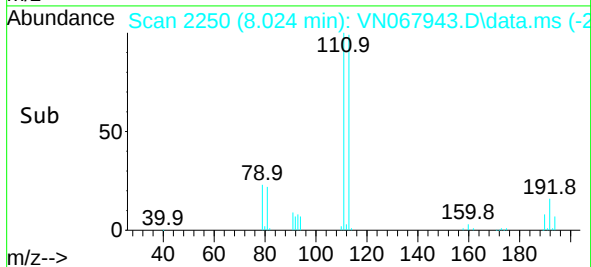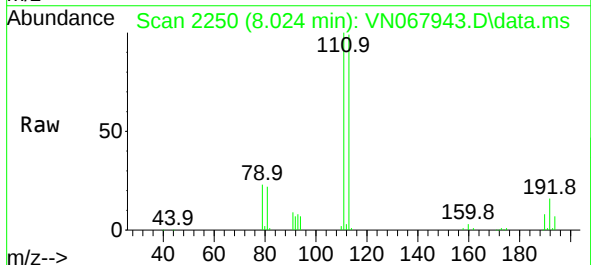






#36
1,1-Dichloropropene
Concen: 4.959 ug/l
RT: 8.085 min Scan# 2273
Delta R.T. -0.137 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Instrument :
MSVOA_N
ClientSampled :



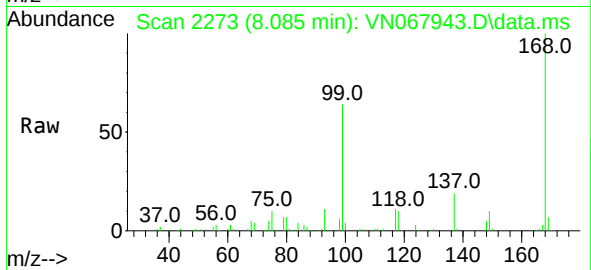



Tgt Ion: 75 Resp: 28456
Ion Ratio Lower Upper
75 100
110 8.2 15.7 47.0#
77 0.0 24.6 37.0#

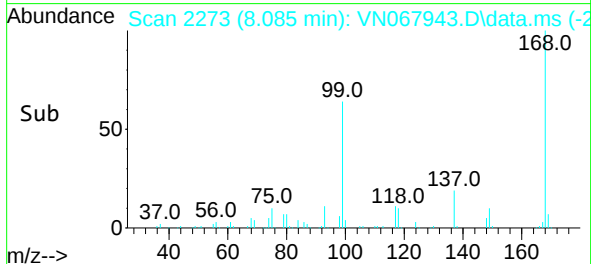

#37
Ethyl Acetate
Concen: 1.456 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. -0.070 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17


Tgt Ion: 43 Resp: 8094
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.1 12.1#

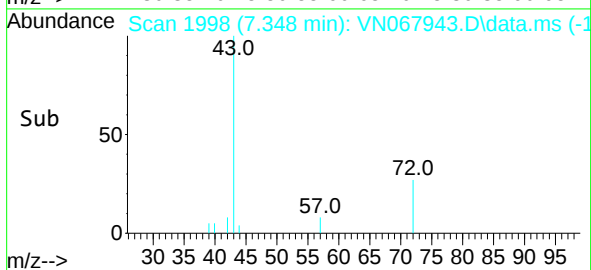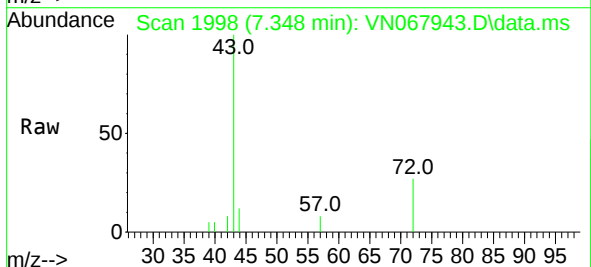



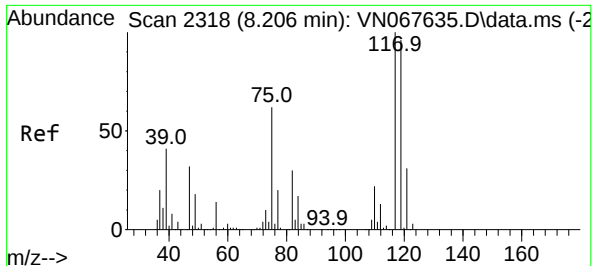


#38
Carbon Tetrachloride
Concen: 6.110 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Instrument :
MSVOA_N
ClientSampled :



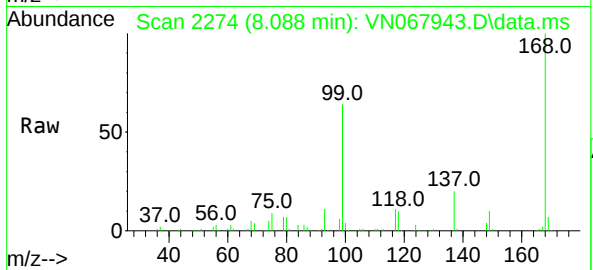



Tgt Ion:117 Resp: 34579
Ion Ratio Lower Upper
117 100
119 3.7 75.4 113.2#
121 0.0 23.5 35.3#

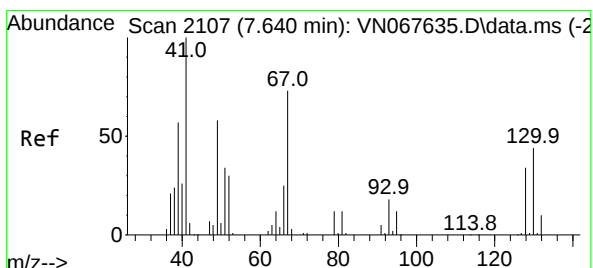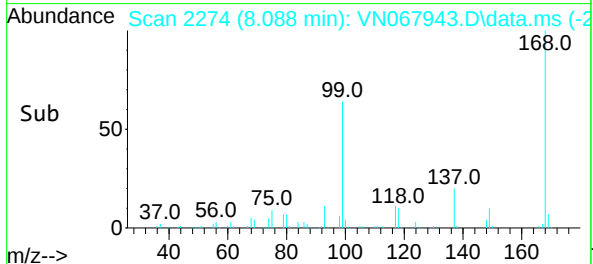

#41
Methacrylonitrile
Concen: 0.357 ug/l
RT: 7.697 min Scan# 2128
Delta R.T. 0.057 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion: 41 Resp: 1019
Ion Ratio Lower Upper
41 100
39 124.0 47.6 71.4#
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#


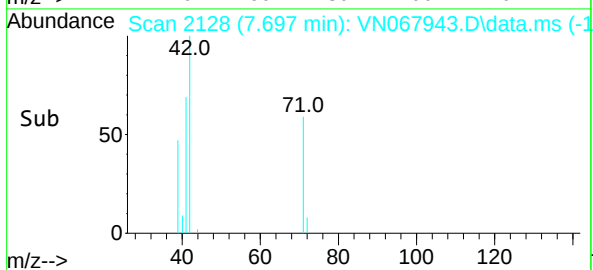

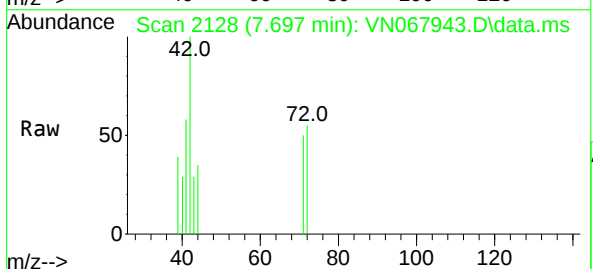




#43
Isopropyl Acetate
Concen: 4.444 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.003 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 43459
Ion Ratio Lower Upper
43 100
61 17.1 19.0 28.4#
87 11.3 9.5 14.3

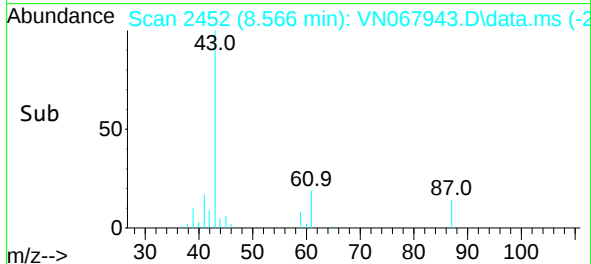

#45
1,2-Dichloropropane
Concen: 0.645 ug/l
RT: 9.630 min Scan# 2849
Delta R.T. 0.139 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion: 63 Resp: 2804
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#


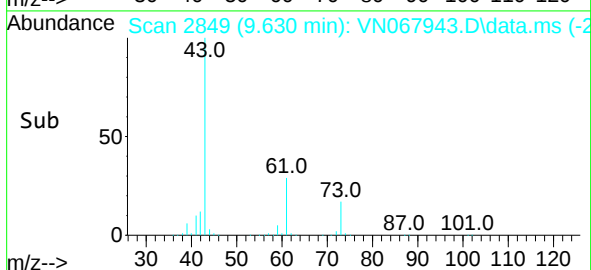






#48
Methyl methacrylate
Concen: 2.399 ug/l
RT: 9.550 min Scan# 2819
Delta R.T. -0.013 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 10376
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

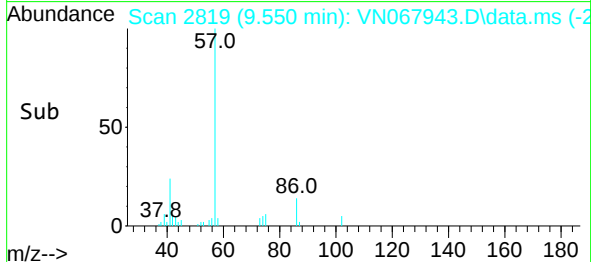

#49
1,4-Dioxane
Concen: 35.114 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.057 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion: 88 Resp: 265
Ion Ratio Lower Upper
88 100
43 878966.0 28.8 43.2#
58 4032.8 60.4 90.6#


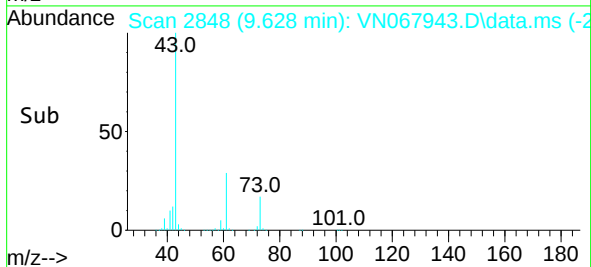

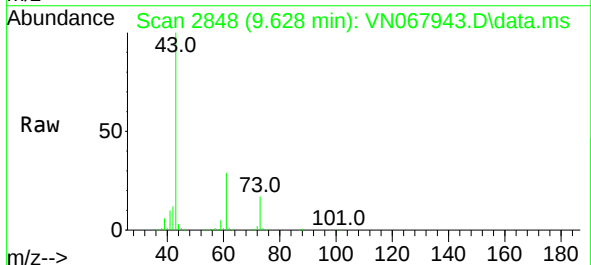




#50
Toluene-d8
Concen: 51.323 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 801712
Ion Ratio Lower Upper
98 100
100 63.9 51.7 77.5

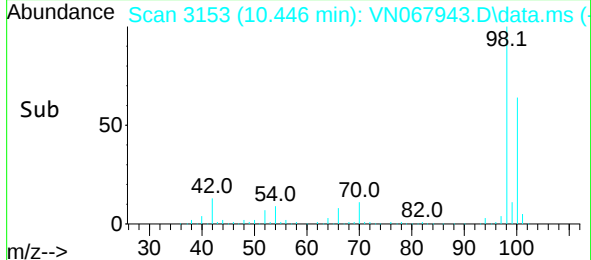

#51
4-Methyl-2-Pentanone
Concen: 1.813 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion: 43 Resp: 10891
Ion Ratio Lower Upper
43 100
58 40.6 28.6 43.0


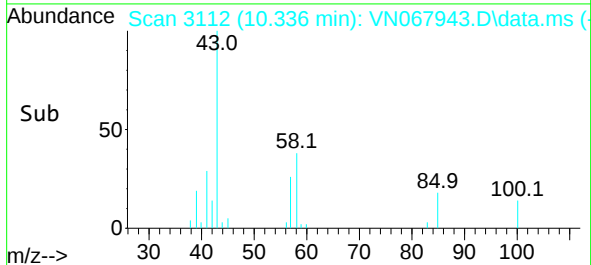

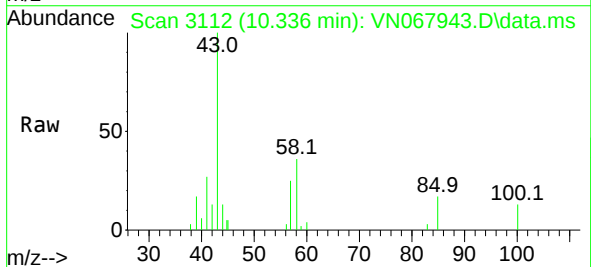




#53
t-1,3-Dichloropropene
Concen: 1.755 ug/l
RT: 10.717 min Scan# 3254
Delta R.T. -0.005 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 78
Ion Ratio Lower Upper
75 100
77 115.1 25.1 37.7#

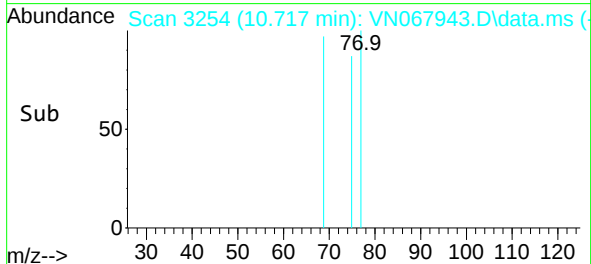

#54
cis-1,3-Dichloropropene
Concen: 10.472 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion: 75 Resp: 70247
Ion Ratio Lower Upper
75 100
77 0.0 24.6 37.0#
39 37.1 50.7 76.1#


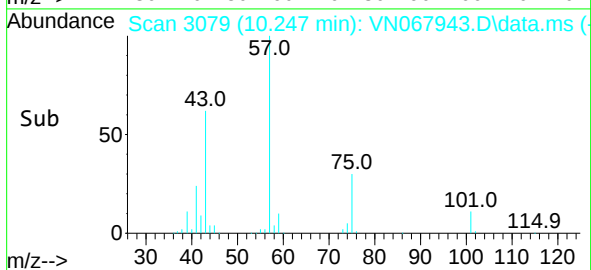

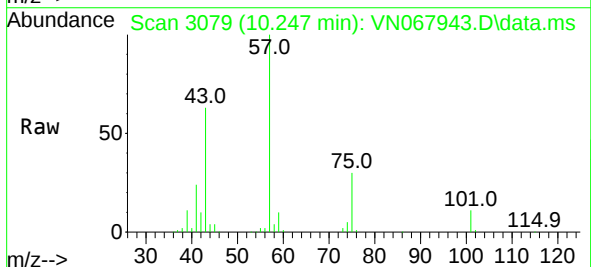




#57
1,3-Dichloropropane
Concen: 6.109 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.045 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 45167
Ion Ratio Lower Upper
76 100
78 0.4 25.7 38.5#

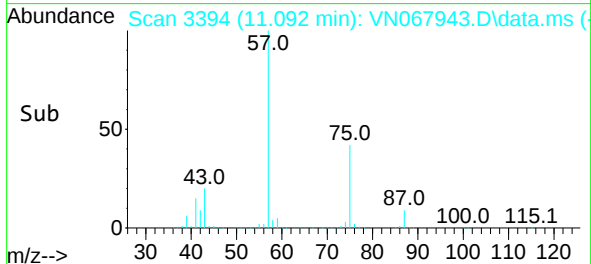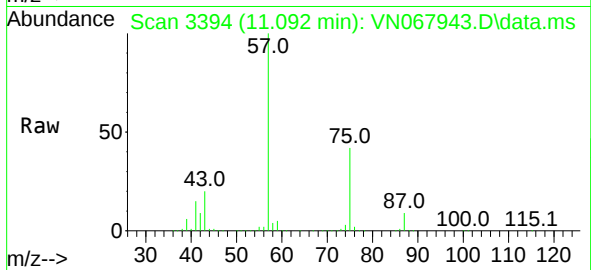

#59
2-Hexanone
Concen: 153.958 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion: 43 Resp: 645637
Ion Ratio Lower Upper
43 100
58 18.2 24.7 74.1#


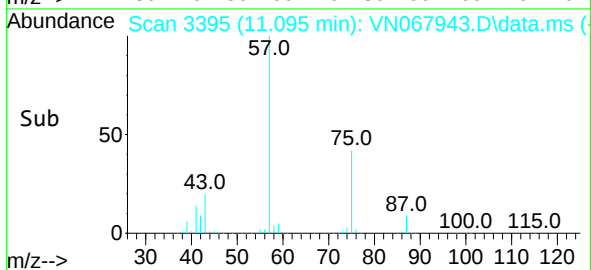

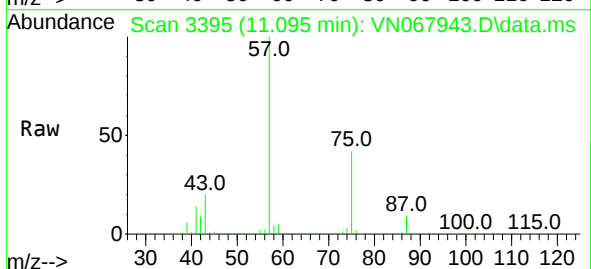




#60
Dibromochloromethane
Concen: 2.437 ug/l
RT: 11.497 min Scan# 3545
Delta R.T. 0.255 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:129 Resp: 445
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

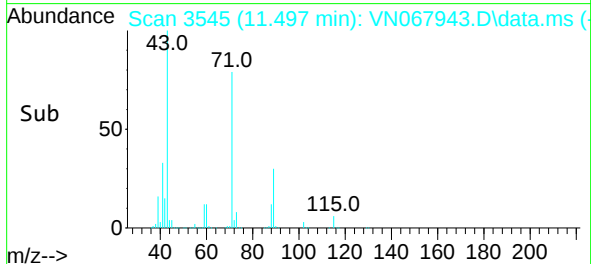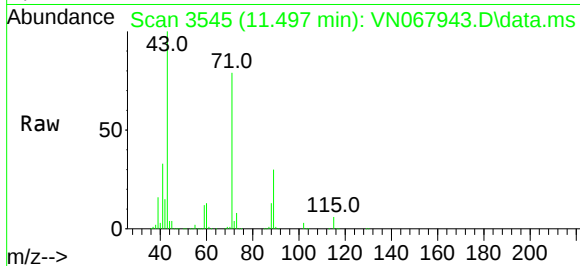

#62
4-Bromofluorobenzene
Concen: 48.433 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion: 95 Resp: 267261
Ion Ratio Lower Upper
95 100
174 73.0 0.0 122.0
176 69.7 0.0 117.6


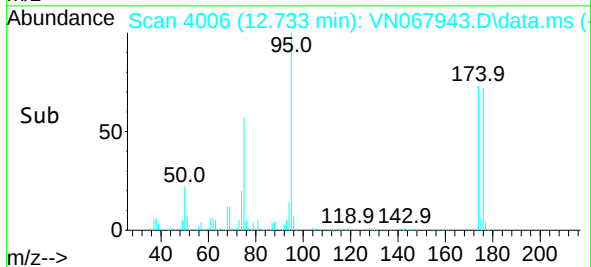

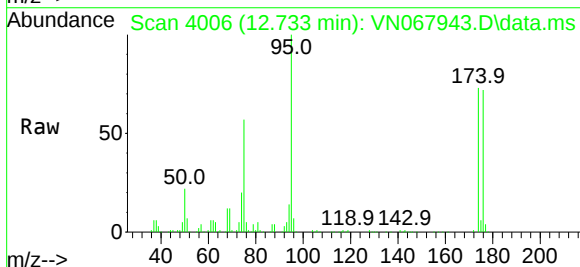


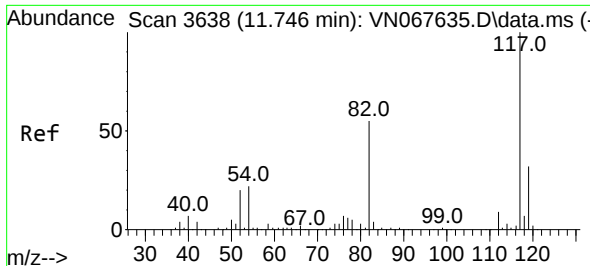

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 638390
Ion Ratio Lower Upper
117 100
82 54.2 53.1 79.7
119 31.6 25.5 38.3

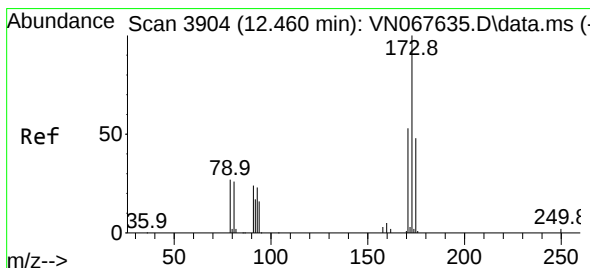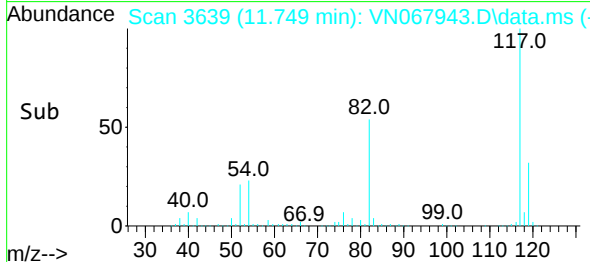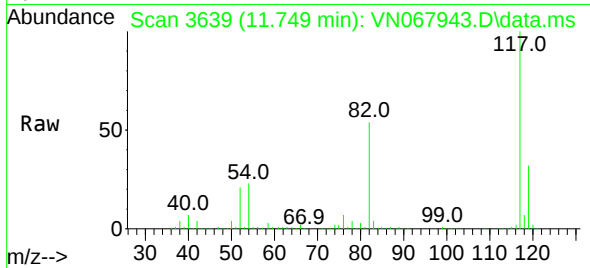

#71
Bromoform
Concen: 3.192 ug/l
RT: 12.712 min Scan# 3998
Delta R.T. 0.252 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

Tgt Ion:173 Resp: 69
Ion Ratio Lower Upper
173 100
175 0.0 23.9 71.8#
254 0.0 0.0 0.0


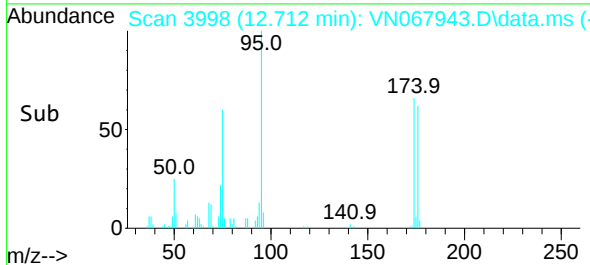

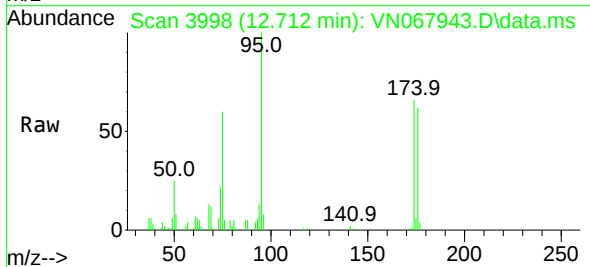


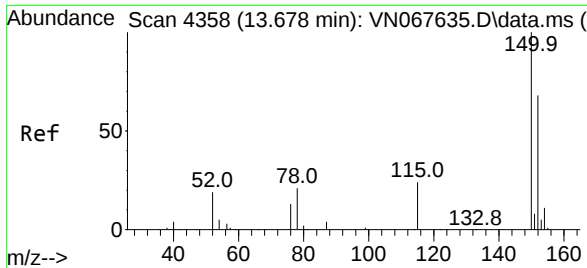

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.677 min Scan# 4358
 Delta R.T. -0.000 min
 Lab File: VN067943.D
 Acq: 27 Jul 2021 21:17




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion:152 Resp: 225214
 Ion Ratio Lower Upper
 152 100
 115 61.5 36.1 108.5
 150 155.5 0.0 351.8

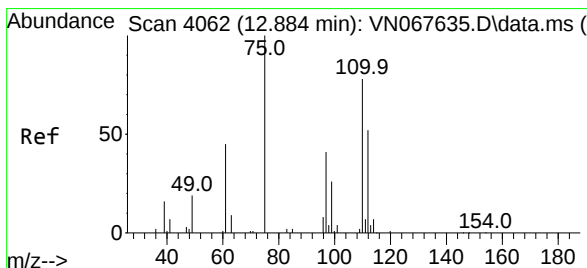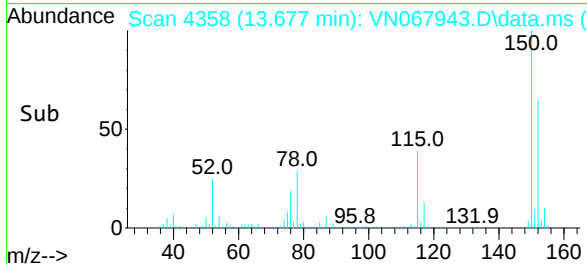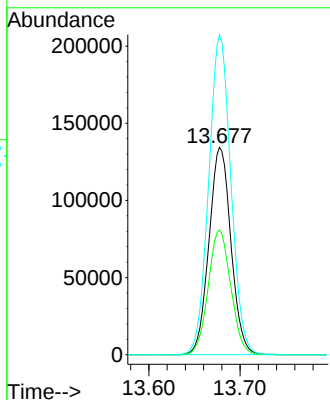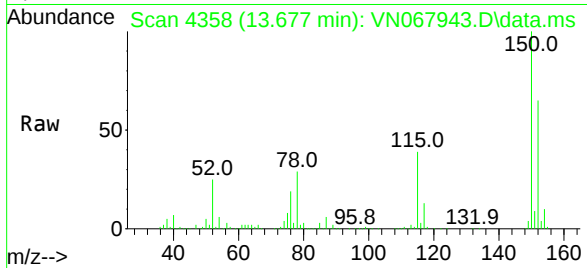

#76
 1,2,3-Trichloropropane
 Concen: 32.327 ug/l
 RT: 12.733 min Scan# 4006
 Delta R.T. -0.151 min
 Lab File: VN067943.D
 Acq: 27 Jul 2021 21:17

Tgt Ion: 75 Resp: 148681
 Ion Ratio Lower Upper
 75 100
 77 0.4 0.0 0.0#


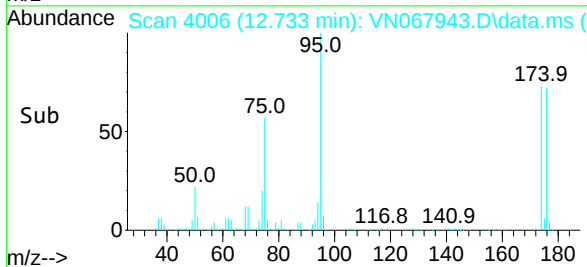
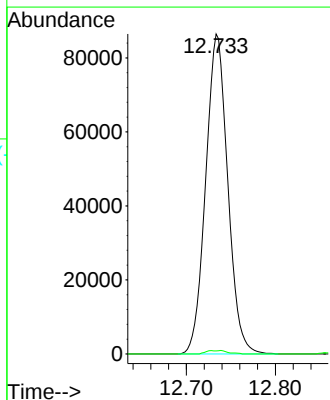
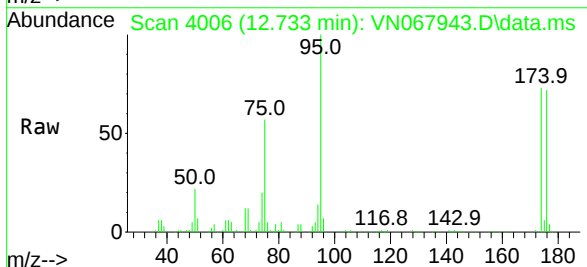


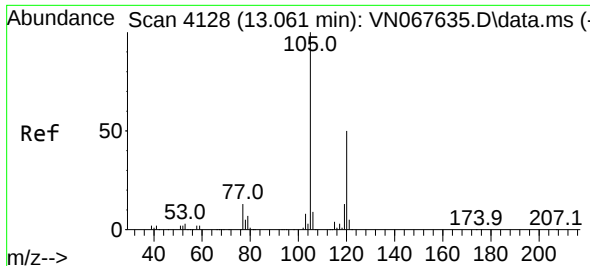

#80
1,3,5-Trimethylbenzene
Concen: 0.246 ug/l
RT: 13.066 min Scan# 4130
Delta R.T. 0.005 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 3626
Ion Ratio Lower Upper
105 100
120 50.7 22.2 66.6

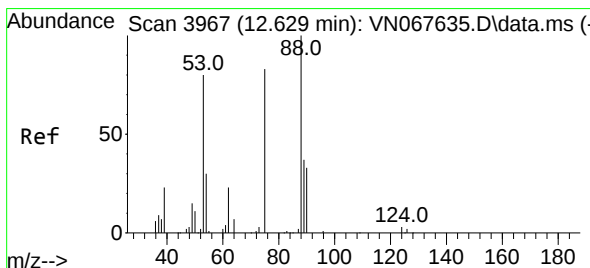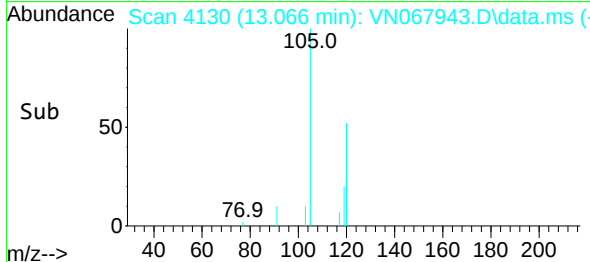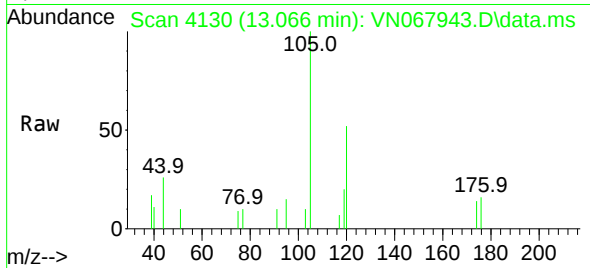

#81
trans-1,4-Dichloro-2-butene
Concen: 104.226 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17


Tgt Ion: 75 Resp: 148681
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

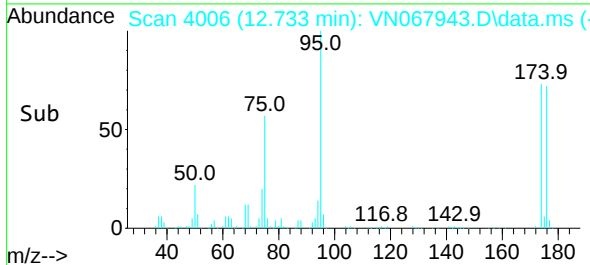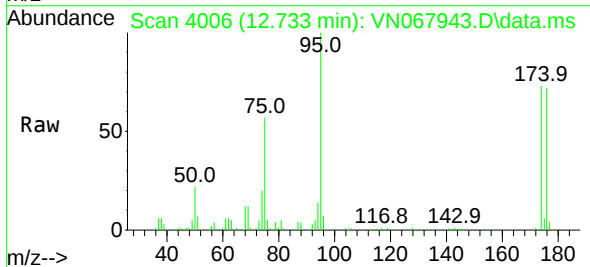



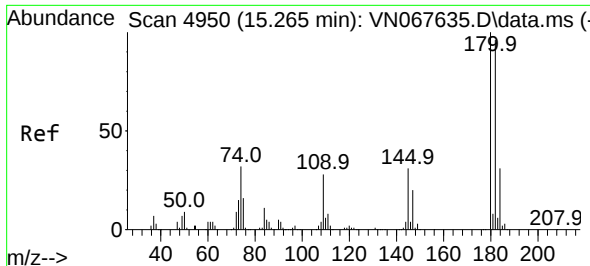


#93
1,2,4-Trichlorobenzene
Concen: 2.821 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17


Instrument :
MSVOA_N
ClientSampled :

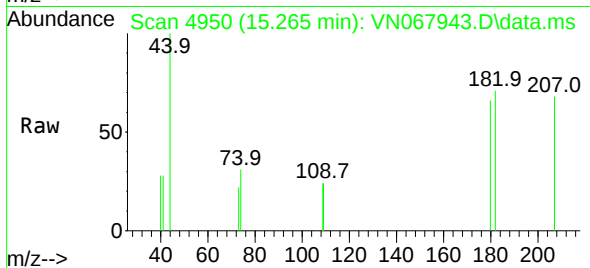



Tgt Ion:180 Resp: 580
Ion Ratio Lower Upper
180 100
182 152.6 47.5 142.5#
145 12.8 17.2 51.6#

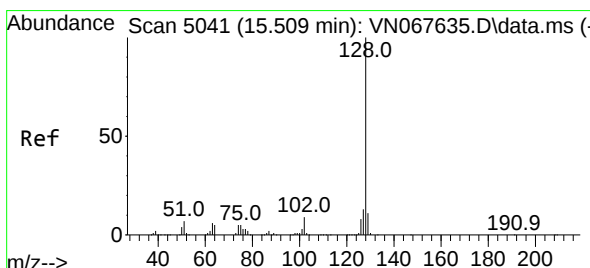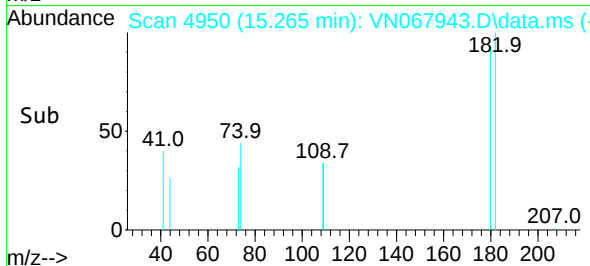


#95
Naphthalene
Concen: 3.377 ug/l
RT: 15.512 min Scan# 5042
Delta R.T. 0.003 min
Lab File: VN067943.D
Acq: 27 Jul 2021 21:17

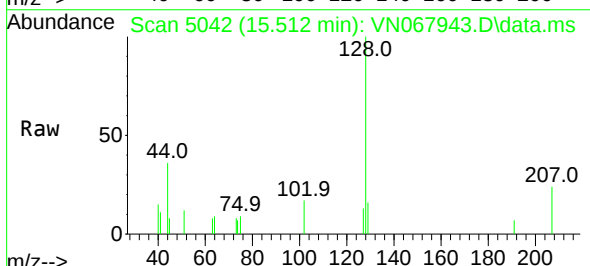


Tgt Ion:128 Resp: 4279
Ion Ratio Lower Upper
128 100
127 11.8 10.6 15.8
129 11.2 8.6 12.8

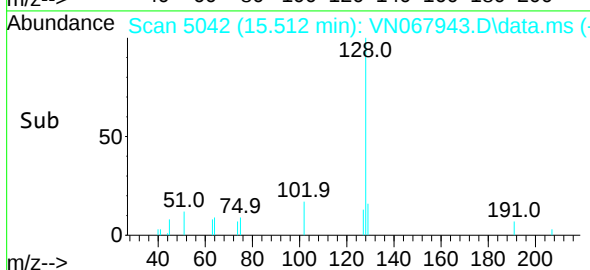



#96
 1,2,3-Trichlorobenzene
 Concen: 2.743 ug/l
 RT: 15.697 min Scan# 5111
 Delta R.T. -0.005 min
 Lab File: VN067943.D
 Acq: 27 Jul 2021 21:17

Instrument :
 MSVOA_N
 ClientSampleId :

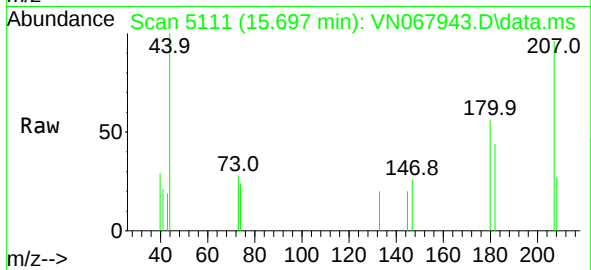

Tgt Ion:180 Resp: 421
 Ion Ratio Lower Upper
 180 100
 182 91.4 47.8 143.3
 145 12.8 18.2 54.6#

