


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072721\
 Data File : VN067920.D
 Acq On : 27 Jul 2021 10:42
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Title : SW846 8260
 Last Update : Wed Jul 07 16:18:53 2021

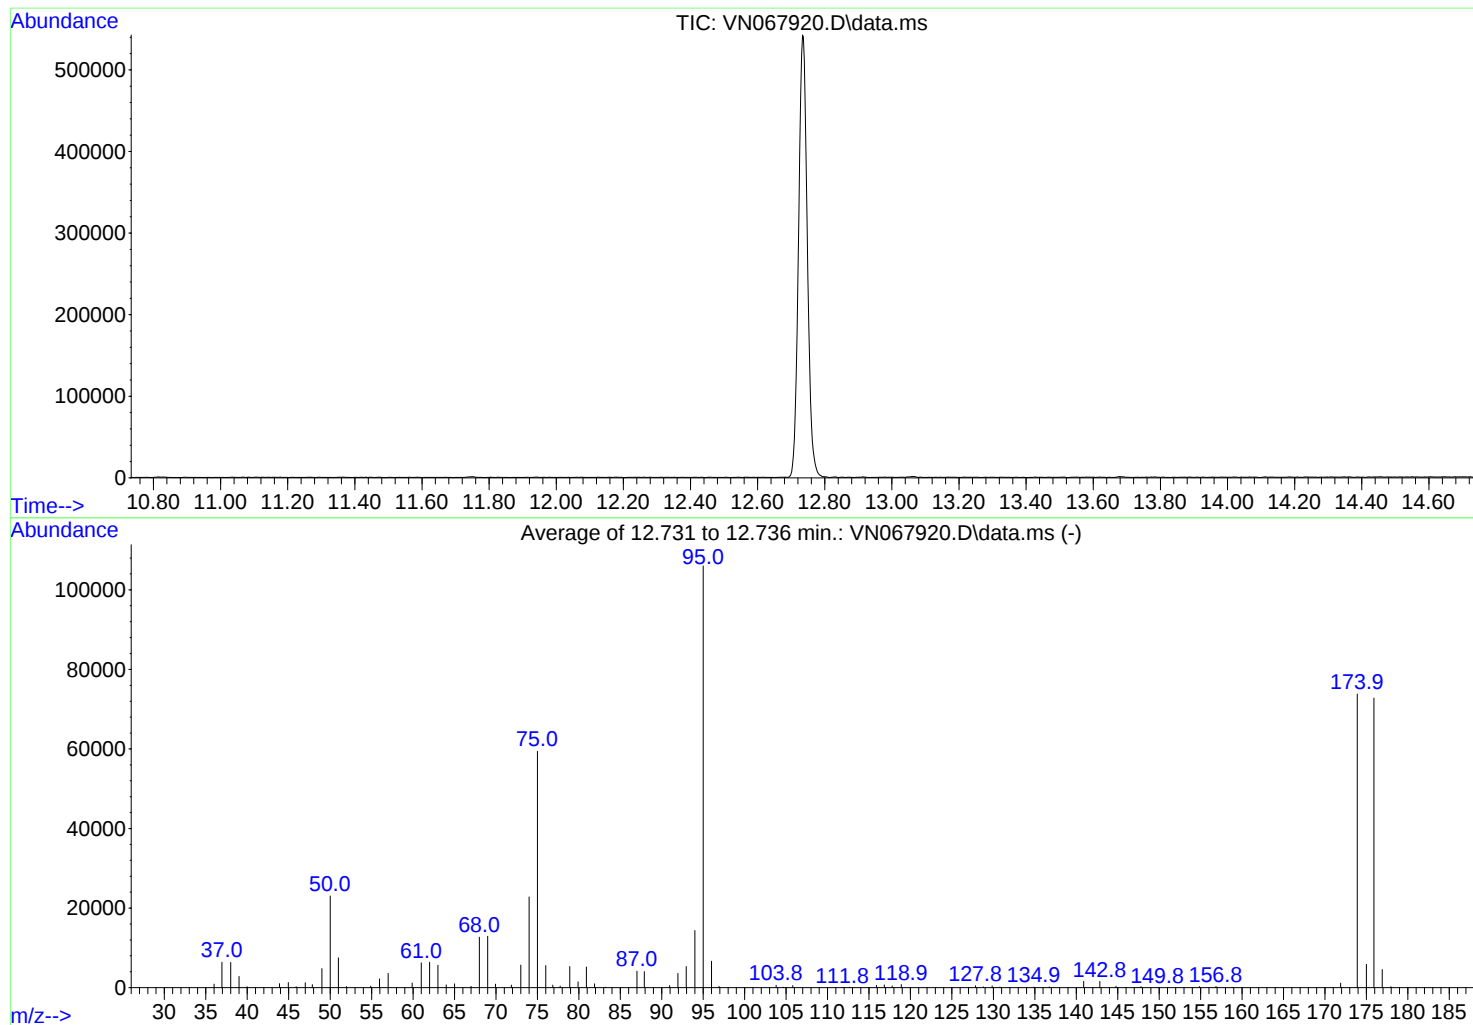

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	23069	PASS
75	95	30	60	56.0	59416	PASS
95	95	100	100	100.0	106037	PASS
96	95	5	9	6.3	6639	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.6	73813	PASS
175	174	5	9	8.0	5875	PASS
176	174	95	101	98.6	72792	PASS
177	176	5	9	6.2	4528	PASS