
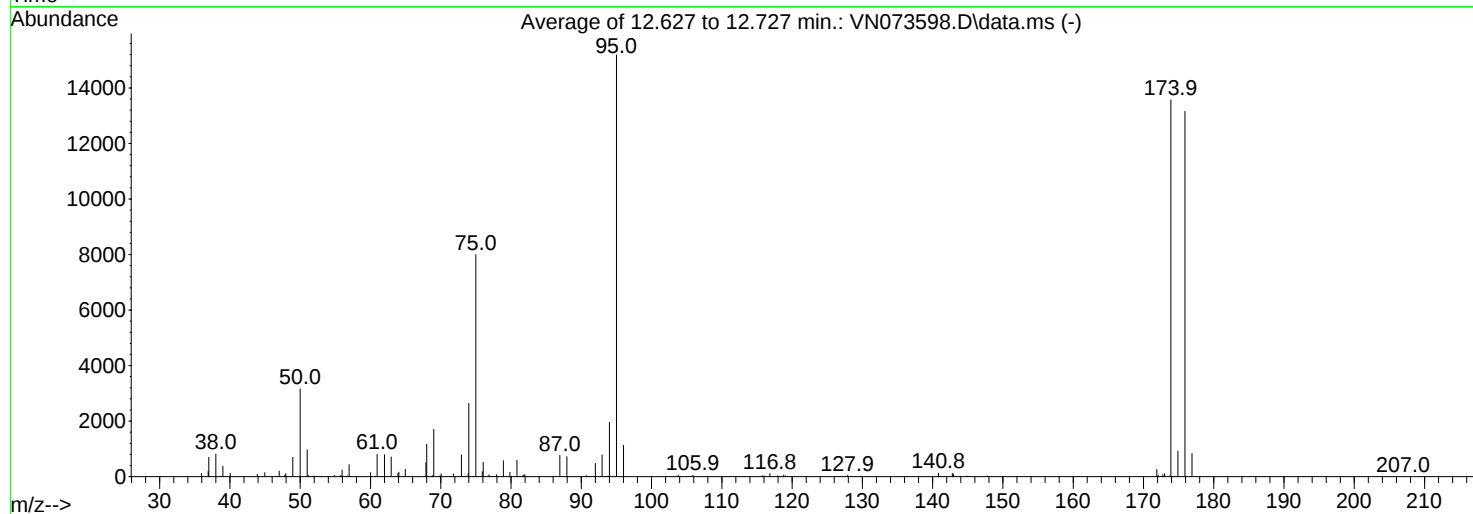


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072722\
Data File : VN073598.D
Acq On : 27 Jul 2022 10:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N072722W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Jul 27 18:07:26 2022

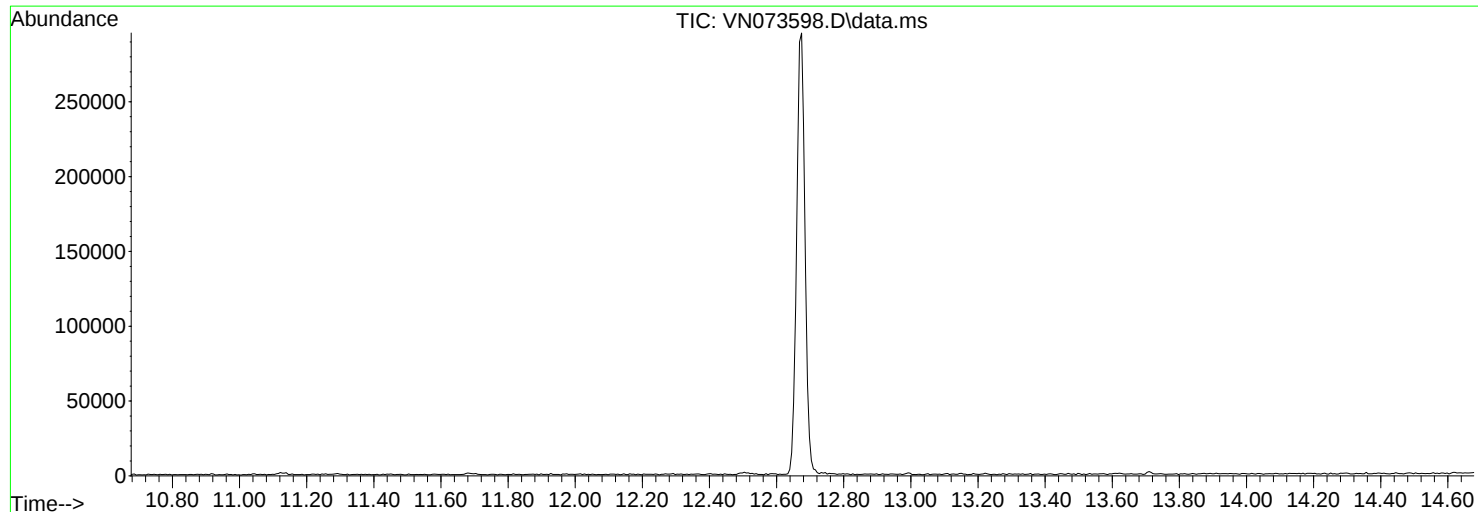

Spectrum Information: Average of 12.627 to 12.727 min.

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.8	3166	PASS
75	95	30	60	52.6	7992	PASS
95	95	100	100	100.0	15191	PASS
96	95	5	9	7.4	1128	PASS
173	174	0.00	2	0.8	109	PASS
174	95	50	100	89.4	13574	PASS
175	174	5	9	6.8	923	PASS
176	174	95	101	96.9	13157	PASS
177	176	5	9	6.4	837	PASS