

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072723\
 Data File : VN078672.D
 Acq On : 27 Jul 2023 20:11
 Operator : JC\MD
 Sample : 03770-08
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 28 01:12:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 10 16:13:53 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) Pentafluorobenzene	8.236	168	424229	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	780459	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	753343	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	296762	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	277542	48.801	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.600%
35) Dibromofluoromethane	8.177	113	276408	52.172	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.340%
50) Toluene-d8	10.577	98	955566	47.744	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	95.480%
62) 4-Bromofluorobenzene	12.853	95	327834	53.178	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	106.360%
Target Compounds						
					Qvalue	
3) Chloromethane	2.377	50	1996	0.353	ug/l #	74
5) Bromomethane	2.989	94	2244	Below Cal	#	45
6) Chloroethane	3.136	64	2703	Below Cal	#	43
11) Tert butyl alcohol	5.547	59	1094	1.247	ug/l #	72
13) Acrolein	4.200	56	555	0.643	ug/l #	16
16) Acetone	4.448	43	104122	58.774	ug/l	98
18) Methyl Acetate	5.048	43	5406	0.721	ug/l #	82
20) Methylene Chloride	5.295	84	22089	3.202	ug/l	93
25) 2-Butanone	7.500	43	57827	20.736	ug/l	91
29) Tetrahydrofuran	7.853	42	1563	0.854	ug/l #	50
31) Cyclohexane	8.224	56	9506	1.237	ug/l #	54
36) 1,1-Dichloropropene	8.230	75	34156	4.465	ug/l #	48
37) Ethyl Acetate	7.571	43	17694	2.775	ug/l #	89
38) Carbon Tetrachloride	8.241	117	42761	5.143	ug/l #	15
42) 1,2-Dichloroethane	8.688	62	1878	0.244	ug/l #	73
43) Isopropyl Acetate	8.700	43	467810	44.558	ug/l #	73
48) Methyl methacrylate	9.677	41	6968	1.433	ug/l #	30
49) 1,4-Dioxane	9.753	88	241	2.272	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	249719	39.988	ug/l	91
53) t-1,3-Dichloropropene	10.735	75	2065	0.249	ug/l #	1
54) cis-1,3-Dichloropropene	10.365	75	118336	13.381	ug/l #	72
57) 1,3-Dichloropropane	11.206	76	13912	1.478	ug/l #	43
59) 2-Hexanone	11.177	43	267457	60.261	ug/l #	19
71) Bromoform	12.853	173	2565	0.585	ug/l #	28
74) N-amyl acetate	12.600	43	3225	0.336	ug/l #	36
75) 1,1,2,2-Tetrachloroethane	12.941	83	149	Below Cal	#	27
76) 1,2,3-Trichloropropane	12.853	75	171621	23.926	ug/l #	1
77) Bromobenzene	12.982	156	99	Below Cal	#	1
81) trans-1,4-Dichloro-2-b...	12.853	75	171621	62.872	ug/l #	15
90) Hexachloroethane	14.341	117	215	Below Cal		82
92) 1,2-Dibromo-3-Chloropr...	14.700	75	62	Below Cal	#	4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072723\
Data File : VN078672.D
Acq On : 27 Jul 2023 20:11
Operator : JC\MD
Sample : 03770-08
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 28 01:12:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 10 16:13:53 2023
Response via : Initial Calibration

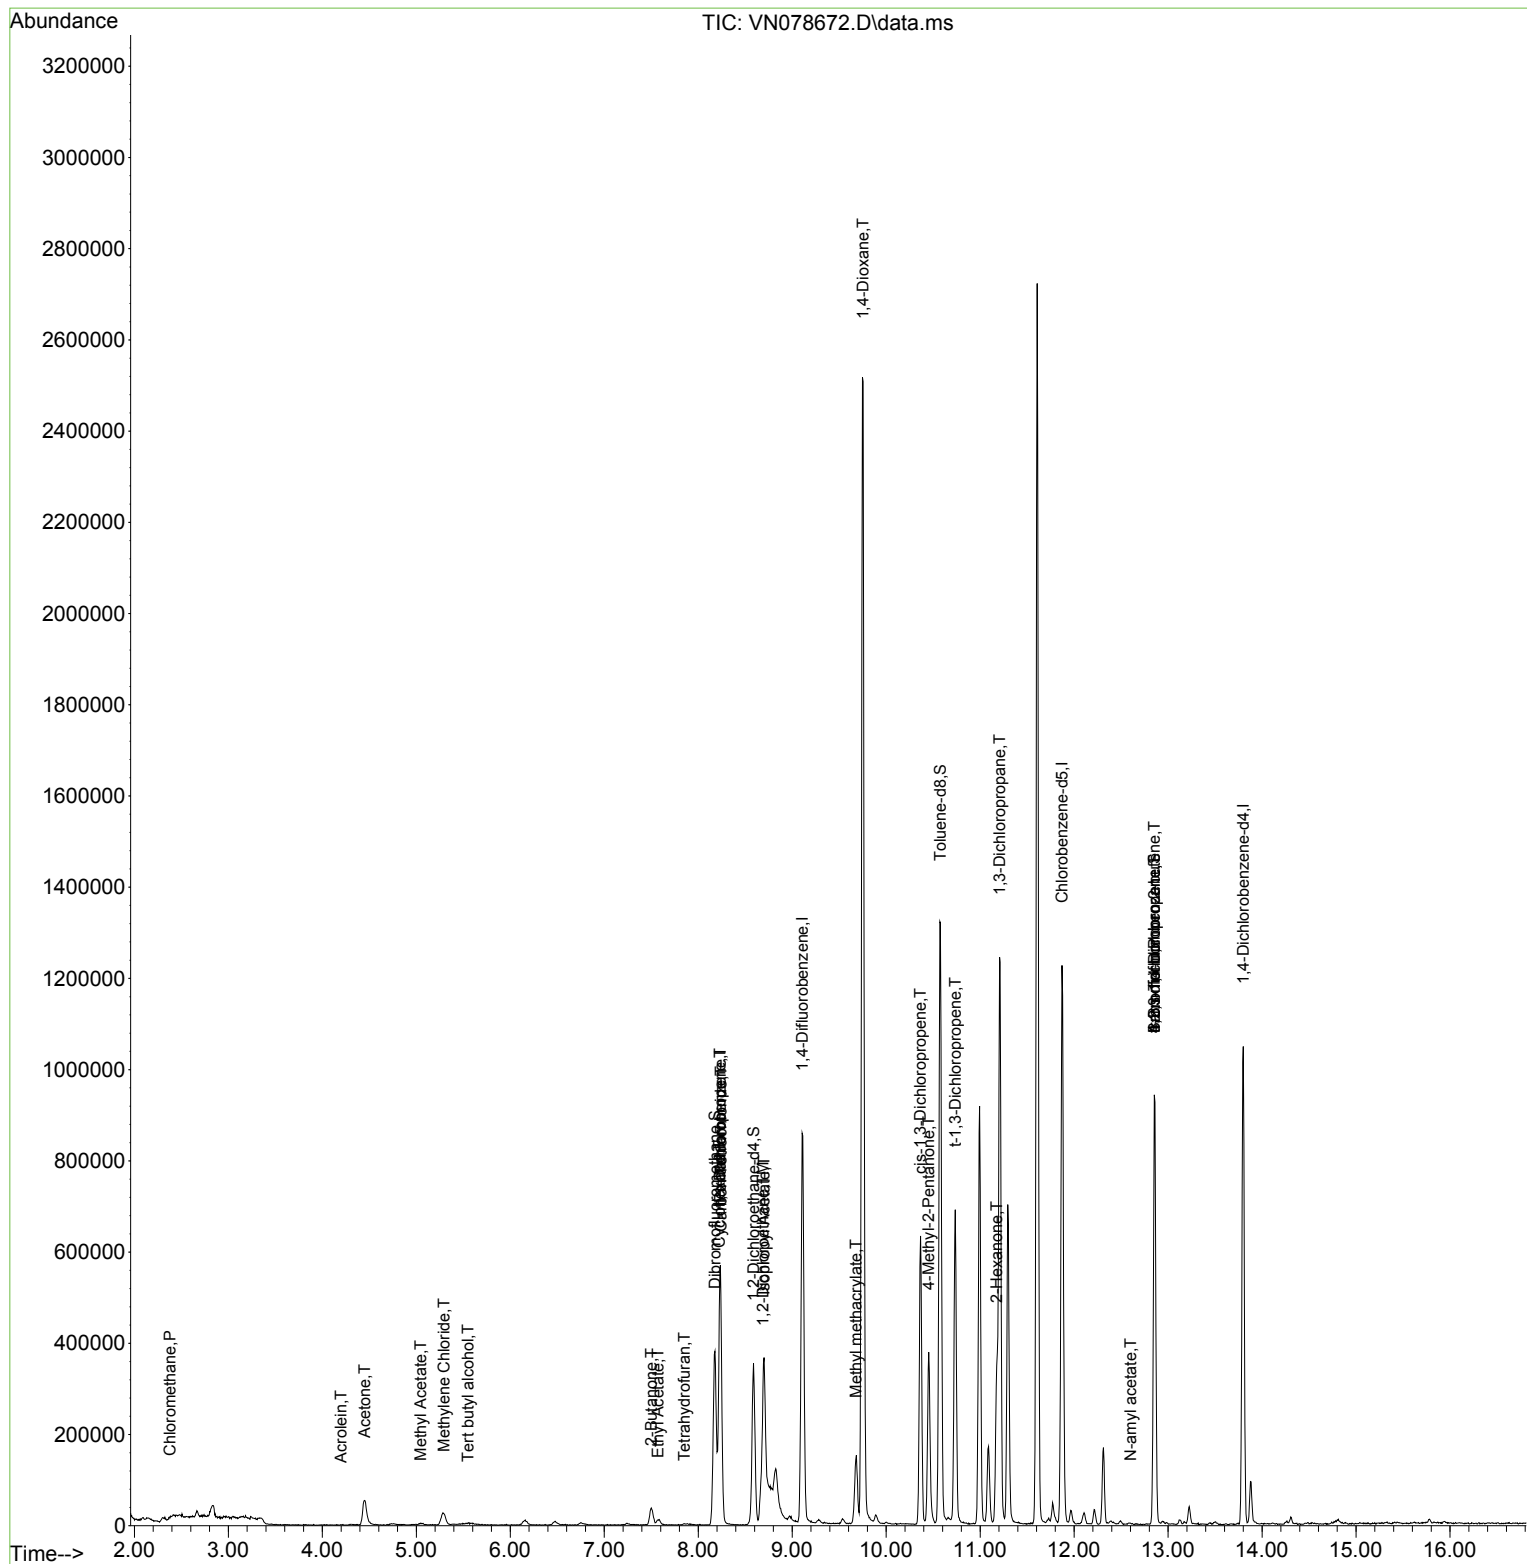



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.236 min Scan# 10

Delta R.T. 0.006 min

Lab File: VN078672.D

Acq: 27 Jul 2023 20:11

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:168 Resp: 424229

Ion Ratio Lower Upper

168 100

99 56.4 53.0 79.6

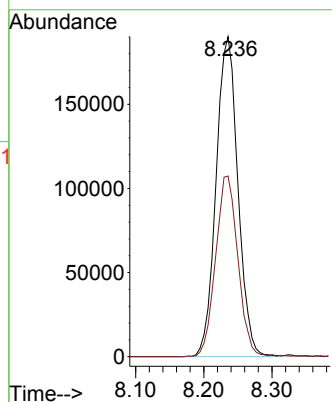

#3

Chloromethane

Concen: 0.353 ug/l

RT: 2.377 min Scan# 72

Delta R.T. 0.006 min

Lab File: VN078672.D




Acq: 27 Jul 2023 20:11


Tgt Ion: 50 Resp: 1996

Ion Ratio Lower Upper

50 100

52 18.6 26.5 39.7#


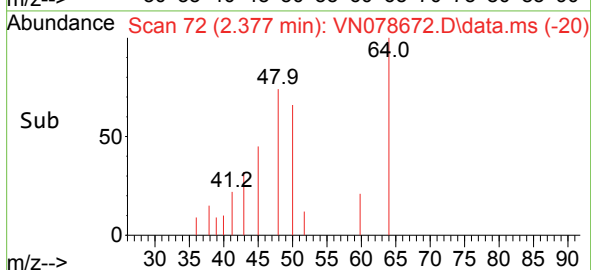






#5
Bromomethane
Concen: Below Cal
RT: 2.989 min Scan# 11
Delta R.T. 0.035 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 2244
Ion Ratio Lower Upper
94 100
96 39.1 73.1 109.7#

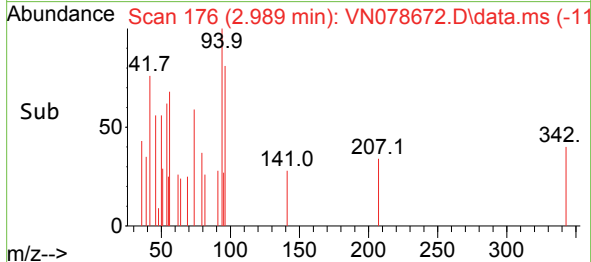

#6
Chloroethane
Concen: Below Cal
RT: 3.136 min Scan# 201
Delta R.T. 0.018 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Tgt Ion: 64 Resp: 2703
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#


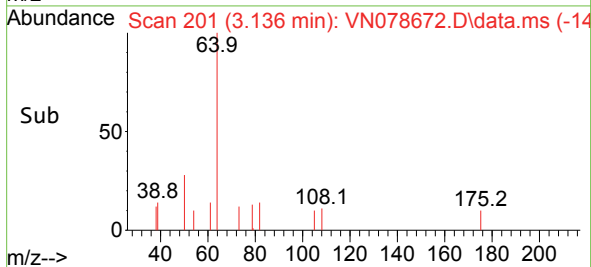

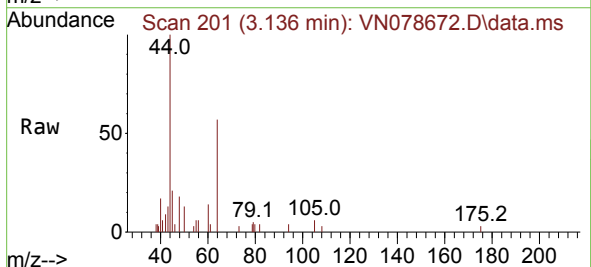




#11
Tert butyl alcohol
Concen: 1.247 ug/l
RT: 5.547 min Scan# 611
Delta R.T. 0.011 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 59 Resp: 1094
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

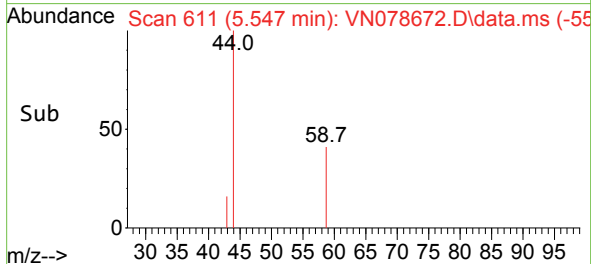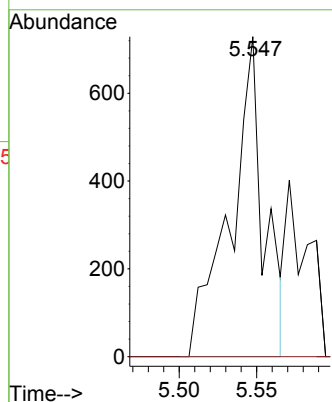

#13
Acrolein
Concen: 0.643 ug/l
RT: 4.200 min Scan# 382
Delta R.T. 0.011 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Tgt Ion: 56 Resp: 555
Ion Ratio Lower Upper
56 100
55 0.0 54.5 81.7#


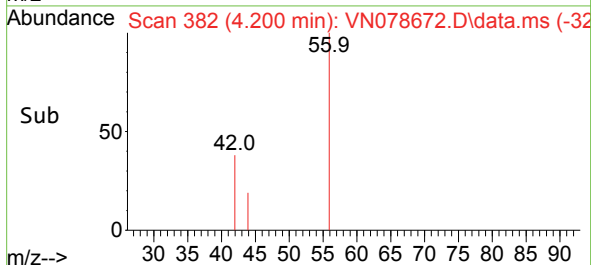

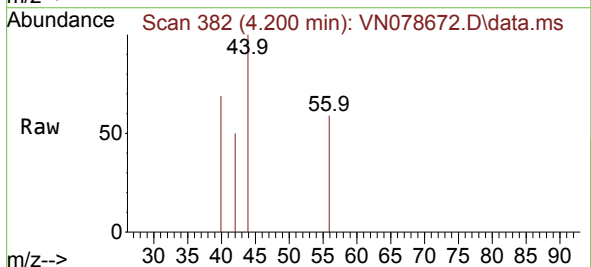




#16
Acetone
Concen: 58.774 ug/l
RT: 4.448 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 104122
Ion Ratio Lower Upper
43 100
58 33.8 28.0 42.0

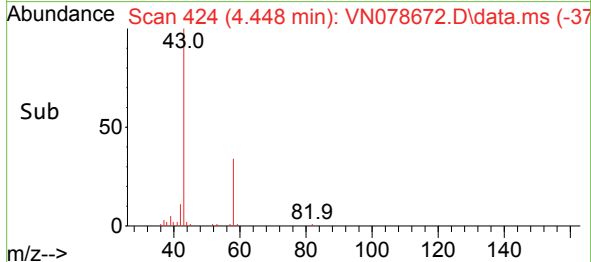

#18
Methyl Acetate
Concen: 0.721 ug/l
RT: 5.048 min Scan# 526
Delta R.T. 0.012 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11


Tgt Ion: 43 Resp: 5406
Ion Ratio Lower Upper
43 100
74 22.6 26.2 39.4#

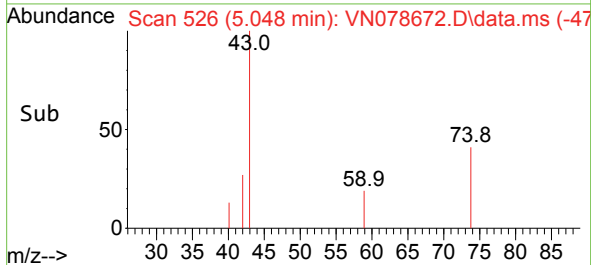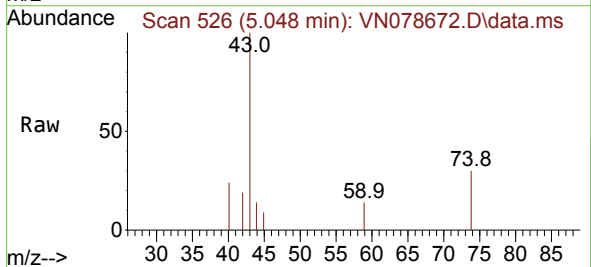






#20
Methylene Chloride
Concen: 3.202 ug/l
RT: 5.295 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:	84	Resp:	22089
Ion	Ratio	Lower	Upper
84	100		
49	102.5	79.7	119.5
51	32.5	25.2	37.8
86	53.9	53.3	79.9

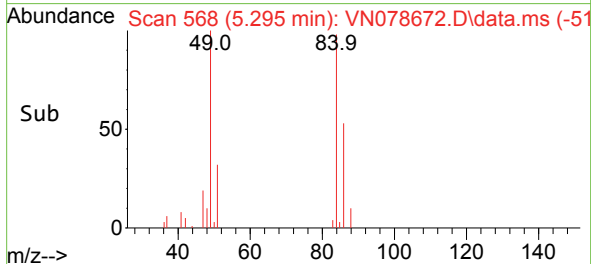

#25
2-Butanone
Concen: 20.736 ug/l
RT: 7.500 min Scan# 943
Delta R.T. 0.011 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Tgt Ion:	43	Resp:	57827
Ion	Ratio	Lower	Upper
43	100		
72	32.3	30.2	45.2

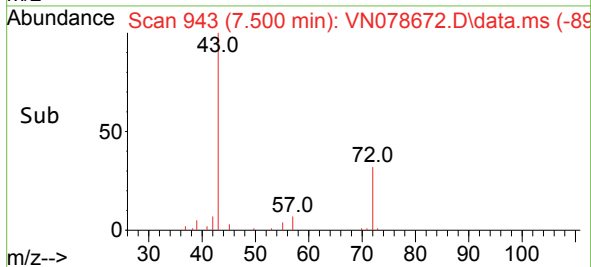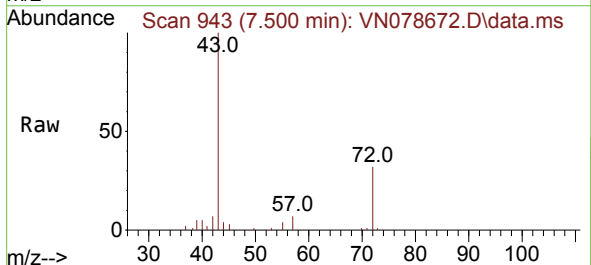



#29

Tetrahydrofuran

Concen: 0.854 ug/l

RT: 7.853 min Scan# 1003

Delta R.T. 0.006 min


Lab File: VN078672.D

Acq: 27 Jul 2023 20:11




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	42	Resp:	1563
Ion Ratio	Lower	Upper	
42	100		
72	28.5	49.8	74.6#
71	17.0	47.4	71.2#

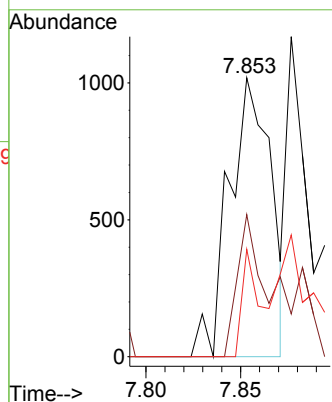

#31

Cyclohexane

Concen: 1.237 ug/l




RT: 8.224 min Scan# 1066


Delta R.T. -0.041 min

Lab File: VN078672.D

Acq: 27 Jul 2023 20:11

Tgt Ion:	56	Resp:	9506
Ion Ratio	Lower	Upper	
56	100		
69	135.1	26.8	40.2#
84	104.2	81.8	122.6

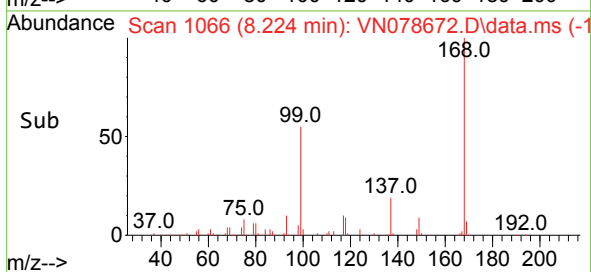



#33

1,2-Dichloroethane-d4

Concen: 48.801 ug/l

RT: 8.588 min Scan# 1127

Delta R.T. 0.005 min

Lab File: VN078672.D

Acq: 27 Jul 2023 20:11

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 277542

Ion Ratio Lower Upper

65 100

67 52.2 0.0 106.6

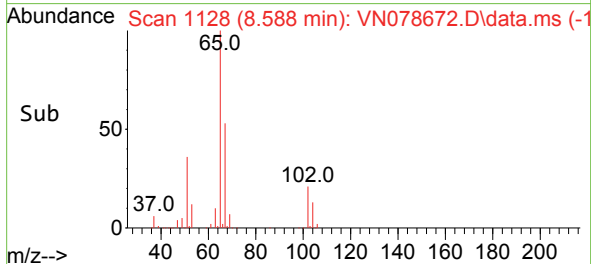

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.000 min

Lab File: VN078672.D

Acq: 27 Jul 2023 20:11




Tgt Ion: 114 Resp: 780459


Ion Ratio Lower Upper

114 100

63 17.7 0.0 36.4


88 14.0 0.0 30.6

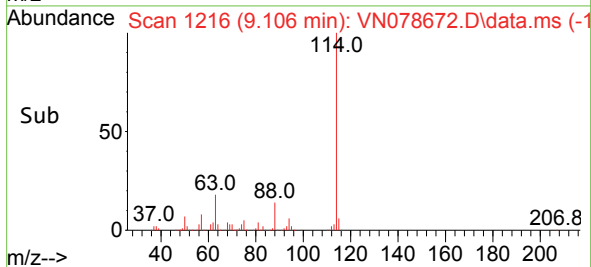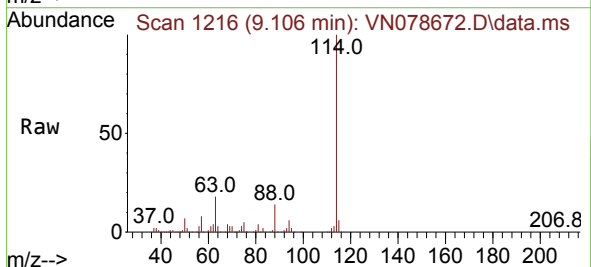






#35
Dibromofluoromethane
Concen: 52.172 ug/l
RT: 8.177 min Scan# 1058
Delta R.T. -0.000 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:113 Resp: 276408
Ion Ratio Lower Upper
113 100
111 103.4 82.6 123.8
192 18.0 12.7 19.1

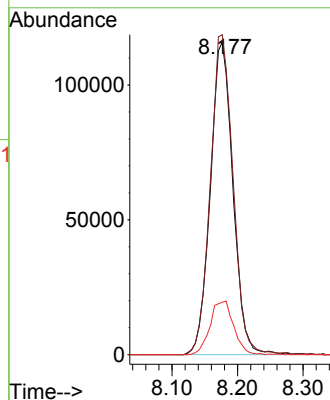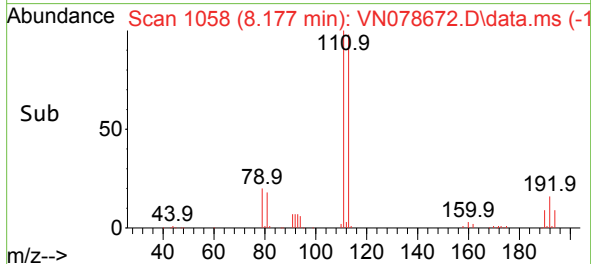

#36
1,1-Dichloropropene
Concen: 4.465 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Tgt Ion: 75 Resp: 34156
Ion Ratio Lower Upper
75 100
110 9.3 19.1 57.3#
77 0.0 25.0 37.4#

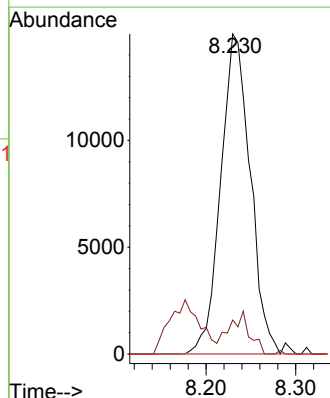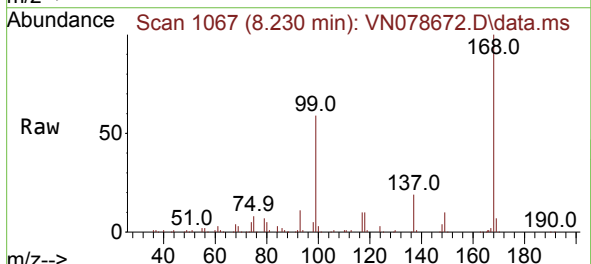



#37

Ethyl Acetate

Concen: 2.775 ug/l

RT: 7.571 min Scan# 91

Delta R.T. -0.000 min


Lab File: VN078672.D

Acq: 27 Jul 2023 20:11




Instrument :

MSVOA_N

ClientSampleId :

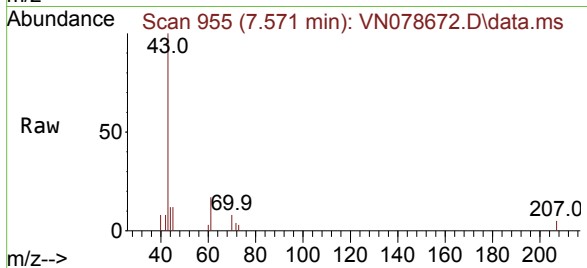

Tgt Ion:	43	Resp:	17694
Ion	Ratio	Lower	Upper
43	100		
61	15.2	13.2	19.8
70	6.0	11.3	16.9

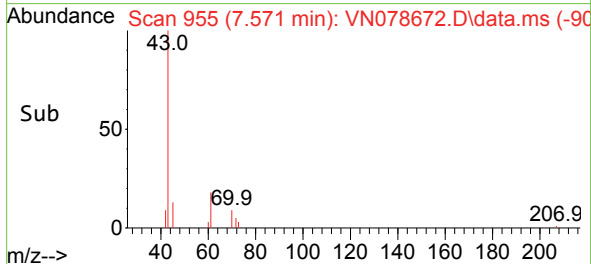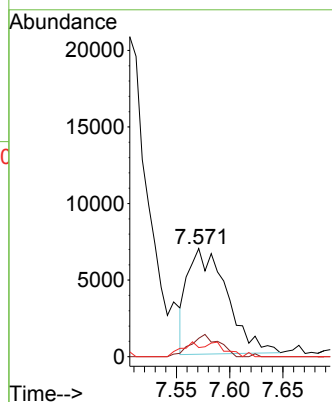

#38

Carbon Tetrachloride

Concen: 5.143 ug/l




RT: 8.241 min Scan# 1069


Delta R.T. -0.124 min

Lab File: VN078672.D

Acq: 27 Jul 2023 20:11

Tgt Ion:	117	Resp:	42761
Ion	Ratio	Lower	Upper
117	100		
119	4.0	77.3	115.9
121	0.0	23.3	34.9

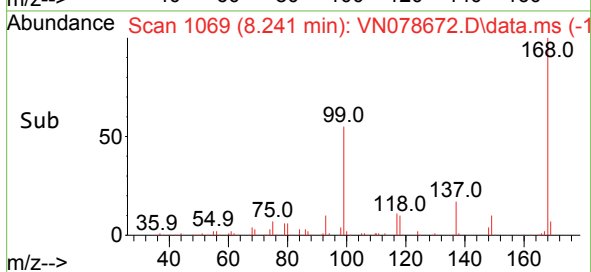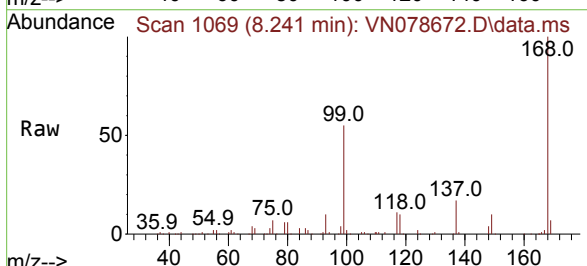



#42

1,2-Dichloroethane

Concen: 0.244 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.011 min

Lab File: VN078672.D

Acq: 27 Jul 2023 20:11

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 1878

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.8

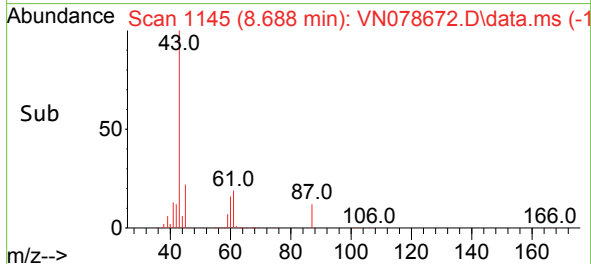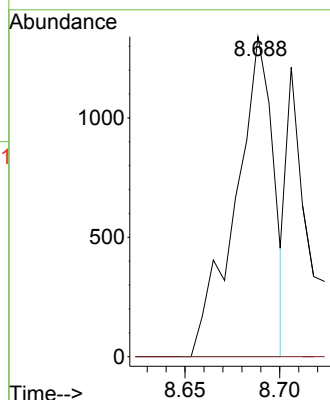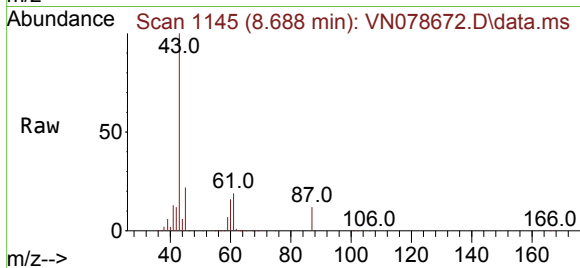

#43

Isopropyl Acetate

Concen: 44.558 ug/l

RT: 8.700 min Scan# 1147

Delta R.T. 0.006 min

Lab File: VN078672.D

Acq: 27 Jul 2023 20:11




Tgt Ion: 43 Resp: 467810


Ion Ratio Lower Upper

43 100

61 13.6 24.7 37.1#

87 9.8 14.6 21.8#


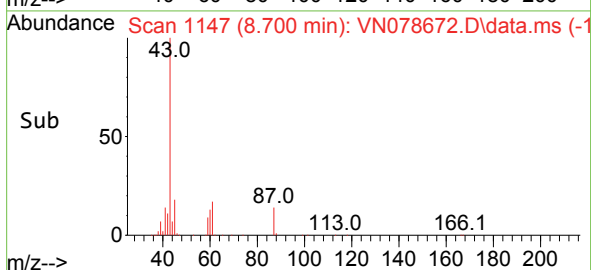
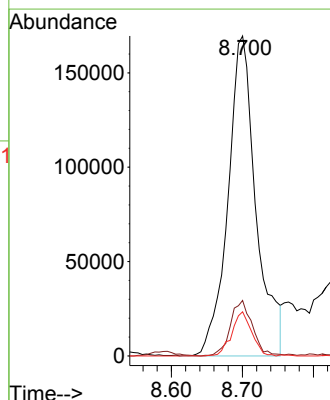
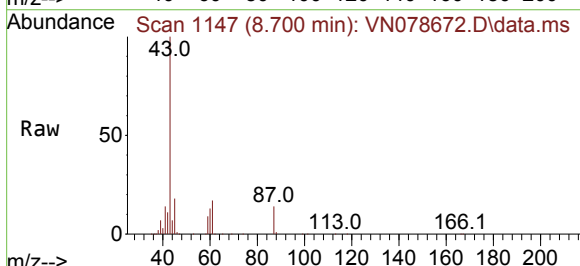




#48
Methyl methacrylate
Concen: 1.433 ug/l
RT: 9.677 min Scan# 11
Delta R.T. -0.011 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 41 Resp: 6968
Ion Ratio Lower Upper
41 100
69 0.8 90.4 135.6#
39 77.8 54.6 81.8

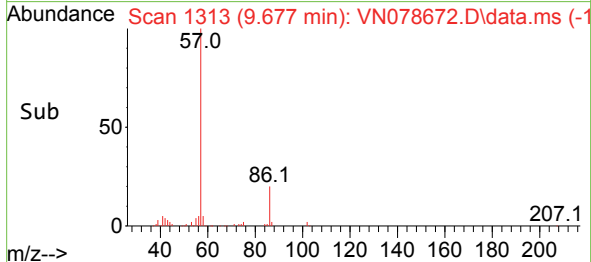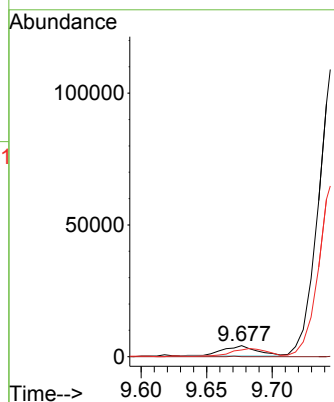

#49
1,4-Dioxane
Concen: 2.272 ug/l
RT: 9.753 min Scan# 1326
Delta R.T. 0.053 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Tgt Ion: 88 Resp: 241
Ion Ratio Lower Upper
88 100
43 990676.8 17.0 25.6#
58 5430.7 47.0 70.4#


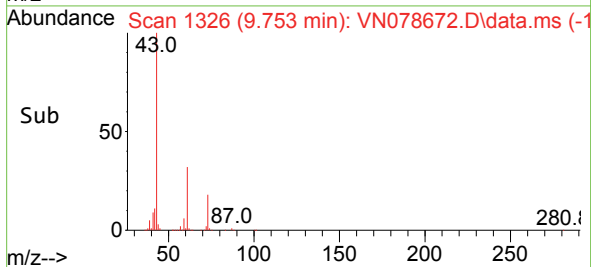
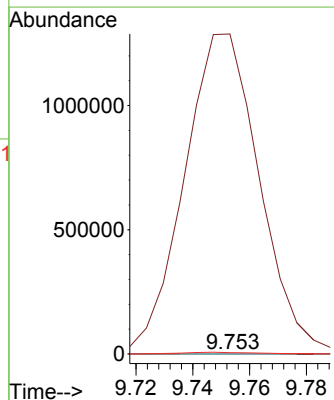
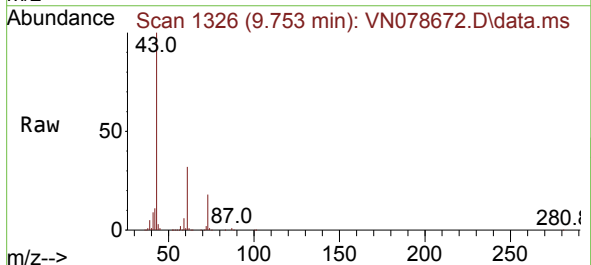




#50
Toluene-d8
Concen: 47.744 ug/l
RT: 10.577 min Scan# 1466
Delta R.T. 0.006 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 955566
Ion Ratio Lower Upper
98 100
100 63.5 52.0 78.0

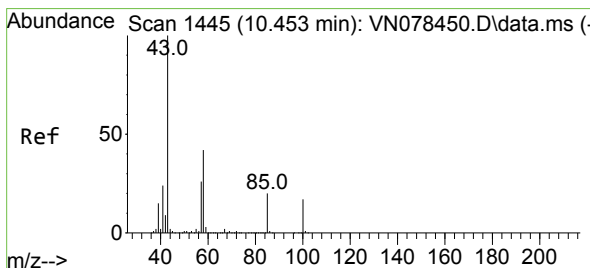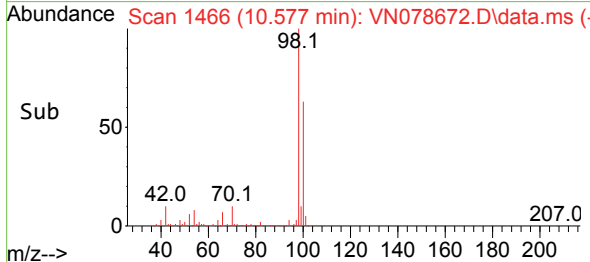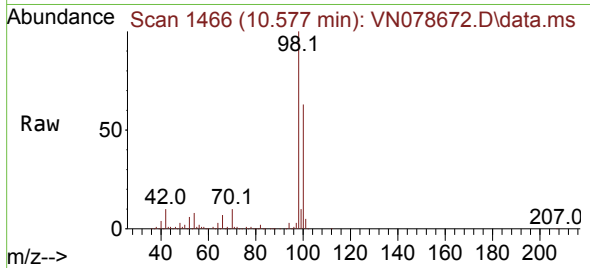

#51
4-Methyl-2-Pentanone
Concen: 39.988 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. 0.000 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Tgt Ion: 43 Resp: 249719
Ion Ratio Lower Upper
43 100
58 40.0 36.6 54.8


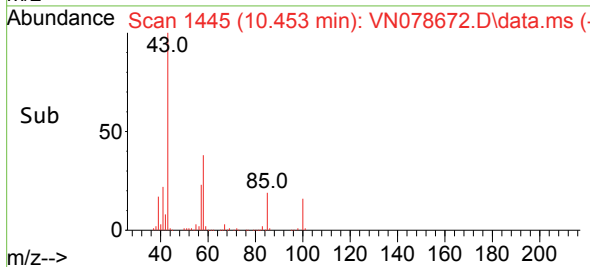

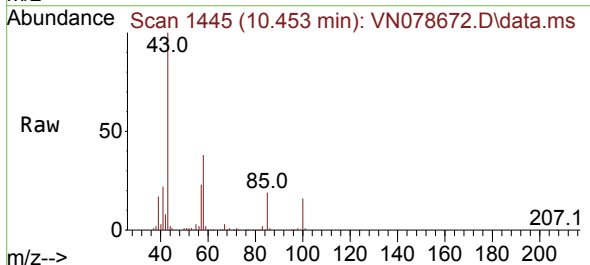




#53
 t-1,3-Dichloropropene
 Concen: 0.249 ug/l
 RT: 10.735 min Scan# 14
 Delta R.T. -0.106 min
 Lab File: VN078672.D
 Acq: 27 Jul 2023 20:11




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 2065
 Ion Ratio Lower Upper
 75 100
 77 90.7 25.4 38.0#

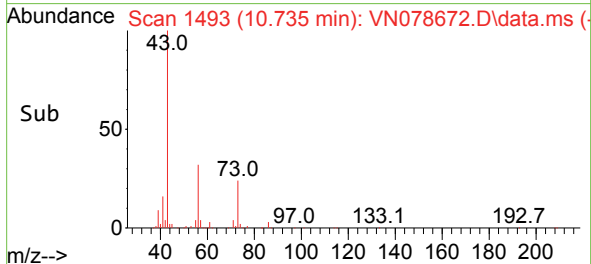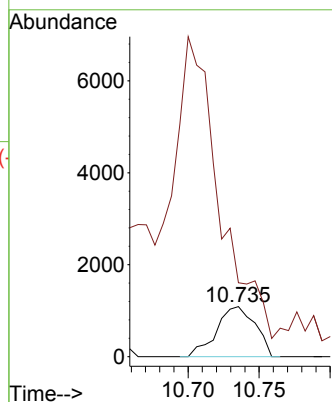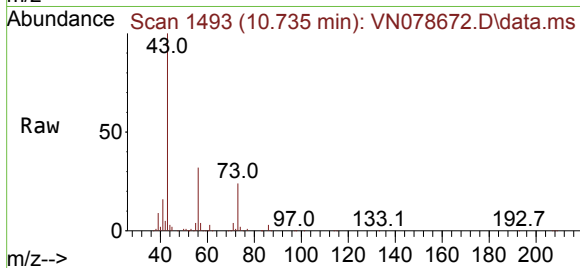

#54
 cis-1,3-Dichloropropene
 Concen: 13.381 ug/l
 RT: 10.365 min Scan# 1430
 Delta R.T. 0.047 min
 Lab File: VN078672.D
 Acq: 27 Jul 2023 20:11

Tgt Ion: 75 Resp: 118336
 Ion Ratio Lower Upper
 75 100
 77 1.6 26.1 39.1#
 39 35.5 31.6 47.4

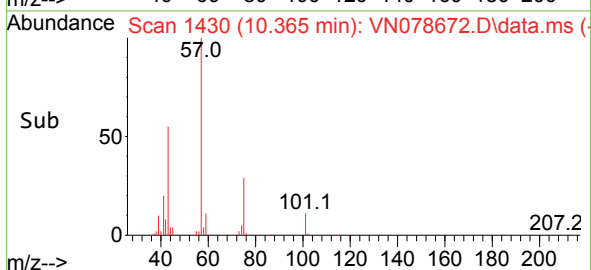



#57

1,3-Dichloropropane

Concen: 1.478 ug/l

RT: 11.206 min Scan# 11

Delta R.T. 0.035 min

Lab File: VN078672.D

Acq: 27 Jul 2023 20:11

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 76 Resp: 13912

Ion Ratio Lower Upper

76 100

78 0.4 26.1 39.1#

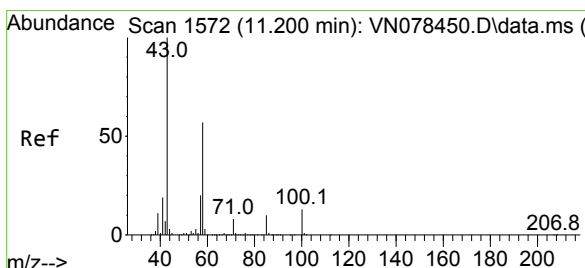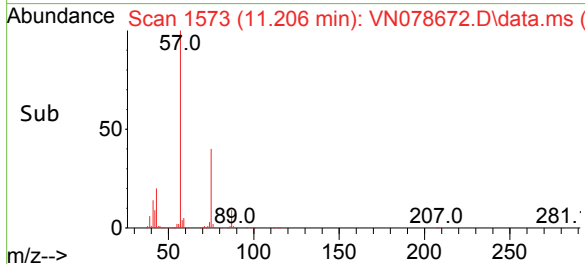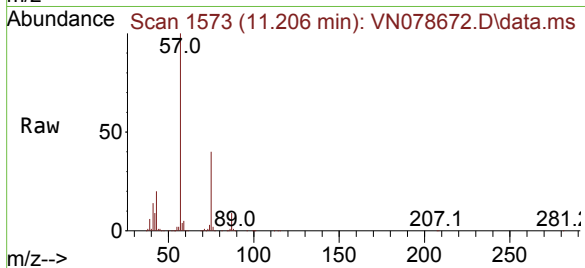

#59

2-Hexanone

Concen: 60.261 ug/l

RT: 11.177 min Scan# 1568

Delta R.T. -0.023 min

Lab File: VN078672.D




Acq: 27 Jul 2023 20:11


Tgt Ion: 43 Resp: 267457

Ion Ratio Lower Upper

43 100

58 0.0 31.7 95.1#


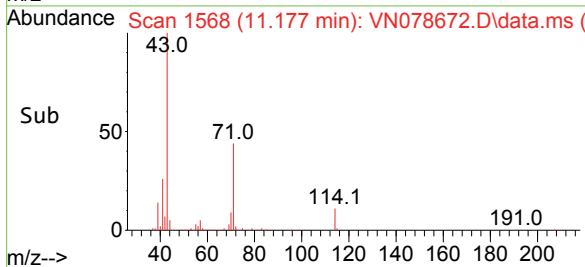

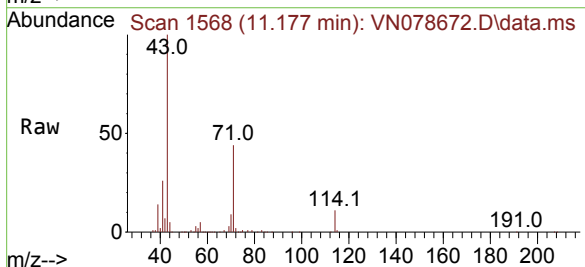




#62
4-Bromofluorobenzene
Concen: 53.178 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 327834
Ion Ratio Lower Upper
95 100
174 82.1 0.0 143.8
176 79.2 0.0 135.8

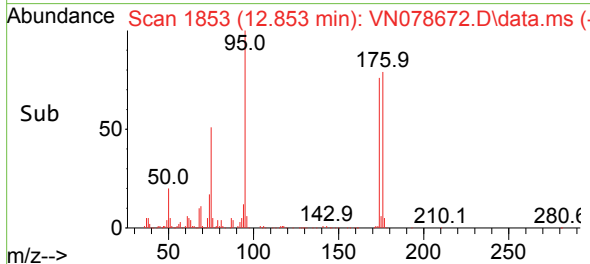

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11


Tgt Ion: 117 Resp: 753343
Ion Ratio Lower Upper
117 100
82 52.0 44.0 66.0
119 33.4 25.6 38.4

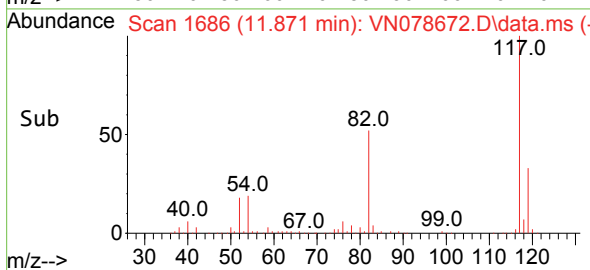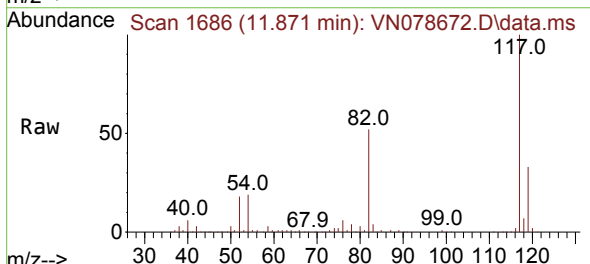






#71
Bromoform
Concen: 0.585 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.271 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Instrument :
MSVOA_N
ClientSampleId :



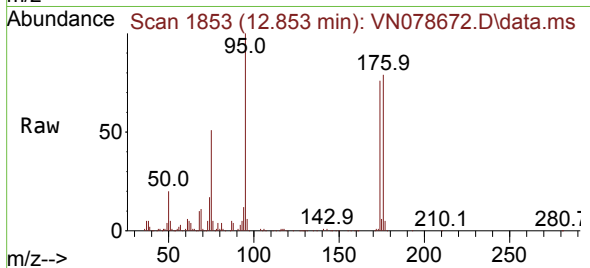



Tgt Ion:173 Resp: 2565
Ion Ratio Lower Upper
173 100
175 0.0 24.3 73.0#
254 0.0 0.0 0.0

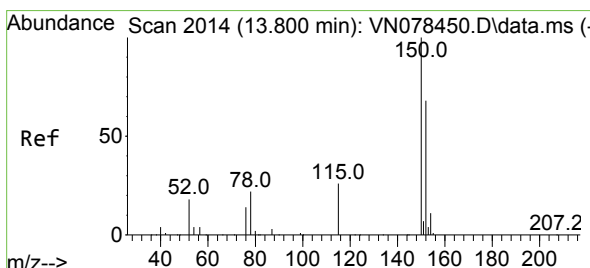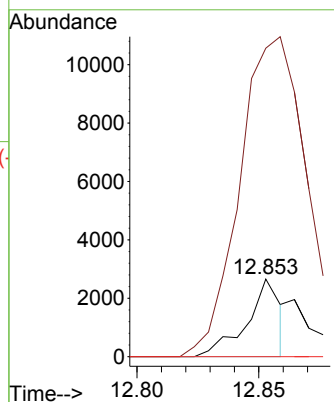

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11


Tgt Ion:152 Resp: 296762
Ion Ratio Lower Upper
152 100
115 58.3 32.3 96.8
150 155.5 0.0 355.8

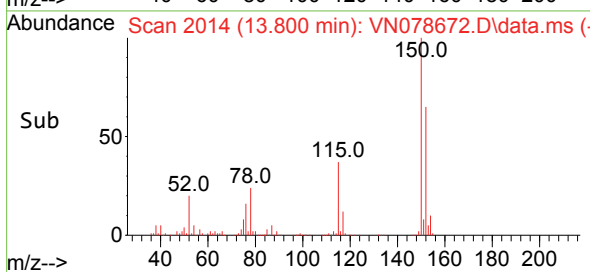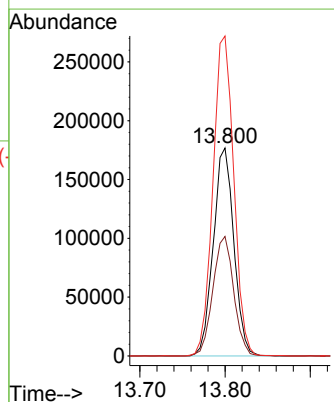



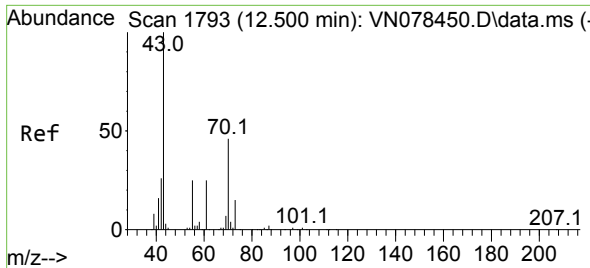


#74
N-amy1 acetate
Concen: 0.336 ug/l
RT: 12.600 min Scan# 1810
Delta R.T. 0.100 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Instrument :
MSVOA_N
ClientSampleId :



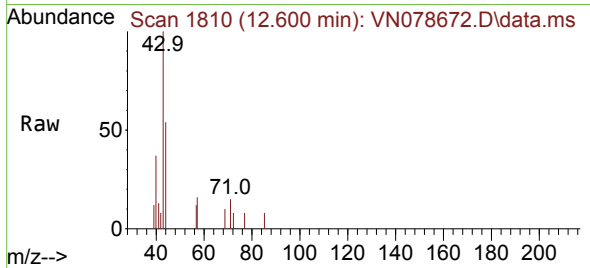



Tgt Ion: 43 Resp: 3225
Ion Ratio Lower Upper
43 100
70 0.0 43.4 65.2#
55 0.0 21.4 32.0#
61 0.0 22.8 34.2#

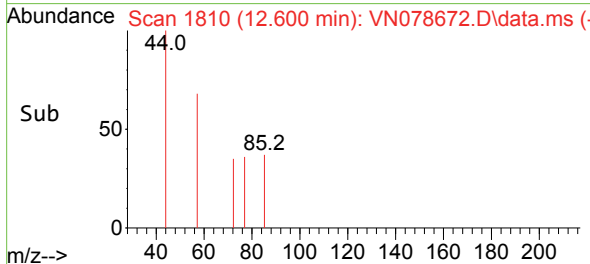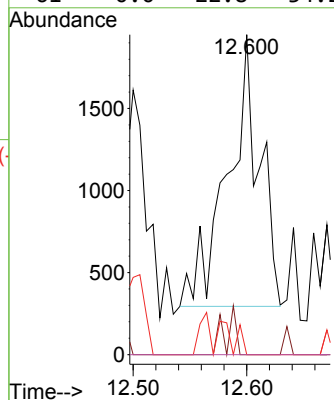

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.941 min Scan# 1868
Delta R.T. 0.000 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Tgt Ion: 83 Resp: 149
Ion Ratio Lower Upper
83 100
131 0.0 5.0 15.0#
85 126.2 31.9 95.7#


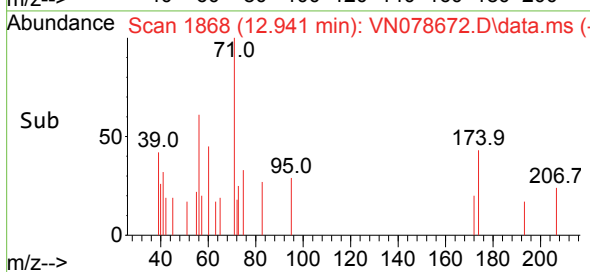
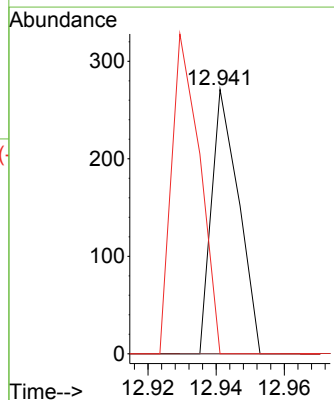





#76
1,2,3-Trichloropropane
Concen: 23.926 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 171621
Ion Ratio Lower Upper
75 100
77 1.5 84.5 253.5#

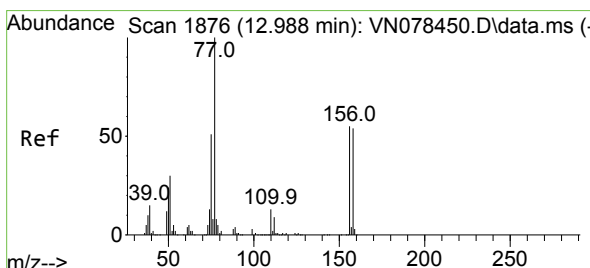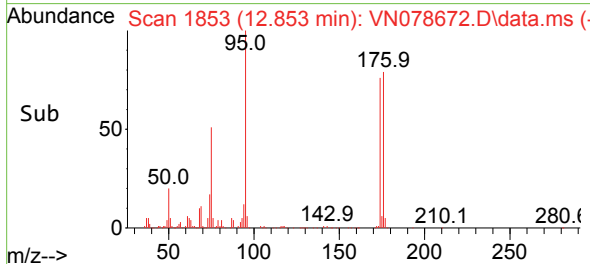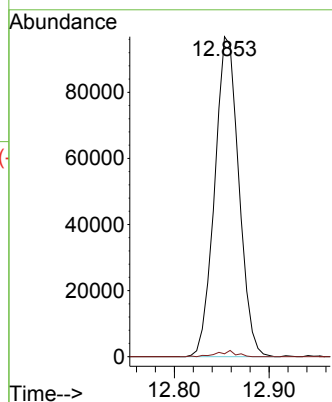

#77
Bromobenzene
Concen: Below Cal
RT: 12.982 min Scan# 1875
Delta R.T. -0.006 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11

Tgt Ion:156 Resp: 99
Ion Ratio Lower Upper
156 100
77 641.4 107.7 323.3#
158 82.8 48.4 145.3


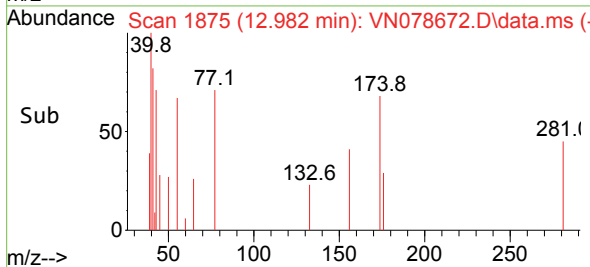

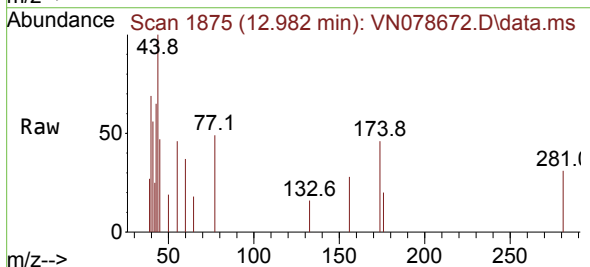


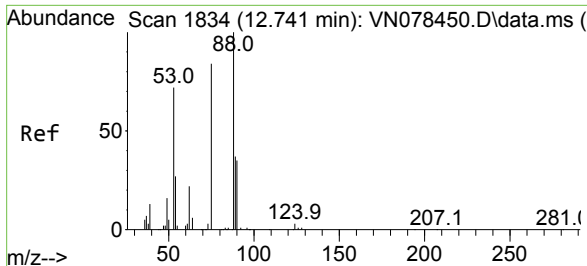

#81
trans-1,4-Dichloro-2-butene
Concen: 62.872 ug/l
RT: 12.853 min Scan# 11
Delta R.T. 0.112 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 171621
Ion Ratio Lower Upper
75 100
53 0.2 67.4 101.2#
89 0.0 38.8 58.2#

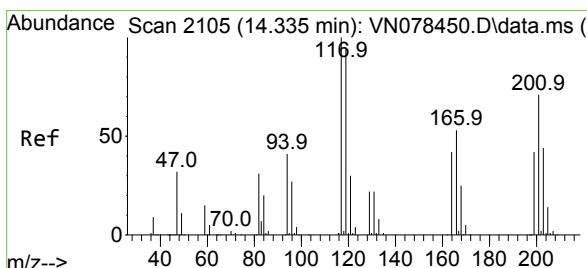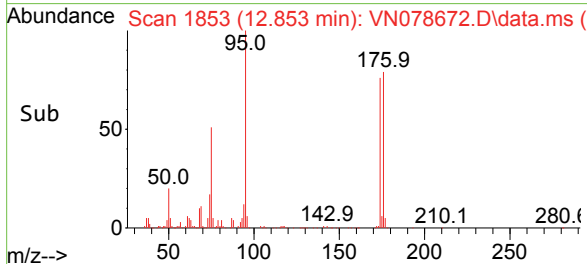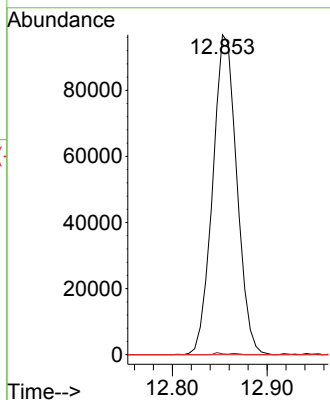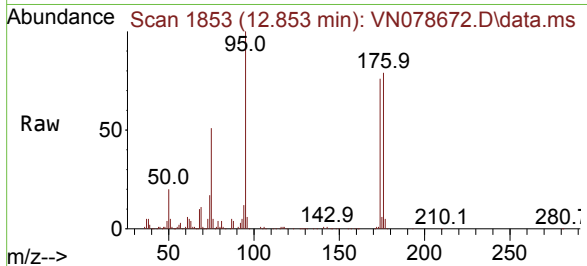

#90
Hexachloroethane
Concen: Below Cal
RT: 14.341 min Scan# 2106
Delta R.T. 0.006 min
Lab File: VN078672.D
Acq: 27 Jul 2023 20:11


Tgt Ion: 117 Resp: 215
Ion Ratio Lower Upper
117 100
201 72.1 29.3 88.0

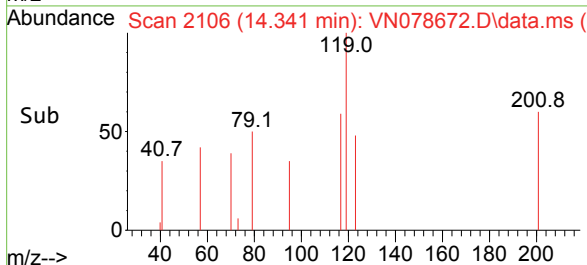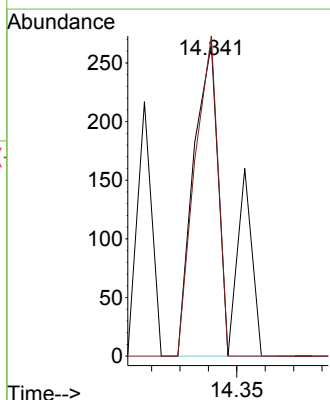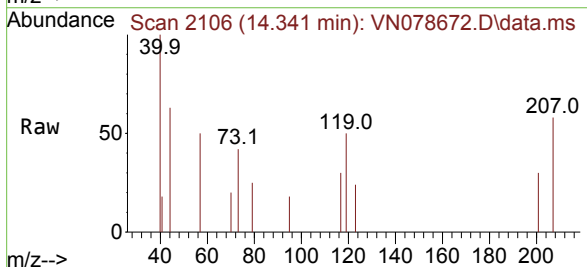

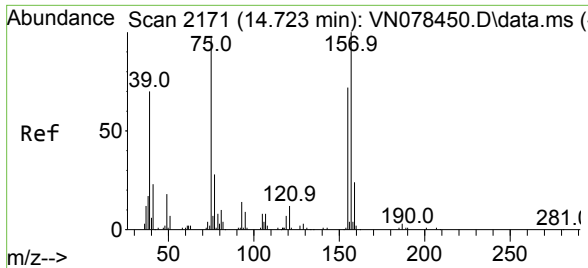

#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 14.700 min Scan# 21
 Delta R.T. -0.023 min
 Lab File: VN078672.D
 Acq: 27 Jul 2023 20:11

Instrument :
 MSVOA_N
 ClientSampleId :

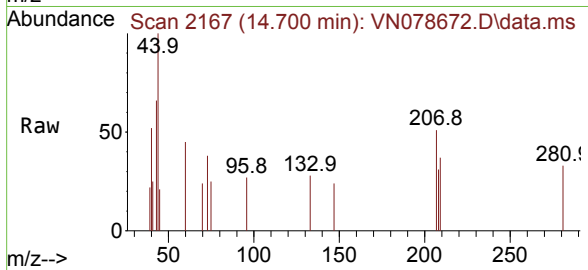

Tgt Ion:	75	Resp:	62
Ion	Ratio	Lower	Upper
75	100		
155	0.0	39.1	117.2#
157	0.0	50.3	150.9#

