
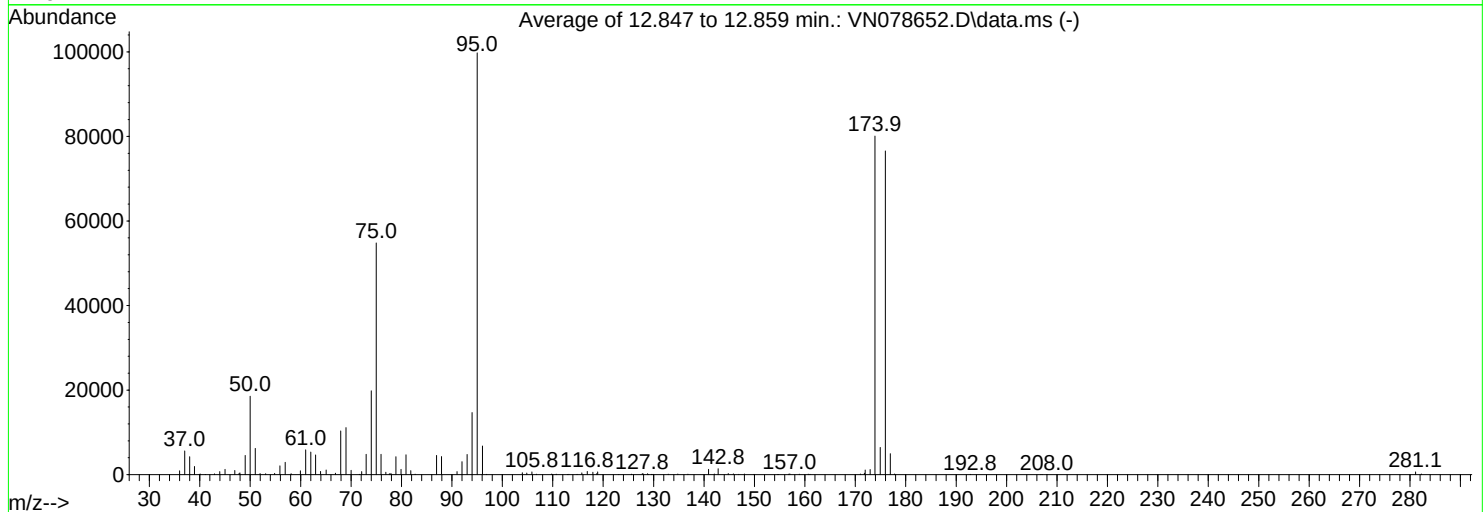


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072723\
Data File : VN078652.D
Acq On : 27 Jul 2023 09:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

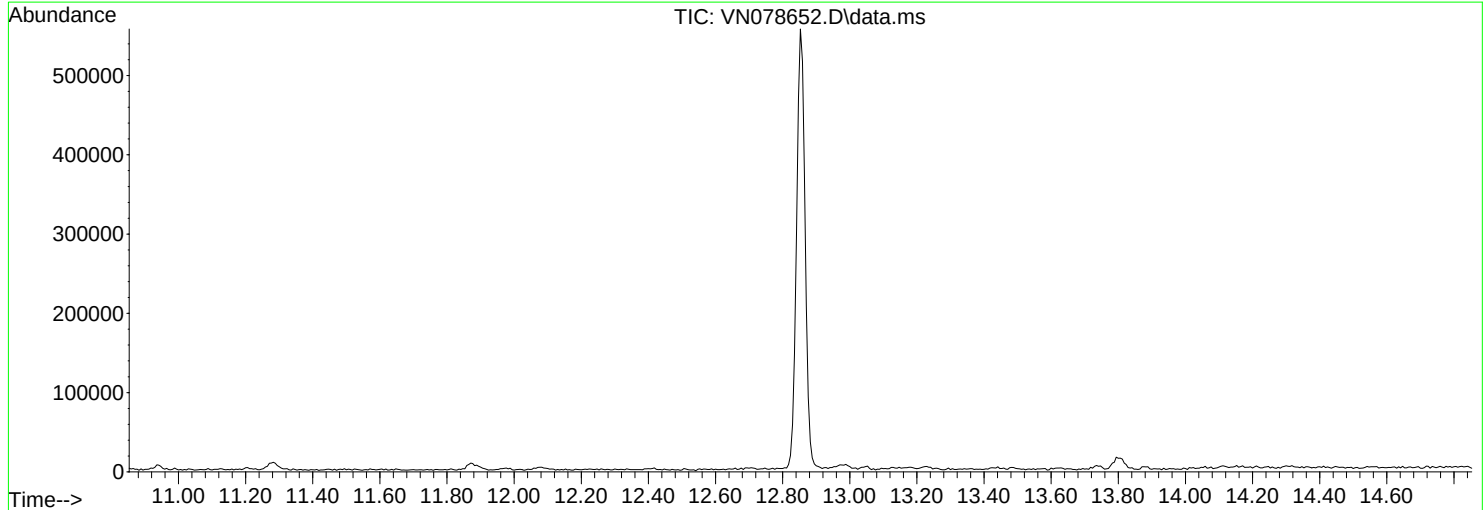

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	18536	PASS
75	95	30	60	54.9	54789	PASS
95	95	100	100	100.0	99771	PASS
96	95	5	9	6.8	6781	PASS
173	174	0.00	2	1.5	1215	PASS
174	95	50	100	80.3	80096	PASS
175	174	5	9	8.0	6425	PASS
176	174	95	101	95.6	76576	PASS
177	176	5	9	6.5	4970	PASS

Average of 12.847 to 12.859 min.: VN078652.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	898	47.80	323	59.95	906	72.10	711
37.00	5591	47.95	405	61.00	5865	73.00	479
38.00	4234	49.00	4554	62.00	5337	74.00	1982
38.95	1919	50.00	18536	62.95	4640	75.00	5478
39.90	74	51.00	6219	63.95	769	75.95	4819
40.10	169	51.95	286	65.05	1114	76.90	581
41.10	54	53.05	232	66.90	329	77.60	241
42.90	190	54.85	295	67.95	10324	77.90	307
43.95	716	55.90	2064	69.00	11127	78.90	4250
45.00	1265	56.95	2915	70.00	1036	79.90	1270
46.95	996	58.10	230	71.70	90	80.90	4699

Average of 12.847 to 12.859 min.: VN078652.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	948	103.95	456	117.95	566	132.90	96
82.70	96	104.85	366	118.70	243	134.80	150
86.95	4551	105.85	648	118.90	642	136.80	100
87.95	4285	106.75	119	123.10	53	140.90	1247
91.00	736	109.80	162	125.60	114	142.05	169
92.00	3061	110.70	133	127.75	268	142.80	1413
93.00	4756	112.90	59	128.00	169	144.80	254
94.00	14669	113.20	84	128.80	219	145.80	184
95.00	99771	114.80	63	129.00	52	146.90	60
96.05	6781	115.75	437	129.60	74	148.00	168
96.90	85	116.85	745	129.90	78	149.90	72

Average of 12.847 to 12.859 min.: VN078652.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.60	52	173.90	80096				
154.80	51	174.95	6425				
156.80	98	175.95	76576				
157.00	174	176.95	4970				
158.90	100	177.80	146				
160.65	129	192.80	62				
161.00	81	206.80	50				
171.00	156	207.05	30				
171.80	348	208.00	54				
171.95	1113	281.10	653				
172.95	1215	282.25	161				