


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072820\
 Data File : VN062625.D
 Acq On : 28 Jul 2020 8:56
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072120W.M
 Title : SW846 8260
 Last Update : Tue Jul 21 18:48:59 2020

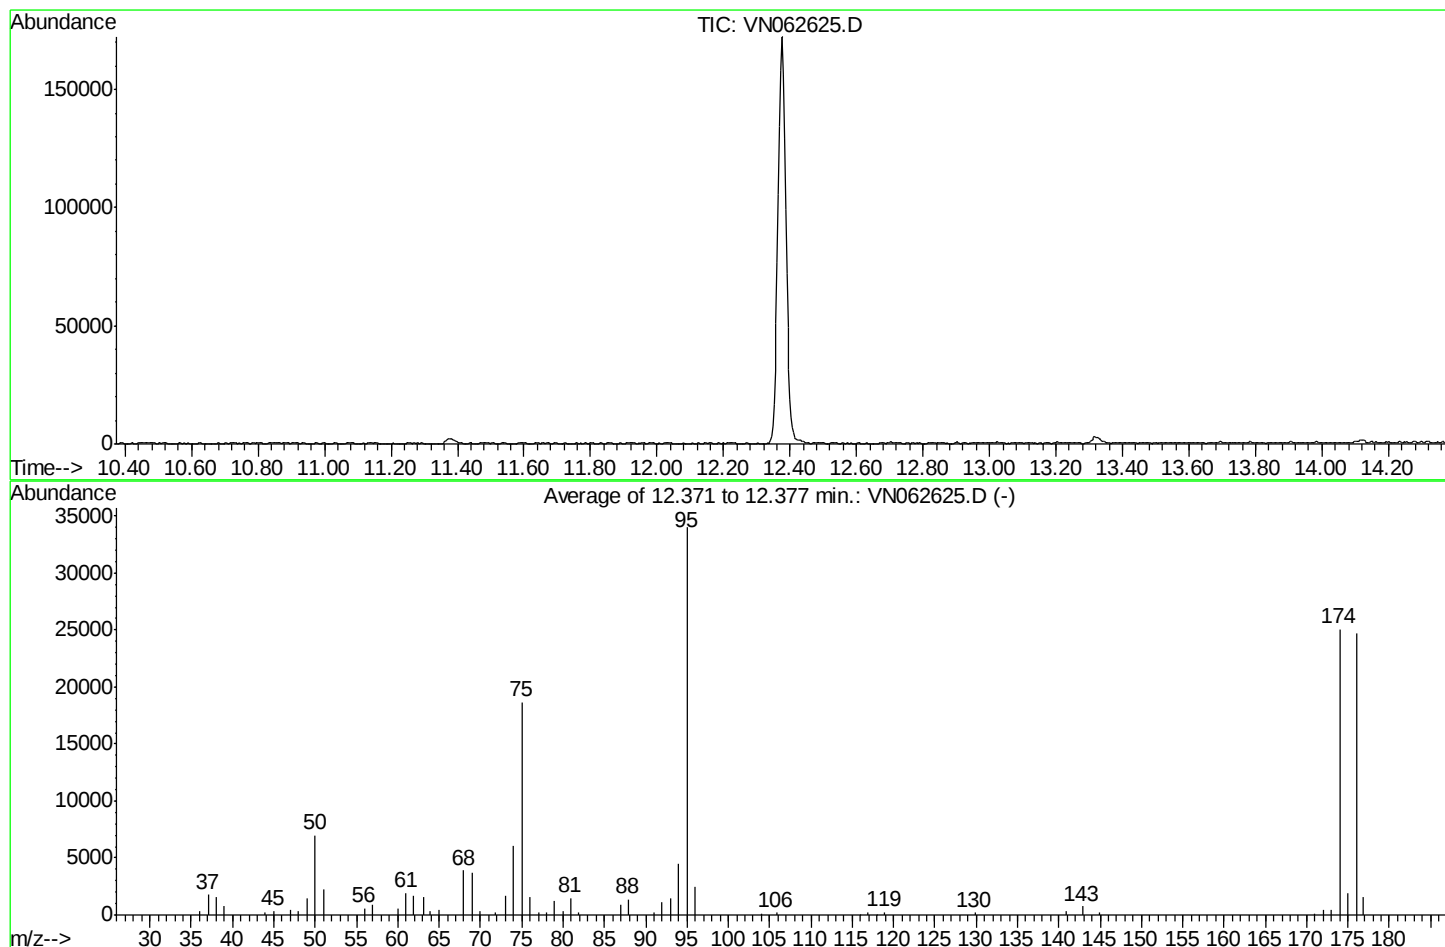

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3283

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	6966	PASS
75	95	30	60	54.9	18682	PASS
95	95	100	100	100.0	34005	PASS
96	95	5	9	7.4	2512	PASS
173	174	0.00	2	1.9	477	PASS
174	95	50	100	73.7	25058	PASS
175	174	5	9	7.8	1960	PASS
176	174	95	101	98.4	24658	PASS
177	176	5	9	6.6	1627	PASS