
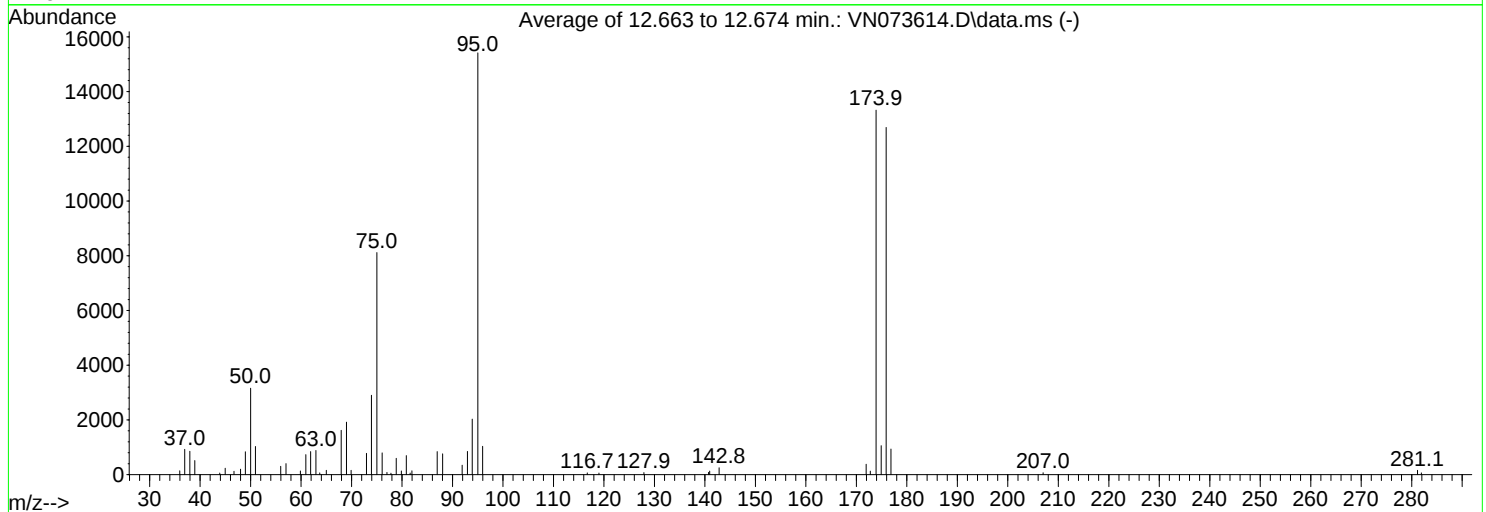


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072822\
Data File : VN073614.D
Acq On : 28 Jul 2022 09:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072822W.M
Title : SW846 8260
Last Update : Fri Jul 29 02:20:25 2022

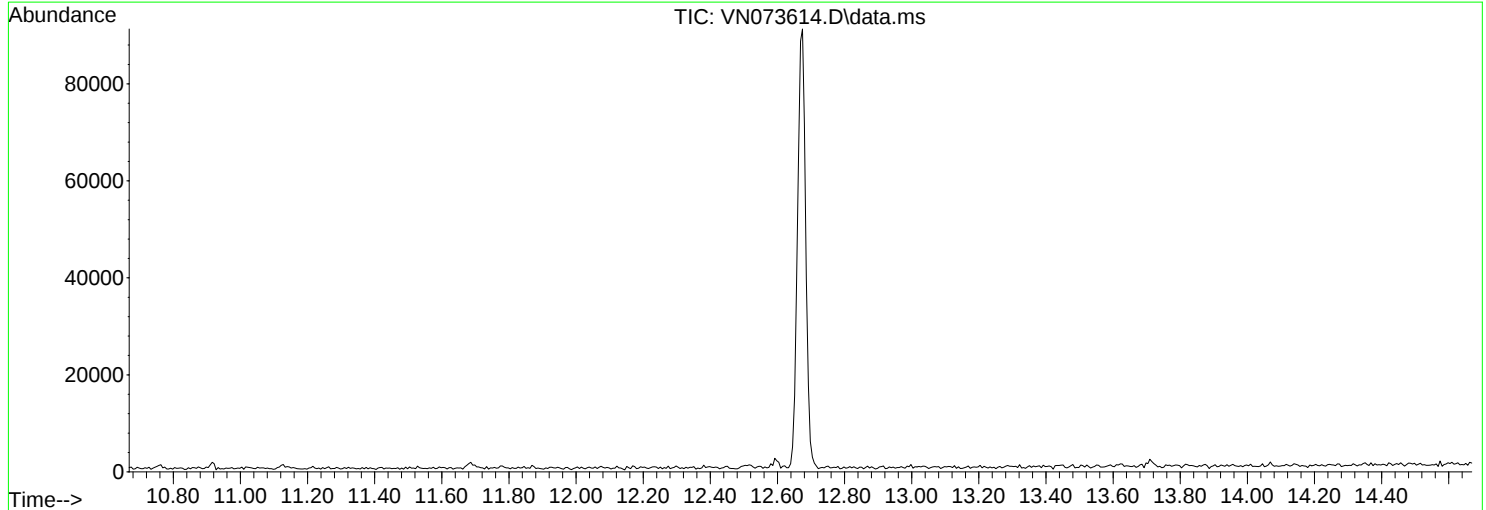

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1825

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	3157	PASS
75	95	30	60	52.7	8118	PASS
95	95	100	100	100.0	15415	PASS
96	95	5	9	6.7	1036	PASS
173	174	0.00	2	1.0	128	PASS
174	95	50	100	86.4	13318	PASS
175	174	5	9	7.9	1057	PASS
176	174	95	101	95.3	12692	PASS
177	176	5	9	7.4	934	PASS