

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072823\
 Data File : VN078678.D
 Acq On : 28 Jul 2023 11:23
 Operator : JC\MD
 Sample : VN0728WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0728WBL01

Quant Time: Jul 29 00:44:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 10 16:13:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	704844	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	1263345	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	1148012	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	404532	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	452835	47.923	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	95.840%		
35) Dibromofluoromethane	8.177	113	446263	52.036	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	104.080%		
50) Toluene-d8	10.570	98	1517271	46.833	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	93.660%		
62) 4-Bromofluorobenzene	12.853	95	521231	52.232	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	104.460%		
Target Compounds					Qvalue	
3) Chloromethane	2.371	50	2051	0.218	ug/l #	35
5) Bromomethane	2.965	94	3641	Below Cal	#	59
6) Chloroethane	3.142	64	1471	Below Cal	#	43
10) Methyl Iodide	4.606	142	2293	0.217	ug/l #	79
11) Tert butyl alcohol	5.518	59	8904	6.111	ug/l #	72
13) Acrolein	4.212	56	1013	0.707	ug/l #	38
15) Acrylonitrile	5.747	53	833	0.226	ug/l #	23
16) Acetone	4.430	43	738	0.251	ug/l #	40
17) Carbon Disulfide	4.724	76	4652	0.216	ug/l #	75
18) Methyl Acetate	5.036	43	4614	0.370	ug/l	91
20) Methylene Chloride	5.277	84	3851	Below Cal	#	80
25) 2-Butanone	7.512	43	1329	0.287	ug/l #	37
29) Tetrahydrofuran	7.859	42	875	0.288	ug/l #	36
31) Cyclohexane	8.235	56	14340	1.123	ug/l #	4
36) 1,1-Dichloropropene	8.235	75	55093	4.449	ug/l #	48
38) Carbon Tetrachloride	8.235	117	72631	5.397	ug/l #	16
43) Isopropyl Acetate	8.729	43	41276	2.429	ug/l #	52
49) 1,4-Dioxane	9.694	88	54	0.314	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	2300	0.228	ug/l #	85
59) 2-Hexanone	11.206	43	3188	0.444	ug/l	85
75) 1,1,2,2-Tetrachloroethane	12.947	83	989	Below Cal	#	86
76) 1,2,3-Trichloropropane	12.853	75	266001	27.204	ug/l #	1
77) Bromobenzene	12.988	156	799	Below Cal		62
81) trans-1,4-Dichloro-2-b...	12.853	75	266001	71.487	ug/l #	15
90) Hexachloroethane	14.341	117	317	Below Cal		98
92) 1,2-Dibromo-3-Chloropr...	14.723	75	454	Below Cal	#	38
93) 1,2,4-Trichlorobenzene	15.388	180	2023	0.436	ug/l	80
94) Hexachlorobutadiene	15.505	225	1936	Below Cal		69
95) Naphthalene	15.647	128	6315	0.399	ug/l	99
96) 1,2,3-Trichlorobenzene	15.847	180	2435	0.457	ug/l	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072823\
Data File : VN078678.D
Acq On : 28 Jul 2023 11:23
Operator : JC\MD
Sample : VN0728WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01

Quant Time: Jul 29 00:44:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 10 16:13:53 2023
Response via : Initial Calibration

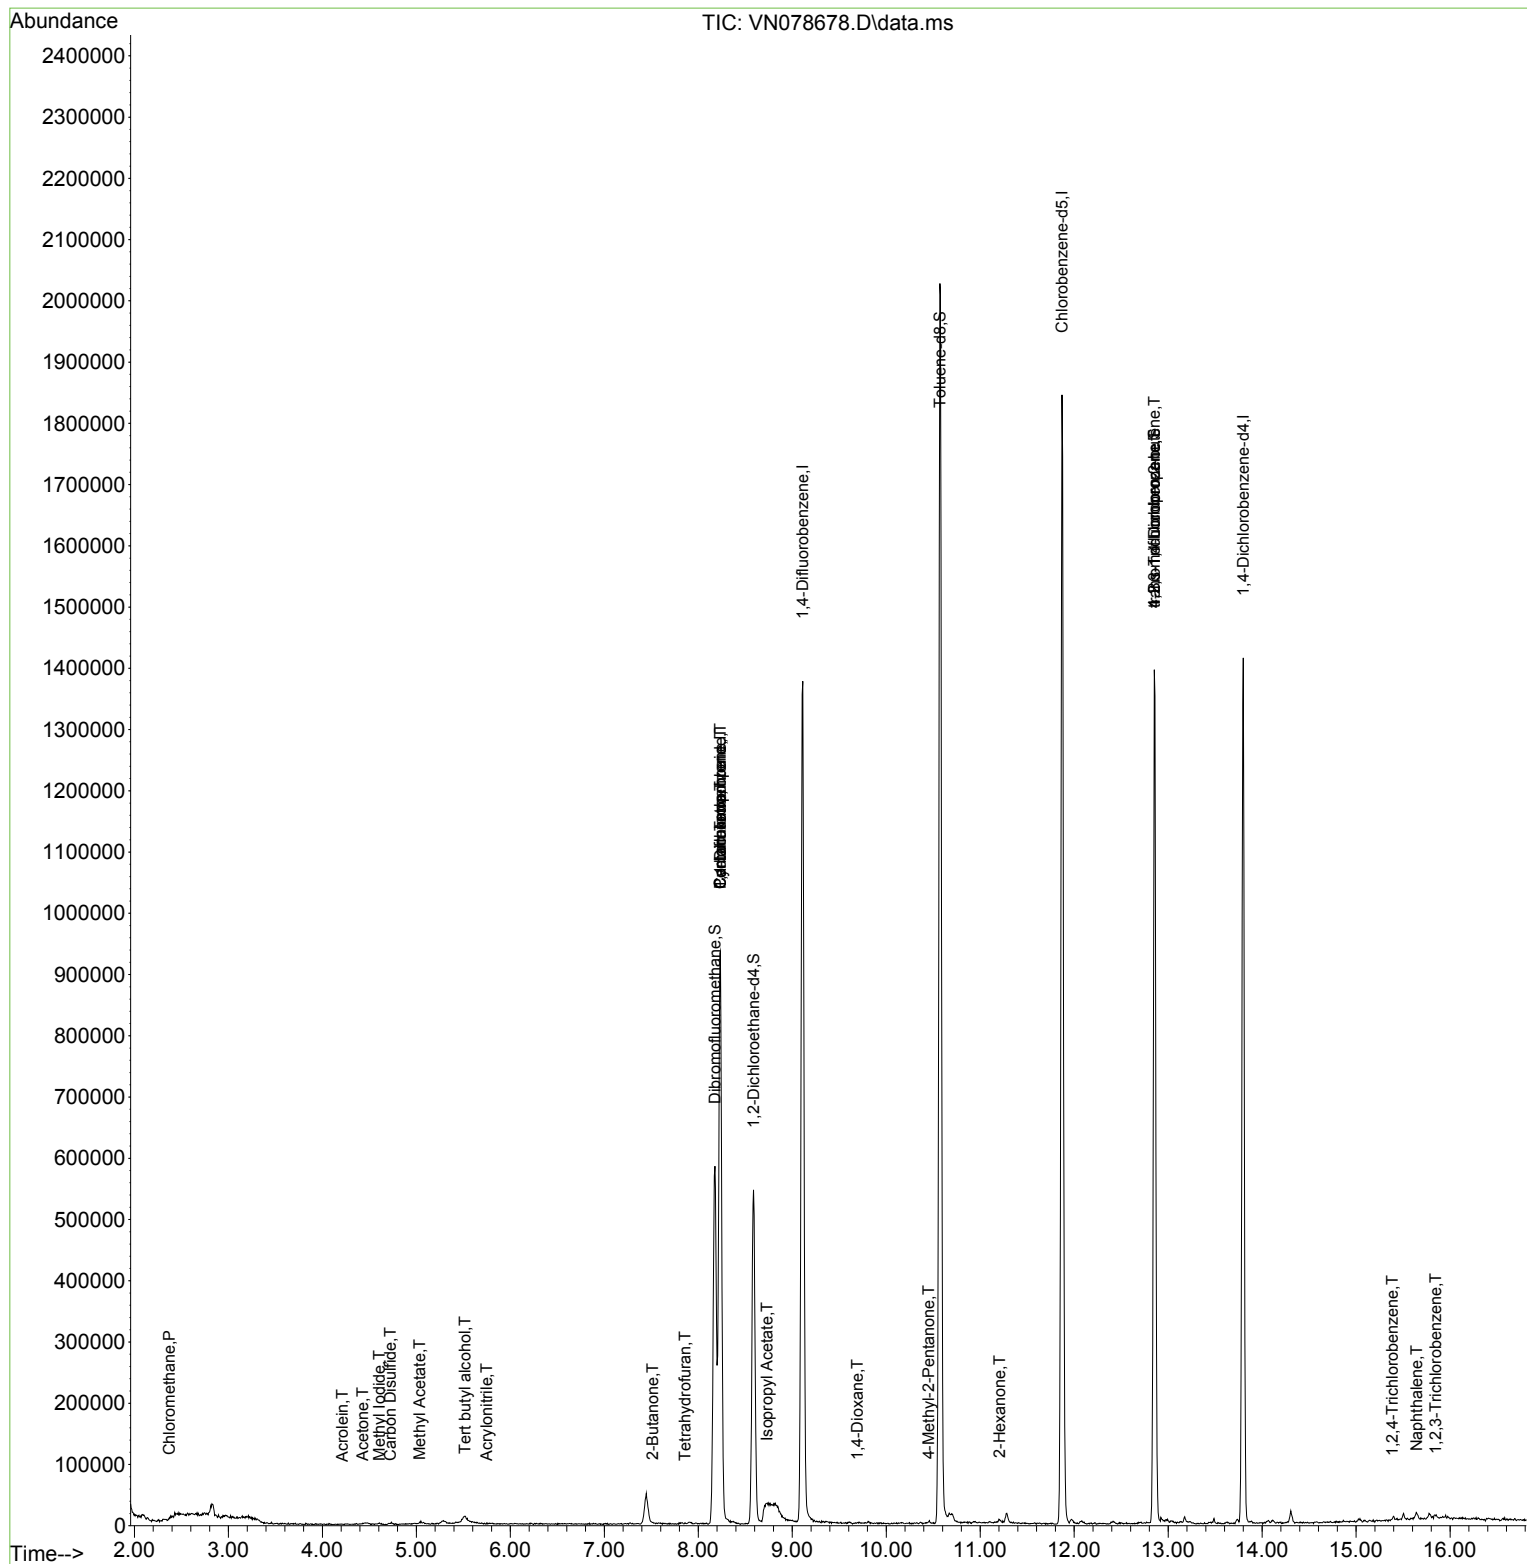



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.235 min Scan# 10

Delta R.T. 0.005 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23

Instrument :

MSVOA_N

ClientSampleId :





VN0728WBL01

Tgt Ion:168 Resp: 704844

Ion Ratio Lower Upper

168 100

99 59.0 53.0 79.6

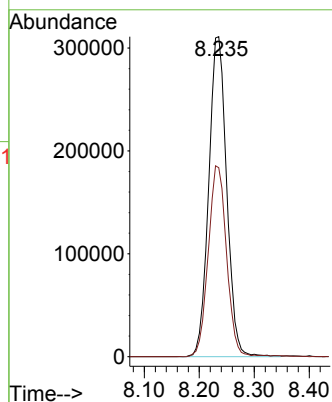

#3

Chloromethane

Concen: 0.218 ug/l

RT: 2.371 min Scan# 71

Delta R.T. 0.000 min

Lab File: VN078678.D




Acq: 28 Jul 2023 11:23


Tgt Ion: 50 Resp: 2051

Ion Ratio Lower Upper

50 100

52 69.8 26.5 39.7#


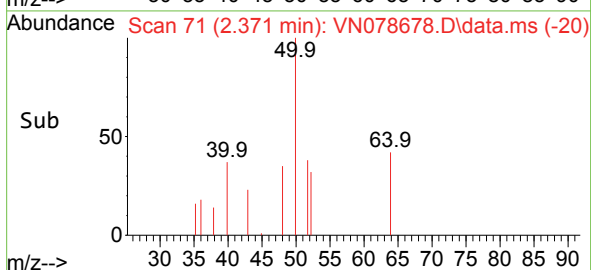






#5
Bromomethane
Concen: Below Cal
RT: 2.965 min Scan# 11
Delta R.T. 0.011 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion: 94 Resp: 3641
Ion Ratio Lower Upper
94 100
96 52.2 73.1 109.7#



#6
Chloroethane
Concen: Below Cal
RT: 3.142 min Scan# 202
Delta R.T. 0.024 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23


Tgt Ion: 64 Resp: 1471
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

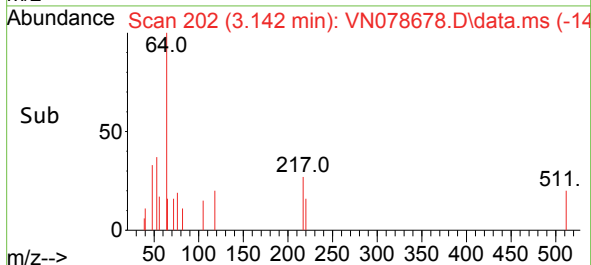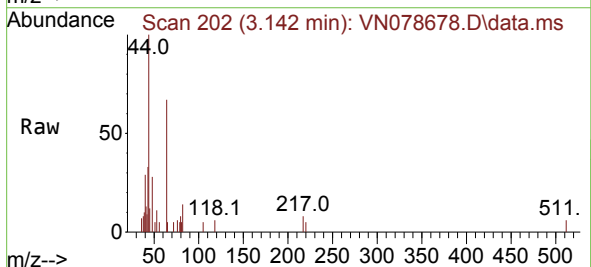






#10
Methyl Iodide
Concen: 0.217 ug/l
RT: 4.606 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01







Tgt Ion:142 Resp: 2293
Ion Ratio Lower Upper
142 100
127 35.2 37.6 56.4#
141 27.8 11.4 17.0#

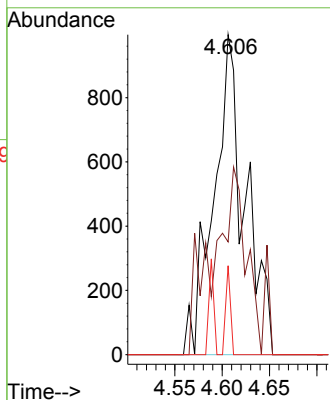

#11
Tert butyl alcohol
Concen: 6.111 ug/l
RT: 5.518 min Scan# 606
Delta R.T. -0.018 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 59 Resp: 8904
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#


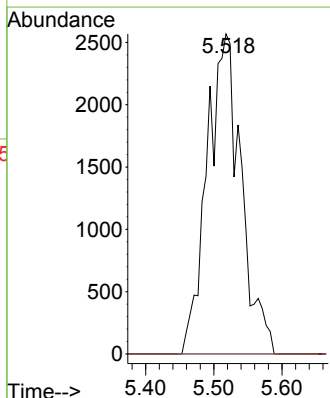






#13
Acrolein
Concen: 0.707 ug/l
RT: 4.212 min Scan# 31
Delta R.T. 0.023 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion: 56 Resp: 1013
Ion Ratio Lower Upper
56 100
55 18.0 54.5 81.7#

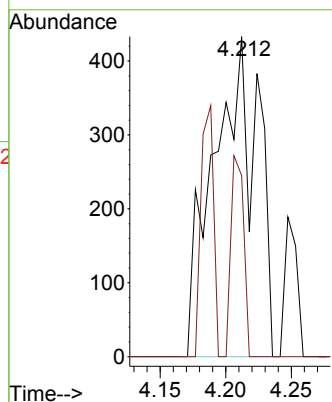

#15
Acrylonitrile
Concen: 0.226 ug/l
RT: 5.747 min Scan# 645
Delta R.T. 0.017 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 53 Resp: 833
Ion Ratio Lower Upper
53 100
52 0.0 65.3 97.9#
51 10.2 28.9 43.3#









#16
Acetone
Concen: 0.251 ug/l
RT: 4.430 min Scan# 41
Delta R.T. -0.012 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion: 43 Resp: 738
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#

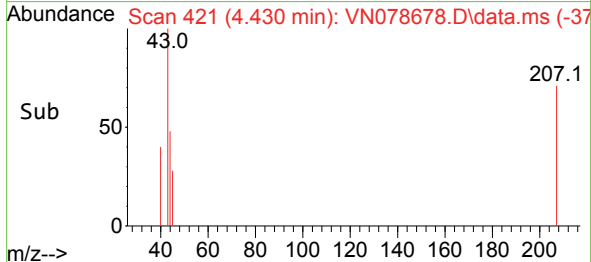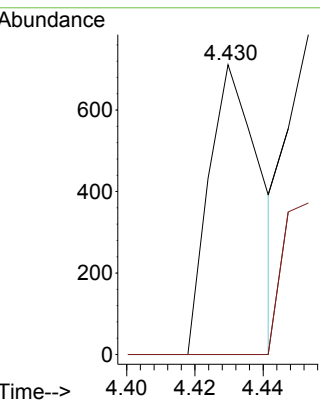

#17
Carbon Disulfide
Concen: 0.216 ug/l
RT: 4.724 min Scan# 471
Delta R.T. 0.006 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 76 Resp: 4652
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#


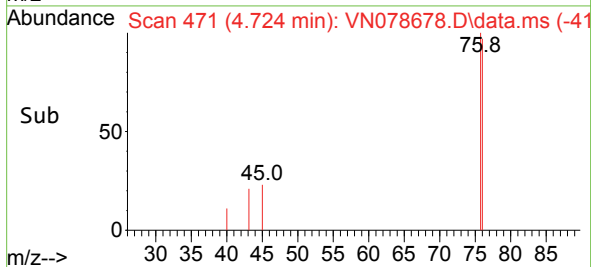
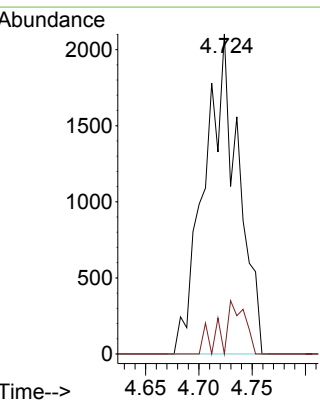
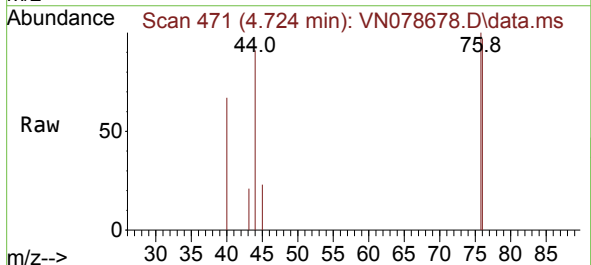




#18
Methyl Acetate
Concen: 0.370 ug/l
RT: 5.036 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion: 43 Resp: 4614
Ion Ratio Lower Upper
43 100
74 37.8 26.2 39.4



#20
Methylene Chloride
Concen: Below Cal
RT: 5.277 min Scan# 565
Delta R.T. -0.006 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 84 Resp: 3851
Ion Ratio Lower Upper
84 100
49 63.8 79.7 119.5#
51 37.2 25.2 37.8
86 64.9 53.3 79.9



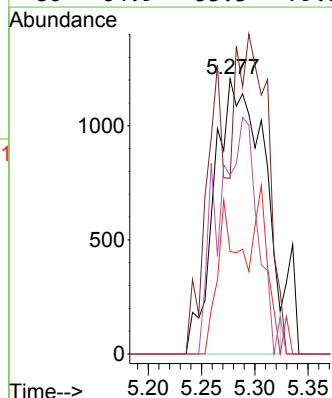





#25
2-Butanone
Concen: 0.287 ug/l
RT: 7.512 min Scan# 941
Delta R.T. 0.023 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion: 43 Resp: 1329
Ion Ratio Lower Upper
43 100
72 0.0 30.2 45.2#

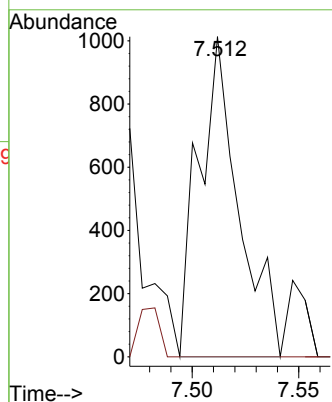

#29
Tetrahydrofuran
Concen: 0.288 ug/l
RT: 7.859 min Scan# 1004
Delta R.T. 0.012 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 42 Resp: 875
Ion Ratio Lower Upper
42 100
72 9.6 49.8 74.6#
71 13.9 47.4 71.2#


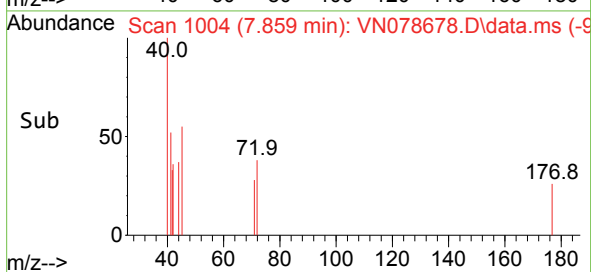
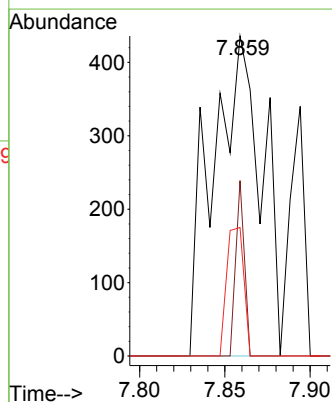
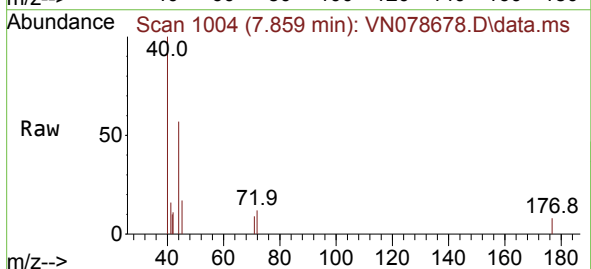




#31
Cyclohexane
Concen: 1.123 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.030 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion: 56 Resp: 14340
Ion Ratio Lower Upper
56 100
69 164.5 26.8 40.2#
84 155.5 81.8 122.6#



#33
1,2-Dichloroethane-d4
Concen: 47.923 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. 0.005 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 65 Resp: 452835
Ion Ratio Lower Upper
65 100
67 54.6 0.0 106.6

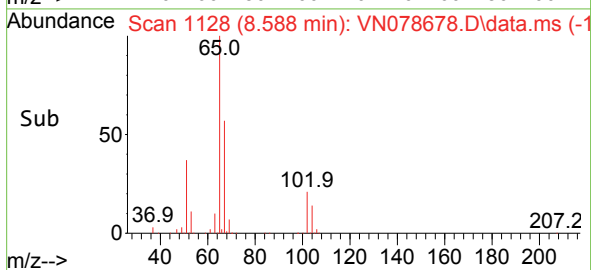



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23

Instrument :

MSVOA_N

ClientSampleId :

VN0728WBL01





Tgt Ion:114 Resp: 1263345

Ion Ratio Lower Upper

114 100

63 20.1 0.0 36.4

88 16.4 0.0 30.6

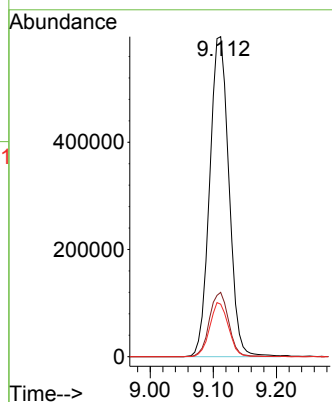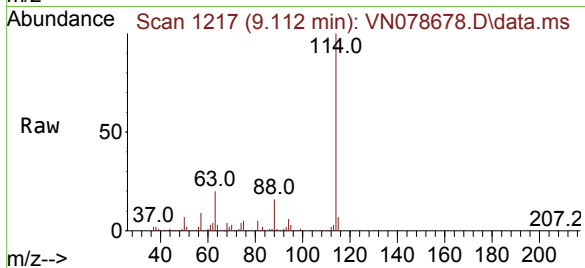

#35

Dibromofluoromethane

Concen: 52.036 ug/l

RT: 8.177 min Scan# 1058

Delta R.T. -0.000 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23




Tgt Ion:113 Resp: 446263


Ion Ratio Lower Upper

113 100

111 104.8 82.6 123.8

192 18.0 12.7 19.1

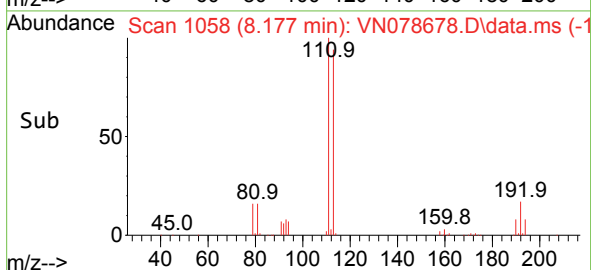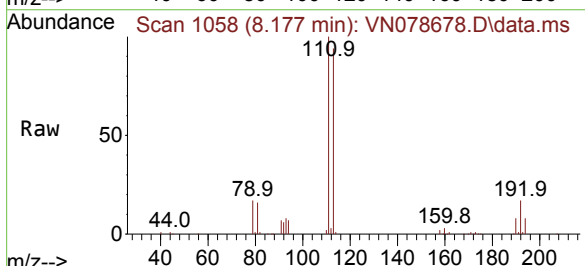



#36

1,1-Dichloropropene

Concen: 4.449 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.142 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23

Instrument :

MSVOA_N

ClientSampleId :

VN0728WBL01





Tgt Ion: 75 Resp: 55093

Ion Ratio Lower Upper

75 100

110 8.8 19.1 57.3#

77 0.0 25.0 37.4#

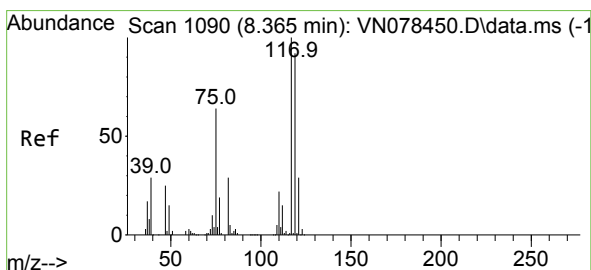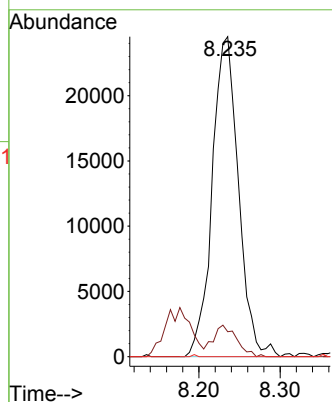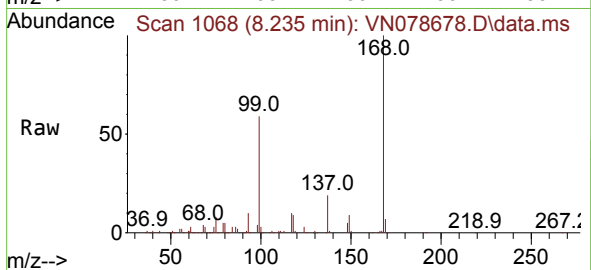

#38

Carbon Tetrachloride

Concen: 5.397 ug/l

RT: 8.235 min Scan# 1068

Delta R.T. -0.130 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23




Tgt Ion: 117 Resp: 72631


Ion Ratio Lower Upper

117 100

119 5.6 77.3 115.9#

121 0.0 23.3 34.9#


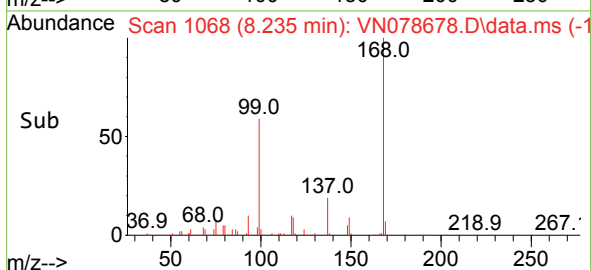

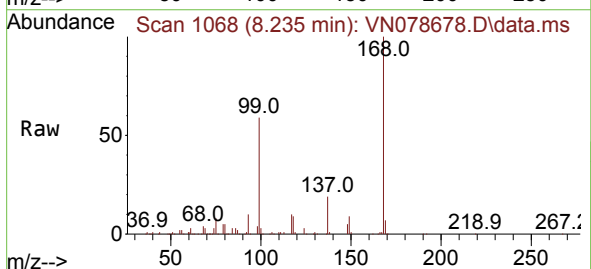




#43
Isopropyl Acetate
Concen: 2.429 ug/l
RT: 8.729 min Scan# 1152
Delta R.T. 0.035 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion: 43 Resp: 41276
Ion Ratio Lower Upper
43 100
61 2.0 24.7 37.1#
87 0.0 14.6 21.8#

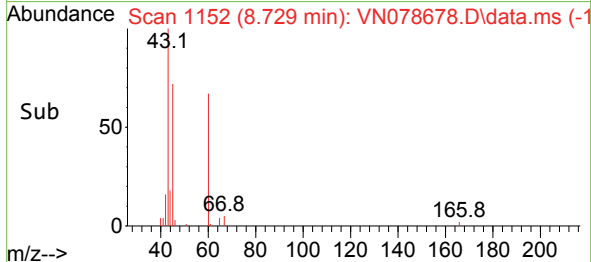

#49
1,4-Dioxane
Concen: 0.314 ug/l
RT: 9.694 min Scan# 1316
Delta R.T. -0.006 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 88 Resp: 54
Ion Ratio Lower Upper
88 100
43 464.8 17.0 25.6#
58 0.0 47.0 70.4#


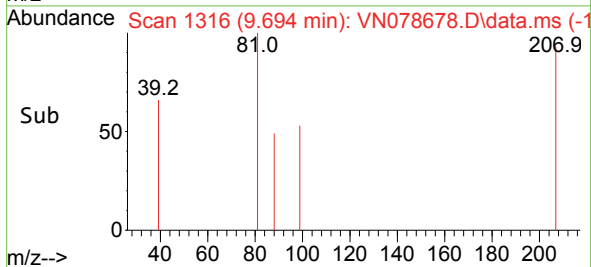

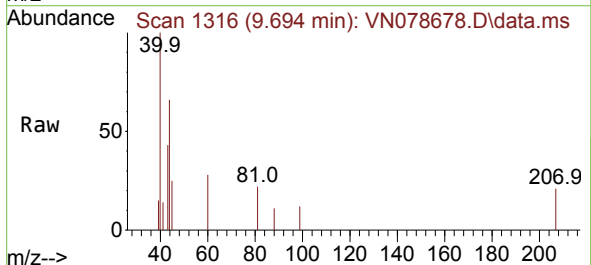




#50
Toluene-d8
Concen: 46.833 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.001 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion: 98 Resp: 1517271
Ion Ratio Lower Upper
98 100
100 63.5 52.0 78.0

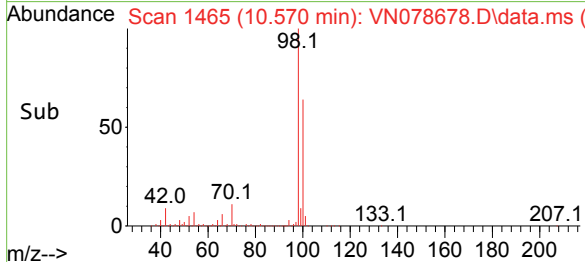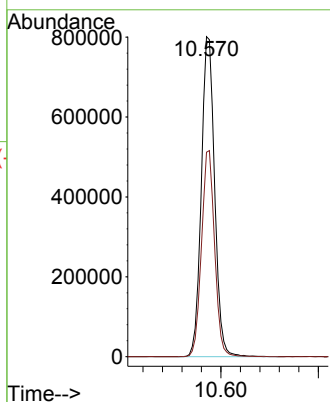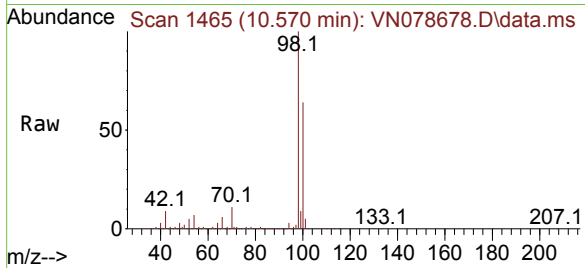

#51
4-Methyl-2-Pentanone
Concen: 0.228 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. -0.000 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 43 Resp: 2300
Ion Ratio Lower Upper
43 100
58 35.8 36.6 54.8#


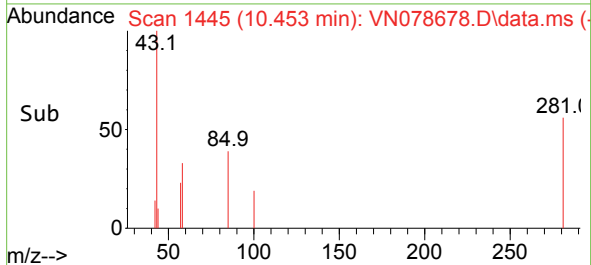
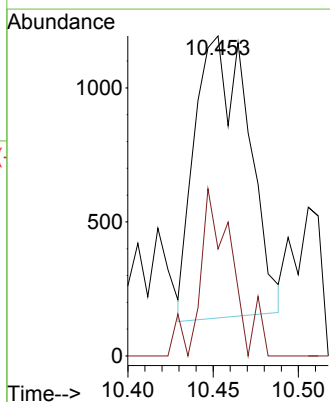
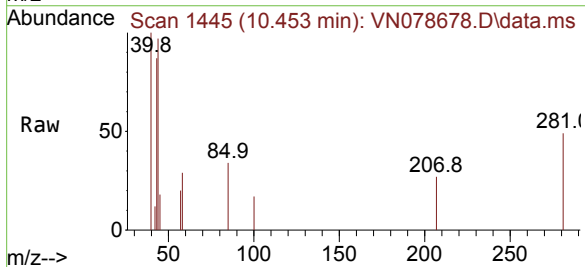




#59
2-Hexanone
Concen: 0.444 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion: 43 Resp: 3188
Ion Ratio Lower Upper
43 100
58 51.5 31.7 95.1

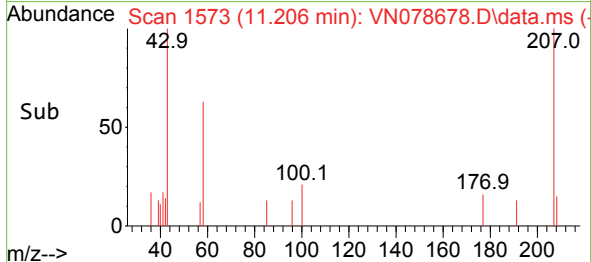

#62
4-Bromofluorobenzene
Concen: 52.232 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 95 Resp: 521231
Ion Ratio Lower Upper
95 100
174 76.9 0.0 143.8
176 72.7 0.0 135.8


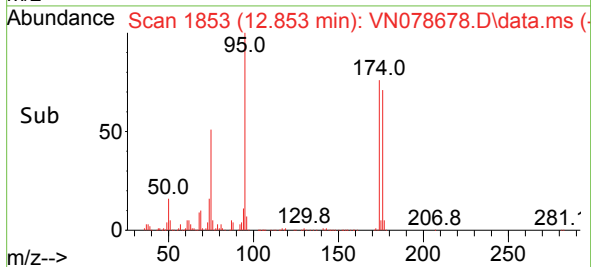

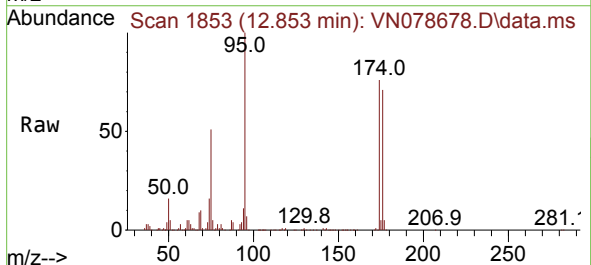


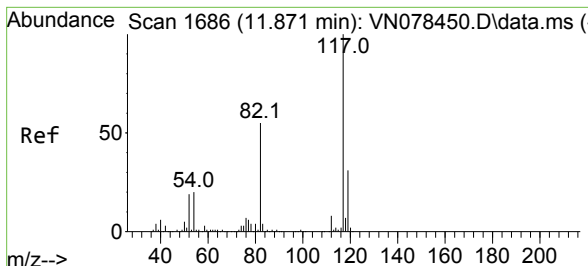

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 11
Delta R.T. -0.001 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion:117 Resp: 1148012
Ion Ratio Lower Upper
117 100
82 56.9 44.0 66.0
119 31.5 25.6 38.4

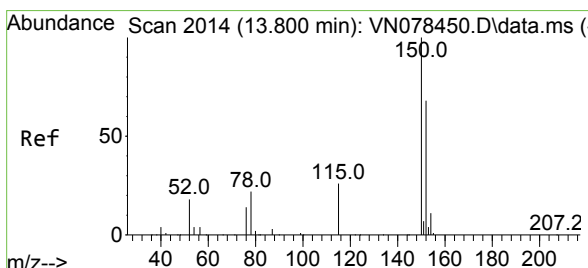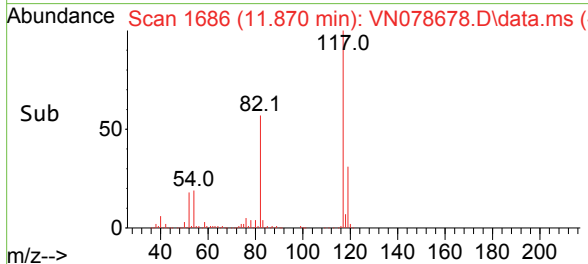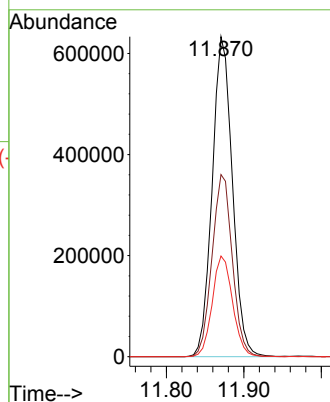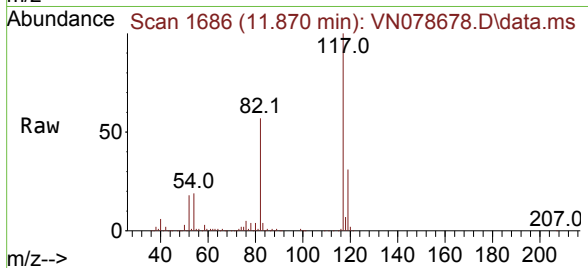

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion:152 Resp: 404532
Ion Ratio Lower Upper
152 100
115 61.6 32.3 96.8
150 157.7 0.0 355.8

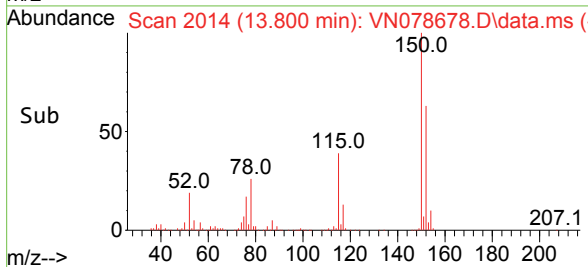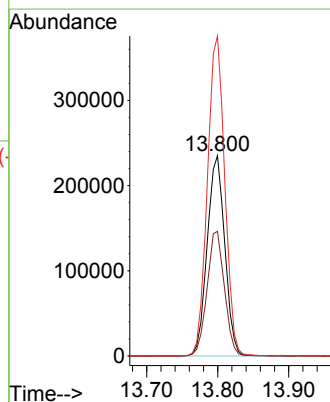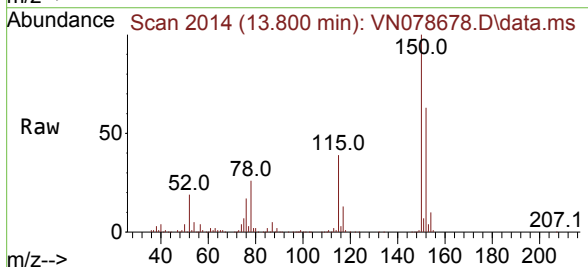

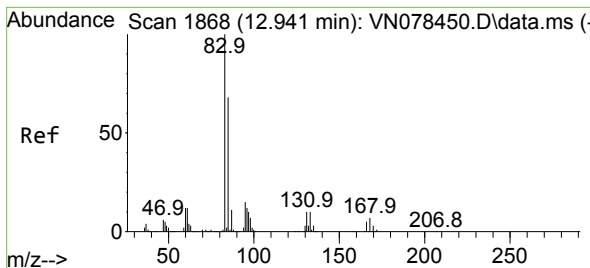

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.947 min Scan# 1868

Delta R.T. 0.006 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23

Instrument :

MSVOA_N

ClientSampleId :

VN0728WBL01





Tgt Ion: 83 Resp: 989

Ion Ratio Lower Upper

83 100

131 0.0 5.0 15.0#

85 73.2 31.9 95.7

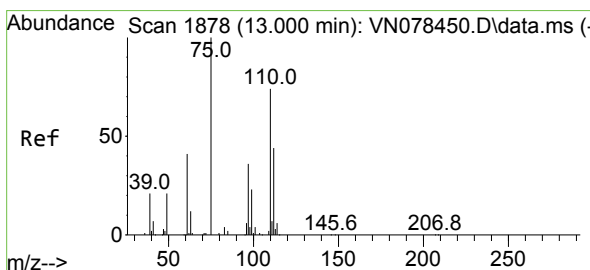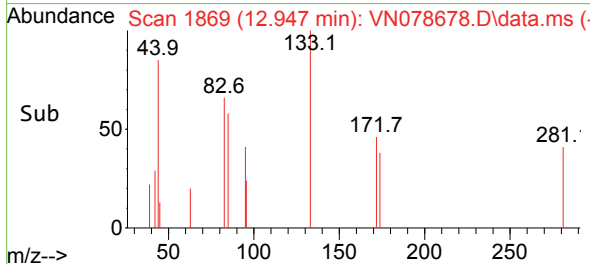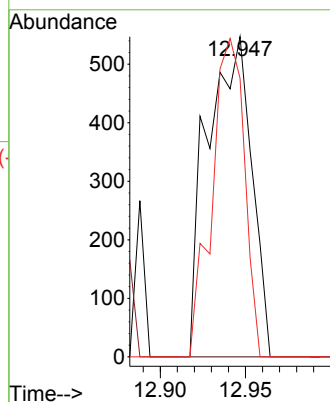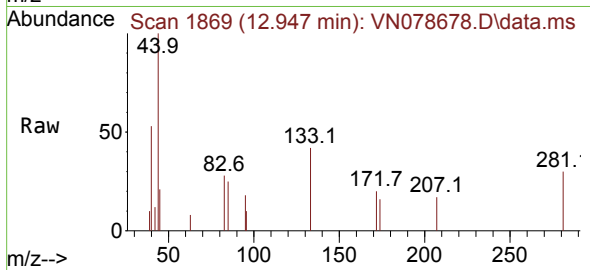

#76

1,2,3-Trichloropropane

Concen: 27.204 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN078678.D




Acq: 28 Jul 2023 11:23


Tgt Ion: 75 Resp: 266001

Ion Ratio Lower Upper

75 100

77 1.4 84.5 253.5#


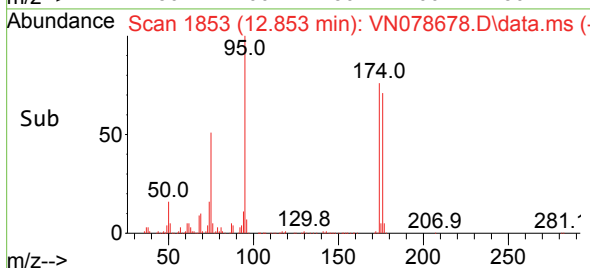
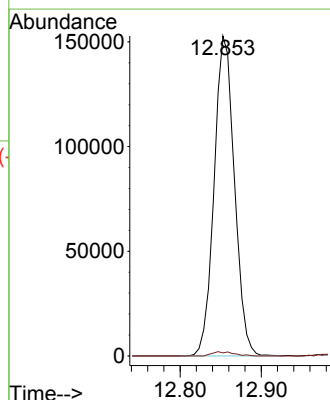
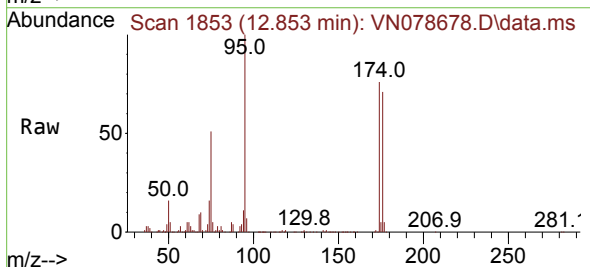




#77
Bromobenzene
Concen: Below Cal
RT: 12.988 min Scan# 1876
Delta R.T. -0.000 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23




Instrument :
MSVOA_N
ClientSampleId :
VN0728WBL01


Tgt Ion:156 Resp: 799
Ion Ratio Lower Upper
156 100
77 295.2 107.7 323.3
158 106.3 48.4 145.3

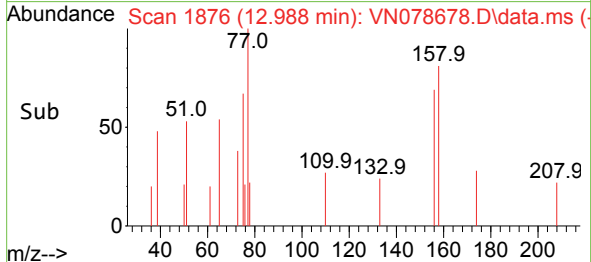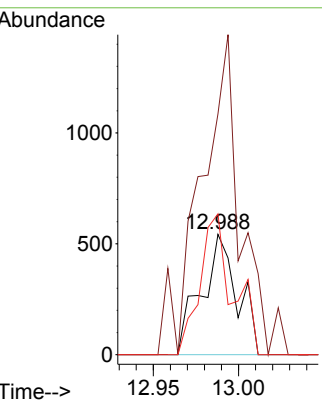

#81
trans-1,4-Dichloro-2-butene
Concen: 71.487 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN078678.D
Acq: 28 Jul 2023 11:23

Tgt Ion: 75 Resp: 266001
Ion Ratio Lower Upper
75 100
53 0.1 67.4 101.2#
89 0.0 38.8 58.2#

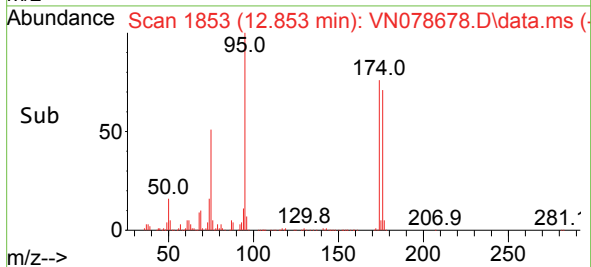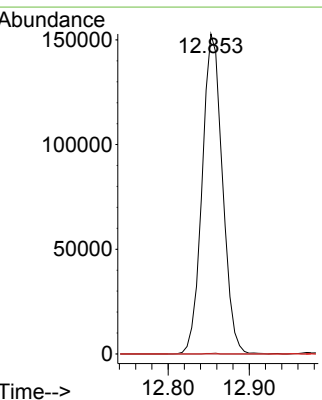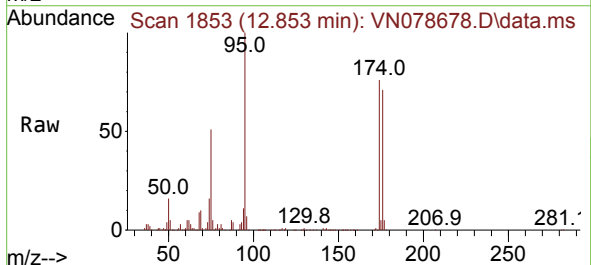



#90

Hexachloroethane

Concen: Below Cal

RT: 14.341 min Scan# 2105

Delta R.T. 0.006 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23

Instrument :

MSVOA_N

ClientSampleId :





VN0728WBL01

Tgt Ion:117 Resp: 317

Ion Ratio Lower Upper

117 100

201 57.4 29.3 88.0

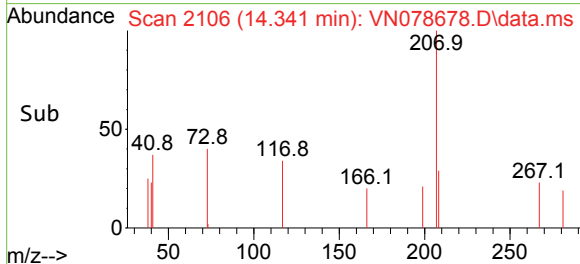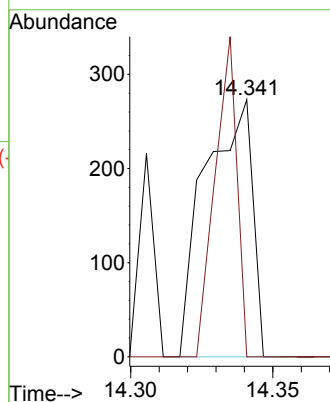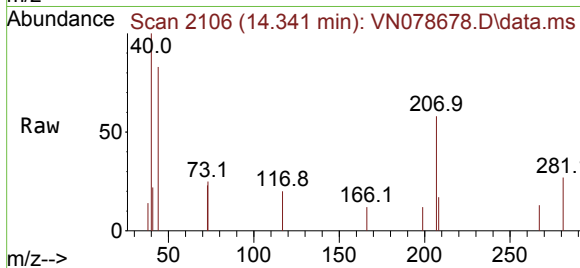

#92

1,2-Dibromo-3-Chloropropane

Concen: Below Cal

RT: 14.723 min Scan# 2171

Delta R.T. 0.000 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23




Tgt Ion: 75 Resp: 454


Ion Ratio Lower Upper

75 100

155 16.1 39.1 117.2#

157 46.3 50.3 150.9#

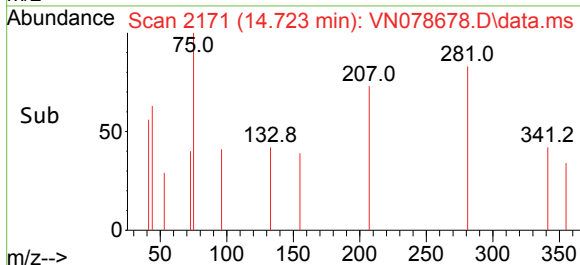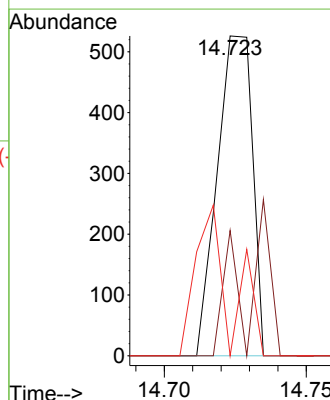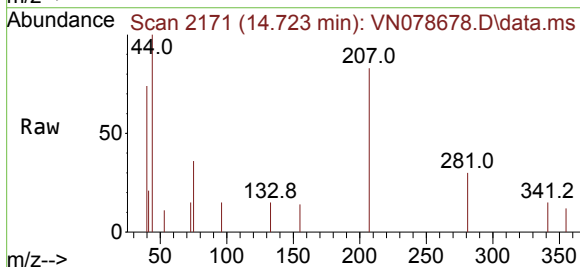



#93

1,2,4-Trichlorobenzene

Concen: 0.436 ug/l

RT: 15.388 min Scan# 21

Delta R.T. -0.012 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23

Instrument :

MSVOA_N

ClientSampleId :

VN0728WBL01





Tgt Ion:180 Resp: 2023

Ion Ratio Lower Upper

180 100

182 73.0 46.1 138.2

145 22.7 16.6 49.8



#94

Hexachlorobutadiene

Concen: Below Cal

RT: 15.505 min Scan# 2304

Delta R.T. -0.001 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23




Tgt Ion:225 Resp: 1936


Ion Ratio Lower Upper

225 100

223 42.3 31.3 93.8

227 35.5 31.9 95.9

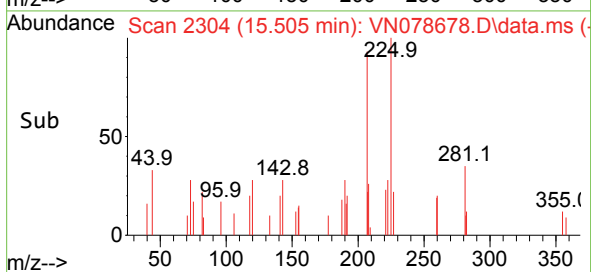



#95

Naphthalene

Concen: 0.399 ug/l

RT: 15.647 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23





Instrument :

MSVOA_N

ClientSampleId :

VN0728WBL01

Tgt Ion:	128	Resp:	6315
Ion	Ratio	Lower	Upper
128	100		
127	13.0	10.0	15.0
129	11.0	8.7	13.1

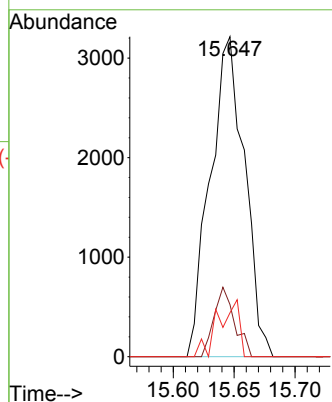

#96

1,2,3-Trichlorobenzene

Concen: 0.457 ug/l

RT: 15.847 min Scan# 2362

Delta R.T. -0.000 min

Lab File: VN078678.D

Acq: 28 Jul 2023 11:23

Tgt Ion:	180	Resp:	2435
Ion	Ratio	Lower	Upper
180	100		
182	77.5	46.2	138.6
145	36.4	17.5	52.6

