

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072823\
 Data File : VN078677.D
 Acq On : 28 Jul 2023 10:59
 Operator : JC\MD
 Sample : VN0728MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0728MBL01

Quant Time: Jul 29 00:44:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 10 16:13:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.229	168	429129	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	758424	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	689560	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	237759	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	277185	48.182	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	96.360%
35) Dibromofluoromethane	8.171	113	271317	52.699	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	105.400%
50) Toluene-d8	10.576	98	906820	46.625	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	93.260%
62) 4-Bromofluorobenzene	12.853	95	286823	47.878	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072823\
Data File : VN078677.D
Acq On : 28 Jul 2023 10:59
Operator : JC\MD
Sample : VN0728MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0728MBL01

Quant Time: Jul 29 00:44:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 10 16:13:53 2023
Response via : Initial Calibration




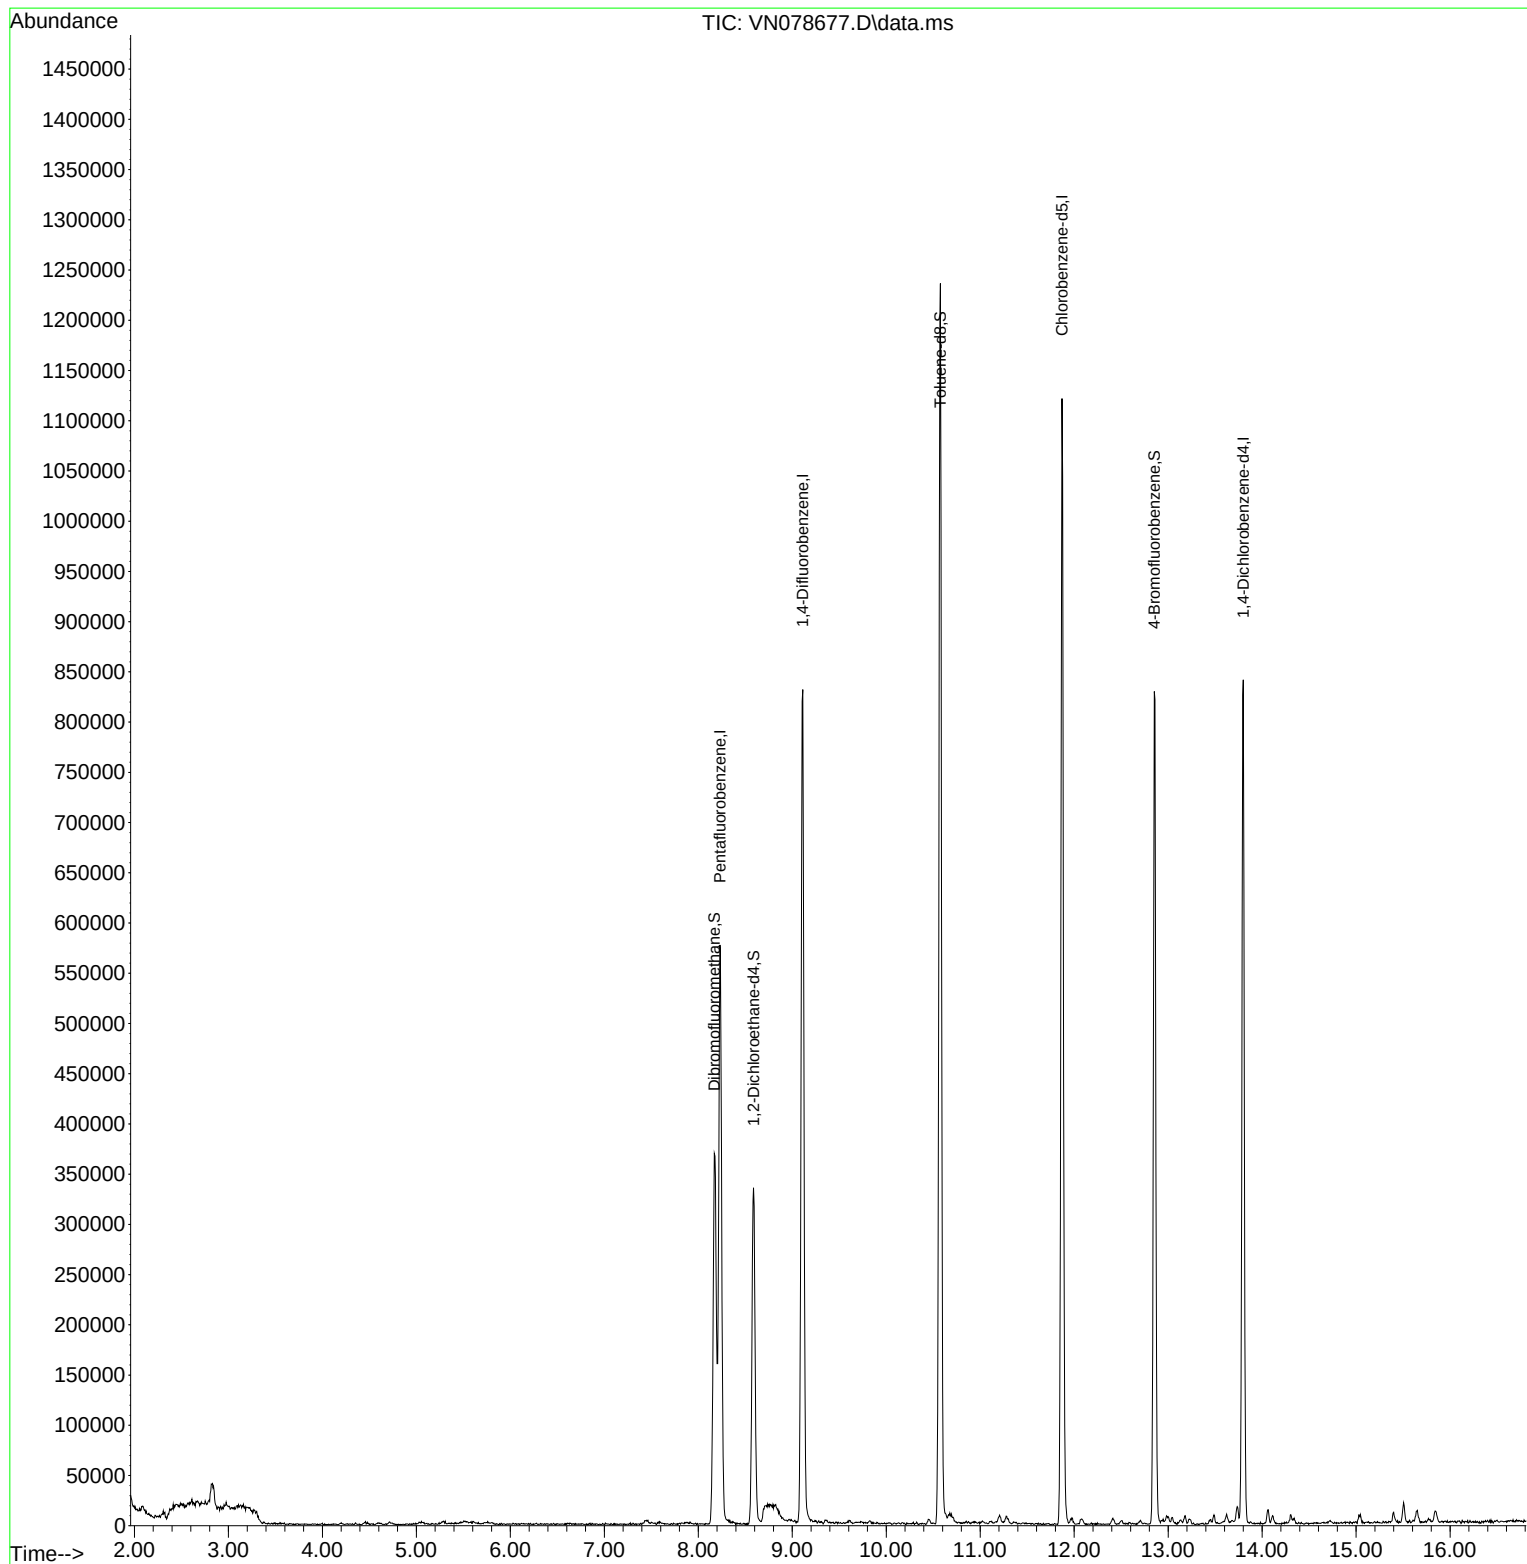


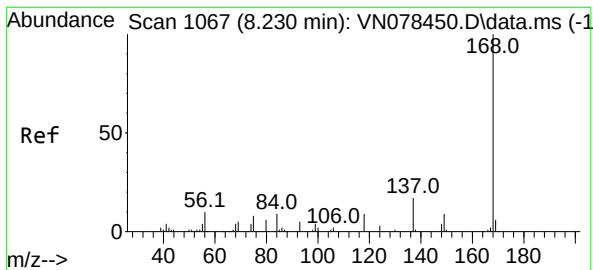

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.001 min
Lab File: VN078677.D
Acq: 28 Jul 2023 10:59




Instrument :
MSVOA_N
ClientSampleId :
VN0728MBL01


Tgt Ion:168 Resp: 429129
Ion Ratio Lower Upper
168 100
99 54.3 53.0 79.6

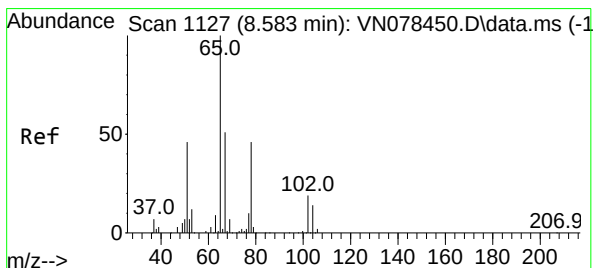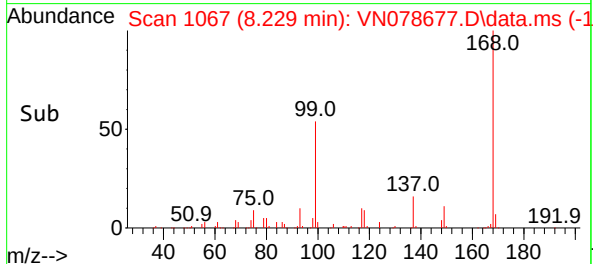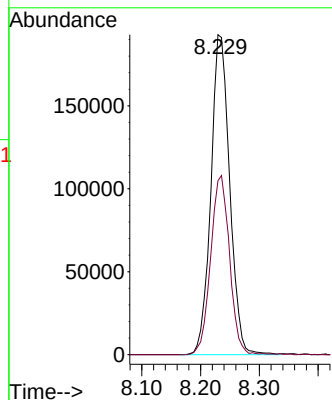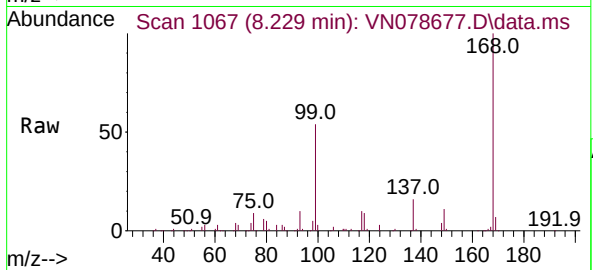

#33
1,2-Dichloroethane-d4
Concen: 48.182 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. 0.005 min
Lab File: VN078677.D
Acq: 28 Jul 2023 10:59

Tgt Ion: 65 Resp: 277185
Ion Ratio Lower Upper
65 100
67 53.3 0.0 106.6

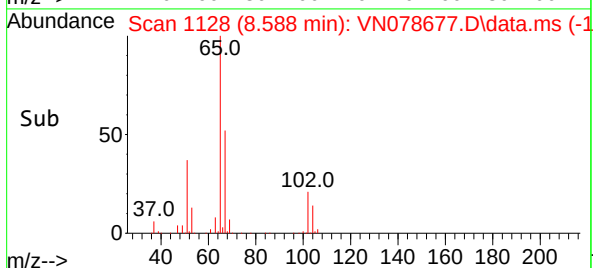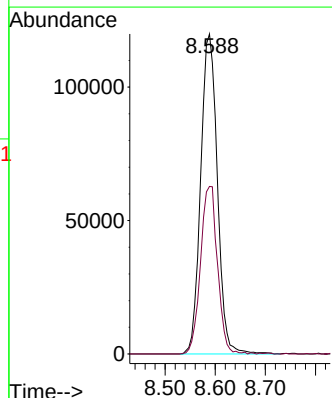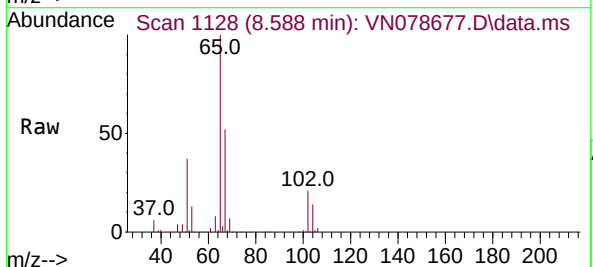

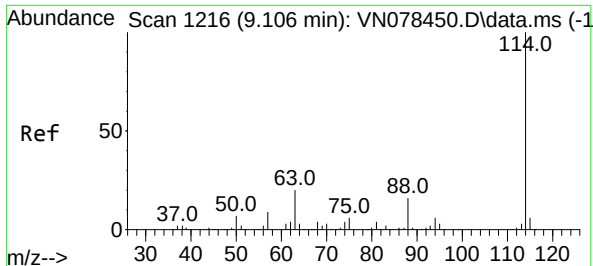

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN078677.D

Acq: 28 Jul 2023 10:59

Instrument :

MSVOA_N

ClientSampleId :

VN0728MBL01





Tgt Ion:114 Resp: 758424

Ion Ratio Lower Upper

114 100

63 19.1 0.0 36.4

88 15.3 0.0 30.6

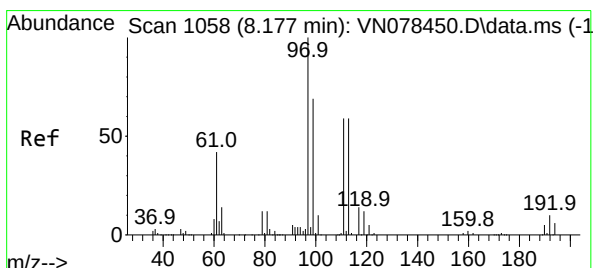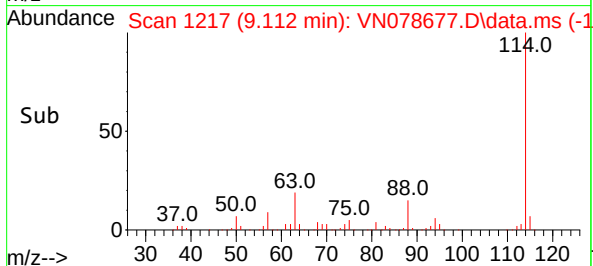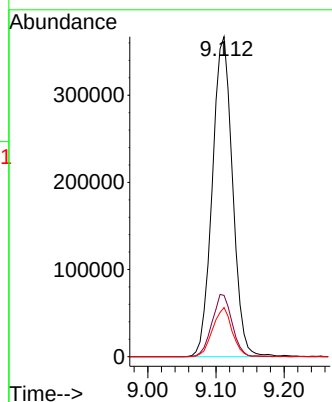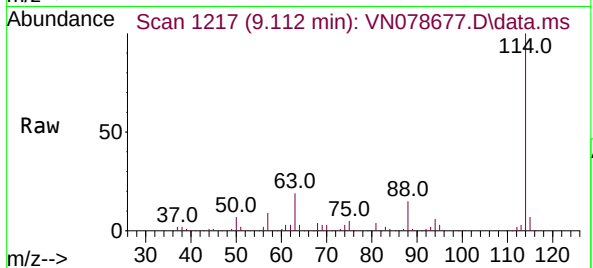

#35

Dibromofluoromethane

Concen: 52.699 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.006 min

Lab File: VN078677.D

Acq: 28 Jul 2023 10:59




Tgt Ion:113 Resp: 271317


Ion Ratio Lower Upper

113 100

111 103.7 82.6 123.8

192 18.3 12.7 19.1


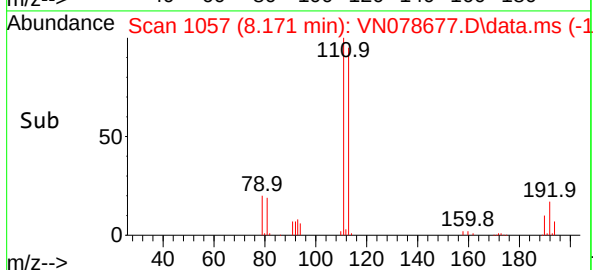
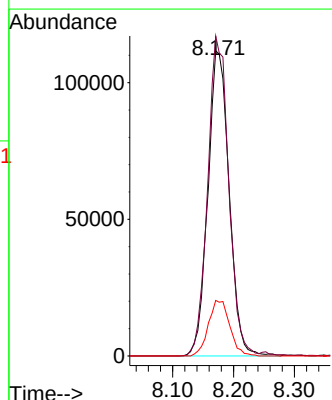
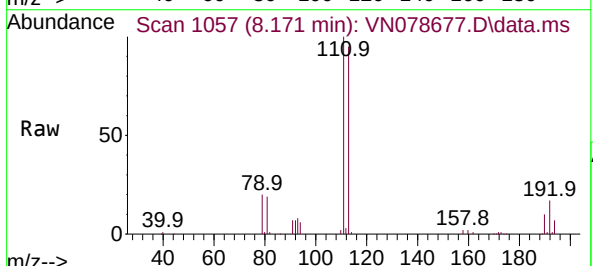


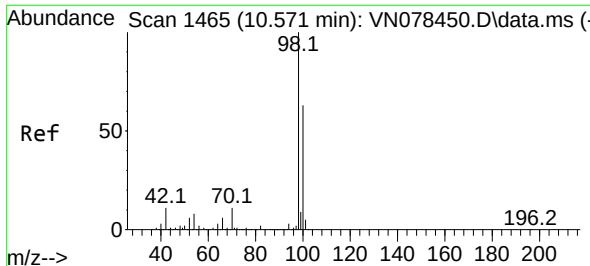

#50
Toluene-d8
Concen: 46.625 ug/l
RT: 10.576 min Scan# 1466
Delta R.T. 0.005 min
Lab File: VN078677.D
Acq: 28 Jul 2023 10:59




Instrument :
MSVOA_N
ClientSampleId :
VN0728MBL01


Tgt Ion: 98 Resp: 906820
Ion Ratio Lower Upper
98 100
100 62.9 52.0 78.0

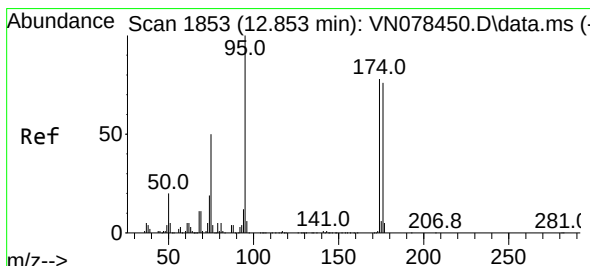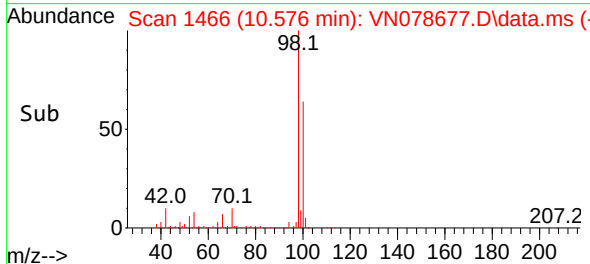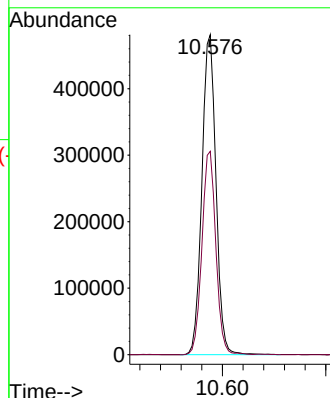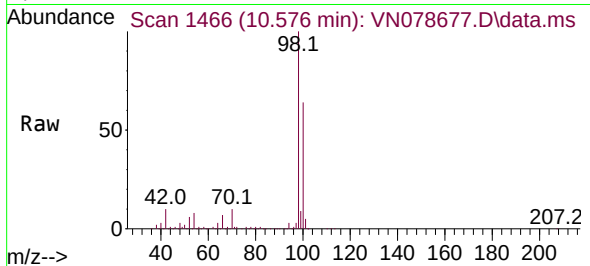

#62
4-Bromofluorobenzene
Concen: 47.878 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN078677.D
Acq: 28 Jul 2023 10:59

Tgt Ion: 95 Resp: 286823
Ion Ratio Lower Upper
95 100
174 84.0 0.0 143.8
176 79.2 0.0 135.8

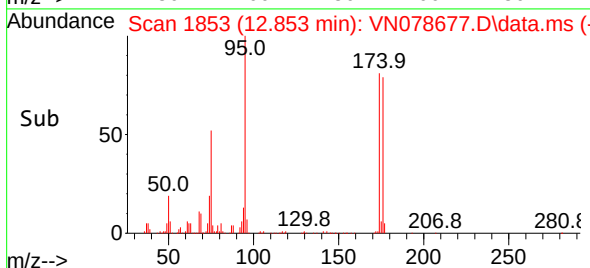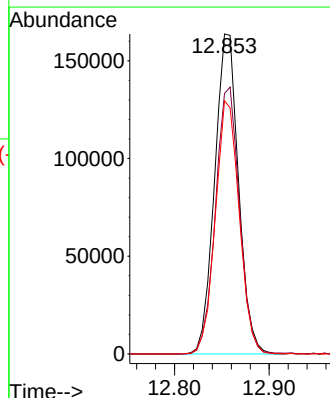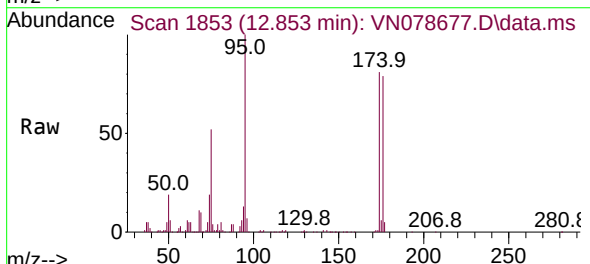

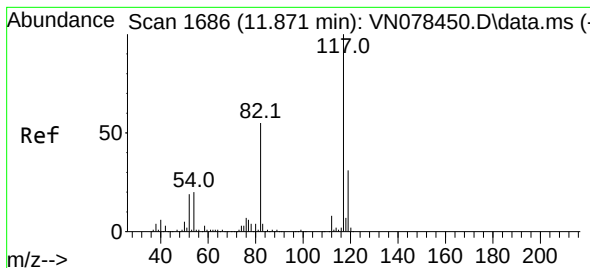

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.870 min Scan# 1

Delta R.T. -0.001 min

Lab File: VN078677.D

Acq: 28 Jul 2023 10:59

Instrument :

MSVOA_N

ClientSampleId :

VN0728MBL01





Tgt Ion:117 Resp: 689560

Ion Ratio Lower Upper

117 100

82 52.9 44.0 66.0

119 32.3 25.6 38.4

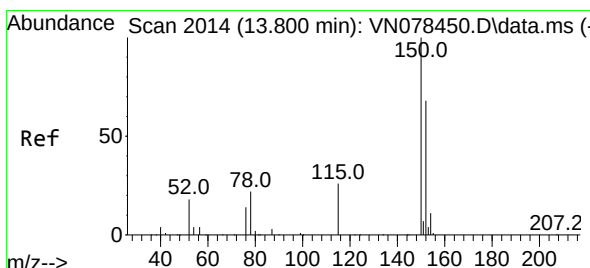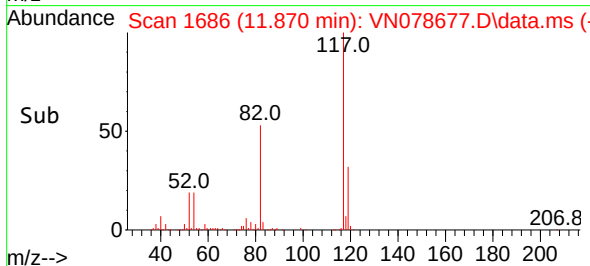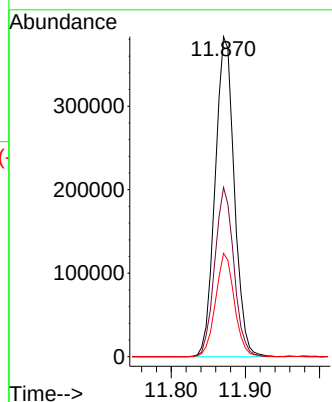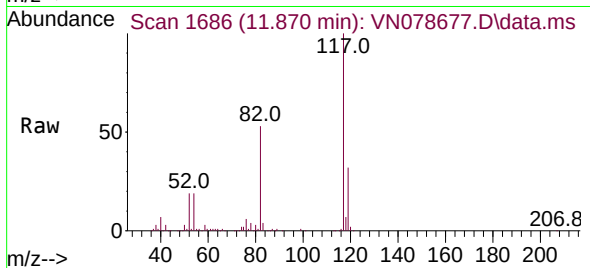

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.800 min Scan# 2014

Delta R.T. -0.000 min

Lab File: VN078677.D

Acq: 28 Jul 2023 10:59

Tgt Ion:152 Resp: 237759

Ion Ratio Lower Upper

152 100

115 59.4 32.3 96.8

150 156.7 0.0 355.8

