

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN072919\
 Data File : VN056962.D
 Acq On : 29 Jul 2019 19:48
 Operator : JC/SP
 Sample : VSSTDICV005
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 ICVVN072919

Quant Time: Jul 30 01:55:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 30 01:50:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	36769	5.00	ug/l	0.01
4) 1,4-Difluorobenzene	8.58	114	51197	5.00	ug/l	0.01
8) Chlorobenzene-d5	11.40	117	35168	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.35	152	5299	5.00	ug/l	0.00

System Monitoring Compounds

3) 1,2-Dichloroethane-d4	8.00	65	21563	4.73	ug/l	0.00
Spiked Amount	5.000	Range	81 - 118	Recovery	=	94.60%
5) Dibromofluoromethane	7.57	113	18206	5.23	ug/l	0.00
Spiked Amount	5.000	Range	80 - 119	Recovery	=	104.60%
6) Toluene-d8	10.08	98	36846	5.19	ug/l	0.00
Spiked Amount	5.000	Range	89 - 112	Recovery	=	103.80%
7) 4-Bromofluorobenzene	12.39	95	8754	5.28	ug/l	0.00
Spiked Amount	5.000	Range	85 - 114	Recovery	=	105.60%


Target Compounds					Qvalue
2) Vinyl Chloride	2.16	62	17823	5.250 ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN072919\
Data File : VN056962.D
Acq On : 29 Jul 2019 19:48
Operator : JC/SP
Sample : VSSTDICV005
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
ICVVN072919

Quant Time: Jul 30 01:55:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Tue Jul 30 01:50:04 2019
Response via : Initial Calibration

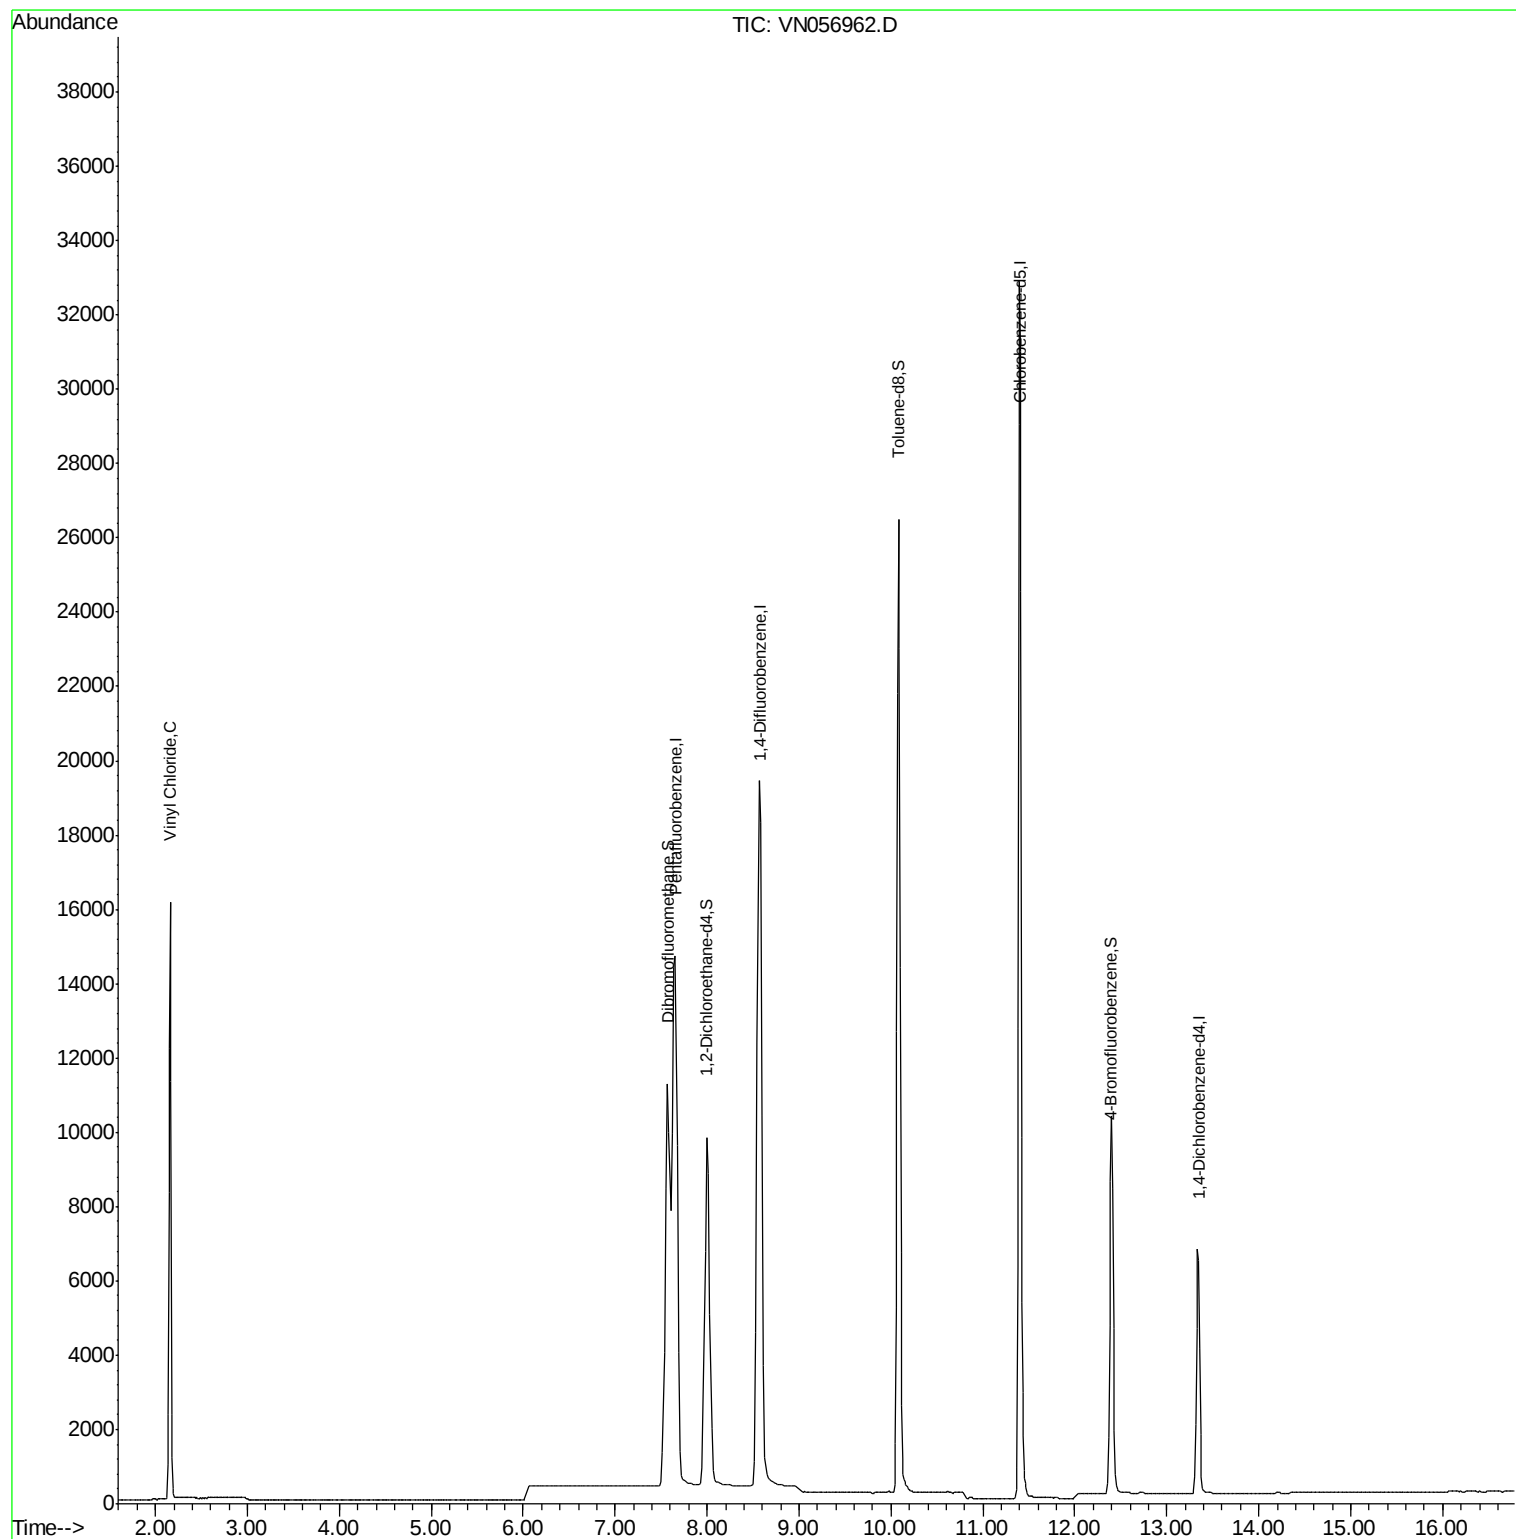

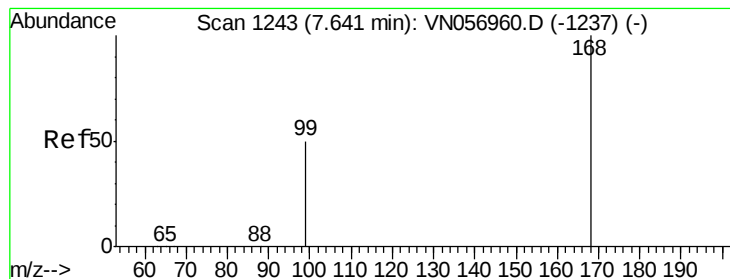

#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.65 min Scan# 1243

Delta R.T. 0.01 min

Lab File: VN056962.D

Acq: 29 Jul 2019 19:48

Instrument :

MSVOA_N

ClientSampleId :


ICVVN072919

Tot Ion:168 Resp: 36769

Ion Ratio Lower Upper




168 100

99 43.2 40.0 60.0

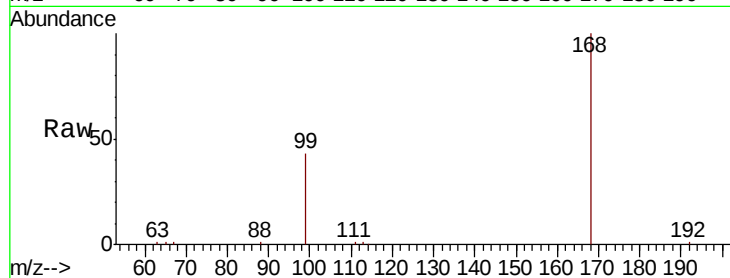

Abundance Ion 168.00 (167.70 to 168.70): V

Ion 99.00 (98.70 to 99.70): VNO

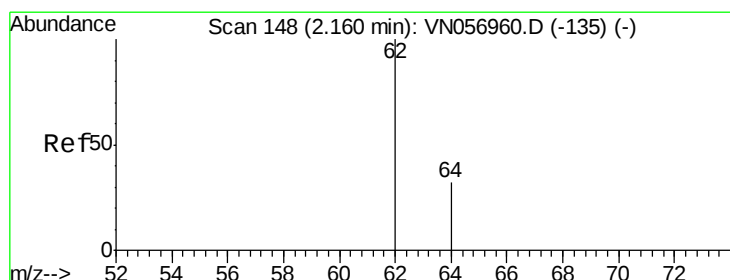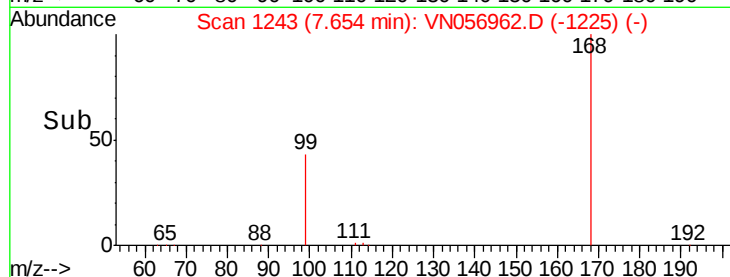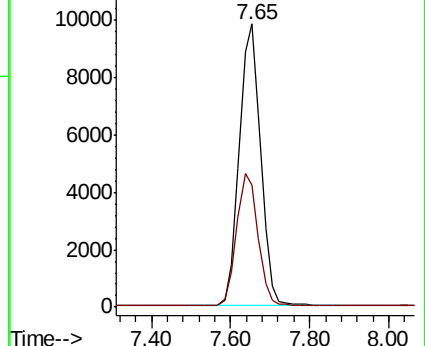

#2

Vinyl Chloride

Concen: 5.250 ug/l

RT: 2.16 min Scan# 148

Delta R.T. -0.00 min

Lab File: VN056962.D


Acq: 29 Jul 2019 19:48

Tgt Ion: 62 Resp: 17823

Ion Ratio Lower Upper



62 100


64 32.6 26.4 39.6

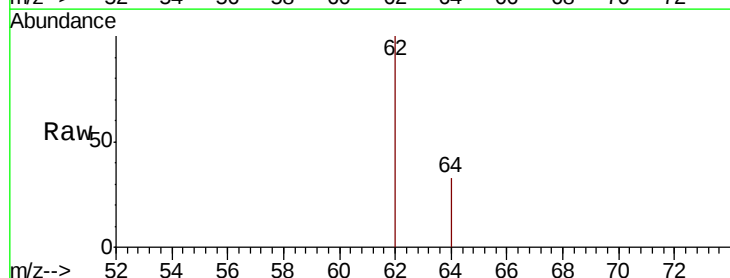

Abundance Ion 62.00 (61.70 to 62.70): VNO

Ion 64.00 (63.70 to 64.70): VNO

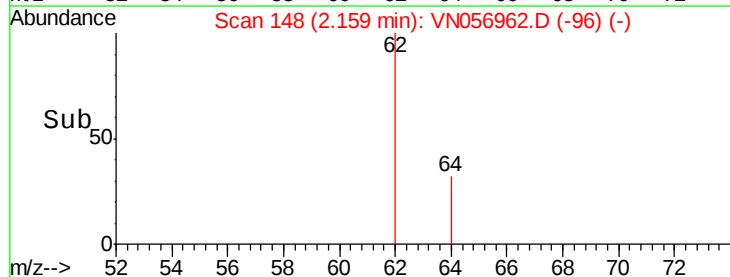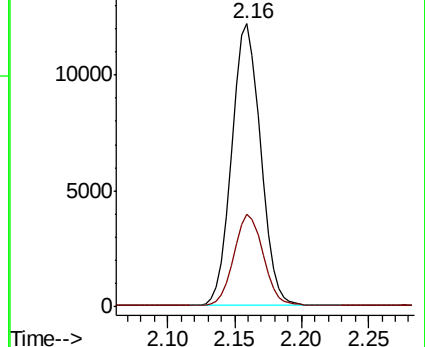

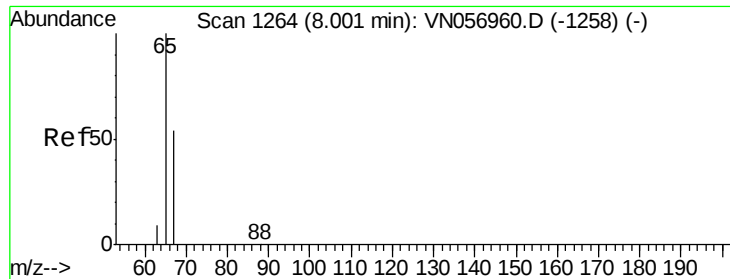

#3

1,2-Dichloroethane-d4

Concen: 4.732 ug/l

RT: 8.00 min Scan# 1263

Delta R.T. -0.00 min

Lab File: VN056962.D

Acq: 29 Jul 2019 19:48

Instrument :

MSVOA_N

ClientSampleId :


ICVVN072919

Tot Ion: 65 Resp: 21563

Ion Ratio Lower Upper




65 100

67 54.0 0.0 109.6

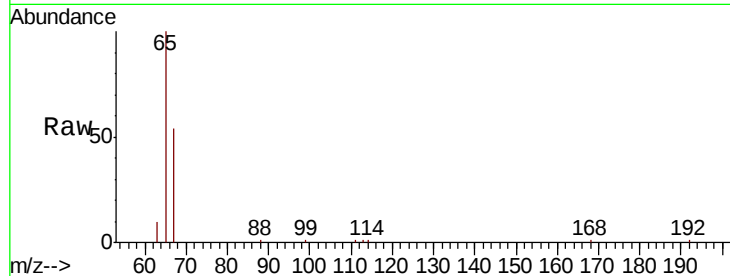

Abundance Ion 65.00 (64.70 to 65.70): VN056960.D (-1258) (-)

Ion 67.00 (66.70 to 67.70): VN056960.D (-1258) (-)

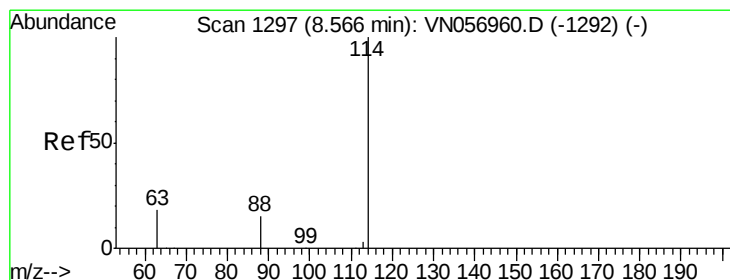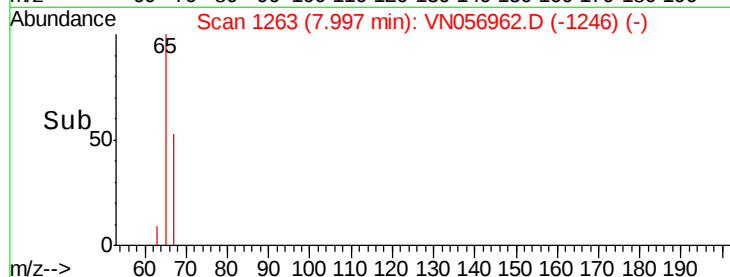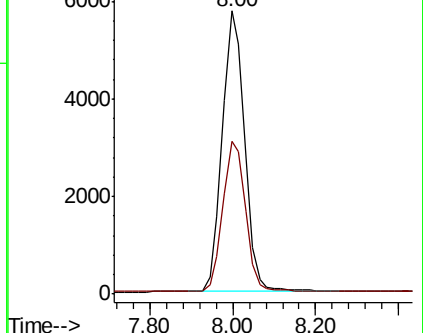

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.58 min Scan# 1297

Delta R.T. 0.01 min

Lab File: VN056962.D

Acq: 29 Jul 2019 19:48


Tgt Ion: 114 Resp: 51197

Ion Ratio Lower Upper

114 100

63 14.5 0.0 37.6



88 13.5 0.0 31.0

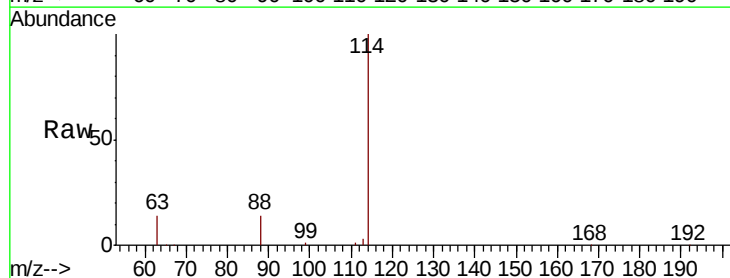


Abundance Ion 114.00 (113.70 to 114.70): VN056960.D (-1292) (-)

Ion 63.00 (62.70 to 63.70): VN056960.D (-1292) (-)

Ion 88.00 (87.70 to 88.70): VN056960.D (-1292) (-)

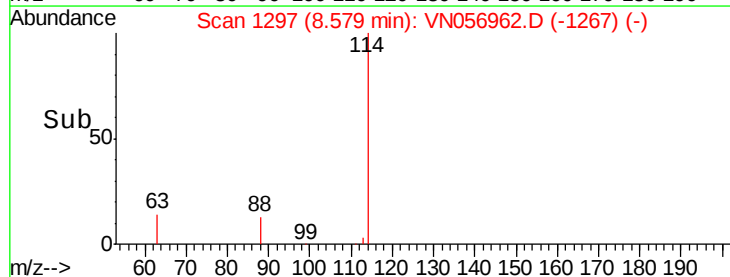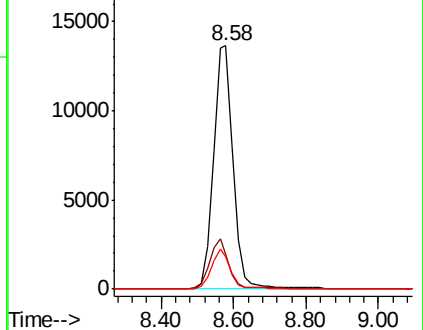

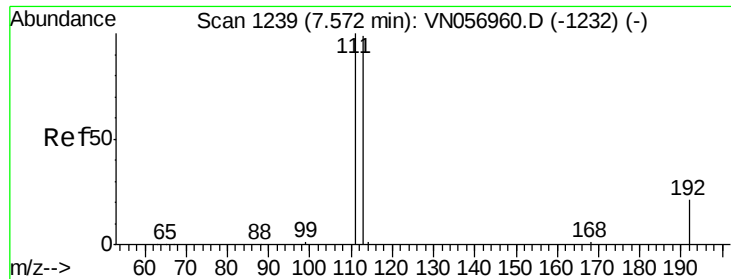

#5

Dibromofluoromethane

Concen: 5.235 ug/l

RT: 7.57 min Scan# 1238

Delta R.T. -0.00 min

Lab File: VN056962.D

Acq: 29 Jul 2019 19:48

Instrument :

MSVOA_N

ClientSampleId :

ICVVN072919


Tot Ion:113 Resp: 18206

Ion Ratio Lower Upper

113 100

111 102.6 81.1 121.7




192 21.4 17.9 26.9

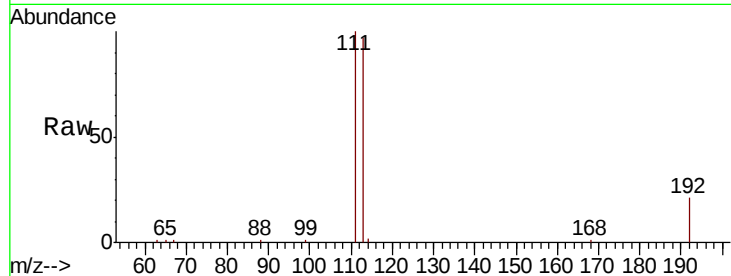

Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V

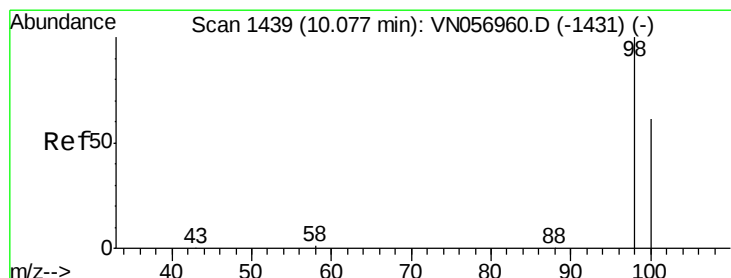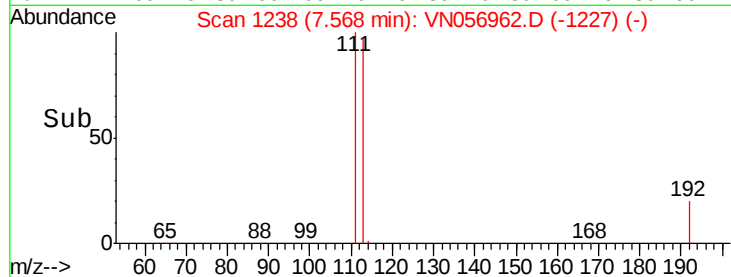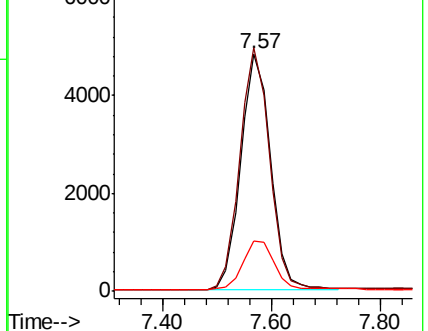

#6

Toluene-d8

Concen: 5.191 ug/l

RT: 10.08 min Scan# 1439

Delta R.T. 0.00 min

Lab File: VN056962.D


Acq: 29 Jul 2019 19:48

Tgt Ion: 98 Resp: 36846

Ion Ratio Lower Upper



98 100


100 62.7 49.0 73.4

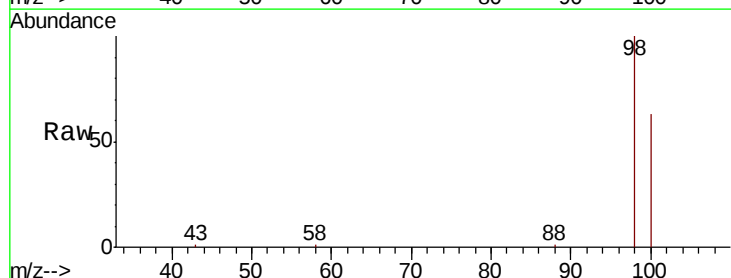

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0

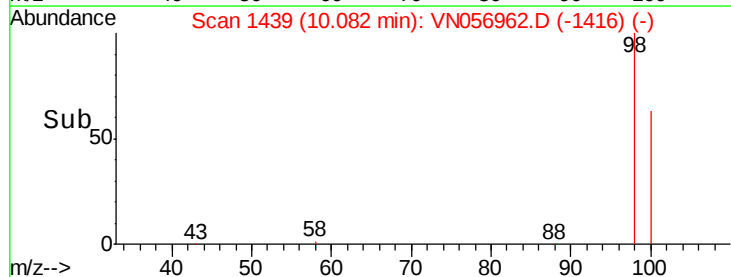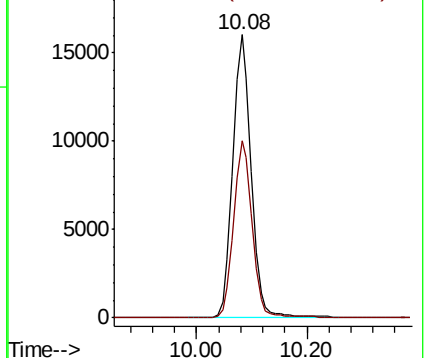

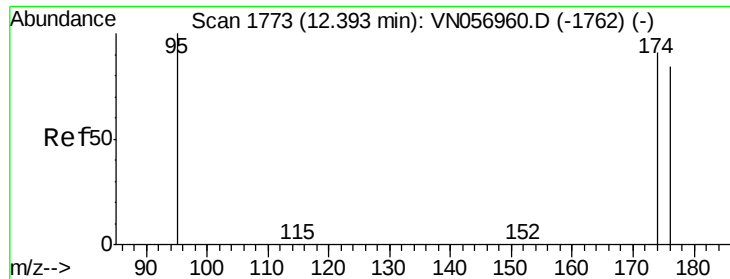

#7

4-Bromofluorobenzene

Concen: 5.284 ug/l

RT: 12.39 min Scan# 1772

Delta R.T. -0.01 min

Lab File: VN056962.D

Acq: 29 Jul 2019 19:48

Instrument :

MSVOA_N

ClientSampleId :

ICVVN072919


Tot Ion: 95 Resp: 8754

Ion Ratio Lower Upper

95 100

174 77.0 0.0 181.4




176 67.1 0.0 168.2

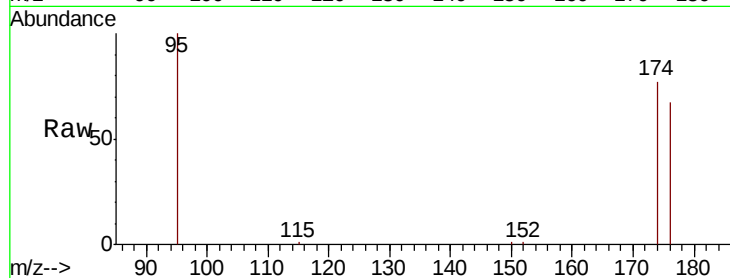

Abundance Ion 95.00 (94.70 to 95.70): VN056962.D (-1762) (-)

Ion 174.00 (173.70 to 174.70): VN056962.D (-1762) (-)

Ion 176.00 (175.70 to 176.70): VN056962.D (-1762) (-)

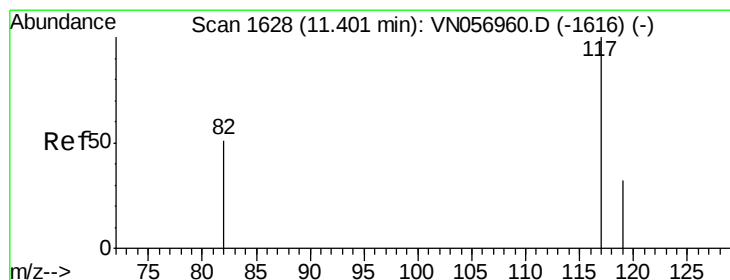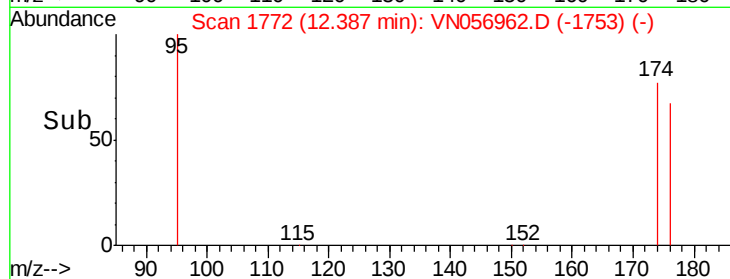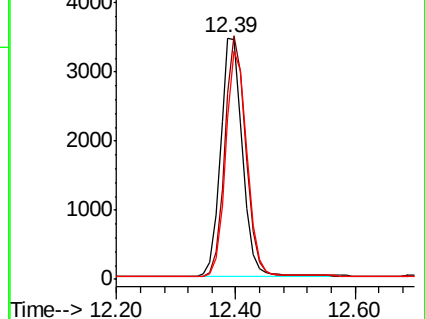

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.40 min Scan# 1627

Delta R.T. -0.00 min

Lab File: VN056962.D

Acq: 29 Jul 2019 19:48


Tgt Ion: 117 Resp: 35168

Ion Ratio Lower Upper

117 100

82 52.1 40.7 61.1



119 31.8 25.6 38.4



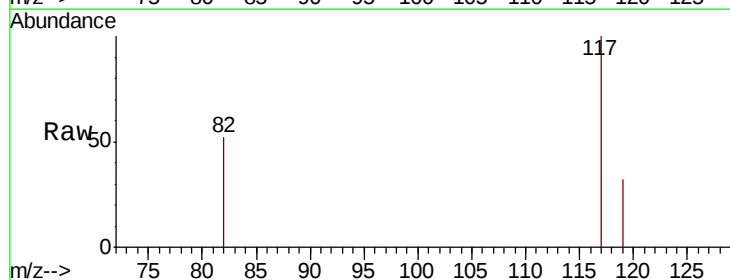


Abundance Ion 117.00 (116.70 to 117.70): VN056962.D (-1590) (-)

Ion 82.00 (81.70 to 82.70): VN056962.D (-1590) (-)

Ion 119.00 (118.70 to 119.70): VN056962.D (-1590) (-)

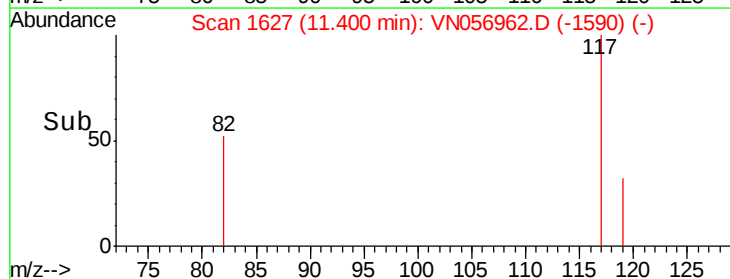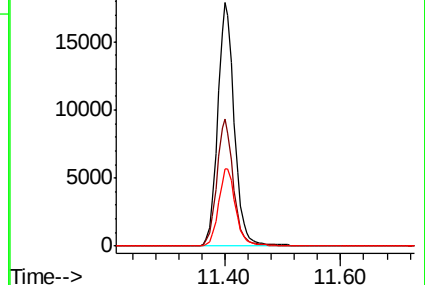

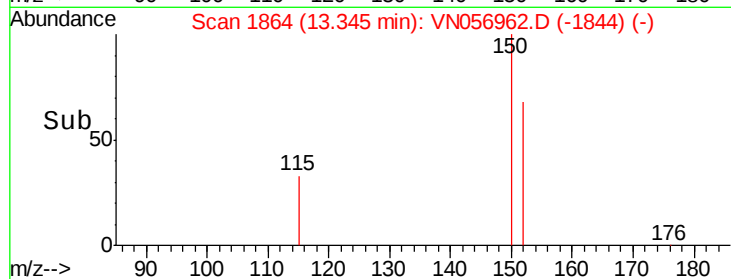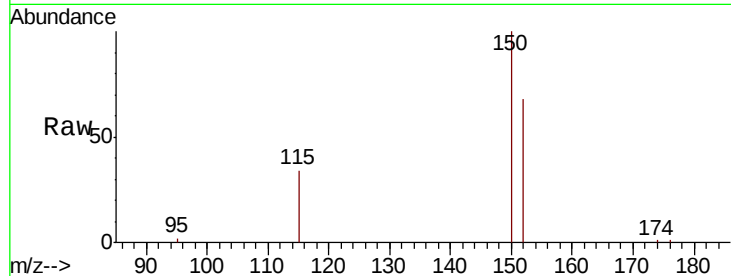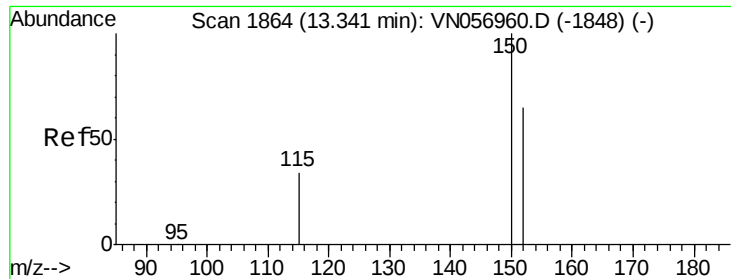

#9

1,4-Dichlorobenzene-d4

Concen: 5.000 ug/l

RT: 13.35 min Scan# 1864

Delta R.T. 0.00 min

Lab File: VN056962.D

Acq: 29 Jul 2019 19:48

Instrument :

MSVOA_N

ClientSampleId :

ICVVN072919

Tot Ion:152 Resp: 5299

Ion Ratio Lower Upper

152 100

115 49.5 27.0 80.8

150 146.3 0.0 306.8

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

