


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072920\
Data File : VN062642.D
Acq On : 29 Jul 2020 8:49
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072120W.M
Title : SW846 8260
Last Update : Tue Jul 21 18:48:59 2020

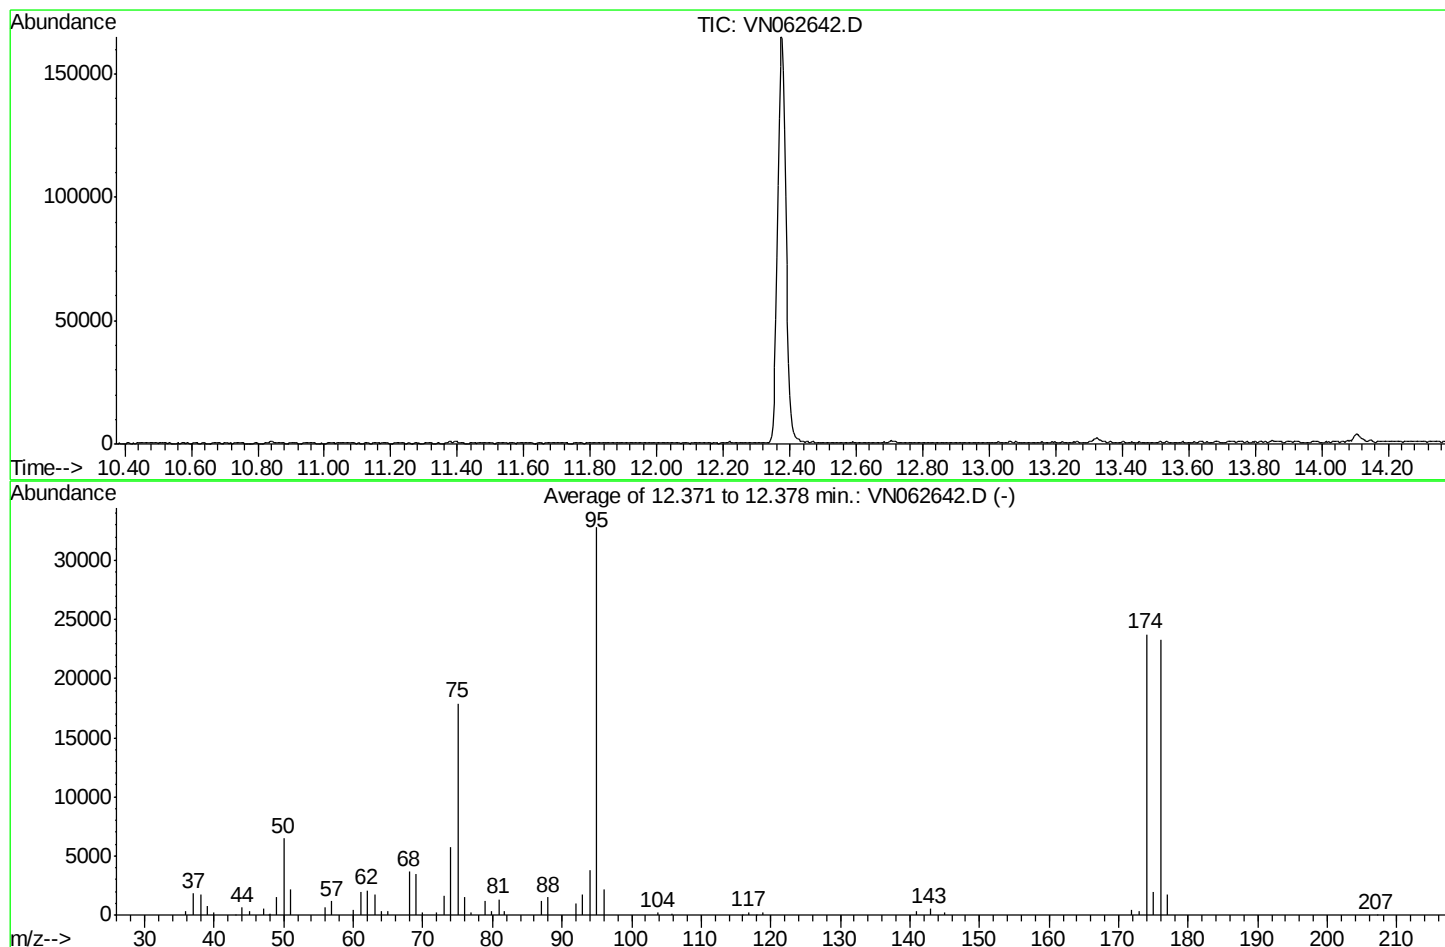

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	6466	PASS
75	95	30	60	54.6	17914	PASS
95	95	100	100	100.0	32810	PASS
96	95	5	9	6.5	2121	PASS
173	174	0.00	2	1.2	282	PASS
174	95	50	100	72.4	23744	PASS
175	174	5	9	8.3	1968	PASS
176	174	95	101	98.0	23258	PASS
177	176	5	9	7.3	1704	PASS