


Methyl Iodide

Response Ratio

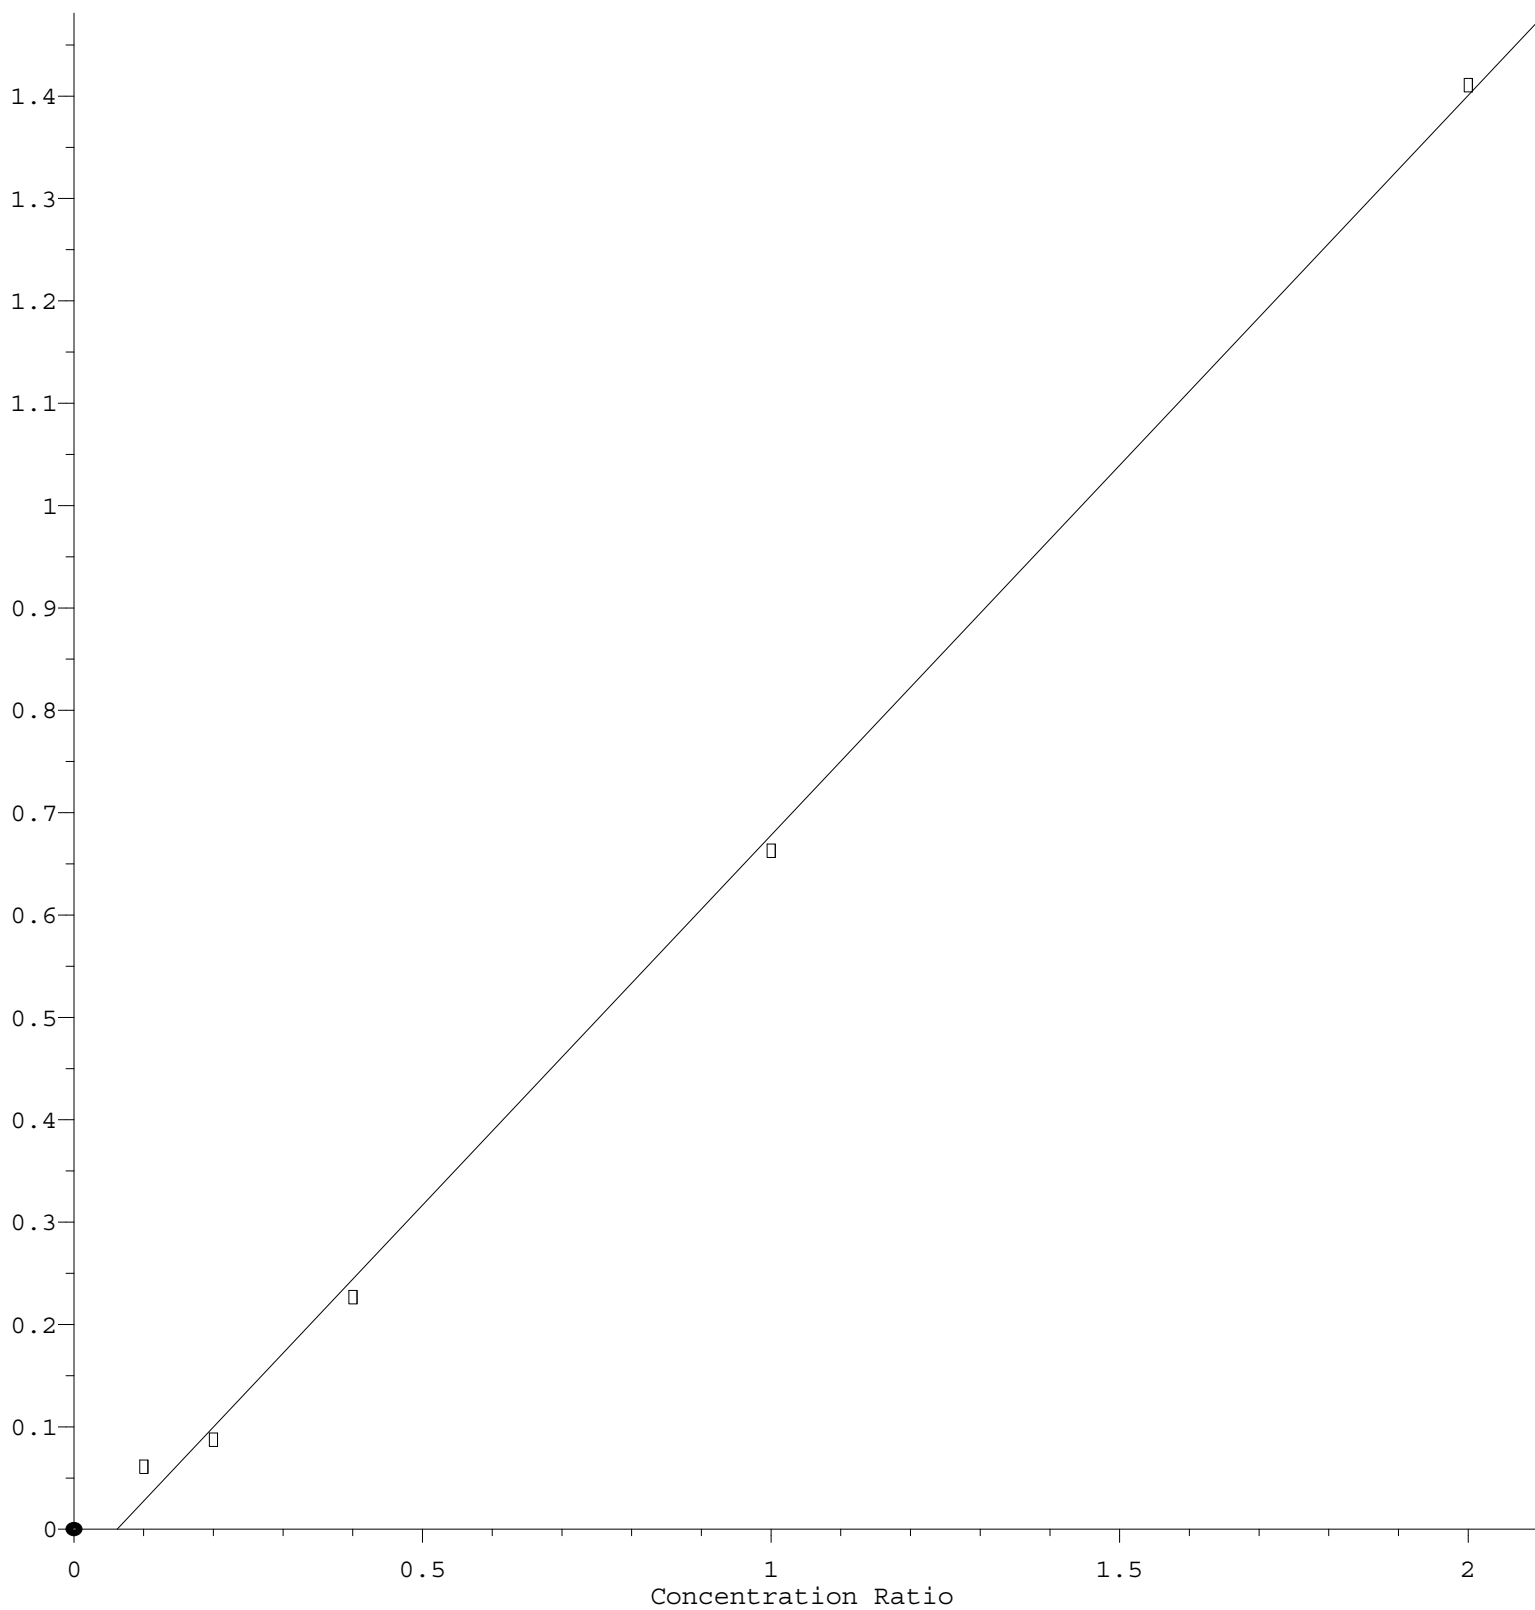

$$\text{Response} = 7.227\text{e-}001 * \text{Amt} - 4.512\text{e-}002$$


Coef of Det (r^2) = 0.998520 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Naphthalene

Response Ratio

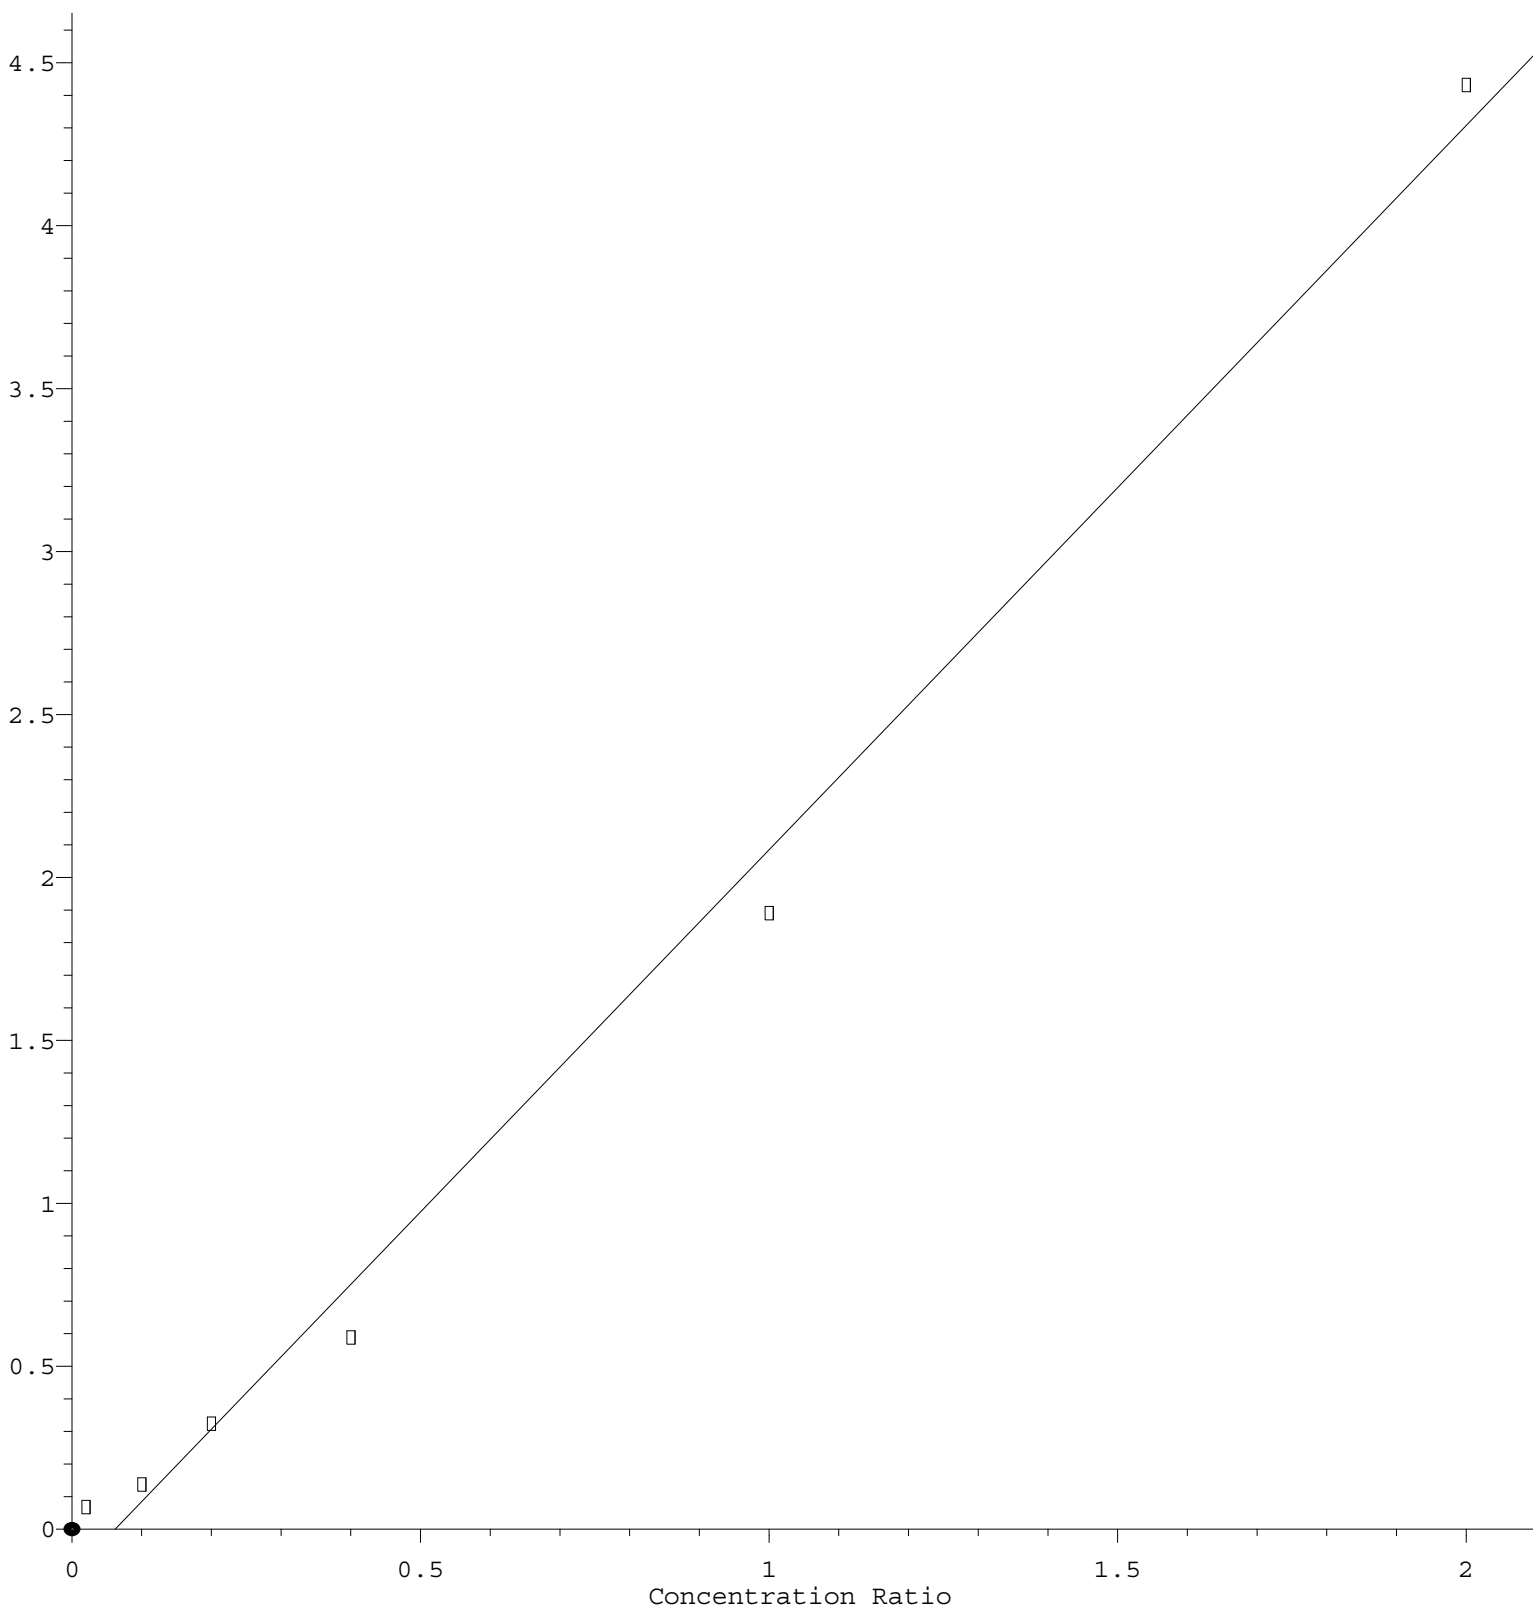

$$\text{Response} = 2.223\text{e}+000 * \text{Amt} - 1.387\text{e}-001$$


Coef of Det (r^2) = 0.992474 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

1,2,3-Trichlorobenzene

Response Ratio

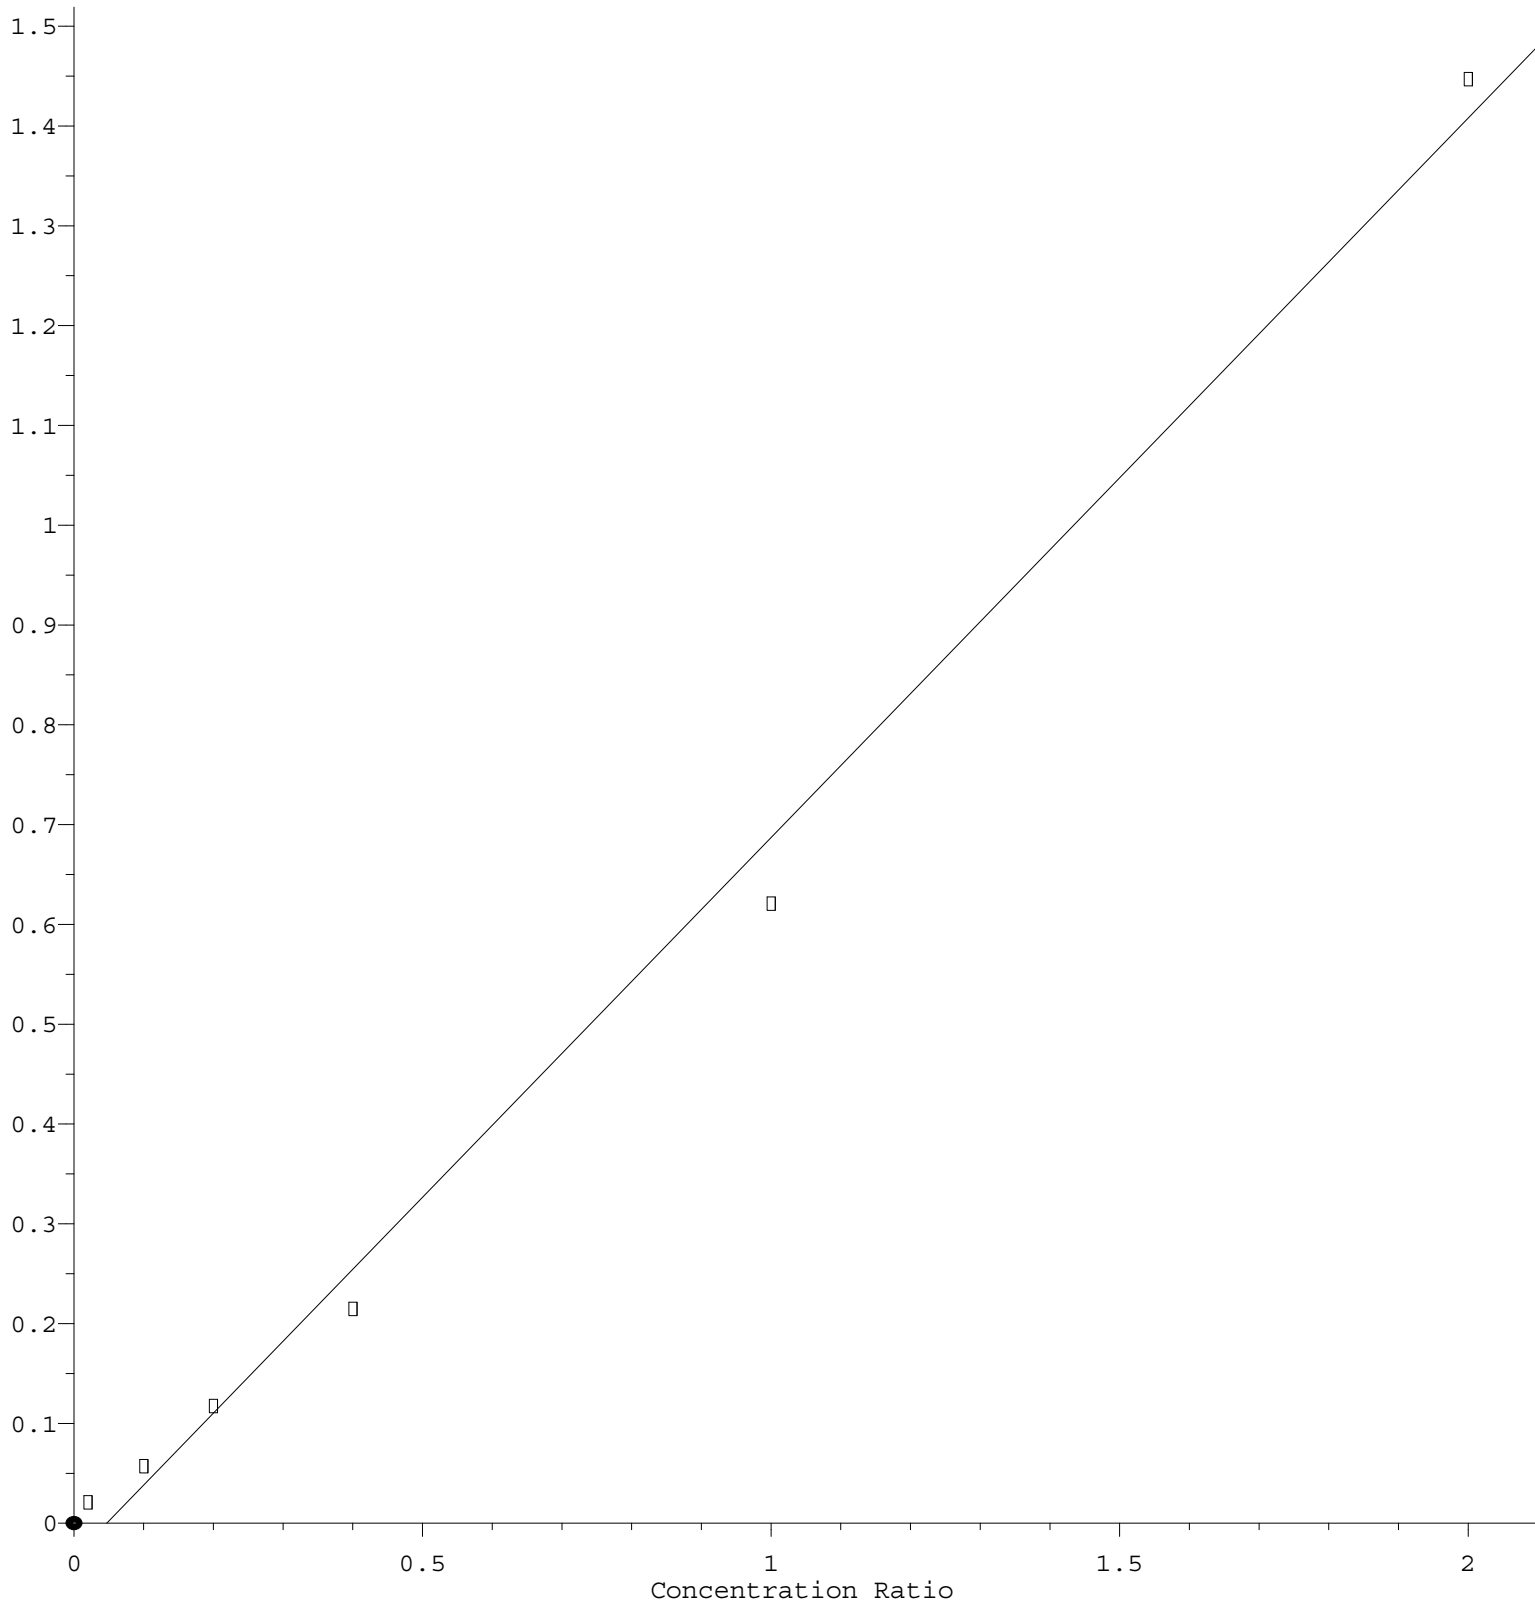

$$\text{Response} = 7.210\text{e-}001 * \text{Amt} - 3.413\text{e-}002$$


Coef of Det (r^2) = 0.993739 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Methyl Acetate

Response Ratio

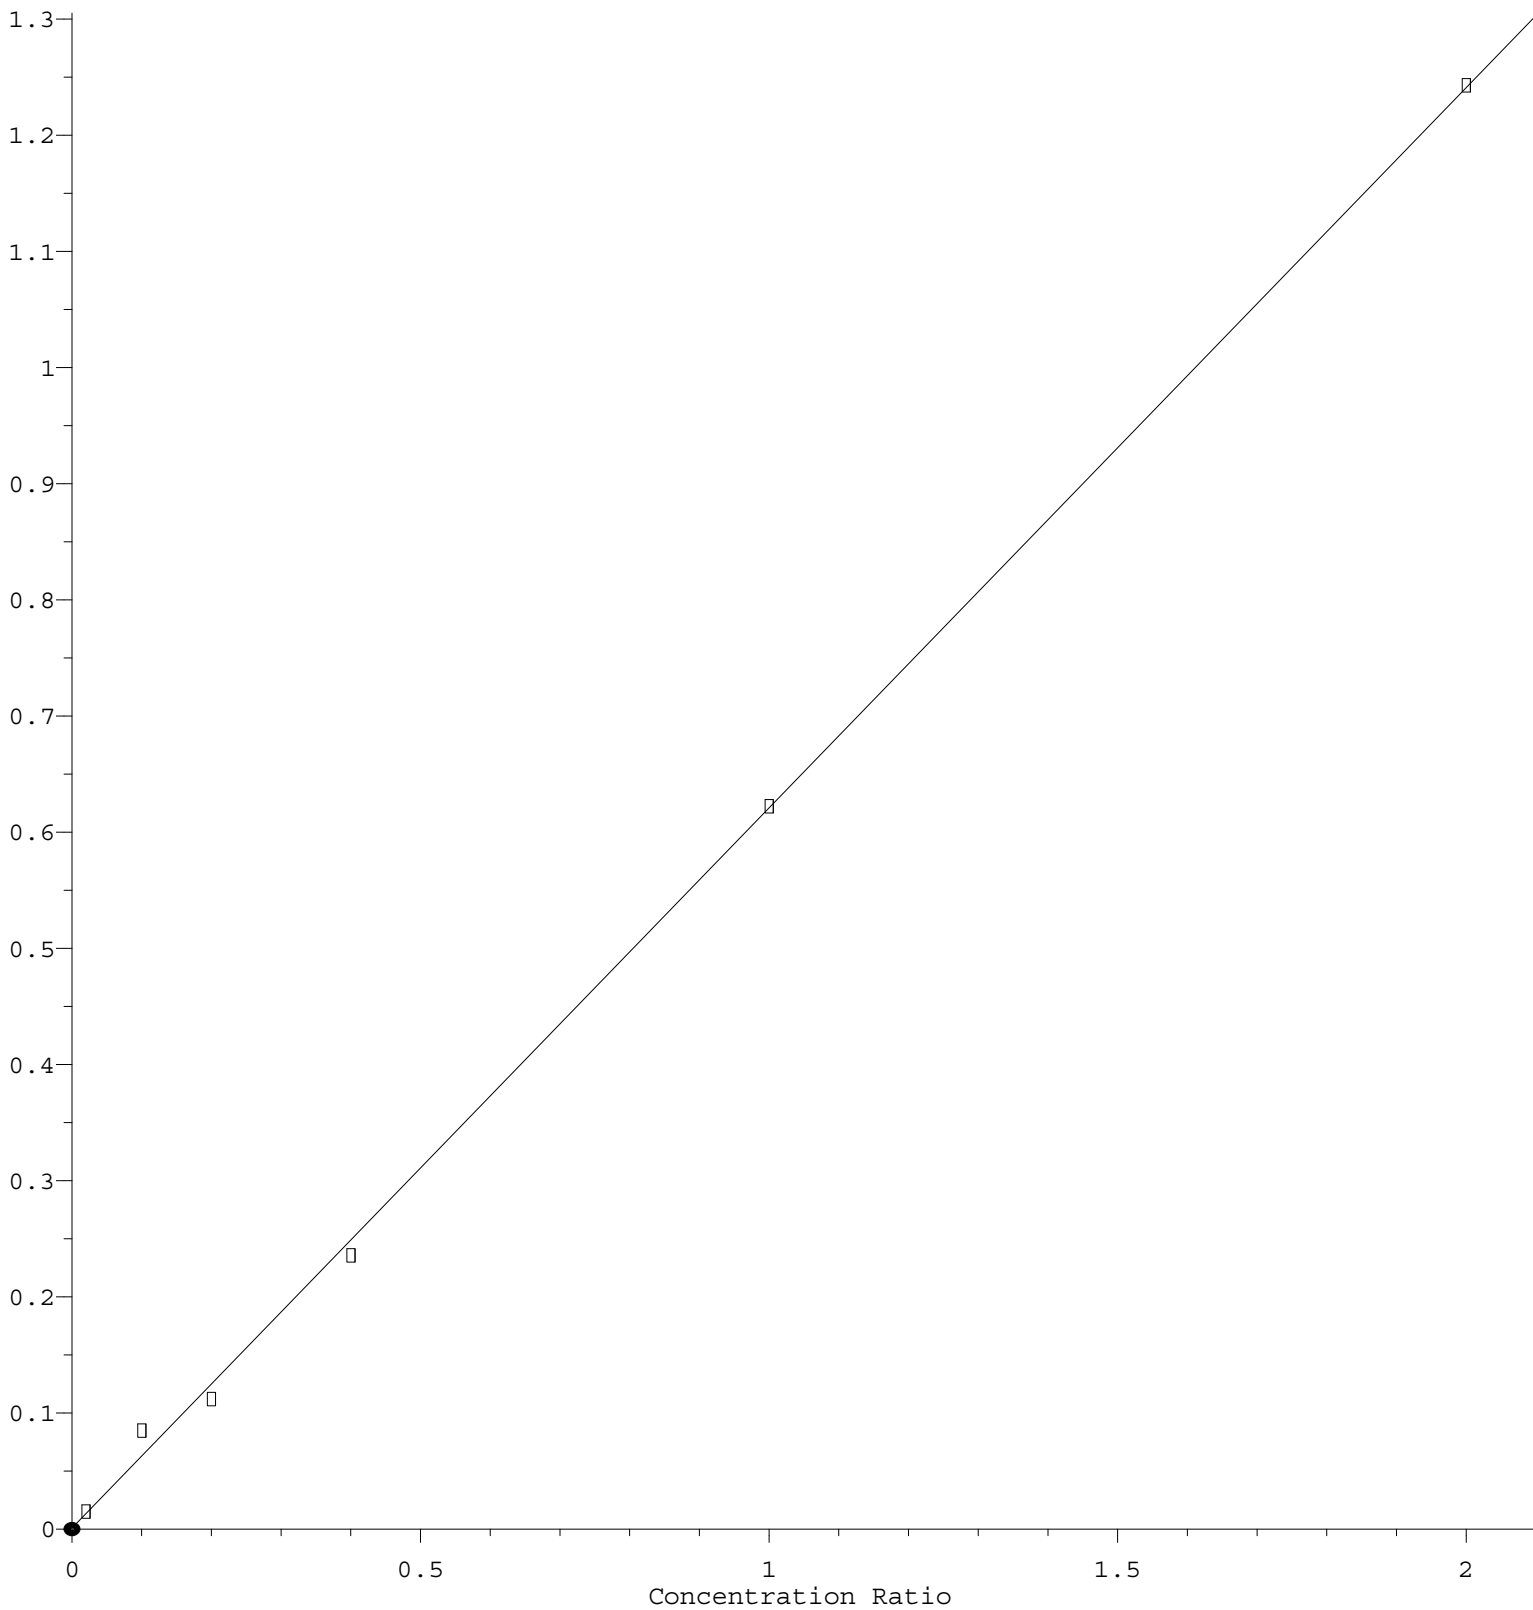

$$\text{Response} = 6.197\text{e-}001 * \text{Amt} + 1.271\text{e-}003$$


Coef of Det (r^2) = 0.999252 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Methylene Chloride

Response Ratio

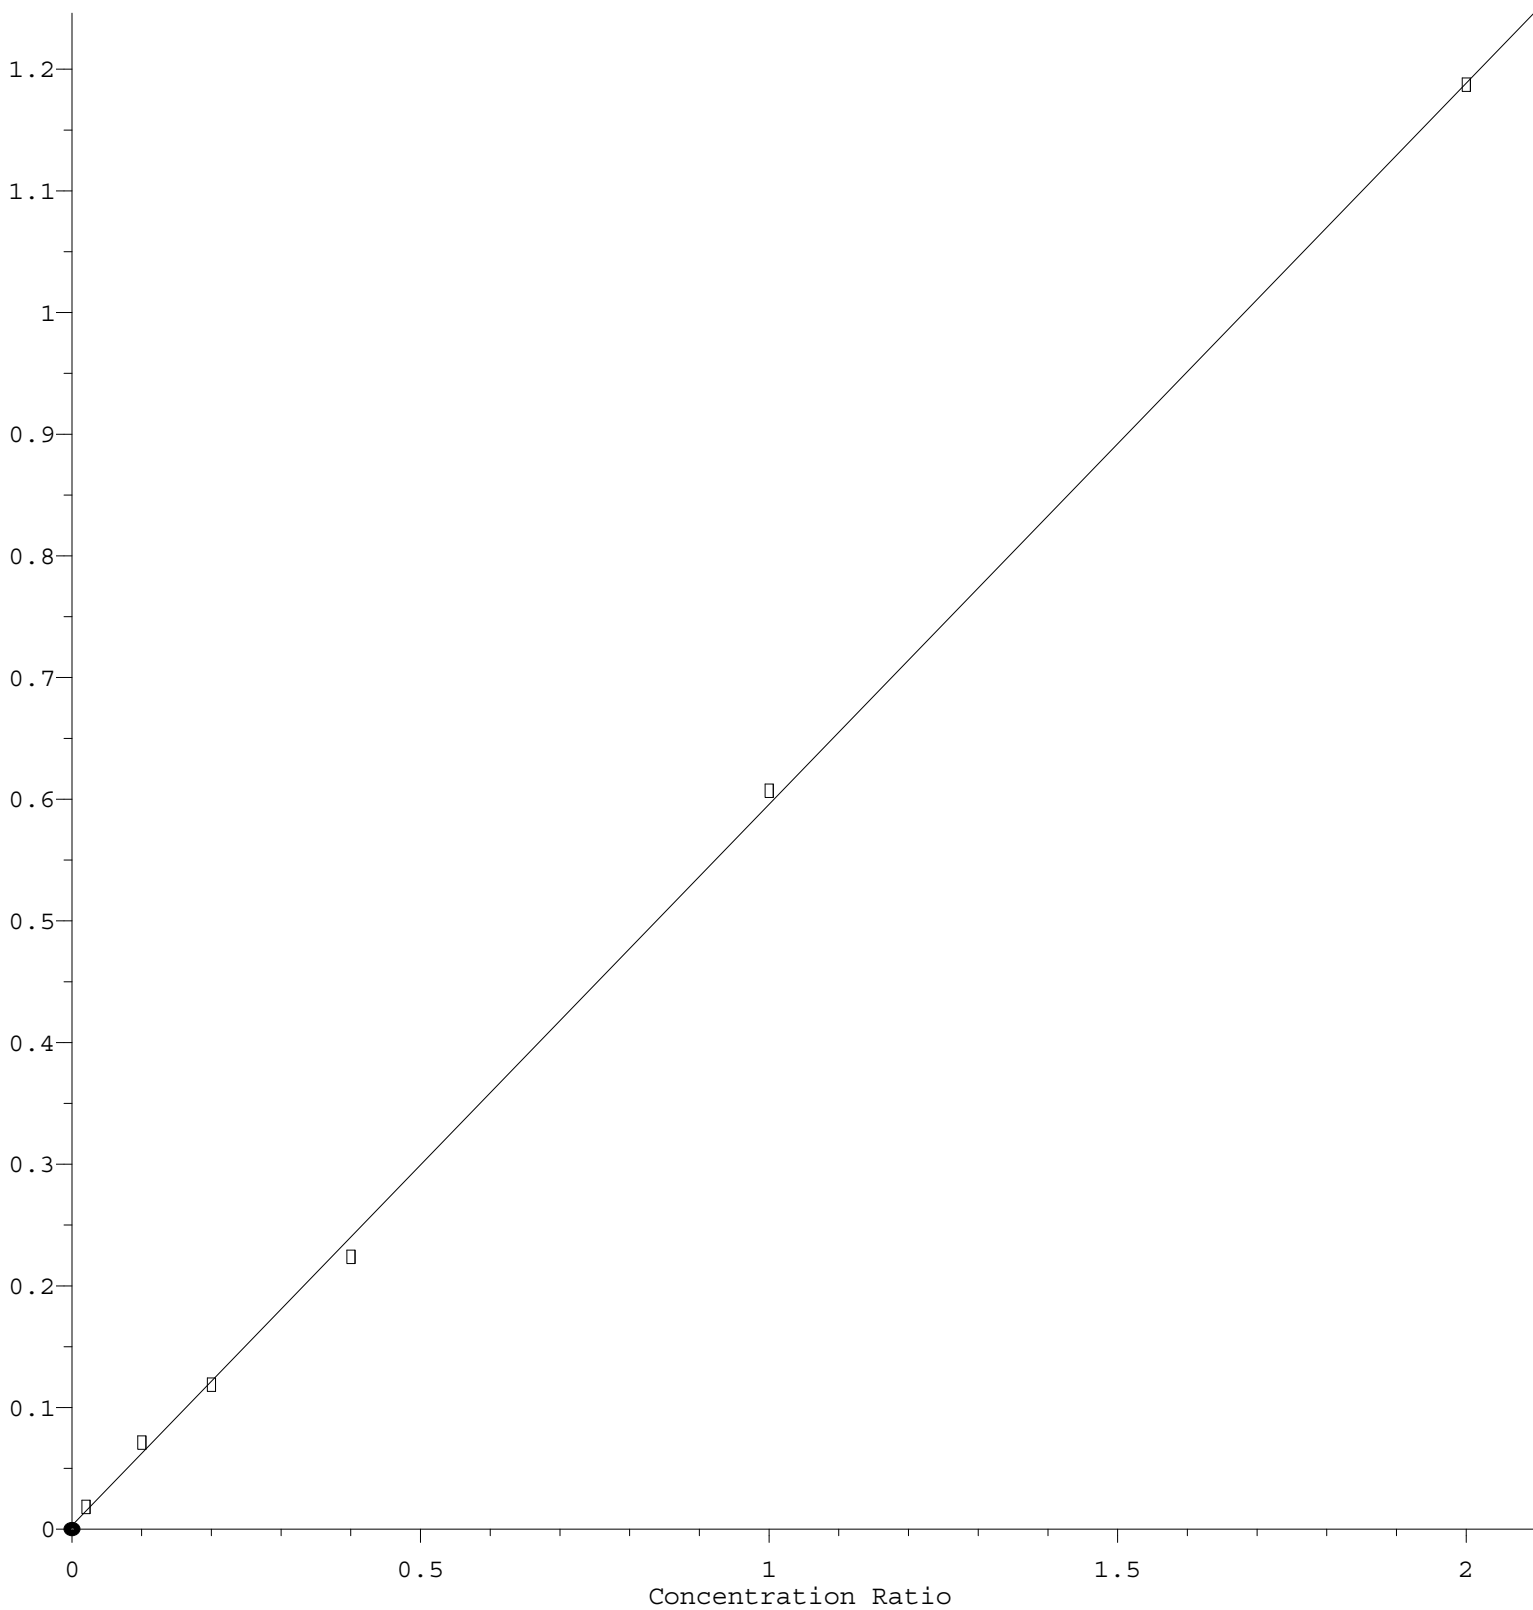

$$\text{Response} = 5.930\text{e-}001 * \text{Amt} + 3.392\text{e-}003$$


Coef of Det (r^2) = 0.999521 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Vinyl Acetate

Response Ratio

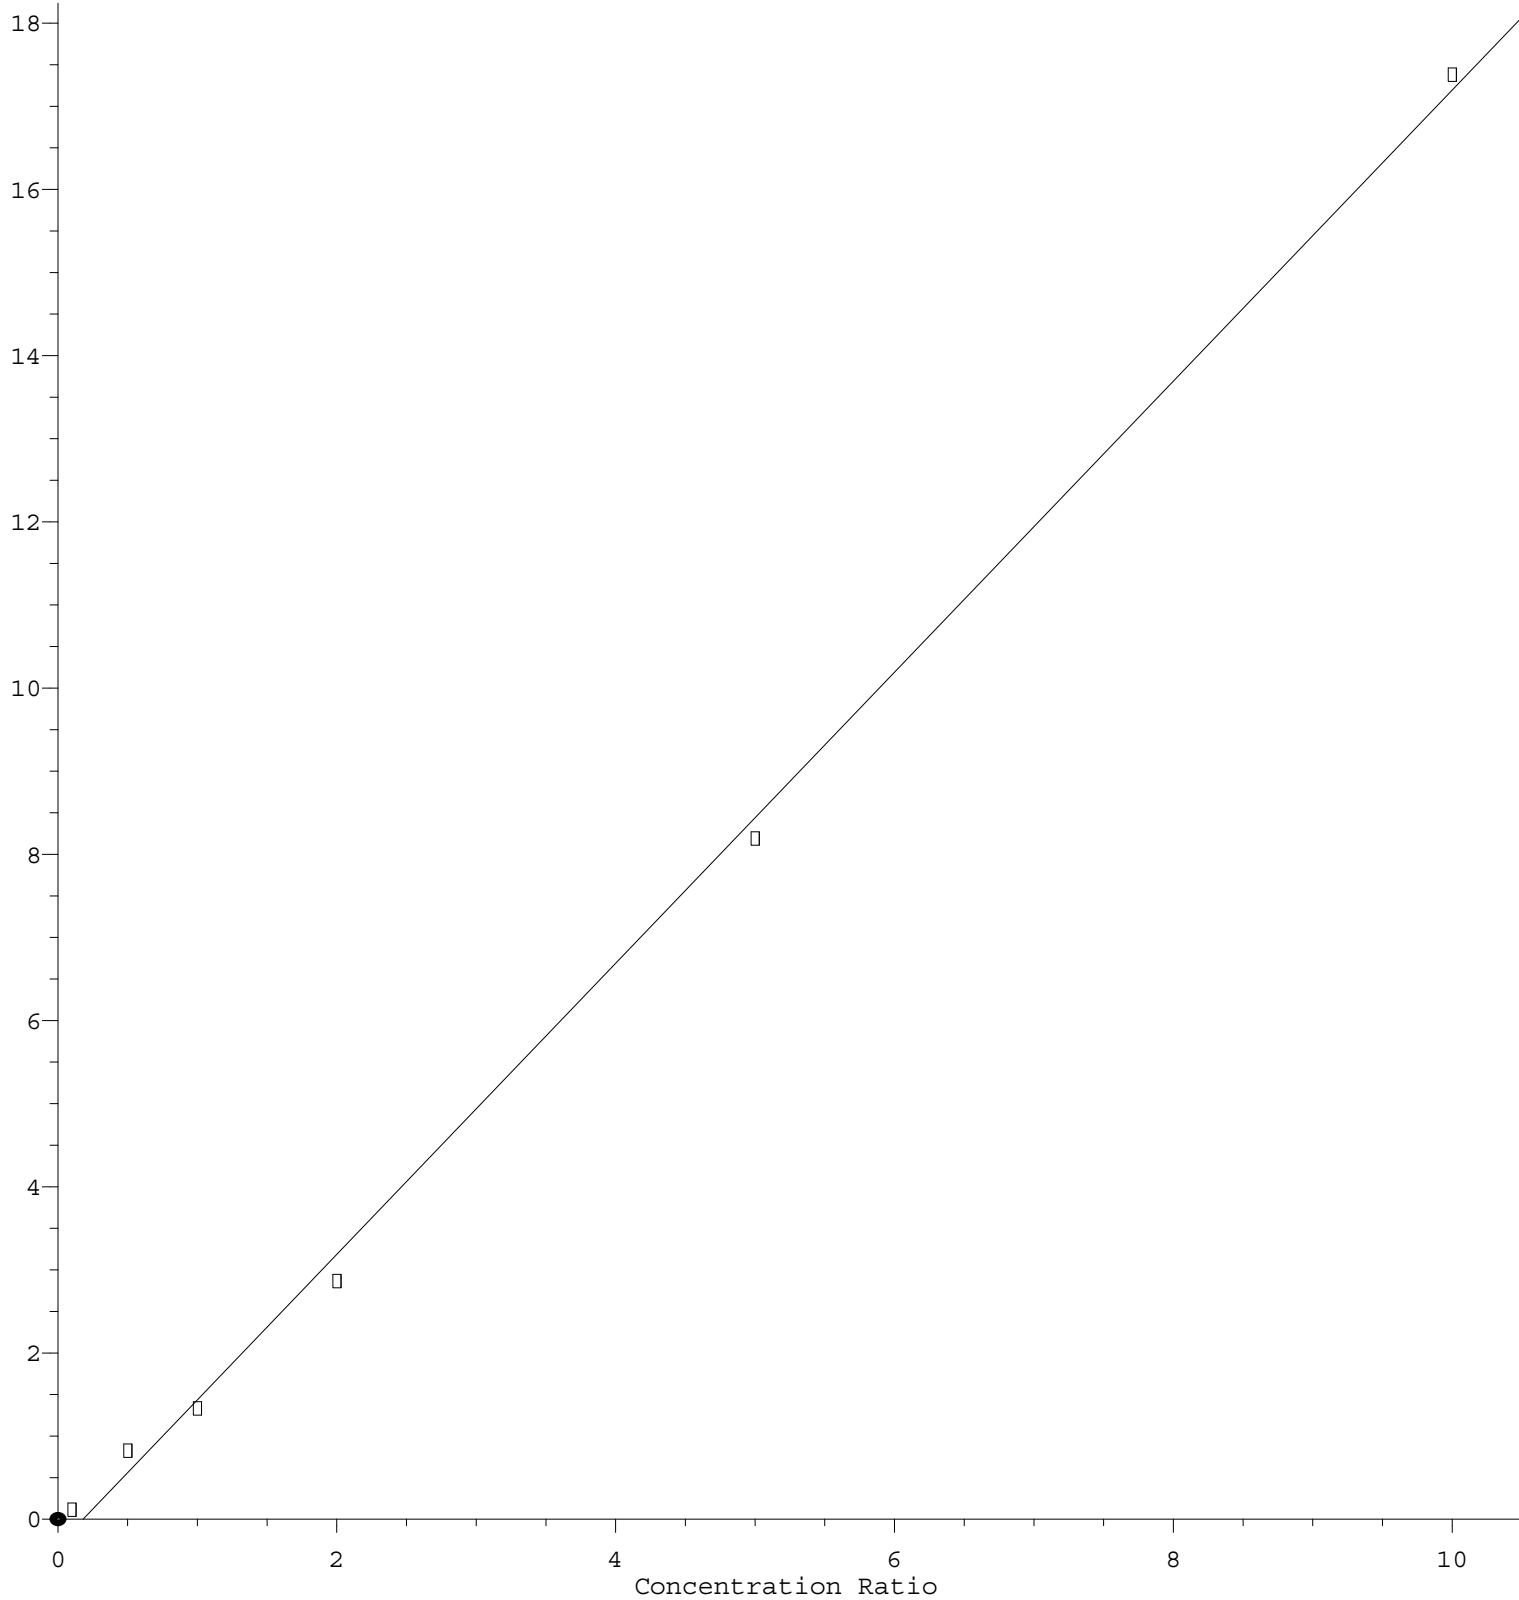


$$\text{Response} = 1.750\text{e}+000 * \text{Amt} - 3.080\text{e}-001$$

Coef of Det (r^2) = 0.998447 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Methyl methacrylate

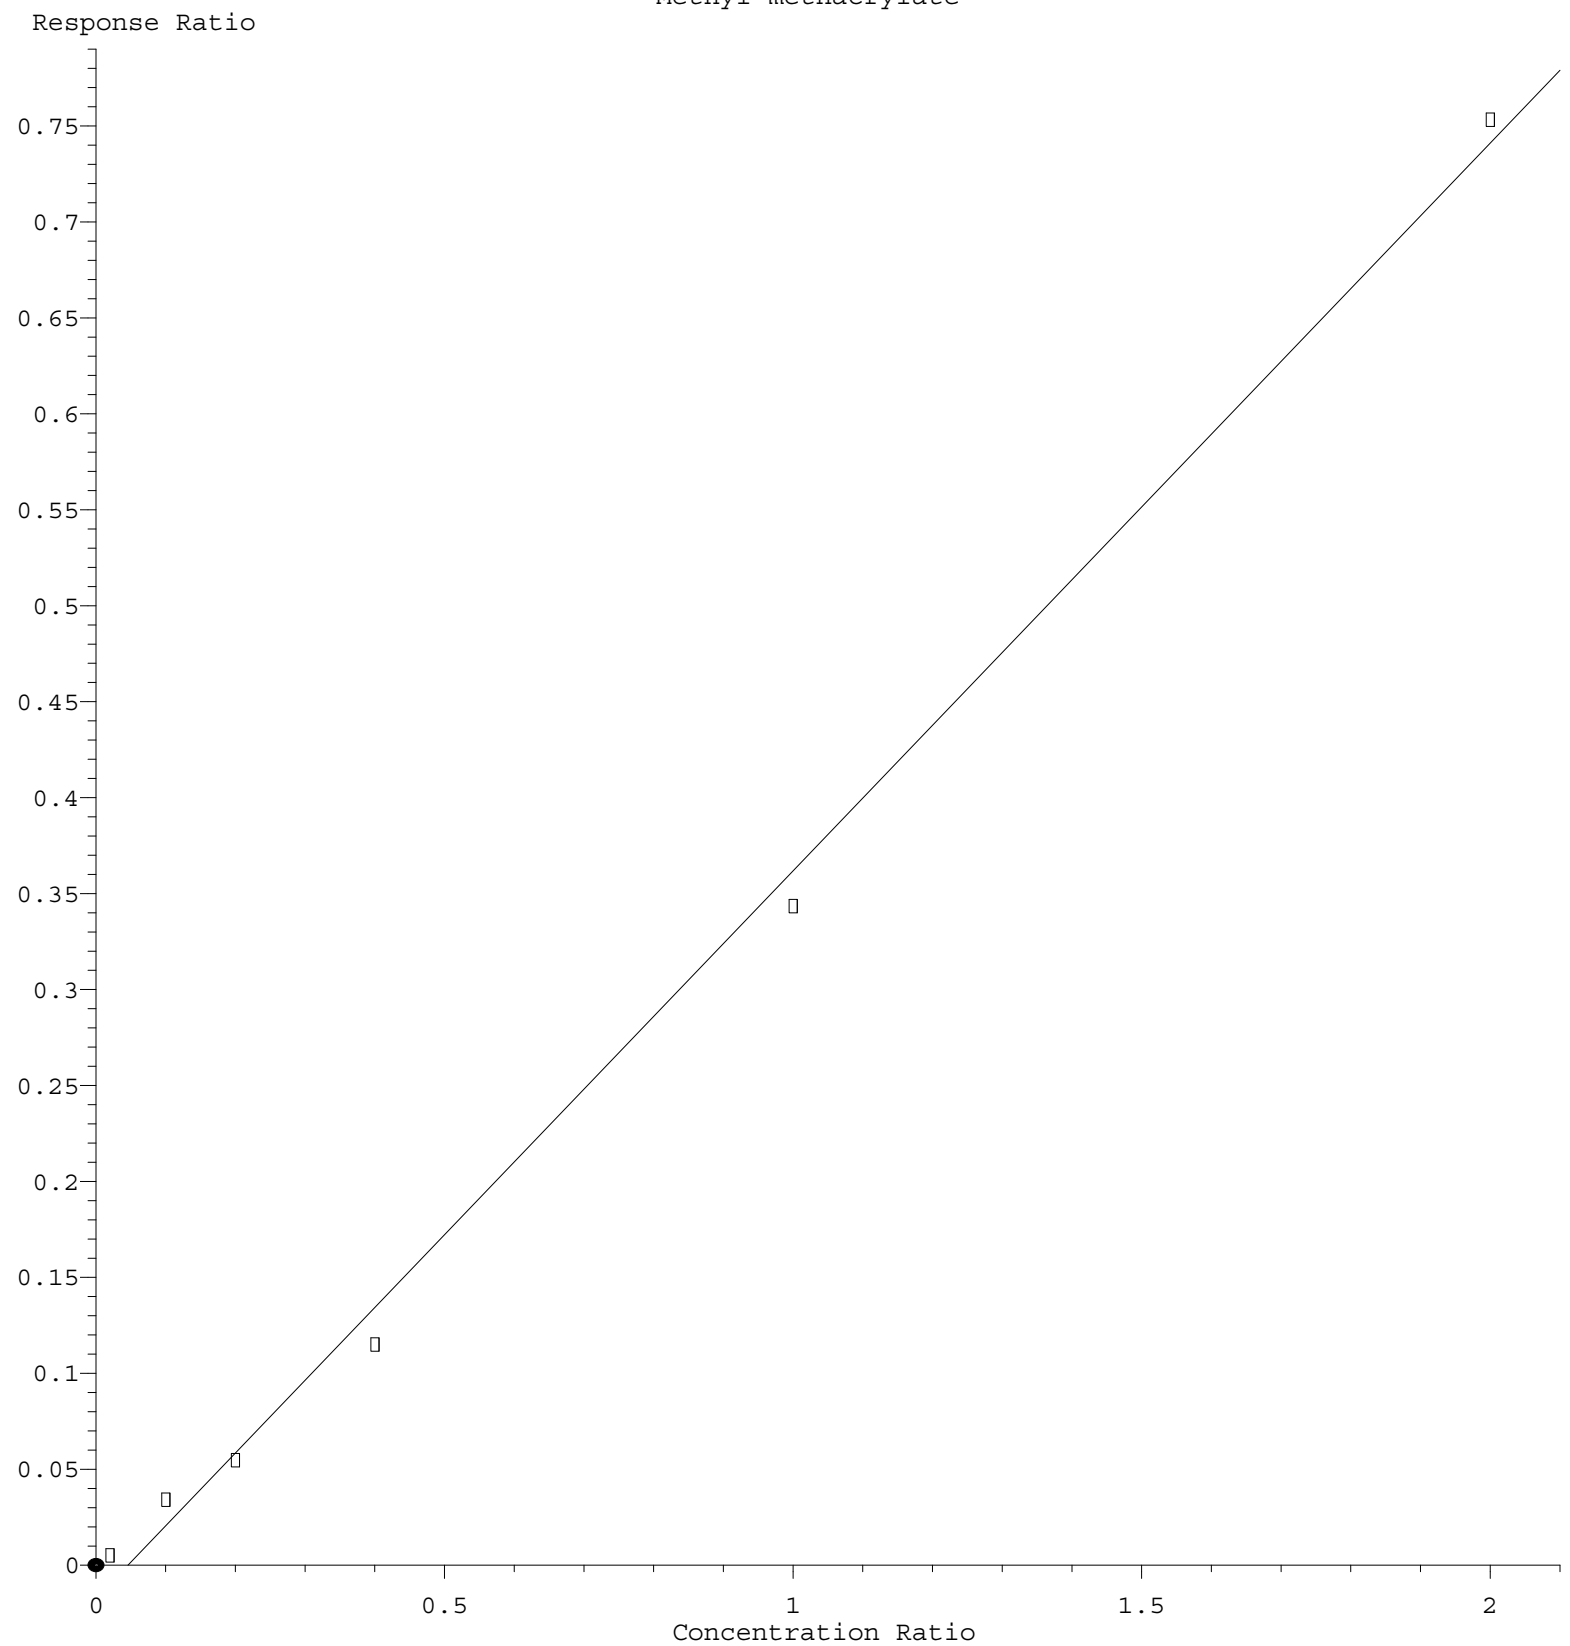

$$\text{Response} = 3.791\text{e-}001 * \text{Amt} - 1.748\text{e-}002$$


Coef of Det (r^2) = 0.996937 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Toluene-d8


Response Ratio

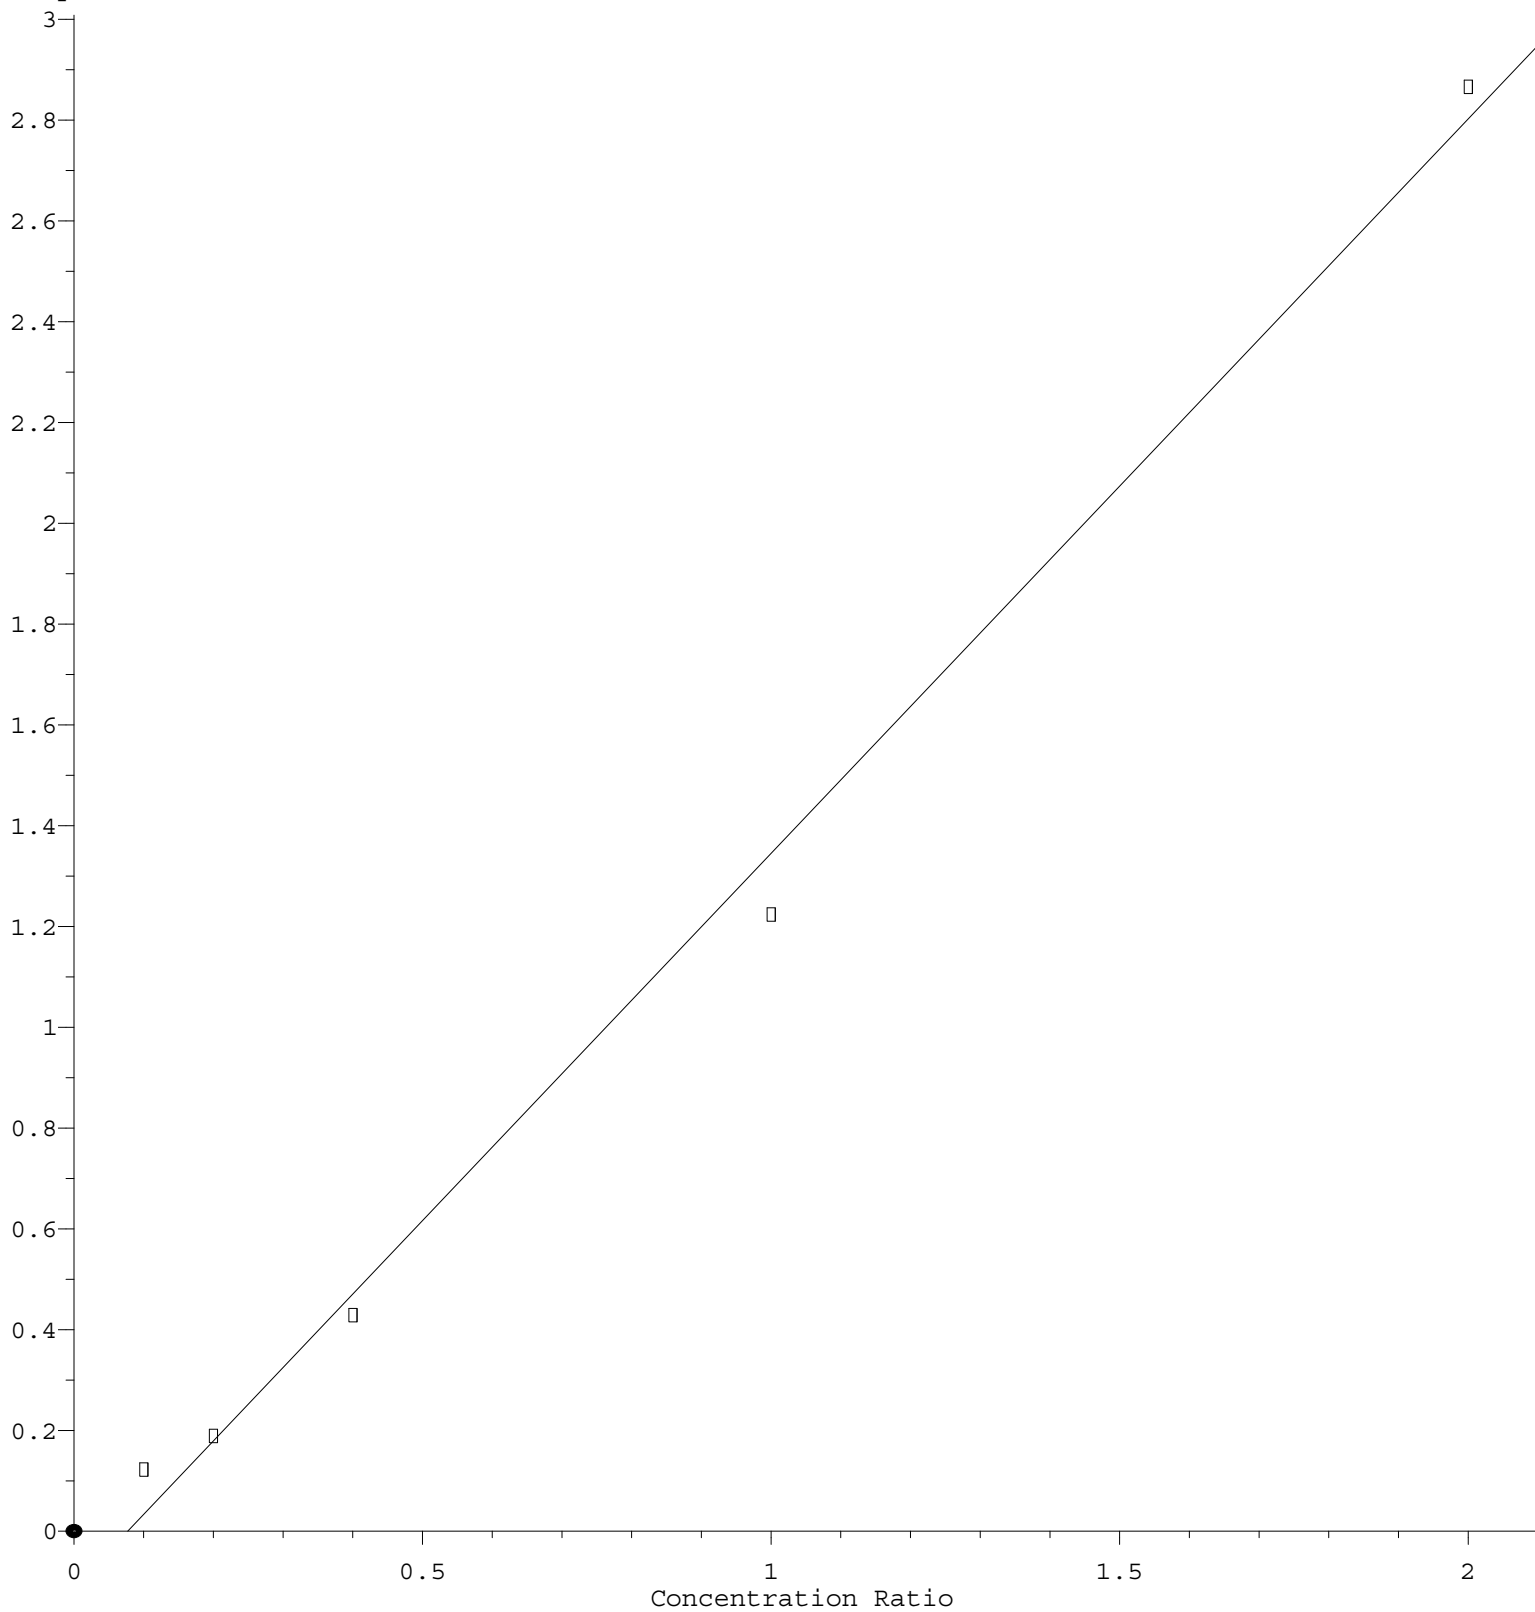

Response = 1.457e+000 * Amt - 1.126e-001
Coef of Det (r^2) = 0.994601 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M
Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

4-Methyl-2-Pentanone

Response Ratio

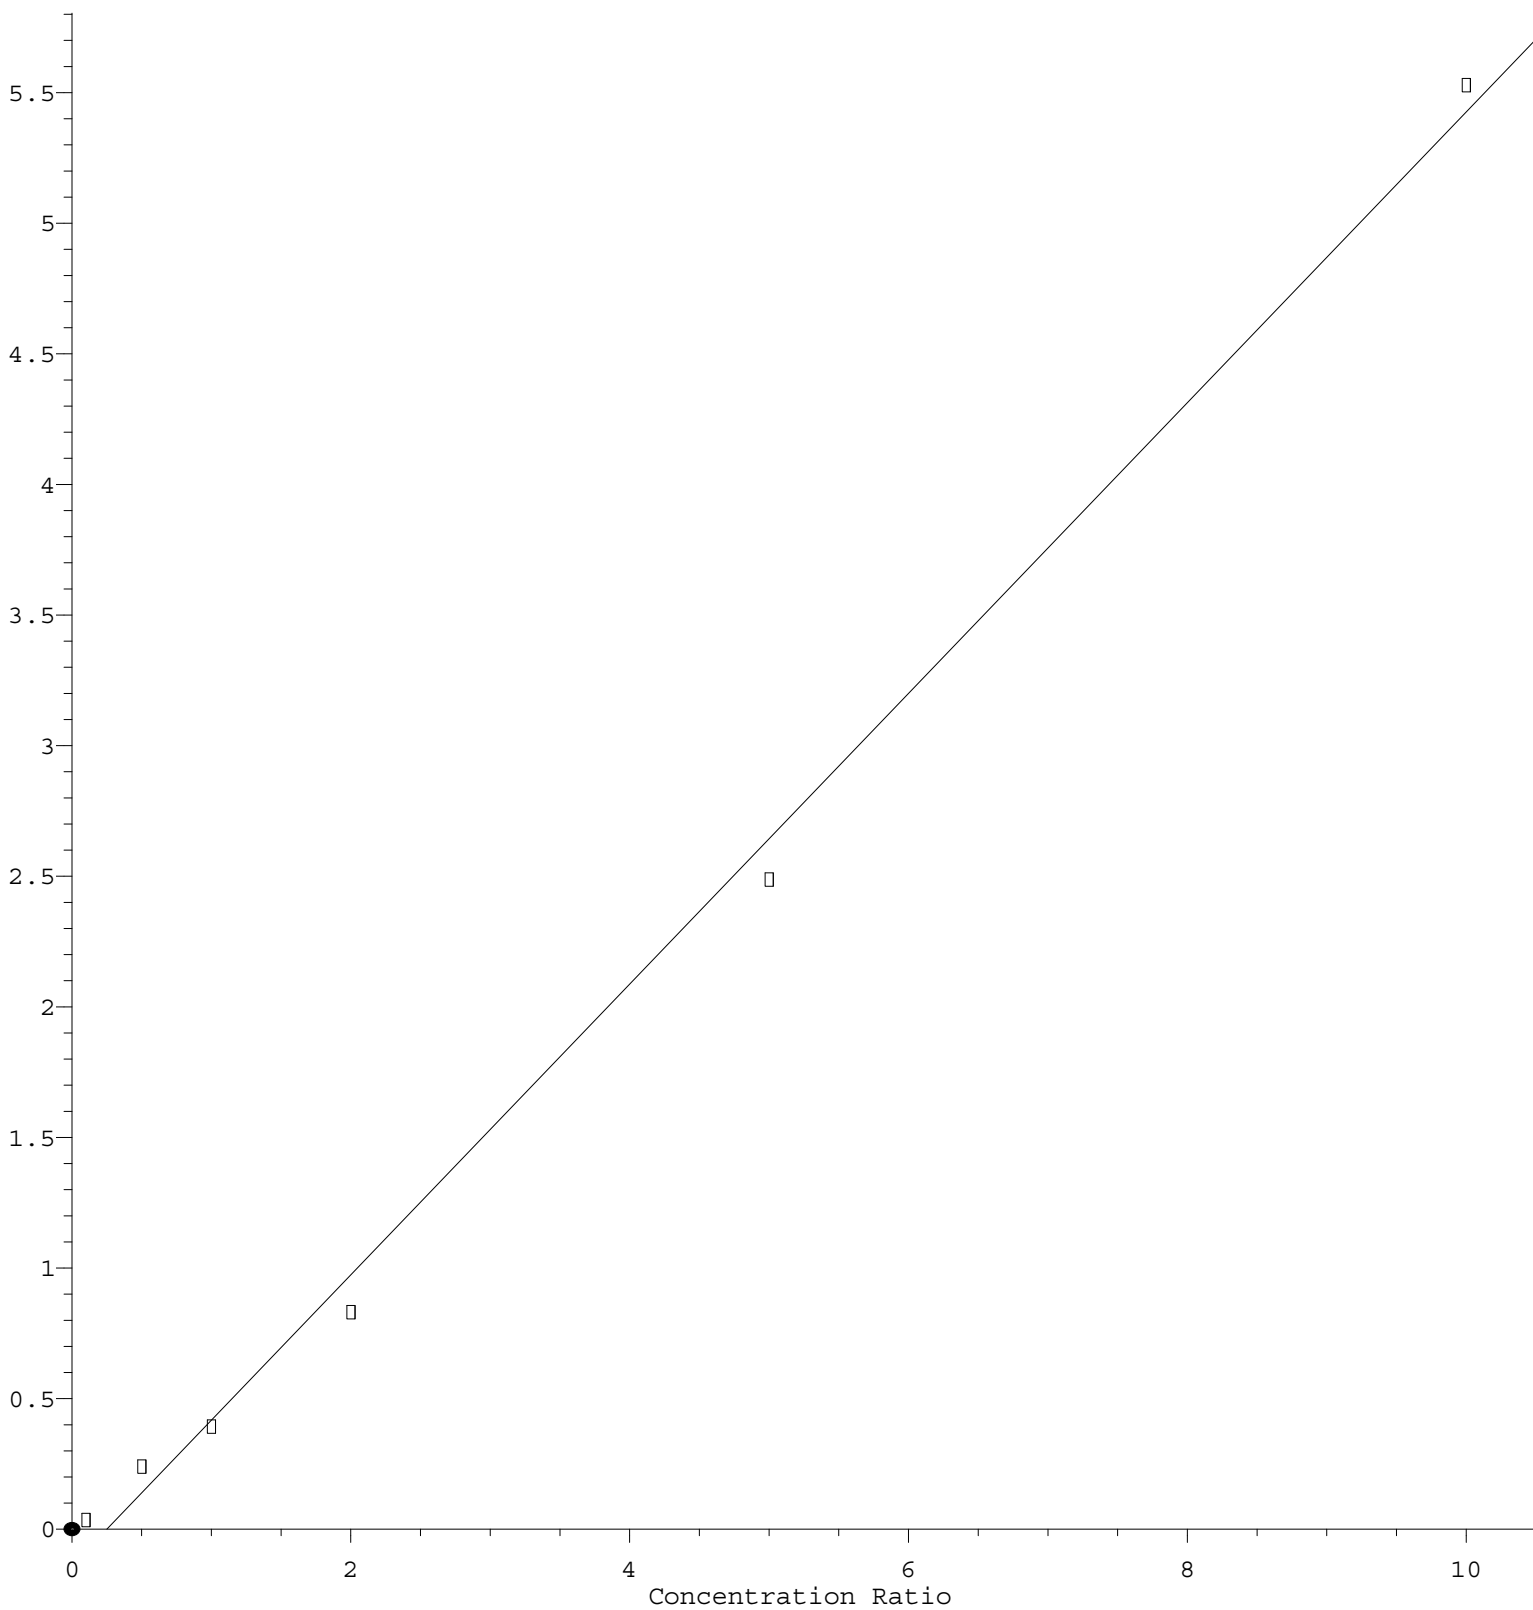

$$\text{Response} = 5.566\text{e-}001 * \text{Amt} - 1.399\text{e-}001$$


Coef of Det (r^2) = 0.996443 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

t-1,3-Dichloropropene

Response Ratio

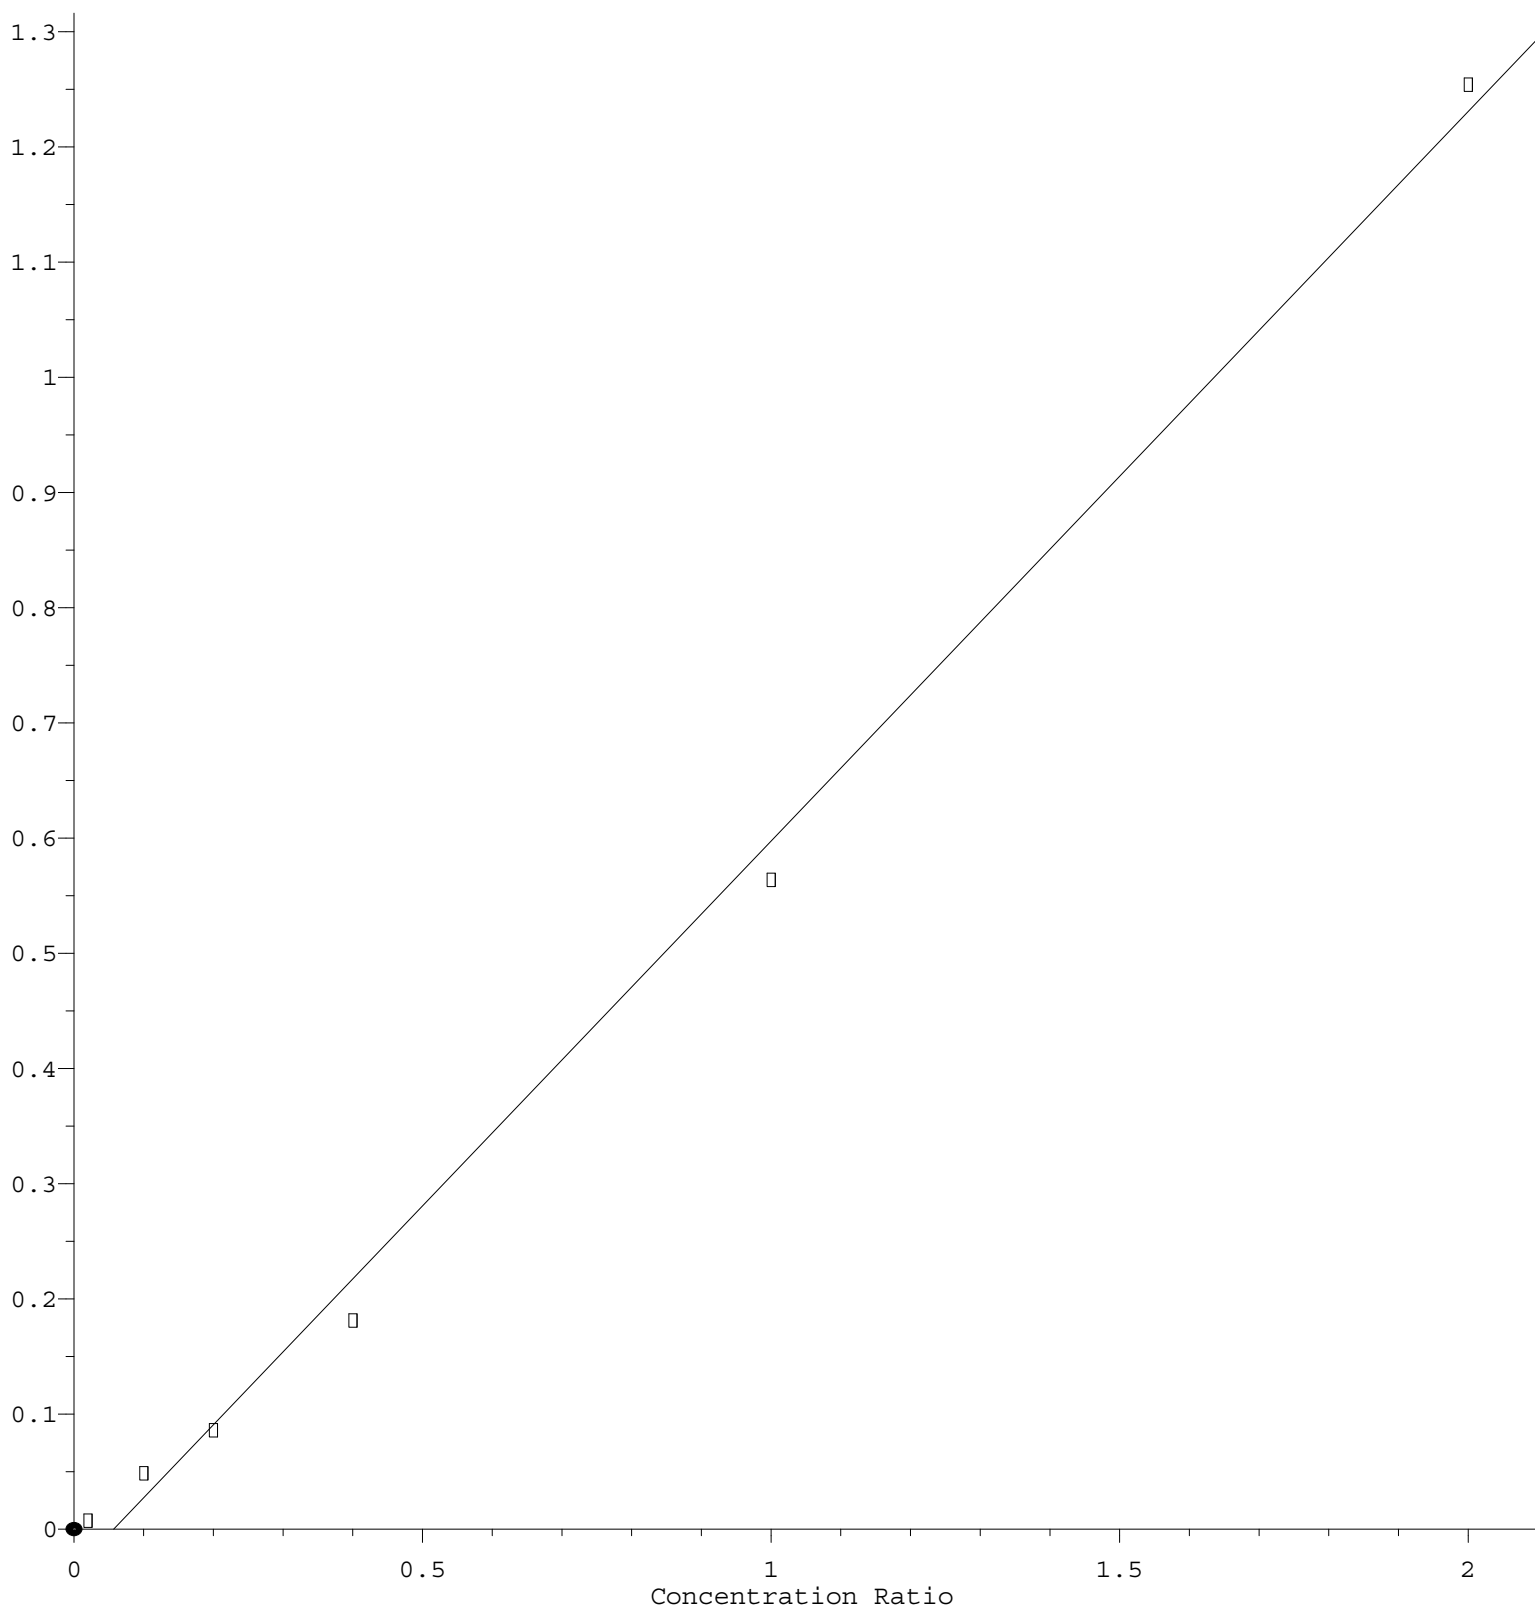

$$\text{Response} = 6.333\text{e-}001 * \text{Amt} - 3.588\text{e-}002$$


Coef of Det (r^2) = 0.996232 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

cis-1,3-Dichloropropene

Response Ratio

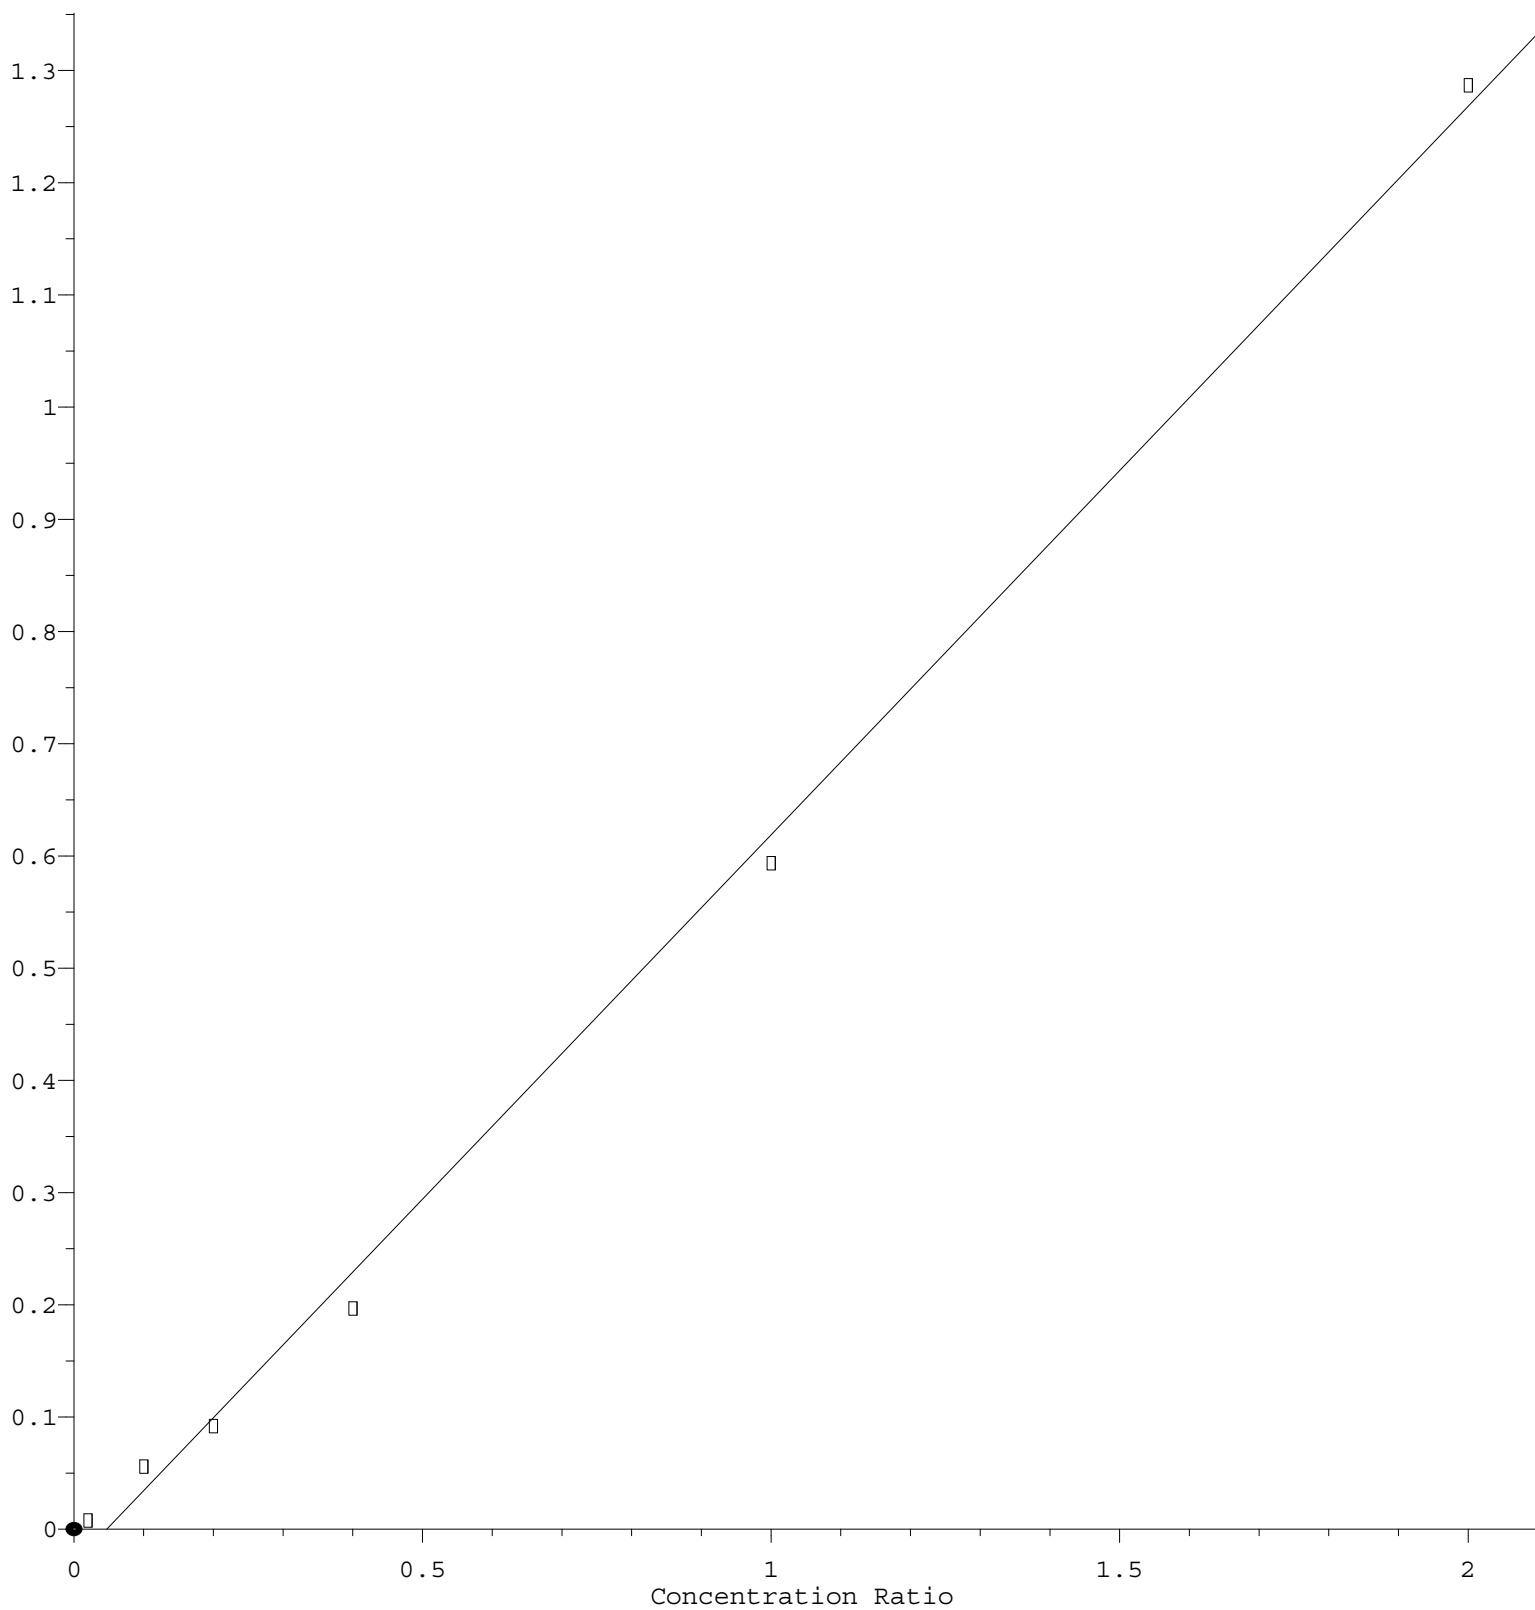

$$\text{Response} = 6.494\text{e-}001 * \text{Amt} - 3.058\text{e-}002$$


Coef of Det (r^2) = 0.997387 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Ethyl methacrylate

Response Ratio

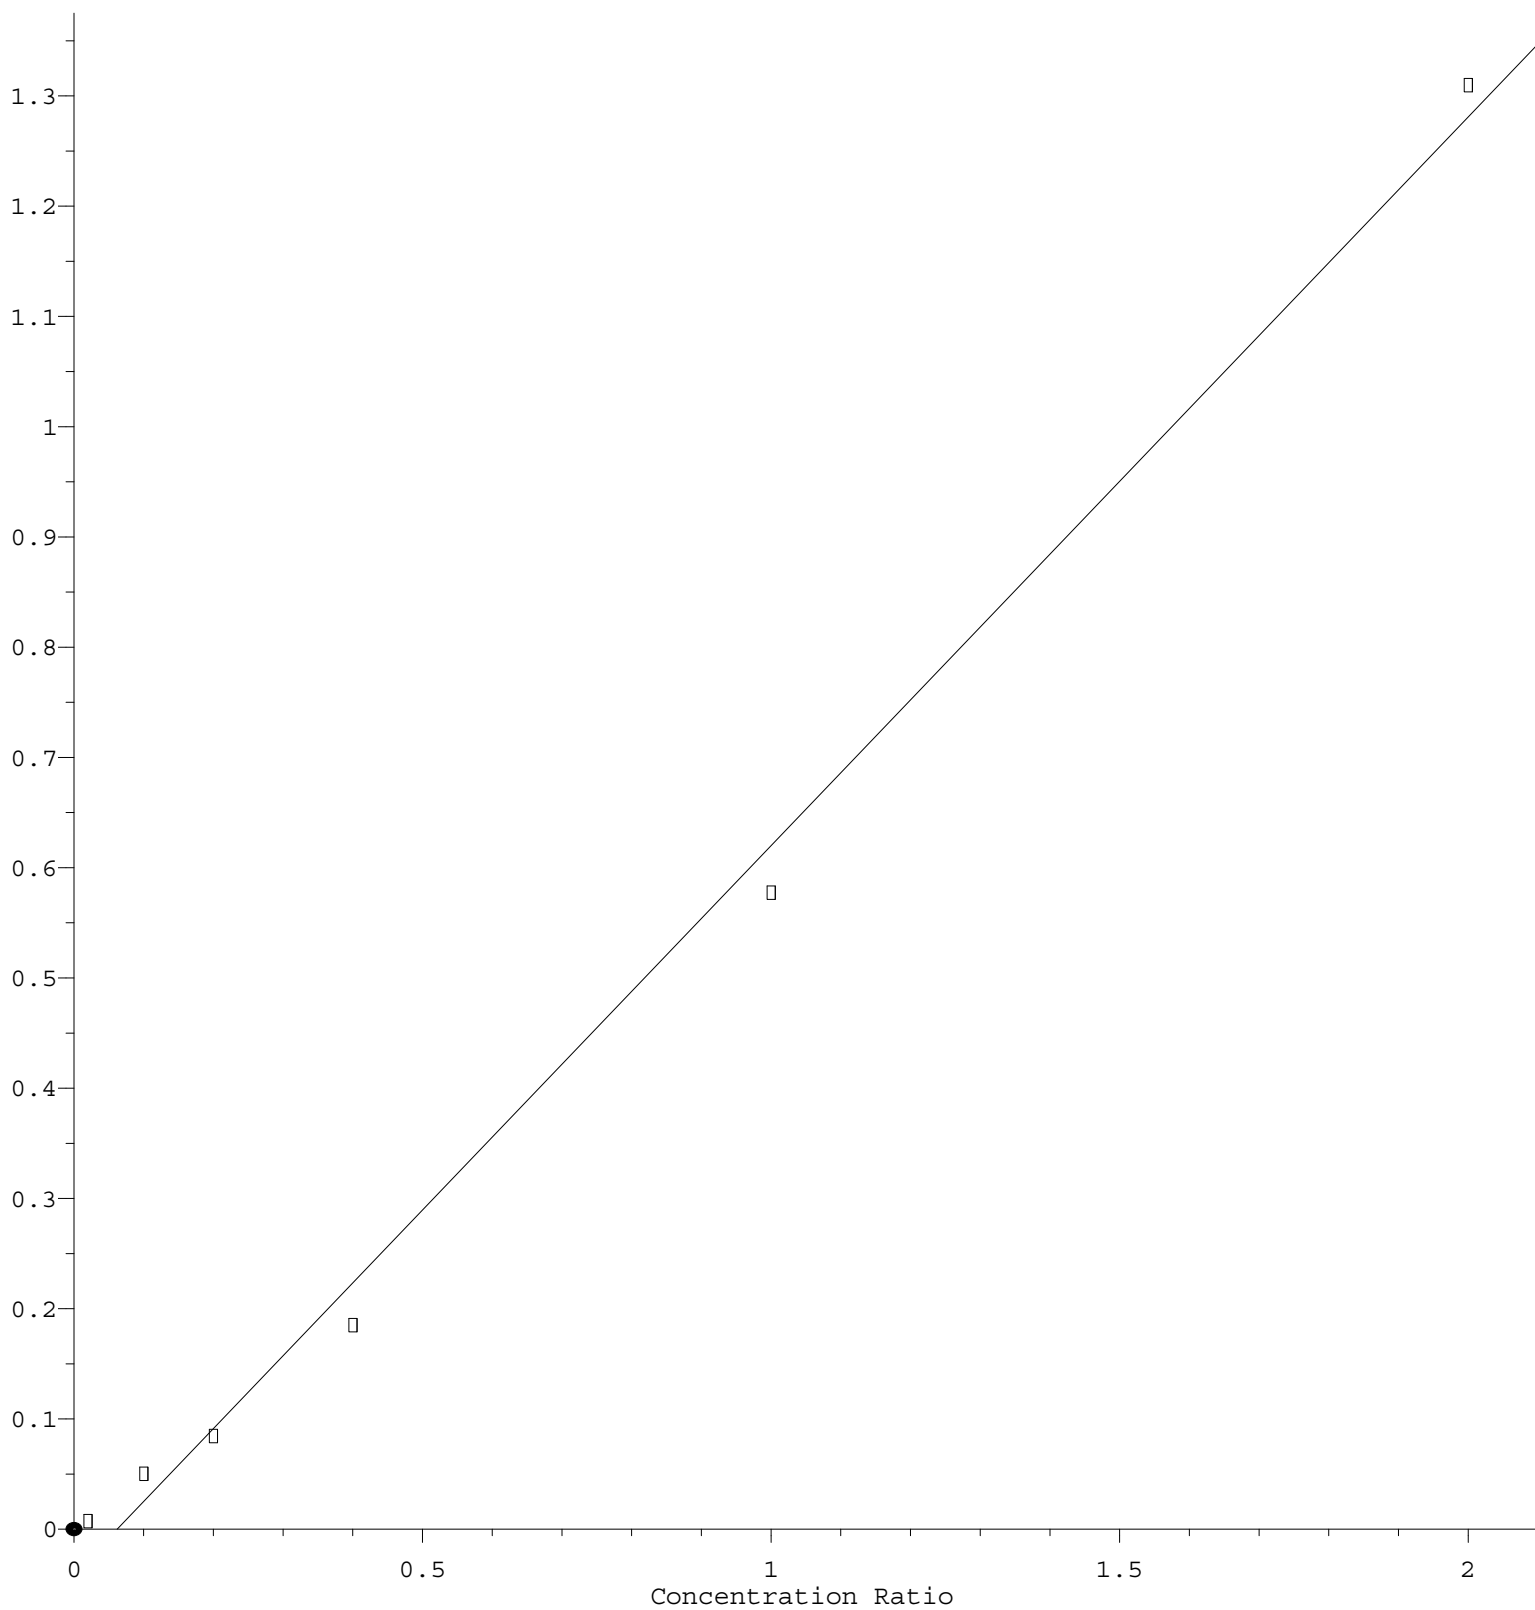

$$\text{Response} = 6.612\text{e-}001 * \text{Amt} - 4.098\text{e-}002$$


Coef of Det (r^2) = 0.995277 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

2-Chloroethyl Vinyl ether

Response Ratio

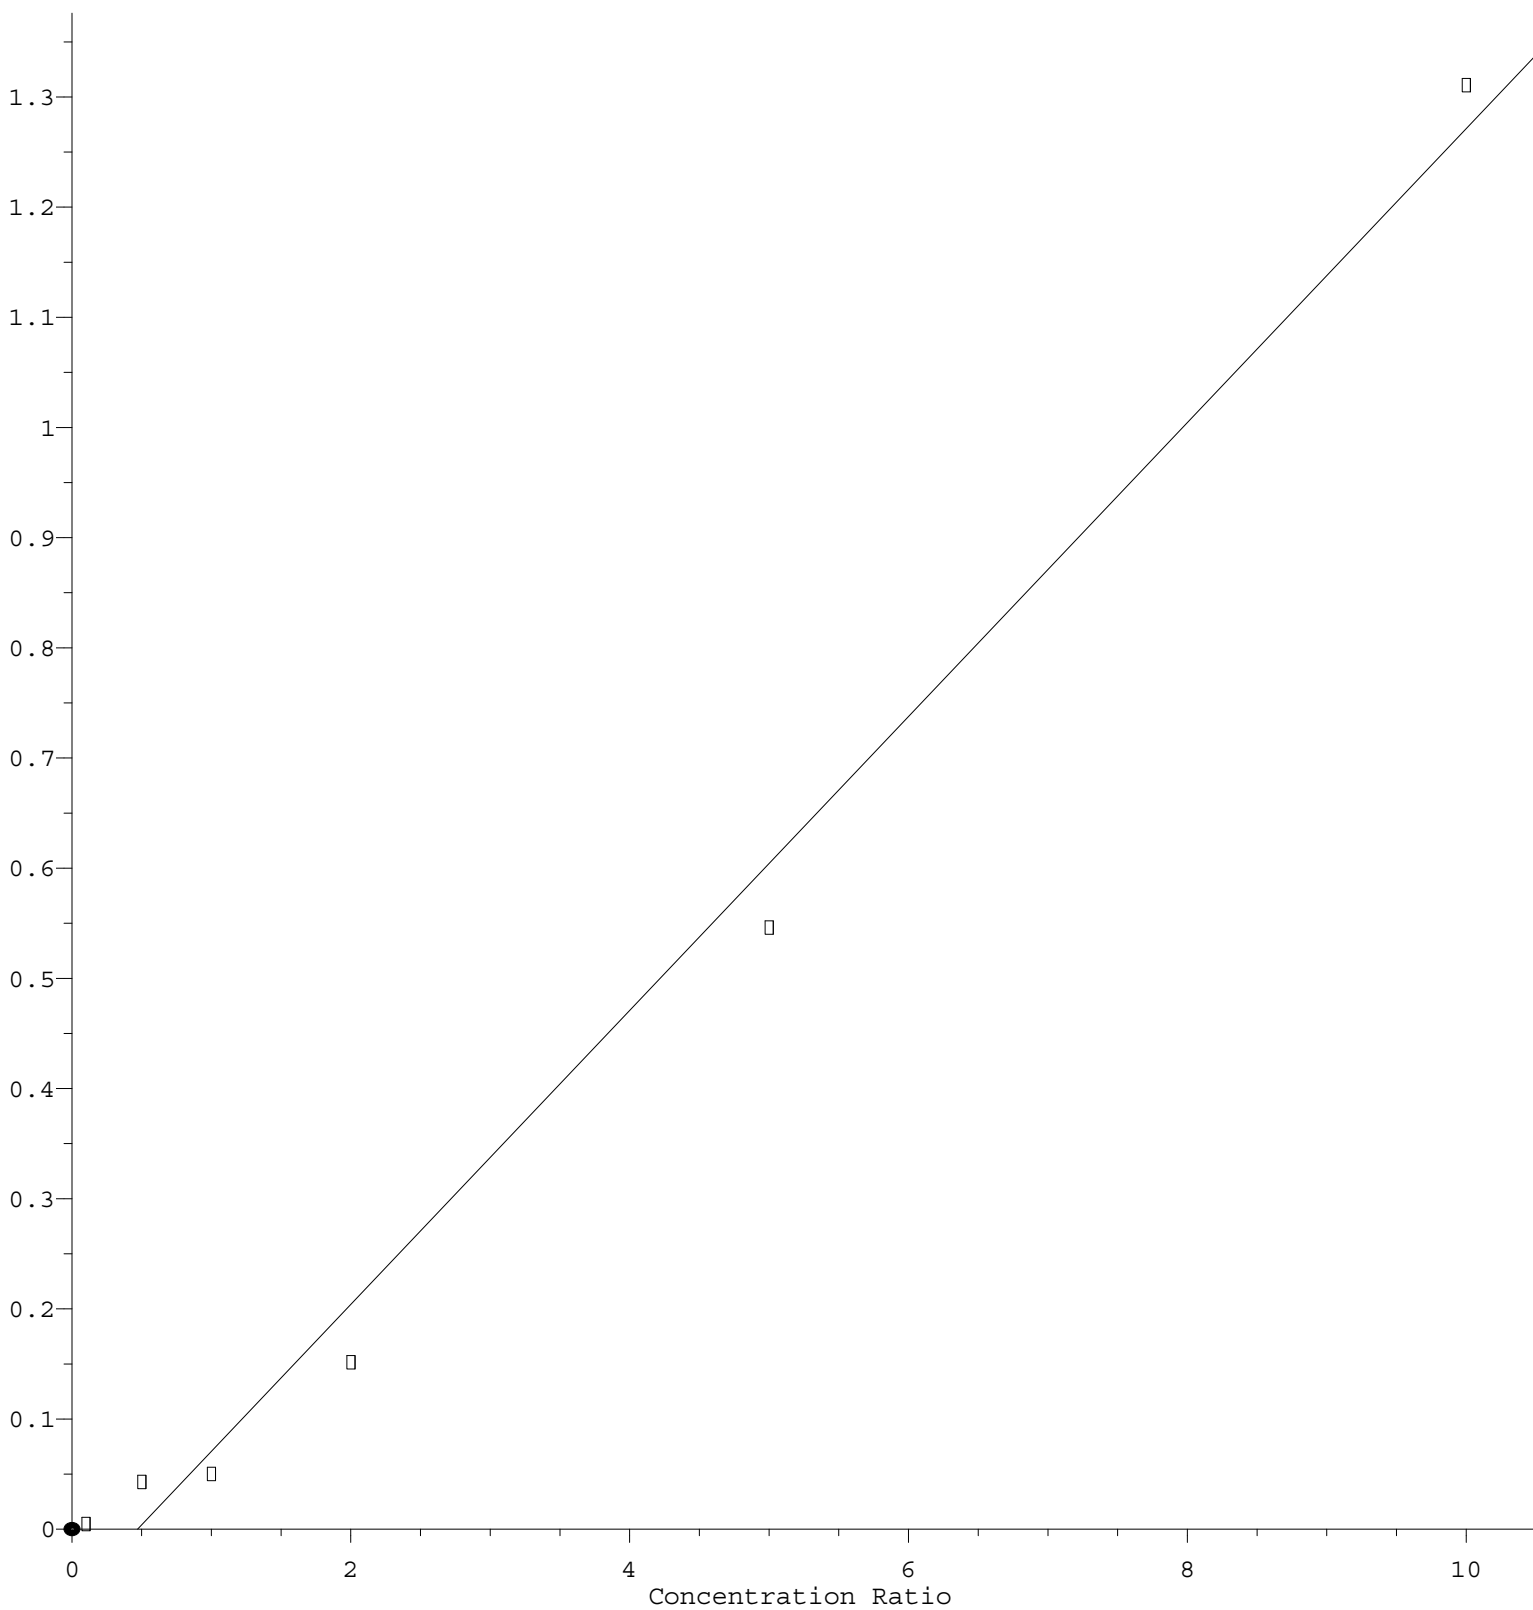

$$\text{Response} = 1.334\text{e-}001 * \text{Amt} - 6.251\text{e-}002$$


Coef of Det (r^2) = 0.990379 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

2-Hexanone

Response Ratio

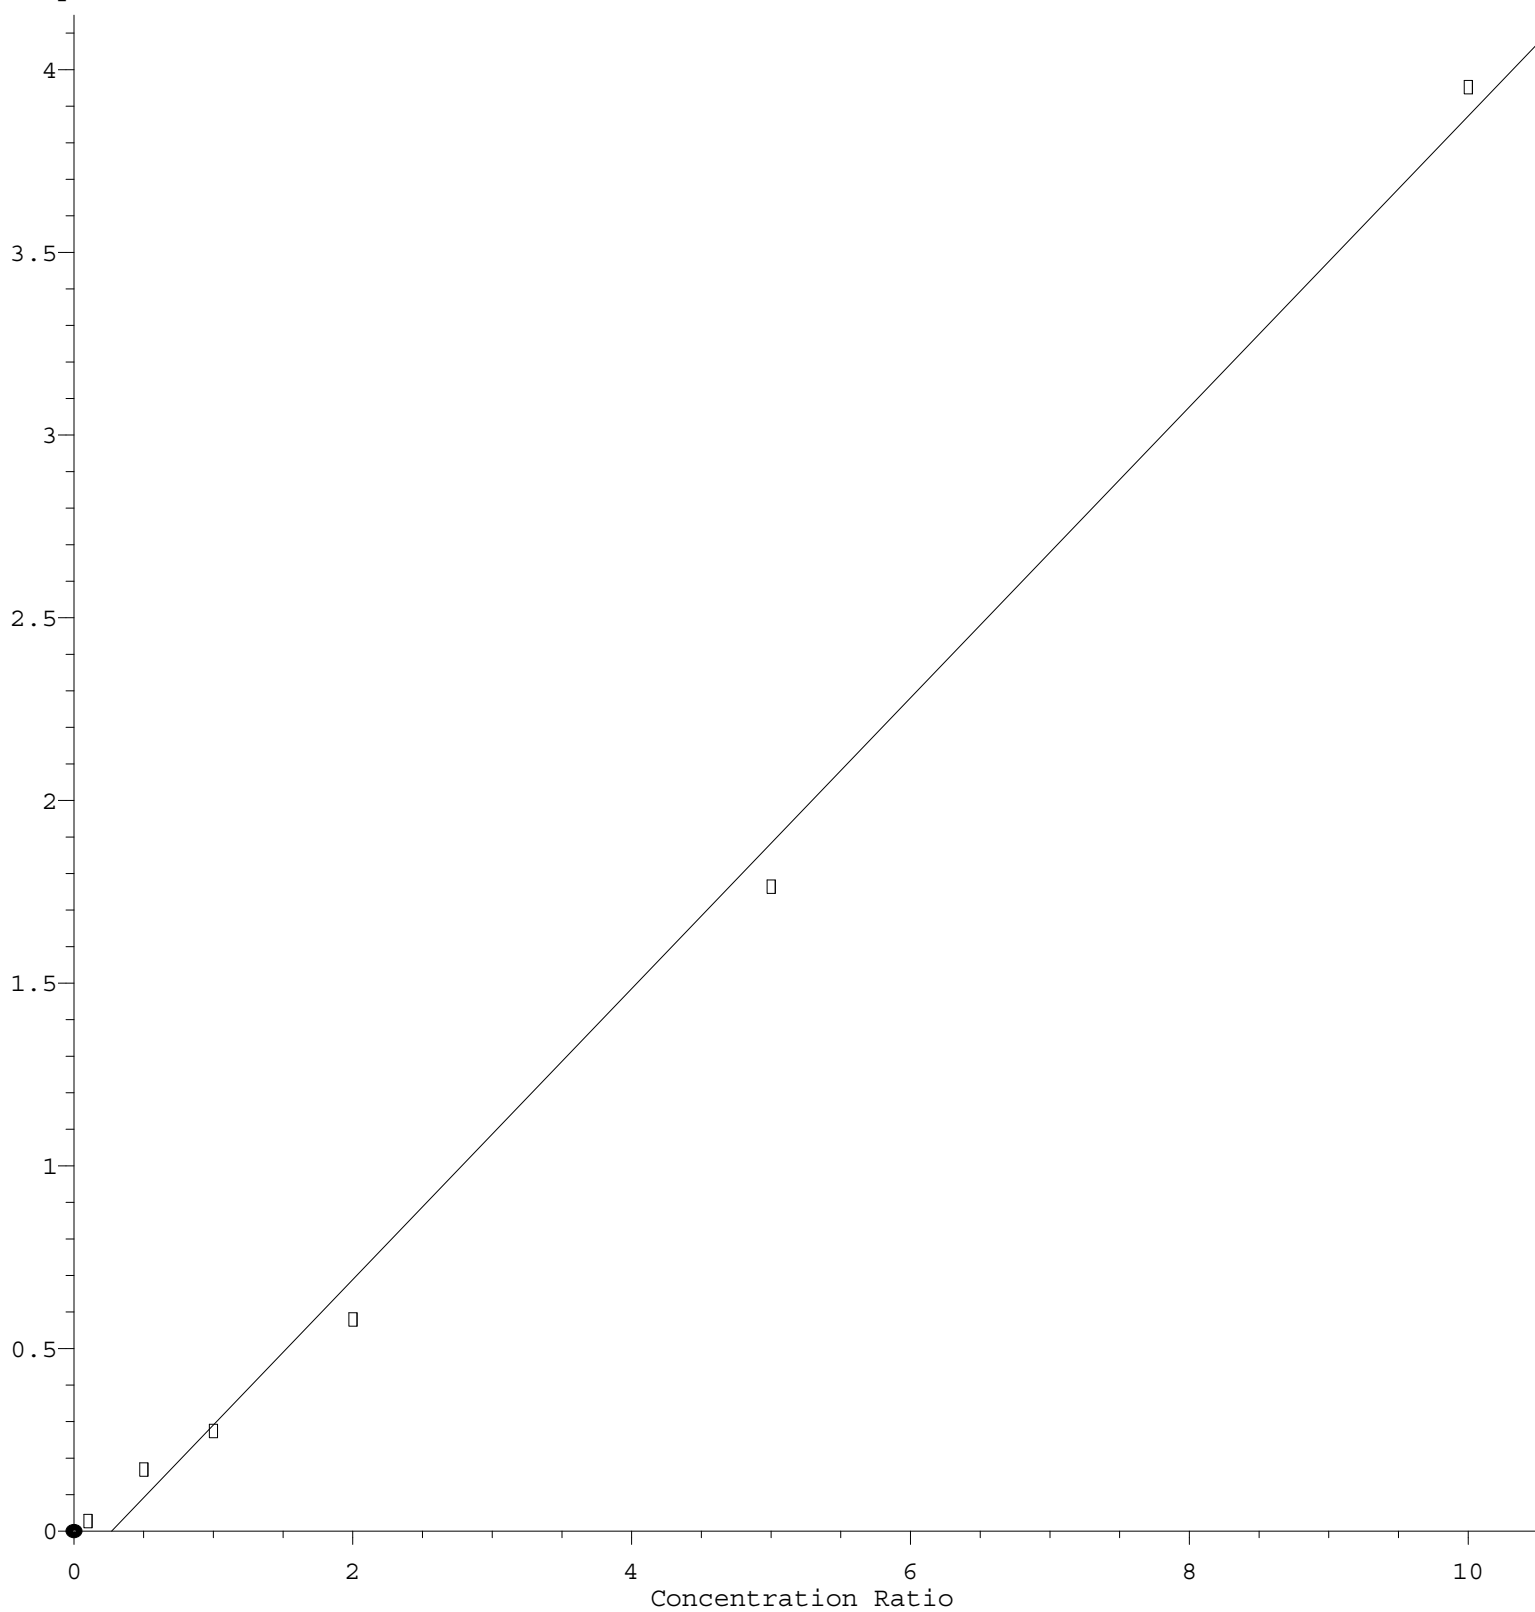

$$\text{Response} = 3.979\text{e-}001 * \text{Amt} - 1.057\text{e-}001$$


Coef of Det (r^2) = 0.995872 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Dibromochloromethane

Response Ratio

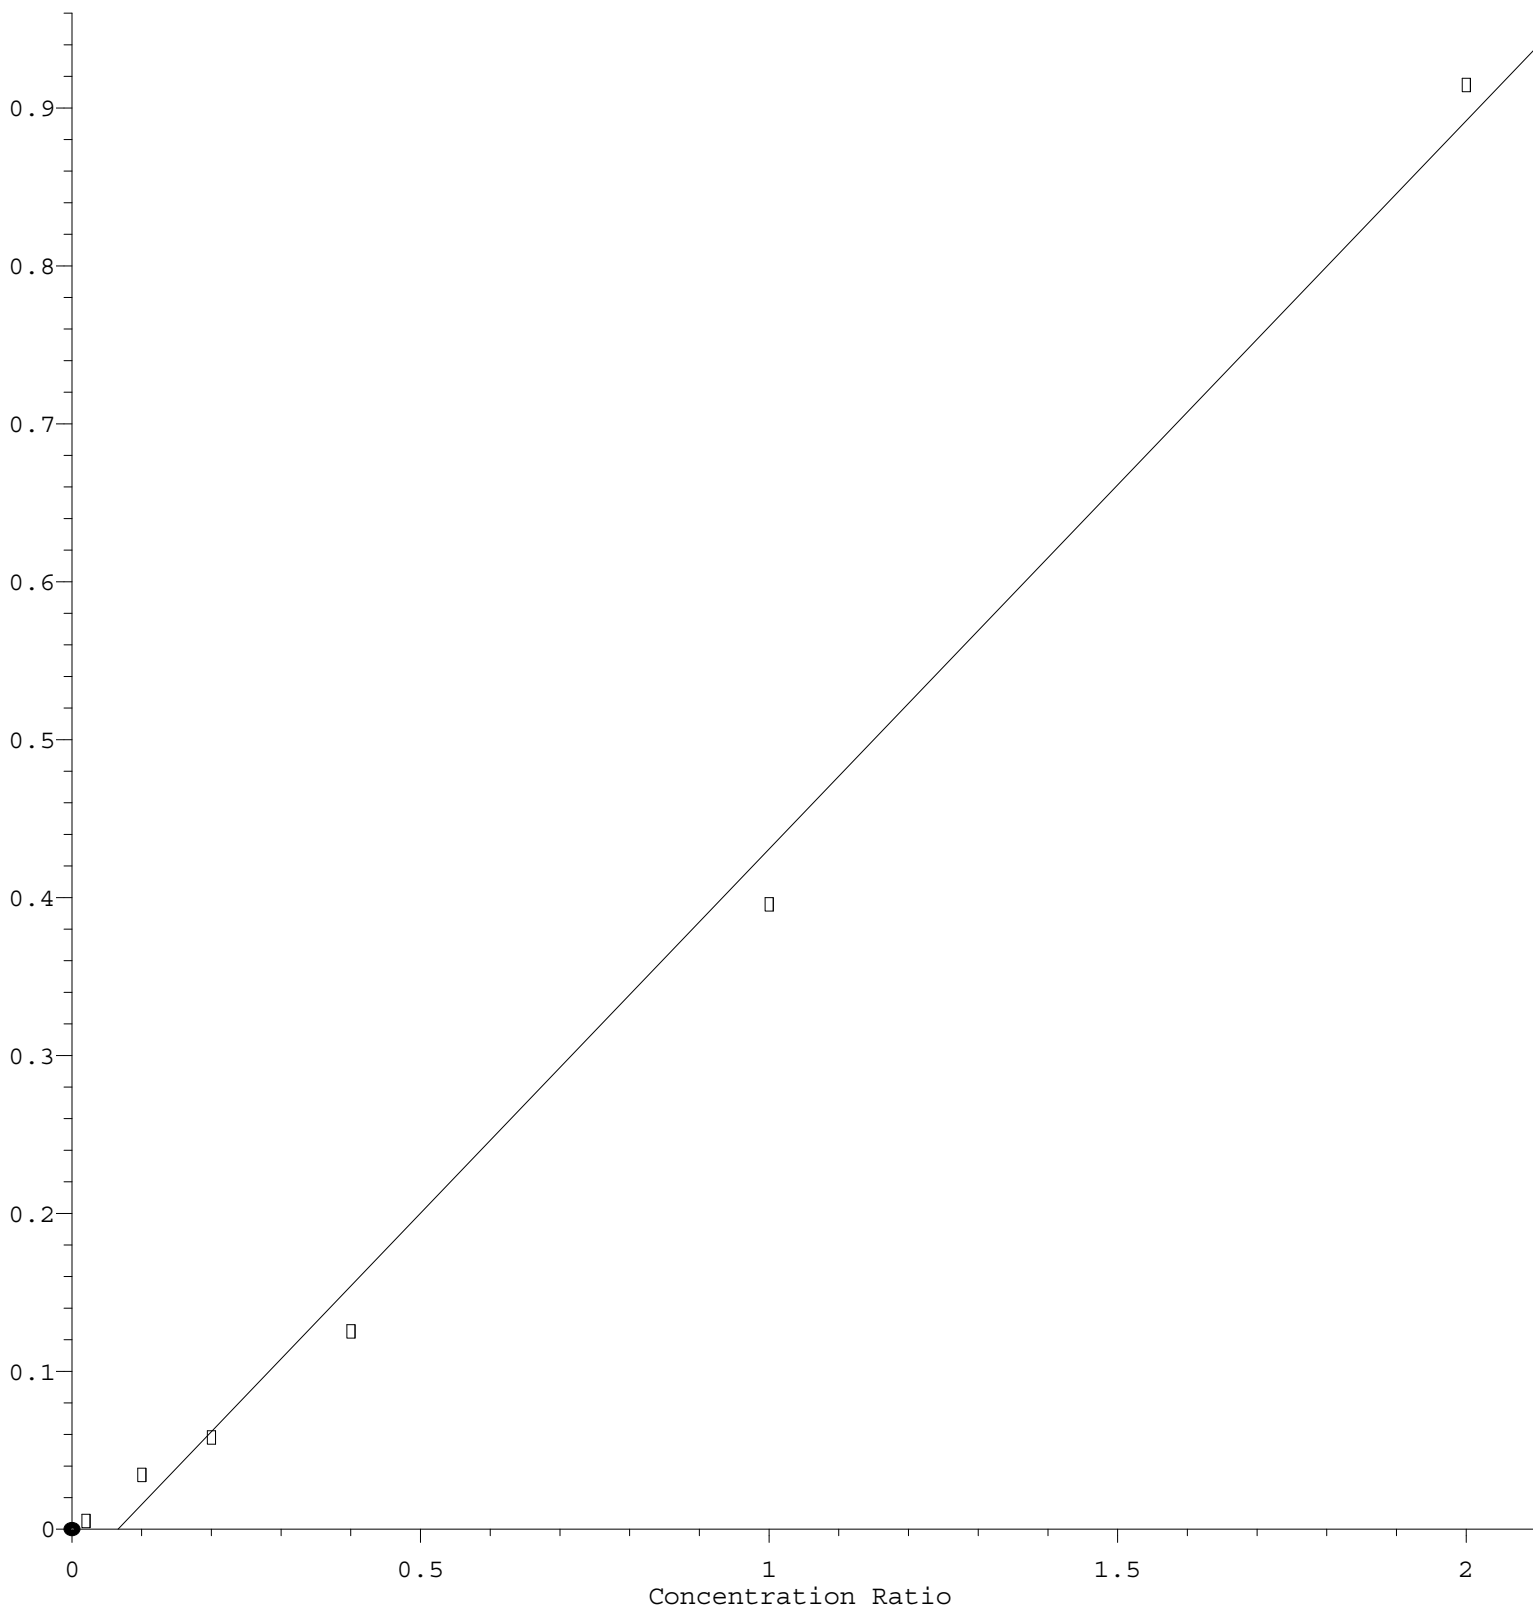

$$\text{Response} = 4.612\text{e-}001 * \text{Amt} - 3.046\text{e-}002$$


Coef of Det (r^2) = 0.994167 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

4-Bromofluorobenzene

Response Ratio

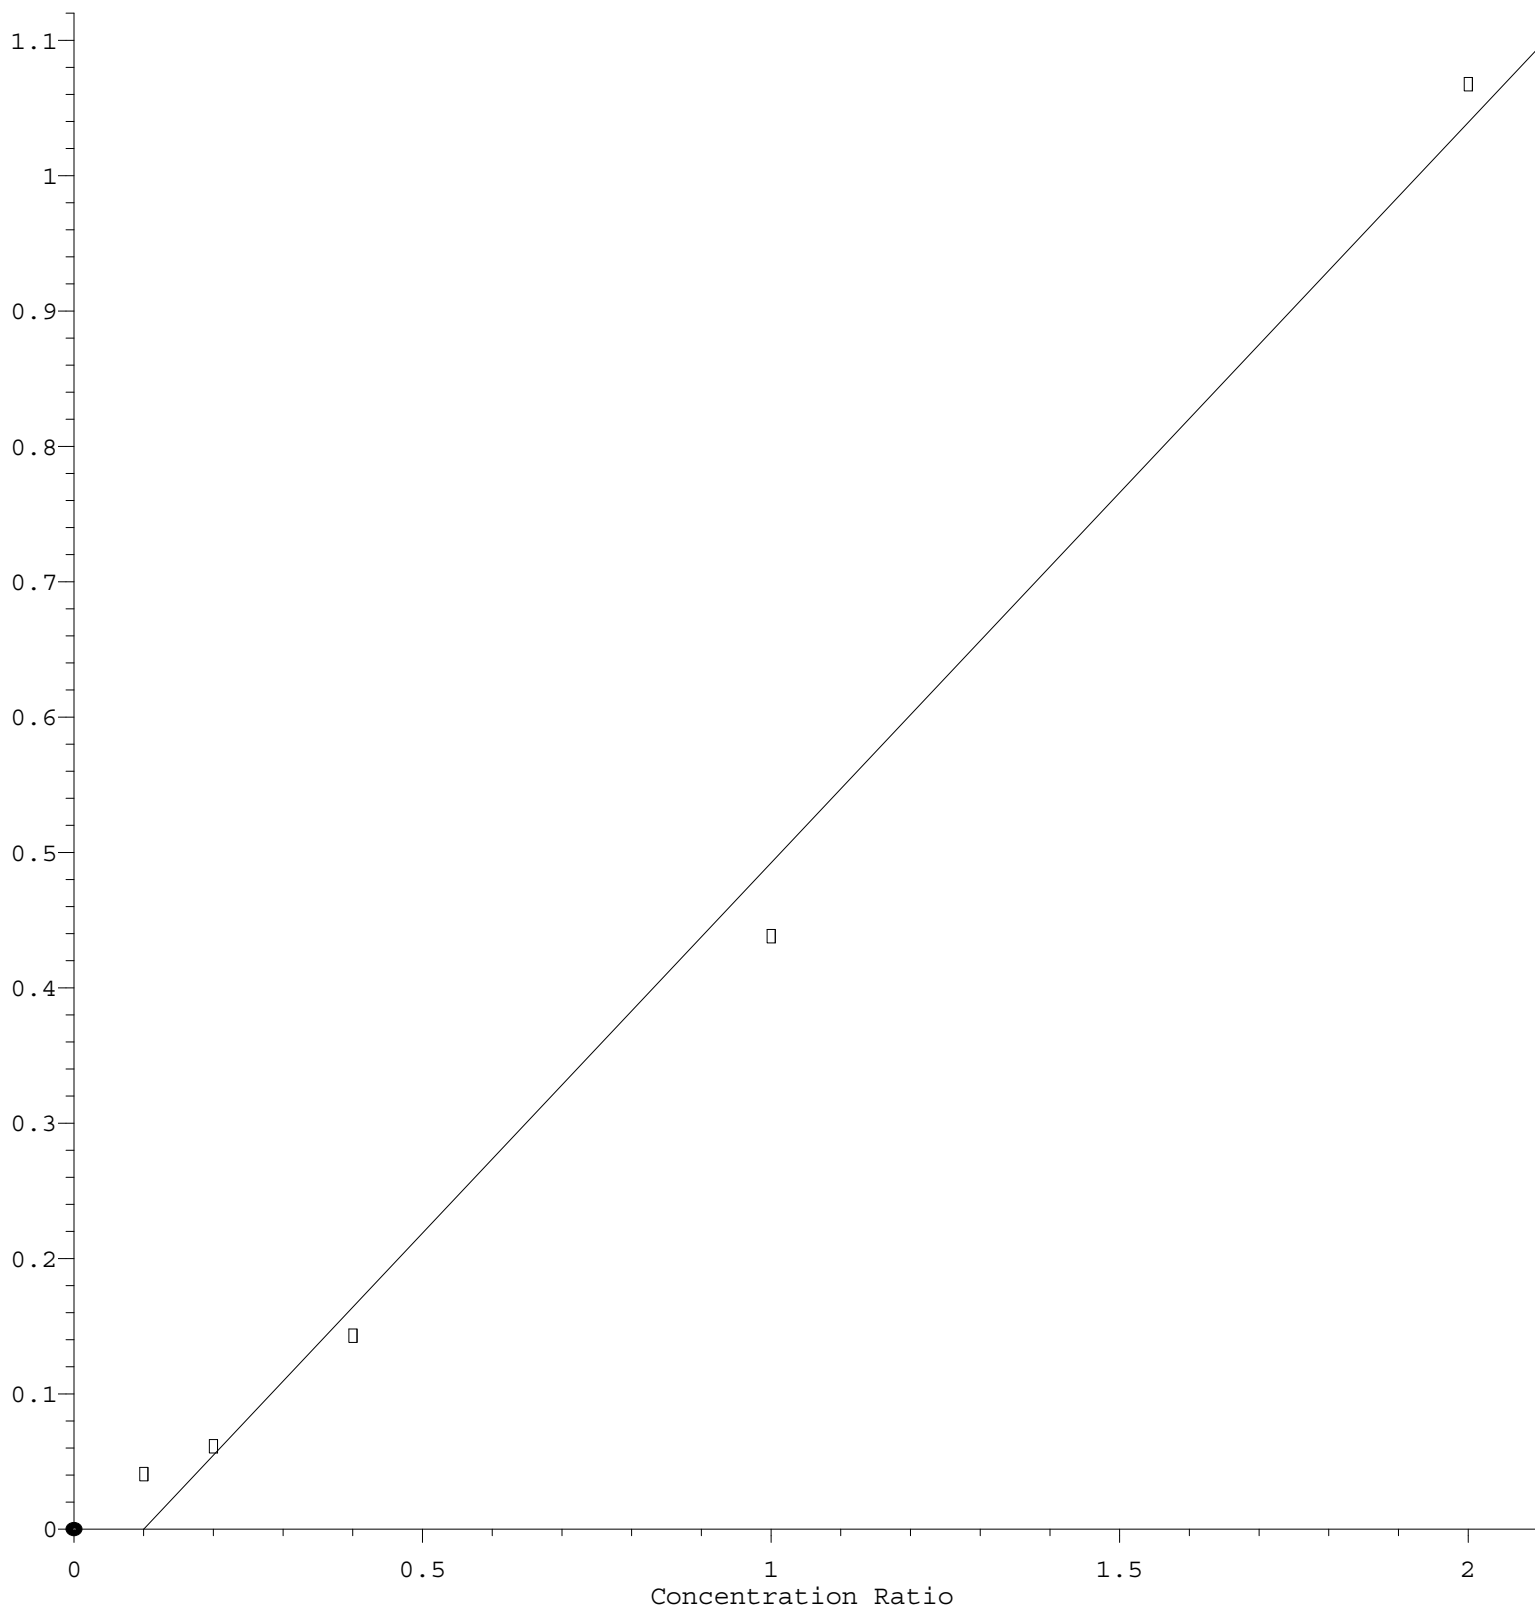


$$\text{Response} = 5.466\text{e-}001 * \text{Amt} - 5.440\text{e-}002$$

Coef of Det (r^2) = 0.992099 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021


1,1,1,2-Tetrachloroethane

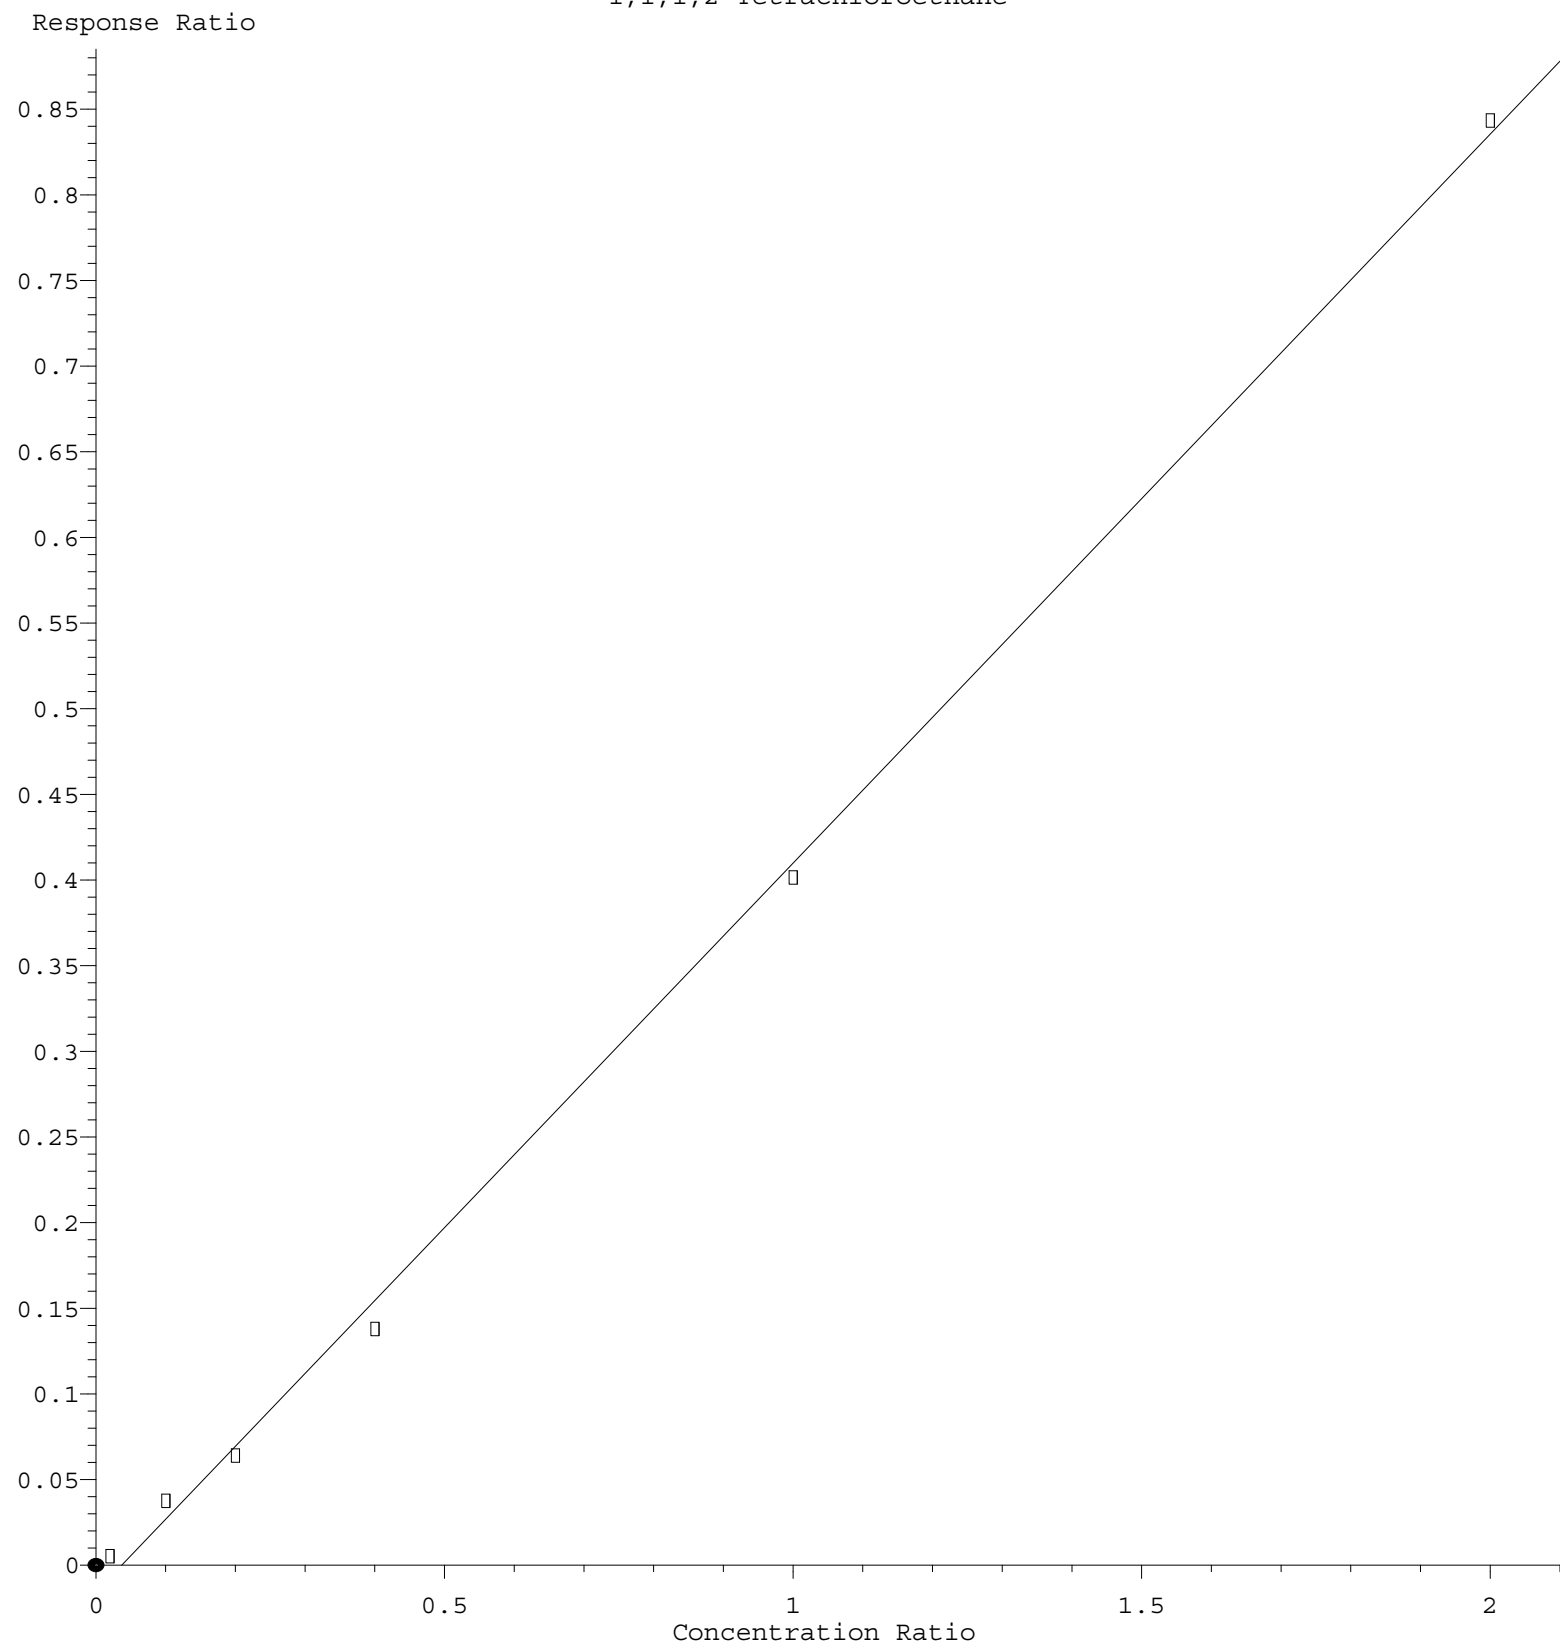

Response = $4.258 \times 10^{-1} \times \text{Amt} - 1.575 \times 10^{-2}$
 Coef of Det (r^2) = 0.998650 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M
 Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

m/p-Xylenes

Response Ratio

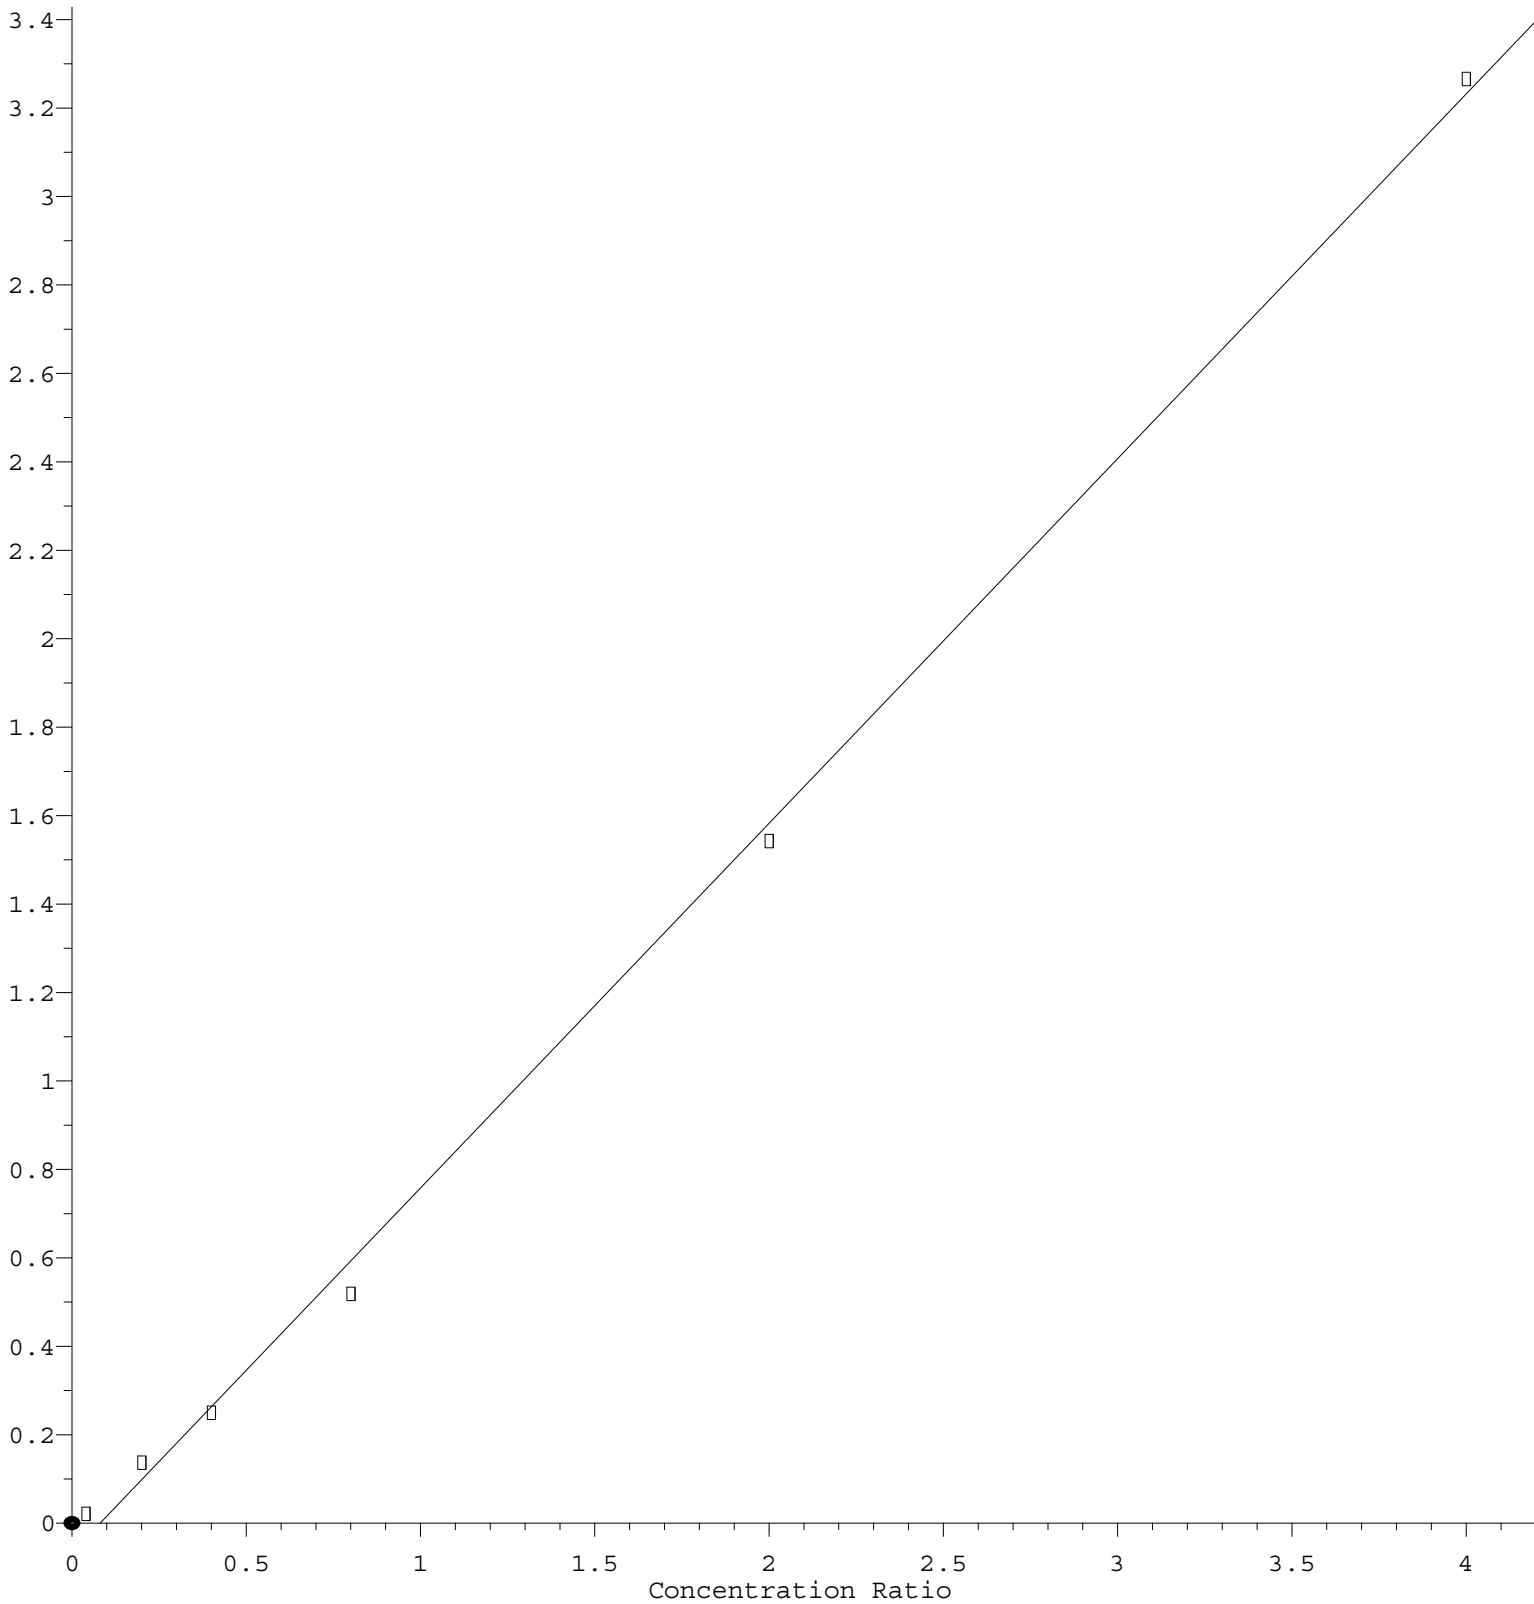

$$\text{Response} = 8.247\text{e-}001 * \text{Amt} - 6.700\text{e-}002$$


Coef of Det (r^2) = 0.998355 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Styrene

Response Ratio

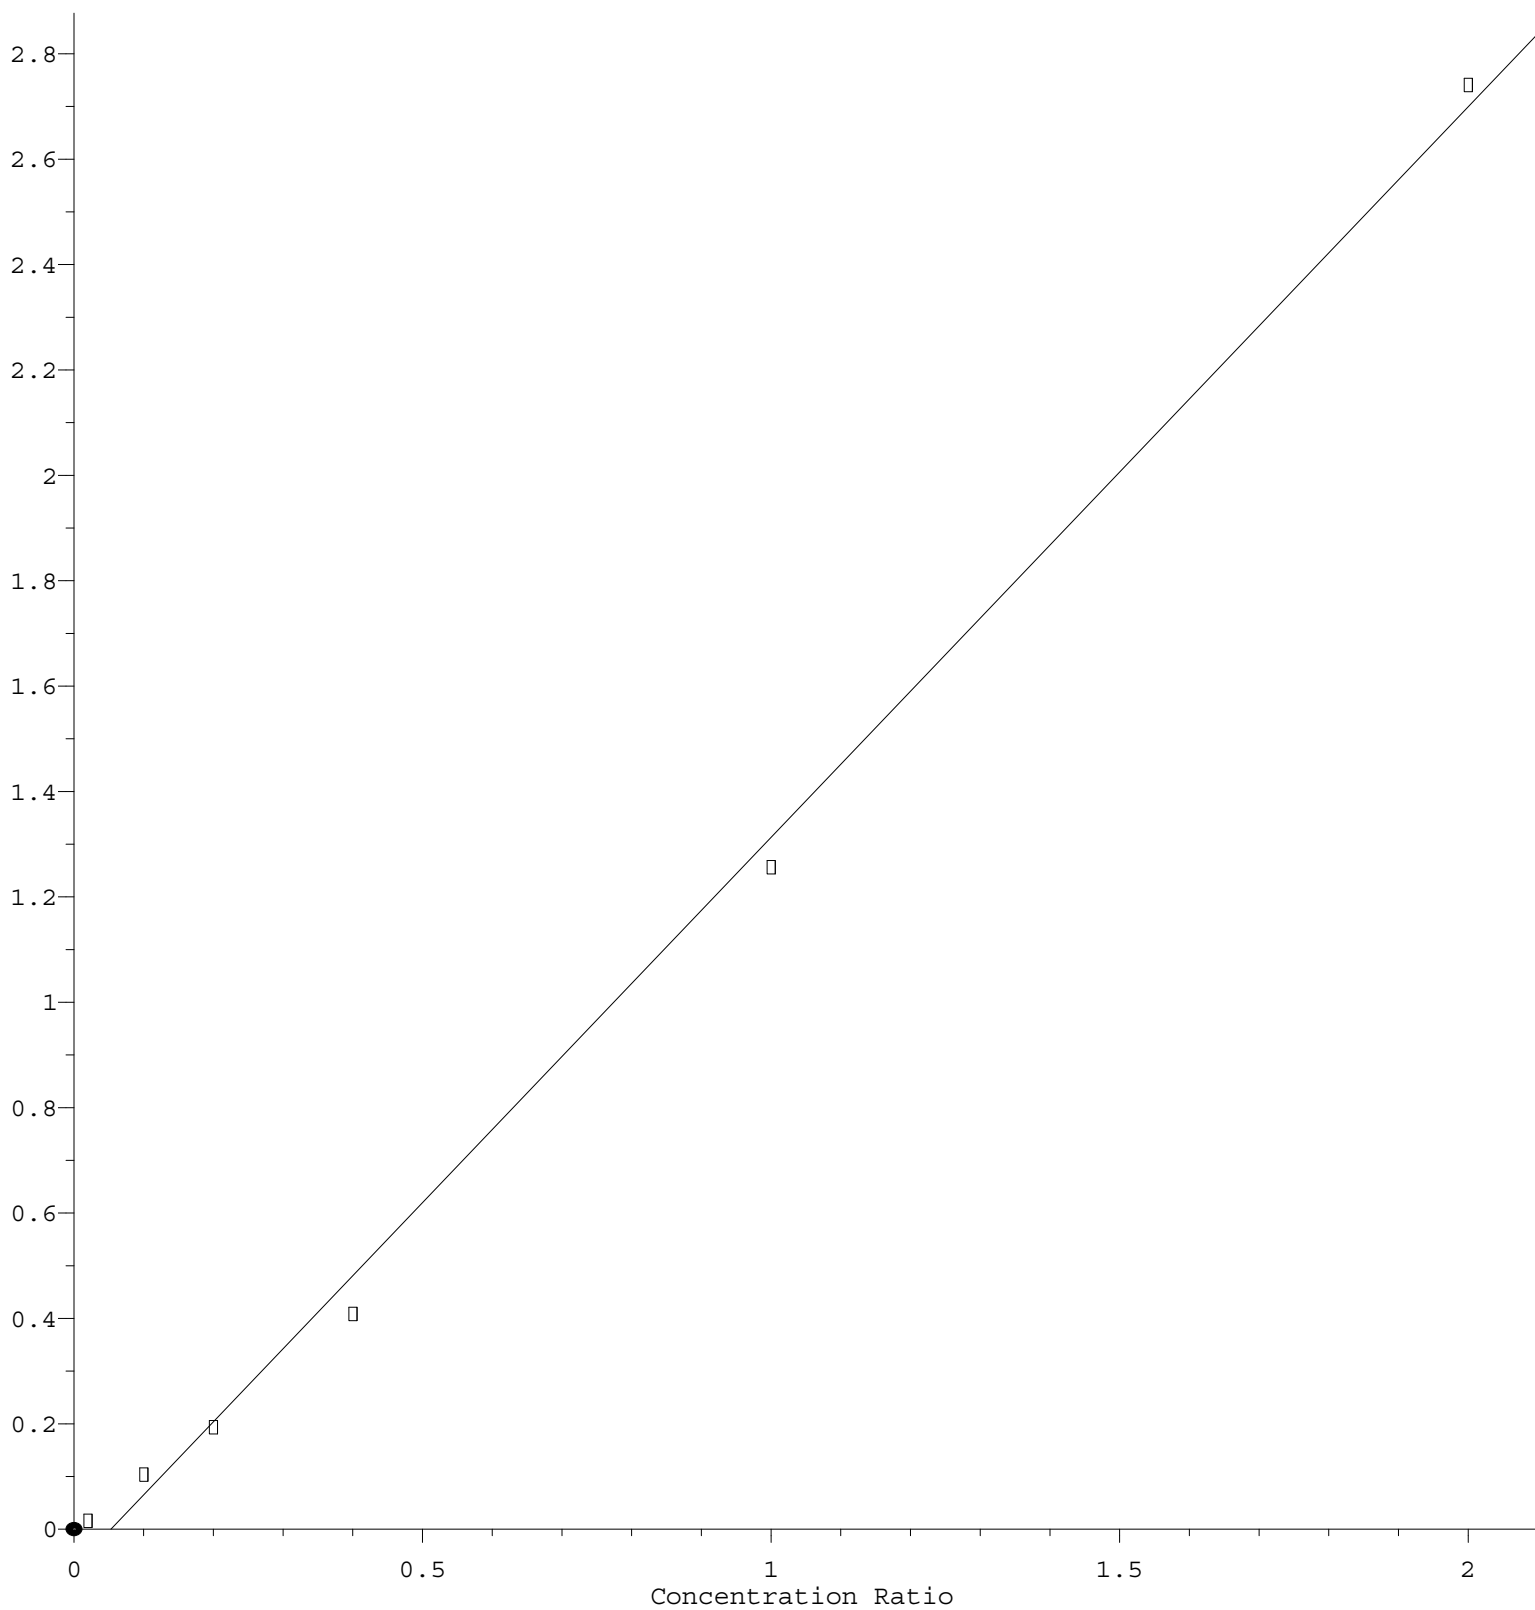


$$\text{Response} = 1.386\text{e}+000 * \text{Amt} - 7.295\text{e}-002$$

Coef of Det (r^2) = 0.997215 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M


Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

Bromoform

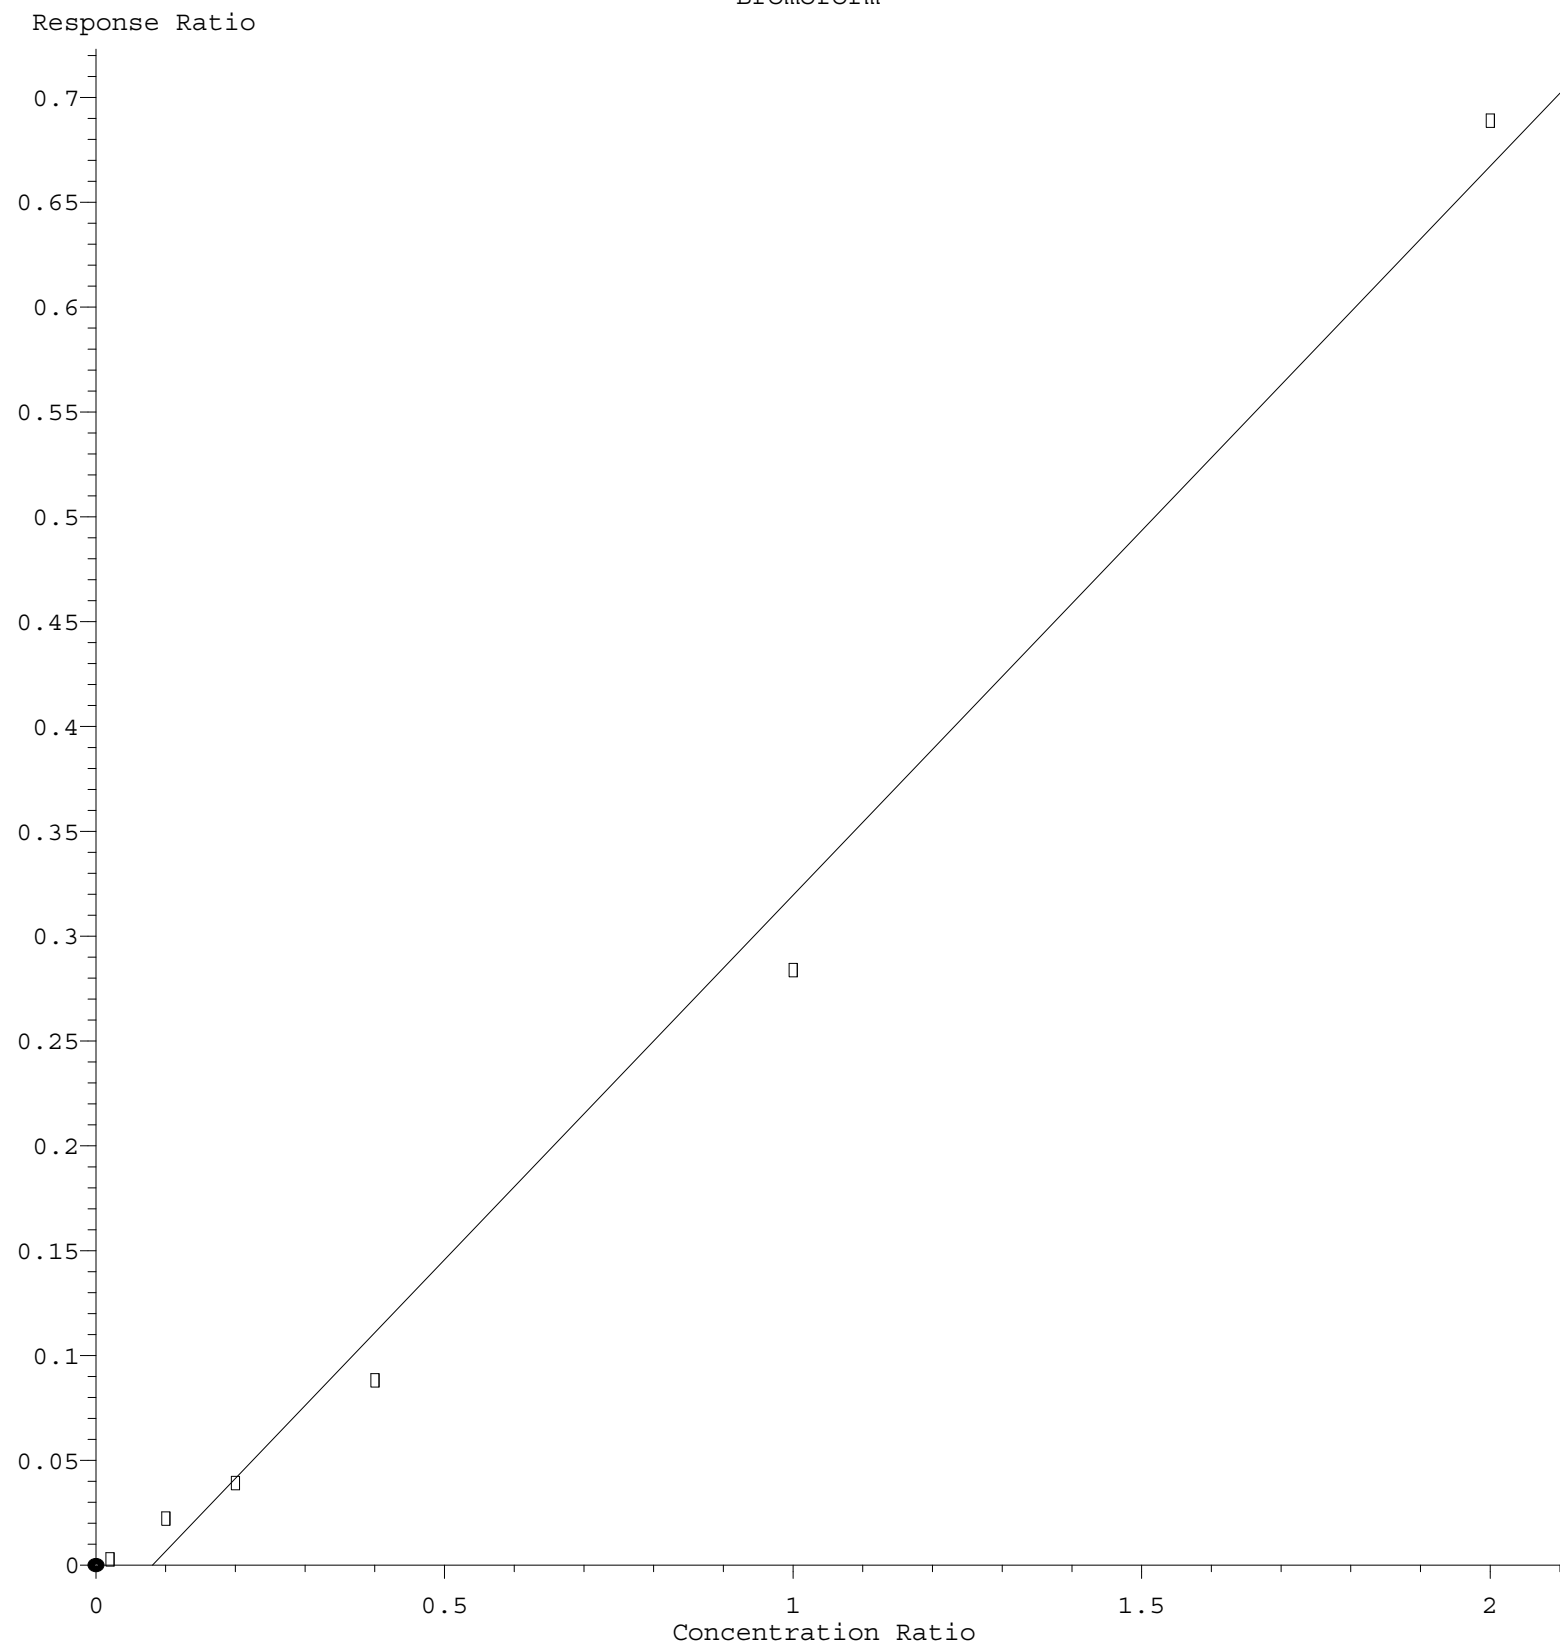

Response = 3.476e-001 * Amt - 2.802e-002
 Coef of Det (r^2) = 0.991272 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M
 Calibration Table Last Updated: Thu Jul 29 15:02:35 2021


trans-1,4-Dichloro-2-butene

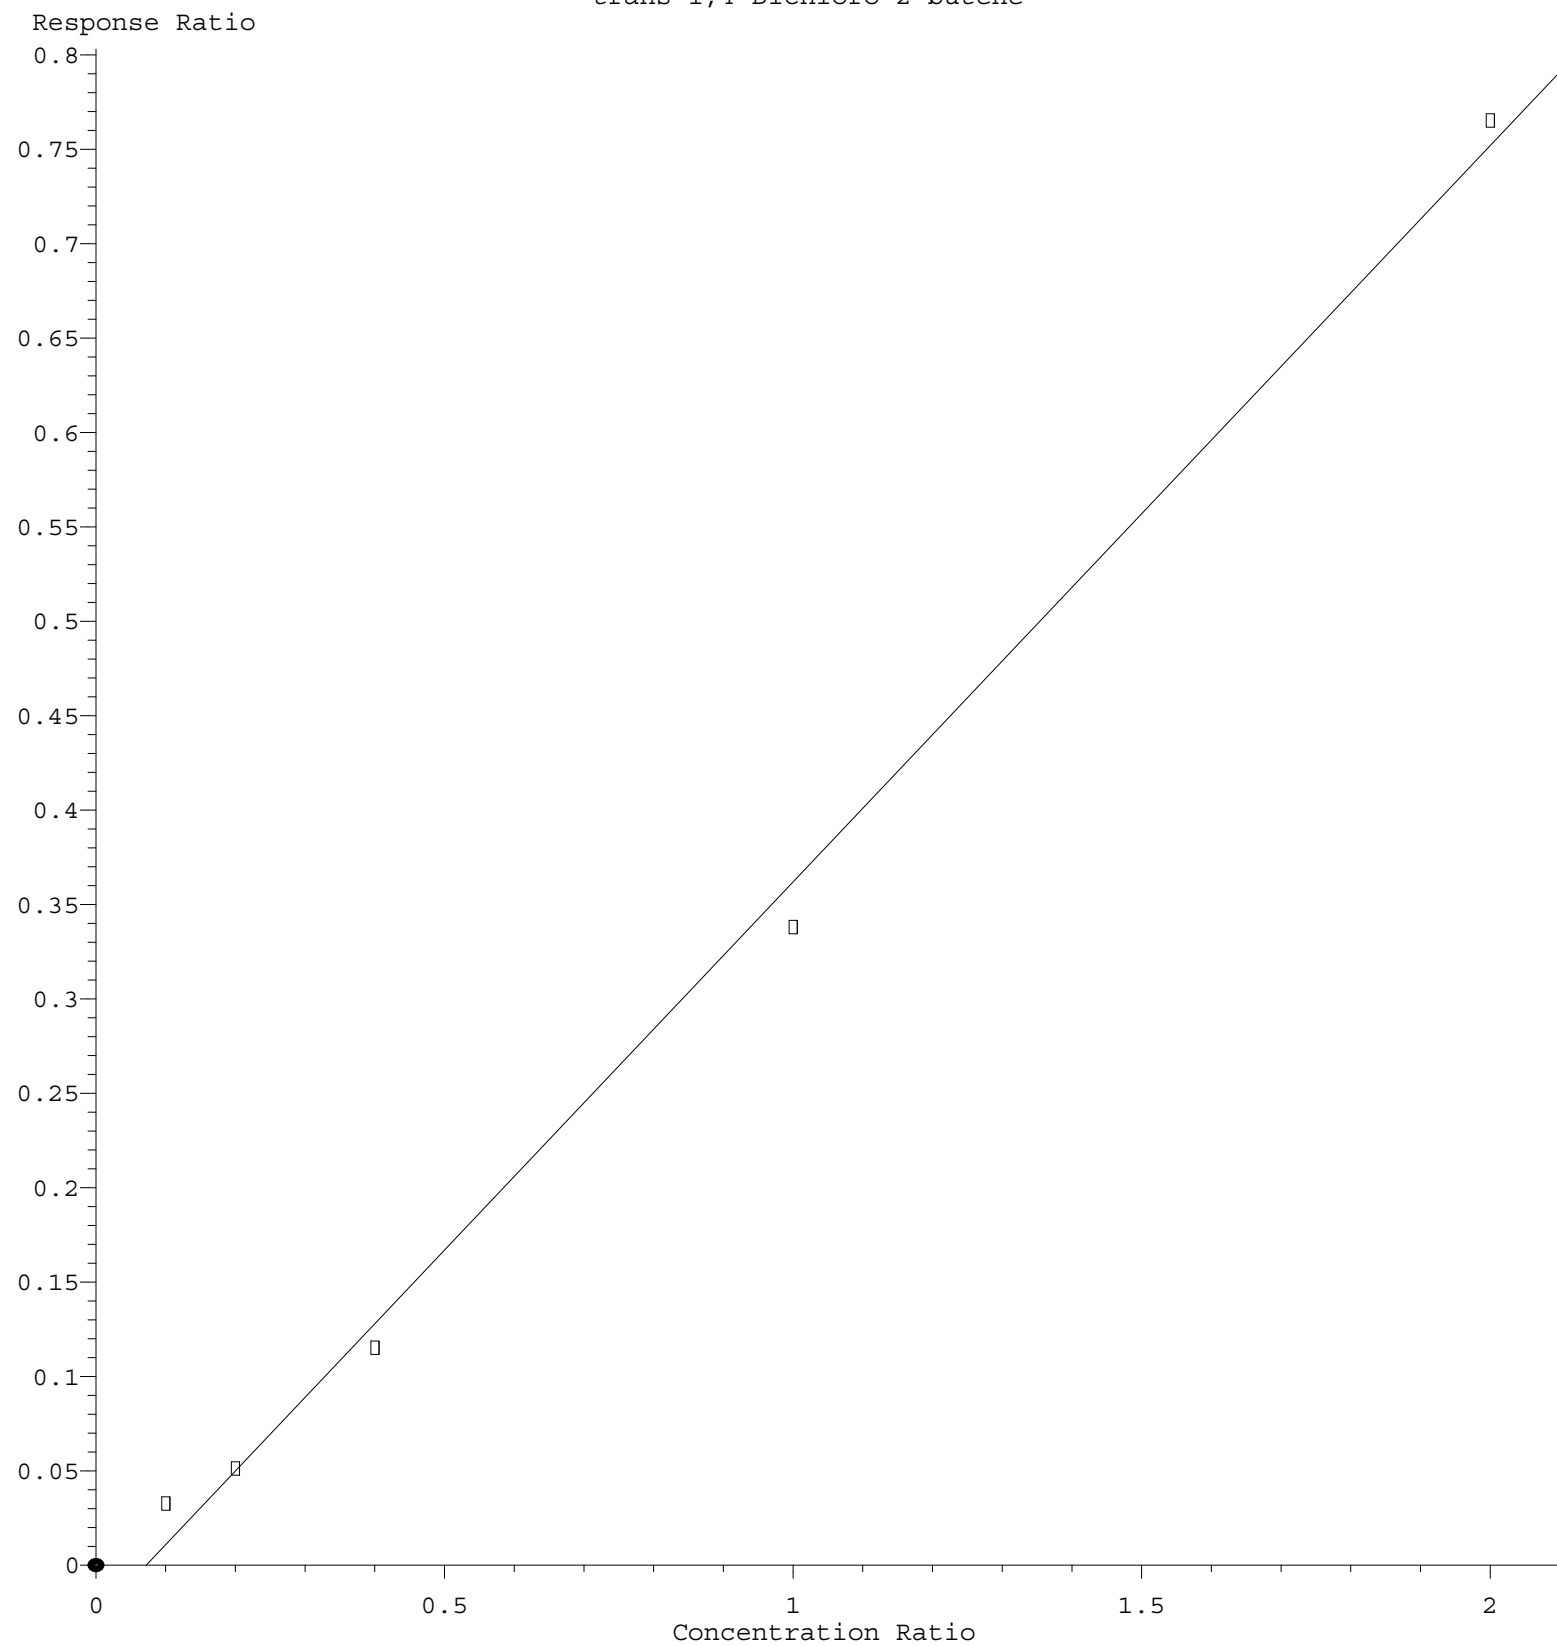

Response = $3.901 \times 10^{-1} \times \text{Amt} - 2.825 \times 10^{-2}$
Coef of Det (r^2) = 0.996338 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M
Calibration Table Last Updated: Thu Jul 29 15:02:35 2021

1,2,4-Trichlorobenzene

Response Ratio

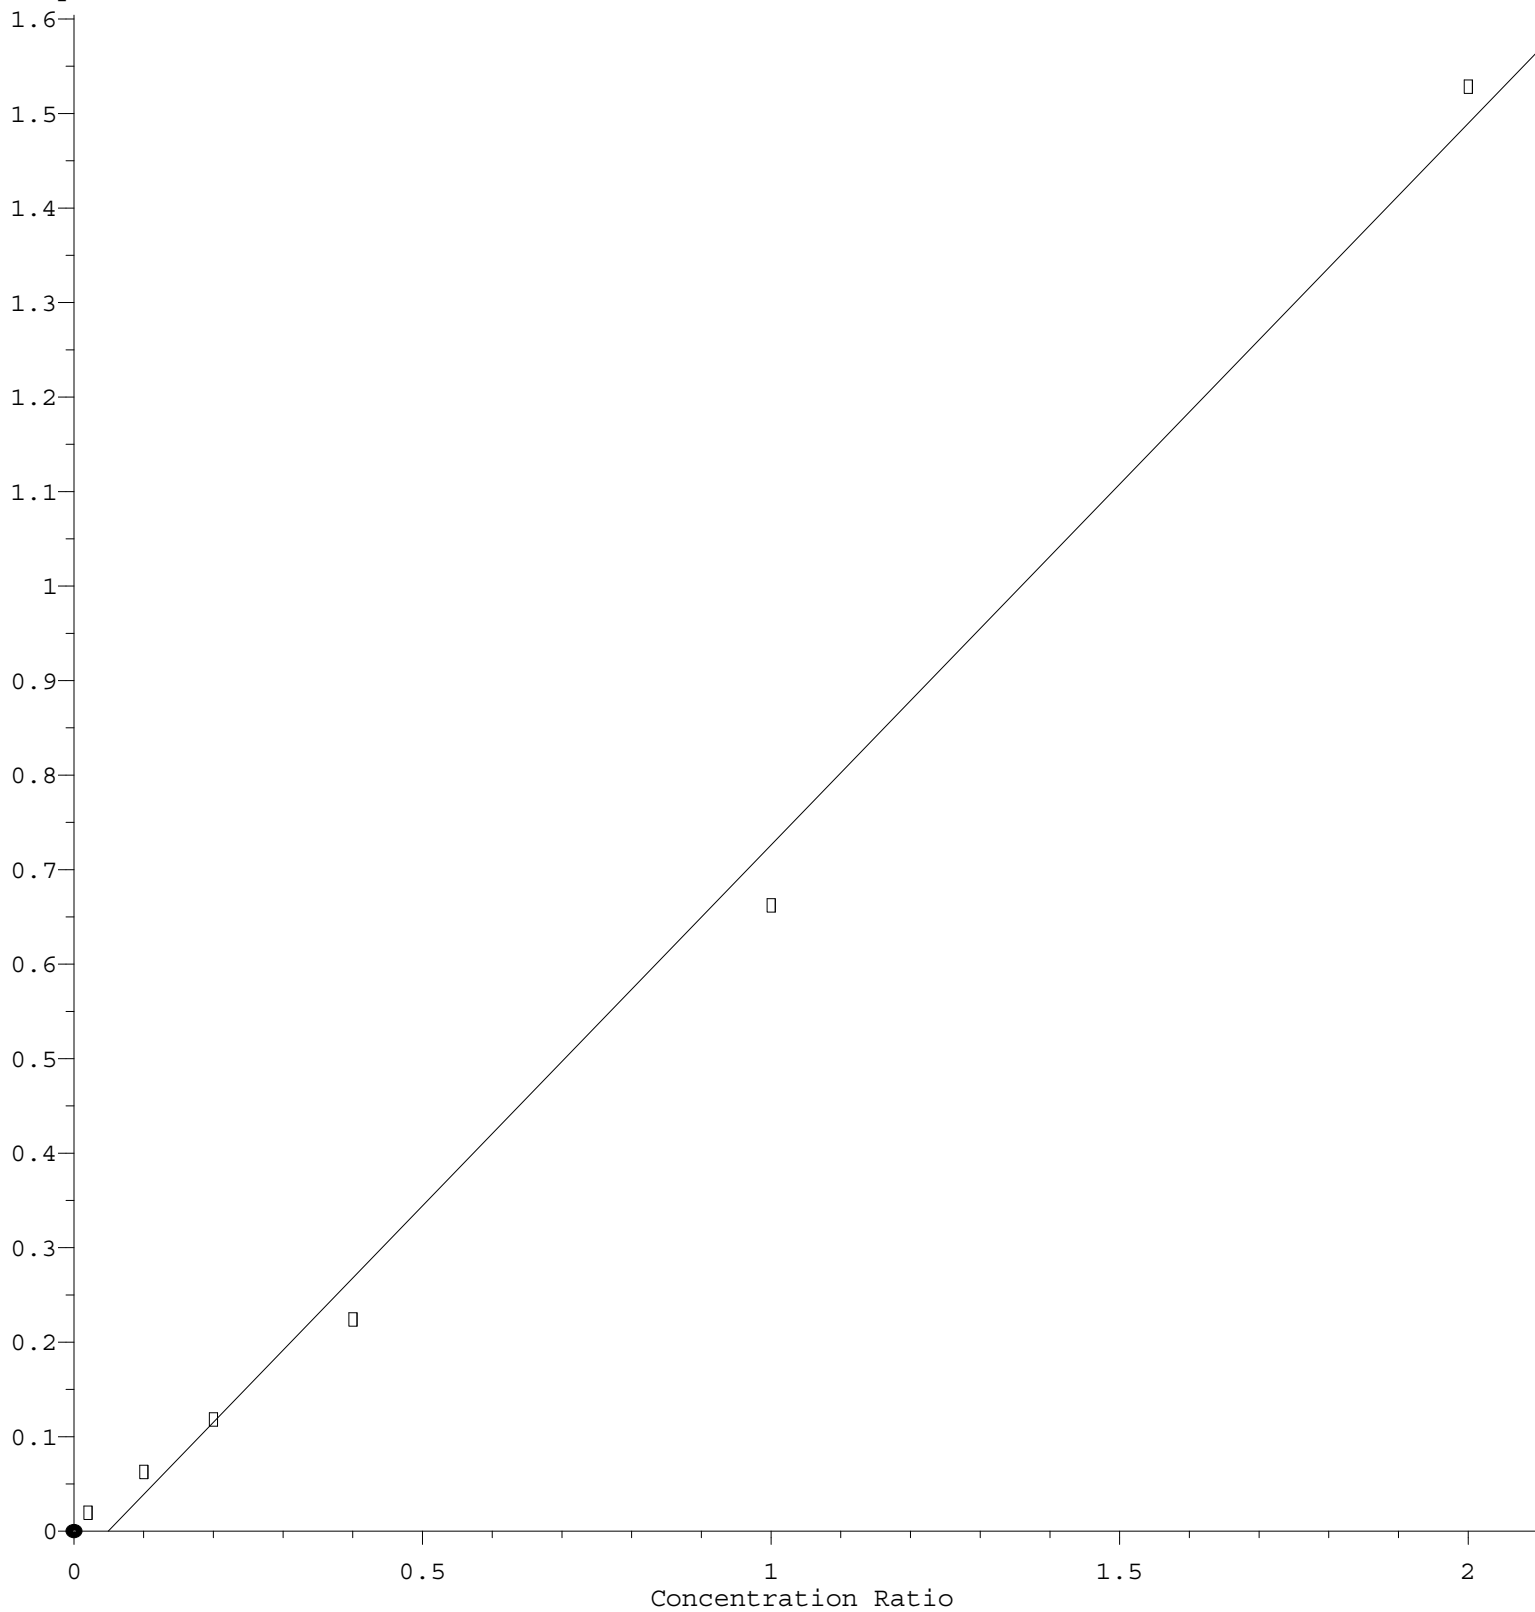

$$\text{Response} = 7.636\text{e-}001 * \text{Amt} - 3.767\text{e-}002$$

Coef of Det (r^2) = 0.994216 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N072921W.M

Calibration Table Last Updated: Thu Jul 29 15:02:35 2021