


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072921\
Data File : VN067955.D
Acq On : 29 Jul 2021 9:07
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
Title : SW846 8260
Last Update : Thu Jul 29 15:02:35 2021

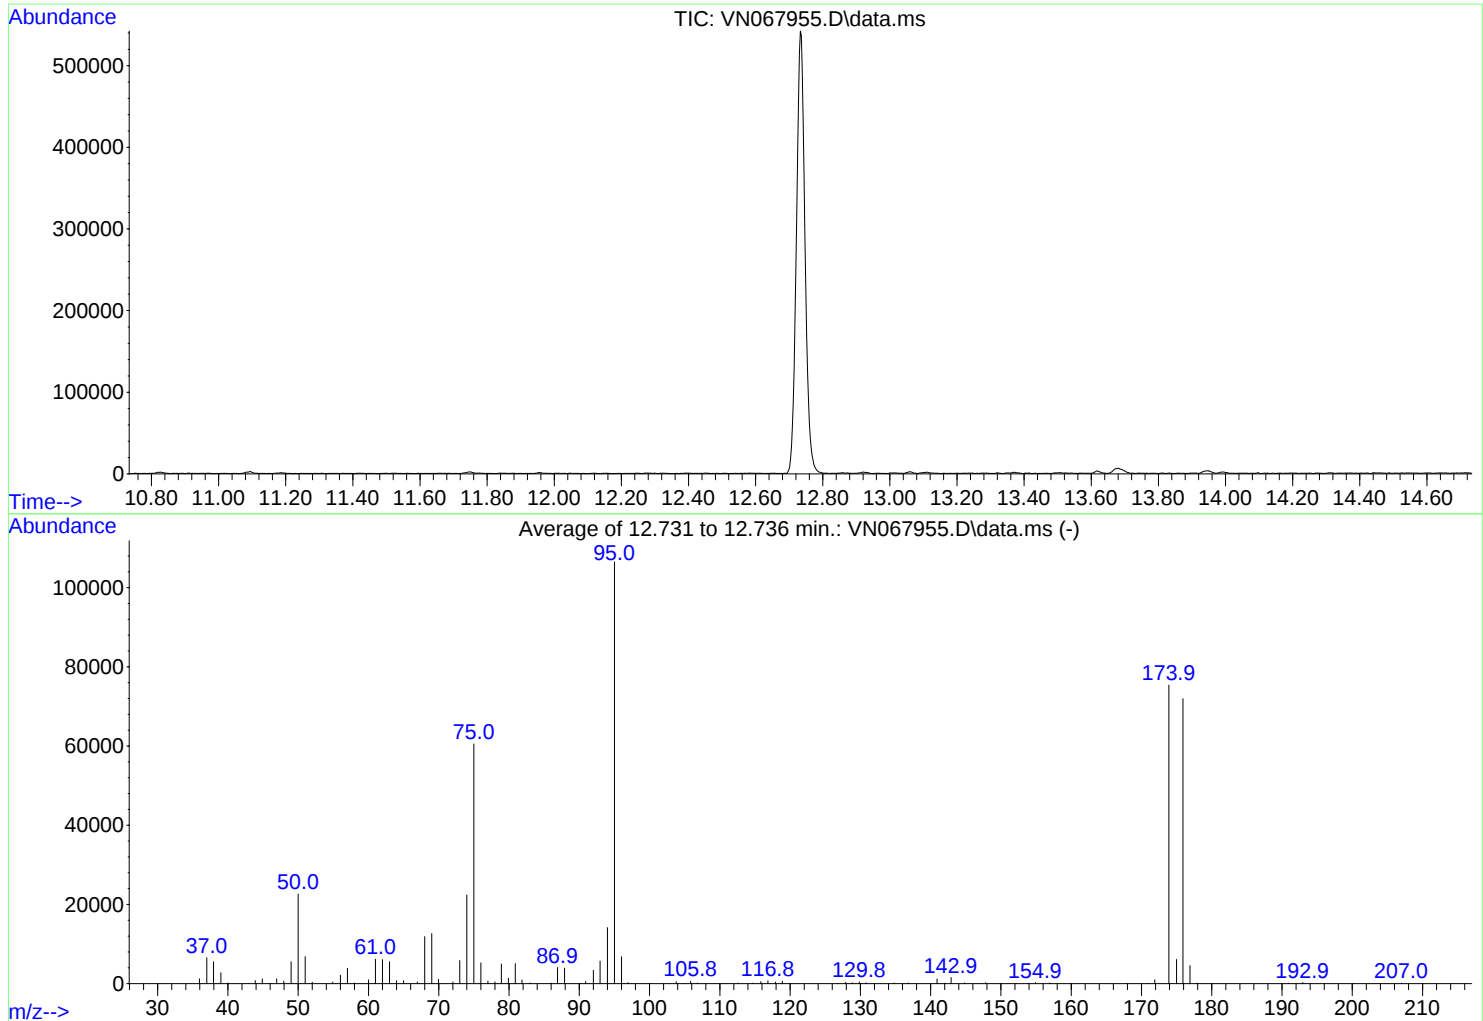

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.2	22600	PASS
75	95	30	60	56.8	60531	PASS
95	95	100	100	100.0	106525	PASS
96	95	5	9	6.4	6781	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.8	75392	PASS
175	174	5	9	8.1	6088	PASS
176	174	95	101	95.4	71960	PASS
177	176	5	9	6.3	4554	PASS