
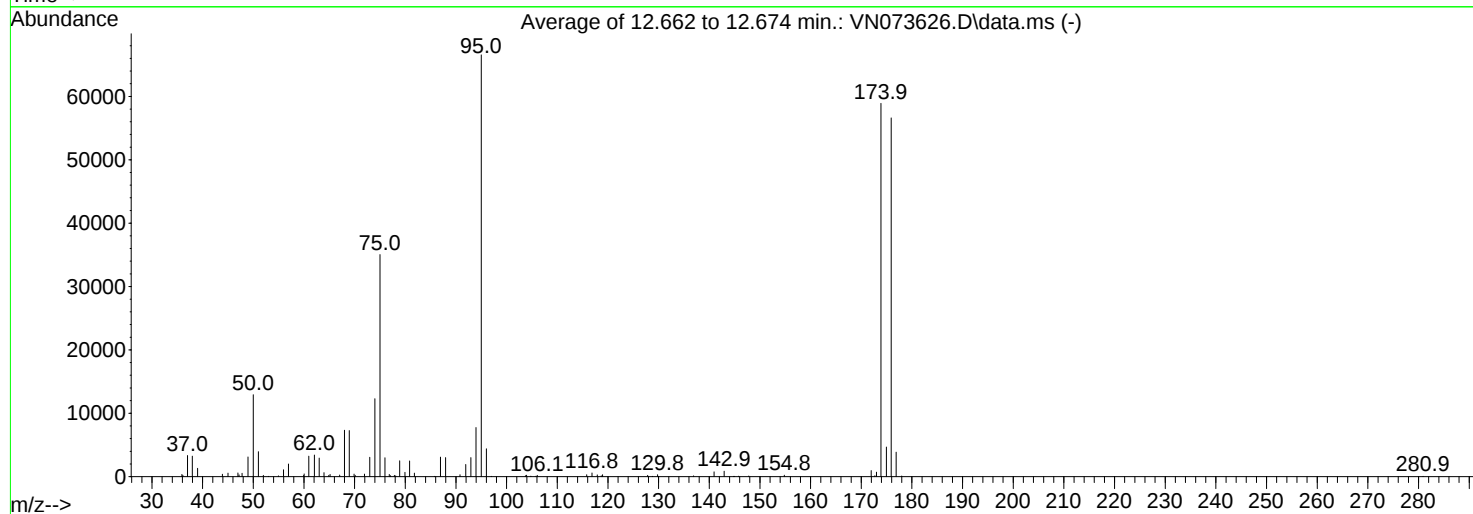


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072922\
 Data File : VN073626.D
 Acq On : 29 Jul 2022 09:46
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N072722W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Jul 27 18:07:26 2022

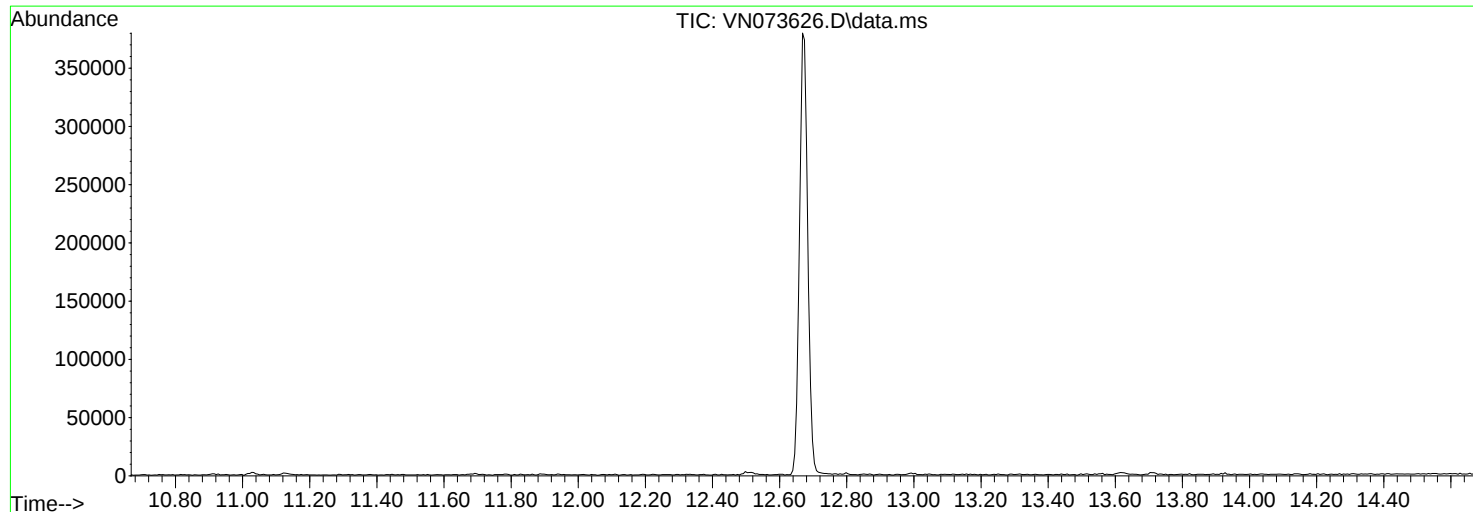

Spectrum Information: Average of 12.662 to 12.674 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	12937	PASS
75	95	30	60	52.6	35043	PASS
95	95	100	100	100.0	66560	PASS
96	95	5	9	6.6	4387	PASS
173	174	0.00	2	1.2	704	PASS
174	95	50	100	88.5	58899	PASS
175	174	5	9	7.9	4671	PASS
176	174	95	101	96.1	56608	PASS
177	176	5	9	6.8	3856	PASS