


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN073018\
Data File : VN050175.D
Acq On : 30 Jul 2018 9:32
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072418W.M
Title : SW846 8260
Last Update : Thu Jul 26 18:10:10 2018

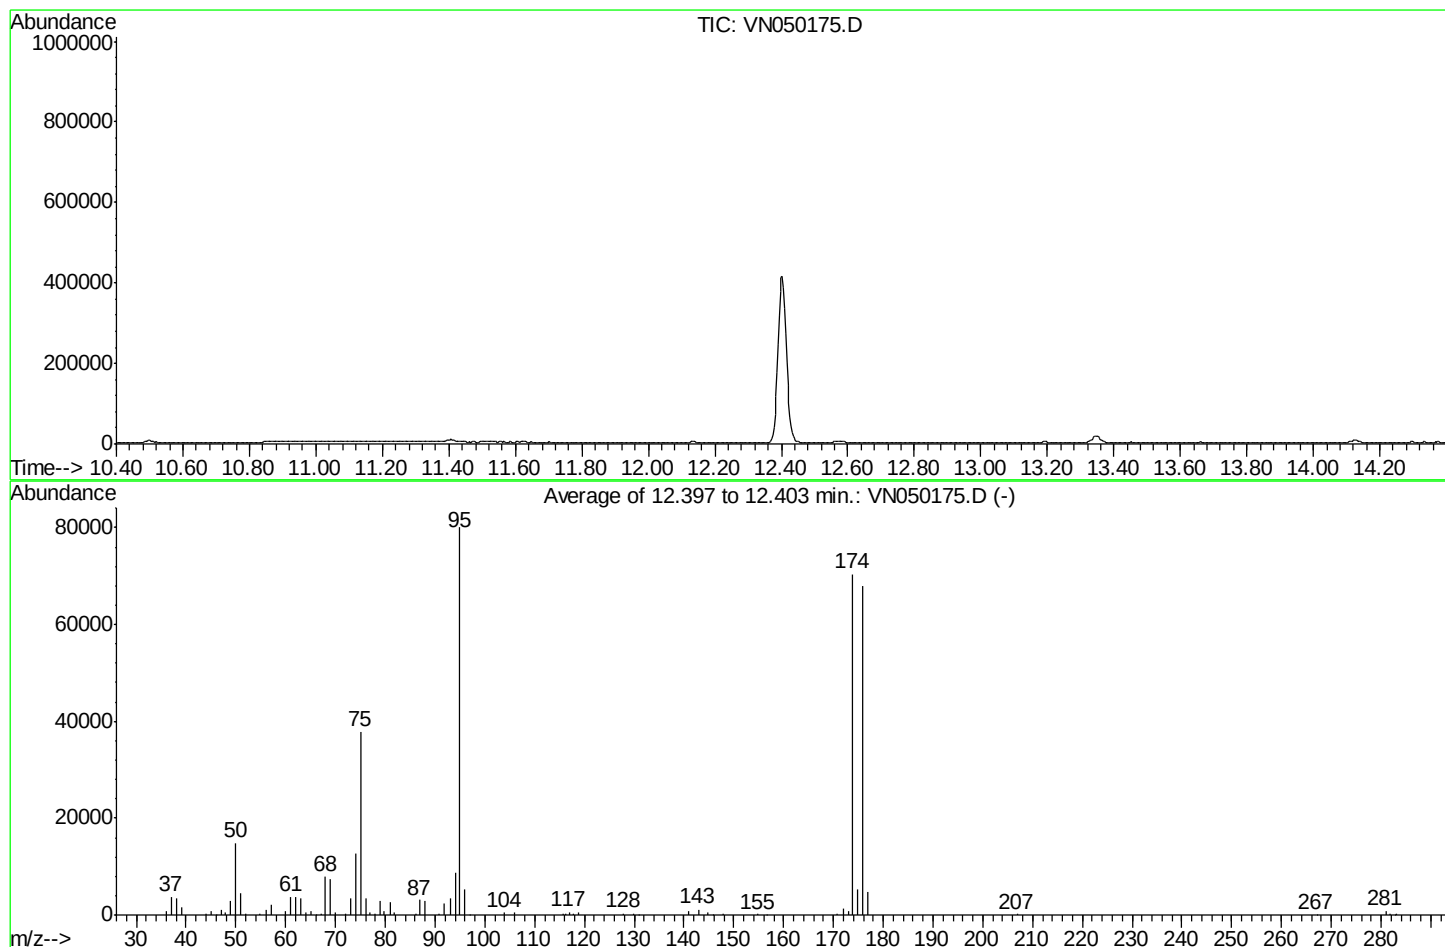

AutoFind: Scans 3361, 3362, 3363; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	14831	PASS
75	95	30	60	47.3	37896	PASS
95	95	100	100	100.0	80053	PASS
96	95	5	9	6.5	5169	PASS
173	174	0.00	2	1.0	699	PASS
174	95	50	100	87.9	70362	PASS
175	174	5	9	7.5	5268	PASS
176	174	95	101	96.6	67954	PASS
177	176	5	9	6.8	4645	PASS