

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN073019\
 Data File : VN056983.D
 Acq On : 30 Jul 2019 17:53
 Operator : JC/SP
 Sample : K4017-06
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 31 04:16:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 30 01:50:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	36718	5.00	ug/l	0.01
4) 1,4-Difluorobenzene	8.58	114	59083	5.00	ug/l	0.01
8) Chlorobenzene-d5	11.40	117	34212	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.35	152	4787	5.00	ug/l	0.00

System Monitoring Compounds

3) 1,2-Dichloroethane-d4	8.00	65	20126	4.42	ug/l	0.00
Spiked Amount	5.000	Range	81 - 118	Recovery	=	88.40%
5) Dibromofluoromethane	7.57	113	17060	4.25	ug/l	0.00
Spiked Amount	5.000	Range	80 - 119	Recovery	=	85.00%
6) Toluene-d8	10.08	98	32942	4.02	ug/l	0.00
Spiked Amount	5.000	Range	89 - 112	Recovery	=	80.40%#
7) 4-Bromofluorobenzene	12.40	95	7514	3.93	ug/l	0.00
Spiked Amount	5.000	Range	85 - 114	Recovery	=	78.60%#


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN073019\
Data File : VN056983.D
Acq On : 30 Jul 2019 17:53
Operator : JC/SP
Sample : K4017-06
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 31 04:16:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Tue Jul 30 01:50:04 2019
Response via : Initial Calibration

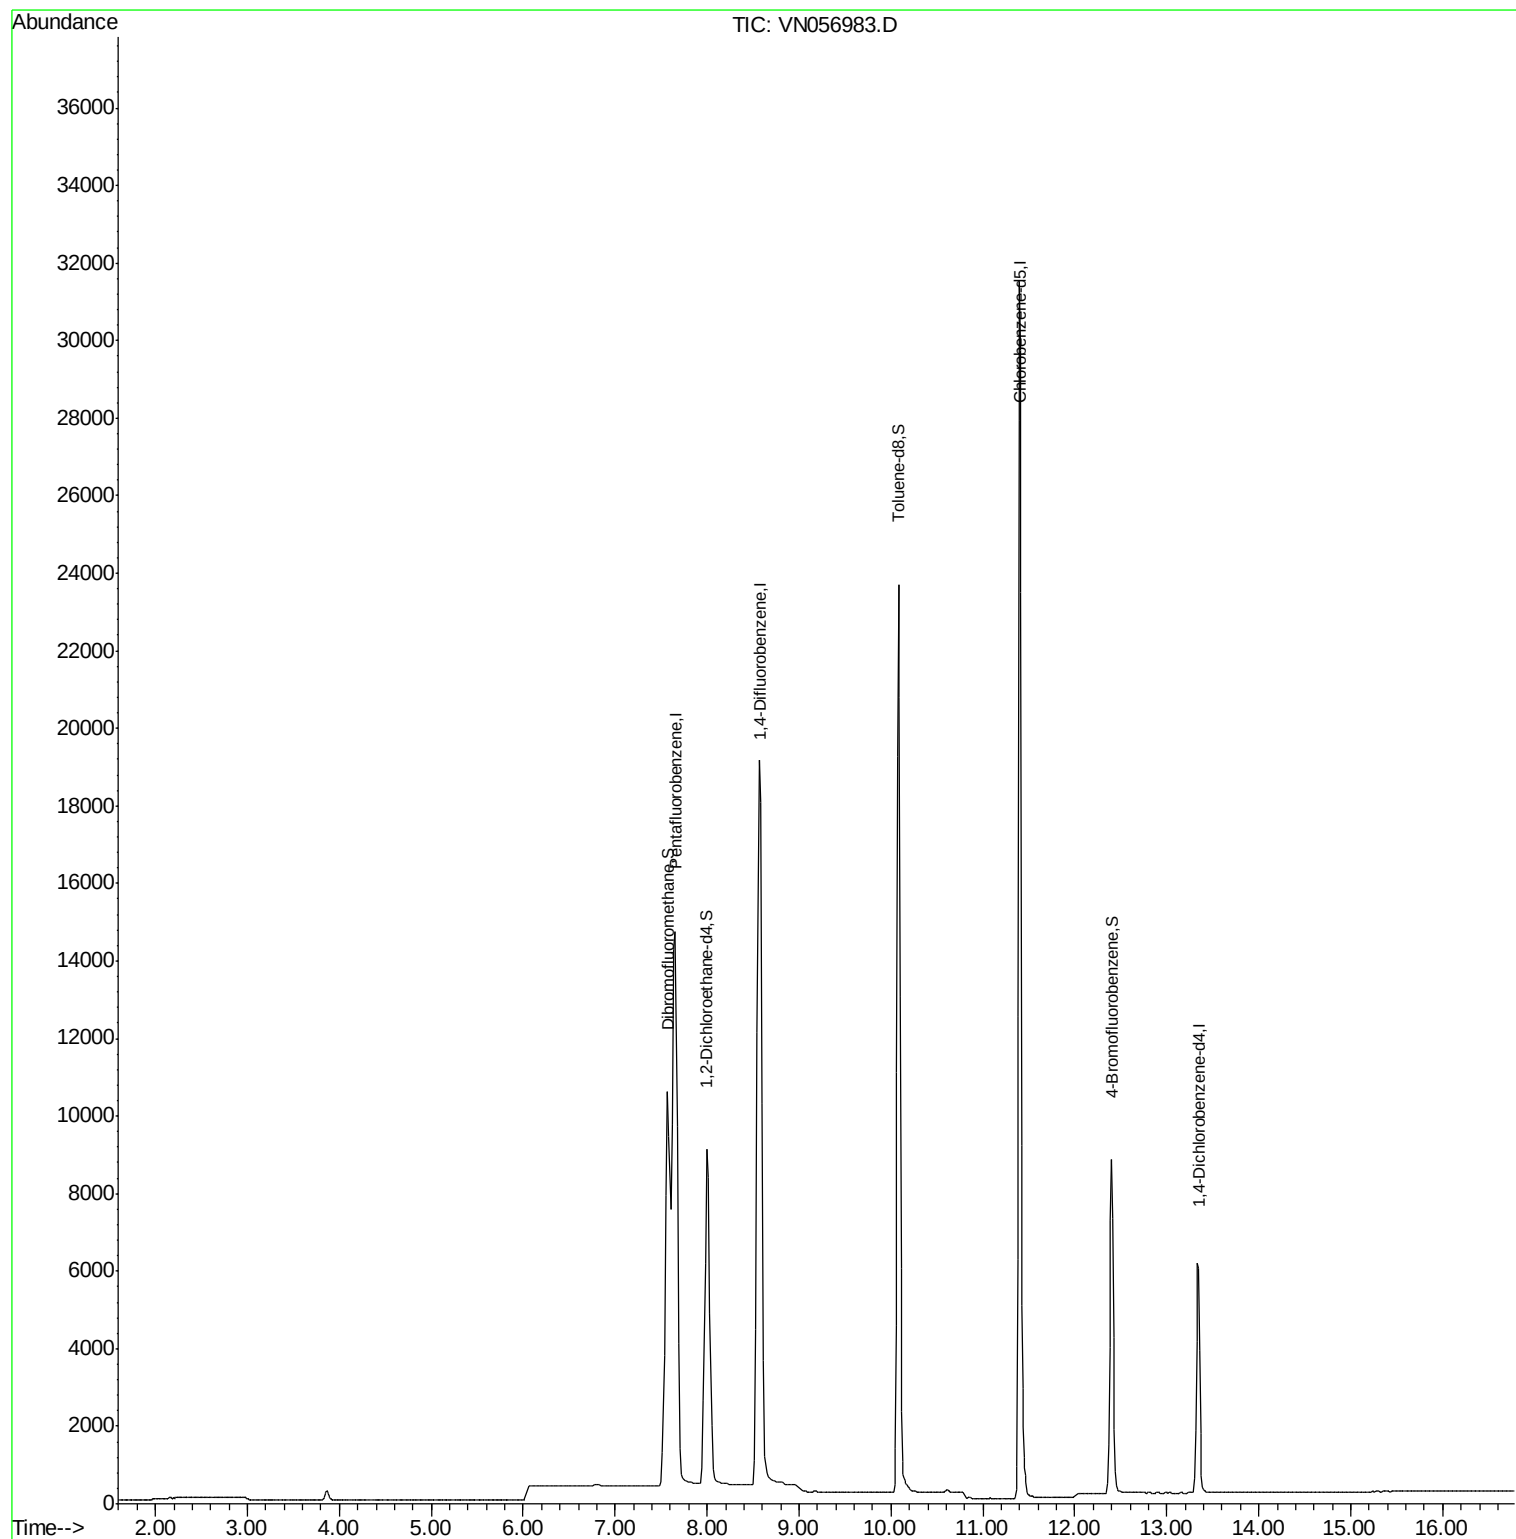

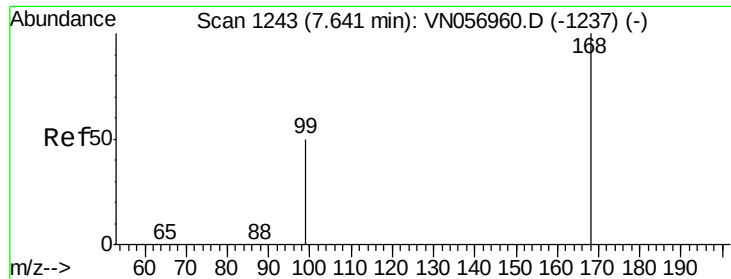

#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.65 min Scan# 1243

Delta R.T. 0.01 min

Lab File: VN056983.D

Acq: 30 Jul 2019 17:53


Instrument :
MSVOA_N
ClientSampled :

Tot Ion:168 Resp: 36718

Ion Ratio Lower Upper




168 100

99 43.2 40.0 60.0

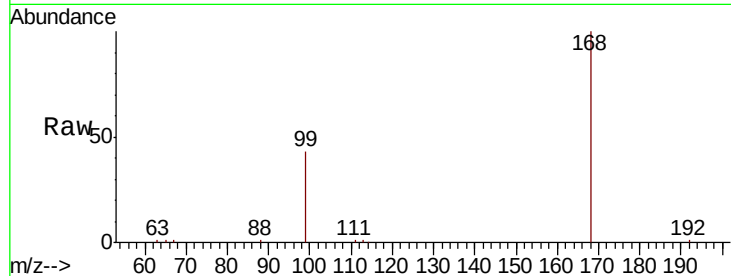

Abundance Ion 168.00 (167.70 to 168.70): V

Ion 99.00 (98.70 to 99.70): VN

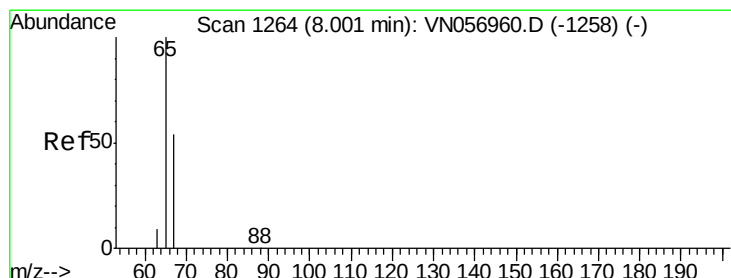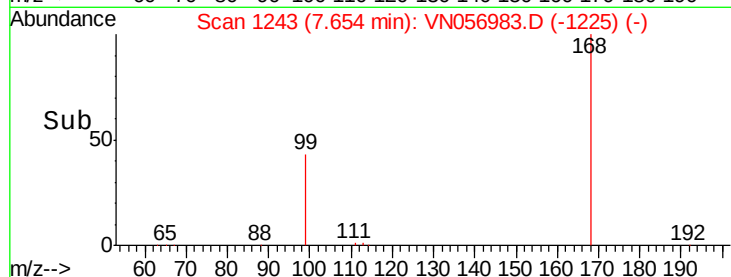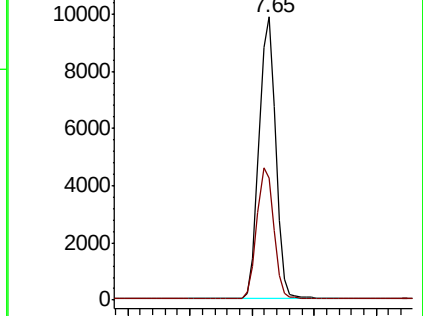

#3

1,2-Dichloroethane-d4

Concen: 4.423 ug/l

RT: 8.00 min Scan# 1263

Delta R.T. -0.00 min

Lab File: VN056983.D


Acq: 30 Jul 2019 17:53

Tgt Ion: 65 Resp: 20126

Ion Ratio Lower Upper



65 100


67 54.4 0.0 109.6

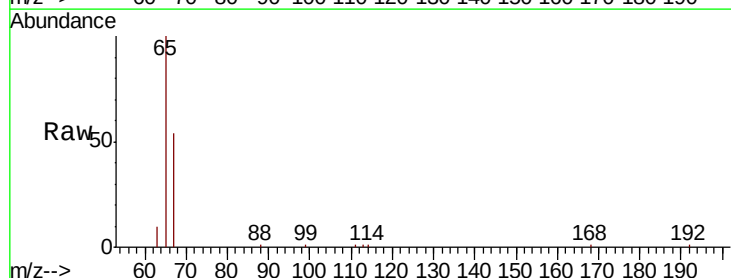

Abundance Ion 65.00 (64.70 to 65.70): VN

Ion 67.00 (66.70 to 67.70): VN

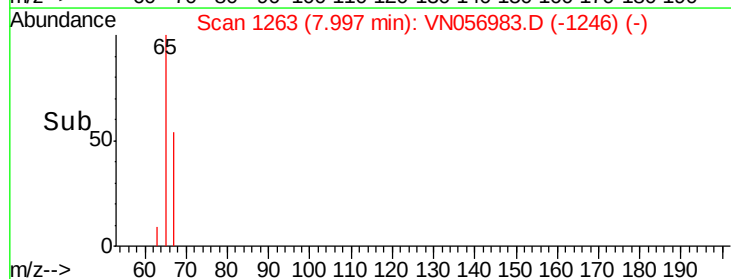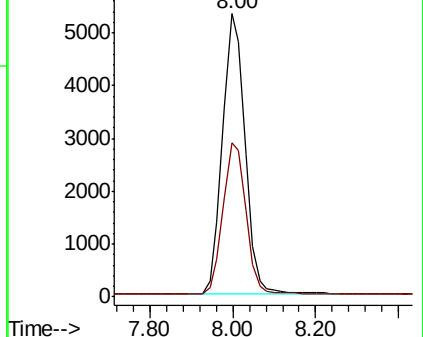

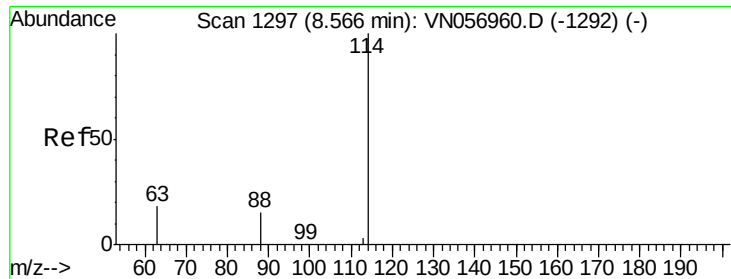

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.58 min Scan# 1297

Delta R.T. 0.01 min

Lab File: VN056983.D

Acq: 30 Jul 2019 17:53

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:114 Resp: 59083

Ion Ratio Lower Upper

114 100

63 14.5 0.0 37.6




88 13.6 0.0 31.0

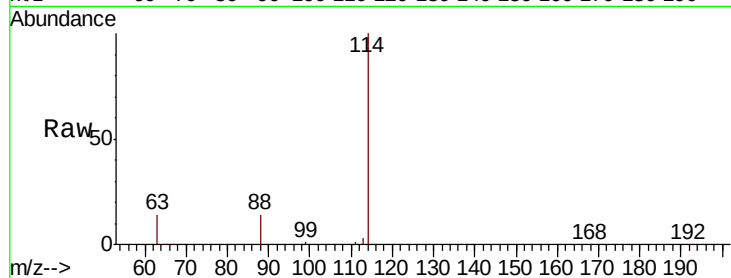

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VN

Ion 88.00 (87.70 to 88.70): VN

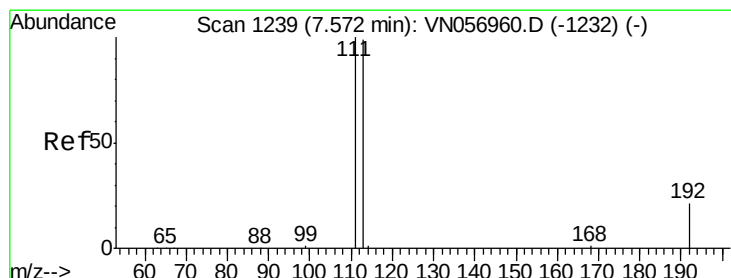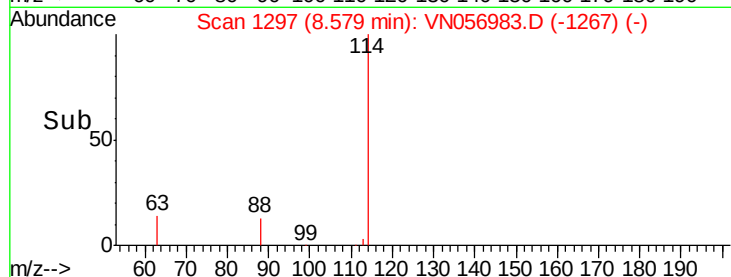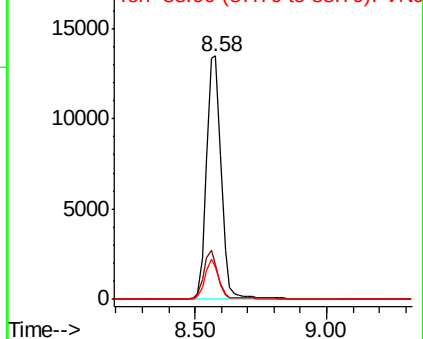

#5

Dibromofluoromethane

Concen: 4.250 ug/l

RT: 7.57 min Scan# 1238

Delta R.T. -0.00 min

Lab File: VN056983.D

Acq: 30 Jul 2019 17:53


Tgt Ion:113 Resp: 17060

Ion Ratio Lower Upper

113 100

111 103.8 81.1 121.7



192 21.7 17.9 26.9

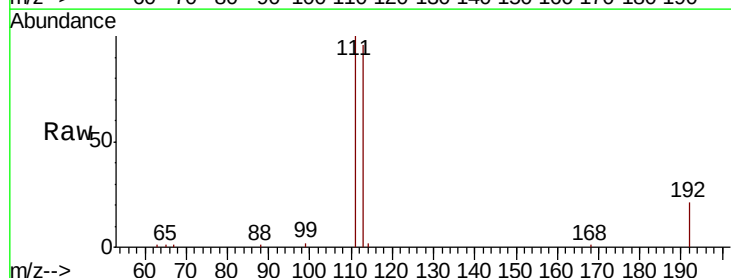


Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V

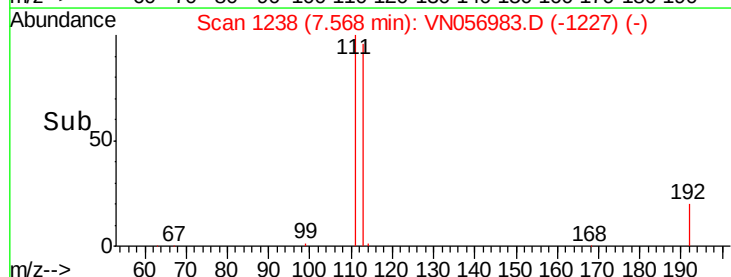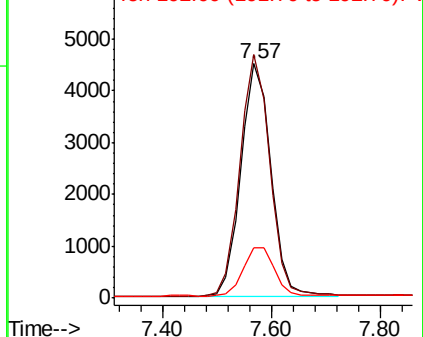

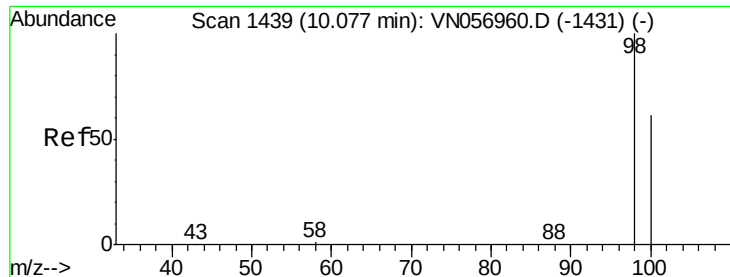

#6

Toluene-d8

Concen: 4.022 ug/l

RT: 10.08 min Scan# 1439

Delta R.T. 0.00 min

Lab File: VN056983.D

Acq: 30 Jul 2019 17:53

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion: 98 Resp: 32942

Ion Ratio Lower Upper




98 100

100 62.6 49.0 73.4

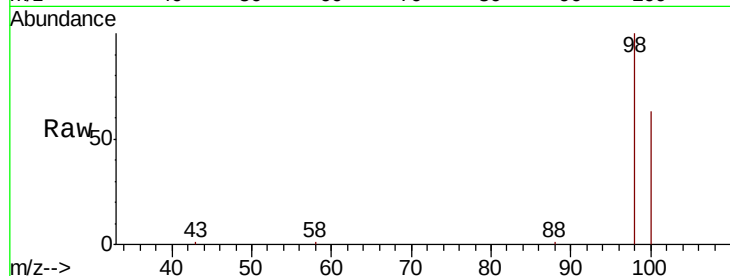

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

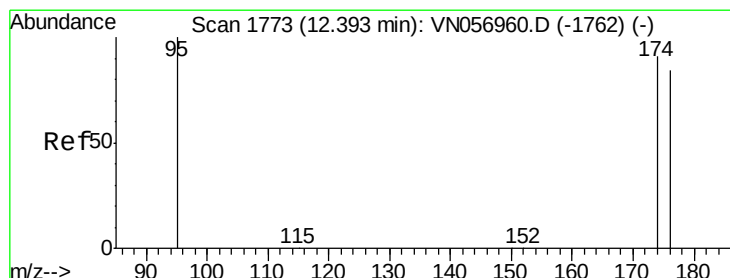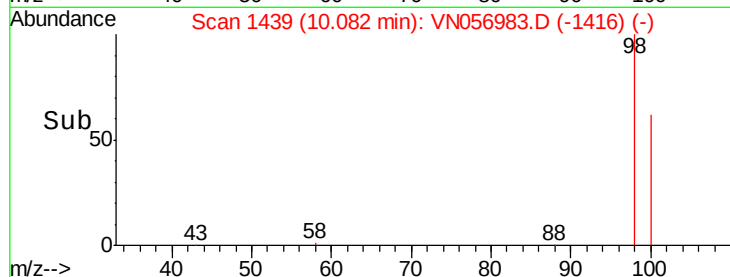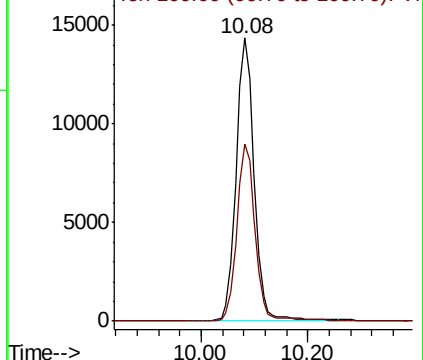

#7

4-Bromofluorobenzene

Concen: 3.930 ug/l

RT: 12.40 min Scan# 1773

Delta R.T. 0.00 min

Lab File: VN056983.D

Acq: 30 Jul 2019 17:53


Tgt Ion: 95 Resp: 7514

Ion Ratio Lower Upper

95 100

174 100.0 0.0 181.4



176 94.7 0.0 168.2

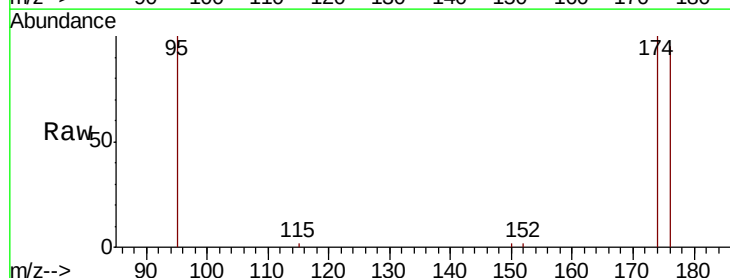


Abundance Ion 95.00 (94.70 to 95.70): VN0

Ion 174.00 (173.70 to 174.70): V

Ion 176.00 (175.70 to 176.70): V

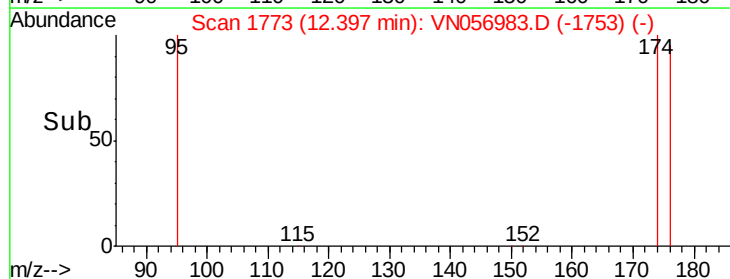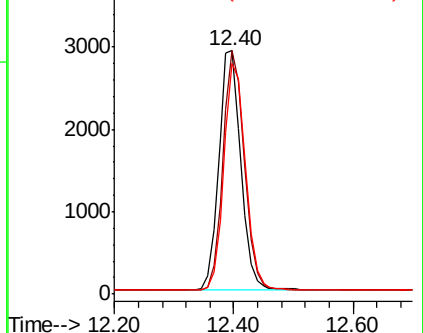

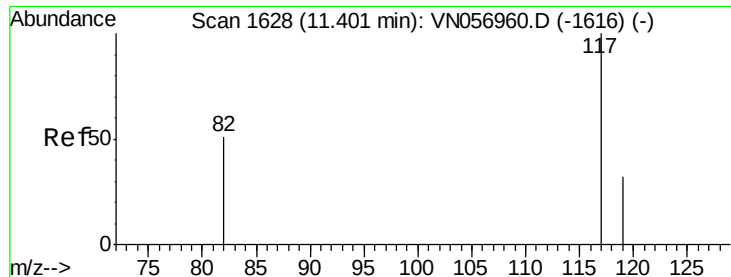

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.40 min Scan# 1627

Delta R.T. -0.00 min

Lab File: VN056983.D

Acq: 30 Jul 2019 17:53

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:117 Resp: 34212

Ion Ratio Lower Upper

117 100

82 51.7 40.7 61.1




119 31.8 25.6 38.4

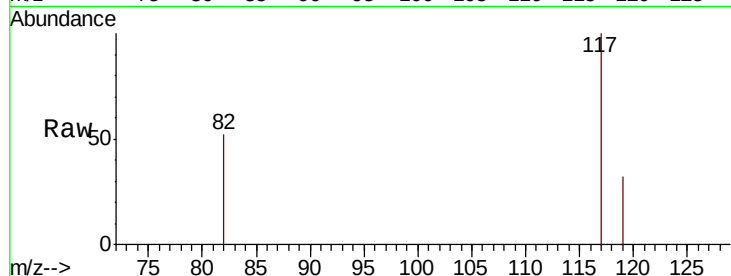

Abundance Ion 117.00 (116.70 to 117.70): V

Ion 82.00 (81.70 to 82.70): VN

Ion 119.00 (118.70 to 119.70): V

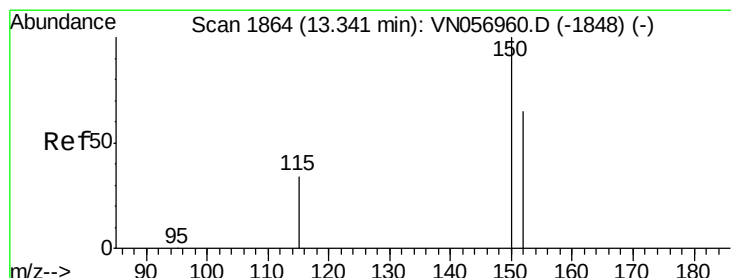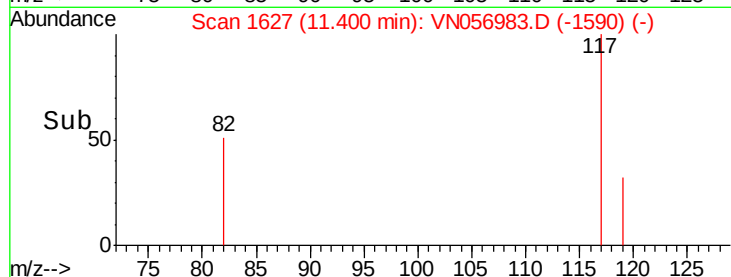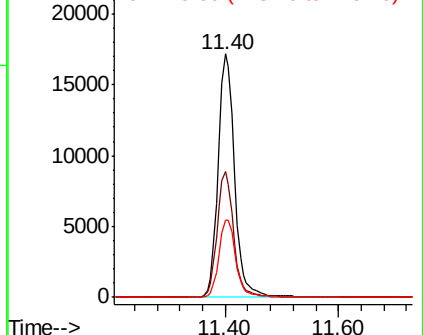

#9

1,4-Dichlorobenzene-d4

Concen: 5.000 ug/l

RT: 13.35 min Scan# 1864

Delta R.T. 0.00 min

Lab File: VN056983.D

Acq: 30 Jul 2019 17:53


Tgt Ion:152 Resp: 4787

Ion Ratio Lower Upper

152 100

115 51.4 27.0 80.8

150 149.9 0.0 306.8

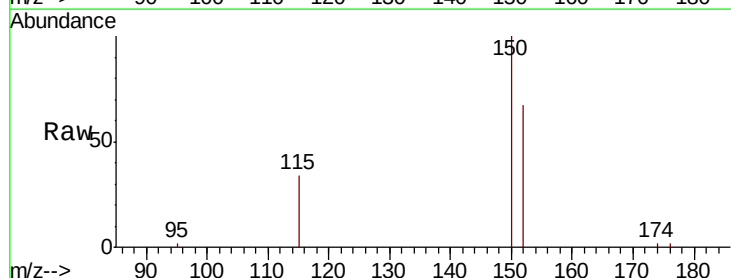

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

