

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN073019\
 Data File : VN056987.D
 Acq On : 30 Jul 2019 19:26
 Operator : JC/SP
 Sample : K4017-10
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 31 04:16:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 30 01:50:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	36004	5.00	ug/l	0.01
4) 1,4-Difluorobenzene	8.58	114	58138	5.00	ug/l	0.01
8) Chlorobenzene-d5	11.40	117	33736	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.35	152	4825	5.00	ug/l	0.00

System Monitoring Compounds

3) 1,2-Dichloroethane-d4	8.00	65	20663	4.63	ug/l	0.00
Spiked Amount	5.000	Range	81 - 118	Recovery	=	92.60%
5) Dibromofluoromethane	7.57	113	17406	4.41	ug/l	0.00
Spiked Amount	5.000	Range	80 - 119	Recovery	=	88.20%
6) Toluene-d8	10.08	98	33735	4.19	ug/l	0.00
Spiked Amount	5.000	Range	89 - 112	Recovery	=	83.80%#
7) 4-Bromofluorobenzene	12.40	95	7814	4.15	ug/l	0.00
Spiked Amount	5.000	Range	85 - 114	Recovery	=	83.00%#

Target Compounds


	R.T.	QIon	Response	Conc	Units	Qvalue
2) Vinyl Chloride	2.16	62	86	0.026	ug/l #	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN073019\
Data File : VN056987.D
Acq On : 30 Jul 2019 19:26
Operator : JC/SP
Sample : K4017-10
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 31 04:16:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Tue Jul 30 01:50:04 2019
Response via : Initial Calibration

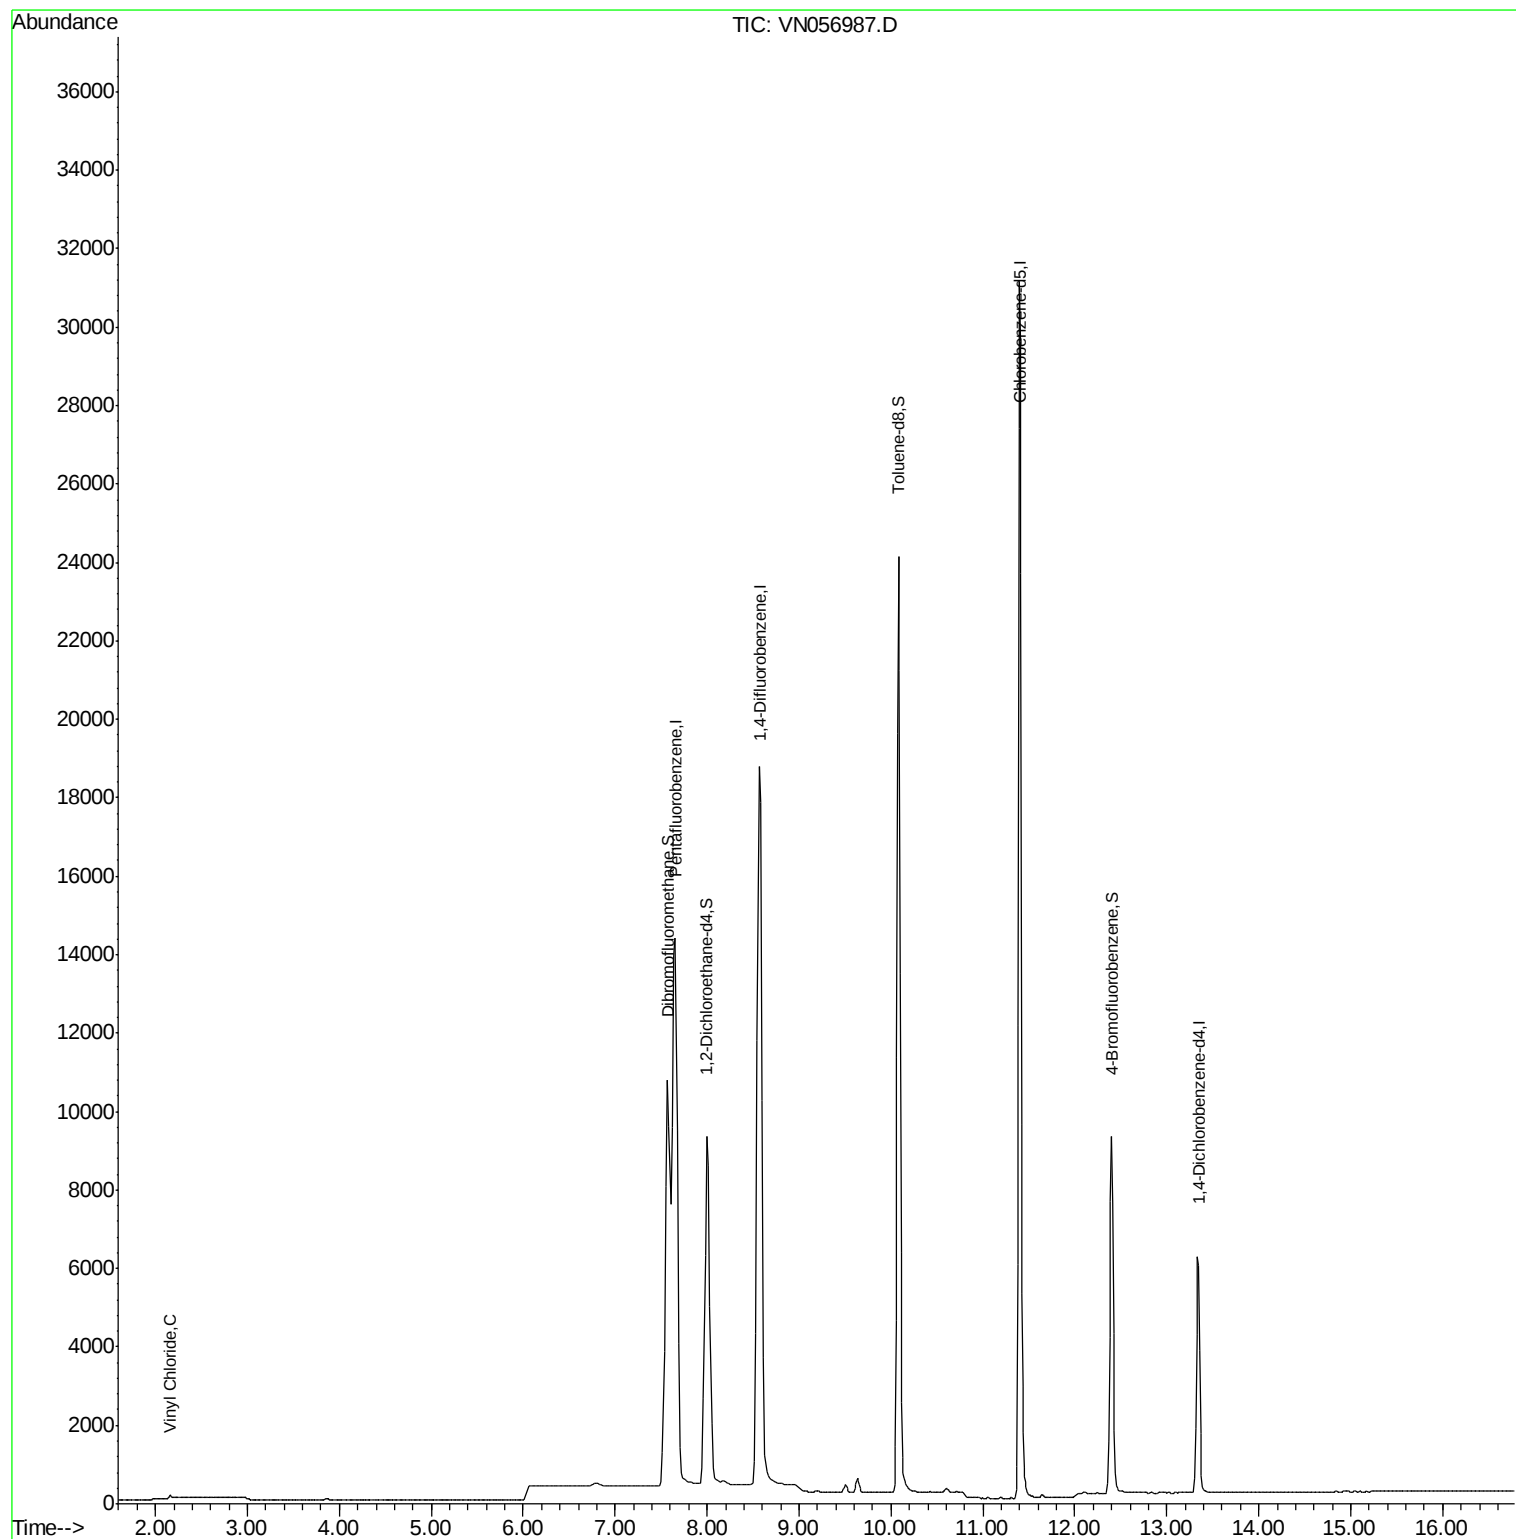

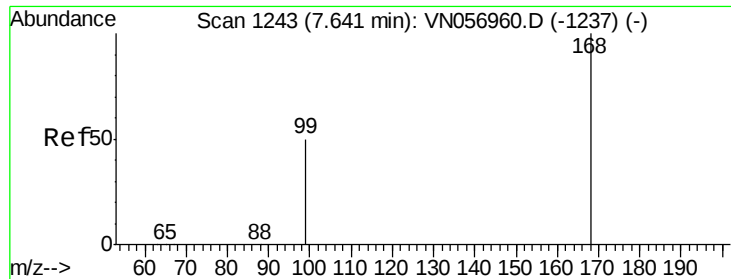

#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.65 min Scan# 1243

Delta R.T. 0.01 min

Lab File: VN056987.D

Acq: 30 Jul 2019 19:26

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion:168 Resp: 36004

Ion Ratio Lower Upper




168 100

99 42.7 40.0 60.0

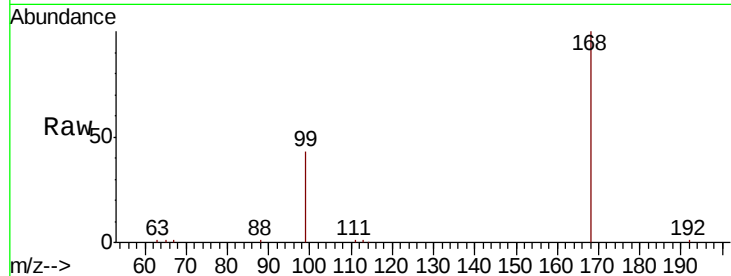

Abundance Ion 168.00 (167.70 to 168.70): V

Ion 99.00 (98.70 to 99.70): VN

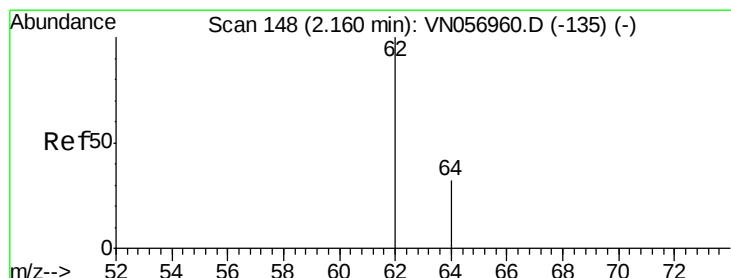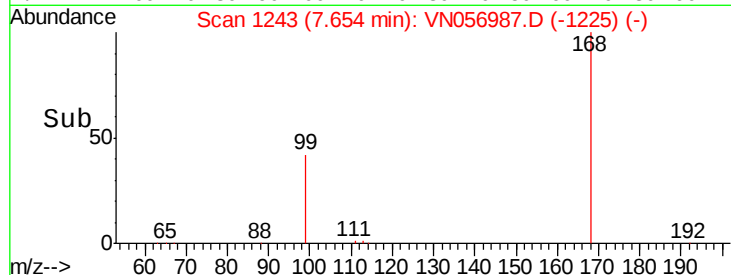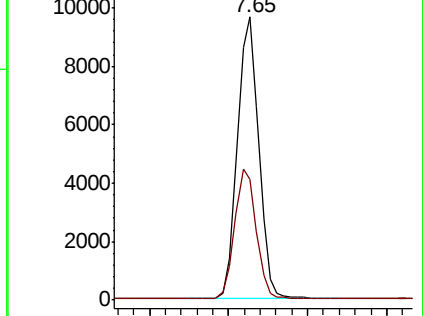

#2

Vinyl Chloride

Concen: 0.026 ug/l

RT: 2.16 min Scan# 148

Delta R.T. 0.00 min

Lab File: VN056987.D


Acq: 30 Jul 2019 19:26

Tgt Ion: 62 Resp: 86

Ion Ratio Lower Upper



62 100


64 85.3 26.4 39.6#

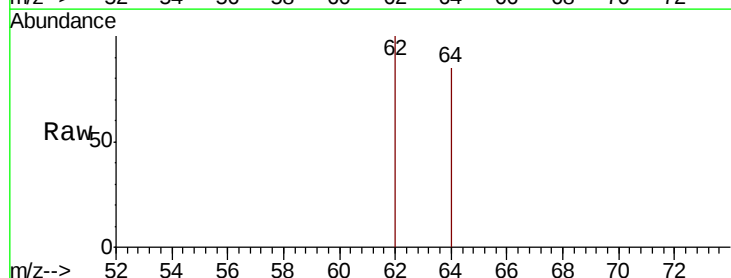

Abundance Ion 62.00 (61.70 to 62.70): VN

Ion 64.00 (63.70 to 64.70): VN

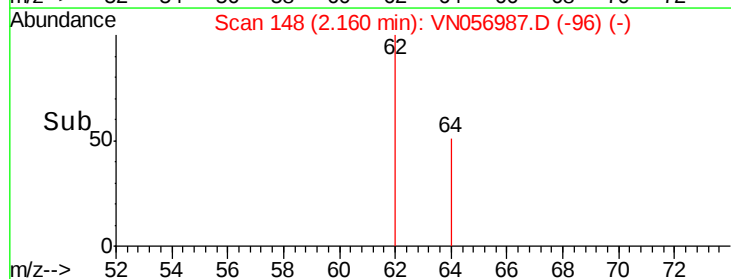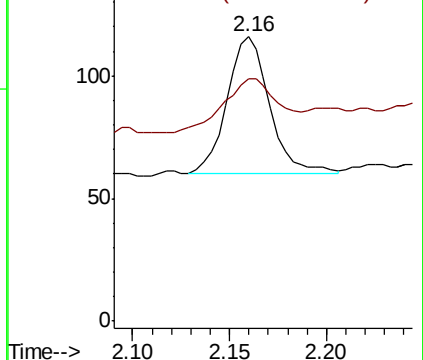

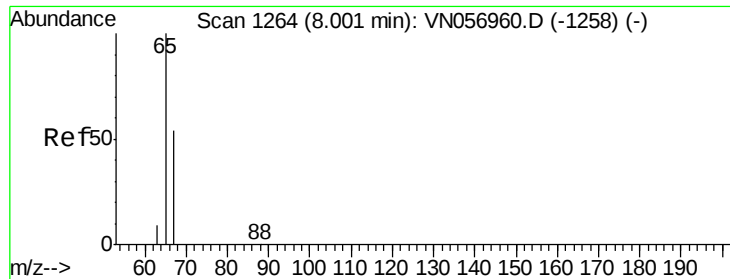

#3

1,2-Dichloroethane-d4

Concen: 4.631 ug/l

RT: 8.00 min Scan# 1263

Delta R.T. -0.00 min





Lab File: VN056987.D

Acq: 30 Jul 2019 19:26

Instrument :
MSVOA_N
ClientSampleId :

Tot Ion: 65 Resp: 20663

Ion	Ratio	Lower	Upper
65	100		
67	54.1	0.0	109.6

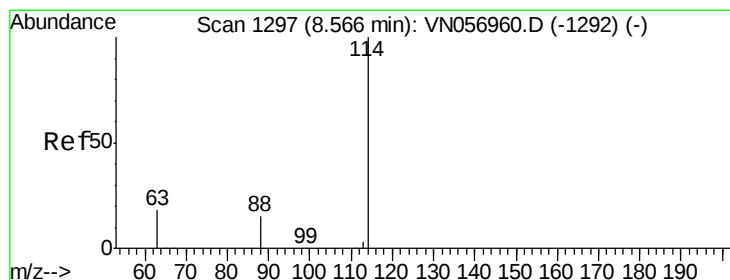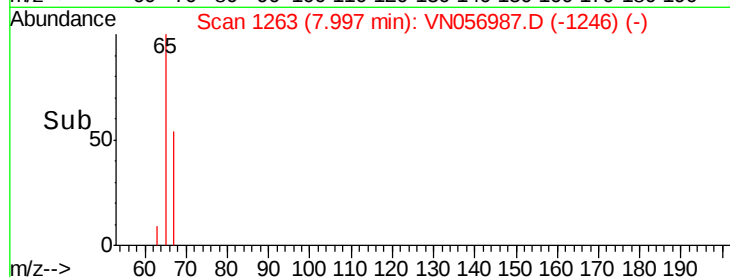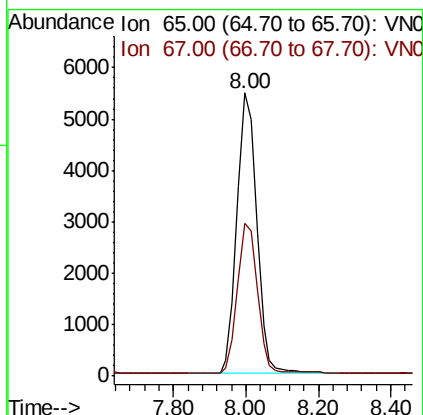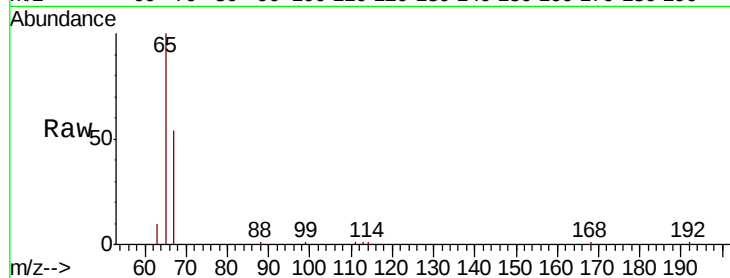

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.58 min Scan# 1297




Delta R.T. 0.01 min


Lab File: VN056987.D

Acq: 30 Jul 2019 19:26

Tgt Ion: 114 Resp: 58138

Ion	Ratio	Lower	Upper
114	100		
63	14.5	0.0	37.6
88	13.5	0.0	31.0

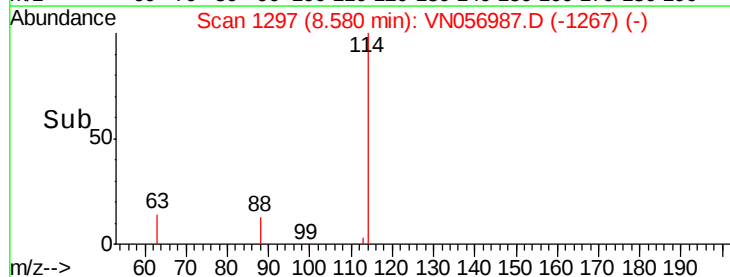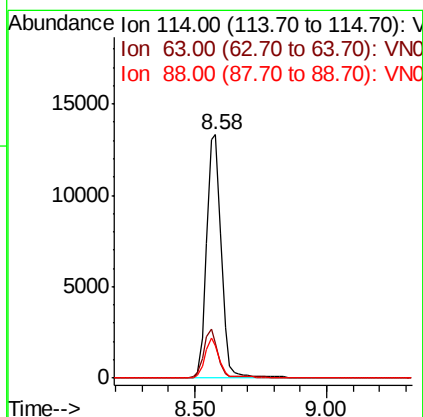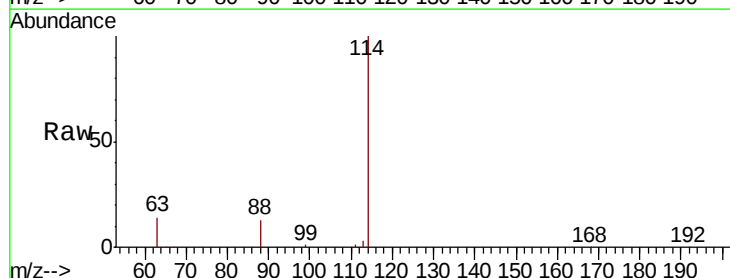

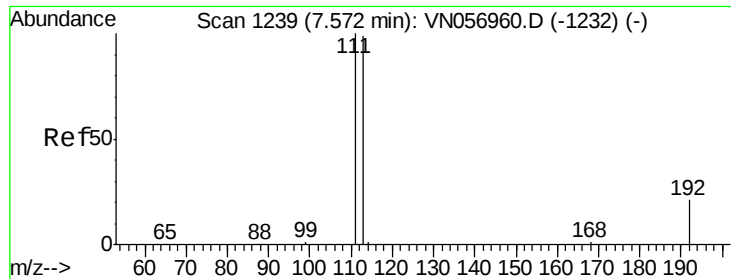

#5

Dibromofluoromethane

Concen: 4.407 ug/l

RT: 7.57 min Scan# 1238

Delta R.T. -0.00 min

Lab File: VN056987.D

Acq: 30 Jul 2019 19:26

Instrument :
MSVOA_N
ClientSampled :


Tot Ion:113 Resp: 17406

Ion Ratio Lower Upper




113 100

111 103.3 81.1 121.7

192 21.8 17.9 26.9

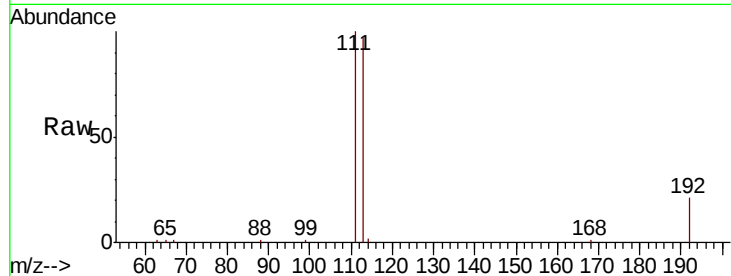

Abundance Ion 113.00 (112.70 to 113.70): V
Ion 111.00 (110.70 to 111.70): V
Ion 192.00 (191.70 to 192.70): V

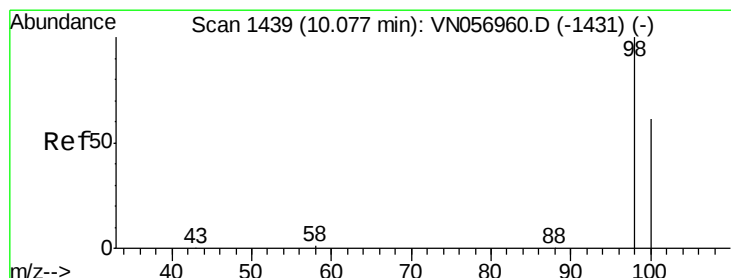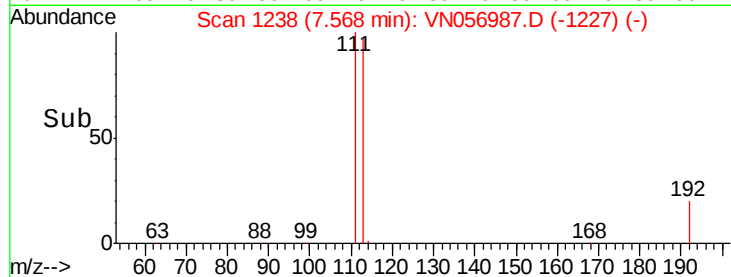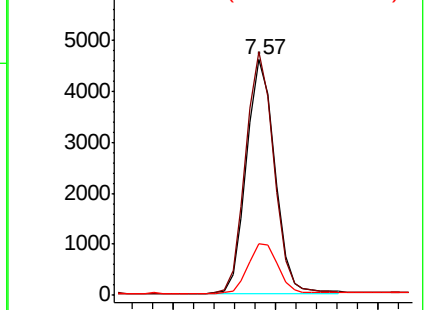

#6

Toluene-d8

Concen: 4.185 ug/l

RT: 10.08 min Scan# 1439

Delta R.T. 0.00 min

Lab File: VN056987.D


Acq: 30 Jul 2019 19:26

Tgt Ion: 98 Resp: 33735



Ion Ratio Lower Upper


98 100

100 62.6 49.0 73.4

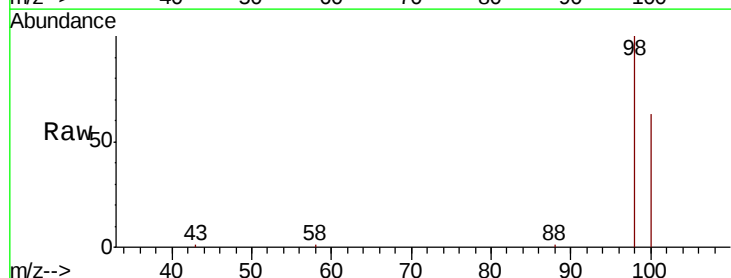

Abundance Ion 98.00 (97.70 to 98.70): VN
Ion 100.00 (99.70 to 100.70): VN

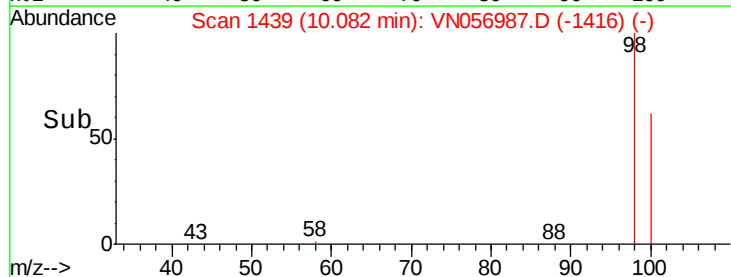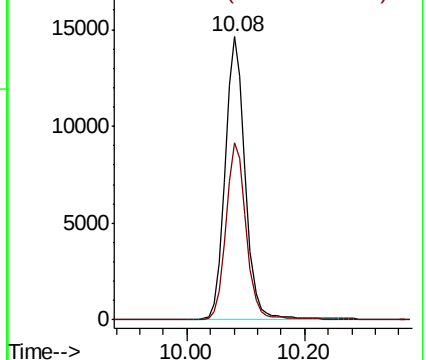

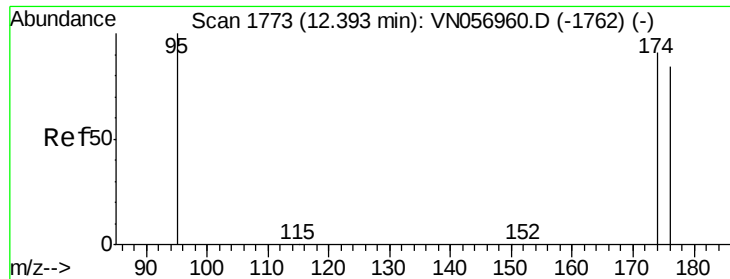

#7

4-Bromofluorobenzene

Concen: 4.154 ug/l

RT: 12.40 min Scan# 1773

Delta R.T. 0.00 min

Lab File: VN056987.D

Acq: 30 Jul 2019 19:26

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 95 Resp: 7814

Ion Ratio Lower Upper

95 100

174 101.1 0.0 181.4




176 95.6 0.0 168.2

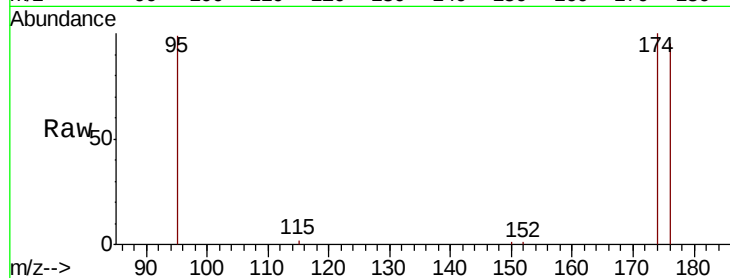

Abundance Ion 95.00 (94.70 to 95.70): VN056960.D (-1762) (-)

Ion 174.00 (173.70 to 174.70): VN056960.D (-1762) (-)

Ion 176.00 (175.70 to 176.70): VN056960.D (-1762) (-)

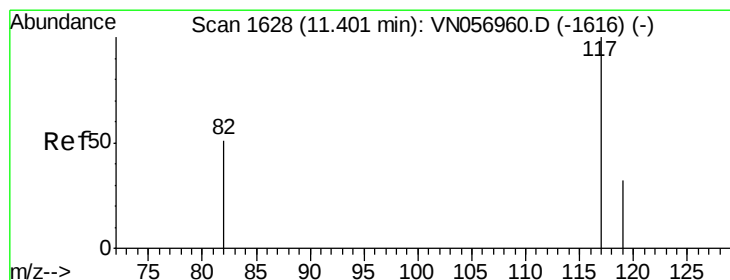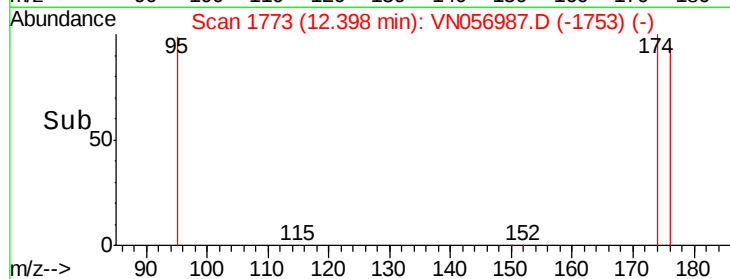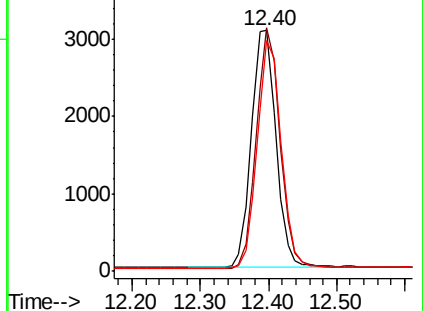

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.40 min Scan# 1627

Delta R.T. -0.00 min

Lab File: VN056987.D

Acq: 30 Jul 2019 19:26


Tgt Ion: 117 Resp: 33736

Ion Ratio Lower Upper

117 100

82 52.0 40.7 61.1



119 31.9 25.6 38.4



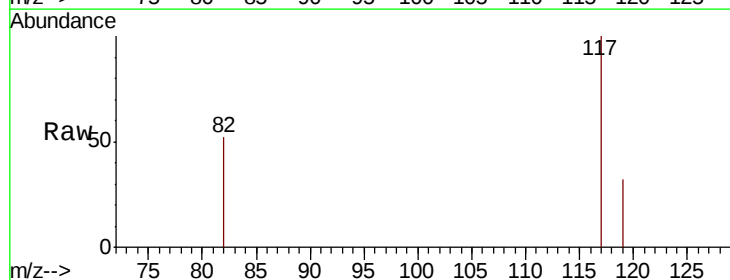


Abundance Ion 117.00 (116.70 to 117.70): VN056960.D (-1616) (-)

Ion 82.00 (81.70 to 82.70): VN056960.D (-1616) (-)

Ion 119.00 (118.70 to 119.70): VN056960.D (-1616) (-)

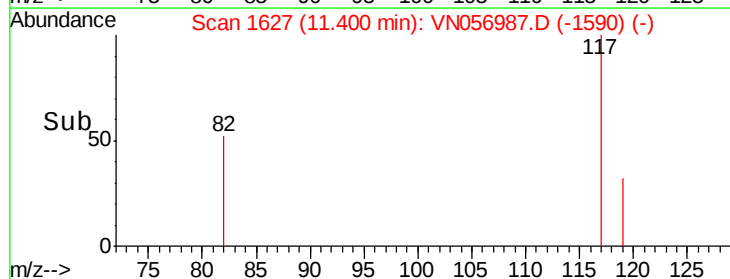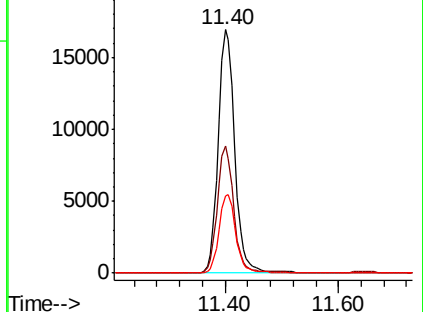

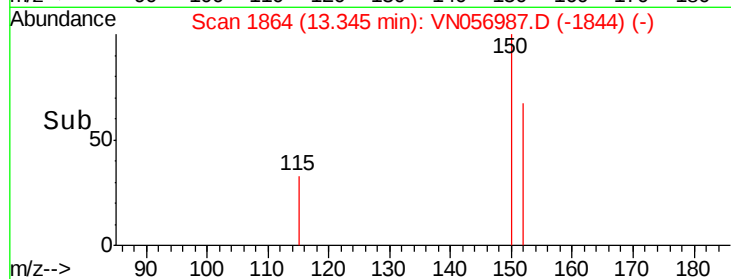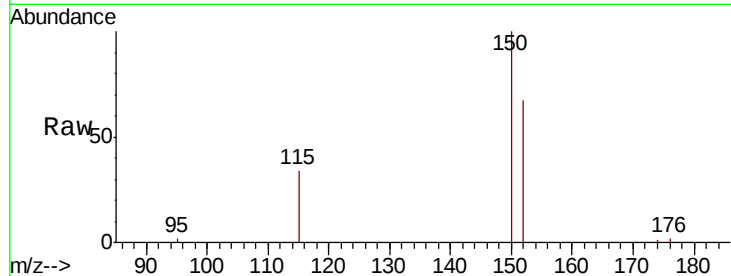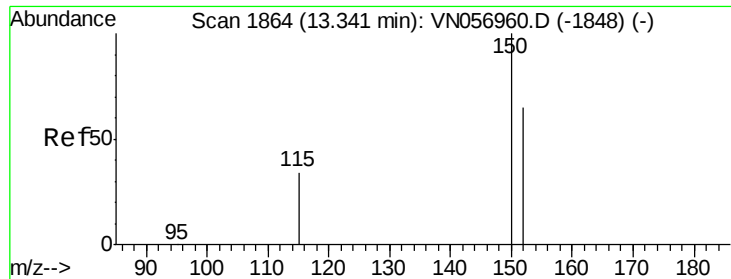

#9

1,4-Dichlorobenzene-d4

Concen: 5.000 ug/l

RT: 13.35 min Scan# 1864

Delta R.T. 0.00 min

Lab File: VN056987.D

Acq: 30 Jul 2019 19:26

Instrument :

MSVOA_N

ClientSampleId :

Tot Ion:152 Resp: 4825

Ion Ratio Lower Upper

152 100

115 50.6 27.0 80.8

150 148.6 0.0 306.8

