

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN073019\
 Data File : VN056968.D
 Acq On : 30 Jul 2019 12:05
 Operator : JC/SP
 Sample : VN0730WBS01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0730WBS01

Quant Time: Jul 31 04:14:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 30 01:50:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	48575	5.00	ug/l	0.01
4) 1,4-Difluorobenzene	8.58	114	62301	5.00	ug/l	0.01
8) Chlorobenzene-d5	11.40	117	38725	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.35	152	5730	5.00	ug/l	0.00

System Monitoring Compounds

3) 1,2-Dichloroethane-d4	8.00	65	25724	4.27	ug/l	0.00
Spiked Amount	5.000	Range	81 - 118	Recovery	=	85.40%
5) Dibromofluoromethane	7.57	113	21535	5.09	ug/l	0.00
Spiked Amount	5.000	Range	80 - 119	Recovery	=	101.80%
6) Toluene-d8	10.08	98	41481	4.80	ug/l	0.00
Spiked Amount	5.000	Range	89 - 112	Recovery	=	96.00%
7) 4-Bromofluorobenzene	12.39	95	9071	4.50	ug/l	0.00
Spiked Amount	5.000	Range	85 - 114	Recovery	=	90.00%


Target Compounds					Qvalue
2) Vinyl Chloride	2.16	62	17977	4.008	ug/l 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN073019\
Data File : VN056968.D
Acq On : 30 Jul 2019 12:05
Operator : JC/SP
Sample : VN0730WBS01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0730WBS01

Quant Time: Jul 31 04:14:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Tue Jul 30 01:50:04 2019
Response via : Initial Calibration

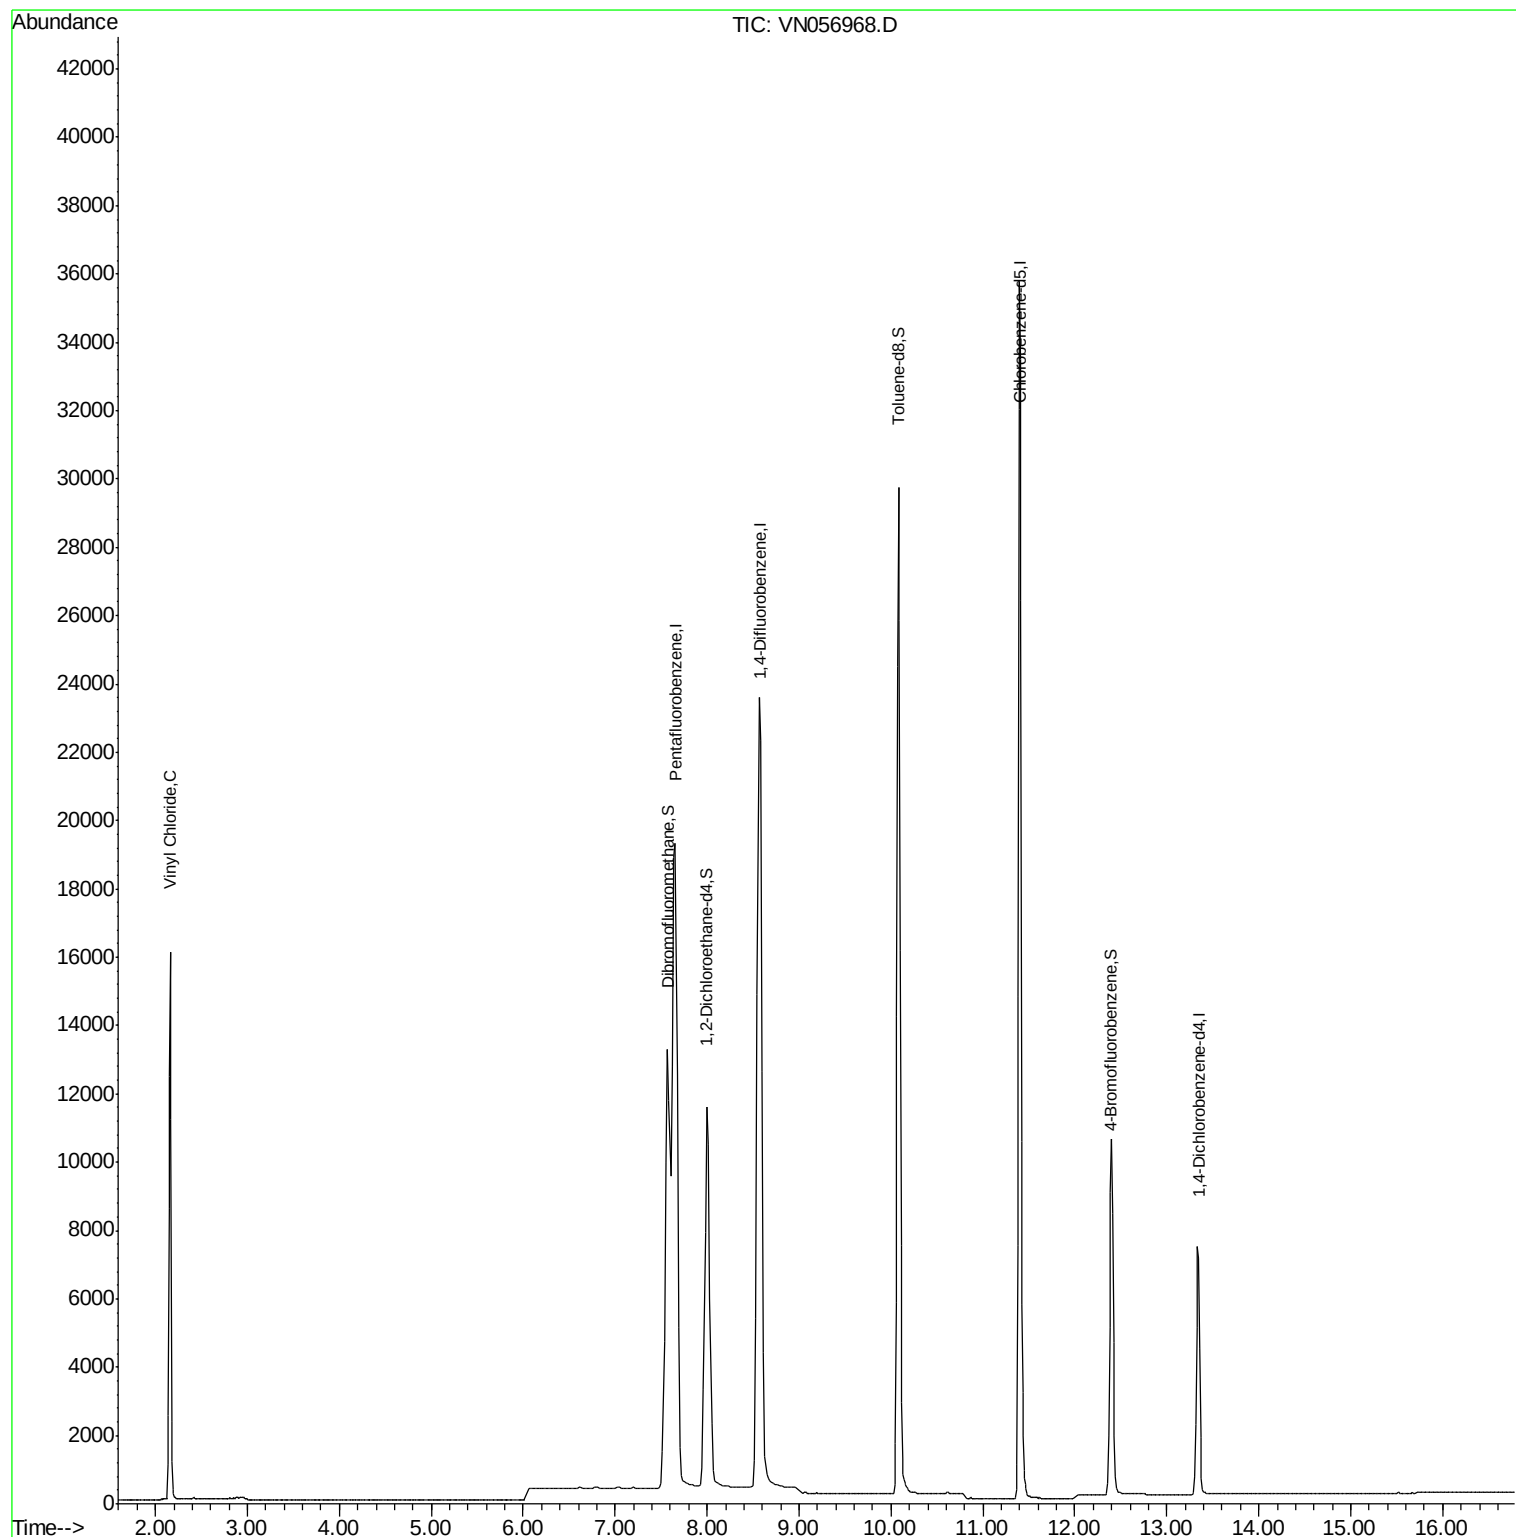

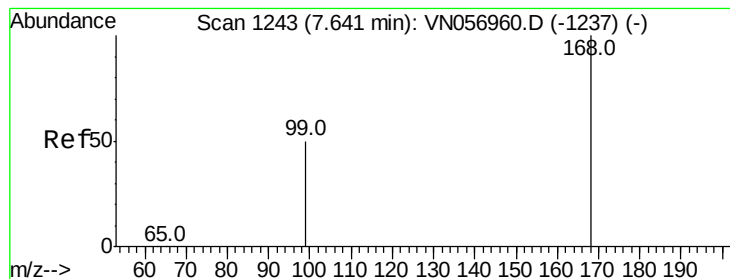

#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.65 min Scan# 1243

Delta R.T. 0.01 min

Lab File: VN056968.D

Acq: 30 Jul 2019 12:05

Instrument :

MSVOA_N

ClientSampled :


VN0730WBS01

Tot Ion:168 Resp: 48575

Ion Ratio Lower Upper




168 100

99 43.4 40.0 60.0

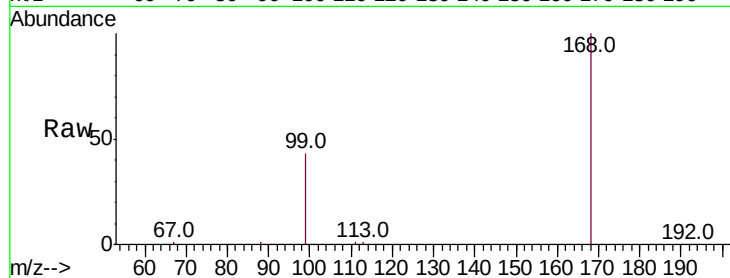

Abundance Ion 168.00 (167.70 to 168.70): V

Ion 99.00 (98.70 to 99.70): VN

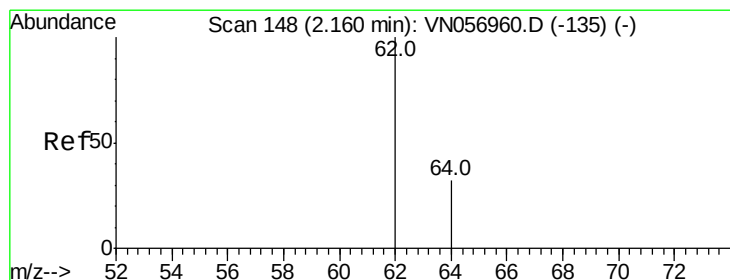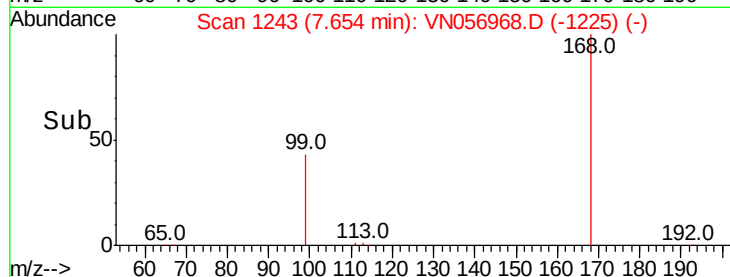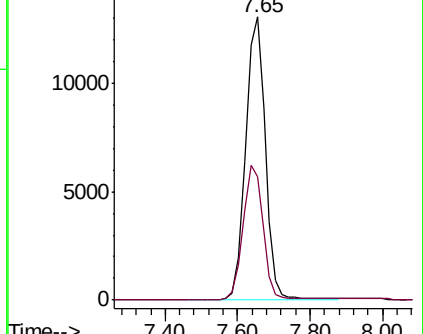

#2

Vinyl Chloride

Concen: 4.008 ug/l

RT: 2.16 min Scan# 148

Delta R.T. -0.00 min

Lab File: VN056968.D


Acq: 30 Jul 2019 12:05

Tgt Ion: 62 Resp: 17977

Ion Ratio Lower Upper



62 100


64 32.7 26.4 39.6

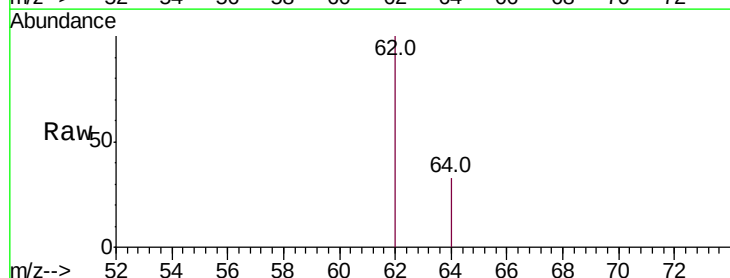

Abundance Ion 62.00 (61.70 to 62.70): VN

Ion 64.00 (63.70 to 64.70): VN

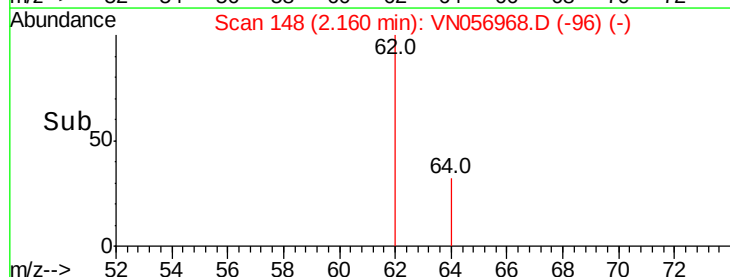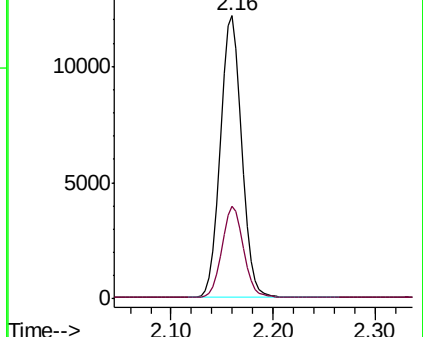

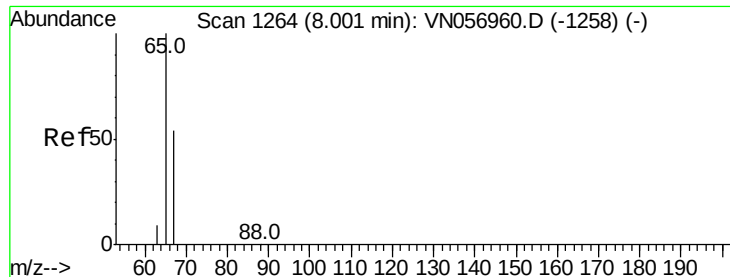

#3

1,2-Dichloroethane-d4

Concen: 4.273 ug/l

RT: 8.00 min Scan# 1263

Delta R.T. -0.00 min

Lab File: VN056968.D

Acq: 30 Jul 2019 12:05

Instrument :

MSVOA_N

ClientSampleId :


VN0730WBS01

Tot Ion: 65 Resp: 25724

Ion Ratio Lower Upper

65 100

67 53.6 0.0 109.6

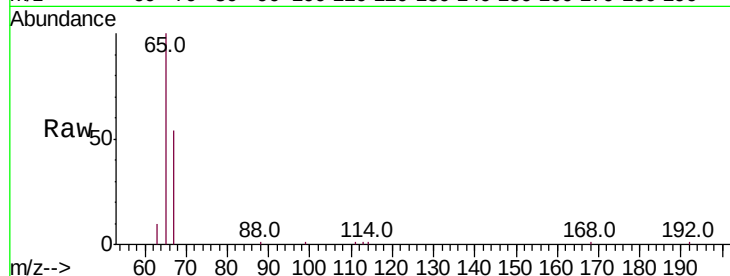

Abundance Ion 65.00 (64.70 to 65.70): VN0

Ion 67.00 (66.70 to 67.70): VN0

8.00

6000



4000

2000

0

Time-->

7.80 8.00 8.20 8.40

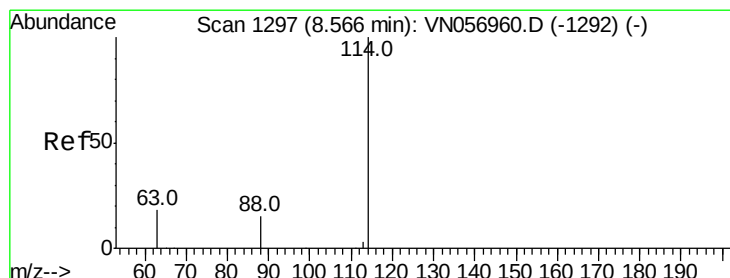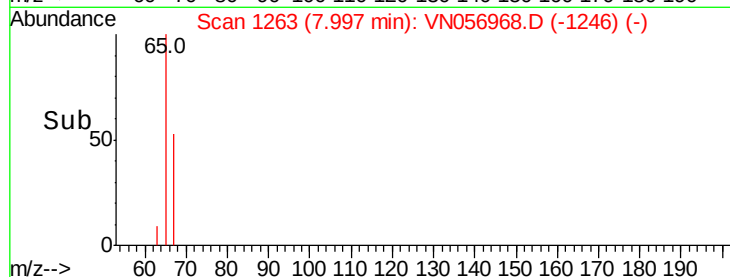

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.58 min Scan# 1297

Delta R.T. 0.01 min

Lab File: VN056968.D

Acq: 30 Jul 2019 12:05


Tgt Ion: 114 Resp: 62301

Ion Ratio Lower Upper

114 100

63 14.4 0.0 37.6

88 13.4 0.0 31.0

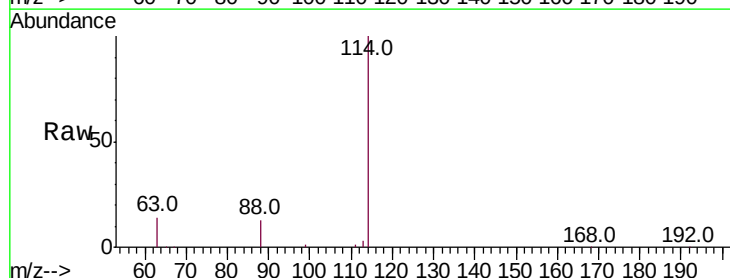

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VN0

Ion 88.00 (87.70 to 88.70): VN0

8.58

20000

15000


10000


5000

0

Time-->

8.40 8.60 8.80 9.00

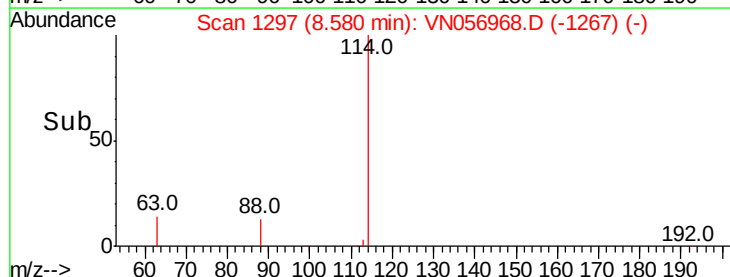

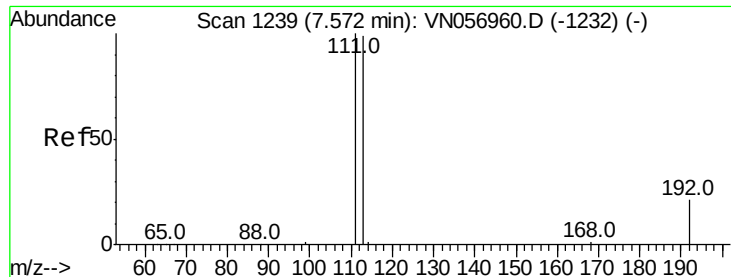

#5

Dibromofluoromethane

Concen: 5.088 ug/l

RT: 7.57 min Scan# 1238

Delta R.T. -0.00 min

Lab File: VN056968.D

Acq: 30 Jul 2019 12:05

Instrument :

MSVOA_N

ClientSampleId :

VN0730WBS01


Tot Ion:113 Resp: 21535

Ion Ratio Lower Upper

113 100

111 102.9 81.1 121.7




192 21.5 17.9 26.9

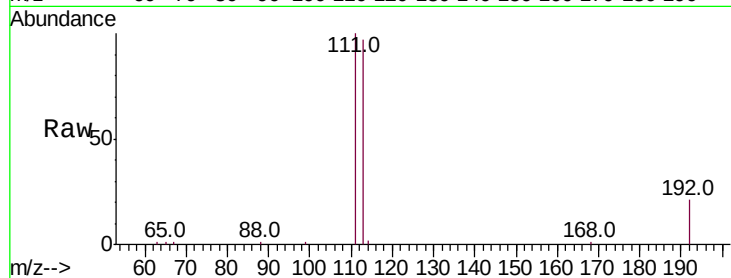

Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V

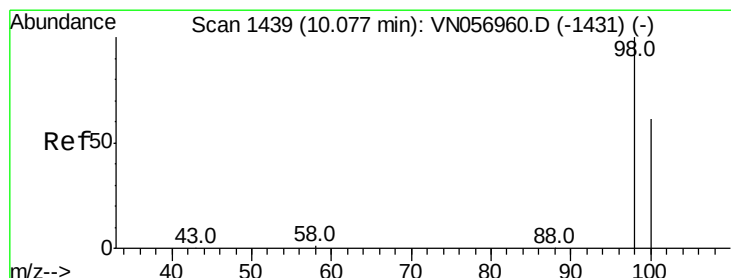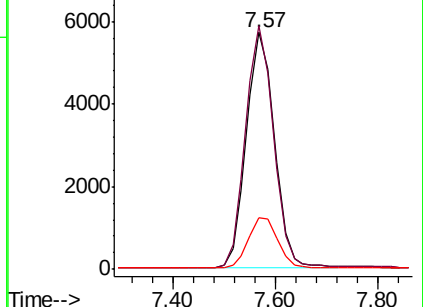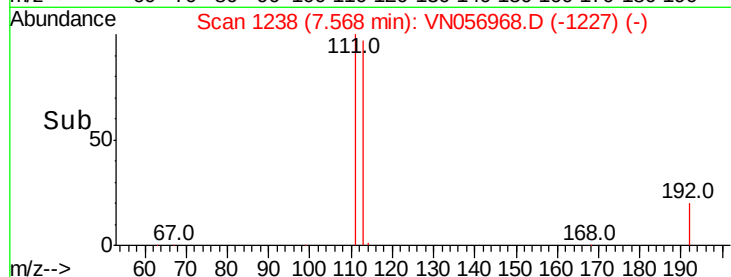

#6

Toluene-d8

Concen: 4.803 ug/l

RT: 10.08 min Scan# 1439

Delta R.T. 0.00 min

Lab File: VN056968.D


Acq: 30 Jul 2019 12:05

Tgt Ion: 98 Resp: 41481

Ion Ratio Lower Upper



98 100


100 62.5 49.0 73.4

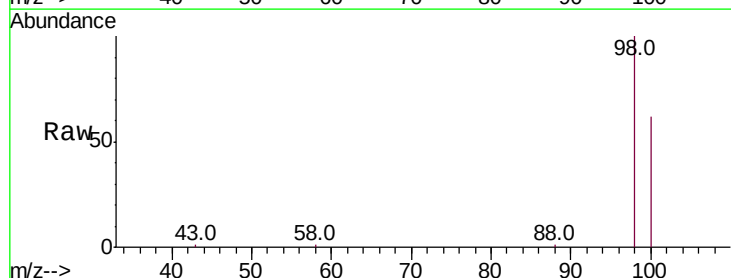

Abundance Ion 98.00 (97.70 to 98.70): VN

Ion 100.00 (99.70 to 100.70): VN

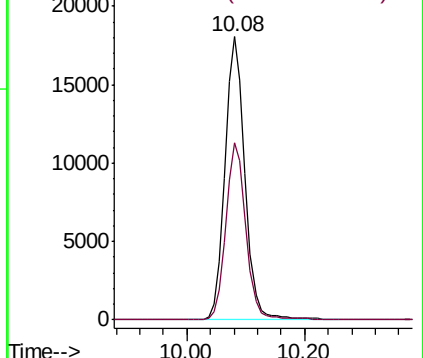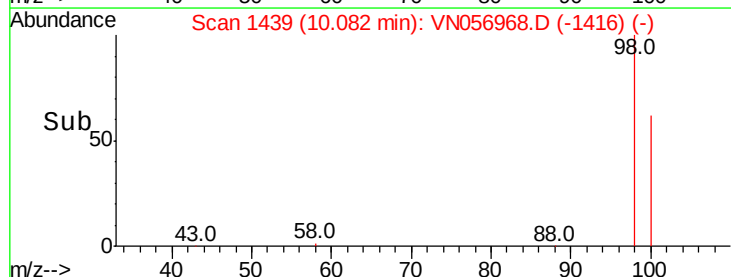

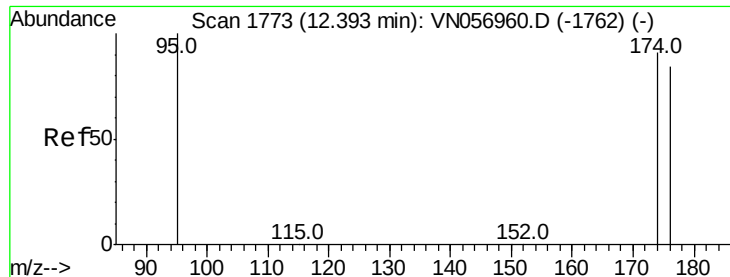

#7

4-Bromofluorobenzene

Concen: 4.500 ug/l

RT: 12.39 min Scan# 1772

Delta R.T. -0.01 min

Lab File: VN056968.D

Acq: 30 Jul 2019 12:05

Instrument :

MSVOA_N

ClientSampleId :

VN0730WBS01


Tot Ion: 95 Resp: 9071

Ion Ratio Lower Upper

95 100

174 77.8 0.0 181.4




176 69.0 0.0 168.2

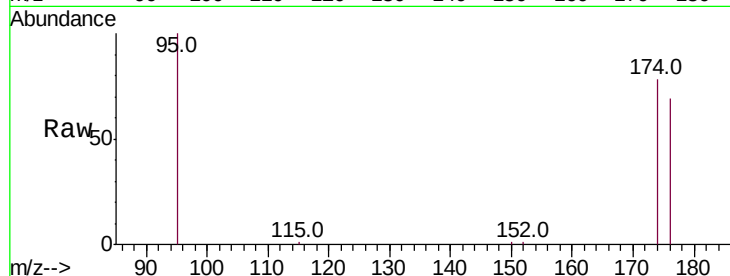

Abundance Ion 95.00 (94.70 to 95.70): VN056960.D (-1762) (-)

Ion 174.00 (173.70 to 174.70): VN056960.D (-1762) (-)

Ion 176.00 (175.70 to 176.70): VN056960.D (-1762) (-)

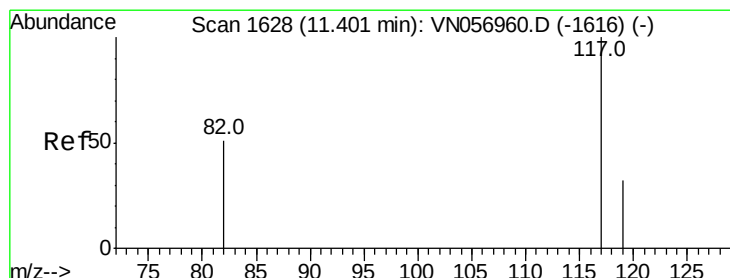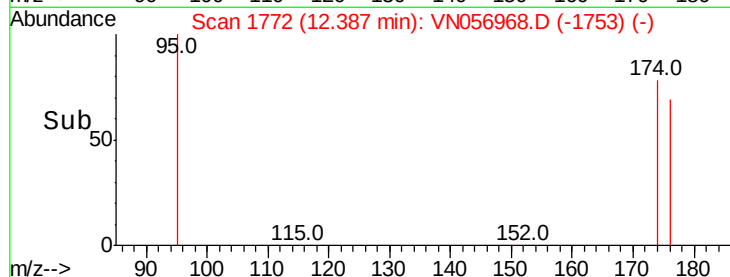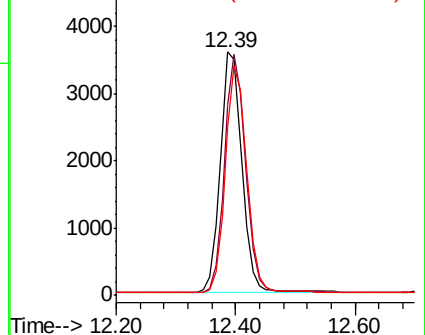

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.40 min Scan# 1627

Delta R.T. -0.00 min

Lab File: VN056968.D

Acq: 30 Jul 2019 12:05


Tgt Ion: 117 Resp: 38725

Ion Ratio Lower Upper

117 100

82 51.7 40.7 61.1



119 31.8 25.6 38.4



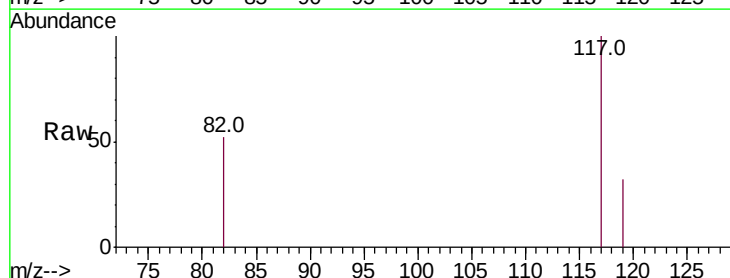


Abundance Ion 117.00 (116.70 to 117.70): VN056960.D (-1616) (-)

Ion 82.00 (81.70 to 82.70): VN056960.D (-1616) (-)

Ion 119.00 (118.70 to 119.70): VN056960.D (-1616) (-)

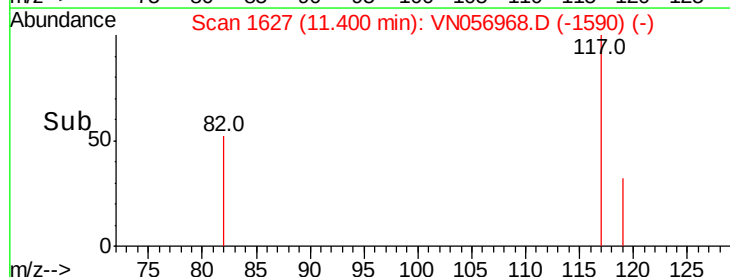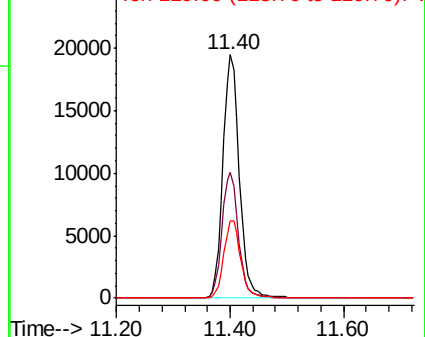

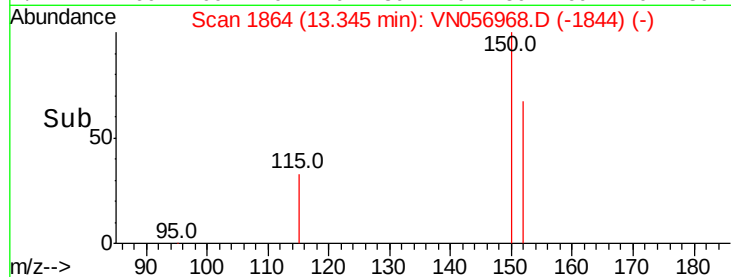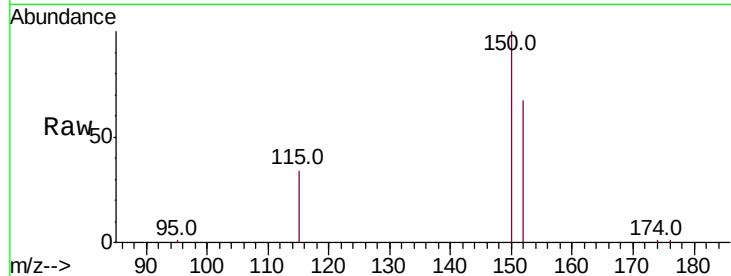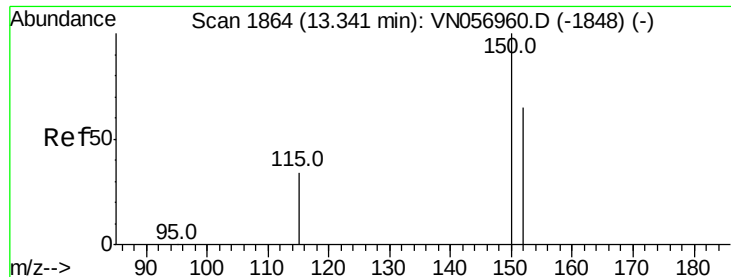

#9

1,4-Dichlorobenzene-d4

Concen: 5.000 ug/l

RT: 13.35 min Scan# 1864

Delta R.T. 0.00 min

Lab File: VN056968.D

Acq: 30 Jul 2019 12:05

Instrument :

MSVOA_N

ClientSampleId :

VN0730WBS01

Tot Ion:152 Resp: 5730

Ion Ratio Lower Upper

152 100

115 50.1 27.0 80.8

150 149.3 0.0 306.8

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

