

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN073019\
 Data File : VN056995.D
 Acq On : 31 Jul 2019 00:51
 Operator : JC/SP
 Sample : K4018-03
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SU19-MSW0413

Quant Time: Jul 31 04:17:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 30 01:50:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.65	168	34071	5.00	ug/l	0.01
4) 1,4-Difluorobenzene	8.58	114	47184	5.00	ug/l	0.01
8) Chlorobenzene-d5	11.40	117	31492	5.00	ug/l	0.00
9) 1,4-Dichlorobenzene-d4	13.35	152	4254	5.00	ug/l	0.00

System Monitoring Compounds

3) 1,2-Dichloroethane-d4	8.00	65	19799	4.69	ug/l	0.00
Spiked Amount	5.000	Range	81 - 118	Recovery	=	93.80%
5) Dibromofluoromethane	7.57	113	16751	5.23	ug/l	0.00
Spiked Amount	5.000	Range	80 - 119	Recovery	=	104.60%
6) Toluene-d8	10.08	98	32195	4.92	ug/l	0.00
Spiked Amount	5.000	Range	89 - 112	Recovery	=	98.40%
7) 4-Bromofluorobenzene	12.40	95	7007	4.59	ug/l	0.00
Spiked Amount	5.000	Range	85 - 114	Recovery	=	91.80%


Target Compounds					Qvalue
2) Vinyl Chloride	2.16	62	250	0.079 ug/l #	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN073019\
Data File : VN056995.D
Acq On : 31 Jul 2019 00:51
Operator : JC/SP
Sample : K4018-03
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SU19-MSW0413

Quant Time: Jul 31 04:17:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
Quant Title : SW846 8260
QLast Update : Tue Jul 30 01:50:04 2019
Response via : Initial Calibration

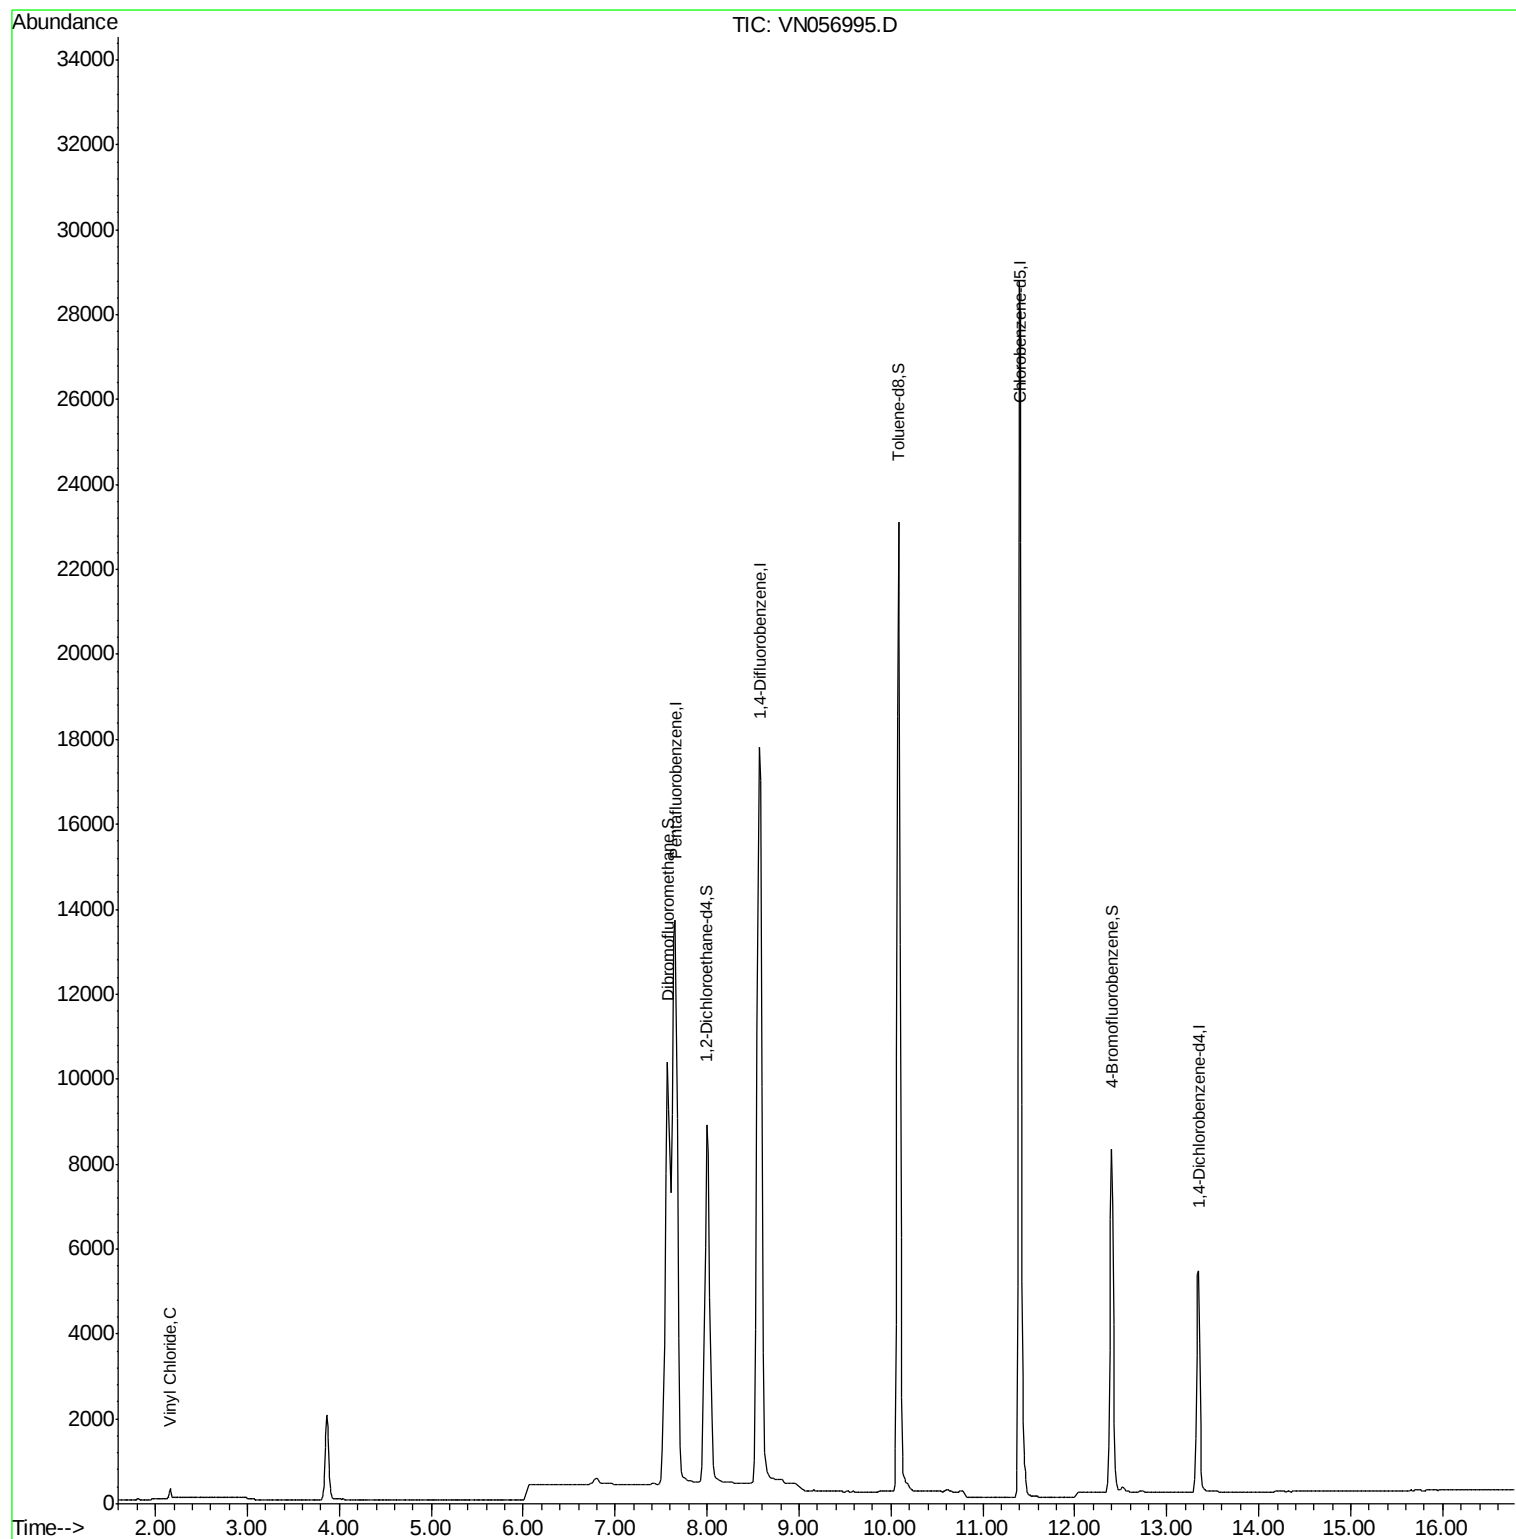

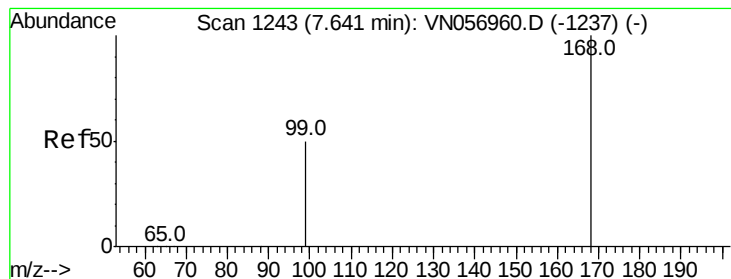

#1

Pentafluorobenzene

Concen: 5.000 ug/l

RT: 7.65 min Scan# 1243

Delta R.T. 0.01 min

Lab File: VN056995.D

Acq: 31 Jul 2019 00:51

Instrument :

MSVOA_N

ClientSampleId :


SU19-MSW0413

Tot Ion:168 Resp: 34071

Ion Ratio Lower Upper

168 100

99 43.4 40.0 60.0

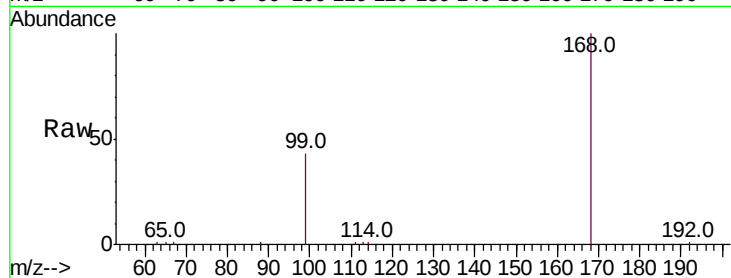

Abundance Ion 168.00 (167.70 to 168.70): VN056960.D (-1237) (-)

Ion 99.00 (98.70 to 99.70): VN056960.D (-1237) (-)

7.65

10000

8000



6000

4000

2000

0

Time-->

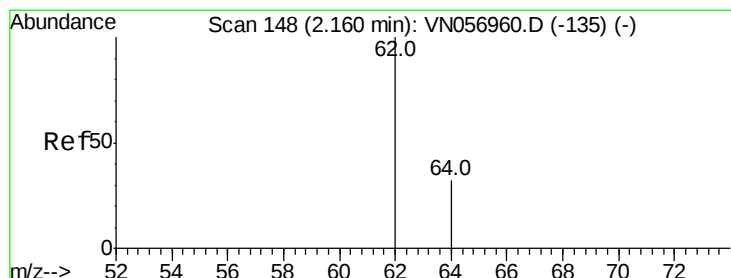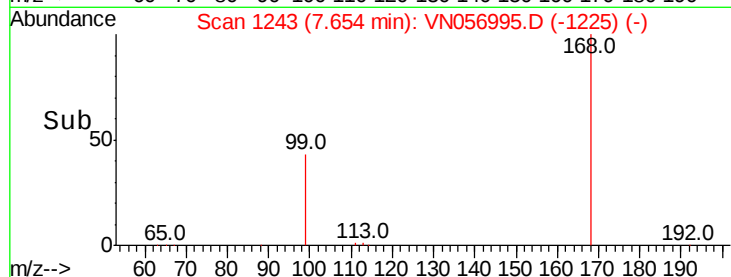

#2

Vinyl Chloride

Concen: 0.079 ug/l

RT: 2.16 min Scan# 148

Delta R.T. -0.00 min

Lab File: VN056995.D


Acq: 31 Jul 2019 00:51

Tgt Ion: 62 Resp: 250

Ion Ratio Lower Upper

62 100

64 56.8 26.4 39.6#

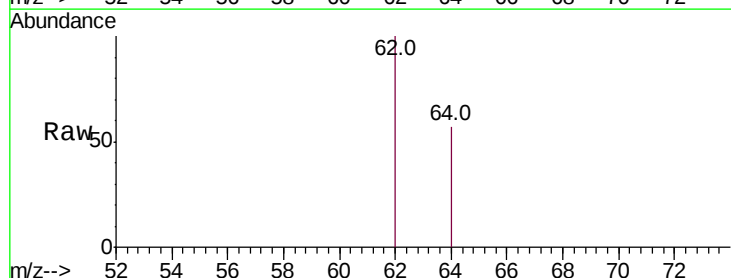

Abundance Ion 62.00 (61.70 to 62.70): VN056960.D (-135) (-)

Ion 64.00 (63.70 to 64.70): VN056960.D (-135) (-)

2.16

250

200


150


100

50

0

Time-->

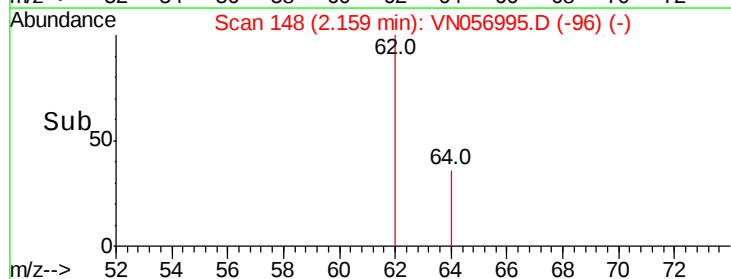

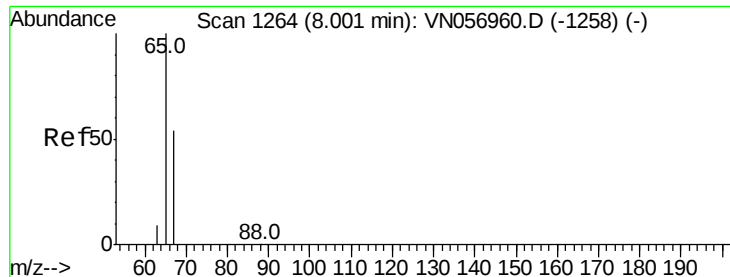

#3

1,2-Dichloroethane-d4

Concen: 4.689 ug/l

RT: 8.00 min Scan# 1263

Delta R.T. -0.00 min

Lab File: VN056995.D

Acq: 31 Jul 2019 00:51

Instrument :

MSVOA_N

ClientSampleId :


SU19-MSW0413

Tot Ion: 65 Resp: 19799




Ion Ratio Lower Upper

65 100

67 53.4 0.0 109.6

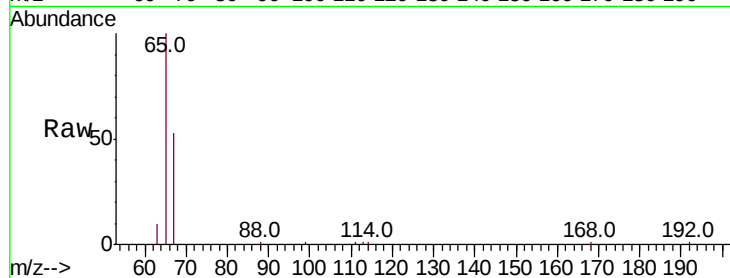

Abundance Ion 65.00 (64.70 to 65.70): VN056995.D (-1263) (-)

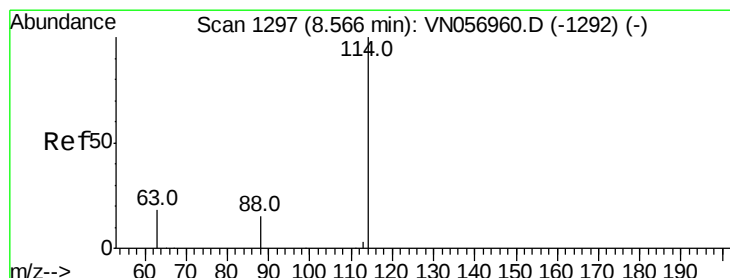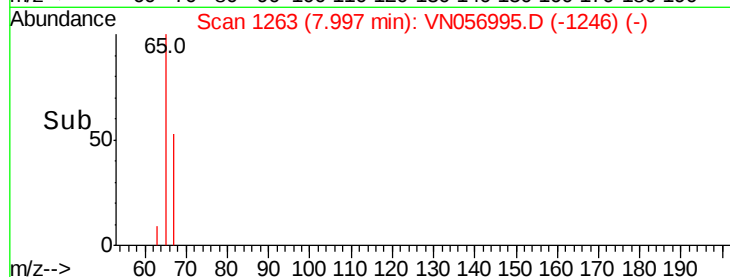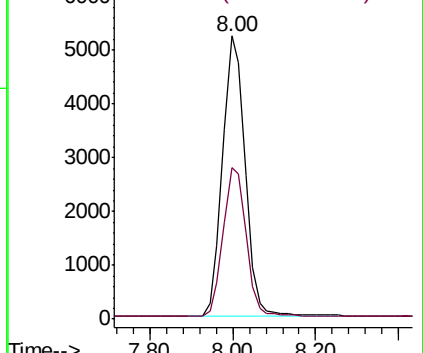

#4

1,4-Difluorobenzene

Concen: 5.000 ug/l

RT: 8.58 min Scan# 1297

Delta R.T. 0.01 min

Lab File: VN056995.D

Acq: 31 Jul 2019 00:51


Tgt Ion: 114 Resp: 47184

Ion Ratio Lower Upper



114 100


63 14.6 0.0 37.6

88 13.6 0.0 31.0

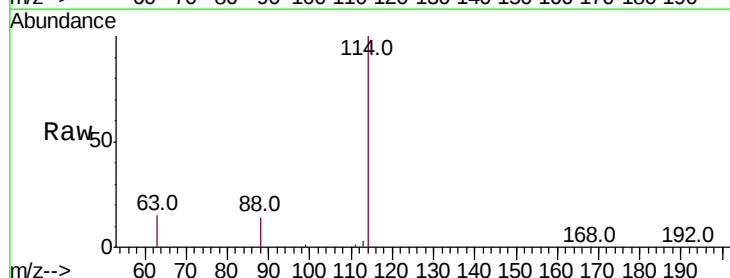

Abundance Ion 114.00 (113.70 to 114.70): VN056995.D (-1297) (-)

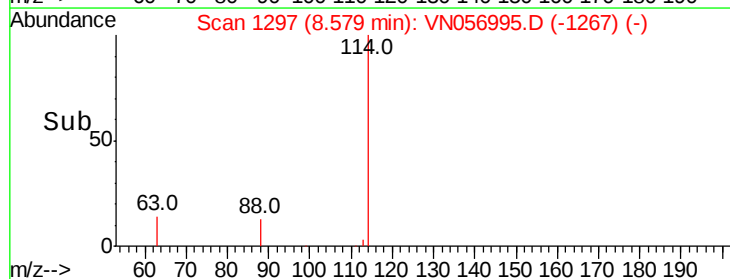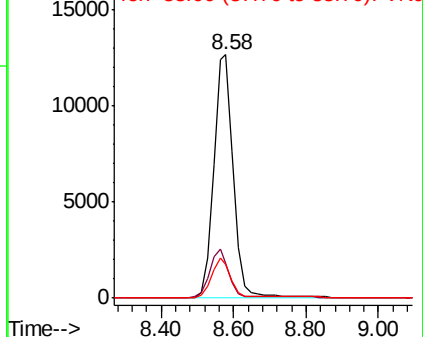

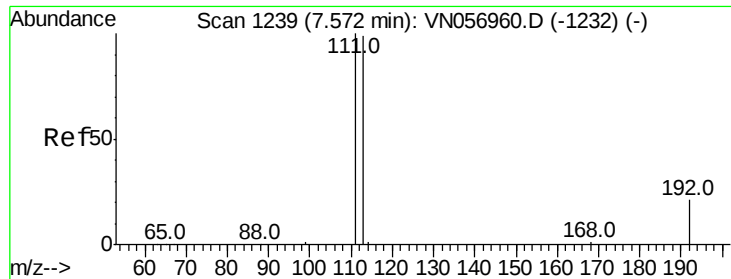

#5

Dibromofluoromethane

Concen: 5.226 ug/l

RT: 7.57 min Scan# 1238

Delta R.T. -0.00 min

Lab File: VN056995.D

Acq: 31 Jul 2019 00:51

Instrument :

MSVOA_N

ClientSampleId :

SU19-MSW0413


Tot Ion:113 Resp: 16751

Ion Ratio Lower Upper

113 100

111 103.0 81.1 121.7




192 21.9 17.9 26.9

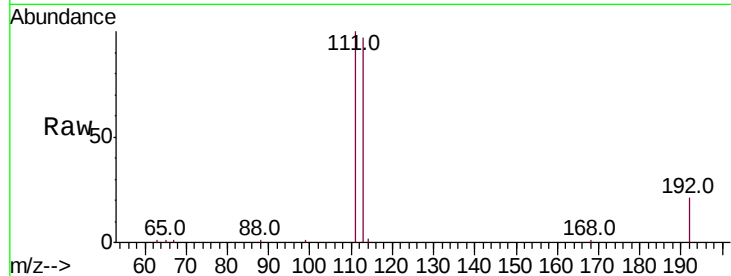

Abundance Ion 113.00 (112.70 to 113.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 192.00 (191.70 to 192.70): V

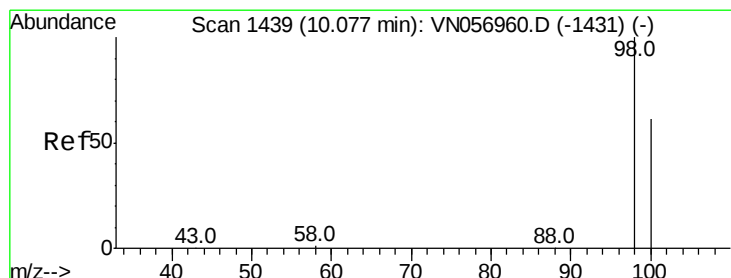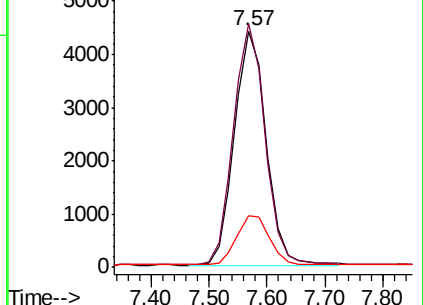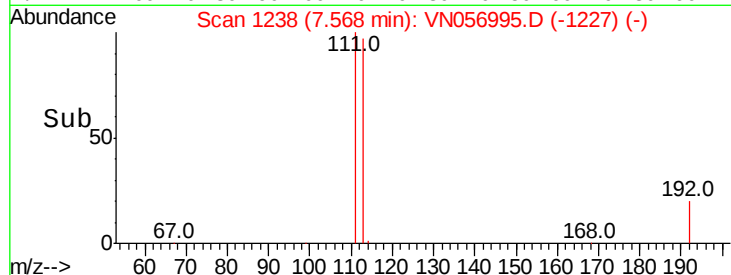

#6

Toluene-d8

Concen: 4.922 ug/l

RT: 10.08 min Scan# 1439

Delta R.T. 0.00 min

Lab File: VN056995.D


Acq: 31 Jul 2019 00:51

Tgt Ion: 98 Resp: 32195

Ion Ratio Lower Upper



98 100


100 62.2 49.0 73.4

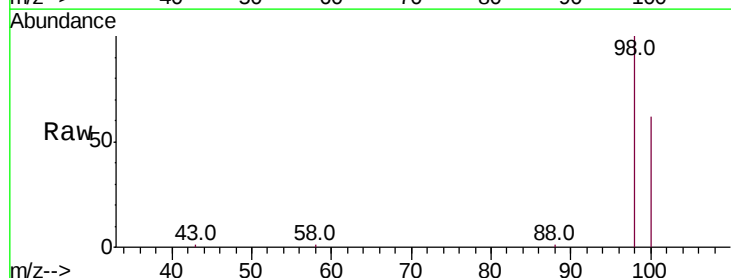

Abundance Ion 98.00 (97.70 to 98.70): VN

Ion 100.00 (99.70 to 100.70): VN

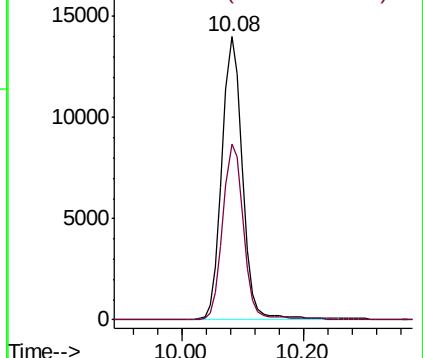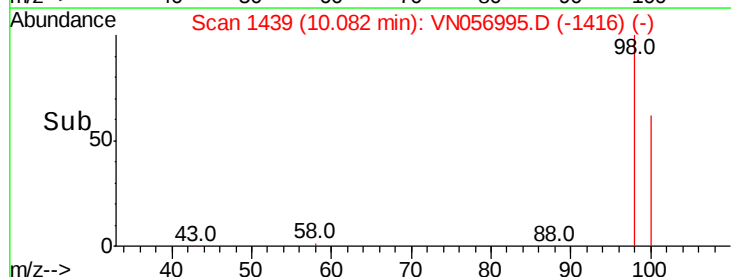

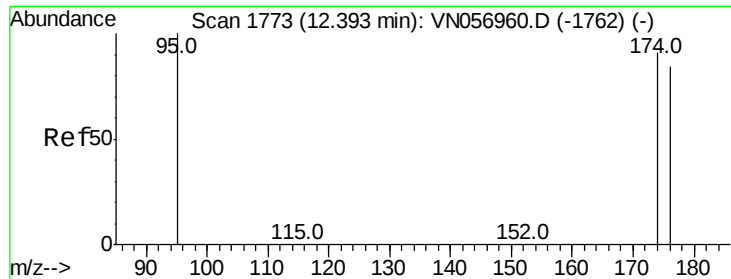

#7

4-Bromofluorobenzene

Concen: 4.589 ug/l

RT: 12.40 min Scan# 1773

Delta R.T. 0.00 min

Lab File: VN056995.D

Acq: 31 Jul 2019 00:51

Instrument :

MSVOA_N

ClientSampleId :

SU19-MSW0413


Tot Ion: 95 Resp: 7007

Ion Ratio Lower Upper

95 100

174 99.6 0.0 181.4




176 94.2 0.0 168.2

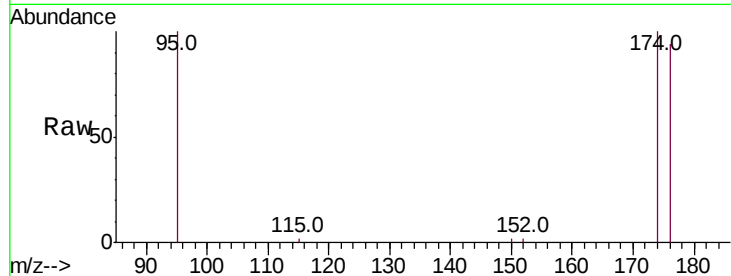

Abundance Ion 95.00 (94.70 to 95.70): VN056995.D (-1753) (-)

Ion 174.00 (173.70 to 174.70): VN056995.D (-1753) (-)

Ion 176.00 (175.70 to 176.70): VN056995.D (-1753) (-)

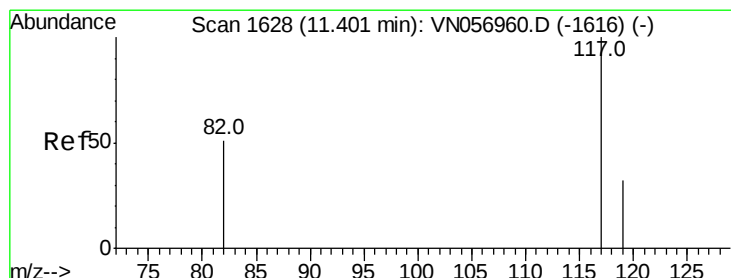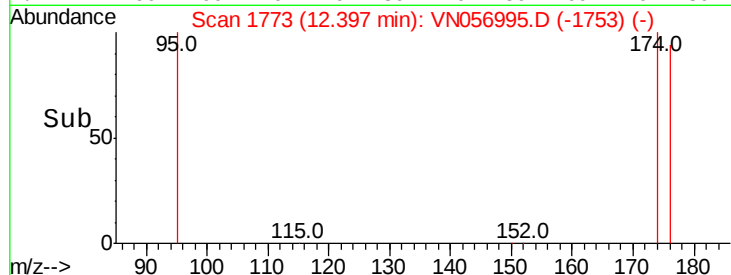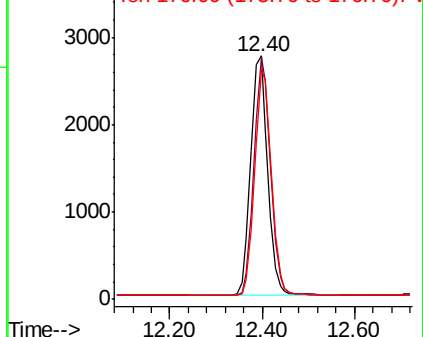

#8

Chlorobenzene-d5

Concen: 5.000 ug/l

RT: 11.40 min Scan# 1627

Delta R.T. -0.00 min

Lab File: VN056995.D

Acq: 31 Jul 2019 00:51


Tgt Ion: 117 Resp: 31492

Ion Ratio Lower Upper

117 100

82 51.8 40.7 61.1



119 31.4 25.6 38.4

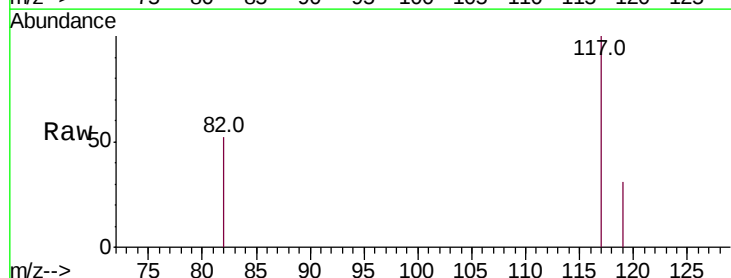


Abundance Ion 117.00 (116.70 to 117.70): VN056995.D (-1590) (-)

Ion 82.00 (81.70 to 82.70): VN056995.D (-1590) (-)

Ion 119.00 (118.70 to 119.70): VN056995.D (-1590) (-)

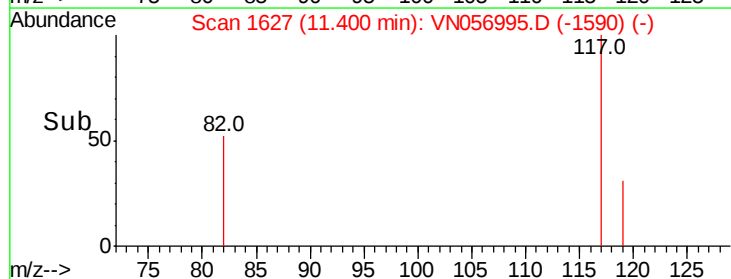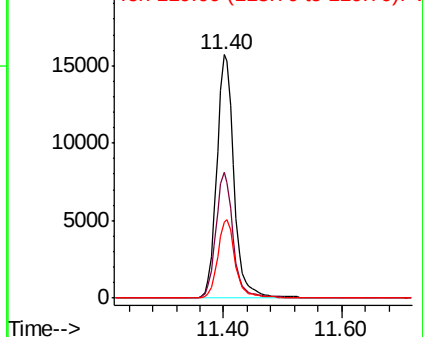

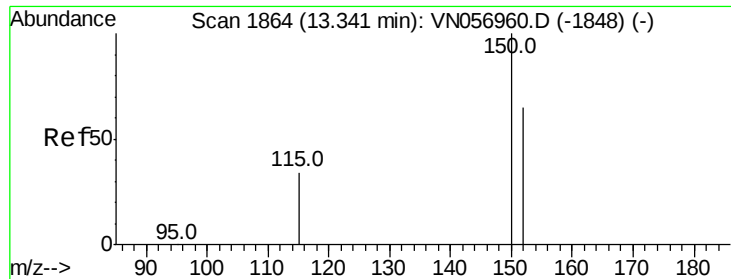

#9

1,4-Dichlorobenzene-d4

Concen: 5.000 ug/l

RT: 13.35 min Scan# 1864

Delta R.T. 0.00 min

Lab File: VN056995.D


Acq: 31 Jul 2019 00:51

Instrument :

MSVOA_N

ClientSampleId :

SU19-MSW0413

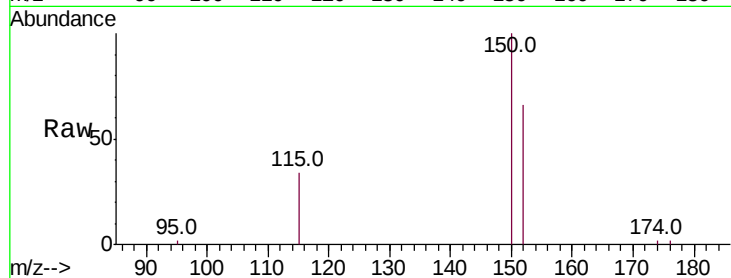

Tot Ion:152 Resp: 4254

Ion Ratio Lower Upper

152 100

115 51.0 27.0 80.8

150 150.8 0.0 306.8

Abundance Ion 152.00 (151.70 to 152.70): V

Ion 115.00 (114.70 to 115.70): V

Ion 150.00 (149.70 to 150.70): V

