


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN073019\
Data File : VN056990.D
Acq On : 30 Jul 2019 21:22
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072919SIM-VINYL.M
Title : SW846 8260
Last Update : Tue Jul 30 01:50:04 2019

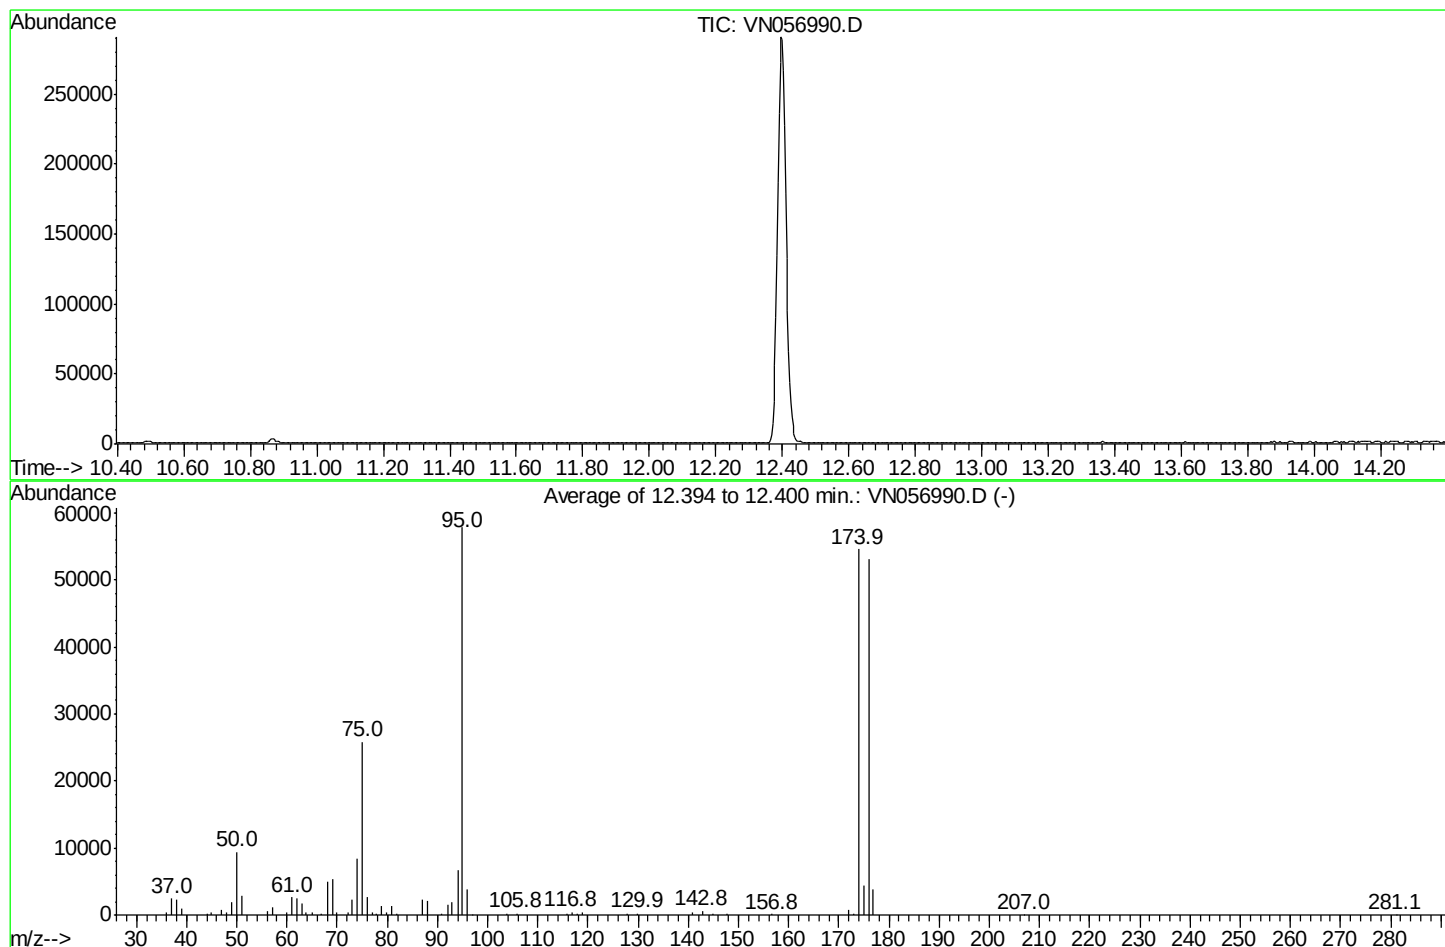

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	9403	PASS
75	95	30	60	44.7	25861	PASS
95	95	100	100	100.0	57845	PASS
96	95	5	9	6.7	3871	PASS
173	174	0.00	2	0.4	230	PASS
174	95	50	100	94.4	54616	PASS
175	174	5	9	7.9	4325	PASS
176	174	95	101	97.4	53178	PASS
177	176	5	9	7.0	3742	PASS