

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN073024\
 Data File : VN083082.D
 Acq On : 30 Jul 2024 21:06
 Operator : JC\MD
 Sample : PB162353ZHE#17
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB162353ZHE#17

Quant Time: Jul 31 06:09:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 08 13:46:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	127573	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	259134	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	270550	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	103765	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	131141	73.332	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 146.660%#	
35) Dibromofluoromethane	8.171	113	106184	63.859	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 127.720%#	
50) Toluene-d8	10.571	98	345183	56.205	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 112.400%	
62) 4-Bromofluorobenzene	12.853	95	100131	45.389	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	= 90.780%	
Target Compounds						
						Qvalue
20) Methylene Chloride	5.289	84	8354	5.494	ug/l #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN073024\
Data File : VN083082.D
Acq On : 30 Jul 2024 21:06
Operator : JC\MD
Sample : PB162353ZHE#17
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB162353ZHE#17

Quant Time: Jul 31 06:09:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 08 13:46:04 2024
Response via : Initial Calibration




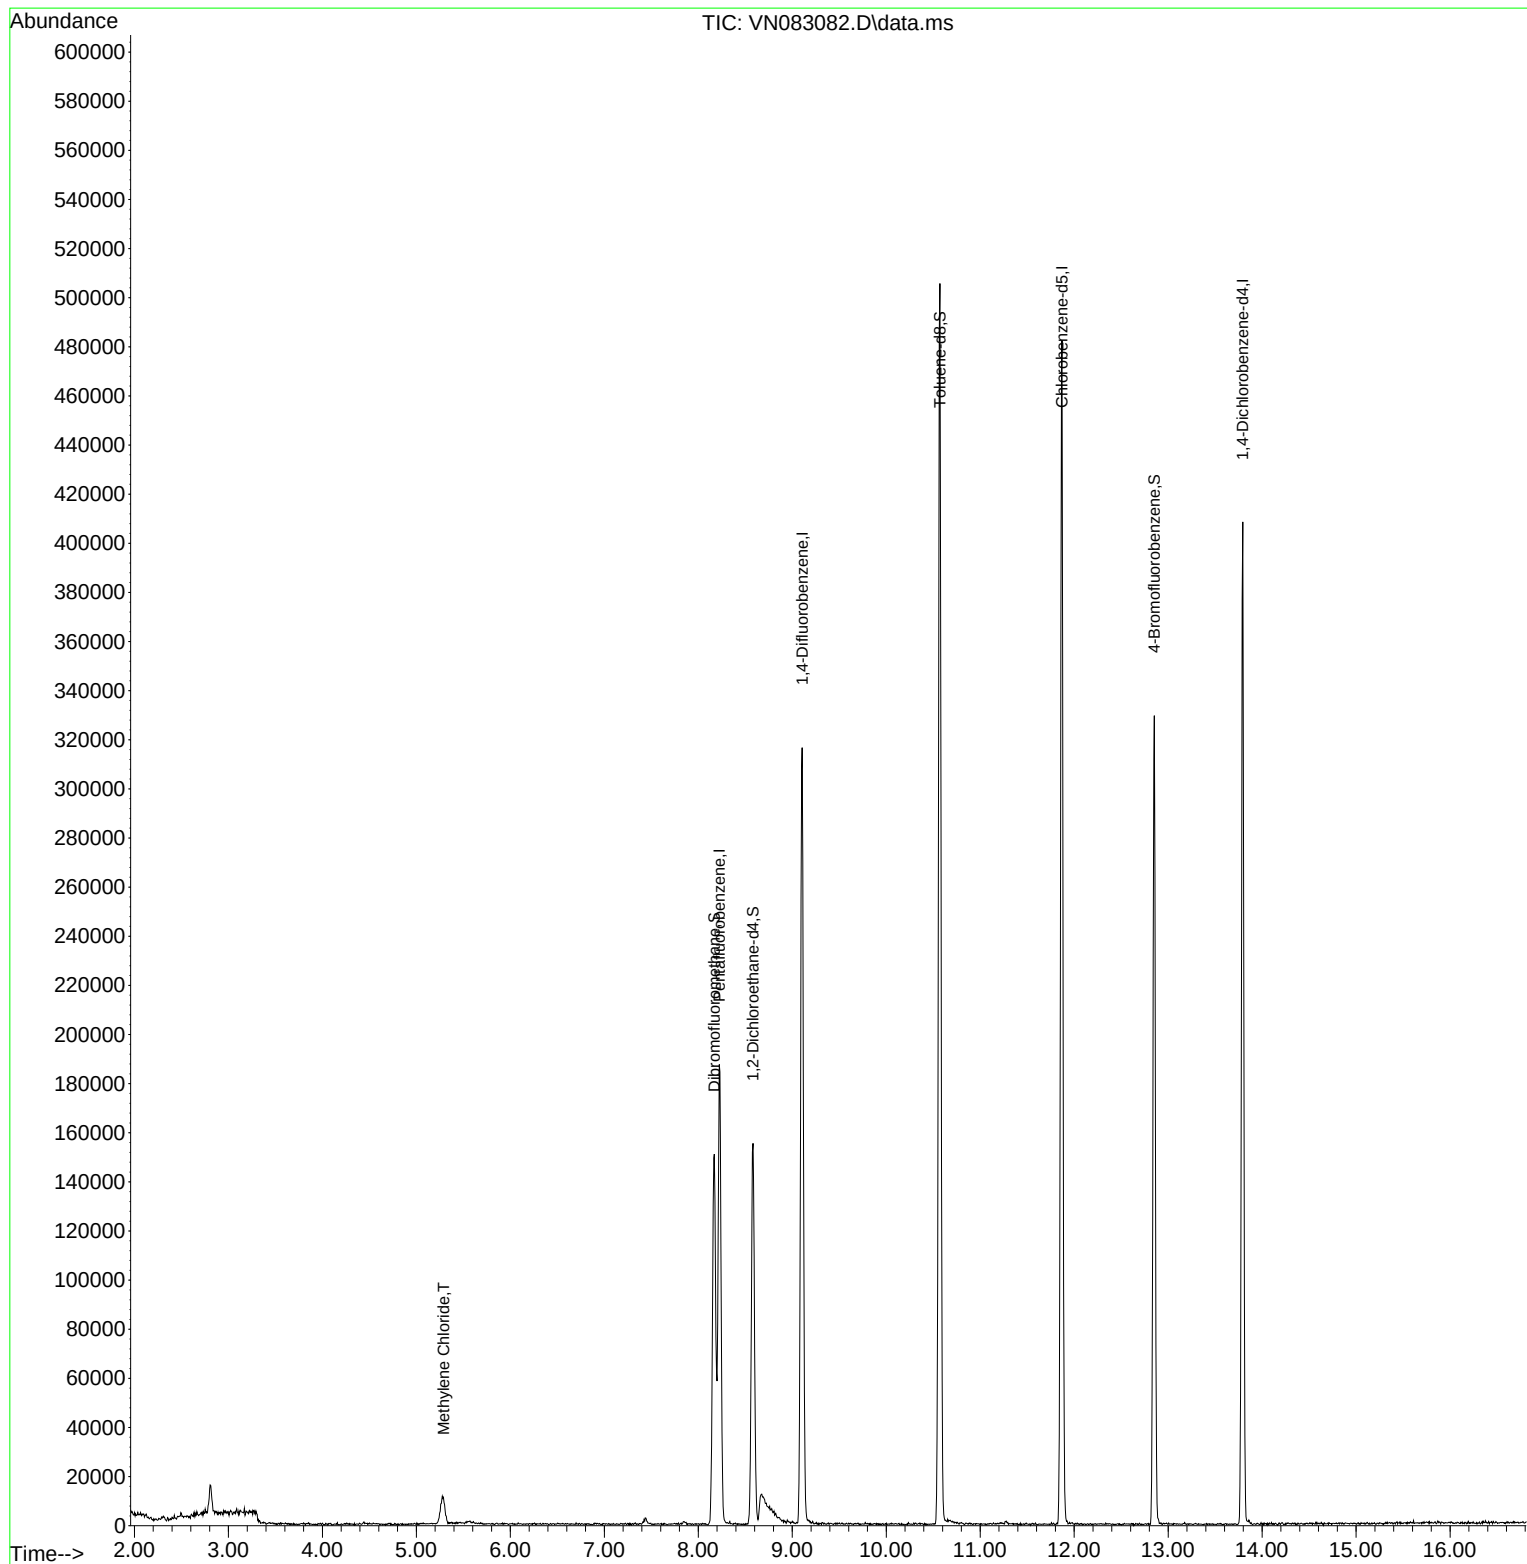


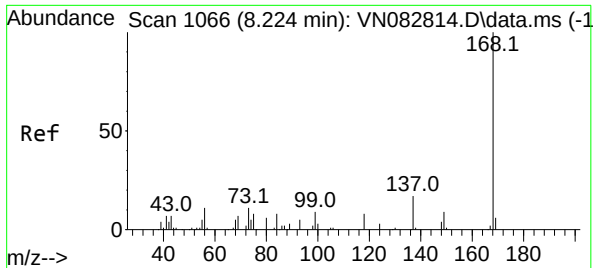

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.005 min
Lab File: VN083082.D
Acq: 30 Jul 2024 21:06




Instrument :
MSVOA_N
ClientSampleId :
PB162353ZHE#17


Tgt Ion:168 Resp: 127573
Ion Ratio Lower Upper
168 100
99 59.9 48.2 72.4

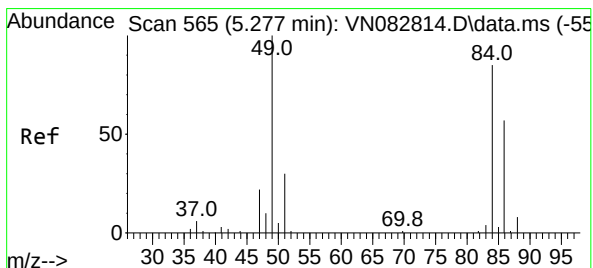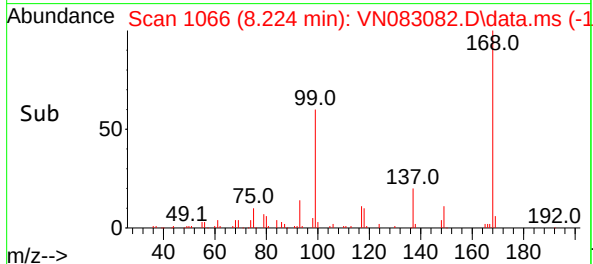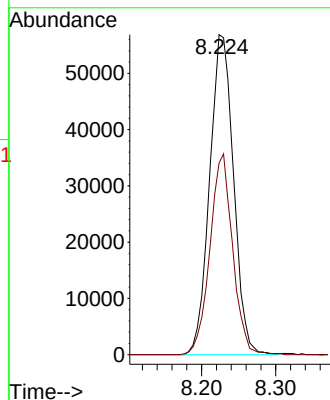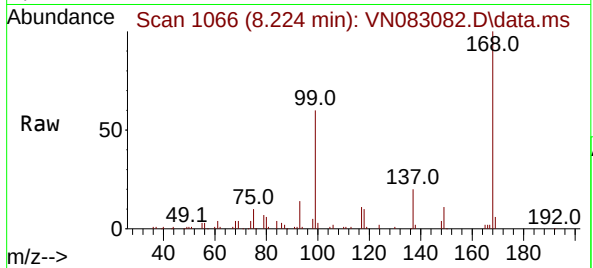

#20
Methylene Chloride
Concen: 5.494 ug/l
RT: 5.289 min Scan# 567
Delta R.T. 0.012 min
Lab File: VN083082.D
Acq: 30 Jul 2024 21:06

Tgt Ion: 84 Resp: 8354
Ion Ratio Lower Upper
84 100
49 93.7 119.6 179.4#
51 54.1 34.8 52.2#
86 71.6 52.9 79.3

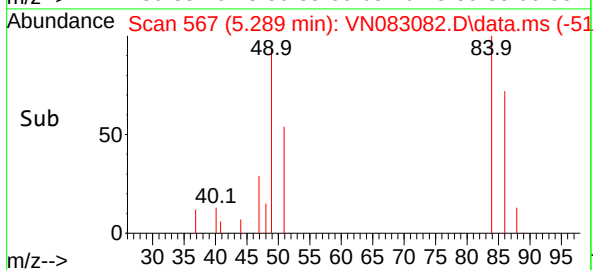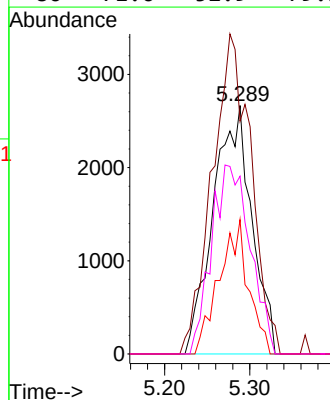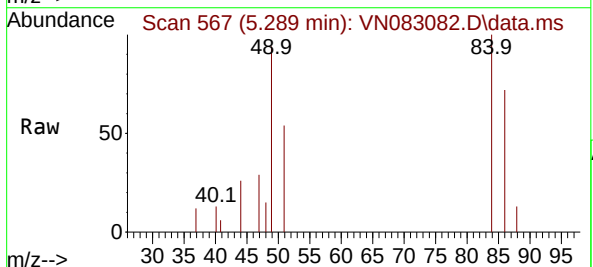

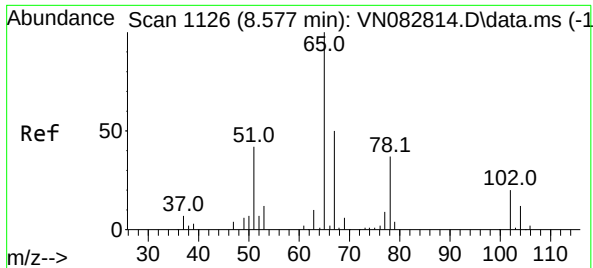

#33

1,2-Dichloroethane-d4

Concen: 73.332 ug/l

RT: 8.582 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VN083082.D

Acq: 30 Jul 2024 21:06

Instrument :

MSVOA_N

ClientSampleId :





PB162353ZHE#17

Tgt Ion: 65 Resp: 131141

Ion Ratio Lower Upper

65 100

67 50.1 0.0 104.4

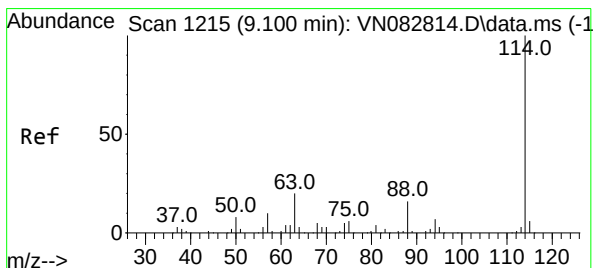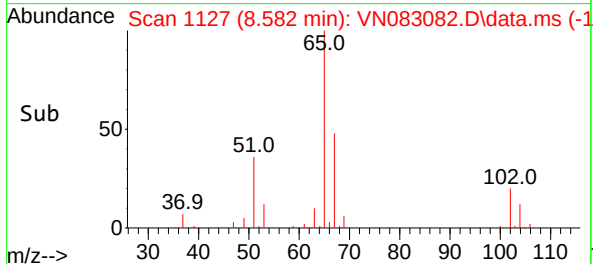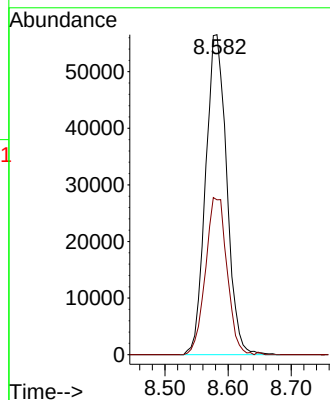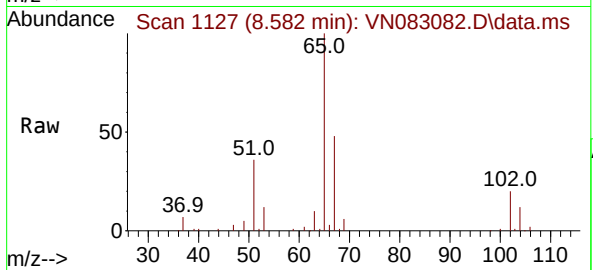

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.000 min

Lab File: VN083082.D

Acq: 30 Jul 2024 21:06




Tgt Ion: 114 Resp: 259134


Ion Ratio Lower Upper

114 100

63 18.2 0.0 44.6

88 15.3 0.0 31.4


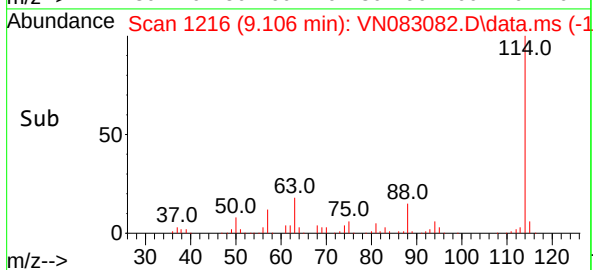
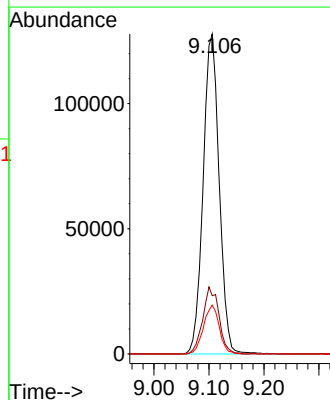
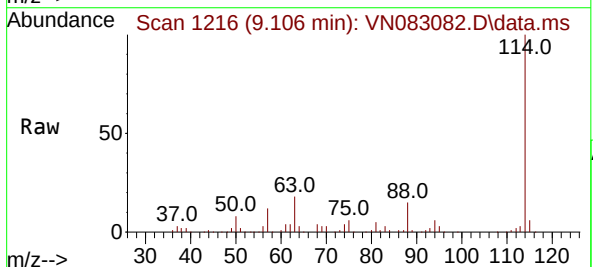


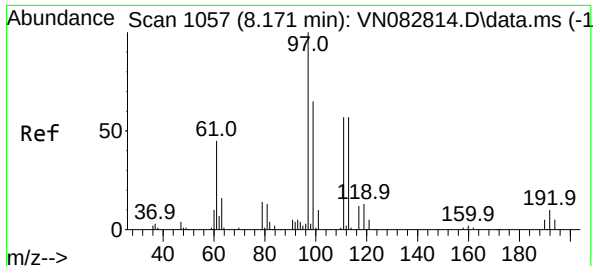

#35
Dibromofluoromethane
Concen: 63.859 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. 0.006 min
Lab File: VN083082.D
Acq: 30 Jul 2024 21:06




Instrument :
MSVOA_N
ClientSampleId :
PB162353ZHE#17


Tgt Ion:113 Resp: 106184
Ion Ratio Lower Upper
113 100
111 102.6 82.4 123.6
192 18.0 14.9 22.3

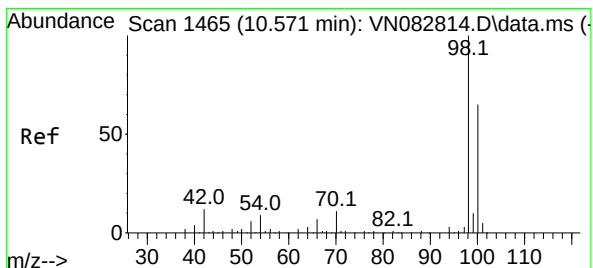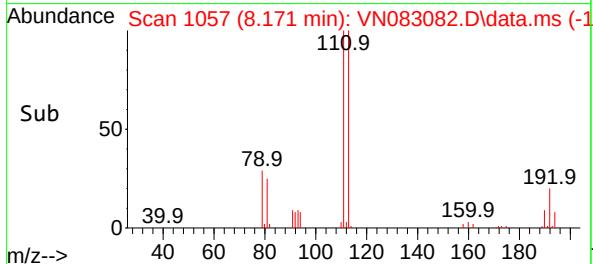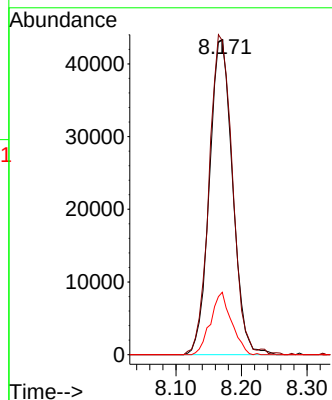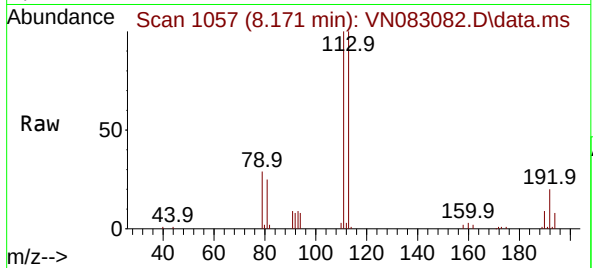

#50
Toluene-d8
Concen: 56.205 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.001 min
Lab File: VN083082.D
Acq: 30 Jul 2024 21:06

Tgt Ion: 98 Resp: 345183
Ion Ratio Lower Upper
98 100
100 63.3 51.5 77.3


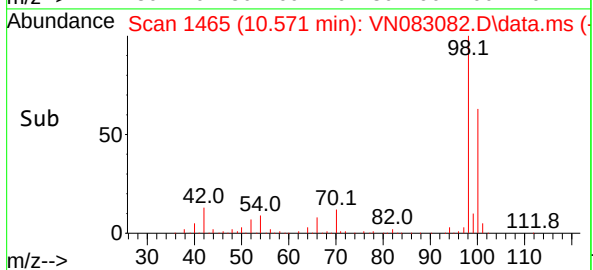
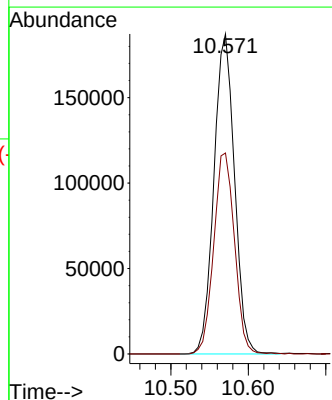
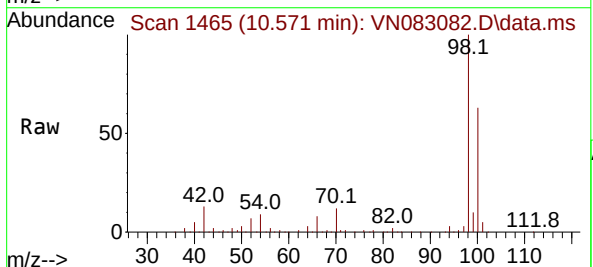


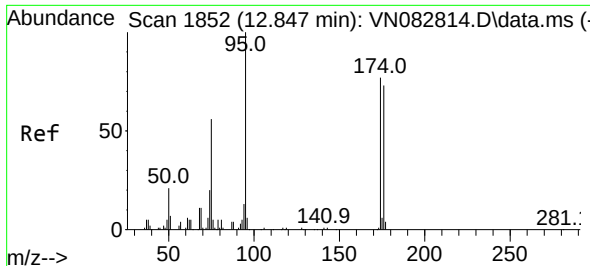

#62
4-Bromofluorobenzene
Concen: 45.389 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN083082.D
Acq: 30 Jul 2024 21:06




Instrument :
MSVOA_N
ClientSampleId :
PB162353ZHE#17


Tgt Ion: 95 Resp: 100131
Ion Ratio Lower Upper
95 100
174 84.5 0.0 159.2
176 80.3 0.0 147.6

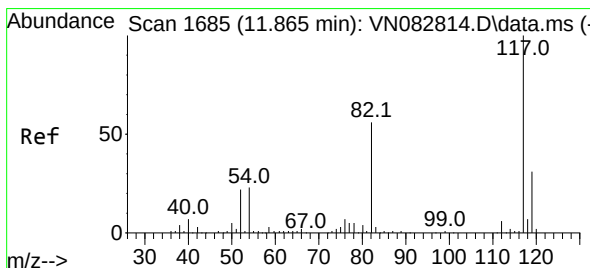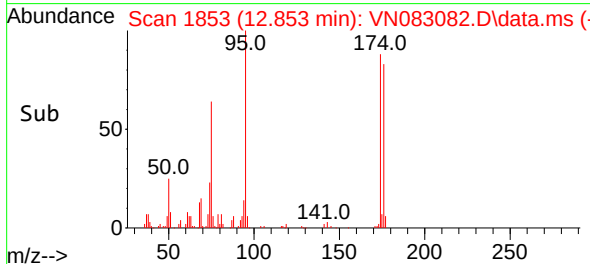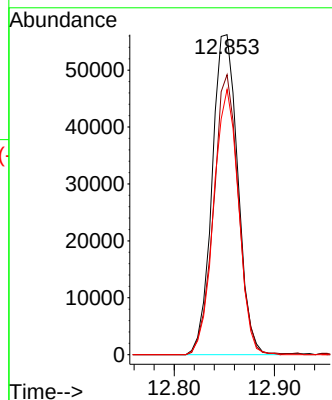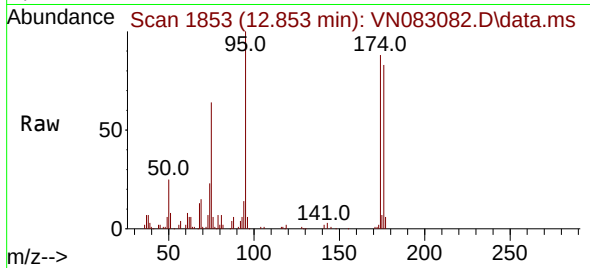

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1686
Delta R.T. 0.000 min
Lab File: VN083082.D
Acq: 30 Jul 2024 21:06


Tgt Ion: 117 Resp: 270550
Ion Ratio Lower Upper
117 100
82 54.4 47.5 71.3
119 29.6 25.6 38.4

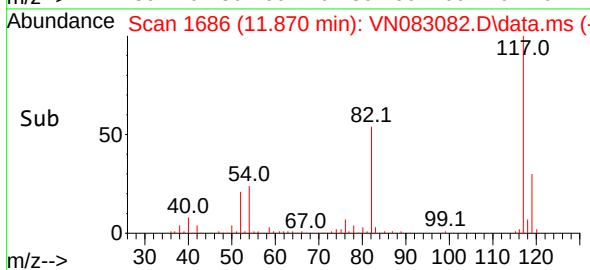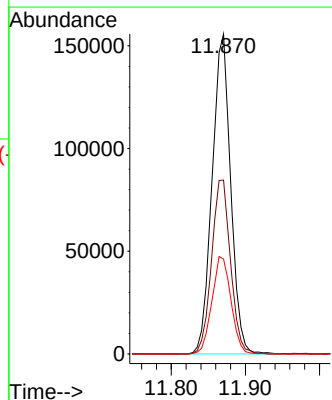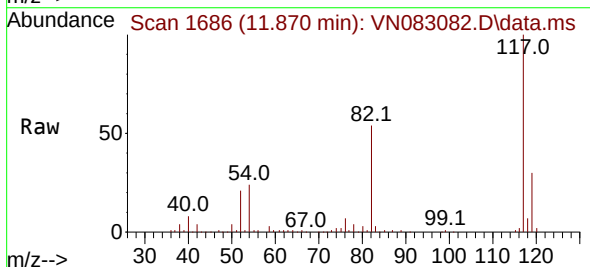

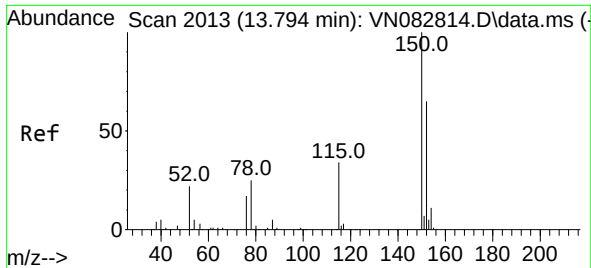

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN083082.D
 Acq: 30 Jul 2024 21:06

Instrument :
 MSVOA_N
 ClientSampleId :
 PB162353ZHE#17

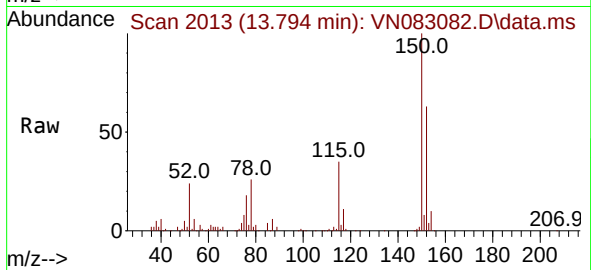

Tgt Ion:152 Resp: 103765
 Ion Ratio Lower Upper
 152 100
 115 59.9 30.6 91.6
 150 159.0 0.0 348.6

