
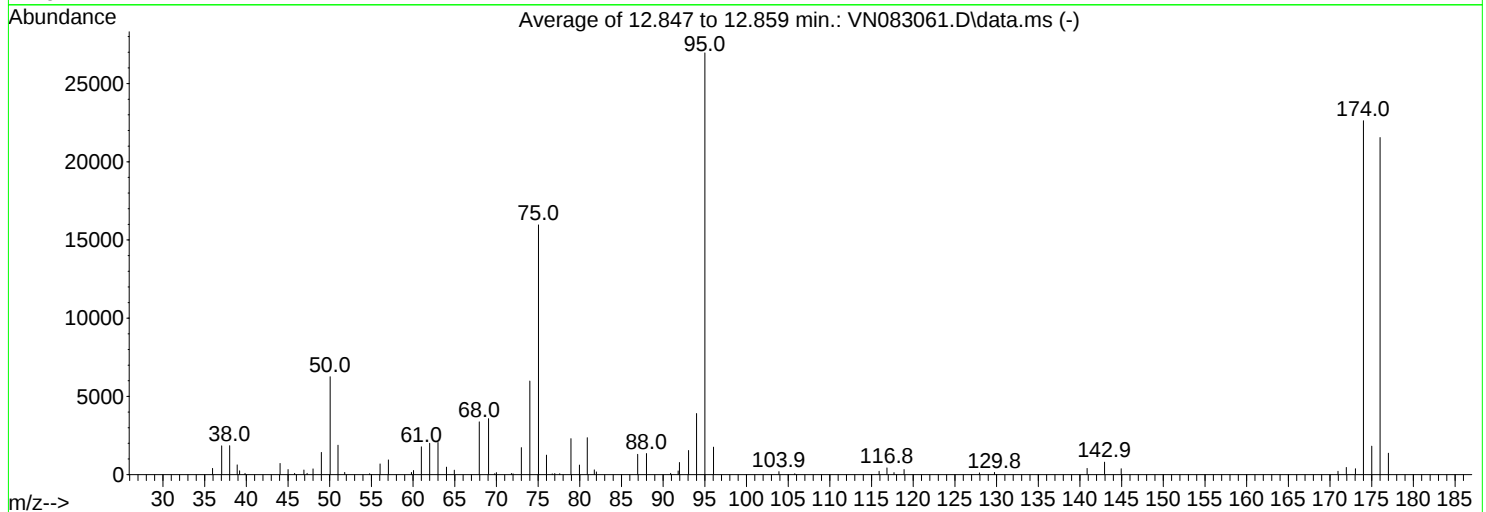


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN073024\
Data File : VN083061.D
Acq On : 30 Jul 2024 11:10
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

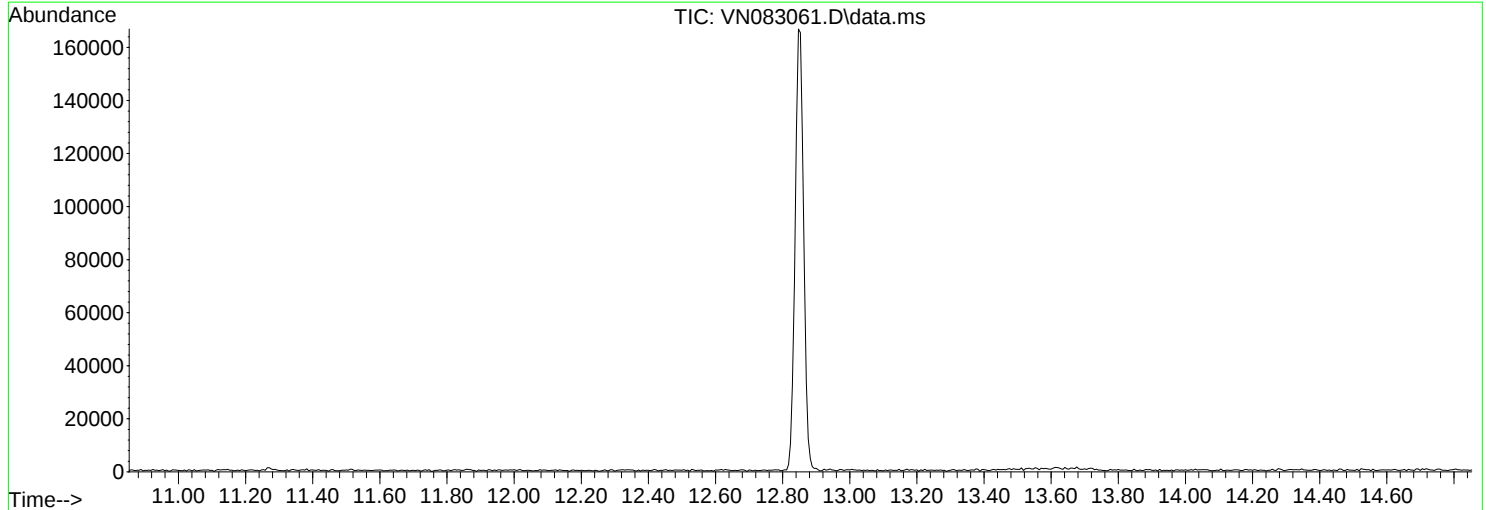

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	6263	PASS
75	95	30	60	59.2	15963	PASS
95	95	100	100	100.0	26963	PASS
96	95	5	9	6.5	1764	PASS
173	174	0.00	2	1.7	380	PASS
174	95	50	100	83.9	22624	PASS
175	174	5	9	8.1	1823	PASS
176	174	95	101	95.3	21552	PASS
177	176	5	9	6.3	1368	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	399	48.00	367	62.00	2008	74.00	597
37.05	1844	49.00	1426	63.00	2057	75.05	1596
38.00	1856	50.05	6263	64.00	485	76.00	124
38.90	627	51.00	1885	64.95	288	76.70	5
39.20	249	51.80	147	67.95	3376	77.00	71
39.85	79	54.80	61	69.05	3583	77.60	61
44.05	718	56.05	690	69.80	60	78.95	2298
45.00	323	57.05	940	70.00	136	79.95	617
45.80	81	59.80	143	71.80	76	80.90	2366
46.90	302	60.05	265	72.00	51	81.75	307
47.30	87	61.00	1782	73.00	1732	82.00	172

Average of 12.847 to 12.859 min.: VN083061.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	1299	115.90	210	173.05	380		
88.00	1346	116.85	428	174.00	22624		
90.90	80	117.70	137	175.00	1823		
91.80	239	118.90	327	176.00	21552		
91.95	774	127.95	117	177.00	1368		
93.05	1543	129.75	141				
94.00	3912	140.85	399				
95.00	26963	142.95	797				
96.05	1764	144.95	382				
103.90	194	170.95	214				
105.80	63	171.95	460				

Instrument :

MSVOA_N

ClientSampleId :

BFB